

TABLE OF CONTENTS

Case Narrative.....	1
Chain of Custody and Supporting Documentation.....	3
Radiological Analysis.....	10
Sample Data Summary.....	21
Quality Control Data.....	31
Raw Data.....	36
Method Calibration Data.....	196
Continuing Calibration Data.....	407
Background and Efficiency Data.....	425
Quality Control Charts.....	483
Standards Data.....	549
Runlogs.....	581

Case Narrative

CASE NARRATIVE
for
MWH LABORATORIES
MWH PROJECT: 99-22192/169555
TRONOX HENDERSON SITE
SDG: 158269

April 20, 2006

Laboratory Identification:

General Engineering Laboratories, LLC
2040 Savage Road
Charleston, South Carolina 29407
(843) 556-8171

Summary

Sample receipt The samples arrived at General Engineering Laboratories, LLC, Charleston, South Carolina on March 16, 2006 for analysis. Shipping container temperatures were checked, documented, and within specifications. There was no collection time listed on the chain of custody for sample 2603140364 M121-5D. The chain of custody was not signed as relinquished by the sampler. The client was notified of both issues. Please refer to the enclosed e-mails. All sample containers arrived without any visible signs of tampering or breakage. There are no additional comments concerning sample receipt.

Sample Identification The laboratory received the following samples:

<u>Laboratory ID</u>	<u>Client ID</u>
158269001	2603140361 M121-0.5
158269002	2603140362 M121-5
158269003	2603140364 M121-5D
158269004	2603140365 M121-80

Case Narrative

Sample analyses were conducted using methodology as outlined in General Engineering Laboratories (GEL) Standard Operating Procedures. Any technical or administrative problems during analysis, data review, and reduction are contained in the analytical case narratives in the enclosed data package.

Data Package

The enclosed data package contains the following sections: Case Narrative, Chain of Custody, Cooler Receipt Checklist, Data Package Qualifier Definitions and data from the following fractions: Radiochemistry.

This data package, to the best of my knowledge, is in compliance with technical and administrative requirements.

Edith M. Kent

Edith Kent

Project Manager

Chain of Custody and Supporting Documentation



MWH Laboratories
A Division of MWH Americas, Inc.
750 Royal Oaks Drive Suite 100
Monrovia, CA 91016-3629
Ph (626) 386-1100 Fax (626) 386-1095

Ship To **Edie Kent**

General Engineering Laboratories, LLC
2040 Savage Road
Charleston, SC 29414

(843) 556-8171 X4433 Fax (843) 766-1178

MWH Project # Report Due: Sub PO#
169555 03/30/06 99-22192

JDL

Use MWH
Lab # for ID

Date 03/15/06 Submittal Form & Purchase Order 99-22192

*REPORTING REQUIREMENTS: Do Not Combine Report with any other samples submitted under different MWH project numbers!
Report & Invoice must have the MWH Project Number 169555 and Job # Find Out
Sub PO# 99-22192

Report all quality control data according to Method. Include dates analyzed, date extracted (if extracted) and Method reference on the report.
Results must have Complete data & QC with Approval Signature. See reverse side for List of Terms and Conditions

Reports: Julie Lee Sub-contracting Administrator
EMAIL TO: Julie.Lee@mwhglobal.com
MWH Laboratories 750 Royal Oaks Dr. Ste. 100, Monrovia, CA. 91016
Phone (626) 386-1136 Fax (626) 386-1095
Invoices to: MWH LABORATORIES
Accounts Payable PO BOX 6610, Broomfield, CO 80021

Provide in each Report
the Specified State
Certification # & Exp Date for
requested tests + matrix

CA ELAP OK

Container

Analysis Requested Date & Time Matrix

Client Sample ID for reference only

1	2	3	4	5	6	7	8	9	10	11	12	13	14
custsub	2603140361	M121-0.5	RADIUM 226	03/10/06	7:46	soil	5 1L poly bottles						
			RADIUM 228										
			LEAD 210										
			LEAD212										
			THORIUM (ISOTOPIC)										
			URANIUM (ISOTOPIC)										
			URANIUM (TOTAL)										
	2603140362	M121-5	RADIUM 226	03/10/06	7:55	soil	5 1L poly bottles						
			RADIUM 228										
			LEAD 210										
			LEAD212										
			THORIUM (ISOTOPIC)										
			URANIUM (ISOTOPIC)										
			URANIUM (TOTAL)										

Relinquished by:

Sample Control

Date 03/15/06

Time 1457

MUST HAVE NOTIFICATION IF TEMP IS GREATER THAN 6 OR LESS THAN 2 CELSIUS
Page 1

Received by: C. Devi cotts

Date 3/14/04

Time 0915

An Acknowledgement of Receipt is requested to attn: Julie Lee

Container

Matrix

Sample Date & Time

Analysis Requested

Client Sample ID for reference only

Row

Row	Client Sample ID for reference only	Analysis Requested	Sample Date & Time	Matrix	Container
15	2603140364	RADIUM 226	03/10/06	soil	5 1L poly bottles
16	M121-5D	RADIUM 228			
17		LEAD 210			
18		LEAD212			
19		THORIUM (ISOTOPIC)			
20		URANIUM (ISOTOPIC)			
21		URANIUM (TOTAL)			
22	2603140365	RADIUM 226	03/10/06 12:00	soil	5 1L poly bottles
23	M121-80	RADIUM 228			
24		LEAD 210			
25		LEAD212			
26		THORIUM (ISOTOPIC)			
27		URANIUM (ISOTOPIC)			
28		URANIUM (TOTAL)			



Relinquished by: _____ Date 03/15/06 Time 1457 MUST HAVE NOTIFICATION IF TEMP IS GREATER THAN 6 OR LESS THAN 2 CELSIUS

Received by: C. Dennis Date 3/14/06 Time 0915 An Acknowledgement of Receipt is requested to attn: Julie Lee



SAMPLE RECEIPT & REVIEW FORM

PM use only

Client: <u>MWH Labs.</u>	SDG/ARCO/Work Order:
Date Received: <u>3/16/06</u>	PM(A) Review (ensure non-conforming items are resolved prior to signing):
Received By: <u>C. Denicoto</u>	<u>EM</u>

Sample Receipt Criteria	Yes	NA	No	Comments/Qualifiers (Required for Non-Conforming Items)
1 Shipping containers received intact and sealed?	✓			Circle Applicable: seals broken damaged container leaking container other (describe)
2 Samples requiring cold preservation within (4 +/- 2 C)? Record preservation method.	✓			Circle Coolant # ice bags <u>blue ice</u> dry ice none other describe) 4°C
3 Chain of custody documents included with shipment?	✓			
4 Sample containers intact and sealed?	✓			Circle Applicable: seals broken damaged container leaking container other (describe)
5 Samples requiring chemical preservation at proper pH?	✓			Sample ID's, containers affected and observed pH:
6 VOA vials free of headspace (defined as < 6mm bubble)?			✓	Sample ID's and containers affected:
7 Are Encore containers present? (If yes, immediately deliver to VOA laboratory)			✓	
8 Samples received within holding time?	✓			Id's and tests affected:
9 Sample ID's on COC match ID's on bottles?	✓			Sample ID's and containers affected:
10 Date & time on COC match date & time on bottles?	✓			Sample ID's affected: (C) 1.250 mL 1. meat Pipe
11 Number of containers received match number indicated on COC?			✓	Sample ID's affected: <u>Received</u> M121-0.5 = 2.250 mL g/jars # M121-80 M121-5 = 2.250 mL g/jars # M121-5D = 2 g/jars
12 COC form is properly signed in relinquished/received sections?	✓			
14 Air Bill, Tracking #'s, & Additional Comments				Fed Ex TRK # 6912 3665 2641 6912 3665 2560

Suspected Hazard Information	Non-Regulated	Regulated	High Level	RSO RAD Receipt # _____ *If > x2 area background is observed on samples identified as "non-regulated/non-radioactive", contact the Radiation Safety group for further investigation.
A Radiological Classification?	✓			Maximum Counts Observed*: <u>30 CPM</u>
B PCB Regulated?	✓			Comments:
C Shipped as DOT Hazardous Material? If yes, contact Waste Manager or ESH Manager.	✓			Hazard Class Shipped: UN#:

PM (or PMA) review of Hazard classification: EM Initials 3/16/06 Date:

Subject: Re: Please provide time of collection for sample 2603140364, M121-5D, MWH Project # 169555
From: Linda Geddes <Linda.Geddes@us.mwhglobal.com>
Date: Thu, 16 Mar 2006 15:43:32 -0800
To: Edie Kent <emk@gel.com>

That is correct - the D stands for Duplicate

This transmission and/or attachments contain information which are confidential and/or privileged. The information is intended for the addressee only. If you are not the intended recipient, any dissemination, distribution or copying of this communication is prohibited. If you have received this communication in error, please notify and return the original communication to the sender.

Linda Geddes
Project Manager
MWH Laboratories
750 Royal Oaks Drive, Suite 100
Monrovia, CA 91016
(626) 386-1163

Edie Kent <emk@gel.com>

03/16/2006 03:43 PM

To Linda Geddes <Linda.Geddes@us.mwhglobal.com>, benjamin Jenkins <ben01079@gel.com>

cc

Subject Re: Please provide time of collection for sample 2603140364, M121-5D, MWH Project # 169555

Looks like they didn't give you a time of collection either. Sample must be a duplicate.

Edie

Linda Geddes wrote:

This transmission and/or attachments contain information which are confidential and/or privileged. The information is intended for the addressee only. If you are not the intended recipient, any dissemination, distribution or copying of this communication is prohibited. If you have received this communication in error, please notify and return the original communication to the sender.

Linda Geddes
Project Manager
MWH Laboratories
750 Royal Oaks Drive, Suite 100
Monrovia, CA 91016
(626) 386-1163

Edie Kent <emk@gel.com>

03/16/2006 03:20 PM

To Linda Geddes <Linda.Geddes@us.mwhglobal.com>, benjamin Jenkins <ben01079@gel.com>

cc

Subject Please provide time of collection for sample 2603140364, M121-5D, MWH Project # 169555

Linda:
There is no time of collection on the chain of custody for this sample

and the time has been crossed off the sample container. Can you provide us with a time of collection?

Edie

--

Edith M. Kent
Project Manager
General Engineering Laboratories, LLC
2040 Savage Road
PO Box 30712
Charleston, SC 29407
Phone: 843-556-8171, ext. 4453
Fax: 843-766-1178
e-mail: emk@gel.com
web-site: www.gel.com

--

Edith M. Kent
Project Manager
General Engineering Laboratories, LLC
2040 Savage Road
PO Box 30712
Charleston, SC 29407
Phone: 843-556-8171, ext. 4453
Fax: 843-766-1178
e-mail: emk@gel.com
web-site: www.gel.com

Subject: Chains Received Today
From: Edie Kent <emk@gel.com>
Date: Thu, 16 Mar 2006 18:49:49 -0500
To: Linda.Geddes@mwhglobal.com
CC: benjamin Jenkins <ben01079@gel.com>

Linda:

Just for your information, there are no relinquished by signatures on any of the chains received today.

Edie

--

Edith M. Kent
Project Manager
General Engineering Laboratories, LLC
2040 Savage Road
PO Box 30712
Charleston, SC 29407
Phone: 843-556-8171, ext. 4453
Fax: 843-766-1178
e-mail: emk@gel.com
web-site: www.gel.com

RADIOLOGICAL ANALYSIS

**Radiochemistry Case Narrative
MWH Laboratories (MWHL)
Work Order 158269**

Method/Analysis Information

Product:	Alphaspec Th, Solid
Analytical Method:	DOE EML HASL-300, Th-01-RC Modified
Prep Method:	Ash Soil Prep
Dry Soil Prep GL-RAD-A-021 Method:	Dry Soil Prep
Analytical Batch Number:	517153
Prep Batch Number:	512732
Dry Soil Prep GL-RAD-A-021 Batch Number:	512731

Sample ID	Client ID
158269001	2603140361 M121-0.5
158269002	2603140362 M121-5
158269003	2603140364 M121-5D
158269004	2603140365 M121-80
1201062927	Method Blank (MB)
1201062928	158269001(2603140361 M121-0.5) Sample Duplicate (DUP)
1201062929	158269001(2603140361 M121-0.5) Matrix Spike (MS)
1201062930	Laboratory Control Sample (LCS)

SOP Reference

Procedure for preparation, analysis and reporting of analytical data are controlled by General Engineering Laboratories, LLC as Standard Operating Procedure (SOP). The data discussed in this narrative has been analyzed in accordance with GL-RAD-A-038 REV# 9.

Calibration Information:

Calibration Information

All initial and continuing calibration requirements have been met.

Standards Information

Standard solution(s) for these analyses are NIST traceable and used before the expiration date(s).

Sample Geometry

All counting sources were prepared in the same geometry as the calibration standards.

Quality Control (QC) Information:

Blank Information

The blank volume is representative of the sample volume in this batch.

Designated QC

The following sample was used for QC: 158269001 (2603140361 M121-0.5).

QC Information

All of the QC samples met the required acceptance limits.

Technical Information:

Holding Time

All sample procedures for this sample set were performed within the required holding time.

Preparation Information

All preparation criteria have been met for these analyses.

Sample Re-prep/Re-analysis

Sample 1201062930 (LCS) was recounted due to poor resolution.

Miscellaneous Information:

NCR Documentation

Nonconformance reports are generated to document any procedural anomalies that may deviate from referenced SOP or contractual documents. A nonconformance report (NCR) was not generated for this SDG.

Manual Integration

No manual integrations were performed on data in this batch.

Additional Comments

The Th-230 blank result is greater than the MDA, but less than the detection limit. The sample and duplicate, 1201062928 (2603140361 M121-0.5) and 158269001 (2603140361 M121-0.5), do not meet the relative percent difference requirements for Th-228, Th-230, and Th-232; however they do meet the relative error ratio requirements with the values of 2.31 for Th-228, 2.01 for Th-230, and 1.71 for Th-232.

Qualifier information

Manual qualifiers were not required.

Method/Analysis Information

Product: Alphaspec U, Solid
Analytical Method: DOE EML HASL-300, U-02-RC Modified
Prep Method: Ash Soil Prep
Dry Soil Prep GL-RAD-A-021 Method: Dry Soil Prep
Analytical Batch Number: 517155
Prep Batch Number: 512732
Dry Soil Prep GL-RAD-A-021 Batch Number: 512731

Sample ID	Client ID
158269001	2603140361 M121-0.5
158269002	2603140362 M121-5
158269003	2603140364 M121-5D
158269004	2603140365 M121-80
1201062931	Method Blank (MB)
1201062932	158269001(2603140361 M121-0.5) Sample Duplicate (DUP)
1201062933	158269001(2603140361 M121-0.5) Matrix Spike (MS)
1201062934	Laboratory Control Sample (LCS)

SOP Reference

Procedure for preparation, analysis and reporting of analytical data are controlled by General Engineering Laboratories, LLC as Standard Operating Procedure (SOP). The data discussed in this narrative has been analyzed in accordance with GL-RAD-A-011 REV# 14.

Calibration Information:

Calibration Information

All initial and continuing calibration requirements have been met.

Standards Information

Standard solution(s) for these analyses are NIST traceable and used before the expiration date(s).

Sample Geometry

All counting sources were prepared in the same geometry as the calibration standards.

Quality Control (QC) Information:

Blank Information

The blank volume is representative of the sample volume in this batch.

Designated QC

The following sample was used for QC: 158269001 (2603140361 M121-0.5).

QC Information

All of the QC samples met the required acceptance limits.

Technical Information:

Holding Time

All sample procedures for this sample set were performed within the required holding time.

Preparation Information

All preparation criteria have been met for these analyses.

Sample Re-prep/Re-analysis

None of the samples in this sample set required reprep or reanalysis.

Miscellaneous Information:

NCR Documentation

Nonconformance reports are generated to document any procedural anomalies that may deviate from referenced SOP or contractual documents. A nonconformance report (NCR) was not generated for this SDG.

Manual Integration

No manual integrations were performed on data in this batch.

Additional Comments

Additional comments were not required for this sample set.

Qualifier information

Manual qualifiers were not required.

Method/Analysis Information

Product:	Gamma, (Pb-212,Ra-226,Ra-228)
Analytical Method:	EML HASL 300, 4.5.2.3
Prep Method:	Dry Soil Prep
Analytical Batch Number:	513802
Prep Batch Number:	512731

Sample ID	Client ID
158269001	2603140361 M121-0.5
158269002	2603140362 M121-5
158269003	2603140364 M121-5D
158269004	2603140365 M121-80
1201055607	Method Blank (MB)
1201055608	158269001(2603140361 M121-0.5) Sample Duplicate (DUP)
1201055609	Laboratory Control Sample (LCS)

SOP Reference

Procedure for preparation, analysis and reporting of analytical data are controlled by General Engineering Laboratories, LLC as Standard Operating Procedure (SOP). The data discussed in this narrative has been analyzed in accordance with GL-RAD-A-013 REV# 10.

Calibration Information:

Calibration Information

All initial and continuing calibration requirements have been met.

Standards Information

Standard solution(s) for these analyses are NIST traceable and used before the expiration date(s).

Sample Geometry

All counting sources were prepared in the same geometry as the calibration standards.

Quality Control (QC) Information:

Blank Information

The blank volume is representative of the sample volume in this batch.

Designated QC

The following sample was used for QC: 158269001 (2603140361 M121-0.5).

QC Information

All of the QC samples met the required acceptance limits.

Technical Information:

Holding Time

All sample procedures for this sample set were performed within the required holding time.

Preparation Information

All preparation criteria have been met for these analyses.

Sample Re-prep/Re-analysis

None of the samples in this sample set required reprep or reanalysis.

Miscellaneous Information:

NCR Documentation

Nonconformance reports are generated to document any procedural anomalies that may deviate from referenced SOP or contractual documents. A nonconformance report (NCR) was not generated for this SDG.

Additional Comments

Additional comments were not required for this sample set.

Qualifier information

Qualifier	Reason	Analyte	Sample
UI	Data rejected due to low abundance.	Lead-212	1201055607

Method/Analysis Information

Product:	GFPC, Pb210, Solid
Analytical Method:	DOE RP280 Modified
Prep Method:	Ash Soil Prep
Dry Soil Prep GL-RAD-A-021 Method:	Dry Soil Prep
Analytical Batch Number:	517517
Prep Batch Number:	512732
Dry Soil Prep GL-RAD-A-021 Batch Number:	512731

Sample ID	Client ID
158269001	2603140361 M121-0.5
158269002	2603140362 M121-5
158269003	2603140364 M121-5D
158269004	2603140365 M121-80
1201063764	Method Blank (MB)
1201063765	158048005(2603090029) Sample Duplicate (DUP)
1201063766	158048005(2603090029) Matrix Spike (MS)
1201063767	Laboratory Control Sample (LCS)

SOP Reference

Procedure for preparation, analysis and reporting of analytical data are controlled by General Engineering Laboratories, LLC as Standard Operating Procedure (SOP). The data discussed in this narrative has been analyzed in accordance with GL-RAD-A-018 REV# 5.

Calibration Information:

Calibration Information

All initial and continuing calibration requirements have been met.

Standards Information

Standard solution(s) for these analyses are NIST traceable and used before the expiration date(s).

Sample Geometry

All counting sources were prepared in the same geometry as the calibration standards.

Quality Control (QC) Information:

Blank Information

The blank volume is representative of the sample volume in this batch.

Designated QC

The following sample was used for QC: 158048005 (2603090029).

QC Information

All of the QC samples met the required acceptance limits.

Technical Information:

Holding Time

All sample procedures for this sample set were performed within the required holding time.

Preparation Information

All preparation criteria have been met for these analyses.

Sample Re-prep/Re-analysis

None of the samples in this sample set required reprep or reanalysis.

Chemical Recoveries

All chemical recoveries meet the required acceptance limits for this sample set.

Miscellaneous Information:

NCR Documentation

Nonconformance reports are generated to document any procedural anomalies that may deviate from referenced SOP or contractual documents. A nonconformance report (NCR) was not generated for this SDG.

Additional Comments

Additional comments were not required for this sample set.

Qualifier information

Manual qualifiers were not required.

Method/Analysis Information

Product:	KPA, Total U, Solid
Analytical Method:	ASTM D 5174
Prep Method:	Ash Soil Prep
Dry Soil Prep GL-RAD-A-021 Method:	Dry Soil Prep
Analytical Batch Number:	521637
Prep Batch Number:	512732
Dry Soil Prep GL-RAD-A-021 Batch Number:	512731

Sample ID	Client ID
158269001	2603140361 M121-0.5
158269002	2603140362 M121-5
158269003	2603140364 M121-5D
158269004	2603140365 M121-80
1201073174	Method Blank (MB)
1201073175	158269001(2603140361 M121-0.5) Sample Duplicate (DUP)
1201073176	158269001(2603140361 M121-0.5) Matrix Spike (MS)
1201073177	Laboratory Control Sample (LCS)
1201073178	Laboratory Control Sample Duplicate (LCSD)

SOP Reference

Procedure for preparation, analysis and reporting of analytical data are controlled by General Engineering Laboratories, LLC as Standard Operating Procedure (SOP). The data discussed in this narrative has been analyzed in accordance with GL-RAD-A-023 REV# 11.

Calibration Information:

Calibration Information

All initial and continuing calibration requirements have been met. The calibration for Total Uranium is performed prior to each analysis and is located in the raw data section.

Standards Information

Standard solution(s) for these analyses are NIST traceable and used before the expiration date(s).

Sample Geometry

All counting sources were prepared in the same geometry as the calibration standards.

Quality Control (QC) Information:

Blank Information

The blank volume is representative of the sample volume in this batch.

Designated QC

The following sample was used for QC: 158269001 (2603140361 M121-0.5).

QC Information

All of the QC samples met the required acceptance limits.

Technical Information:**Holding Time**

All sample procedures for this sample set were performed within the required holding time.

Preparation Information

All preparation criteria have been met for these analyses.

Sample Re-prep/Re-analysis

The following samples, 1201073175 (2603140361 M121-0.5) and 1201073176 (2603140361 M121-0.5), failed lifetime, were reanalyzed and failed lifetime on the reanalysis. The samples were diluted 1:1 and reanalyzed. The reanalysis passed lifetime. The samples were then reanalyzed again to verify the results greater than the RDL. The results from the dilution are reported. The following samples, 158269001 (2603140361 M121-0.5), 158269002 (2603140362 M121-5), 158269003 (2603140364 M121-5D) and 158269004 (2603140365 M121-80), were greater than the RDL. The samples were reanalyzed and verified.

Miscellaneous Information:**NCR Documentation**

Nonconformance reports are generated to document any procedural anomalies that may deviate from referenced SOP or contractual documents. A nonconformance report (NCR) was not generated for this SDG.

Additional Comments

Additional comments were not required for this sample set.

Qualifier information

Manual qualifiers were not required.

Certification Statement

Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless otherwise noted in the analytical case narrative.

Review Validation:

GEL requires all analytical data to be verified by a qualified data validator. In addition, all data designated for CLP or CLP-like packaging will receive a third level validation upon completion of the data package.

The following data validator verified the information presented in this case narrative:

Reviewer/Date: A/ cull G Chude 4/21/06

SAMPLE DATA SUMMARY

GENERAL ENGINEERING LABORATORIES, LLC
2040 Savage Road Charleston SC 29407 - (843) 556-8171 - www.gel.com

**Certificate of Analysis Report
for**

MWHL002 MWH Laboratories
Client SDG: 158269 GEL Work Order: 158269

The Qualifiers in this report are defined as follows:

- * Indicates that a quality control analyte recovery is outside of specified acceptance criteria.
- < Result is less than amount reported.
- > Result is greater than amount reported.
- B Target analyte was detected in the sample as well as the associated blank.
- BD Results below the MDC or low tracer recovery.
- D Sample has been diluted and reanalyzed after initially exceeding inst. calibration range
- E Concentration of the target analyte exceeds the instrument calibration range.
- H Analytical holding time exceeded.
- J Indicates an estimated value.
- P The response between the confirmation and the primary columns is >40% Different.
- R Sample results are rejected.
- U Target analyte was analyzed for but not detected above the MDL, MDA, or LOD.
- UI Uncertain identification for gamma spectroscopy.
- X Lab-specific qualifier-please see case narrative, data summary package or contact your project manager for details.
- Y QC Samples were not spiked with this compound.
- Z Paint Filter qualifier: Particulates passed through the filter. No free liquids were observed.
- d The 2:1 depletion requirement was not met for this sample
- h Sample preparation or preservation holding time exceeded.
- ND The analyte concentration is not detected above the reporting limit.

Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless qualified on the Certificate of Analysis.

** Indicates the analyte is a surrogate compound.

This data report has been prepared and reviewed in accordance with General Engineering Laboratories, LLC standard operating procedures. Please direct any questions to your Project Manager, Edith Kent.



Reviewed by _____

GENERAL ENGINEERING LABORATORIES, LLC

2040 Savage Road Charleston SC 29407 – (843) 556-8171 – www.gel.com

Certificate of Analysis

Company : MWH Laboratories
 Address : 750 Royal Oaks Drive, Suite 100
 Monrovia, California 91016

Report Date: April 21, 2006

Contact: Ms. Julie Lee
 Project: **Tronox Henderson**

Client Sample ID:	2603140361 M121-0.5	Project:	MWHL00106
Sample ID:	158269001	Client ID:	MWHL002
Matrix:	Soil		
Collect Date:	10-MAR-06 07:46		
Receive Date:	16-MAR-06		
Collector:	Client		

Parameter	Qualifier	Result	Uncertainty	DL	RL	Units	DF	Analyst	Date	Time	Batch	Method
Rad Alpha Spec Analysis												
<i>Alphaspec Th, Solid</i>												
Thorium-228		3.04	+/-0.921	0.446	1.00	pCi/g		LCW1	04/07/06	1807	517153	1
Thorium-230		0.824	+/-0.407	0.349	1.00	pCi/g						
Thorium-232		2.42	+/-0.774	0.241	1.00	pCi/g						
<i>Alphaspec U, Solid</i>												
Uranium-233/234		0.804	+/-0.329	0.281	1.00	pCi/g		LCW1	04/08/06	1543	517155	2
Uranium-235/236		0.162	+/-0.159	0.121	1.00	pCi/g						
Uranium-238		1.21	+/-0.397	0.247	1.00	pCi/g						
Rad Gamma Spec Analysis												
<i>Gamma, (Pb-212, Ra-226, Ra-228)</i>												
Lead-212		2.13	+/-0.236	0.0892	10.0	pCi/g		MJH1	04/10/06	2153	513802	3
Radium-226		1.06	+/-0.184	0.107	2.00	pCi/g						
Radium-228		1.86	+/-0.377	0.179	1.00	pCi/g						
Rad Gas Flow Proportional Counting												
<i>GFPC, Pb210, Solid</i>												
Lead-210	U	0.582	+/-0.396	0.722	3.00	pCi/g		BXF1	04/09/06	0957	517517	4
Rad Total Uranium												
<i>KPA, Total U, Solid</i>												
Total Uranium		2.45	+/-0.158	0.108	1.00	ug/g		DRS1	04/19/06	1006	521637	5

The following Prep Methods were performed

Method	Description	Analyst	Date	Time	Prep Batch
Ash Soil Prep	Ash Soil Prep, GL-RAD-A-021B	JMB1	03/21/06	0958	512732
Dry Soil Prep	Dry Soil Prep GL-RAD-A-021	JMB1	03/20/06	1527	512731

The following Analytical Methods were performed

Method	Description	Analyst Comments
1	DOE EML HASL-300, Th-01-RC Modified	
2	DOE EML HASL-300, U-02-RC Modified	
3	EML HASL 300, 4.5.2.3	
4	DOE RP280 Modified	
5	ASTM D 5174	

Surrogate/Tracer recovery	Test	Result	Nominal	Recovery%	Acceptable Limits

GENERAL ENGINEERING LABORATORIES, LLC

2040 Savage Road Charleston SC 29407 – (843) 556-8171 – www.gel.com

Certificate of Analysis

Company : MWH Laboratories
 Address : 750 Royal Oaks Drive, Suite 100
 Monrovia, California 91016

Report Date: April 21, 2006

Contact: Ms. Julie Lee
 Project: **Tronox Henderson**

Client Sample ID: 2603140361 M121-0.5
 Sample ID: 158269001

Project: MWHL00106
 Client ID: MWHL002

Parameter	Qualifier	Result	Uncertainty	DL	RL	Units	DF	AnalystDate	Time	Batch	Method
Surrogate/Tracer recovery	Test					Result	Nominal	Recovery%		Acceptable Limits	
Actinium-227	Alphaspec Th, Solid							80			
Actinium-227	Alphaspec Th, Solid							80			
Actinium-227	Alphaspec Th, Solid							80			
Uranium-232	Alphaspec U, Solid							82		(25%–125%)	
Uranium-232	Alphaspec U, Solid							82		(25%–125%)	
Uranium-232	Alphaspec U, Solid							82		(25%–125%)	
Lead-210	GFPC, Pb210, Solid							66		(25%–125%)	

GENERAL ENGINEERING LABORATORIES, LLC

2040 Savage Road Charleston SC 29407 – (843) 556–8171 – www.gel.com

Certificate of Analysis

Company : MWH Laboratories
 Address : 750 Royal Oaks Drive, Suite 100
 Monrovia, California 91016

Report Date: April 21, 2006

Contact: Ms. Julie Lee
 Project: **Tronox Henderson**

Client Sample ID:	2603140362 M121-5	Project:	MWHL00106
Sample ID:	158269002	Client ID:	MWHL002
Matrix:	Soil		
Collect Date:	10-MAR-06 07:55		
Receive Date:	16-MAR-06		
Collector:	Client		

Parameter	Qualifier	Result	Uncertainty	DL	RL	Units	DF	Analyst	Date	Time	Batch	Method
Rad Alpha Spec Analysis												
<i>Alphaspec Th, Solid</i>												
Thorium-228		1.21	+/-0.408	0.295	1.00	pCi/g		LCW1	04/07/06	1807	517153	1
Thorium-230		1.32	+/-0.424	0.251	1.00	pCi/g						
Thorium-232		1.23	+/-0.402	0.204	1.00	pCi/g						
<i>Alphaspec U, Solid</i>												
Uranium-233/234		1.79	+/-0.505	0.291	1.00	pCi/g		LCW1	04/08/06	1543	517155	2
Uranium-235/236	U	0.0889	+/-0.123	0.133	1.00	pCi/g						
Uranium-238		1.22	+/-0.418	0.272	1.00	pCi/g						
Rad Gamma Spec Analysis												
<i>Gamma, (Pb-212, Ra-226, Ra-228)</i>												
Lead-212		1.34	+/-0.141	0.0494	10.0	pCi/g		MJH1	04/10/06	2357	513802	3
Radium-226		1.39	+/-0.146	0.0579	2.00	pCi/g						
Radium-228		1.24	+/-0.210	0.0948	1.00	pCi/g						
Rad Gas Flow Proportional Counting												
<i>GFPC, Pb210, Solid</i>												
Lead-210	U	-0.0573	+/-0.261	0.688	3.00	pCi/g		BXF1	04/09/06	0958	517517	4
Rad Total Uranium												
<i>KPA, Total U, Solid</i>												
Total Uranium		3.02	+/-0.101	0.109	1.00	ug/g		DRS1	04/19/06	1008	521637	5

The following Prep Methods were performed

Method	Description	Analyst	Date	Time	Prep Batch
Ash Soil Prep	Ash Soil Prep, GL-RAD-A-021B	JMB1	03/21/06	0958	512732
Dry Soil Prep	Dry Soil Prep GL-RAD-A-021	JMB1	03/20/06	1527	512731

The following Analytical Methods were performed

Method	Description	Analyst Comments
1	DOE EML HASL-300, Th-01-RC Modified	
2	DOE EML HASL-300, U-02-RC Modified	
3	EML HASL 300, 4.5.2.3	
4	DOE RP280 Modified	
5	ASTM D 5174	

Surrogate/Tracer recovery	Test	Result	Nominal	Recovery%	Acceptable Limits

GENERAL ENGINEERING LABORATORIES, LLC

2040 Savage Road Charleston SC 29407 – (843) 556-8171 – www.gel.com

Certificate of Analysis

Company : MWH Laboratories
Address : 750 Royal Oaks Drive, Suite 100
Monrovia, California 91016

Report Date: April 21, 2006

Contact: Ms. Julie Lee
Project: **Tronox Henderson**

Client Sample ID: 2603140362 M121-5
Sample ID: 158269002

Project: MWHL00106
Client ID: MWHL002

Parameter	Qualifier	Result	Uncertainty	DL	RL	Units	DF	Analyst	Date	Time	Batch	Method
Surrogate/Tracer recovery	Test					Result	Nominal	Recovery%				Acceptable Limits
Actinium-227	Alphaspec Th, Solid							119				
Actinium-227	Alphaspec Th, Solid							119				
Actinium-227	Alphaspec Th, Solid							119				
Uranium-232	Alphaspec U, Solid							71				(25%-125%)
Uranium-232	Alphaspec U, Solid							71				(25%-125%)
Uranium-232	Alphaspec U, Solid							71				(25%-125%)
Lead-210	GFPC, Pb210, Solid							76				(25%-125%)

GENERAL ENGINEERING LABORATORIES, LLC

2040 Savage Road Charleston SC 29407 – (843) 556–8171 – www.gel.com

Certificate of Analysis

Company : MWH Laboratories
 Address : 750 Royal Oaks Drive, Suite 100
 Monrovia, California 91016

Report Date: April 21, 2006

Contact: Ms. Julie Lee
 Project: **Tronox Henderson**

Client Sample ID:	2603140364 M121–5D	Project:	MWHL00106
Sample ID:	158269003	Client ID:	MWHL002
Matrix:	Soil		
Collect Date:	10–MAR–06 12:00		
Receive Date:	16–MAR–06		
Collector:	Client		

Parameter	Qualifier	Result	Uncertainty	DL	RL	Units	DF	AnalystDate	Time	Batch	Method
Rad Alpha Spec Analysis											
<i>Alphaspec Th, Solid</i>											
Thorium–228		1.71	+/-0.655	0.472	1.00	pCi/g		LCW1 04/07/06	1807	517153	1
Thorium–230		1.26	+/-0.523	0.216	1.00	pCi/g					
Thorium–232		1.37	+/-0.554	0.255	1.00	pCi/g					
<i>Alphaspec U, Solid</i>											
Uranium–233/234		1.47	+/-0.444	0.360	1.00	pCi/g		LCW1 04/08/06	1543	517155	2
Uranium–235/236	U	0.111	+/-0.161	0.322	1.00	pCi/g					
Uranium–238		0.689	+/-0.328	0.416	1.00	pCi/g					
Rad Gamma Spec Analysis											
<i>Gamma, (Pb–212,Ra–226,Ra–228)</i>											
Lead–212		1.55	+/-0.169	0.0632	10.0	pCi/g		MJH1 04/11/06	0614	513802	3
Radium–226		1.28	+/-0.159	0.0682	2.00	pCi/g					
Radium–228		1.35	+/-0.262	0.143	1.00	pCi/g					
Rad Gas Flow Proportional Counting											
<i>GFPC, Pb210, Solid</i>											
Lead–210	U	0.171	+/-0.366	0.839	3.00	pCi/g		BXF1 04/09/06	0958	517517	4
Rad Total Uranium											
<i>KPA, Total U, Solid</i>											
Total Uranium		2.62	+/-0.0898	0.107	1.00	ug/g		DRS1 04/19/06	1010	521637	5

The following Prep Methods were performed

Method	Description	Analyst	Date	Time	Prep Batch
Ash Soil Prep	Ash Soil Prep, GL–RAD–A–021B	JMB1	03/21/06	0958	512732
Dry Soil Prep	Dry Soil Prep GL–RAD–A–021	JMB1	03/20/06	1527	512731

The following Analytical Methods were performed

Method	Description	Analyst Comments
1	DOE EML HASL–300, Th–01–RC Modified	
2	DOE EML HASL–300, U–02–RC Modified	
3	EML HASL 300, 4.5.2.3	
4	DOE RP280 Modified	
5	ASTM D 5174	

Surrogate/Tracer recovery	Test	Result	Nominal	Recovery%	Acceptable Limits
---------------------------	------	--------	---------	-----------	-------------------

GENERAL ENGINEERING LABORATORIES, LLC

2040 Savage Road Charleston SC 29407 – (843) 556-8171 – www.gel.com

Certificate of Analysis

Company : MWH Laboratories
 Address : 750 Royal Oaks Drive, Suite 100
 Monrovia, California 91016

Report Date: April 21, 2006

Contact: Ms. Julie Lee
 Project: **Tronox Henderson**

Client Sample ID: 2603140364 M121-5D
 Sample ID: 158269003

Project: MWHL00106
 Client ID: MWHL002

Parameter	Qualifier	Result	Uncertainty	DL	RL	Units	DF	AnalystDate	Time	Batch	Method
Surrogate/Tracer recovery	Test					Result	Nominal	Recovery%		Acceptable Limits	
Actinium-227	Alphaspec Th, Solid							65			
Actinium-227	Alphaspec Th, Solid							65			
Actinium-227	Alphaspec Th, Solid							65			
Uranium-232	Alphaspec U, Solid							78		(25%–125%)	
Uranium-232	Alphaspec U, Solid							78		(25%–125%)	
Uranium-232	Alphaspec U, Solid							78		(25%–125%)	
Lead-210	GFPC, Pb210, Solid							74		(25%–125%)	

GENERAL ENGINEERING LABORATORIES, LLC

2040 Savage Road Charleston SC 29407 – (843) 556–8171 – www.gel.com

Certificate of Analysis

Company : MWH Laboratories
 Address : 750 Royal Oaks Drive, Suite 100
 Monrovia, California 91016

Report Date: April 21, 2006

Contact: Ms. Julie Lee
 Project: **Tronox Henderson**

Client Sample ID:	2603140365 M121–80	Project:	MWHL00106
Sample ID:	158269004	Client ID:	MWHL002
Matrix:	Soil		
Collect Date:	10–MAR–06 12:00		
Receive Date:	16–MAR–06		
Collector:	Client		

Parameter	Qualifier	Result	Uncertainty	DL	RL	Units	DF	Analyst	Date	Time	Batch	Method
Rad Alpha Spec Analysis												
<i>Alphaspec Th, Solid</i>												
Thorium–228		1.25	+/-0.419	0.371	1.00	pCi/g		LCW1	04/07/06	1807	517153	1
Thorium–230		1.13	+/-0.380	0.259	1.00	pCi/g						
Thorium–232		0.965	+/-0.344	0.227	1.00	pCi/g						
<i>Alphaspec U, Solid</i>												
Uranium–233/234		0.914	+/-0.333	0.310	1.00	pCi/g		LCW1	04/08/06	1543	517155	2
Uranium–235/236	U	0.186	+/-0.171	0.244	1.00	pCi/g						
Uranium–238		0.905	+/-0.322	0.230	1.00	pCi/g						
Rad Gamma Spec Analysis												
<i>Gamma, (Pb–212, Ra–226, Ra–228)</i>												
Lead–212		1.48	+/-0.163	0.0666	10.0	pCi/g		MJH1	04/11/06	1022	513802	3
Radium–226		1.09	+/-0.155	0.0731	2.00	pCi/g						
Radium–228		1.38	+/-0.267	0.150	1.00	pCi/g						
Rad Gas Flow Proportional Counting												
<i>GFPC, Pb210, Solid</i>												
Lead–210	U	0.0537	+/-0.504	1.24	3.00	pCi/g		BXF1	04/09/06	0958	517517	4
Rad Total Uranium												
<i>KPA, Total U, Solid</i>												
Total Uranium		2.53	+/-0.100	0.106	1.00	ug/g		DRS1	04/19/06	1012	521637	5

The following Prep Methods were performed

Method	Description	Analyst	Date	Time	Prep Batch
Ash Soil Prep	Ash Soil Prep, GL–RAD–A–021B	JMB1	03/21/06	0958	512732
Dry Soil Prep	Dry Soil Prep GL–RAD–A–021	JMB1	03/20/06	1527	512731

The following Analytical Methods were performed

Method	Description	Analyst Comments
1	DOE EML HASL–300, Th–01–RC Modified	
2	DOE EML HASL–300, U–02–RC Modified	
3	EML HASL 300, 4.5.2.3	
4	DOE RP280 Modified	
5	ASTM D 5174	

Surrogate/Tracer recovery	Test	Result	Nominal	Recovery%	Acceptable Limits

GENERAL ENGINEERING LABORATORIES, LLC

2040 Savage Road Charleston SC 29407 – (843) 556-8171 – www.gel.com

Certificate of Analysis

Company : MWH Laboratories
 Address : 750 Royal Oaks Drive, Suite 100
 Monrovia, California 91016

Report Date: April 21, 2006

Contact: Ms. Julie Lee
 Project: **Tronox Henderson**

Client Sample ID: 2603140365 M121-80
 Sample ID: 158269004

Project: MWHL00106
 Client ID: MWHL002

Parameter	Qualifier	Result	Uncertainty	DL	RL	Units	DF	AnalystDate	Time	Batch	Method
Surrogate/Tracer recovery	Test					Result	Nominal	Recovery%			Acceptable Limits
Actinium-227	Alphaspec Th, Solid							116			
Actinium-227	Alphaspec Th, Solid							116			
Actinium-227	Alphaspec Th, Solid							116			
Uranium-232	Alphaspec U, Solid							90			(25%-125%)
Uranium-232	Alphaspec U, Solid							90			(25%-125%)
Uranium-232	Alphaspec U, Solid							90			(25%-125%)
Lead-210	GFPC, Pb210, Solid							45			(25%-125%)

QUALITY CONTROL DATA

GENERAL ENGINEERING LABORATORIES, LLC

2040 Savage Road Charleston, SC 29407 - (843) 556-8171 - www.gel.com

QC Summary

Report Date: April 21, 2006

Page 1 of 4

MWH Laboratories
750 Royal Oaks Drive, Suite 100
Monrovia, California

Contact: Ms. Julie Lee

Workorder: 158269

Parmname	NOM	Sample	Qual	QC	Units	RPD%	REC%	Range	Anlst	Date	Time
Rad Alpha Spec											
Batch	517153										
QC1201062928	158269001	DUP									
Thorium-228		3.04		1.77	pCi/g	53*		(0%-20%)	LCW1	04/07/06	18:07
		+/-0.921		+/-0.556							
Thorium-230		0.824		1.46	pCi/g	56*		(0%-20%)			
		+/-0.407		+/-0.469							
Thorium-232		2.42		1.62	pCi/g	40*		(0%-20%)			
		+/-0.774		+/-0.496							
QC1201062930	LCS										
Thorium-228			U	-0.0451	pCi/g			(75%-125%)		04/08/06	08:46
				+/-0.162							
Thorium-230	46.7			39.9	pCi/g		85	(75%-125%)			
				+/-8.09							
Thorium-232				0.238	pCi/g			(75%-125%)			
				+/-0.193							
QC1201062927	MB										
Thorium-228			U	0.265	pCi/g					04/07/06	18:07
				+/-0.193							
Thorium-230				0.350	pCi/g						
				+/-0.191							
Thorium-232			U	0.00663	pCi/g						
				+/-0.0513							
QC1201062929	158269001	MS									
Thorium-228		3.04		2.04	pCi/g			(75%-125%)			
		+/-0.921		+/-0.597							
Thorium-230	53.1	0.824		46.2	pCi/g		85	(75%-125%)			
		+/-0.407		+/-7.98							
Thorium-232		2.42		2.32	pCi/g			(75%-125%)			
		+/-0.774		+/-0.638							
Batch	517155										
QC1201062932	158269001	DUP									
Uranium-233/234		0.804		1.45	pCi/g	57*		(0%-20%)	LCW1	04/08/06	15:43
		+/-0.329		+/-0.475							
Uranium-235/236		0.162	U	0.122	pCi/g	28*		(0%-20%)			
		+/-0.159		+/-0.168							
Uranium-238		1.21		1.35	pCi/g	11		(0%-20%)			
		+/-0.397		+/-0.463							
QC1201062934	LCS										
Uranium-233/234				10.1	pCi/g			(75%-125%)			
				+/-1.11							
Uranium-235/236				0.834	pCi/g			(75%-125%)			
				+/-0.362							
Uranium-238	11.4			11.6	pCi/g		102	(75%-125%)			
				+/-1.19							
QC1201062931	MB										

GENERAL ENGINEERING LABORATORIES, LLC

2040 Savage Road Charleston, SC 29407 - (843) 556-8171 - www.gel.com

QC Summary

Workorder: 158269

Page 2 of 4

Parmname	NOM	Sample	Qual	QC	Units	RPD%	REC%	Range	Anlst	Date	Time
Rad Alpha Spec											
Batch	517155										
Uranium-233/234			U	0.149 +/-0.142	pCi/g						
Uranium-235/236			U	-0.0238 +/-0.0269	pCi/g				LCW1	04/08/06	15:43
Uranium-238			U	0.0406 +/-0.0761	pCi/g						
QC1201062933	158269001	MS									
Uranium-233/234		0.804 +/-0.329		14.4 +/-1.37	pCi/g			(75%-125%)			
Uranium-235/236		0.162 +/-0.159		0.578 +/-0.308	pCi/g			(75%-125%)			
Uranium-238	13.0	1.21 +/-0.397		15.7 +/-1.43	pCi/g		111	(75%-125%)			
Rad Gamma Spec											
Batch	513802										
QC1201055608	158269001	DUP									
Lead-212		2.13 +/-0.236		2.02 +/-0.209	pCi/g	5			MJH1	04/11/06	23:19
Radium-226		1.06 +/-0.184		0.963 +/-0.126	pCi/g	10		(0%-20%)			
Radium-228		1.86 +/-0.377		1.86 +/-0.290	pCi/g	0		(0%-20%)			
QC1201055609	LCS										
Americium-241	24.4			25.1 +/-1.13	pCi/g		103	(75%-125%)		04/11/06	14:31
Cesium-137	9.29			9.64 +/-0.657	pCi/g		104	(75%-125%)			
Cobalt-60	13.4			13.7 +/-0.825	pCi/g		102	(75%-125%)			
Lead-212			U	0.0816 +/-0.198	pCi/g						
Radium-226			U	0.0371 +/-0.308	pCi/g			(75%-125%)			
Radium-228			U	0.121 +/-0.806	pCi/g			(75%-125%)			
QC1201055607	MB										
Lead-212			UUI	0.00 +/-0.0278	pCi/g					04/11/06	23:19
Radium-226			U	0.0337 +/-0.0732	pCi/g						
Radium-228			U	0.00569 +/-0.0777	pCi/g						
Rad Gas Flow											
Batch	517517										
QC1201063765	158048005	DUP									
Lead-210		0.533 +/-0.462	U	0.0696 +/-0.366	pCi/g	0		(0%-20%)	BXF1	04/09/06	09:57
QC1201063767	LCS										

GENERAL ENGINEERING LABORATORIES, LLC

2040 Savage Road Charleston, SC 29407 - (843) 556-8171 - www.gel.com

QC Summary

Workorder: 158269

Page 3 of 4

Parmname	NOM	Sample	Qual	QC	Units	RPD%	REC%	Range	Anlst	Date	Time
Rad Gas Flow											
Batch	517517										
Lead-210	7.02			5.38 +/-0.793	pCi/g		77	(75%-125%)			
QC1201063764		MB									
Lead-210			U	0.0926 +/-0.347	pCi/g				BXF1	04/09/06	09:57
QC1201063766		158048005	MS								
Lead-210	7.67	U	0.533 +/-0.462	6.53 +/-1.01	pCi/g		85	(75%-125%)			
Rad Total U											
Batch	521637										
QC1201073175		158269001	DUP								
Total Uranium				2.45 +/-0.158	3.83 +/-0.093	ug/g	44*	(0%-20%)	DRS1	04/20/06	15:13
QC1201073177		LCS									
Total Uranium	10.0				8.04 +/-0.508	ug/g		80	(75%-125%)		04/19/06 10:46
QC1201073178		LCSD									
Total Uranium	1.00				0.859 +/-0.0197	ug/g	161	86			04/19/06 10:48
QC1201073174		MB									
Total Uranium			U	-0.0101 +/-0.000454	ug/g						04/19/06 10:37
QC1201073176		158269001	MS								
Total Uranium	9.43			2.45 +/-0.158	13.0 +/-0.411	ug/g		112	(75%-125%)		04/20/06 15:15

Notes:

The Qualifiers in this report are defined as follows:

- B Target analyte was detected in the sample as well as the associated blank.
- BD Results below the MDC or low tracer recovery.
- E Concentration of the target analyte exceeds the instrument calibration range.
- H Analytical holding time exceeded.
- J Indicates an estimated value.
- U Target analyte was analyzed for but not detected above the MDL, MDA, or LOD.
- UI Uncertain identification for gamma spectroscopy.
- X Lab-specific qualifier-please see case narrative, data summary package or contact your project manager for details.
- d The 2:1 depletion requirement was not met for this sample
- h Sample preparation or preservation holding time exceeded.

GENERAL ENGINEERING LABORATORIES, LLC

2040 Savage Road Charleston, SC 29407 - (843) 556-8171 - www.gel.com

QC Summary

Workorder: 158269

Page 4 of 4

<u>Parmname</u>	<u>NOM</u>	<u>Sample</u>	<u>Qual</u>	<u>QC</u>	<u>Units</u>	<u>RPD%</u>	<u>REC%</u>	<u>Range</u>	<u>Anlst</u>	<u>Date</u>	<u>Time</u>
-----------------	------------	---------------	-------------	-----------	--------------	-------------	-------------	--------------	--------------	-------------	-------------

N/A indicates that spike recovery limits do not apply when sample concentration exceeds spike conc. by a factor of 4 or more.

^ The Relative Percent Difference (RPD) obtained from the sample duplicate (DUP) is evaluated against the acceptance criteria when the sample is greater than five times (5X) the contract required detection limit (RL). In cases where either the sample or duplicate value is less than 5X the RL, a control limit of +/- the RL is used to evaluate the DUP result.

For PS, PSD, and SDILT results, the values listed are the measured amounts, not final concentrations.

Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless qualified on the QC Summary.

RAW DATA

Radiochemistry Batch Checklist, Rev 4

Batch# 517153 Product: Th Date: 04/8/06

Criteria:	Yes	No	Comments
Sample Solids are less than 100 mg for GAB.			N/A
If activity less 10* MDA, error is 150% or less of sample activity. If greater 10* MDA, error is 40% or less. If below the MDA, error is okay.	✓		
Instrument source check is within limits. Instrument bkg check is within limits.	✓		
Method RDL has been met.	✓		
If duplicate activities are less 5* MDA, then rpd is 100% or less. If greater 5* MDA, then rpd 20% or less. If below the MDA, the rpd is 0%. Or meets the client's required RER acceptance criteria.	✓		case narrative
Tracer yield is 15-125% . Carrier yield 25-125%. Or meets the client's contract acceptance criteria.	✓		
Method blank is less than the RDL. (If rad samples, < 5% of lowest activity)	✓		case narrative
Sample was run within hold time.	✓		
Special requirements page checked	✓		
Sample was correctly preserved if required.	✓		
Smears Taken for Radioactive batches.			N/A
Method Spike and LCS are within 75-125% or meets the client's contract acceptance criteria.	✓		
No blank spaces on data forms. All lineouts initialed and dated. No transcription errors are apparent.	✓		
QC data entered into QC database. Batch entered into Case Narrative.	✓		
Batch non-conformances completed If applicable.			N/A

General Engineering Laboratories

2/22/2006
Primary Review Performed By: Penelope Halley 04/8/06

Secondary Review Performed By: [Signature]

04/8-04/15

Thorium-228 Que Sheet

03-APR-06

Batch #: 517153 Analyst: LCW1 Minimum Due Date: 08-APR-06
 Tracer Isotope: Ac-227 Tracer Code: 081-0101 Expiration Date: 1/1/06
 LCS Isotope: Th-230 LCS Code: 01690 Expiration Date: 1/1/06
 Spike Isotope: Th-230 Spike Code: 01690 Expiration Date: 1/1/06
 Prep Date: 4/10/06 Initials: LWW Pipet ID: 2107545 Balance ID: 50410211
 Ac-227 Separation Date/Time: 4/11/06 11:00
 Witness: SLC YL-06

Sample I	Client Description	Type	Hazard Code	Min CRDL	Matrix	Client	Collection Date	Label #	Aliquot (g/L/F)	Th Det #	Ash Weight (g)
158269001	2603140361 M121-0.5	SAMPLE		1 pCi/g	SOIL	MWHL002	10-MAR-06	81	0.116	1	0.116
158269002	2603140362 M121-5	SAMPLE		1 pCi/g	SOIL	MWHL002	10-MAR-06	82	0.111	3	0.111
158269003	2603140364 M121-5D	SAMPLE		1 pCi/g	SOIL	MWHL002	10-MAR-06	83	0.111	4	0.116
158269004	2603140365 M121-80	SAMPLE		1 pCi/g	SOIL	MWHL002	10-MAR-06	84	0.111	5	0.114
158270001	2603100106 M118-0.5	SAMPLE		1 pCi/g	SOIL	MWHL002	08-MAR-06	85	0.117	7	0.111
158270002	2603100107 M118-5	SAMPLE		1 pCi/g	SOIL	MWHL002	08-MAR-06	86	0.104	9	0.108
158437001	2603150347 M119-0.5	SAMPLE		1 pCi/g	SOIL	MWHL002	14-MAR-06	87	0.106	10	0.105
158437002	2603150349 M119-0.5D	SAMPLE		1 pCi/g	SOIL	MWHL002	14-MAR-06	88	0.111	11	0.105
158437003	2603150350 M119-5	SAMPLE		1 pCi/g	SOIL	MWHL002	14-MAR-06	89	0.101	16	0.109
158437004	2603150352 M119-50	SAMPLE		1 pCi/g	SOIL	MWHL002	14-MAR-06	90	0.117	21	0.110
158438001	2603150303 M116-0.5	SAMPLE		1 pCi/g	SOIL	MWHL002	11-MAR-06	91	0.101	23	0.109
158438002	2603150304 M11600.5D	SAMPLE		1 pCi/g	SOIL	MWHL002	11-MAR-06	92	0.111	26	0.116
158438003	2603150305 M116-5	SAMPLE		1 pCi/g	SOIL	MWHL002	11-MAR-06	93	0.115	27	0.102
158438004	2603150307 M117-0.5	SAMPLE		1 pCi/g	SOIL	MWHL002	11-MAR-06	94	0.111	17	0.100
158438005	2603150308 M117-5	SAMPLE		1 pCi/g	SOIL	MWHL002	11-MAR-06	95	0.115	24	0.106
1201062927	MB for batch 517153	MB		1 pCi/g	SOIL	QC ACCOUNT		96	0.251	30	N/A
1201062928	2603140361 M121-0.5(158269001)DU	DUP		1 pCi/g	SOIL	QC ACCOUNT	10-MAR-06	97	0.105	32	0.100
1201062929	2603140361 M121-0.5(158269001)MS	MS		1 pCi/g	SOIL	QC ACCOUNT	10-MAR-06	98	0.105	34	0.109
1201062930	LCS for batch 517153	LCS		1 pCi/g	SOIL	QC ACCOUNT		99	0.251	18	N/A

Handwritten signature
4/11/06

Data Reviewed By: *Handwritten signature*
4/11/06

LEACH or DIGESTION
Circle One

Solid Sample Dissolution by: **LEACH or DIGESTION**
General Engineering Laboratories, Radiochemistry Division



Weight/Loss Aliquot Correction Report



Select What to Correct Aliquot to

Dry Weight Wet Weight

Batch ID: 517153

Aliquot Correction to Dry Weight for Batch 517153

Sample Id	Aliquot (G)	Sample Type	Parent Sample Id	Loss (Dec)	Corrected Aliquot (G)
158269001	.212	SAMPLE	NA	.0257	0.21759460
158269002	.222	SAMPLE	NA	.0386	0.23092117
158269003	.218	SAMPLE	NA	.0392	0.22691164
158269004	.214	SAMPLE	NA	.0352	0.22182665
158270001	.211	SAMPLE	NA	.0280	0.21708541
158270002	.198	SAMPLE	NA	.0280	0.20372448
158437001	.203	SAMPLE	NA	.0244	0.20808790
158437002	.205	SAMPLE	NA	.0279	0.21088368
158437003	.196	SAMPLE	NA	.0274	0.20152307
158437004	.210	SAMPLE	NA	.0304	0.21658415
158438001	.196	SAMPLE	NA	.0227	0.20056275
158438002	.215	SAMPLE	NA	.0263	0.22081785
158438003	.206	SAMPLE	NA	.0328	0.21300110
158438004	.206	SAMPLE	NA	.0213	0.21050402

PH 4/18/06

DD 4/10/06

158438005	.208	SAMPLE	NA	.0253	0.21340148
1201062927		MB	NA	NA	
1201062928	.200	DUP	158269001	.0257	0.20527793
1201062929	.198	MS	158269001	.0257	0.20322515
1201062930		LCS	NA	NA	

General Engineering Laboratories, LLC

04/18/06

Quinda

GENERAL ENGINEERING LABORATORIES, LLC.
ALPHA SPECTROSCOPY REPORT

BATCH NUMBER: 517153
SAMPLE DATE : 7-APR-2006 11:00:00.

SAMPLE ID : S0158269001_TH
SAMPLE QTY: 0.218 G

DETECTOR NUMBER :33088
AVERAGE %EFFICIENCY :27.8191
% YIELD : 80.055

COUNT DATE: 7-APR-2006 18:07:51
ELAPSED LIVE TIME(SEC): 14400.00
ANALYST :LCW1

MS : 0159-O
MSD : 0159-O
LCS : 0159-O
TRACER : 0387-B-102
BKG FILE: B001.CNF;687
BKG DATE: 2-APR-2006

MS PCI/G : 49.47609
MSD PCI/G : 49.47609
LCS PCI/G : 49.47609
TRACER DPM : 4.3582
EFF FILE : W001.CNF;233
CAL DATE: 3-APR-2006

MS ISOTOPE : TH-230
MSD ISOTOPE: TH-230
LCS ISOTOPE: TH-230
TRACER ISOTOPE: AC227
LIB FILE : ENV_ALPHA_TH.N

NUCLIDE ACTIVITY SUMMARY


NUCLIDE	ENERGY	NET AREA	BKG AREA	%ABUN	ACTIVITY pCi/G	ERROR 2-SIGMA	MDA pCi/G
AC-227	5978.000	125.760	0.240	54.75400	9.01E+00	2.38E+00	3.78E-01
TH-228	5363.000	78.640	3.360	99.94000	3.04E+00	9.21E-01	4.46E-01
TH229	4900.000	-1.160	2.160	99.52000	-4.51E-02	9.61E-02	3.82E-01
TH-230	4625.000	21.320	1.680	100.0000	8.24E-01	4.07E-01	3.49E-01
TH-232	3972.000	62.520	0.480	100.0000	2.42E+00	7.74E-01	2.41E-01

REVIEWED BY:

DATE :

Handwritten signature

Handwritten date: 4/18/06

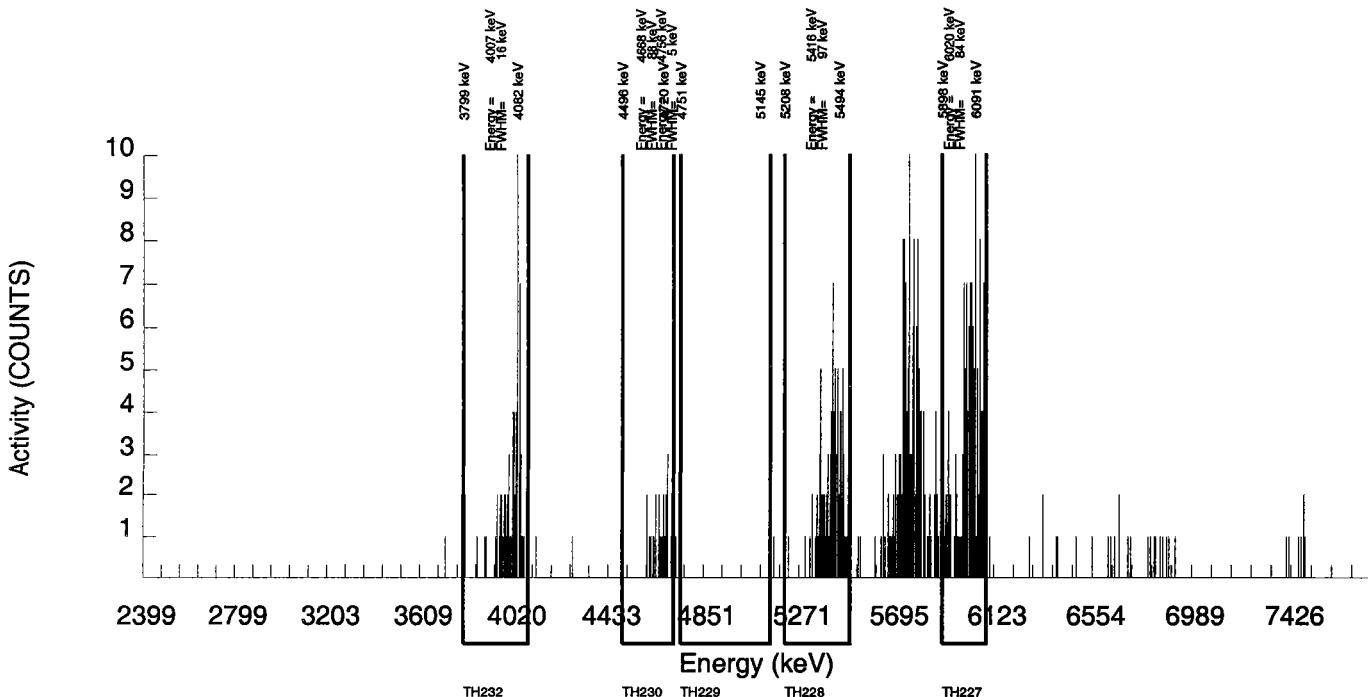

GENERAL ENGINEERING LABORATORIES, LLC.
ALPHA SPECTROSCOPY REPORT

BATCH NUMBER: 517153
SAMPLE DATE : 7-APR-2006 11:00:00.

SAMPLE ID : S0158269002_TH
SAMPLE QTY: 0.231 G

DETECTOR NUMBER :20659
AVERAGE %EFFICIENCY :28.8062
% YIELD : 118.500

COUNT DATE: 7-APR-2006 18:07:51
ELAPSED LIVE TIME(SEC): 14400.00
ANALYST :LCW1

MS : 0159-O
MSD : 0159-O
LCS : 0159-O
TRACER : 0387-B-102
BKG FILE: B003.CNF;676
BKG DATE: 2-APR-2006

MS PCI/G : 46.69172
MSD PCI/G : 46.69172
LCS PCI/G : 46.69172
TRACER DPM : 4.3582
EFF FILE : W003.CNF;192
CAL DATE: 3-APR-2006

MS ISOTOPE : TH-230
MSD ISOTOPE: TH-230
LCS ISOTOPE: TH-230
TRACER ISOTOPE: AC227
LIB FILE : ENV_ALPHA_TH.N


NUCLIDE ACTIVITY SUMMARY

NUCLIDE	ENERGY	NET AREA	BKG AREA	%ABUN	ACTIVITY pCi/G	ERROR 2-SIGMA	MDA pCi/G
AC-227	5978.000	192.760	0.240	54.75400	8.50E+00	1.85E+00	2.33E-01
TH-228	5363.000	50.920	4.080	99.94000	1.21E+00	4.08E-01	2.95E-01
TH229	4900.000	-1.880	2.880	99.52000	-4.50E-02	6.26E-02	2.60E-01
TH-230	4625.000	55.360	2.640	100.0000	1.32E+00	4.24E-01	2.51E-01
TH-232	3972.000	51.560	1.440	100.0000	1.23E+00	4.02E-01	2.04E-01

REVIEWED BY:

DATE :

PLH 4/18/06

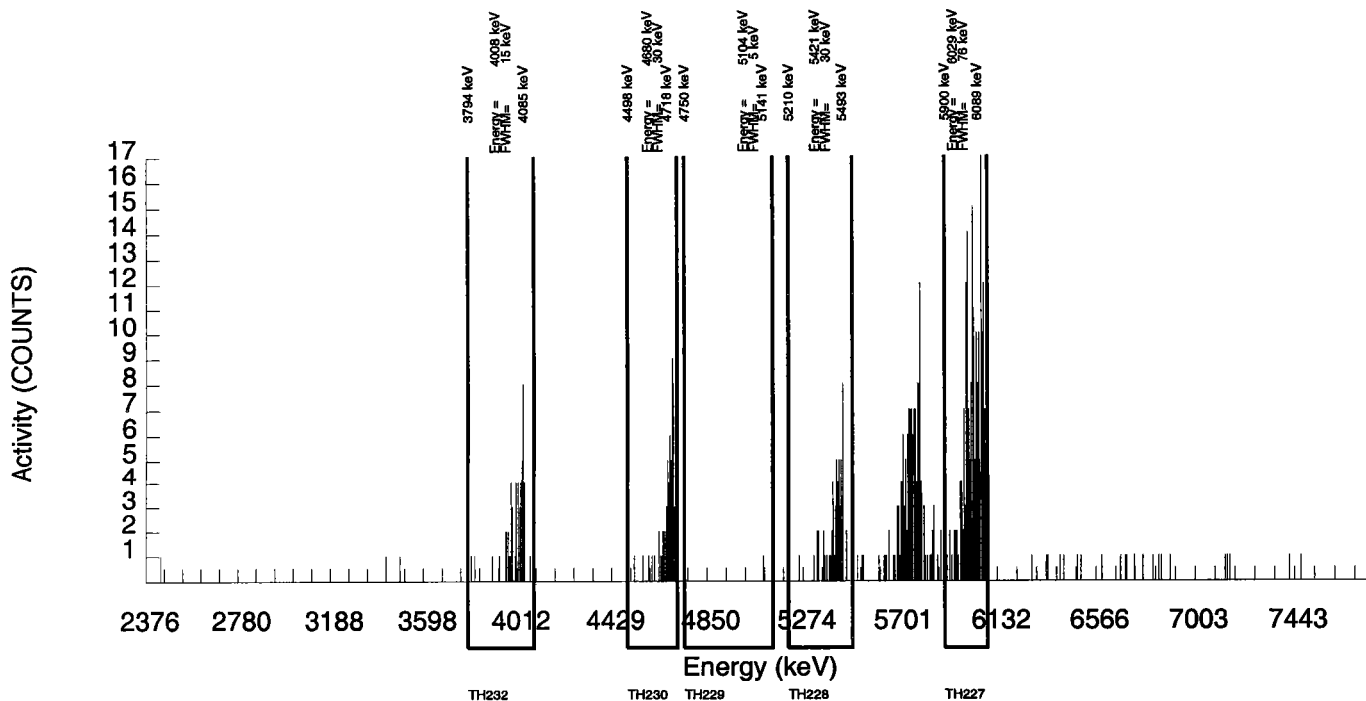

GENERAL ENGINEERING LABORATORIES, LLC.
ALPHA SPECTROSCOPY REPORT

BATCH NUMBER: 517153
SAMPLE DATE : 7-APR-2006 11:00:00.

SAMPLE ID : S0158269003_TH
SAMPLE QTY: 0.227 G

DETECTOR NUMBER :33077
AVERAGE %EFFICIENCY :30.9867
% YIELD : 65.173

COUNT DATE: 7-APR-2006 18:07:51
ELAPSED LIVE TIME(SEC): 14400.00
ANALYST :LCW1

MS : 0159-O
MSD : 0159-O
LCS : 0159-O
TRACER : 0387-B-102
BKG FILE: B004.CNF;685
BKG DATE: 2-APR-2006

MS PCI/G : 47.51448
MSD PCI/G : 47.51448
LCS PCI/G : 47.51448
TRACER DPM : 4.3582
EFF FILE : W004.CNF;184
CAL DATE: 3-APR-2006


MS ISOTOPE : TH-230
MSD ISOTOPE: TH-230
LCS ISOTOPE: TH-230
TRACER ISOTOPE: AC227
LIB FILE : ENV_ALPHA_TH.N

NUCLIDE ACTIVITY SUMMARY

NUCLIDE	ENERGY	NET AREA	BKG AREA	%ABUN	ACTIVITY pCi/G	ERROR 2-SIGMA	MDA pCi/G
AC-227	5978.000	114.040	0.960	54.75400	8.65E+00	2.40E+00	5.73E-01
TH-228	5363.000	41.640	3.360	99.94000	1.71E+00	6.55E-01	4.72E-01
TH229	4900.000	4.600	2.400	99.52000	1.89E-01	2.30E-01	4.20E-01
TH-230	4625.000	30.760	0.240	100.0000	1.26E+00	5.23E-01	2.16E-01
TH-232	3972.000	33.520	0.480	100.0000	1.37E+00	5.54E-01	2.55E-01

REVIEWED BY:

DATE : *PH 04/10/06*

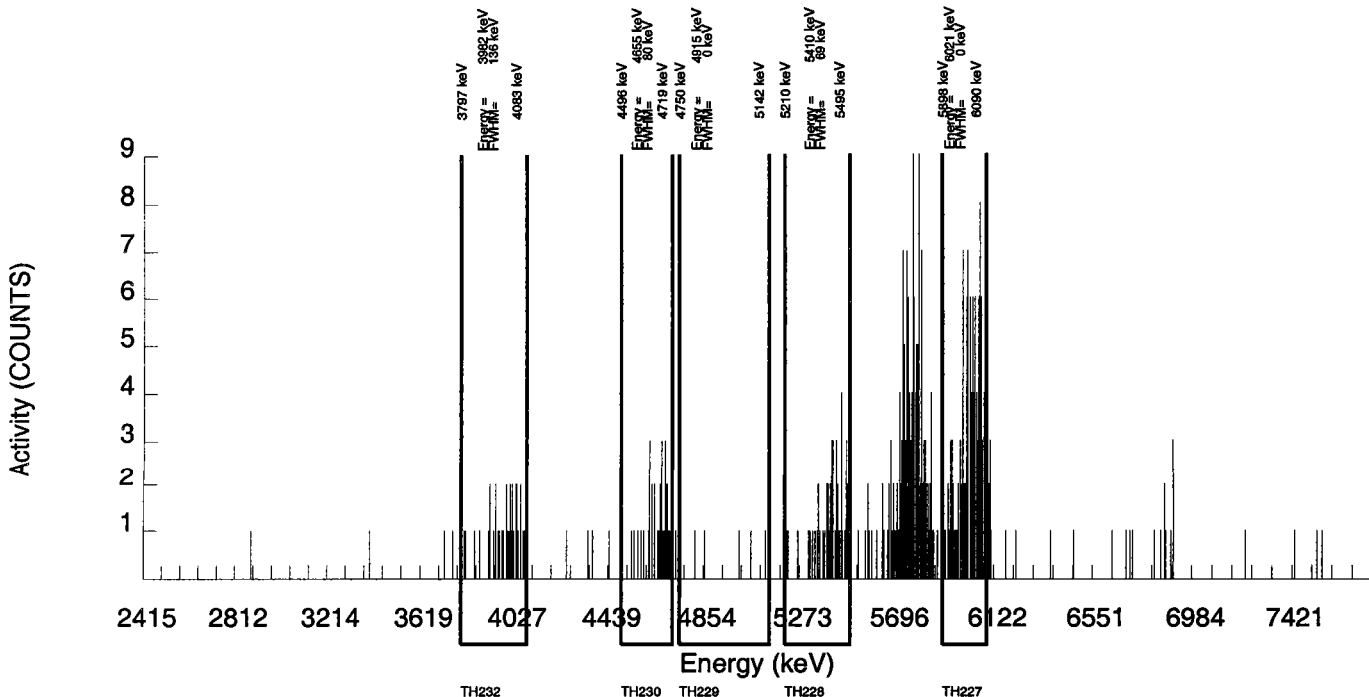

GENERAL ENGINEERING LABORATORIES, LLC.
ALPHA SPECTROSCOPY REPORT

BATCH NUMBER: 517153
SAMPLE DATE : 7-APR-2006 11:00:00.

SAMPLE ID : S0158269004_TH
SAMPLE QTY: 0.222 G

DETECTOR NUMBER :28642
AVERAGE %EFFICIENCY :31.5810
% YIELD : 116.096

COUNT DATE: 7-APR-2006 18:07:51
ELAPSED LIVE TIME(SEC): 14400.00
ANALYST :LCW1

MS : 0159-O
MSD : 0159-O
LCS : 0159-O
TRACER : 0387-B-102
BKG FILE: B005.CNF;673
BKG DATE: 2-APR-2006

MS PCI/G : 48.58463
MSD PCI/G : 48.58463
LCS PCI/G : 48.58463
TRACER DPM : 4.3582
EFF FILE : W005.CNF;190
CAL DATE: 3-APR-2006

MS ISOTOPE : TH-230
MSD ISOTOPE: TH-230
LCS ISOTOPE: TH-230
TRACER ISOTOPE: AC227
LIB FILE : ENV_ALPHA_TH.N


NUCLIDE ACTIVITY SUMMARY

NUCLIDE	ENERGY	NET AREA	BKG AREA	%ABUN	ACTIVITY pCi/G	ERROR 2-SIGMA	MDA pCi/G
AC-227	5978.000	207.040	0.960	54.75400	8.84E+00	1.87E+00	3.23E-01
TH-228	5363.000	54.080	7.920	99.94000	1.25E+00	4.19E-01	3.71E-01
TH229	4900.000	3.840	2.160	99.52000	8.90E-02	1.19E-01	2.28E-01
TH-230	4625.000	48.880	3.120	100.0000	1.13E+00	3.80E-01	2.59E-01
TH-232	3972.000	41.840	2.160	100.0000	9.65E-01	3.44E-01	2.27E-01

REVIEWED BY:

DATE :

JH 04/8/06

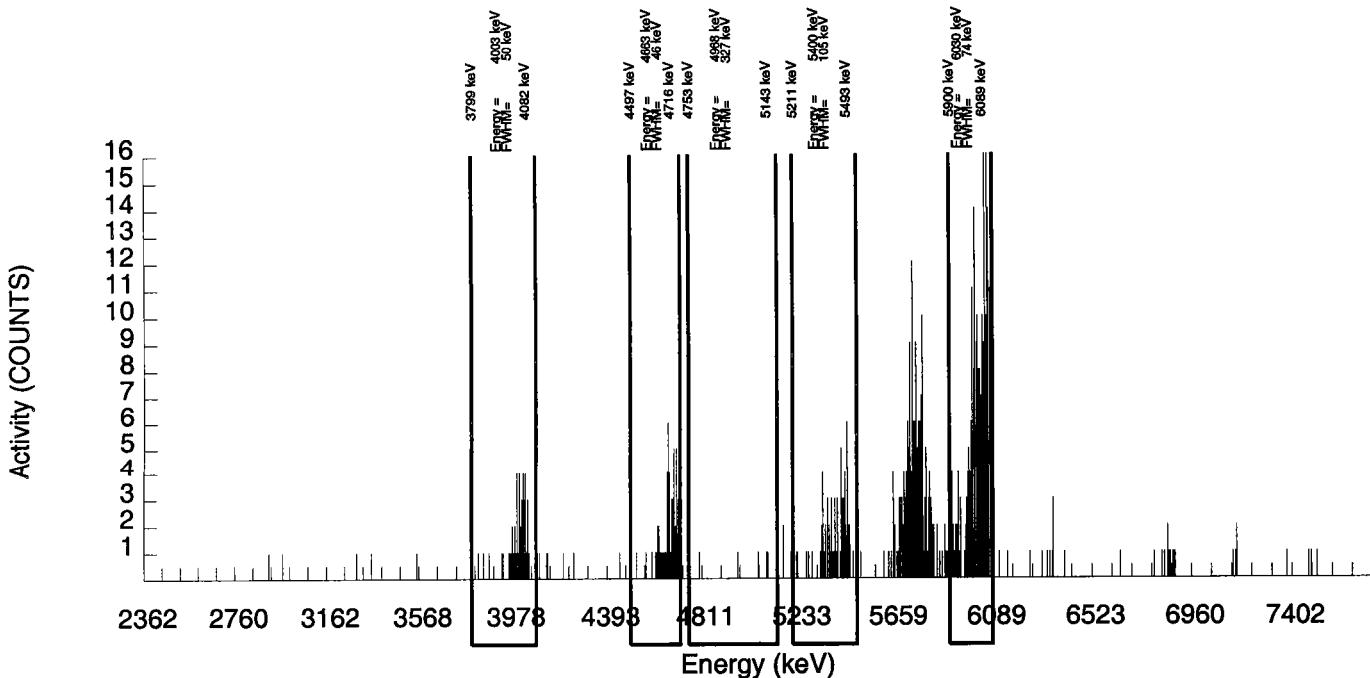

GENERAL ENGINEERING LABORATORIES, LLC.
ALPHA SPECTROSCOPY REPORT

BATCH NUMBER: 517153
SAMPLE DATE : 7-APR-2006 11:00:00.

SAMPLE ID : S1201062927_TH
SAMPLE QTY: 0.231 G

DETECTOR NUMBER :30420
AVERAGE %EFFICIENCY :30.3262
% YIELD : 113.145

COUNT DATE: 7-APR-2006 18:07:57
ELAPSED LIVE TIME(SEC): 14400.00
ANALYST :LCW1

MS : 0159-O
MSD : 0159-O
LCS : 0159-O
TRACER : 0387-B-102
BKG FILE: B030.CNF;686
BKG DATE: 2-APR-2006

MS PCI/G : 46.69172
MSD PCI/G : 46.69172
LCS PCI/G : 46.69172
TRACER DPM : 4.3582
EFF FILE : W030.CNF;200
CAL DATE: 4-APR-2006


MS ISOTOPE : TH-230
MSD ISOTOPE: TH-230
LCS ISOTOPE: TH-230
TRACER ISOTOPE: AC227
LIB FILE : ENV_ALPHA_TH.N

NUCLIDE ACTIVITY SUMMARY

NUCLIDE	ENERGY	NET AREA	BKG AREA	%ABUN	ACTIVITY pCi/G	ERROR 2-SIGMA	MDA pCi/G
AC-227	5978.000	193.760	0.240	54.75400	8.50E+00	1.79E+00	2.31E-01
TH-228	5363.000	11.160	3.840	99.94000	2.65E-01	1.93E-01	2.87E-01
TH229	4900.000	-0.400	2.400	99.52000	-9.52E-03	7.64E-02	2.43E-01
TH-230	4625.000	14.760	0.240	100.0000	3.50E-01	1.91E-01	1.25E-01
TH-232	3972.000	0.280	0.720	100.0000	6.63E-03	5.13E-02	1.64E-01

REVIEWED BY:

DATE :

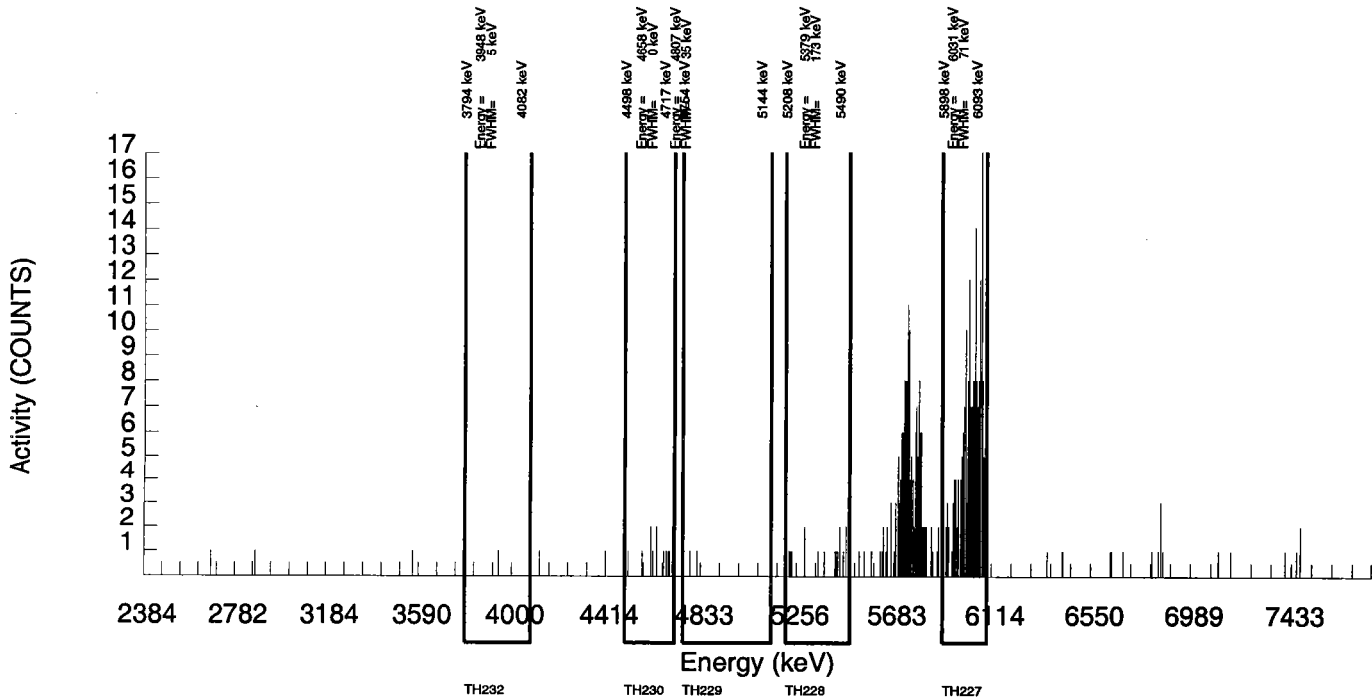

GENERAL ENGINEERING LABORATORIES, LLC.
ALPHA SPECTROSCOPY REPORT

BATCH NUMBER: 517153
SAMPLE DATE : 7-APR-2006 11:00:00.

SAMPLE ID : S1201062928_TH
SAMPLE QTY: 0.205 G

DETECTOR NUMBER :33207
AVERAGE %EFFICIENCY :32.1060
% YIELD : 107.711

COUNT DATE: 7-APR-2006 18:07:59
ELAPSED LIVE TIME(SEC): 14399.99
ANALYST :LCW1

MS : 0159-O
MSD : 0159-O
LCS : 0159-O
TRACER : 0387-B-102
BKG FILE: B032.CNF;697
BKG DATE: 2-APR-2006

MS PCI/G : 52.61360
MSD PCI/G : 52.61360
LCS PCI/G : 52.61360
TRACER DPM : 4.3582
EFF FILE : W032.CNF;242
CAL DATE: 4-APR-2006

MS ISOTOPE : TH-230
MSD ISOTOPE: TH-230
LCS ISOTOPE: TH-230
TRACER ISOTOPE: AC227
LIB FILE : ENV_ALPHA_TH.N


NUCLIDE ACTIVITY SUMMARY

NUCLIDE	ENERGY	NET AREA	BKG AREA	%ABUN	ACTIVITY pCi/G	ERROR 2-SIGMA	MDA pCi/G
AC-227	5978.000	195.280	0.720	54.75400	9.58E+00	2.10E+00	3.41E-01
TH-228	5363.000	66.920	10.080	99.94000	1.77E+00	5.56E-01	4.71E-01
TH229	4900.000	1.120	2.880	99.52000	2.98E-02	1.15E-01	2.90E-01
TH-230	4625.000	55.320	1.680	100.0000	1.46E+00	4.69E-01	2.39E-01
TH-232	3972.000	61.040	0.960	100.0000	1.62E+00	4.96E-01	2.00E-01

REVIEWED BY:

DATE :

RPD
 Th 228 = 39.8% act ~~54~~ MDA
 Th 230 = 55.7% act ~~54~~ MDA
 Th 232 = ~~39.6%~~ 39.6% act ~~54~~ MDA
 Th 228 Ref = 2.31
 Th 230 Ref = 2.01
 Th 232 Ref = 1.71

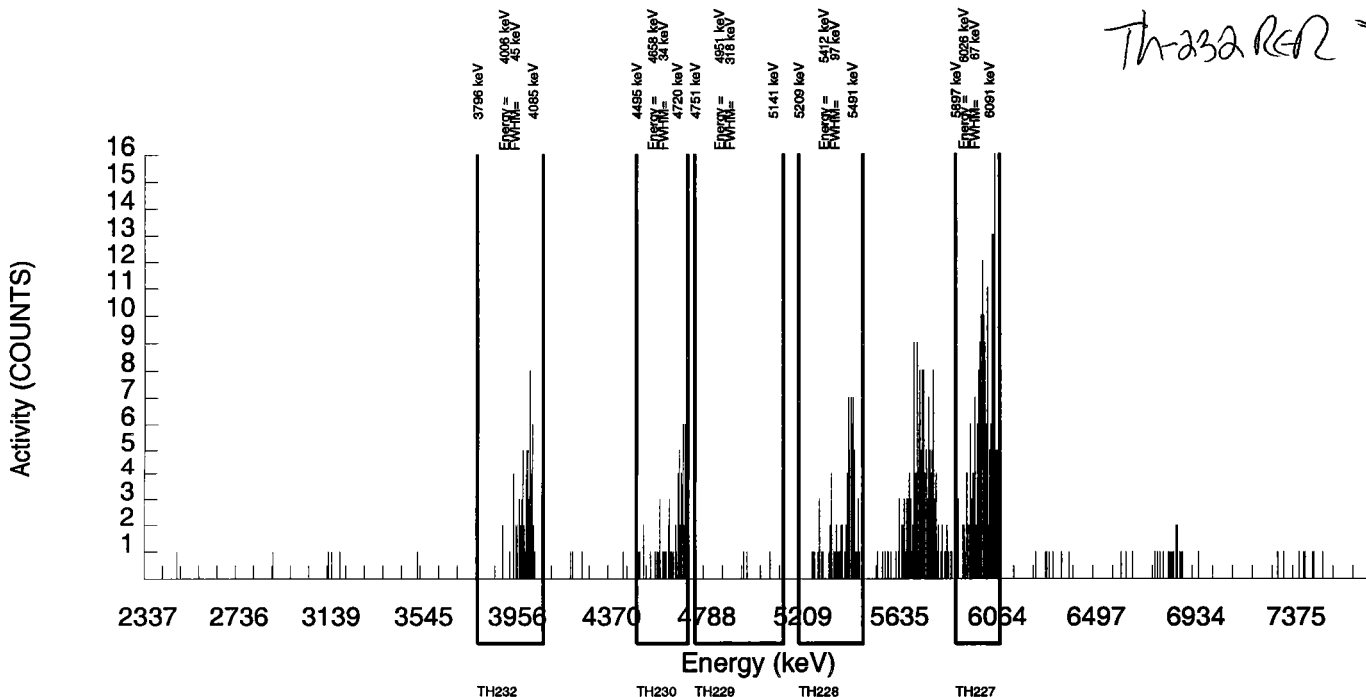

GENERAL ENGINEERING LABORATORIES, LLC.
ALPHA SPECTROSCOPY REPORT

BATCH NUMBER: 517153
SAMPLE DATE : 7-APR-2006 11:00:00.

SAMPLE ID : S1201062929_TH
SAMPLE QTY: 0.203 G

DETECTOR NUMBER :32697
AVERAGE %EFFICIENCY :32.8564
% YIELD : 105.273

COUNT DATE: 7-APR-2006 18:07:59
ELAPSED LIVE TIME(SEC): 14399.99
ANALYST :LCW1

MS : 0159-O
MSD : 0159-O
LCS : 0159-O
TRACER : 0387-B-102
BKG FILE: B034.CNF;686
BKG DATE: 2-APR-2006

MS PCI/G : 53.13196
MSD PCI/G : 53.13196
LCS PCI/G : 53.13196
TRACER DPM : 4.3582
EFF FILE : W034.CNF;217
CAL DATE: 4-APR-2006

MS ISOTOPE : TH-230
MSD ISOTOPE: TH-230
LCS ISOTOPE: TH-230
TRACER ISOTOPE: AC227
LIB FILE : ENV_ALPHA_TH.N

NUCLIDE ACTIVITY SUMMARY


NUCLIDE	ENERGY	NET AREA	BKG AREA	%ABUN	ACTIVITY pCi/G	ERROR 2-SIGMA	MDA pCi/G
AC-227	5978.000	195.320	1.680	54.75400	9.67E+00	2.12E+00	4.47E-01
TH-228	5363.000	76.280	6.720	99.94000	2.04E+00	5.97E-01	4.03E-01
TH229	4900.000	1.280	6.720	99.52000	3.44E-02	1.67E-01	4.04E-01
TH-230	4625.000	1727.400	3.600	100.0000	4.62E+01	7.98E+00	3.16E-01
TH-232	3972.000	86.640	3.360	100.0000	2.32E+00	6.38E-01	3.08E-01

REVIEWED BY:

DATE :

Handwritten signature

$$\frac{ms = 46.2 - .824}{53.1} = 85.4\%$$

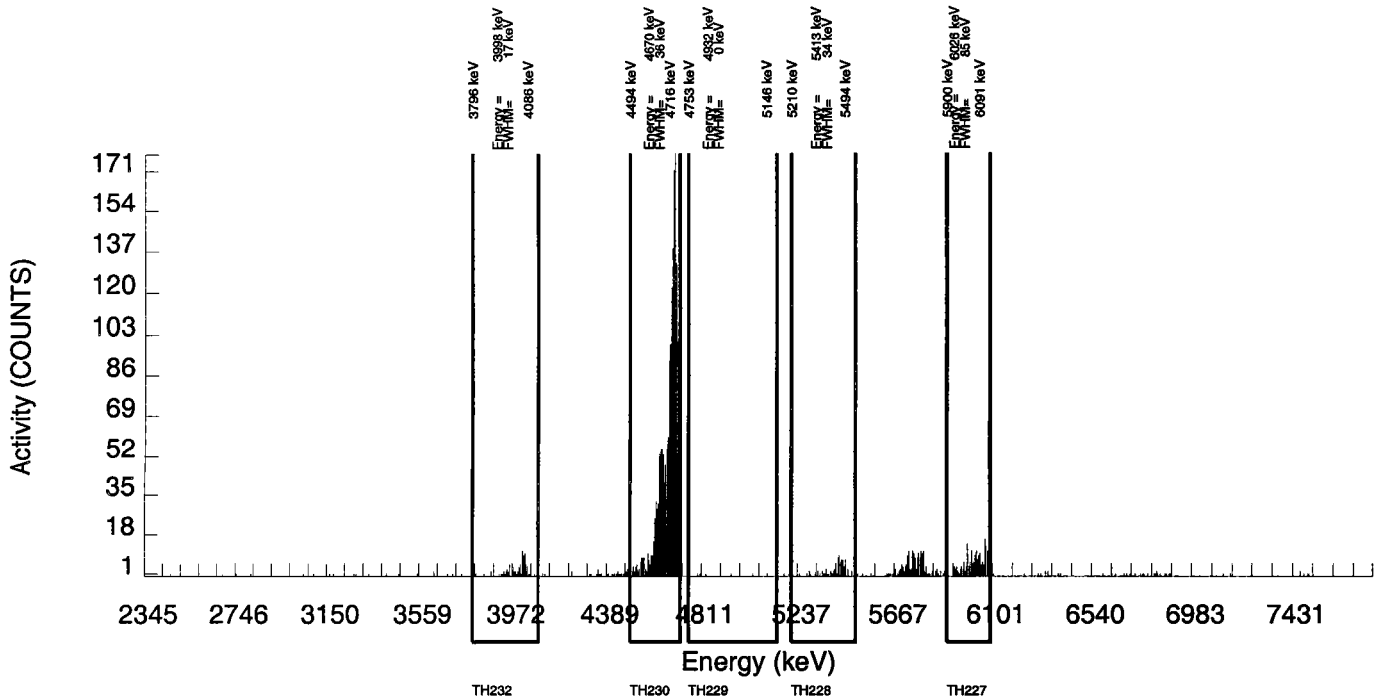

GENERAL ENGINEERING LABORATORIES, LLC.
ALPHA SPECTROSCOPY REPORT

BATCH NUMBER: 517153 SAMPLE DATE : 7-APR-2006 11:00:00.		SAMPLE ID : S1201062930_TH SAMPLE QTY: 0.231 G	
DETECTOR NUMBER :21063 AVERAGE %EFFICIENCY :25.5920 % YIELD : 90.256		COUNT DATE: 8-APR-2006 08:46:45 ELAPSED LIVE TIME(SEC): 14399.99 ANALYST :LCW1	
MS : 0159-O MSD : 0159-O LCS : 0159-O TRACER : 0387-B-102 BKG FILE: B018.CNF;666 BKG DATE: 2-APR-2006		MS PCI/G : 46.69172 MSD PCI/G : 46.69172 LCS PCI/G : 46.69172 TRACER DPM : 4.3582 EFF FILE : W018.CNF;190 CAL DATE: 3-APR-2006	
		MS ISOTOPE : TH-230 MSD ISOTOPE: TH-230 LCS ISOTOPE: TH-230 TRACER ISOTOPE: AC227 LIB FILE : ENV_ALPHA_TH.N	

NUCLIDE ACTIVITY SUMMARY


NUCLIDE	ENERGY	NET AREA	BKG AREA	%ABUN	ACTIVITY pCi/G	ERROR 2-SIGMA	MDA pCi/G
AC-227	5978.000	127.520	0.480	54.75400	8.50E+00	2.23E+00	4.15E-01
TH-228	5363.000	-1.280 ✓	5.280	99.94000	-4.51E-02	1.62E-01	4.82E-01
TH229	4900.000	1.080	1.920	99.52000	3.82E-02	1.32E-01	3.34E-01
TH-230	4625.000	1134.760	0.240	100.0000	3.99E+01	8.09E+00	1.86E-01
TH-232	3972.000	6.760	0.240	100.0000	2.38E-01	1.93E-01	1.86E-01

REVIEWED BY:

DATE:

gwd4/10/06

py4/18/06
 $LCS = \frac{39.9}{46.7} = 85.4\%$

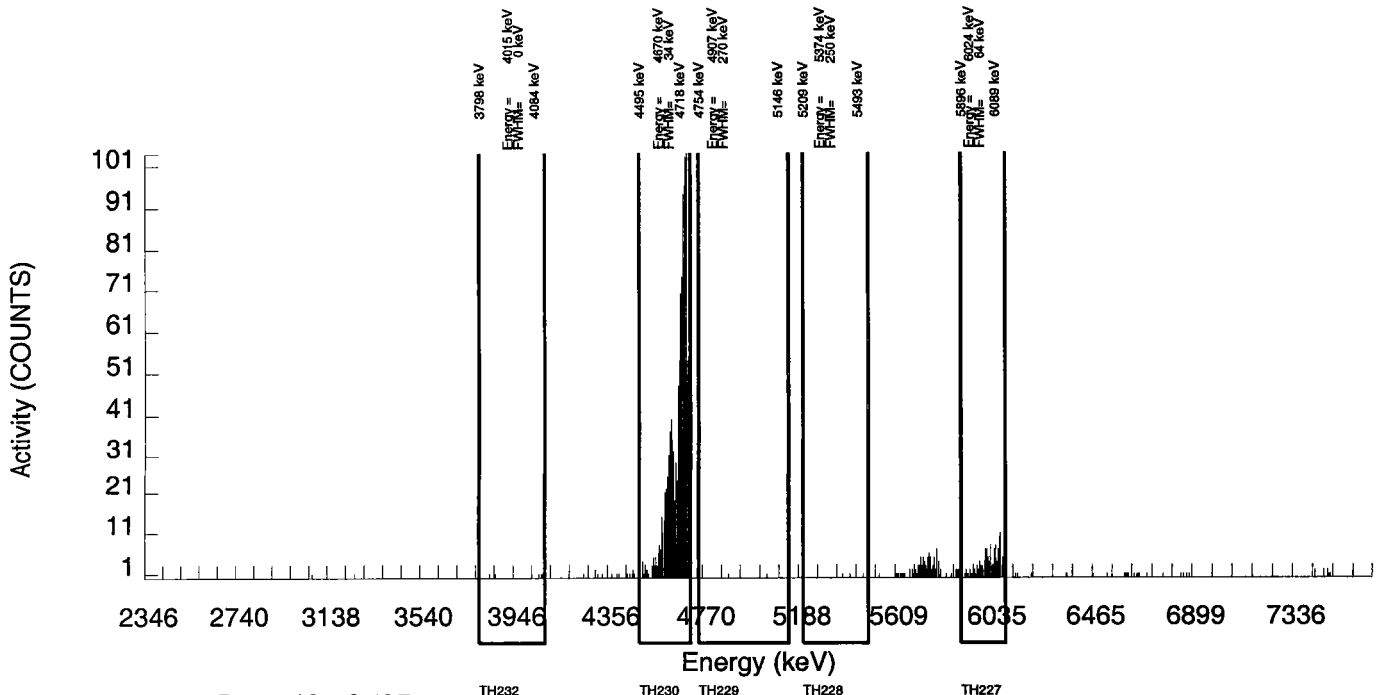

Radiochemistry Batch Checklist, Rev 4

Batch# 517155 Product: U Date: 4/10/06

Criteria:	Yes	No	Comments
Sample Solids are less than 100 mg for GAB.			NA
If activity less 10* MDA, error is 150% or less of sample activity. If greater 10* MDA, error is 40% or less. If below the MDA, error is okay.	/		
Instrument source check is within limits.	/		
Instrument bkg check is within limits.	/		
Method RDL has been met.	/		
If duplicate activities are less 5* MDA, then rpd is 100% or less. If greater 5* MDA, then rpd 20% or less. If below the MDA, the rpd is 0%.	/		
Or meets the client's required RER acceptance criteria.	/		
Tracer yield is 15-125% . Carrier yield 25-125%.	/		
Or meets the client's contract acceptance criteria.	/		
Method blank is less than the RDL. (If rad samples, < 5% of lowest activity)	/		
Sample was run within hold time.	/		
Special requirements page checked	/		
Sample was correctly preserved if required.	/		
Smears Taken for Radioactive batches.			NA
Method Spike and LCS are within 75-125% or meets the client's contract acceptance criteria.	/		
No blank spaces on data forms.	/		
All lineouts initialed and dated.	/		
No transcription errors are apparent.	/		
QC data entered into QC database.	/		
Batch entered into Case Narrative.	/		
Batch non-conformances completed If applicable.			NA

General Engineering Laboratories

2/22/2005
Primary Review Performed By: Carson 4/10/06

Secondary Review Performed By: Paralel Kelley 04/10/06

3/8 - 3/19

MWHL

Uranium Que Sheet

03-APR-06

Batch #: 517155 Analyst: LCW1 Minimum Due Date: 08-APR-06
 Tracer Isotope: U-232/U-236 Tracer Code: 006004 Expiration Date: 11/1/07 Vol: 0.1
 LCS Isotope: U-238 LCS Code: 089800 Expiration Date: 11/21/00 Vol: 0.1
 Spike Isotope: U-238 Spike Code: 089800 Expiration Date: 11/21/00 Vol: 0.1
 Prep Date: 4/6/06 Initials: LW Pipet ID: 50410211 Balance ID: 50410211

Witness: SLG 4-6-06

Sample ID	Client Description	Type	Hazard Code	Min CRDL	Matrix	Client	Collection Date	Label #	Aliquot (g/1/f)	U Det #	Ash Weight (g)
158269001	2603140361 M121-0.5	SAMPLE		1 pCi/g	SOIL	MWHL002	10-MAR-06	81	0.118	32	0.114
158269002	2603140362 M121-5	SAMPLE		1 pCi/g	SOIL	MWHL002	10-MAR-06	82	0.111	33	0.114
158269003	2603140364 M121-5D	SAMPLE		1 pCi/g	SOIL	MWHL002	10-MAR-06	83	0.117	34	0.118
158269004	2603140365 M121-80	SAMPLE		1 pCi/g	SOIL	MWHL002	10-MAR-06	84	0.114	37	0.114
158270001	2603100106 M118-0.5	SAMPLE		1 pCi/g	SOIL	MWHL002	08-MAR-06	85	0.117	38	0.111
158270002	2603100107 M118-5	SAMPLE		1 pCi/g	SOIL	MWHL002	08-MAR-06	86	0.104	40	0.108
158437001	2603150347 M119-0.5	SAMPLE		1 pCi/g	SOIL	MWHL002	14-MAR-06	87	0.106	41	0.105
158437002	2603150349 M119-0.5D	SAMPLE		1 pCi/g	SOIL	MWHL002	14-MAR-06	88	0.111	42	0.105
158437003	2603150350 M119-5	SAMPLE		1 pCi/g	SOIL	MWHL002	14-MAR-06	89	0.104	43	0.106
158437004	2603150352 M119-50	SAMPLE		1 pCi/g	SOIL	MWHL002	14-MAR-06	90	0.117	44	0.110
158438001	2603150303 M116-0.5	SAMPLE		1 pCi/g	SOIL	MWHL002	11-MAR-06	91	0.101	45	0.106
158438002	2603150304 M11600-5D	SAMPLE		1 pCi/g	SOIL	MWHL002	11-MAR-06	92	0.111	45	0.115
158438003	2603150305 M116-5	SAMPLE		1 pCi/g	SOIL	MWHL002	11-MAR-06	93	0.113	47	0.100
158438004	2603150307 M117-0.5	SAMPLE		1 pCi/g	SOIL	MWHL002	11-MAR-06	94	0.111	48	0.100
158438005	2603150308 M117-5	SAMPLE		1 pCi/g	SOIL	MWHL002	11-MAR-06	96	0.113	77	0.108
1201062931	MB for batch 517155	MB		1 pCi/g	SOIL	QC ACCOUNT		90	0.231	78	NA
1201062932	2603140361 M121-0.5(158269001)DU	DUP		1 pCi/g	SOIL	QC ACCOUNT	10-MAR-06	91	0.106	79	0.100
1201062933	2603140361 M121-0.5(158269001)MS	MS		1 pCi/g	SOIL	QC ACCOUNT	10-MAR-06	98	0.103	80	0.108
1201062934	LCS for batch 517155	LCS		1 pCi/g	SOIL	QC ACCOUNT		99	0.231	81	NA

Choose SOP used: GL-RAD-A-011
GL-RAD-A-038
GL-RAD-A-045
 GL-RAD-A-043

Solid Sample Dissolution by: LEACH or DIGESTION
 Circle One

Data Reviewed By: Paula y/10/06



Weight/Loss Aliquot Correction Report



Select What to Correct Aliquot to

Dry Weight Wet Weight

Submit

Batch ID: 517155

Calculate Corrected Aliquot

Aliquot Correction to Dry Weight for Batch 517153

Sample Id	Aliquot (G)	Sample Type	Parent Sample Id	Loss (Dec)	Corrected Aliquot (G)
158269001	.212	SAMPLE	NA	.0257	0.21759460
158269002	.222	SAMPLE	NA	.0386	0.23092117
158269003	.218	SAMPLE	NA	.0392	0.22691164
158269004	.214	SAMPLE	NA	.0352	0.22182665
158270001	.211	SAMPLE	NA	.0280	0.21708541
158270002	.198	SAMPLE	NA	.0280	0.20372448
158437001	.203	SAMPLE	NA	.0244	0.20808790
158437002	.205	SAMPLE	NA	.0279	0.21088368
158437003	.196	SAMPLE	NA	.0274	0.20152307
158437004	.210	SAMPLE	NA	.0304	0.21658415
158438001	.196	SAMPLE	NA	.0227	0.20056275
158438002	.215	SAMPLE	NA	.0263	0.22081785
158438003	.206	SAMPLE	NA	.0328	0.21300110
158438004	.206	SAMPLE	NA	.0213	0.21050402

Handwritten signature

Handwritten signature

158438005	.208	SAMPLE	NA	.0253	0.21340148
1201062927		MB	NA	NA	
1201062928	.200	DUP	158269001	.0257	0.20527793
1201062929	.198	MS	158269001	.0257	0.20322515
1201062930		LCS	NA	NA	

General Engineering Laboratories, LLC

pg 41/106

PLM

GENERAL ENGINEERING LABORATORIES, LLC.
ALPHA SPECTROSCOPY REPORT

BATCH NUMBER: 517155 SAMPLE DATE : 10-MAR-2006 00:00:00		SAMPLE ID : S0158269001_UU SAMPLE QTY: 0.218 G	
DETECTOR NUMBER :33207 AVERAGE %EFFICIENCY :32.1060 % YIELD : 81.934		COUNT DATE: 8-APR-2006 15:43:12 ELAPSED LIVE TIME(SEC): 14400.00 ANALYST :LCW1	
MS : 0858-B MSD : 0858-B LCS : 0858-B TRACER : 0688-H BKG FILE: B032.CNF;697 BKG DATE: 2-APR-2006		MS PCI/G : 12.06122 MSD PCI/G : 12.06122 LCS PCI/G : 12.06122 TRACER DPM : 5.4124 EFF FILE : W032.CNF;242 CAL DATE: 4-APR-2006	
		MS ISOTOPE : U-238 MSD ISOTOPE: U-238 LCS ISOTOPE: U-238 TRACER ISOTOPE: U232 LIB FILE : ENV_ALPHA_UU.N	


NUCLIDE ACTIVITY SUMMARY

NUCLIDE	ENERGY	NET AREA	BKG AREA	%ABUN	ACTIVITY pCi/G	TPU 1.96-SIGMA	MDA pCi/G	UNC pCi/G
U-3/4	4763.020	24.560	1.440	100.0000	8.04E-01	3.51E-01	2.81E-01	3.29E-01
U232	5302.100	341.440	4.560	100.0000	1.12E+01	2.08E+00	4.24E-01	1.20E+00
U-235	4391.000	4.000	0.000	80.90000	1.62E-01	1.60E-01	1.21E-01	1.59E-01
U-238	4184.730	37.040	0.960	100.0000	1.21E+00	4.37E-01	2.47E-01	3.97E-01

REVIEWED BY:

DATE: *DH 4/11/06*

AD 4/11/06

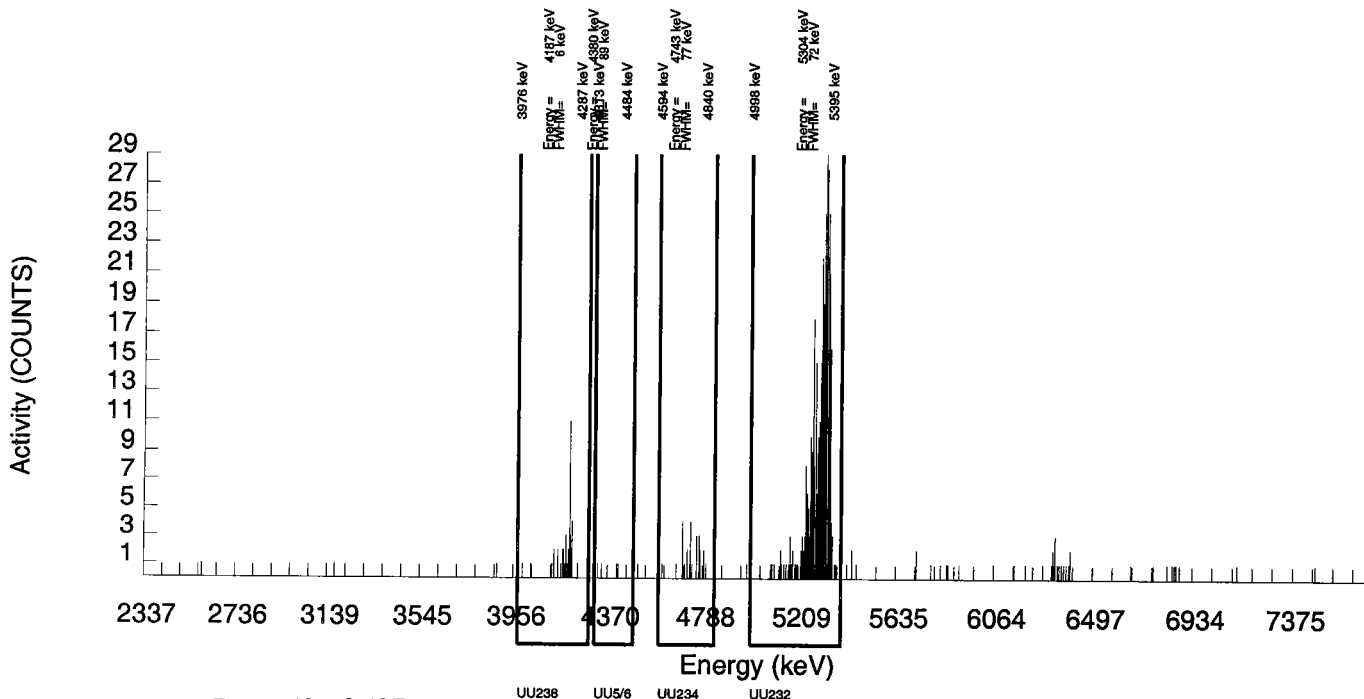

GENERAL ENGINEERING LABORATORIES, LLC.
ALPHA SPECTROSCOPY REPORT

BATCH NUMBER: 517155 SAMPLE DATE : 10-MAR-2006 00:00:00		SAMPLE ID : S0158269002_UU SAMPLE QTY: 0.231 G	
DETECTOR NUMBER :28647 AVERAGE %EFFICIENCY :31.8935 % YIELD : 70.866		COUNT DATE: 8-APR-2006 15:43:12 ELAPSED LIVE TIME(SEC): 14400.00 ANALYST :LCW1	
MS : 0858-B MSD : 0858-B LCS : 0858-B TRACER : 0688-H BKG FILE: B033.CNF;686 BKG DATE: 2-APR-2006	MS PCI/G : 11.38245 MSD PCI/G : 11.38245 LCS PCI/G : 11.38245 TRACER DPM : 5.4124 EFF FILE : W033.CNF;217 CAL DATE: 4-APR-2006	MS ISOTOPE : U-238 MSD ISOTOPE: U-238 LCS ISOTOPE: U-238 TRACER ISOTOPE: U232 LIB FILE : ENV_ALPHA_UU.N	


NUCLIDE ACTIVITY SUMMARY

NUCLIDE	ENERGY	NET AREA	BKG AREA	%ABUN	ACTIVITY pCi/G	TPU 1.96-SIGMA	MDA pCi/G	UNC pCi/G
U-3/4	4763.020	49.800	1.200	100.0000	1.79E+00	5.79E-01	2.91E-01	5.05E-01
U232	5302.100	293.360	8.640	100.0000	1.06E+01	2.08E+00	6.00E-01	1.23E+00
U-235	4391.000	2.000	0.000	80.90000	8.89E-02	1.24E-01	1.33E-01	1.23E-01
U-238	4184.730	34.040	0.960	100.0000	1.22E+00	4.61E-01	2.72E-01	4.18E-01

REVIEWED BY:

DATE: *2006 4/11/06*

LCW

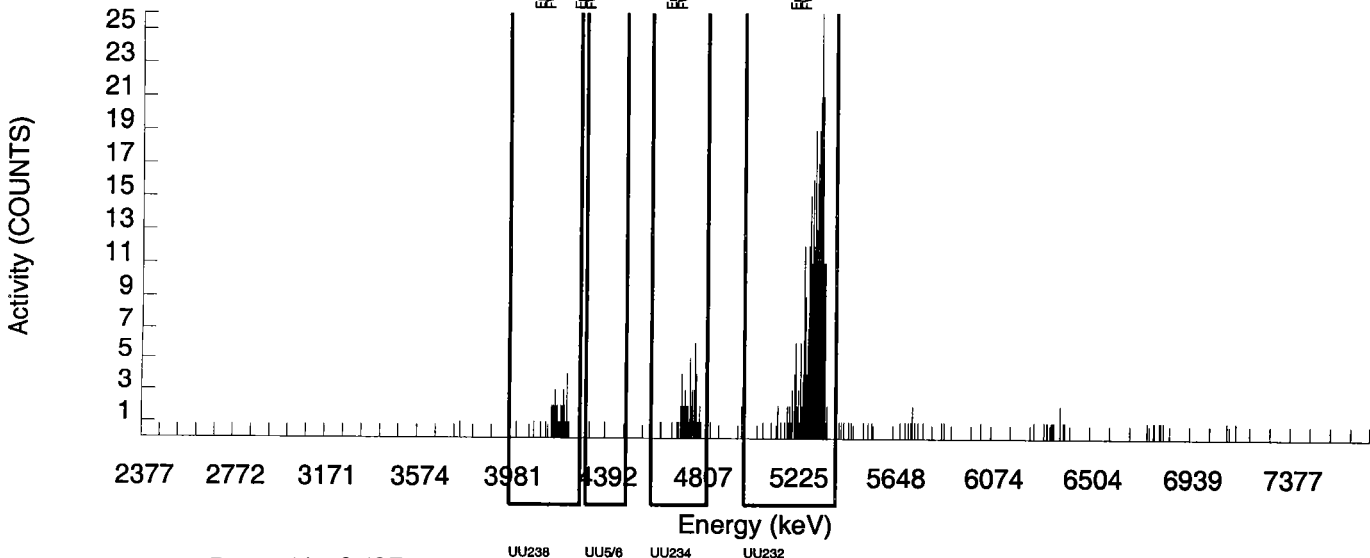

GENERAL ENGINEERING LABORATORIES, LLC.
ALPHA SPECTROSCOPY REPORT

BATCH NUMBER: 517155 SAMPLE DATE : 10-MAR-2006 00:00:00		SAMPLE ID : S0158269003_UU SAMPLE QTY: 0.227 G	
DETECTOR NUMBER :32697 AVERAGE %EFFICIENCY :32.8564 % YIELD : 78.281		COUNT DATE: 8-APR-2006 15:43:12 ELAPSED LIVE TIME(SEC): 14400.00 ANALYST :LCW1	
MS : 0858-B MSD : 0858-B LCS : 0858-B TRACER : 0688-H BKG FILE: B034.CNF;686 BKG DATE: 2-APR-2006	MS PCI/G : 11.58303 MSD PCI/G : 11.58303 LCS PCI/G : 11.58303 TRACER DPM : 5.4124 EFF FILE : W034.CNF;217 CAL DATE: 4-APR-2006	MS ISOTOPE : U-238 MSD ISOTOPE: U-238 LCS ISOTOPE: U-238 TRACER ISOTOPE: U232 LIB FILE : ENV_ALPHA_UU.N	

NUCLIDE ACTIVITY SUMMARY


NUCLIDE	ENERGY	NET AREA	BKG AREA	%ABUN	ACTIVITY pCi/G	TPU 1.96-SIGMA	MDA pCi/G	UNC pCi/G
U-3/4	4763.020	45.880	3.120	100.0000	1.47E+00	4.98E-01	3.60E-01	4.44E-01
U232	5302.100	333.840	8.160	100.0000	1.07E+01	2.02E+00	5.24E-01	1.17E+00
U-235	4391.000	2.800	1.200	80.90000	1.11E-01	1.62E-01	3.22E-01	1.61E-01
U-238	4184.730	21.440	4.560	100.0000	6.89E-01	3.44E-01	4.16E-01	3.28E-01

REVIEWED BY:

DATE :

Handwritten signature

Handwritten date: 24 04/11/06

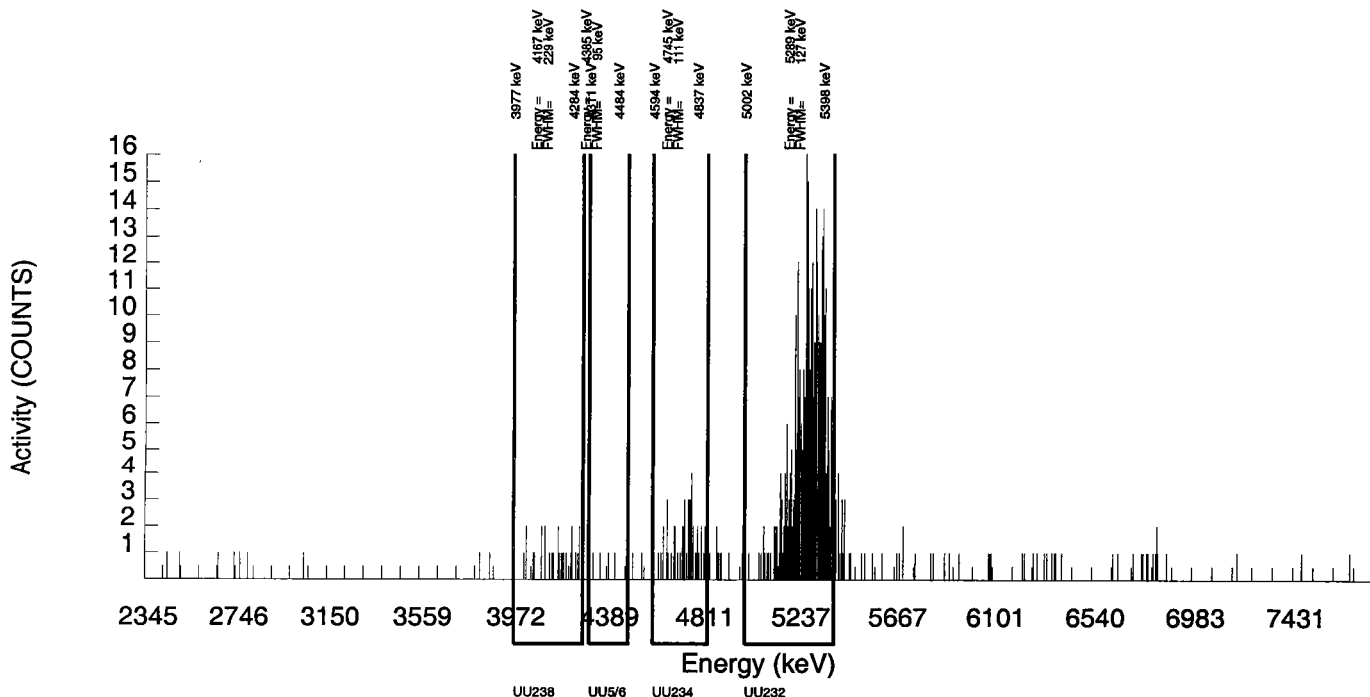

GENERAL ENGINEERING LABORATORIES, LLC.
ALPHA SPECTROSCOPY REPORT

BATCH NUMBER: 517155 SAMPLE DATE : 10-MAR-2006 00:00:00		SAMPLE ID : S0158269004_UU SAMPLE QTY: 0.222 G	
DETECTOR NUMBER :32690 AVERAGE %EFFICIENCY :32.9828 % YIELD : 90.081		COUNT DATE: 8-APR-2006 15:43:13 ELAPSED LIVE TIME(SEC): 14399.99 ANALYST :LCW1	
MS : 0858-B MSD : 0858-B LCS : 0858-B TRACER : 0688-H BKG FILE: B037.CNF;689 BKG DATE: 2-APR-2006		MS PCI/G : 11.84390 MSD PCI/G : 11.84390 LCS PCI/G : 11.84390 TRACER DPM : 5.4124 EFF FILE : W037.CNF;206 CAL DATE: 4-APR-2006	
		MS ISOTOPE : U-238 MSD ISOTOPE: U-238 LCS ISOTOPE: U-238 TRACER ISOTOPE: U232 LIB FILE : ENV_ALPHA_UU.N	

NUCLIDE ACTIVITY SUMMARY

NUCLIDE	ENERGY	NET AREA	BKG AREA	%ABUN	ACTIVITY pCi/G	TPU 1.96-SIGMA	MDA pCi/G	UNC pCi/G
U-3/4	4763.020	32.120	2.880	100.0000	9.14E-01	3.55E-01	3.10E-01	3.33E-01
U232	5302.100	385.640	3.360	100.0000	1.10E+01	1.84E+00	3.28E-01	1.10E+00
U-235	4391.000	5.280	0.720	80.90000	1.86E-01	1.73E-01	2.44E-01	1.71E-01
U-238	4184.730	31.800	1.200	100.0000	9.05E-01	3.44E-01	2.30E-01	3.22E-01


REVIEWED BY:

DATE:

Handwritten signature

Handwritten date: 7/4/10

Activity (COUNTS)

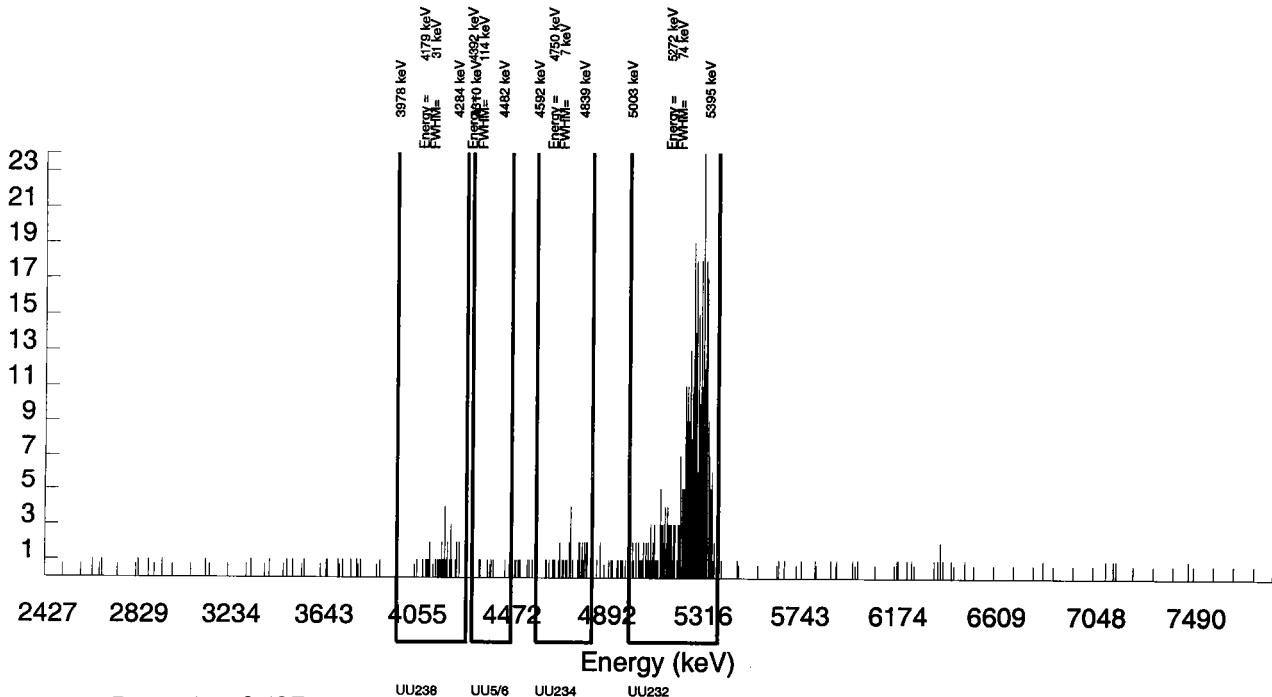

GENERAL ENGINEERING LABORATORIES, LLC.
ALPHA SPECTROSCOPY REPORT

BATCH NUMBER: 517155
SAMPLE DATE : 6-APR-2006 00:00:00.

SAMPLE ID : S1201062931_UU
SAMPLE QTY: 0.231 G

DETECTOR NUMBER :34425
AVERAGE %EFFICIENCY :32.6623
% YIELD : 93.135

COUNT DATE: 8-APR-2006 15:43:20
ELAPSED LIVE TIME(SEC): 14400.00
ANALYST :LCW1

MS : 0858-B
MSD : 0858-B
LCS : 0858-B
TRACER : 0688-H
BKG FILE: B078.CNF;598
BKG DATE: 2-APR-2006

MS PCI/G : 11.38245
MSD PCI/G : 11.38245
LCS PCI/G : 11.38245
TRACER DPM : 5.4086
EFF FILE : W078.CNF;154
CAL DATE: 3-APR-2006


MS ISOTOPE : U-238
MSD ISOTOPE: U-238
LCS ISOTOPE: U-238
TRACER ISOTOPE: U232
LIB FILE : ENV_ALPHA_UU.N

NUCLIDE ACTIVITY SUMMARY

NUCLIDE	ENERGY	NET AREA	BKG AREA	%ABUN	ACTIVITY pCi/G	TPU 1.96-SIGMA	MDA pCi/G	UNC pCi/G
U-3/4	4763.020	5.560	1.440	100.0000	1.49E-01	1.43E-01	2.29E-01	1.42E-01
U232	5302.100	394.840	2.160	100.0000	1.05E+01	1.74E+00	2.63E-01	1.04E+00
U-235	4391.000	-0.720	0.720	80.90000	-2.38E-02	2.71E-02	2.29E-01	2.69E-02
U-238	4184.730	1.520	0.480	100.0000	4.06E-02	7.63E-02	1.66E-01	7.61E-02

REVIEWED BY:

DATE: 7/4/06/11/06

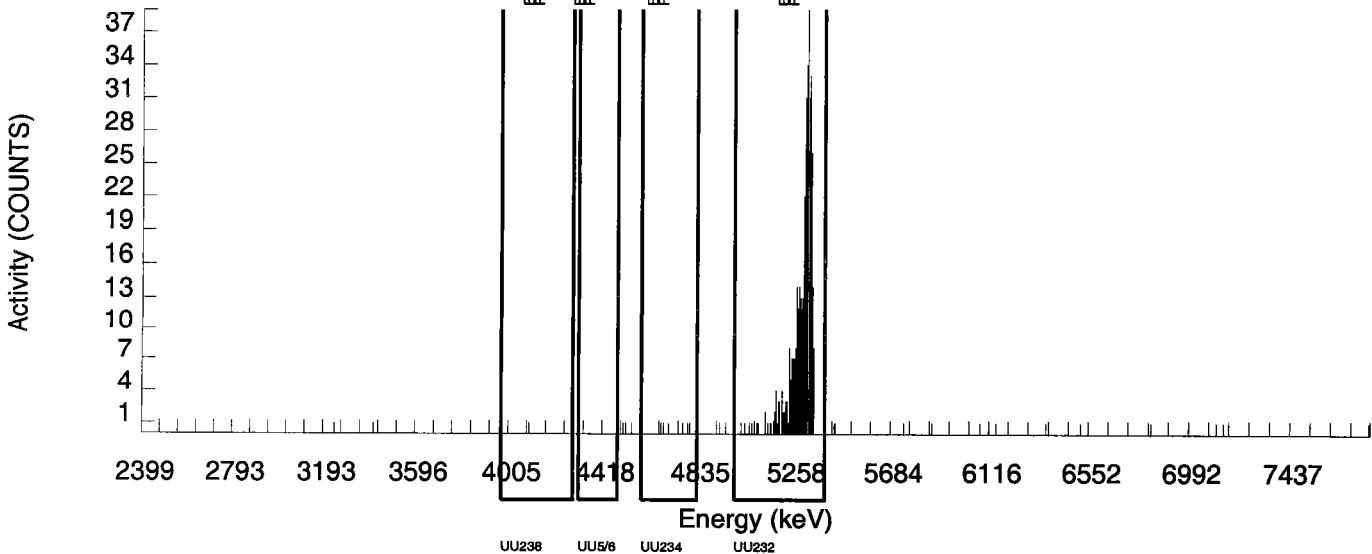

GENERAL ENGINEERING LABORATORIES, LLC.
ALPHA SPECTROSCOPY REPORT

BATCH NUMBER: 517155 SAMPLE DATE : 10-MAR-2006 00:00:00		SAMPLE ID : S1201062932_UU SAMPLE QTY: 0.205 G	
DETECTOR NUMBER :28408 AVERAGE %EFFICIENCY :33.8151 % YIELD : 69.062		COUNT DATE: 8-APR-2006 15:43:20 ELAPSED LIVE TIME(SEC): 14400.00 ANALYST :LCW1	
MS : 0858-B MSD : 0858-B LCS : 0858-B TRACER : 0688-H BKG FILE: B079.CNF;596 BKG DATE: 2-APR-2006		MS PCI/G : 12.82608 MSD PCI/G : 12.82608 LCS PCI/G : 12.82608 TRACER DPM : 5.4124 EFF FILE : W079.CNF;154 CAL DATE: 3-APR-2006	
		MS ISOTOPE : U-238 MSD ISOTOPE: U-238 LCS ISOTOPE: U-238 TRACER ISOTOPE: U232 LIB FILE : ENV_ALPHA_UU.N	

NUCLIDE ACTIVITY SUMMARY

NUCLIDE	ENERGY	NET AREA	BKG AREA	%ABUN	ACTIVITY pCi/G	TPU 1.96-SIGMA	MDA pCi/G	UNC pCi/G
U-3/4	4763.020	37.040	0.960	100.0000	1.45E+00	5.19E-01	2.96E-01	4.75E-01
U232	5302.100	303.120	2.880	100.0000	1.19E+01	2.18E+00	4.27E-01	1.35E+00
U-235	4391.000	2.520	0.480	80.90000	1.22E-01	1.69E-01	3.01E-01	1.68E-01
U-238	4184.730	34.560	1.440	100.0000	1.35E+00	5.03E-01	3.36E-01	4.63E-01


REVIEWED BY:

DATE:

Handwritten signature
04/10/06

Handwritten notes:
 RPD
 U-3/4 = 57.3 ACTL SXMPA
 U-235 = 28.2 ACTL SXMPA
 U-238 = 10.9

Handwritten date: 04/10/06

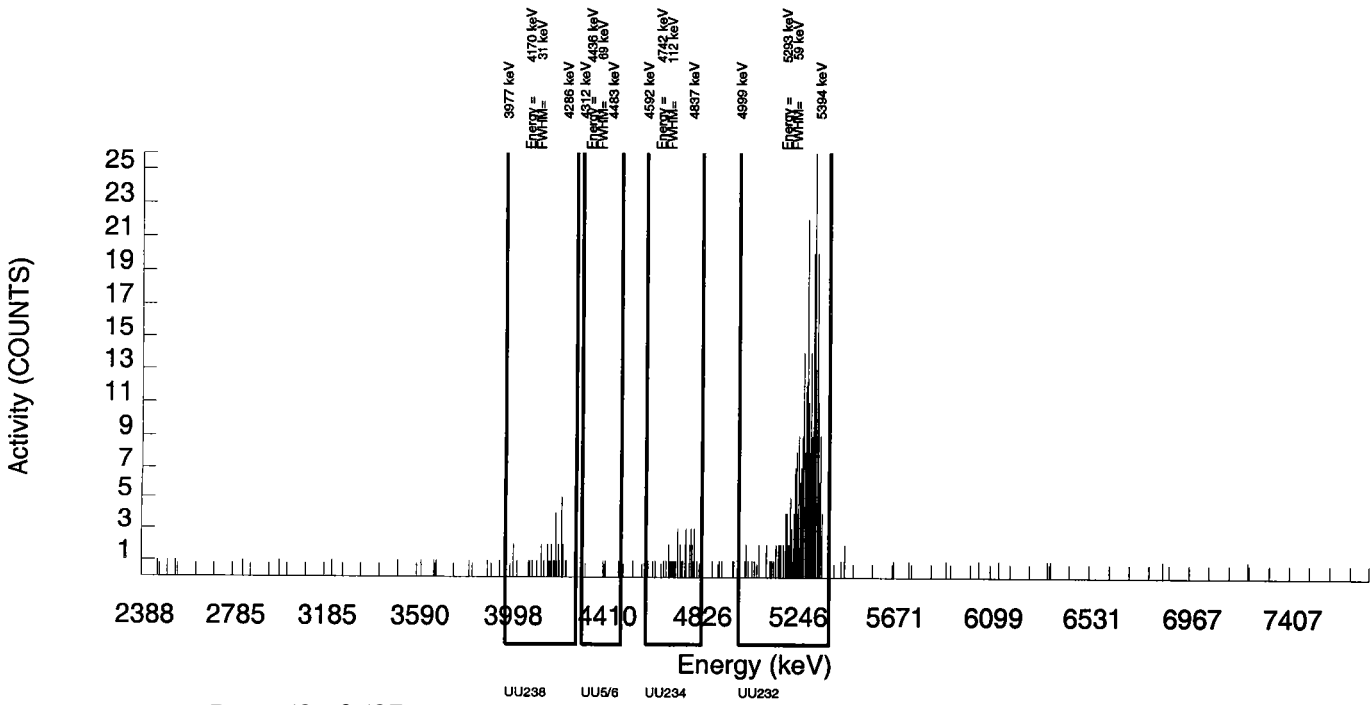

GENERAL ENGINEERING LABORATORIES, LLC.
ALPHA SPECTROSCOPY REPORT

BATCH NUMBER: 517155 SAMPLE DATE : 10-MAR-2006 00:00:00		SAMPLE ID : S1201062933_UU SAMPLE QTY: 0.203 G	
DETECTOR NUMBER :29269 AVERAGE %EFFICIENCY :34.1362 % YIELD : 79.752		COUNT DATE: 8-APR-2006 15:43:20 ELAPSED LIVE TIME(SEC): 14400.00 ANALYST :LCW1	
MS : 0858-B MSD : 0858-B LCS : 0858-B TRACER : 0688-H BKG FILE: B080.CNF;599 BKG DATE: 2-APR-2006		MS PCI/G : 12.95245 MSD PCI/G : 12.95245 LCS PCI/G : 12.95245 TRACER DPM : 5.4124 EFF FILE : W080.CNF;153 CAL DATE: 3-APR-2006	
		MS ISOTOPE : U-238 MSD ISOTOPE: U-238 LCS ISOTOPE: U-238 TRACER ISOTOPE: U232 LIB FILE : ENV_ALPHA_UU.N	

NUCLIDE ACTIVITY SUMMARY

NUCLIDE	ENERGY	NET AREA	BKG AREA	%ABUN	ACTIVITY pCi/G	TPU 1.96-SIGMA	MDA pCi/G	UNC pCi/G
U-3/4	4763.020	423.320	1.680	100.0000	1.44E+01	2.41E+00	3.07E-01	1.37E+00
U232	5302.100	353.360	2.640	100.0000	1.20E+01	2.08E+00	3.59E-01	1.26E+00
U-235	4391.000	13.760	0.240	80.90000	5.78E-01	3.19E-01	2.22E-01	3.08E-01
U-238	4184.730	462.800	1.200	100.0000	1.57E+01	2.59E+00	2.75E-01	1.43E+00


REVIEWED BY:

DATE:

gyp 4/11/06

gyp 4/11/06

MS = $\frac{13.7 - 1.221}{13.0} = 111\%$

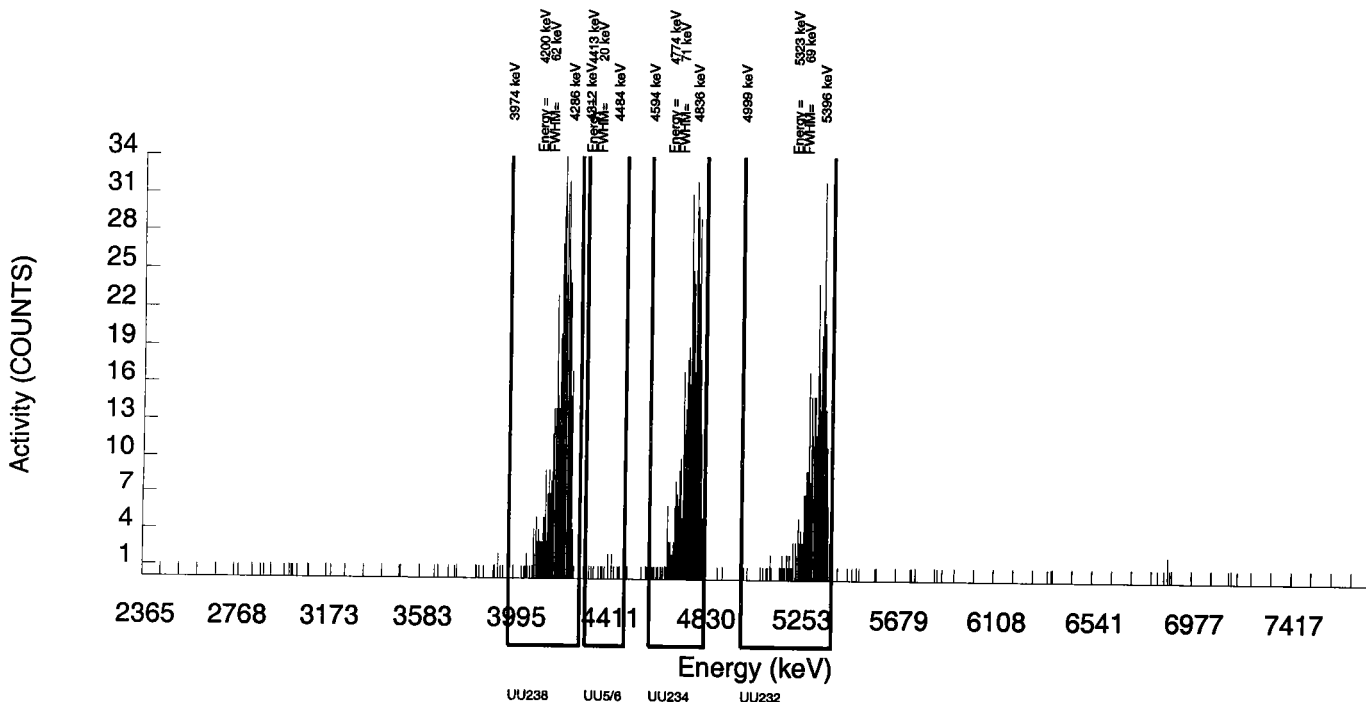

GENERAL ENGINEERING LABORATORIES, LLC.
ALPHA SPECTROSCOPY REPORT

BATCH NUMBER: 517155
SAMPLE DATE : 6-APR-2006 00:00:00.

SAMPLE ID : S1201062934_UU
SAMPLE QTY: 0.231 G

DETECTOR NUMBER :28243
AVERAGE %EFFICIENCY :27.0915
% YIELD : 94.586

COUNT DATE: 8-APR-2006 15:43:20
ELAPSED LIVE TIME(SEC): 14400.00
ANALYST :LCW1

MS : 0858-B
MSD : 0858-B
LCS : 0858-B
TRACER : 0688-H
BKG FILE: B081.CNF;603
BKG DATE: 2-APR-2006

MS PCI/G : 11.38245
MSD PCI/G : 11.38245
LCS PCI/G : 11.38245
TRACER DPM : 5.4086
EFF FILE : W081.CNF;154
CAL DATE: 5-APR-2006

MS ISOTOPE : U-238
MSD ISOTOPE: U-238
LCS ISOTOPE: U-238
TRACER ISOTOPE: U232
LIB FILE : ENV_ALPHA_UU.N

NUCLIDE ACTIVITY SUMMARY

NUCLIDE	ENERGY	NET AREA	BKG AREA	%ABUN	ACTIVITY pCi/G	TPU 1.96-SIGMA	MDA pCi/G	UNC pCi/G
U-3/4	4763.020	317.520	0.480	100.0000	1.01E+01	1.79E+00	1.97E-01	1.11E+00
U232	5302.100	332.600	2.400	100.0000	1.05E+01	1.86E+00	3.24E-01	1.14E+00
U-235	4391.000	21.280	0.720	80.90000	8.34E-01	3.80E-01	2.72E-01	3.62E-01
U-238	4184.730	366.800	1.200	100.0000	1.16E+01	2.01E+00	2.57E-01	1.19E+00


REVIEWED BY:

[Handwritten signature]

DATE :

[Handwritten date]

$$LCS = \frac{11.6}{11.4} = 102\%$$

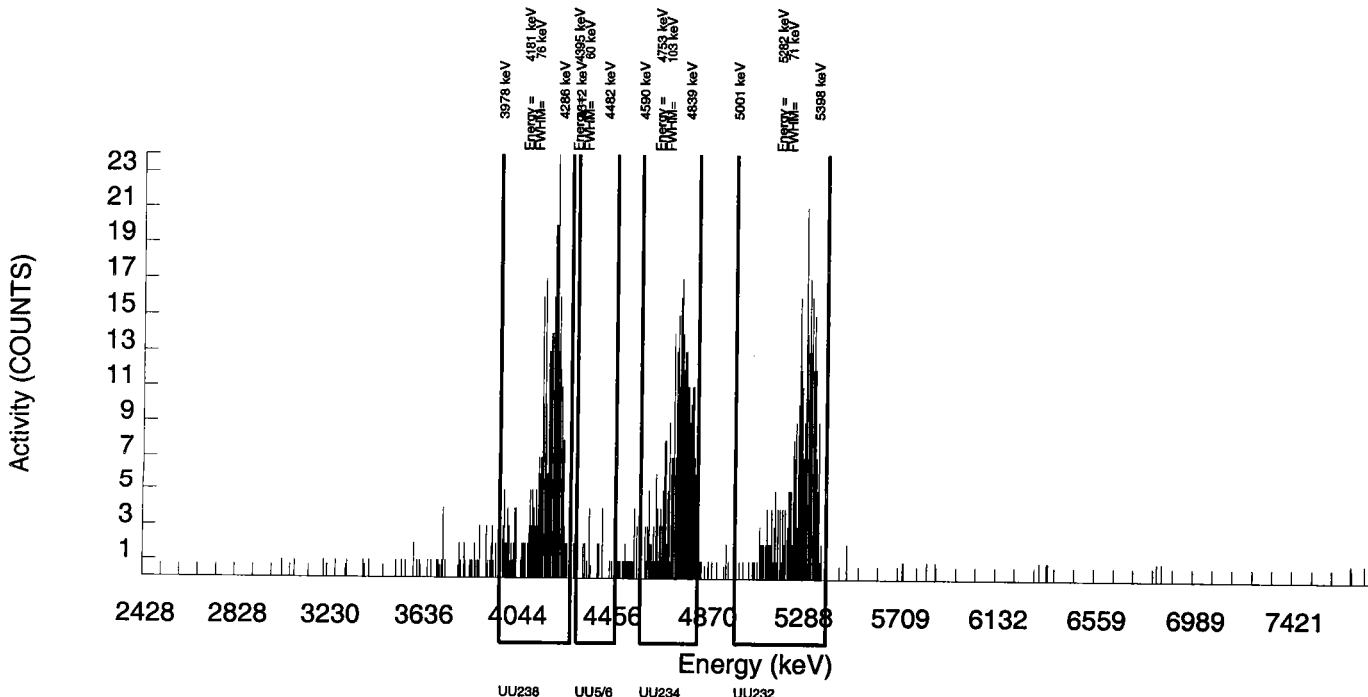

Radiochemistry Batch Checklist, Rev 4

Batch# 513802 Product: 85 / MWHC Date: 4/13/06

Criteria:	Yes	No	Comments
Sample Solids are less than 100 mg for GAB.			NA
If activity less 10* MDA, error is 150% or less of sample activity. If greater 10* MDA, error is 40% or less. If below the MDA, error is okay.	✓		
Instrument source check is within limits. Instrument bkg check is within limits.	✓		
Method RDL has been met.	✓		
If duplicate activities are less 5* MDA, then rpd is 100% or less. If greater 5* MDA, then rpd 20% or less. If below the MDA, the rpd is 0%. Or meets the client's required RER acceptance criteria.	✓		
Tracer yield is 15-125% . Carrier yield 25-125%. Or meets the client's contract acceptance criteria.			NA
Method blank is less than the RDL. (If rad samples, < 5% of lowest activity)	✓		
Sample was run within hold time.	✓		
Special requirements page checked	✓		
Sample was correctly preserved if required.	✓		
Smears Taken for Radioactive batches.			NA
Method Spike and LCS are within 75-125% or meets the client's contract acceptance criteria.	✓		
No blank spaces on data forms. All lineouts initialed and dated. No transcription errors are apparent.	✓		
QC data entered into QC database. Batch entered into Case Narrative.	✓		
Batch non-conformances completed If applicable.			NA

General Engineering Laboratories

2/22/2005

Primary Review Performed By: Jodi Cummings 4/13/06

Secondary Review Performed By: Hecan J. Garcia 4/13/06

MWHC

4/8/06 - 4/15/06

Gamma Spec Que Sheet

Batch #: 513802 *below unml 3/28* 03/22/2006

Analyst: MJHI Minimum Due Date: 04/08/2006
 Gamma Spike Isotope: Mixed Gamma Spike Code: NA Vol: NA Nominal Concentration: NA
 Gamma LCS Isotope: Mixed Gamma LCS Code: 0781-A Vol: 1.0ml Nominal Concentration: 987-9.285 G10-1335
 Initials: JM Prep Date: 3/21/06 Witness: NA AMT/1-24.38

Sample ID	Client Description / Container ID	Type	Hazard Code	RDL	Client	Matrix	Collect Date	Aliquot (1g/F)	Detector	Sealing Date/Time (if Applicable)
158269001	2603140361 M121-0.5	SAMPLE	1 pCi/g	MWHL002	SOIL	10-MAR-06 07:46:00	148.70	16	3/21/06	
158269002	2603140362 M121-5	SAMPLE	1 pCi/g	MWHL002	SOIL	10-MAR-06 07:55:00	143.55	16		
158269003	2603140364 M121-5D	SAMPLE	1 pCi/g	MWHL002	SOIL	10-MAR-06 12:00:00	129.35	16		
158269004	2603140365 M121-80	SAMPLE	1 pCi/g	MWHL002	SOIL	10-MAR-06 12:00:00	124.66	16		
158270001	2603100106 M118-0.5	SAMPLE	1 pCi/g	MWHL002	SOIL	08-MAR-06 11:10:00	158.02	16		
158270002	2603100107 M118-5	SAMPLE	1 pCi/g	MWHL002	SOIL	08-MAR-06 11:20:00	147.85	10		
1201055607	MB for batch 513802	MB	1 pCi/g	QC ACCOUNT	SOIL	3-21-06	159.64	13		
1201055608	2603140361 M121-0.5(158269001)DUP	DUP	1 pCi/g	QC ACCOUNT	SOIL	10-MAR-06 07:46:00	159.64	16		
1201055609	LCS for batch 513802	LCS	1 pCi/g	QC ACCOUNT	SOIL	3-21-06	100.00	well	3/21/06	

Data Reviewed By: Jodi Cunningham 4/13/06
Adam Garcia Page 1 of 1
 4/13/06

Failed RDL Report

Batch Id	Samp Id	Sample Type	Run Date	Parmname	Result	MDA	RDL
513802	158269001	SAMPLE	10-APR-06				
513802	158269002	SAMPLE	10-APR-06				
513802	158269003	SAMPLE	11-APR-06				
513802	158269004	SAMPLE	11-APR-06				
513802	158270001	SAMPLE	11-APR-06				
513802	158270002	SAMPLE	11-APR-06				
513802	1201055607	MB	11-APR-06				
513802	1201055608	DUP	11-APR-06				
513802	1201055609	LCS	11-APR-06	Radium-228	0.1208	1.405	1.00

Result Greater Than MDA

Batch Id	Sample Id	Sample Type	Run Date	Parmname	Result	Uncertainty	Units	MDA	RDL
513802	158269001	SAMPLE	10-APR-06	Cadmium-115	1874	1605	pCi/g	0	N
				Cerium-143	4.392E+06	1.417E+06	pCi/g	0	N
				Gross Gamma	10.16	2.855	pCi/g	6.65	N
				Iodine-133	9.966E+08	2.941E+09	pCi/g	0	N
				Iodine-135	1.493E+33	5.383E+33	pCi/g	0	N
				Lead-212 ✓	2.13	0.2363	pCi/g	0.08922	10.0
				Manganese-56	1.000E+41	9.848E+41	pCi/g	0	N
				Molybdenum-99	37.11	67	pCi/g	0	N
				Niobium-95m	15.37	47.65	pCi/g	0	N
				Potassium-40 ✓	29.36	2.624	pCi/g	0.5457	N
				Praseodymium-144	1.000E+41	1.730E+41	pCi/g	0	N
				Radium-226 ✓	1.064	0.1842	pCi/g	0.1065	2.00
				Radium-228 ✓	1.856	0.3767	pCi/g	0.1785	1.00
				Technetium-99m	1.253E+36	2.377E+36	pCi/g	0	N
513802	158269002	SAMPLE	10-APR-06	Cerium-143	6.265E+06	1.878E+06	pCi/g	0	N
				Gross Gamma	8.396	1.566	pCi/g	4.362	N
				Iodine-132	1.000E+41	7.541E+41	pCi/g	0	N
				Iodine-133	1.042E+09	1.603E+09	pCi/g	0	N
				Lead-212 ✓	1.338	0.1405	pCi/g	0.04943	10.0
				Niobium-95m	12.27	27.09	pCi/g	0	N
				Potassium-40 ✓	16.81	1.367	pCi/g	0.2856	N
				Radium-226 ✓	1.393	0.1463	pCi/g	0.05789	2.00
				Radium-228 ✓	1.235	0.2104	pCi/g	0.09477	1.00
				Sodium-24	3.418E+13	3.357E+13	pCi/g	0	N
Tellurium-132	6.181	12.19	pCi/g	0	N				
513802	158269003	SAMPLE	11-APR-06	Cerium-143	6.508E+06	2.029E+06	pCi/g	0	N
				Gross Gamma	8.756	1.917	pCi/g	5.839	N
				Iodine-133	9.841E+08	2.248E+09	pCi/g	0	N
				Lead-212 ✓	1.552	0.1688	pCi/g	0.06324	10.0
				Manganese-56	1.000E+41	3.396E+41	pCi/g	0	N
				Niobium-95m	32.23	34.58	pCi/g	0	N
				Potassium-40 ✓	17.28	1.521	pCi/g	0.3301	N
				Promethium-149	4911	11400	pCi/g	0	N
				Radium-226 ✓	1.283	0.1587	pCi/g	0.06824	2.00
				Radium-228 ✓	1.354	0.2619	pCi/g	0.1431	1.00
				Sodium-24	1.385E+12	5.642E+13	pCi/g	0	N
				Tellurium-132	8.532	15.89	pCi/g	0	N

Result Greater Than MDA

Batch Id	Sample Id	Sample Type	Run Date	Parmname	Result	Uncertainty	Units	MDA	RDL
513802	158269004	SAMPLE	11-APR-06	Cadmium-115	203.7	1279	pCi/g	0	N
				Cerium-143	6.736E+06	2.067E+06	pCi/g	0	N
				Gross Gamma	9.034	2	pCi/g	6.424	N
				Lead-212 ✓	1.483	0.1628	pCi/g	0.06663	10.0
				Manganese-56	1.000E+41	1.336E+41	pCi/g	0	N
				Molybdenum-99	31.86	59.63	pCi/g	0	N
				Niobium-95m	13.96	36.1	pCi/g	0	N
				Potassium-40 ✓	21.77	1.871	pCi/g	0.4282	N
				Promethium-149	903	11910	pCi/g	0	N
				Radium-224	5.08	1.01	pCi/g	0.7389	N
				Radium-226 ✓	1.089	0.1549	pCi/g	0.07307	2.00
				Radium-228 ✓	1.38	0.2674	pCi/g	0.1497	1.00
				Technetium-99m	2.821E+36	5.535E+36	pCi/g	0	N
				513802	158270001	SAMPLE	11-APR-06	Cerium-143	1.497E+07
				Gross Gamma	9.012	1.906	pCi/g	5.373	N
				Iodine-132	1.000E+41	7.133E+41	pCi/g	0	N
				Iodine-135	1.746E+36	2.201E+36	pCi/g	0	N
				Lead-212 ✓	1.755	0.1841	pCi/g	0.06102	10.0
				Manganese-56	1.000E+41	1.401E+41	pCi/g	0	N
				Molybdenum-99	17.84	91.19	pCi/g	0	N
				Niobium-95m	70.85	53.53	pCi/g	0	N
				Potassium-40 ✓	21.88	1.777	pCi/g	0.367	N
				Praseodymium-144	1.000E+41	1.002E+42	pCi/g	0	N
				Radium-226 ✓	0.975	0.1213	pCi/g	0.06729	2.00
				Radium-228 ✓	1.8	0.2729	pCi/g	0.1148	1.00
				Technetium-99m	4.064E+38	2.093E+39	pCi/g	0	N
				Tellurium-132	18.95	25.11	pCi/g	0	N
513802	158270002	SAMPLE	11-APR-06	Cerium-143	4.493E+06	2.008E+06	pCi/g	0	N
				Gross Gamma	10.4	2.233	pCi/g	6.519	N
				Iodine-132	1.000E+41	6.545E+41	pCi/g	0	N
				Iodine-133	1.049E+10	1.905E+10	pCi/g	0	N
				Iodine-135	1.181E+36	6.081E+36	pCi/g	0	N
				Krypton-85 ✓	12.07	4.978	pCi/g	8.694	N
				Lead-212 ✓	1.884	0.1711	pCi/g	0.06537	10.0
				Manganese-56	1.000E+41	2.374E+41	pCi/g	0	N
				Molybdenum-99	41.95	94	pCi/g	0	N
				Niobium-95m	8.072	53.98	pCi/g	0	N

Result Greater Than MDA

Batch Id	Sample Id	Sample Type	Run Date	Parmname	Result	Uncertainty	Units	MDA	RDL
513802	158270002	SAMPLE	11-APR-06	Potassium-40 ✓	26.42	2.076	pCi/g	0.3234	N
				Praseodymium-144	1.000E+41	8.201E+43	pCi/g	0	N
				Radium-226 ✓	1.017	0.1462	pCi/g	0.07015	2.00
				Radium-228 ✓	1.772	0.302	pCi/g	0.1333	1.00
				Sodium-24	1.476E+14	9.149E+14	pCi/g	0	N
				Technetium-99m	2.367E+39	5.513E+39	pCi/g	0	N
513802	1201055607	MB	11-APR-06	Cerium-143	629.7	2949	pCi/g	0	N
				Iodine-132	1.000E+41	1.618E+41	pCi/g	0	N
				Iodine-133	4.981E+05	8.239E+05	pCi/g	0	N
				Lead-212 LA 0.05978 0	0.02778	pCi/g	0.05577	10.0 ul	
				Manganese-56	1.000E+41	2.000E+41	pCi/g	0	N
				Praseodymium-144	1.000E+41	1.823E+41	pCi/g	0	N
				Promethium-149	37.52	372.3	pCi/g	0	N
513802	1201055608	DUP	11-APR-06	Cadmium-115	702.7	1483	pCi/g	0	N
				Cerium-143	7.657E+06	2.421E+06	pCi/g	0	N
				Gross Gamma	10.38	2.012	pCi/g	6.021	N
				Lead-212 ✓	2.024	0.2085	pCi/g	0.06231	10.0
				Niobium-95m	14.77	39.95	pCi/g	0	N
				Potassium-40 ✓	27.14	2.114	pCi/g	0.3342	N
				Promethium-149	7977	18550	pCi/g	0	N
				Radium-224	5.431	0.85	pCi/g	0.7087	N
				Radium-226 ✓	0.9629	0.1263	pCi/g	0.07467	2.00
				Radium-228 ✓	1.858	0.2904	pCi/g	0.1452	1.00
				Sodium-24	1.215E+14	1.219E+14	pCi/g	0	N
				Tellurium-132	10.62	18.65	pCi/g	0	N
513802	1201055609	LCS	11-APR-06	Americium-241	25.14	1.131	pCi/g	0.7162	N
				Barium-137m	9.115	0.6215	pCi/g	0.269	N
				Cadmium-109	196	8.169	pCi/g	4.653	N
				Cesium-137	9.635	0.657	pCi/g	0.2844	N
				Cobalt-60	13.66	0.8254	pCi/g	0.2748	N
				Gross Gamma	65.32	12.19	pCi/g	23.1	N
				Iodine-133	7.029E+05	4.933E+06	pCi/g	0	N
				Iodine-135	1.015E+23	1.618E+23	pCi/g	0	N
				Neptunium-237	57.07	2.379	pCi/g	1.36	N
				Promethium-147	6.086E+06	5.220E+05	pCi/g	7.620E+05	N
				Tin-126	19.43	0.8102	pCi/g	0.462	N

GEL QUALS

Batch ID: 513802

Report run on: April 13, 2006 11:20 AM

Samp Id Parmname Cofa Edd Qual Comments Auto Result MDA Uncert SQL

1201055607-1 MB
11-APR-2006 23:19

Lead-212

UI

UI

UI

Data rejected due to low abundance.

0

VAX/VMS Nuclide Identification Report Generated 10-APR-2006 23:53:31.70

```

*****
*                               GENERAL ENG. LABS, LLC.                               *
*                               2040 Savage Road                                       *
*                               Charleston, SC 29414                                   *
*****
Configuration   : DKA300:[CANBERRA.GAMMA.ARCHIVE.GAMMA]G158269001.CNF;1
Sample date     : 10-MAR-2006 07:46:00 Acquisition date : 10-APR-2006 21:53:09
Sample ID      : G158269001 Sample quantity   : 1.48700E+02 GRAM
Detector name   : GAMMA16 Detector geometry: CAN
Elapsed live time: 0 02:00:00.00 Elapsed real time: 0 02:00:01.36 0.0%
Energy tolerance: 2.00000 KEV Analyst Initials : MJH1
Abundance limit : 75.00000 Sensitivity      : 3.00000
Batch ID       : 513802 Detector SN#      : 1922864
Matrix Spike DPM : LCS DPM                  :
*****

```

Pk	It	Energy	Area	Bkgnd	FWHM	Channel	Left	Pw	Cts/Sec	%Err	Fit
1	0	63.43*	26	290	0.98	125.39	123	6	3.66E-03	107.6	
2	3	74.67*	331	418	1.12	147.86	143	15	4.60E-02	11.9	4.53E-01
3	3	77.05*	565	343	1.07	152.60	143	15	7.84E-02	7.0	
4	3	86.95*	284	445	1.42	172.40	163	29	3.94E-02	14.8	3.05E+00
5	3	89.75	144	383	1.29	177.98	163	29	1.99E-02	25.6	
6	3	92.90*	204	415	1.43	184.29	163	29	2.84E-02	20.5	
7	0	99.04	60	362	0.99	196.55	193	8	8.27E-03	56.8	
8	0	120.32	33	231	0.92	239.08	237	6	4.61E-03	74.3	
9	3	128.94*	133	315	1.17	256.31	250	14	1.85E-02	24.0	1.12E+00
10	3	131.25*	29	264	0.99	260.93	250	14	4.02E-03	92.6	
11	0	154.32	52	308	0.53	307.03	304	7	7.24E-03	57.6	
12	0	185.98*	196	363	1.41	370.30	366	10	2.73E-02	20.1	
13	2	209.22	171	229	1.51	416.75	413	13	2.38E-02	16.5	4.67E-01
14	2	212.32	30	225	1.18	422.95	413	13	4.20E-03	84.3	
15	4	238.49*	1656	212	1.18	475.25	468	19	2.30E-01	2.9	1.17E+00
16	4	241.37*	261	250	1.55	481.00	468	19	3.62E-02	16.3	
17	0	259.27	18	134	1.25	516.79	514	6	2.54E-03	102.7	
18	0	269.53	168	331	2.05	537.29	530	15	2.33E-02	24.8	
19	0	277.58	88	218	1.20	553.38	549	10	1.23E-02	33.3	
20	3	295.08*	341	139	1.02	588.36	583	21	4.74E-02	7.8	2.16E+00
21	3	299.91*	105	241	1.72	598.01	583	21	1.46E-02	28.8	
22	0	327.88	97	129	1.24	653.92	651	7	1.35E-02	21.7	
23	0	338.17*	368	168	1.21	674.50	670	10	5.11E-02	8.6	
24	0	351.62*	586	263	1.31	701.37	694	15	8.14E-02	7.4	
25	0	409.31*	29	83	0.77	816.71	814	6	4.02E-03	55.3	
26	0	462.61	90	174	1.09	923.26	917	12	1.25E-02	31.2	
27	0	492.44	27	76	1.57	982.91	979	9	3.74E-03	62.1	
28	0	510.69*	108	224	1.93	1019.39	1011	16	1.50E-02	35.4	
29	0	582.69*	545	140	1.35	1163.34	1155	16	7.57E-02	6.5	
30	0	608.92*	460	145	1.57	1215.78	1208	17	6.38E-02	7.7	
31	0	648.69	22	56	1.33	1295.33	1292	8	3.03E-03	63.8	
32	0	726.66	117	69	1.27	1451.23	1445	12	1.63E-02	16.9	
33	0	767.89*	34	48	1.45	1533.69	1531	7	4.67E-03	40.7	
34	0	794.62*	77	66	2.11	1587.14	1582	15	1.07E-02	26.0	
35	0	839.30*	20	58	1.64	1676.50	1673	9	2.75E-03	74.5	
36	0	860.20*	77	33	1.28	1718.32	1714	9	1.07E-02	18.9	
37	0	874.83*	22	39	2.40	1747.57	1744	10	3.09E-03	58.0	
38	0	910.49*	336	77	1.61	1818.90	1811	17	4.66E-02	8.3	

Pk	It	Energy	Area	Bkgnd	FWHM	Channel	Left	Pw	Cts/Sec	%Err	Fit
39	0	918.77	28	33	1.23	1835.47	1830	12	3.85E-03	45.6	
40	0	940.49	28	25	1.50	1878.92	1876	8	3.93E-03	35.5	
41	1	963.96*	70	46	2.02	1925.85	1919	28	9.69E-03	23.3	9.58E-01
42	1	968.39*	216	40	2.03	1934.71	1919	28	3.00E-02	9.4	
43	0	1000.08*	18	38	1.34	1998.10	1992	10	2.48E-03	75.7	
44	0	1062.39	16	27	1.30	2122.77	2120	8	2.22E-03	61.1	
45	1	1113.68	29	25	2.12	2225.38	2221	23	4.02E-03	37.5	2.85E+00
46	1	1119.10*	76	55	2.12	2236.23	2221	23	1.05E-02	24.4	
47	0	1134.09	19	22	2.19	2266.22	2263	7	2.65E-03	47.0	
48	0	1237.45	41	89	1.69	2473.02	2468	14	5.76E-03	51.1	
49	0	1376.30	12	51	2.83	2750.88	2747	19	1.61E-03	152.1	
50	0	1400.26	5	110	11.19	2798.82	2789	49	6.49E-04	819.8	
51	0	1459.58*	1356	47	2.03	2917.55	2907	21	1.88E-01	3.0	
52	0	1494.44*	19	6	2.19	2987.32	2983	11	2.63E-03	34.4	
53	0	1510.00*	26	7	5.23	3018.47	3011	15	3.61E-03	30.8	
54	4	1586.38	33	2	2.96	3171.35	3166	23	4.52E-03	20.7	2.08E-01
55	4	1591.61*	30	11	3.16	3181.83	3166	23	4.12E-03	30.3	
56	0	1638.59	18	3	3.76	3275.87	3269	14	2.47E-03	32.4	
57	0	1728.47	24	11	1.82	3455.81	3449	16	3.29E-03	38.5	
58	0	1763.32*	79	10	2.14	3525.59	3515	21	1.09E-02	15.7	
59	0	1788.58*	10	3	3.55	3576.17	3570	11	1.32E-03	53.5	
60	3	1840.37	16	1	3.01	3679.87	3674	26	2.26E-03	31.3	3.53E-01
61	3	1846.19*	20	6	3.02	3691.51	3674	26	2.83E-03	35.1	
62	0	1908.44	11	3	1.01	3816.17	3809	12	1.50E-03	44.3	

Flag: "*" = Peak area was modified by background subtraction

VAX/VMS Nuclide Identification Report Generated

 * General Eng. Labs, LLC. *
 * 2040 Savage Road *
 * Charleston, SC 29414 *

DETECTOR DATA

* Configuration : DKA300:[CANBERRA.GAMMA.ARCHIVE.GAMMA]G158269001 *
 * Acquisition date : 10-APR-2006 21:53:09 Detector SN# : 1922864 *
 * Detector ID : GAMMA16 Sensitivity : 3.000 *
 * Geometry : CAN Energy tolerance: 2.000 *
 * Elapsed live time: 0 02:00:00.00 Abundance limit : 75.000 *
 * Elapsed real time: 0 02:00:01.36 Half life ratio : 8.000 *

SAMPLE DATA

* Sample date : 10-MAR-2006 07:46:00 Nuclide Library : *
 * Sample ID : G158269001 Analyst initials: MJH1 *
 * Batch Number : 513802 Sample Quantity : 1.4870E+02 GRAM *
 * Recovery : 1.00000 Carrier Weight : 0.00000 *

QC DATA

* Standard Weight : 0.00000 *
 * CALIB. DATE/TIME : 5-APR-2006 19:34:04 MS Isotope : *
 * MSD DPM : 0.000 MSD Isotope : *
 * LCS DPM : 0.000 LCS Isotope : *
 * LCSD DPM : 0.000 LCSD Isotope : *

Combined Activity-MDA Report

---- Identified Nuclides ----

Nuclide	Activity (pCi/GRAM)	Act error	MDA (pCi/GRAM)	
K-40	2.936E+01	2.624E+00	5.457E-01	0.000E+00
CO-57	1.755E-02	2.611E-02	4.469E-02	0.000E+00
ZN-65	1.142E-01	8.614E-02	1.546E-01	0.000E+00
CD-109	4.284E+00	1.346E+00	1.305E+00	0.000E+00
SN-126	4.185E-01	1.315E-01	1.286E-01	0.000E+00
CS-135	6.349E-01	3.205E-01	2.413E-01	0.000E+00
PM-147	3.540E+04	5.267E+04	8.578E+04	0.000E+00
HG-203	1.127E-01	7.555E-02	8.203E-02	0.000E+00
TL-208	6.915E-01	1.024E-01	5.979E-02	0.000E+00
BI-211	3.281E+00	5.404E-01	3.055E-01	0.000E+00
BI-212	1.268E+00	4.430E-01	3.915E-01	0.000E+00
PB-212	2.130E+00	2.363E-01	8.922E-02	0.000E+00
BI-214	1.064E+00	1.842E-01	1.065E-01	0.000E+00
PB-214	1.141E+00	1.972E-01	1.058E-01	0.000E+00
RA-224	3.821E+00	1.289E+00	1.015E+00	0.000E+00
RA-226	1.064E+00	1.842E-01	1.065E-01	0.000E+00
AC-228	1.856E+00	3.767E-01	1.785E-01	0.000E+00
RA-228	1.856E+00	3.767E-01	1.785E-01	0.000E+00
TH-228	2.130E+00	2.363E-01	8.921E-02	0.000E+00
TH-229	7.183E-02	4.854E-01	8.741E-01	0.000E+00
TH-230	1.064E+00	1.842E-01	1.065E-01	0.000E+00
TH-232	2.064E+00	2.290E-01	8.645E-02	0.000E+00
PA-234M	3.489E+00	5.296E+00	7.258E+00	0.000E+00
TH-234	9.572E-01	2.070E+00	3.249E+00	0.000E+00
U-234	1.143E+00	2.117E-01	2.061E-01	0.000E+00
NP-237	1.229E+00	4.620E-01	3.853E-01	0.000E+00
U-238	9.572E-01	2.070E+00	3.249E+00	0.000E+00
ANH-511	1.013E-01	7.206E-02	4.857E-02	0.000E+00

---- Non-Identified Nuclides ----

Nuclide	Key-Line Activity (pCi/GRAM)	K.L. Act error) Ided	MDA (pCi/GRAM)
---------	-------------------------------------	--------------------------	--------------------

BE-7	-3.741E-02	3.651E-01	6.616E-01	0.000E+00	NOT IDENT.
NA-22	-2.812E-03	3.568E-02	6.445E-02	0.000E+00	NOT IDENT.
NA-24	0.000E+00	5.194E+13	0.000E+00	0.000E+00	SHORT HLIF
AL-26	7.827E-03	2.588E-02	5.273E-02	0.000E+00	FAIL ABUN
SC-46	9.994E-03	4.081E-02	7.338E-02	0.000E+00	FAIL ABUN
V-48	-3.218E-02	1.261E-01	2.273E-01	0.000E+00	NOT IDENT.
CR-51	-2.270E-01	5.181E-01	8.767E-01	0.000E+00	NOT IDENT.
MN-54	5.693E-03	4.029E-02	7.087E-02	0.000E+00	NOT IDENT.
CO-56	4.246E-03	4.159E-02	7.385E-02	0.000E+00	FAIL ABUN
MN-56	0.000E+00	9.848E+41	0.000E+00	0.000E+00	SHORT HLIF
CO-58	9.016E-04	3.753E-02	6.694E-02	0.000E+00	NOT IDENT.
FE-59	-5.260E-02	1.019E-01	1.770E-01	0.000E+00	NOT IDENT.
CO-60	2.867E-03	3.390E-02	6.255E-02	0.000E+00	NOT IDENT.
SE-75	-2.117E-02	5.036E-02	7.644E-02	0.000E+00	FAIL ABUN
KR-85	6.534E+00	7.118E+00	1.221E+01	0.000E+00	NOT IDENT.
SR-85	3.983E-02	4.340E-02	7.446E-02	0.000E+00	NOT IDENT.
Y-88	-5.413E-03	3.128E-02	5.108E-02	0.000E+00	NOT IDENT.
Y-91	1.328E-02	4.137E-02	7.629E-02	0.000E+00	NOT IDENT.
NB-94	2.676E-02	2.856E-02	5.460E-02	0.000E+00	NOT IDENT.
NB-95	7.484E-02	7.479E-02	1.257E-01	0.000E+00	NOT IDENT.
NB-95M	0.000E+00	4.765E+01	0.000E+00	0.000E+00	SHORT HLIF
ZR-95	1.304E-02	7.886E-02	1.413E-01	0.000E+00	NOT IDENT.
MO-99	0.000E+00	6.700E+01	0.000E+00	0.000E+00	SHORT HLIF
TC-99M	0.000E+00	2.377E+36	0.000E+00	0.000E+00	SHORT HLIF
RU-103	1.821E-02	4.871E-02	9.088E-02	0.000E+00	FAIL ABUN
RH-106	-5.034E-02	2.837E-01	5.036E-01	0.000E+00	FAIL ABUN
RU-106	-6.735E-02	2.825E-01	4.989E-01	0.000E+00	NOT IDENT.
AG-108M	1.721E-03	2.824E-02	5.220E-02	0.000E+00	NOT IDENT.
AG-110M	-3.802E-02	3.375E-02	5.469E-02	0.000E+00	NOT IDENT.
SN-113	-1.546E-02	4.373E-02	7.915E-02	0.000E+00	NOT IDENT.
CD-115	0.000E+00	1.605E+03	0.000E+00	0.000E+00	SHORT HLIF
SN-115	5.546E+00	4.196E+00	8.408E+00	0.000E+00	NOT IDENT.
SN-117M	2.584E-02	1.140E-01	2.090E-01	0.000E+00	FAIL ABUN
TE-123M	5.035E-03	2.843E-02	5.197E-02	0.000E+00	NOT IDENT.
SB-124	-1.900E-02	7.777E-02	1.387E-01	0.000E+00	NOT IDENT.
SB-125	-2.811E-02	7.679E-02	1.384E-01	0.000E+00	FAIL ABUN
TE-125M	5.418E+00	1.038E+01	1.964E+01	0.000E+00	NOT IDENT.
I-126	-6.230E-02	4.048E-01	7.125E-01	0.000E+00	NOT IDENT.
SB-126	8.033E-02	3.100E-01	5.640E-01	0.000E+00	NOT IDENT.
SB-127	0.000E+00	2.387E+01	0.000E+00	0.000E+00	SHORT HLIF
I-131	1.183E-01	4.094E-01	7.739E-01	0.000E+00	NOT IDENT.
I-132	0.000E+00	6.330E+41	0.000E+00	0.000E+00	SHORT HLIF
TE-132	0.000E+00	2.177E+01	0.000E+00	0.000E+00	SHORT HLIF
BA-133	-2.409E-03	4.085E-02	6.695E-02	0.000E+00	FAIL ABUN
I-133	0.000E+00	2.941E+09	0.000E+00	0.000E+00	SHORT HLIF
CS-134	0.000E+00	6.553E-02	8.119E-02	0.000E+00	FAIL ABUN
I-135	0.000E+00	5.383E+33	0.000E+00	0.000E+00	SHORT HLIF
CS-136	4.694E-02	2.227E-01	4.161E-01	0.000E+00	FAIL ABUN
BA-137M	1.961E-02	3.308E-02	6.147E-02	0.000E+00	NOT IDENT.
CS-137	2.084E-02	3.498E-02	6.501E-02	0.000E+00	NOT IDENT.
CE-139	-2.080E-02	3.027E-02	5.308E-02	0.000E+00	NOT IDENT.
BA-140	-1.207E-01	5.178E-01	9.250E-01	0.000E+00	NOT IDENT.
LA-140	1.217E-02	1.587E-01	2.658E-01	0.000E+00	FAIL ABUN
CE-141	-3.946E-04	7.789E-02	1.422E-01	0.000E+00	NOT IDENT.
CE-143	0.000E+00	1.417E+06	0.000E+00	0.000E+00	SHORT HLIF
CE-144	1.062E-02	2.068E-01	3.416E-01	0.000E+00	NOT IDENT.
PM-144	1.853E-02	3.206E-02	5.945E-02	0.000E+00	NOT IDENT.
PR-144	0.000E+00	1.730E+41	0.000E+00	0.000E+00	SHORT HLIF
PM-146	1.509E-02	3.989E-02	7.466E-02	0.000E+00	NOT IDENT.
ND-147	-1.415E-01	1.453E+00	2.618E+00	0.000E+00	FAIL ABUN
PM-149	0.000E+00	1.538E+04	0.000E+00	0.000E+00	SHORT HLIF
EU-152	2.478E-04	8.618E-02	1.498E-01	0.000E+00	FAIL ABUN
GD-153	9.613E-02	1.095E-01	1.359E-01	0.000E+00	FAIL ABUN
EU-154	-8.023E-03	9.880E-02	1.784E-01	0.000E+00	FAIL ABUN
EU-155	1.288E-01	1.043E-01	2.015E-01	0.000E+00	FAIL ABUN
TB-160	4.031E-02	1.653E-01	2.622E-01	0.000E+00	FAIL ABUN
TM-171	-2.809E+01	3.723E+01	6.155E+01	0.000E+00	NOT IDENT.
HF-181	-1.913E-03	4.603E-02	8.420E-02	0.000E+00	FAIL ABUN
TA-182	-3.218E-02	1.904E-01	3.367E-01	0.000E+00	FAIL ABUN
IR-192	3.775E-03	3.685E-02	6.472E-02	0.000E+00	FAIL ABUN
BI-207	3.736E-02	4.575E-02	8.645E-02	0.000E+00	FAIL ABUN
BI-210	2.445E+00	1.216E+01	2.006E+01	0.000E+00	NOT IDENT.
PB-210	2.445E+00	1.216E+01	2.006E+01	0.000E+00	NOT IDENT.
PB-211	4.069E-02	8.075E-01	1.494E+00	0.000E+00	NOT IDENT.
RN-219	1.315E-01	3.530E-01	6.657E-01	0.000E+00	FAIL ABUN
RA-223	1.654E-01	6.284E-01	1.108E+00	0.000E+00	FAIL ABUN
AC-227	-2.314E-01	4.127E-01	6.194E-01	0.000E+00	FAIL ABUN

TH-227	-2.274E-01	4.063E-01	6.089E-01	0.000E+00	FAIL	ABUN
PA-231	-1.881E-01	1.421E+00	2.474E+00	0.000E+00	FAIL	ABUN
TH-231	0.000E+00	3.767E-01	3.724E-01	0.000E+00	FAIL	ABUN
PA-233	4.340E-03	6.020E-02	1.055E-01	0.000E+00	FAIL	ABUN
PA-234	-6.910E-02	2.616E-01	4.718E-01	0.000E+00	FAIL	ABUN
U-235	-7.358E-02	1.856E-01	3.327E-01	0.000E+00	FAIL	ABUN
NP-239	-6.734E-02	1.693E-01	3.085E-01	0.000E+00	FAIL	ABUN
AM-241	-1.484E-01	2.433E-01	4.085E-01	0.000E+00	NOT IDENT.	
AM-242	1.493E+00	2.059E+00	3.934E+00	0.000E+00	FAIL	ABUN
CM-247	-1.651E-03	3.199E-02	5.889E-02	0.000E+00	FAIL	ABUN
CF-249	3.075E-02	3.656E-02	7.044E-02	0.000E+00	NOT IDENT.	
CF-251	2.776E-02	1.166E-01	2.123E-01	0.000E+00	NOT IDENT.	

```

*****
*                               GENERAL ENG. LABS, LLC.                               *
*                               2040 Savage Road                                       *
*                               Charleston, SC 29414                                   *
*****
Configuration      : DKA300:[CANBERRA.GAMMA.ARCHIVE.GAMMA]G158269001.CNF;1
Sample date        : 10-MAR-2006 07:46:00 Acquisition date : 10-APR-2006 21:53:09
Sample ID          : G158269001 Sample quantity : 1.48700E+02 GRAM
Detector name     : GAMMA16 Detector geometry: CAN
Elapsed live time : 0 02:00:00.00 Elapsed real time: 0 02:00:01.36 0.0%
Energy tolerance  : 2.00000 KEV Analyst Initials : MJH1
Abundance limit   : 75.00000 Sensitivity : 3.00000
Batch ID          : 513802 Detector SN# : 1922864
Matrix Spike DPM : LCS DPM :
*****
    
```

Nuclide Line Activity Report

Nuclide Type:

Nuclide	Energy	Area	%Abn	%Eff	Uncorrected pCi/GRAM	Decay Corr pCi/GRAM	2-Sigma %Error
K-40	1460.81	1356	10.67*	1.093E+00	2.936E+01	2.936E+01	8.94
CO-57	122.06	33	85.51*	6.055E+00	1.618E-02	1.755E-02	148.81
	136.47	-----	10.47	6.049E+00	-----	Line Not Found	-----
ZN-65	1115.55	29	50.75*	1.379E+00	1.044E-01	1.142E-01	75.40
CD-109	88.03	284	3.79*	4.622E+00	4.086E+00	4.284E+00	31.42
SN-126	64.28	26	9.60	1.830E+00	3.789E-01	3.789E-01	215.99
	86.94	284	8.90	4.622E+00	1.740E+00	1.740E+00	51.22
	87.57	284	37.00*	4.622E+00	4.185E-01	4.185E-01	31.42
CS-135	268.24	168	16.00*	4.178E+00	6.349E-01	6.349E-01	50.49
PM-147	121.30	33	0.00*	6.055E+00	3.460E+04	3.540E+04	148.80
HG-203	70.83	-----	4.75	2.802E+00	-----	Line Not Found	-----
	72.87	331	8.00	3.294E+00	3.175E+00	5.083E+00	27.85
	82.60	-----	3.55	4.202E+00	-----	Line Not Found	-----
	279.20	88	77.30*	4.094E+00	7.039E-02	1.127E-01	67.06
TL-208	75.00	331	3.43	3.294E+00	7.406E+00	7.643E+00	27.43
	277.35	88	6.80	4.094E+00	8.002E-01	8.258E-01	67.60
	510.84	108	21.60	2.690E+00	4.691E-01	4.841E-01	71.60
	583.14	545	84.20*	2.438E+00	6.701E-01	6.915E-01	14.81
	763.30	-----	1.64	1.954E+00	-----	Line Not Found	-----
	860.37	77	12.46	1.756E+00	8.924E-01	9.209E-01	38.91
	1093.90	-----	0.37	1.403E+00	-----	Line Not Found	-----
BI-211	351.07	586	12.94*	3.485E+00	3.281E+00	3.281E+00	16.47
BI-212	727.18	117	11.80*	2.039E+00	1.229E+00	1.268E+00	34.93
PB-212	74.80	331	10.70	3.294E+00	2.374E+00	2.450E+00	27.62
	87.30	284	8.00	4.622E+00	1.936E+00	1.998E+00	32.97
	115.19	-----	0.60	5.993E+00	-----	Line Not Found	-----
	238.63	1656	44.60*	4.541E+00	2.064E+00	2.130E+00	11.09
	300.09	105	3.41	3.884E+00	2.009E+00	2.073E+00	58.36
BI-214	609.31	460	46.30*	2.356E+00	1.064E+00	1.064E+00	17.32
	768.36	34	5.04	1.944E+00	8.655E-01	8.655E-01	81.98
	934.06	-----	3.21	1.627E+00	-----	Line Not Found	-----
	1120.29	76	15.10	1.373E+00	9.238E-01	9.238E-01	49.79

Nuclide Type:

Nuclide	Energy	Area	%Abn	%Eff	Uncorrected pCi/GRAM	Decay Corr pCi/GRAM	2-Sigma %Error
	1238.11	41	5.94	1.252E+00	1.408E+00	1.408E+00	102.49
	1377.67	12	4.11	1.144E+00	6.228E-01	6.228E-01	304.40
PB-214	74.81	331	6.21	3.294E+00	4.091E+00	4.091E+00	27.03
	77.11	565	10.50	3.583E+00	3.788E+00	3.789E+00	19.00
	87.30	284	4.41	4.622E+00	3.512E+00	3.512E+00	32.46
	241.98	261	7.50	4.504E+00	1.950E+00	1.950E+00	34.20
	295.21	341	19.20	3.927E+00	1.143E+00	1.143E+00	18.53
	351.92	586	37.20*	3.485E+00	1.141E+00	1.141E+00	17.28
RA-226	295.21	341	19.20	3.927E+00	1.143E+00	1.143E+00	18.53
	351.92	586	37.20	3.485E+00	1.141E+00	1.141E+00	16.25
	609.31	460	46.30*	2.356E+00	1.064E+00	1.064E+00	17.32
AC-228	209.25	171	4.40	4.952E+00	1.985E+00	2.006E+00	72.14
	338.32	368	11.40	3.579E+00	2.277E+00	2.301E+00	44.43
	463.01	90	4.40	2.886E+00	1.789E+00	1.808E+00	66.59
	794.95	77	4.60	1.886E+00	2.243E+00	2.266E+00	56.99
	911.21	336	27.70*	1.667E+00	1.837E+00	1.856E+00	20.30
	964.77	70	5.20	1.580E+00	2.145E+00	2.167E+00	52.69
RA-228	969.11	216	16.60	1.573E+00	2.086E+00	2.108E+00	30.01
	209.25	171	4.40	4.952E+00	1.985E+00	2.006E+00	72.14
	338.32	368	11.40	3.579E+00	2.277E+00	2.301E+00	44.43
	463.01	90	4.40	2.886E+00	1.789E+00	1.808E+00	66.59
	794.95	77	4.60	1.886E+00	2.243E+00	2.266E+00	56.99
	911.21	336	27.70*	1.667E+00	1.837E+00	1.856E+00	20.30
	964.77	70	5.20	1.580E+00	2.145E+00	2.167E+00	52.69
	969.11	216	16.60	1.573E+00	2.086E+00	2.108E+00	30.01
TH-228	84.40	-----	1.21	4.383E+00	-----	Line Not Found	-----
	238.60	1656	44.60*	4.541E+00	2.064E+00	2.130E+00	11.09
	300.10	105	3.41	3.884E+00	2.009E+00	2.073E+00	82.53
TH-229	85.43	284	16.50	4.622E+00	9.386E-01	9.386E-01	31.42
	88.47	144	27.10	4.858E+00	2.753E-01	2.753E-01	52.14
	100.00	60	12.40	5.469E+00	2.216E-01	2.216E-01	113.89
	193.63	-----	4.59*	5.199E+00	-----	Line Not Found	-----
	210.97	30	3.26	4.905E+00	4.771E-01	4.772E-01	168.72
TH-230	295.21	341	19.20	3.927E+00	1.143E+00	1.143E+00	18.53
	351.92	586	37.20	3.485E+00	1.141E+00	1.141E+00	16.25
	609.31	460	46.30*	2.356E+00	1.064E+00	1.064E+00	17.32
TH-232	238.59	1656	44.60*	4.541E+00	2.064E+00	2.064E+00	11.09
	911.20	336	27.70	1.667E+00	1.837E+00	1.837E+00	20.30
	964.40	70	5.20	1.580E+00	2.145E+00	2.145E+00	52.69
	969.11	216	16.60	1.573E+00	2.086E+00	2.086E+00	30.01
PA-234M	766.40	34	0.21	1.944E+00	2.077E+01	2.077E+01	111.76
	1001.03	18	0.85*	1.526E+00	3.489E+00	3.489E+00	151.79
TH-234	63.29	26	3.80*	1.830E+00	9.572E-01	9.572E-01	216.20
	92.38	204	5.41	5.095E+00	1.870E+00	1.870E+00	45.02
	112.81	-----	0.24	5.950E+00	-----	Line Not Found	-----
U-234	67.67	-----	0.37	2.385E+00	-----	Line Not Found	-----
	241.98	261	7.49	4.504E+00	1.953E+00	1.953E+00	34.20
	295.21	341	19.20*	3.927E+00	1.143E+00	1.143E+00	18.53
	351.92	586	37.20	3.485E+00	1.141E+00	1.141E+00	17.28

Nuclide Type:

Nuclide	Energy	Area	%Abn	%Eff	Uncorrected pCi/GRAM	Decay Corr pCi/GRAM	2-Sigma %Error
NP-237	86.48	284	12.60*	4.622E+00	1.229E+00	1.229E+00	37.59
	95.87	-----	2.60	5.290E+00	-----	Line Not Found	-----
U-238	63.29	26	3.80*	1.830E+00	9.572E-01	9.572E-01	216.20
ANH-511	511.00	108	100.00*	2.690E+00	1.013E-01	1.013E-01	71.11

Nuclide Type: NATURAL

Nuclide	Energy	Area	%Abn	%Eff	Uncorrected pCi/GRAM	Decay Corr pCi/GRAM	2-Sigma %Error
RA-224	240.98	261	3.95*	4.504E+00	3.703E+00	3.821E+00	33.74

Flag: "*" = Keyline

Total number of lines in spectrum 62
 Number of unidentified lines 15
 Number of lines tentatively identified by NID 47 75.81%

Nuclide Type :

Nuclide	Hlife	Decay	Uncorrected pCi/GRAM	Decay Corr pCi/GRAM	Decay Corr 2-Sigma Error	2-Sigma %Error	Flags
K-40	1.28E+09Y	1.00	2.936E+01	2.936E+01	0.262E+01	8.94	
CO-57	270.90D	1.08	1.618E-02	1.755E-02	2.611E-02	148.81	
ZN-65	244.40D	1.09	1.044E-01	1.142E-01	0.861E-01	75.40	
CD-109	464.00D	1.05	4.086E+00	4.284E+00	1.346E+00	31.42	
SN-126	1.00E+05Y	1.00	4.185E-01	4.185E-01	1.315E-01	31.42	
CS-135	2.30E+06Y	1.00	6.349E-01	6.349E-01	3.205E-01	50.49	
PM-147	2.62Y	1.02	3.460E+04	3.540E+04	5.267E+04	148.80	
HG-203	46.61D	1.60	7.039E-02	1.127E-01	0.756E-01	67.06	
TL-208	1.91Y	1.03	6.701E-01	6.915E-01	1.024E-01	14.81	
BI-211	7.04E+08Y	1.00	3.281E+00	3.281E+00	0.540E+00	16.47	
BI-212	1.91Y	1.03	1.229E+00	1.268E+00	0.443E+00	34.93	
PB-212	1.91Y	1.03	2.064E+00	2.130E+00	0.236E+00	11.09	
BI-214	1600.00Y	1.00	1.064E+00	1.064E+00	0.184E+00	17.32	
PB-214	1600.00Y	1.00	1.141E+00	1.141E+00	0.197E+00	17.28	
RA-226	1600.00Y	1.00	1.064E+00	1.064E+00	0.184E+00	17.32	
AC-228	5.75Y	1.01	1.837E+00	1.856E+00	0.377E+00	20.30	
RA-228	5.75Y	1.01	1.837E+00	1.856E+00	0.377E+00	20.30	
TH-228	1.91Y	1.03	2.064E+00	2.130E+00	0.236E+00	11.09	
TH-229	7340.00Y	1.00	2.753E-01	2.753E-01	1.435E-01	52.14	K
TH-230	7.70E+04Y	1.00	1.064E+00	1.064E+00	0.184E+00	17.32	
TH-232	1.41E+10Y	1.00	2.064E+00	2.064E+00	0.229E+00	11.09	
PA-234M	4.47E+09Y	1.00	3.489E+00	3.489E+00	5.296E+00	151.79	
TH-234	4.47E+09Y	1.00	9.572E-01	9.572E-01	20.70E-01	216.20	
U-234	2.45E+05Y	1.00	1.143E+00	1.143E+00	0.212E+00	18.53	
NP-237	2.14E+06Y	1.00	1.229E+00	1.229E+00	0.462E+00	37.59	
U-238	4.47E+09Y	1.00	9.572E-01	9.572E-01	20.70E-01	216.20	
ANH-511	1.00E+09Y	1.00	1.013E-01	1.013E-01	0.721E-01	71.11	
Total Activity :			3.466E+04	3.546E+04			

Nuclide Type : NATURAL

Nuclide	Hlife	Decay	Uncorrected pCi/GRAM	Decay Corr pCi/GRAM	Decay Corr 2-Sigma Error	2-Sigma %Error	Flags
RA-224	1.91Y	1.03	3.703E+00	3.821E+00	1.289E+00	33.74	
Total Activity :			3.703E+00	3.821E+00			

Grand Total Activity : 3.466E+04 3.546E+04

Flags: "K" = Keyline not found "M" = Manually accepted
 "E" = Manually edited "A" = Nuclide specific abn. limit

It	Energy	Area	Bkgnd	FWHM	Channel	Left	Pw	Cts/Sec	%Err	%Eff	Flags
3	128.94	133	315	1.17	256.31	250	14	1.85E-02	48.0	6.08E+00	
3	131.25	29	264	0.99	260.93	250	14	4.02E-03	****	6.08E+00	T
0	154.32	52	308	0.53	307.03	304	7	7.24E-03	****	5.84E+00	T
0	185.98	196	363	1.41	370.30	366	10	2.73E-02	40.3	5.33E+00	T
0	259.27	18	134	1.25	516.79	514	6	2.54E-03	****	4.29E+00	T
0	327.88	97	129	1.24	653.92	651	7	1.35E-02	43.5	3.65E+00	T
0	409.31	29	83	0.77	816.71	814	6	4.02E-03	****	3.14E+00	
0	492.44	27	76	1.57	982.91	979	9	3.74E-03	****	2.76E+00	T
0	648.69	22	56	1.33	1295.33	1292	8	3.03E-03	****	2.24E+00	T
0	839.30	20	58	1.64	1676.50	1673	9	2.75E-03	****	1.80E+00	
0	874.83	22	39	2.40	1747.57	1744	10	3.09E-03	****	1.73E+00	T
0	918.77	28	33	1.23	1835.47	1830	12	3.85E-03	91.2	1.65E+00	T
0	940.49	28	25	1.50	1878.92	1876	8	3.93E-03	71.0	1.62E+00	
0	1062.39	16	27	1.30	2122.77	2120	8	2.22E-03	****	1.44E+00	T
0	1134.09	19	22	2.19	2266.22	2263	7	2.65E-03	94.1	1.36E+00	T
0	1400.26	5	110	11.19	2798.82	2789	49	6.49E-04	****	1.13E+00	T
0	1494.44	19	6	2.19	2987.32	2983	11	2.63E-03	68.8	1.07E+00	
0	1510.00	26	7	5.23	3018.47	3011	15	3.61E-03	61.6	1.07E+00	
4	1586.38	33	2	2.96	3171.35	3166	23	4.52E-03	41.5	1.03E+00	
4	1591.61	30	11	3.16	3181.83	3166	23	4.12E-03	60.5	1.03E+00	
0	1638.59	18	3	3.76	3275.87	3269	14	2.47E-03	64.8	1.01E+00	
0	1728.47	24	11	1.82	3455.81	3449	16	3.29E-03	77.0	9.89E-01	
0	1763.32	79	10	2.14	3525.59	3515	21	1.09E-02	31.5	9.82E-01	
0	1788.58	10	3	3.55	3576.17	3570	11	1.32E-03	****	9.77E-01	
3	1840.37	16	1	3.01	3679.87	3674	26	2.26E-03	62.7	9.69E-01	
3	1846.19	20	6	3.02	3691.51	3674	26	2.83E-03	70.2	9.68E-01	
0	1908.44	11	3	1.01	3816.17	3809	12	1.50E-03	88.6	9.63E-01	

Flags: "T" = Tentatively associated

```

*****
*                                     GENERAL ENG. LABS, LLC.                               *
*                                     2040 Savage Road                                   *
*                                     Charleston, SC 29414                             *
*****
*                                     DETECTOR DATA                                   *
* Configuration      : DKA300:[CANBERRA.GAMMA.ARCHIVE.GAMMA]G158269001.CNF;1          *
* Acquisition date   : 10-APR-2006 21:53:09  Detector SN#      : 1922864              *
* Detector ID        : GAMMA16                Sensitivity       : 3.00000              *
* Geometry           : CAN                    Energy tolerance   : 2.00000              *
* Elapsed live time  : 0 02:00:00.00          Abundance limit      : 75.00000              *
* Elapsed real time  : 0 02:00:01.36          Half life ratio      : 8.00000              *
*****
*                                     SAMPLE DATA                                   *
* Sample date        : 10-MAR-2006 07:46:00  Nuclide Library   : EPI                  *
* Sample ID          : G158269001            Analyst initials    : MJH1                  *
* Batch Number       : 513802                Sample Quantity    : 1.48700E+02 GRAM          *
*****
*                                     QC DATA                                       *
* CALIB. DATE/TIME  : 5-APR-2006 19:34:04.74MS Isotope       :                    *
* MSD DPM           :                        MSD Isotope       :                    *
* LCS DPM           :                        LCS Isotope       :                    *
*****

```

Combined Activity-MDA Report

---- Identified Nuclides ----

Nuclide	Activity (pCi/GRAM)	Act error	MDA (pCi/GRAM)	MDA error	Act/MDA
K-40	2.936E+01	2.624E+00	5.422E-01	3.579E-02	54.158
CO-57	1.755E-02	2.611E-02	4.185E-02	3.243E-03	0.419
ZN-65	1.142E-01	8.614E-02	1.525E-01	1.155E-02	0.749
CD-109	4.284E+00	1.346E+00	1.214E+00	1.285E-01	3.530
SN-126	4.185E-01	1.315E-01	1.195E-01	1.263E-02	3.501
CS-135	6.349E-01	3.205E-01	2.301E-01	2.198E-02	2.759
PM-147	3.540E+04	5.267E+04	8.033E+04	6.229E+03	0.441
HG-203	1.127E-01	7.555E-02	7.830E-02	6.489E-03	1.439
TL-208	6.915E-01	1.024E-01	5.807E-02	4.065E-03	11.908
BI-211	3.281E+00	5.404E-01	2.931E-01	2.151E-02	11.192
BI-212	1.268E+00	4.430E-01	3.824E-01	3.296E-02	3.317
PB-212	2.130E+00	2.363E-01	8.485E-02	8.029E-03	25.107
BI-214	1.064E+00	1.842E-01	1.035E-01	8.339E-03	10.274
PB-214	1.141E+00	1.972E-01	1.015E-01	9.129E-03	11.239
RA-224	3.821E+00	1.289E+00	9.654E-01	8.035E-02	3.958
RA-226	1.064E+00	1.842E-01	1.035E-01	8.339E-03	10.274
AC-228	1.856E+00	3.767E-01	1.753E-01	2.068E-02	10.587
RA-228	1.856E+00	3.767E-01	1.753E-01	2.068E-02	10.587

---- Identified Nuclides ----

Nuclide	Activity (pCi/GRAM)	Act error	MDA (pCi/GRAM)	MDA error	Act/MDA
TH-228	2.130E+00	2.363E-01	8.484E-02	8.028E-03	25.109
TH-229	7.183E-02	4.854E-01	8.273E-01	6.919E-02	0.087
TH-230	1.064E+00	1.842E-01	1.035E-01	8.339E-03	10.274
TH-232	2.064E+00	2.290E-01	8.221E-02	7.780E-03	25.110
PA-234M	3.489E+00	5.296E+00	7.143E+00	7.166E-01	0.488
TH-234	9.572E-01	2.070E+00	2.999E+00	5.968E-01	0.319
U-234	1.143E+00	2.117E-01	1.970E-01	1.973E-02	5.800
NP-237	1.229E+00	4.620E-01	3.581E-01	8.295E-02	3.432
U-238	9.572E-01	2.070E+00	2.999E+00	5.968E-01	0.319
ANH-511	1.013E-01	7.206E-02	4.702E-02	2.861E-03	2.155

---- Non-Identified Nuclides ----

Nuclide	Key-Line Activity (pCi/GRAM)	K.L. Ided	Act error	MDA (pCi/GRAM)	MDA error	Act/MDA
BE-7	-3.741E-02		3.651E-01	6.396E-01	4.439E-02	-0.058
NA-22	-2.812E-03		3.568E-02	6.382E-02	4.147E-03	-0.044
AL-26	7.827E-03		2.588E-02	5.267E-02	3.031E-03	0.149
SC-46	9.994E-03		4.081E-02	7.202E-02	6.673E-03	0.139
V-48	-3.218E-02		1.261E-01	2.236E-01	1.980E-02	-0.144
CR-51	-2.270E-01		5.181E-01	8.395E-01	6.676E-02	-0.270
MN-54	5.693E-03		4.029E-02	6.944E-02	5.867E-03	0.082
CO-56	4.246E-03		4.159E-02	7.239E-02	6.243E-03	0.059
CO-58	9.016E-04		3.753E-02	6.554E-02	5.325E-03	0.014
FE-59	-5.260E-02		1.019E-01	1.746E-01	1.489E-02	-0.301
CO-60	2.867E-03		3.390E-02	6.201E-02	3.859E-03	0.046
SE-75	-2.117E-02		5.036E-02	7.287E-02	5.983E-03	-0.290
KR-85	6.534E+00		7.118E+00	1.183E+01	7.202E-01	0.552
SR-85	3.983E-02		4.340E-02	7.211E-02	4.391E-03	0.552
Y-88	-5.413E-03		3.128E-02	5.105E-02	2.904E-03	-0.106
Y-91	1.328E-02		4.137E-02	7.402E-02	4.547E-03	0.179
NB-94	2.676E-02		2.856E-02	5.327E-02	3.541E-03	0.502
NB-95	7.484E-02		7.479E-02	1.230E-01	9.200E-03	0.609
ZR-95	1.304E-02		7.886E-02	1.381E-01	1.155E-02	0.094
RU-103	1.821E-02		4.871E-02	8.793E-02	1.123E-02	0.207
RH-106	-5.034E-02		2.837E-01	4.899E-01	3.020E-02	-0.103
RU-106	-6.735E-02		2.825E-01	4.854E-01	5.786E-02	-0.139
AG-108M	1.721E-03		2.824E-02	5.034E-02	3.215E-03	0.034
AG-110M	-3.802E-02		3.375E-02	5.327E-02	3.463E-03	-0.714
SN-113	-1.546E-02		4.373E-02	7.615E-02	4.670E-03	-0.203
SN-115	5.546E+00		4.196E+00	8.261E+00	7.603E-01	0.671
SN-117M	2.584E-02		1.140E-01	1.970E-01	1.601E-02	0.131
TE-123M	5.035E-03		2.843E-02	4.897E-02	4.012E-03	0.103
SB-124	-1.900E-02		7.777E-02	1.383E-01	9.005E-03	-0.137
SB-125	-2.811E-02		7.679E-02	1.334E-01	8.164E-03	-0.211
TE-125M	5.418E+00		1.038E+01	1.835E+01	1.842E+00	0.295
I-126	-6.230E-02		4.048E-01	6.943E-01	4.304E-02	-0.090
SB-126	8.033E-02		3.100E-01	5.506E-01	3.786E-02	0.146

---- Non-Identified Nuclides ----

Nuclide	Key-Line Activity (pCi/GRAM)	K.L. Ided	Act error	MDA (pCi/GRAM)	MDA error	Act/MDA
I-131	1.183E-01		4.094E-01	7.433E-01	5.430E-02	0.159
BA-133	-2.409E-03		4.085E-02	6.426E-02	7.727E-03	-0.037
CS-134	1.244E-01	+	6.553E-02	7.946E-02	6.314E-03	1.565
CS-136	4.694E-02		2.227E-01	4.100E-01	3.566E-02	0.114
BA-137M	1.961E-02		3.308E-02	5.989E-02	3.678E-03	0.327
CS-137	2.084E-02		3.498E-02	6.334E-02	3.905E-03	0.329
CE-139	-2.080E-02		3.027E-02	5.006E-02	4.154E-03	-0.416
BA-140	-1.207E-01		5.178E-01	8.967E-01	2.921E-01	-0.135
LA-140	1.217E-02		1.587E-01	2.647E-01	1.636E-02	0.046
CE-141	-3.946E-04		7.789E-02	1.337E-01	1.076E-02	-0.003
CE-144	1.062E-02		2.068E-01	3.206E-01	4.840E-02	0.033
PM-144	1.853E-02		3.206E-02	5.799E-02	3.820E-03	0.320
PM-146	1.509E-02		3.989E-02	7.208E-02	6.292E-03	0.209
ND-147	-1.415E-01		1.453E+00	2.537E+00	3.466E-01	-0.056
EU-152	2.478E-04		8.618E-02	1.437E-01	1.088E-02	0.002
GD-153	9.613E-02	+	1.095E-01	1.267E-01	1.156E-02	0.759
EU-154	-8.023E-03		9.880E-02	1.767E-01	1.728E-02	-0.045
EU-155	1.288E-01		1.043E-01	1.881E-01	1.606E-02	0.685
TB-160	4.031E-02		1.653E-01	2.572E-01	2.345E-02	0.157
TM-171	-2.809E+01		3.723E+01	5.688E+01	6.499E+00	-0.494
HF-181	-1.913E-03		4.603E-02	8.141E-02	4.907E-03	-0.023
TA-182	-3.218E-02		1.904E-01	3.330E-01	2.226E-02	-0.097
IR-192	3.775E-03		3.685E-02	6.195E-02	4.654E-03	0.061
BI-207	3.736E-02	+	4.575E-02	8.522E-02	6.934E-03	0.438
BI-210	2.445E+00		1.216E+01	1.839E+01	1.878E+00	0.133
PB-210	2.445E+00		1.216E+01	1.839E+01	1.878E+00	0.133
PB-211	4.069E-02		8.075E-01	1.438E+00	8.965E-01	0.028
RN-219	1.315E-01		3.530E-01	6.409E-01	8.714E-02	0.205
RA-223	1.654E-01		6.284E-01	1.061E+00	1.817E-01	0.156
AC-227	-2.314E-01		4.127E-01	5.900E-01	9.021E-02	-0.392
TH-227	-2.274E-01		4.063E-01	5.800E-01	1.037E-01	-0.392
PA-231	-1.881E-01		1.421E+00	2.362E+00	3.502E-01	-0.080
TH-231	7.469E-01	+	3.767E-01	3.552E-01	3.283E-02	2.103
PA-233	4.340E-03		6.020E-02	1.009E-01	7.919E-03	0.043
PA-234	-6.910E-02		2.616E-01	4.637E-01	8.810E-02	-0.149
U-235	-7.358E-02		1.856E-01	3.128E-01	5.362E-02	-0.235
NP-239	-6.734E-02		1.693E-01	2.887E-01	2.273E-02	-0.233
AM-241	-1.484E-01		2.433E-01	3.766E-01	5.100E-02	-0.394
AM-242	1.493E+00		2.059E+00	3.671E+00	3.137E-01	0.407
CM-247	-1.651E-03		3.199E-02	5.669E-02	3.279E-03	-0.029
CF-249	3.075E-02		3.656E-02	6.775E-02	3.961E-03	0.454
CF-251	2.776E-02		1.166E-01	2.005E-01	1.668E-02	0.139

```

*****
*
*                               General Engineering Labs, LLC
*                               2040 SAVAGE ROAD
*                               CHARLESTON ,SC 29417
*                               GROSS GAMMA REPORT
*
*****
*
*   BATCH ID      : 513802                SAMPLE ID   : G158269001
*   ANALYST       : MJH1                  DETECTOR    : GAMMA16
*   SAMPLE DATE   : 10-MAR-2006 07:46:00.00  COUNT TIME  : 0 02:00:00.00
*   ANALYSIS DATE: 10-APR-2006 21:53:09.84  SAMPLE ALQT: 148.700 GRAM
*
*****

```

```

GROSS GAMMA ACTIVITY (pCi/GRAM ) : 1.016E+01
GROSS GAMMA ERROR (pCi/GRAM ) : 2.855E+00
GROSS GAMMA MDA (pCi/GRAM ) : 6.650E+00
GROSS GAMMA DLC (pCi/GRAM ) : 3.215E+00

```

VAX/VMS Nuclide Identification Report Generated 11-APR-2006 05:58:24.90

```

*****
*                               GENERAL ENG. LABS, LLC.                               *
*                               2040 Savage Road                                       *
*                               Charleston, SC 29414                                   *
*****
Configuration      : DKA300:[CANBERRA.GAMMA.ARCHIVE.GAMMA]G158269002.CNF;1
Sample date        : 10-MAR-2006 07:55:00 Acquisition date : 10-APR-2006 23:57:35
Sample ID          : G158269002 Sample quantity : 1.43550E+02 GRAM
Detector name     : GAMMA16 Detector geometry: CAN
Elapsed live time : 0 06:00:00.00 Elapsed real time: 0 06:00:03.45 0.0%
Energy tolerance  : 2.00000 KEV Analyst Initials : MJH1
Abundance limit   : 75.00000 Sensitivity : 3.00000
Batch ID          : 513802 Detector SN# : 1922864
Matrix Spike DPM  : LCS DPM :
*****

```

Pk	It	Energy	Area	Bkgnd	FWHM	Channel	Left	Pw	Cts/Sec	%Err	Fit
1	0	62.50*	59	949	1.28	123.53	121	8	2.72E-03	97.3	
2	3	74.74*	884	1156	1.30	147.98	142	17	4.09E-02	7.6	5.30E+00
3	3	77.02*	1301	793	0.99	152.56	142	17	6.02E-02	4.7	
4	5	83.90*	276	846	1.54	166.29	163	27	1.28E-02	19.3	2.24E+00
5	5	87.12*	613	1214	1.71	172.73	163	27	2.84E-02	11.7	
6	5	89.83	340	731	1.06	178.15	163	27	1.57E-02	13.9	
7	5	92.71*	459	980	1.28	183.89	163	27	2.12E-02	13.9	
8	0	128.82*	206	1049	1.61	256.06	251	10	9.52E-03	30.9	
9	0	143.50*	44	790	0.92	285.40	283	7	2.05E-03	113.0	
10	0	154.20	81	984	0.93	306.78	303	9	3.76E-03	70.5	
11	0	185.76*	521	1199	1.06	369.87	364	12	2.41E-02	14.6	
12	0	209.13	274	782	1.08	416.58	413	9	1.27E-02	19.4	
13	3	238.48*	3012	492	1.18	475.24	467	23	1.39E-01	2.3	2.76E+00
14	3	241.59*	950	627	1.71	481.45	467	23	4.40E-02	7.2	
15	0	270.11	242	707	1.41	538.46	534	11	1.12E-02	22.2	
16	0	277.25	132	320	1.40	552.72	550	6	6.09E-03	23.2	
17	0	280.95*	59	432	1.05	560.11	557	8	2.75E-03	63.9	
18	0	295.04*	1299	660	1.18	588.29	582	12	6.01E-02	4.9	
19	0	300.09*	189	506	1.10	598.37	594	10	8.77E-03	24.2	
20	0	304.92	48	266	1.27	608.03	606	6	2.20E-03	56.2	
21	0	314.16	61	444	0.72	626.50	623	10	2.80E-03	66.3	
22	0	327.81	154	377	1.09	653.79	649	8	7.12E-03	23.4	
23	0	338.20*	687	591	1.33	674.56	669	14	3.18E-02	8.8	
24	0	351.64*	2319	557	1.24	701.42	694	14	1.07E-01	3.1	
25	0	409.05*	101	282	1.10	816.19	812	8	4.70E-03	32.6	
26	0	462.63	235	328	1.48	923.30	917	13	1.09E-02	17.2	
27	0	510.67*	301	471	1.94	1019.34	1011	19	1.39E-02	21.5	
28	0	520.47*	18	148	1.36	1038.94	1037	7	8.44E-04	118.8	
29	0	582.80*	935	200	1.44	1163.56	1159	9	4.33E-02	4.4	
30	0	608.91*	1744	352	1.61	1215.77	1211	14	8.07E-02	3.4	
31	0	665.04	44	187	1.45	1328.01	1325	11	2.02E-03	62.8	
32	0	726.77	238	159	1.44	1451.45	1448	11	1.10E-02	12.3	
33	0	754.58	23	153	0.92	1507.08	1504	9	1.04E-03	101.6	
34	0	768.08*	210	223	1.01	1534.08	1527	17	9.72E-03	18.3	
35	0	785.26	63	182	1.64	1568.44	1563	12	2.91E-03	44.8	
36	0	794.21*	98	163	1.69	1586.33	1581	11	4.55E-03	28.3	
37	0	836.13*	16	190	0.99	1670.17	1662	11	7.21E-04	178.1	
38	0	859.92*	144	143	1.93	1717.74	1712	13	6.68E-03	21.7	

Pk	It	Energy	Area	Bkgnd	FWHM	Channel	Left	Pw	Cts/Sec	%Err	Fit
39	0	910.59*	647	161	1.73	1819.11	1813	16	3.00E-02	6.1	
40	0	933.24*	67	112	1.35	1864.41	1859	10	3.11E-03	34.6	
41	1	963.94*	150	119	2.02	1925.81	1919	25	6.92E-03	17.5	1.22E+00
42	1	968.17*	409	116	1.92	1934.27	1919	25	1.90E-02	7.6	
43	0	1073.65	24	63	1.29	2145.29	2142	7	1.11E-03	58.5	
44	0	1119.58*	390	157	1.66	2237.19	2230	15	1.81E-02	8.9	
45	0	1152.68	23	184	0.97	2303.41	2303	15	1.07E-03	129.0	
46	0	1166.04	27	46	1.39	2330.13	2328	6	1.24E-03	44.5	
47	0	1175.29	40	114	4.06	2348.64	2343	11	1.86E-03	54.1	
48	0	1236.96	166	170	1.96	2472.04	2465	16	7.71E-03	19.1	
49	0	1279.81	22	110	1.20	2557.77	2551	12	1.03E-03	96.6	
50	0	1377.33	135	90	1.85	2752.95	2745	18	6.25E-03	18.6	
51	0	1400.39	63	75	4.43	2799.09	2789	19	2.91E-03	35.5	
52	0	1459.64*	2249	91	1.94	2917.68	2907	19	1.04E-01	2.4	
53	0	1496.63	10	70	5.30	2991.70	2985	14	4.63E-04	180.3	
54	5	1507.95*	59	65	3.41	3014.36	3004	21	2.71E-03	37.5	1.82E+00
55	5	1511.77	12	13	1.34	3022.02	3004	21	5.36E-04	62.5	
56	0	1527.52*	6	33	3.36	3053.53	3047	12	2.96E-04	217.9	
57	0	1591.53*	22	39	1.33	3181.67	3178	11	1.00E-03	69.0	
58	0	1620.56*	28	17	1.03	3239.79	3234	12	1.29E-03	40.8	
59	0	1630.09*	24	27	2.62	3258.87	3255	10	1.11E-03	49.1	
60	0	1661.08*	22	37	1.66	3320.89	3314	15	1.03E-03	67.6	
61	0	1674.55	16	22	3.28	3347.87	3343	14	7.63E-04	64.1	
62	4	1728.53	79	25	3.24	3455.94	3446	44	3.64E-03	19.7	1.18E+00
63	4	1738.54	22	21	3.25	3475.98	3446	44	1.03E-03	57.0	
64	0	1763.33*	315	17	2.33	3525.62	3518	19	1.46E-02	7.0	
65	0	1792.11	12	21	5.75	3583.23	3574	14	5.54E-04	86.2	
66	0	1846.76	37	36	2.56	3692.65	3689	18	1.71E-03	41.4	
67	0	1877.19*	40	41	11.80	3753.59	3738	29	1.84E-03	50.7	
68	0	1900.01	16	31	6.01	3799.28	3791	18	7.38E-04	86.2	
69	0	1948.41	12	3	1.08	3896.21	3894	6	5.60E-04	38.5	
70	0	2019.99	21	62	12.23	4039.56	4025	36	9.70E-04	121.7	

Flag: "*" = Peak area was modified by background subtraction

VAX/VMS Nuclide Identification Report Generated

```

*****
*                               General Eng. Labs, LLC.                               *
*                               2040 Savage Road                                       *
*                               Charleston, SC 29414                                   *
*****
*                               DETECTOR DATA                                       *
*
* Configuration      : DKA300:[CANBERRA.GAMMA.ARCHIVE.GAMMA]G158269002
* Acquisition date   : 10-APR-2006 23:57:35 Detector SN#      : 1922864
* Detector ID       : GAMMA16                      Sensitivity    : 3.000
* Geometry          : CAN                          Energy tolerance: 2.000
* Elapsed live time: 0 06:00:00.00                Abundance limit : 75.000
* Elapsed real time: 0 06:00:03.45                Half life ratio  : 8.000
*****
*                               SAMPLE DATA                                         *
*
* Sample date       : 10-MAR-2006 07:55:00 Nuclide Library :
* Sample ID        : G158269002                    Analyst initials: MJH1
* Batch Number     : 513802                         Sample Quantity : 1.4355E+02 GRAM
* Recovery         : 1.00000                        Carrier Weight  : 0.00000
*****
*                               QC DATA                                             *
*
* Standard Weight  : 0.00000
* CALIB. DATE/TIME : 5-APR-2006 19:34:04 MS Isotope      :
* MSD DPM          : 0.000                          MSD Isotope     :
* LCS DPM          : 0.000                          LCS Isotope     :
* LCSD DPM        : 0.000                          LCSD Isotope    :
*****

```

Combined Activity-MDA Report

---- Identified Nuclides ----

Nuclide	Activity (pCi/GRAM)	Act error	MDA (pCi/GRAM)	
K-40	1.681E+01	1.367E+00	2.856E-01	0.000E+00
MN-54	8.098E-03	2.885E-02	3.321E-02	0.000E+00
CD-109	3.188E+00	8.200E-01	6.666E-01	0.000E+00
SN-126	3.114E-01	8.009E-02	6.565E-02	0.000E+00
CS-135	3.155E-01	1.433E-01	1.302E-01	0.000E+00
CE-141	1.880E-02	4.297E-02	7.834E-02	0.000E+00
HG-203	2.645E-02	3.388E-02	4.270E-02	0.000E+00
TL-208	4.098E-01	4.613E-02	2.977E-02	0.000E+00
BI-211	4.482E+00	4.279E-01	1.606E-01	0.000E+00
BI-212	8.899E-01	2.322E-01	2.457E-01	0.000E+00
PB-212	1.338E+00	1.405E-01	4.943E-02	0.000E+00
BI-214	1.393E+00	1.463E-01	5.789E-02	0.000E+00
PB-214	1.559E+00	1.696E-01	5.703E-02	0.000E+00
RA-223	-3.243E-01	3.878E-01	5.532E-01	0.000E+00
RA-224	4.804E+00	8.022E-01	5.623E-01	0.000E+00
RA-226	1.393E+00	1.463E-01	5.789E-02	0.000E+00
AC-228	1.235E+00	2.104E-01	9.477E-02	0.000E+00
RA-228	1.235E+00	2.104E-01	9.477E-02	0.000E+00
TH-228	1.338E+00	1.405E-01	4.943E-02	0.000E+00
TH-230	1.393E+00	1.463E-01	5.789E-02	0.000E+00
TH-232	1.296E+00	1.361E-01	4.789E-02	0.000E+00
TH-234	7.875E-01	1.541E+00	1.731E+00	0.000E+00
U-234	1.502E+00	2.111E-01	1.143E-01	0.000E+00
U-235	6.133E-02	1.390E-01	1.920E-01	0.000E+00
NP-237	9.145E-01	3.015E-01	1.967E-01	0.000E+00
U-238	7.875E-01	1.541E+00	1.731E+00	0.000E+00
ANH-511	9.753E-02	4.240E-02	2.456E-02	0.000E+00

---- Non-Identified Nuclides ----

Nuclide	Key-Line Activity (pCi/GRAM)	K.L. Act error) Ided	MDA (pCi/GRAM)
---------	-------------------------------------	--------------------------	--------------------

BE-7	-6.907E-02	1.917E-01	3.365E-01	0.000E+00	NOT IDENT.
NA-22	3.308E-03	2.394E-02	3.681E-02	0.000E+00	NOT IDENT.
NA-24	0.000E+00	3.357E+13	0.000E+00	0.000E+00	SHORT HLIF
AL-26	1.139E-04	1.234E-02	2.308E-02	0.000E+00	FAIL ABUN
SC-46	6.199E-03	2.023E-02	3.537E-02	0.000E+00	FAIL ABUN
V-48	4.247E-02	6.689E-02	1.240E-01	0.000E+00	NOT IDENT.
CR-51	1.032E-01	2.797E-01	4.839E-01	0.000E+00	NOT IDENT.
CO-56	-1.101E-02	2.024E-02	3.345E-02	0.000E+00	FAIL ABUN
MN-56	0.000E+00	1.839E+41	0.000E+00	0.000E+00	SHORT HLIF
CO-57	6.563E-03	1.261E-02	2.316E-02	0.000E+00	NOT IDENT.
CO-58	-1.092E-02	2.109E-02	3.507E-02	0.000E+00	NOT IDENT.
FE-59	-1.999E-03	5.229E-02	9.264E-02	0.000E+00	NOT IDENT.
CO-60	-1.013E-02	1.727E-02	2.898E-02	0.000E+00	NOT IDENT.
ZN-65	-7.778E-06	4.858E-02	7.454E-02	0.000E+00	NOT IDENT.
SE-75	-1.061E-02	2.408E-02	4.084E-02	0.000E+00	FAIL ABUN
KR-85	2.187E+00	3.686E+00	5.942E+00	0.000E+00	NOT IDENT.
SR-85	1.336E-02	2.251E-02	3.629E-02	0.000E+00	NOT IDENT.
Y-88	-4.126E-03	1.701E-02	3.052E-02	0.000E+00	NOT IDENT.
Y-91	-6.322E-03	2.099E-02	3.651E-02	0.000E+00	NOT IDENT.
NB-94	8.038E-03	1.598E-02	2.837E-02	0.000E+00	NOT IDENT.
NB-95	0.000E+00	3.632E-02	6.238E-02	0.000E+00	NOT IDENT.
NB-95M	0.000E+00	2.709E+01	0.000E+00	0.000E+00	SHORT HLIF
ZR-95	3.558E-03	4.687E-02	7.102E-02	0.000E+00	NOT IDENT.
MO-99	0.000E+00	3.856E+01	0.000E+00	0.000E+00	SHORT HLIF
TC-99M	0.000E+00	2.115E+36	0.000E+00	0.000E+00	SHORT HLIF
RU-103	-9.947E-03	2.566E-02	4.483E-02	0.000E+00	FAIL ABUN
RH-106	8.652E-02	1.507E-01	2.719E-01	0.000E+00	FAIL ABUN
RU-106	1.130E-01	1.527E-01	2.767E-01	0.000E+00	NOT IDENT.
AG-108M	-6.626E-03	1.571E-02	2.771E-02	0.000E+00	NOT IDENT.
AG-110M	-2.079E-02	1.741E-02	2.831E-02	0.000E+00	NOT IDENT.
SN-113	3.266E-03	2.331E-02	4.233E-02	0.000E+00	NOT IDENT.
CD-115	0.000E+00	8.661E+02	0.000E+00	0.000E+00	SHORT HLIF
SN-115	0.000E+00	3.093E+00	4.330E+00	0.000E+00	FAIL ABUN
SN-117M	3.004E-03	6.149E-02	1.097E-01	0.000E+00	FAIL ABUN
TE-123M	-1.095E-03	1.498E-02	2.664E-02	0.000E+00	NOT IDENT.
SB-124	-1.665E-02	4.427E-02	7.461E-02	0.000E+00	NOT IDENT.
SB-125	2.025E-02	4.487E-02	8.197E-02	0.000E+00	FAIL ABUN
TE-125M	2.004E+00	5.430E+00	9.991E+00	0.000E+00	NOT IDENT.
I-126	2.374E-01	2.983E-01	3.648E-01	0.000E+00	FAIL ABUN
SB-126	1.293E-01	1.712E-01	3.080E-01	0.000E+00	FAIL ABUN
SB-127	0.000E+00	1.261E+01	0.000E+00	0.000E+00	SHORT HLIF
I-131	-7.250E-02	2.225E-01	3.995E-01	0.000E+00	NOT IDENT.
I-132	0.000E+00	7.541E+41	0.000E+00	0.000E+00	SHORT HLIF
TE-132	0.000E+00	1.219E+01	0.000E+00	0.000E+00	SHORT HLIF
BA-133	1.016E-02	2.185E-02	3.595E-02	0.000E+00	FAIL ABUN
I-133	0.000E+00	1.603E+09	0.000E+00	0.000E+00	SHORT HLIF
CS-134	0.000E+00	3.125E-02	3.947E-02	0.000E+00	FAIL ABUN
I-135	0.000E+00	3.667E+33	0.000E+00	0.000E+00	SHORT HLIF
CS-136	2.304E-03	1.153E-01	2.060E-01	0.000E+00	FAIL ABUN
BA-137M	2.591E-02	1.833E-02	3.076E-02	0.000E+00	NOT IDENT.
CS-137	2.740E-02	1.938E-02	3.252E-02	0.000E+00	NOT IDENT.
CE-139	-2.368E-03	1.606E-02	2.840E-02	0.000E+00	NOT IDENT.
BA-140	1.494E-01	2.893E-01	5.190E-01	0.000E+00	FAIL ABUN
LA-140	3.313E-02	1.028E-01	1.646E-01	0.000E+00	FAIL ABUN
CE-143	0.000E+00	1.878E+06	0.000E+00	0.000E+00	SHORT HLIF
CE-144	-5.424E-02	1.024E-01	1.814E-01	0.000E+00	NOT IDENT.
PM-144	-1.293E-02	1.653E-02	2.742E-02	0.000E+00	NOT IDENT.
PR-144	0.000E+00	1.279E+41	0.000E+00	0.000E+00	SHORT HLIF
PM-146	1.822E-02	2.061E-02	3.814E-02	0.000E+00	NOT IDENT.
ND-147	1.576E-01	7.078E-01	1.271E+00	0.000E+00	FAIL ABUN
PM-147	-1.244E+03	2.573E+04	4.659E+04	0.000E+00	NOT IDENT.
PM-149	0.000E+00	8.651E+03	0.000E+00	0.000E+00	SHORT HLIF
EU-152	-1.389E-03	4.786E-02	8.108E-02	0.000E+00	FAIL ABUN
GD-153	-1.513E-02	4.008E-02	7.287E-02	0.000E+00	FAIL ABUN
EU-154	8.836E-03	6.629E-02	1.019E-01	0.000E+00	NOT IDENT.
EU-155	1.312E-02	5.154E-02	9.486E-02	0.000E+00	FAIL ABUN
TB-160	-6.873E-02	7.733E-02	1.237E-01	0.000E+00	FAIL ABUN
TM-171	6.345E+00	1.979E+01	3.377E+01	0.000E+00	NOT IDENT.
HF-181	-8.638E-03	2.592E-02	4.556E-02	0.000E+00	NOT IDENT.
TA-182	-1.023E-01	1.070E-01	1.760E-01	0.000E+00	FAIL ABUN
IR-192	2.126E-03	2.209E-02	3.369E-02	0.000E+00	FAIL ABUN
BI-207	1.974E-02	2.416E-02	4.494E-02	0.000E+00	NOT IDENT.
BI-210	-5.823E-01	6.765E+00	1.072E+01	0.000E+00	NOT IDENT.
PB-210	-5.823E-01	6.765E+00	1.072E+01	0.000E+00	NOT IDENT.
PB-211	-9.755E-02	4.599E-01	8.141E-01	0.000E+00	NOT IDENT.
RN-219	1.363E-01	1.992E-01	3.664E-01	0.000E+00	FAIL ABUN
AC-227	-7.112E-02	1.942E-01	3.309E-01	0.000E+00	FAIL ABUN
TH-227	-6.991E-02	1.910E-01	3.253E-01	0.000E+00	FAIL ABUN

TH-229	-7.977E-02	2.596E-01	4.519E-01	0.000E+00	FAIL	ABUN
PA-231	2.362E-01	8.728E-01	1.350E+00	0.000E+00	FAIL	ABUN
TH-231	0.000E+00	1.684E-01	1.904E-01	0.000E+00	FAIL	ABUN
PA-233	2.331E-02	3.493E-02	5.495E-02	0.000E+00	FAIL	ABUN
PA-234	2.763E-02	1.397E-01	2.533E-01	0.000E+00	FAIL	ABUN
PA-234M	3.020E+00	2.165E+00	4.111E+00	0.000E+00	FAIL	ABUN
NP-239	6.801E-04	9.238E-02	1.678E-01	0.000E+00	FAIL	ABUN
AM-241	-4.492E-02	1.296E-01	2.181E-01	0.000E+00	NOT IDENT.	
AM-242	6.846E-03	1.037E+00	1.899E+00	0.000E+00	NOT IDENT.	
CM-247	1.447E-02	1.790E-02	3.316E-02	0.000E+00	FAIL	ABUN
CF-249	2.687E-02	1.937E-02	3.660E-02	0.000E+00	NOT IDENT.	
CF-251	4.187E-02	6.188E-02	1.115E-01	0.000E+00	NOT IDENT.	

```

*****
*                               GENERAL ENG. LABS, LLC.                               *
*                               2040 Savage Road                                       *
*                               Charleston, SC 29414                                   *
*****
Configuration      : DKA300:[CANBERRA.GAMMA.ARCHIVE.GAMMA]G158269002.CNF;1
Sample date        : 10-MAR-2006 07:55:00 Acquisition date : 10-APR-2006 23:57:35
Sample ID          : G158269002 Sample quantity : 1.43550E+02 GRAM
Detector name     : GAMMA16 Detector geometry: CAN
Elapsed live time : 0 06:00:00.00 Elapsed real time: 0 06:00:03.45 0.0%
Energy tolerance  : 2.00000 KEV Analyst Initials : MJH1
Abundance limit   : 75.00000 Sensitivity : 3.00000
Batch ID          : 513802 Detector SN# : 1922864
Matrix Spike DPM : LCS DPM :
*****
    
```

Nuclide Line Activity Report

Nuclide Type:

Nuclide	Energy	Area	%Abn	%Eff	Uncorrected pCi/GRAM	Decay Corr pCi/GRAM	2-Sigma %Error
K-40	1460.81	2249	10.67*	1.093E+00	1.681E+01	1.681E+01	8.13
MN-54	834.83	16	99.83*	1.802E+00	7.547E-03	8.098E-03	356.22
CD-109	88.03	613	3.79*	4.637E+00	3.040E+00	3.188E+00	25.72
SN-126	64.28	59	9.60	1.711E+00	3.117E-01	3.117E-01	195.41
	86.94	613	8.90	4.637E+00	1.295E+00	1.295E+00	47.93
	87.57	613	37.00*	4.637E+00	3.114E-01	3.114E-01	25.72
CS-135	268.24	242	16.00*	4.171E+00	3.155E-01	3.155E-01	45.42
CE-141	145.44	44	48.40*	5.983E+00	1.330E-02	2.621E-02	226.15
HG-203	70.83	-----	4.75	2.802E+00	-----	Line Not Found	-----
	72.87	884	8.00	3.302E+00	2.918E+00	4.682E+00	21.06
	82.60	276	3.55	4.334E+00	1.564E+00	2.509E+00	41.43
	279.20	59	77.30*	4.061E+00	1.649E-02	2.645E-02	128.07
TL-208	75.00	884	3.43	3.302E+00	6.806E+00	7.025E+00	20.50
	277.35	132	6.80	4.098E+00	4.117E-01	4.249E-01	47.99
	510.84	301	21.60	2.690E+00	4.515E-01	4.660E-01	44.26
	583.14	935	84.20*	2.437E+00	3.970E-01	4.098E-01	11.26
	763.30	-----	1.64	1.954E+00	-----	Line Not Found	-----
	860.37	144	12.46	1.757E+00	5.743E-01	5.928E-01	44.47
	1093.90	-----	0.37	1.403E+00	-----	Line Not Found	-----
BI-211	351.07	2319	12.94*	3.485E+00	4.482E+00	4.482E+00	9.55
BI-212	727.18	238	11.80*	2.039E+00	8.622E-01	8.899E-01	26.09
PB-212	74.80	884	10.70	3.302E+00	2.182E+00	2.252E+00	20.76
	87.30	613	8.00	4.637E+00	1.440E+00	1.486E+00	27.60
	115.19	-----	0.60	5.993E+00	-----	Line Not Found	-----
	238.63	3012	44.60*	4.541E+00	1.296E+00	1.338E+00	10.50
	300.09	189	3.41	3.882E+00	1.247E+00	1.287E+00	49.29
BI-214	609.31	1744	46.30*	2.356E+00	1.393E+00	1.393E+00	10.50
	768.36	210	5.04	1.944E+00	1.869E+00	1.869E+00	37.85
	934.06	67	3.21	1.629E+00	1.120E+00	1.120E+00	70.12
	1120.29	390	15.10	1.373E+00	1.642E+00	1.642E+00	20.43
	1238.11	166	5.94	1.253E+00	1.950E+00	1.950E+00	39.13
	1377.67	135	4.11	1.143E+00	2.505E+00	2.505E+00	38.23

Nuclide Type:

Nuclide	Energy	Area	%Abn	%Eff	Uncorrected pCi/GRAM	Decay Corr pCi/GRAM	2-Sigma %Error
PB-214	74.81	884	6.21	3.302E+00	3.759E+00	3.759E+00	19.96
	77.11	1301	10.50	3.581E+00	3.016E+00	3.016E+00	15.95
	87.30	613	4.41	4.637E+00	2.613E+00	2.613E+00	26.98
	241.98	950	7.50	4.501E+00	2.452E+00	2.452E+00	17.61
	295.21	1299	19.20	3.927E+00	1.502E+00	1.502E+00	14.06
RA-223	351.92	2319	37.20*	3.485E+00	1.559E+00	1.559E+00	10.88
	122.32	-----	1.19	6.069E+00	-----	Line Not Found	-----
	144.24	44	3.24	5.983E+00	1.987E-01	1.987E-01	226.19
	154.21	81	5.58	5.844E+00	2.169E-01	2.169E-01	141.29
	269.46	242	13.60	4.171E+00	3.712E-01	3.712E-01	45.18
	323.87	-----	3.88*	3.685E+00	-----	Line Not Found	-----
RA-226	338.28	687	2.73	3.579E+00	6.134E+00	6.134E+00	20.93
	445.03	-----	1.18	2.966E+00	-----	Line Not Found	-----
	295.21	1299	19.20	3.927E+00	1.502E+00	1.502E+00	14.06
	351.92	2319	37.20	3.485E+00	1.559E+00	1.559E+00	9.15
AC-228	609.31	1744	46.30*	2.356E+00	1.393E+00	1.393E+00	10.50
	209.25	274	4.40	4.953E+00	1.097E+00	1.108E+00	74.96
	338.32	687	11.40	3.579E+00	1.469E+00	1.484E+00	44.60
	463.01	235	4.40	2.886E+00	1.613E+00	1.630E+00	41.63
	794.95	98	4.60	1.887E+00	9.870E-01	9.974E-01	61.08
RA-228	911.21	647	27.70*	1.666E+00	1.222E+00	1.235E+00	17.03
	964.77	150	5.20	1.580E+00	1.586E+00	1.603E+00	42.90
	969.11	409	16.60	1.574E+00	1.366E+00	1.381E+00	27.93
	209.25	274	4.40	4.953E+00	1.097E+00	1.108E+00	74.96
	338.32	687	11.40	3.579E+00	1.469E+00	1.484E+00	44.60
	463.01	235	4.40	2.886E+00	1.613E+00	1.630E+00	41.63
TH-228	794.95	98	4.60	1.887E+00	9.870E-01	9.974E-01	61.08
	911.21	647	27.70*	1.666E+00	1.222E+00	1.235E+00	17.03
	964.77	150	5.20	1.580E+00	1.586E+00	1.603E+00	42.90
	969.11	409	16.60	1.574E+00	1.366E+00	1.381E+00	27.93
	84.40	276	1.21	4.334E+00	4.588E+00	4.735E+00	41.23
TH-230	238.60	3012	44.60*	4.541E+00	1.296E+00	1.338E+00	10.50
	300.10	189	3.41	3.882E+00	1.247E+00	1.287E+00	76.38
	295.21	1299	19.20	3.927E+00	1.502E+00	1.502E+00	14.06
TH-232	351.92	2319	37.20	3.485E+00	1.559E+00	1.559E+00	9.15
	609.31	1744	46.30*	2.356E+00	1.393E+00	1.393E+00	10.50
	238.59	3012	44.60*	4.541E+00	1.296E+00	1.296E+00	10.50
	911.20	647	27.70	1.666E+00	1.222E+00	1.222E+00	17.03
TH-234	964.40	150	5.20	1.580E+00	1.586E+00	1.586E+00	42.90
	969.11	409	16.60	1.574E+00	1.366E+00	1.366E+00	27.93
	63.29	59	3.80*	1.711E+00	7.875E-01	7.875E-01	195.65
U-234	92.38	459	5.41	5.082E+00	1.455E+00	1.455E+00	33.55
	112.81	-----	0.24	5.950E+00	-----	Line Not Found	-----
	67.67	-----	0.37	2.385E+00	-----	Line Not Found	-----
	241.98	950	7.49	4.501E+00	2.455E+00	2.455E+00	17.61
U-235	295.21	1299	19.20*	3.927E+00	1.502E+00	1.502E+00	14.06
	351.92	2319	37.20	3.485E+00	1.559E+00	1.559E+00	10.88
U-235	89.95	340	2.70	4.865E+00	2.254E+00	2.254E+00	41.88
	93.35	459	4.50	5.082E+00	1.749E+00	1.749E+00	39.80

Nuclide Type:

Nuclide	Energy	Area	%Abn	%Eff	Uncorrected pCi/GRAM	Decay Corr pCi/GRAM	2-Sigma %Error
	105.00	-----	2.10	5.731E+00	-----	Line Not Found	-----
	143.76	44	10.50*	5.983E+00	6.133E-02	6.133E-02	226.66
	163.33	-----	4.70	5.703E+00	-----	Line Not Found	-----
	185.71	521	54.00	5.329E+00	1.578E-01	1.578E-01	30.36
	205.31	-----	5.00	5.012E+00	-----	Line Not Found	-----
NP-237	86.48	613	12.60*	4.637E+00	9.145E-01	9.145E-01	32.97
	95.87	-----	2.60	5.290E+00	-----	Line Not Found	-----
U-238	63.29	59	3.80*	1.711E+00	7.875E-01	7.875E-01	195.65
ANH-511	511.00	301	100.00*	2.690E+00	9.753E-02	9.753E-02	43.47

Nuclide Type: NATURAL

Nuclide	Energy	Area	%Abn	%Eff	Uncorrected pCi/GRAM	Decay Corr pCi/GRAM	2-Sigma %Error
RA-224	240.98	950	3.95*	4.501E+00	4.655E+00	4.804E+00	16.70

Flag: "*" = Keyline

Total number of lines in spectrum 70
 Number of unidentified lines 26
 Number of lines tentatively identified by NID 44 62.86%

Nuclide Type :

Nuclide	Hlife	Decay	Uncorrected pCi/GRAM	Decay Corr pCi/GRAM	Decay Corr 2-Sigma Error	2-Sigma %Error	Flags
K-40	1.28E+09Y	1.00	1.681E+01	1.681E+01	0.137E+01	8.13	
MN-54	312.70D	1.07	7.547E-03	8.098E-03	28.85E-03	356.22	
CD-109	464.00D	1.05	3.040E+00	3.188E+00	0.820E+00	25.72	
SN-126	1.00E+05Y	1.00	3.114E-01	3.114E-01	0.801E-01	25.72	
CS-135	2.30E+06Y	1.00	3.155E-01	3.155E-01	1.433E-01	45.42	
CE-141	32.50D	1.97	1.330E-02	2.621E-02	5.927E-02	226.15	
HG-203	46.61D	1.60	1.649E-02	2.645E-02	3.388E-02	128.07	
TL-208	1.91Y	1.03	3.970E-01	4.098E-01	0.461E-01	11.26	
BI-211	7.04E+08Y	1.00	4.482E+00	4.482E+00	0.428E+00	9.55	
BI-212	1.91Y	1.03	8.622E-01	8.899E-01	2.322E-01	26.09	
PB-212	1.91Y	1.03	1.296E+00	1.338E+00	0.140E+00	10.50	
BI-214	1600.00Y	1.00	1.393E+00	1.393E+00	0.146E+00	10.50	
PB-214	1600.00Y	1.00	1.559E+00	1.559E+00	0.170E+00	10.88	
RA-223	7.04E+08Y	1.00	3.712E-01	3.712E-01	1.677E-01	45.18	K
RA-226	1600.00Y	1.00	1.393E+00	1.393E+00	0.146E+00	10.50	
AC-228	5.75Y	1.01	1.222E+00	1.235E+00	0.210E+00	17.03	
RA-228	5.75Y	1.01	1.222E+00	1.235E+00	0.210E+00	17.03	
TH-228	1.91Y	1.03	1.296E+00	1.338E+00	0.140E+00	10.50	
TH-230	7.70E+04Y	1.00	1.393E+00	1.393E+00	0.146E+00	10.50	
TH-232	1.41E+10Y	1.00	1.296E+00	1.296E+00	0.136E+00	10.50	
TH-234	4.47E+09Y	1.00	7.875E-01	7.875E-01	15.41E-01	195.65	
U-234	2.45E+05Y	1.00	1.502E+00	1.502E+00	0.211E+00	14.06	
U-235	7.04E+08Y	1.00	6.133E-02	6.133E-02	13.90E-02	226.66	
NP-237	2.14E+06Y	1.00	9.145E-01	9.145E-01	3.015E-01	32.97	
U-238	4.47E+09Y	1.00	7.875E-01	7.875E-01	15.41E-01	195.65	
ANH-511	1.00E+09Y	1.00	9.753E-02	9.753E-02	4.240E-02	43.47	
Total Activity :			4.285E+01	4.317E+01			

Nuclide Type : NATURAL

Nuclide	Hlife	Decay	Uncorrected pCi/GRAM	Decay Corr pCi/GRAM	Decay Corr 2-Sigma Error	2-Sigma %Error	Flags
RA-224	1.91Y	1.03	4.655E+00	4.804E+00	0.802E+00	16.70	
Total Activity :			4.655E+00	4.804E+00			

Grand Total Activity : 4.750E+01 4.797E+01

Flags: "K" = Keyline not found "M" = Manually accepted
 "E" = Manually edited "A" = Nuclide specific abn. limit

It	Energy	Area	Bkgnd	FWHM	Channel	Left	Pw	Cts/Sec	%Err	%Eff	Flags
0	128.82	206	1049	1.61	256.06	251	10	9.52E-03	61.7	6.08E+00	
0	304.92	48	266	1.27	608.03	606	6	2.20E-03	****	3.84E+00	T
0	314.16	61	444	0.72	626.50	623	10	2.80E-03	****	3.76E+00	
0	327.81	154	377	1.09	653.79	649	8	7.12E-03	46.7	3.66E+00	T
0	409.05	101	282	1.10	816.19	812	8	4.70E-03	65.2	3.14E+00	
0	520.47	18	148	1.36	1038.94	1037	7	8.44E-04	****	2.65E+00	
0	665.04	44	187	1.45	1328.01	1325	11	2.02E-03	****	2.20E+00	T
0	754.58	23	153	0.92	1507.08	1504	9	1.04E-03	****	1.97E+00	T
0	785.26	63	182	1.64	1568.44	1563	12	2.91E-03	89.6	1.91E+00	T
0	1073.65	24	63	1.29	2145.29	2142	7	1.11E-03	****	1.43E+00	
0	1152.68	23	184	0.97	2303.41	2303	15	1.07E-03	****	1.34E+00	
0	1166.04	27	46	1.39	2330.13	2328	6	1.24E-03	89.1	1.32E+00	
0	1175.29	40	114	4.06	2348.64	2343	11	1.86E-03	****	1.31E+00	
0	1279.81	22	110	1.20	2557.77	2551	12	1.03E-03	****	1.22E+00	
0	1400.39	63	75	4.43	2799.09	2789	19	2.91E-03	71.0	1.13E+00	T
0	1496.63	10	70	5.30	2991.70	2985	14	4.63E-04	****	1.07E+00	
5	1507.95	59	65	3.41	3014.36	3004	21	2.71E-03	74.9	1.07E+00	
5	1511.77	12	13	1.34	3022.02	3004	21	5.36E-04	****	1.07E+00	
0	1527.52	6	33	3.36	3053.53	3047	12	2.96E-04	****	1.06E+00	
0	1591.53	22	39	1.33	3181.67	3178	11	1.00E-03	****	1.03E+00	
0	1620.56	28	17	1.03	3239.79	3234	12	1.29E-03	81.7	1.02E+00	
0	1630.09	24	27	2.62	3258.87	3255	10	1.11E-03	98.1	1.02E+00	
0	1661.08	22	37	1.66	3320.89	3314	15	1.03E-03	****	1.01E+00	
0	1674.55	16	22	3.28	3347.87	3343	14	7.63E-04	****	1.00E+00	
4	1728.53	79	25	3.24	3455.94	3446	44	3.64E-03	39.5	9.89E-01	
4	1738.54	22	21	3.25	3475.98	3446	44	1.03E-03	****	9.87E-01	
0	1763.33	315	17	2.33	3525.62	3518	19	1.46E-02	13.9	9.82E-01	
0	1792.11	12	21	5.75	3583.23	3574	14	5.54E-04	****	9.76E-01	T
0	1846.76	37	36	2.56	3692.65	3689	18	1.71E-03	82.9	9.68E-01	
0	1877.19	40	41	11.80	3753.59	3738	29	1.84E-03	****	9.65E-01	
0	1900.01	16	31	6.01	3799.28	3791	18	7.38E-04	****	9.63E-01	
0	1948.41	12	3	1.08	3896.21	3894	6	5.60E-04	77.1	9.61E-01	
0	2019.99	21	62	12.23	4039.56	4025	36	9.70E-04	****	9.61E-01	

Flags: "T" = Tentatively associated


```

*****
*                                     GENERAL ENG. LABS, LLC.                               *
*                                     2040 Savage Road                                   *
*                                     Charleston, SC 29414                             *
*****
*                                     DETECTOR DATA                                   *
* Configuration      : DKA300:[CANBERRA.GAMMA.ARCHIVE.GAMMA]G158269002.CNF;1          *
* Acquisition date   : 10-APR-2006 23:57:35  Detector SN#      : 1922864             *
* Detector ID        : GAMMA16                Sensitivity       : 3.00000             *
* Geometry           : CAN                    Energy tolerance   : 2.00000             *
* Elapsed live time  : 0 06:00:00.00          Abundance limit      : 75.00000             *
* Elapsed real time  : 0 06:00:03.45          Half life ratio      : 8.00000             *
*****
*                                     SAMPLE DATA                                   *
* Sample date        : 10-MAR-2006 07:55:00  Nuclide Library   : EPI                 *
* Sample ID          : G158269002            Analyst initials    : MJH1                 *
* Batch Number       : 513802                Sample Quantity     : 1.43550E+02 GRAM          *
*****
*                                     QC DATA                                   *
* CALIB. DATE/TIME  : 5-APR-2006 19:34:04.74MS Isotope       :                 *
* MSD DPM           :                       MSD Isotope       :                 *
* LCS DPM           :                       LCS Isotope       :                 *
*****

```

Combined Activity-MDA Report

---- Identified Nuclides ----

Nuclide	Activity (pCi/GRAM)	Act error	MDA (pCi/GRAM)	MDA error	Act/MDA
K-40	1.681E+01	1.367E+00	2.842E-01	1.876E-02	59.150
MN-54	8.098E-03	2.885E-02	3.264E-02	2.758E-03	0.248
CD-109	3.188E+00	8.200E-01	6.244E-01	6.611E-02	5.106
SN-126	3.114E-01	8.009E-02	6.149E-02	6.497E-03	5.065
CS-135	3.155E-01	1.433E-01	1.248E-01	1.192E-02	2.528
CE-141	1.880E-02	4.297E-02	7.414E-02	5.968E-03	0.254
HG-203	2.645E-02	3.388E-02	4.097E-02	3.395E-03	0.646
TL-208	4.098E-01	4.613E-02	2.902E-02	2.032E-03	14.119
BI-211	4.482E+00	4.279E-01	1.548E-01	1.136E-02	28.949
BI-212	8.899E-01	2.322E-01	2.407E-01	2.075E-02	3.697
PB-212	1.338E+00	1.405E-01	4.727E-02	4.473E-03	28.303
BI-214	1.393E+00	1.463E-01	5.649E-02	4.550E-03	24.665
PB-214	1.559E+00	1.696E-01	5.499E-02	4.944E-03	28.352
RA-223	-3.243E-01	3.878E-01	5.324E-01	9.118E-02	-0.609
RA-224	4.804E+00	8.022E-01	5.378E-01	4.476E-02	8.933
RA-226	1.393E+00	1.463E-01	5.649E-02	4.550E-03	24.665
AC-228	1.235E+00	2.104E-01	9.331E-02	1.101E-02	13.236
RA-228	1.235E+00	2.104E-01	9.331E-02	1.101E-02	13.236

---- Identified Nuclides ----

Nuclide	Activity (pCi/GRAM)	Act error	MDA (pCi/GRAM)	MDA error	Act/MDA
TH-228	1.338E+00	1.405E-01	4.726E-02	4.473E-03	28.306
TH-230	1.393E+00	1.463E-01	5.649E-02	4.550E-03	24.665
TH-232	1.296E+00	1.361E-01	4.579E-02	4.333E-03	28.307
TH-234	7.875E-01	1.541E+00	1.611E+00	3.205E-01	0.489
U-234	1.502E+00	2.111E-01	1.098E-01	1.099E-02	13.681
U-235	6.133E-02	1.390E-01	1.816E-01	3.114E-02	0.338
NP-237	9.145E-01	3.015E-01	1.842E-01	4.267E-02	4.964
U-238	7.875E-01	1.541E+00	1.611E+00	3.205E-01	0.489
ANH-511	9.753E-02	4.240E-02	2.387E-02	1.452E-03	4.086

---- Non-Identified Nuclides ----

Nuclide	Key-Line Activity (pCi/GRAM)	K.L. Ided	Act error	MDA (pCi/GRAM)	MDA error	Act/MDA
BE-7	-6.907E-02		1.917E-01	3.266E-01	2.266E-02	-0.211
NA-22	3.308E-03		2.394E-02	3.652E-02	2.373E-03	0.091
AL-26	1.139E-04		1.234E-02	2.308E-02	1.328E-03	0.005
SC-46	6.199E-03		2.023E-02	3.480E-02	3.225E-03	0.178
V-48	4.247E-02		6.689E-02	1.223E-01	1.083E-02	0.347
CR-51	1.032E-01		2.797E-01	4.656E-01	3.703E-02	0.222
CO-56	-1.101E-02		2.024E-02	3.287E-02	2.835E-03	-0.335
CO-57	6.563E-03		1.261E-02	2.184E-02	1.692E-03	0.301
CO-58	-1.092E-02		2.109E-02	3.444E-02	2.798E-03	-0.317
FE-59	-1.999E-03		5.229E-02	9.160E-02	7.809E-03	-0.022
CO-60	-1.013E-02		1.727E-02	2.878E-02	1.791E-03	-0.352
ZN-65	-7.778E-06		4.858E-02	7.372E-02	5.584E-03	0.000
SE-75	-1.061E-02		2.408E-02	3.914E-02	3.214E-03	-0.271
KR-85	2.187E+00		3.686E+00	5.776E+00	3.517E-01	0.379
SR-85	1.336E-02		2.251E-02	3.528E-02	2.148E-03	0.379
Y-88	-4.126E-03		1.701E-02	3.053E-02	1.737E-03	-0.135
Y-91	-6.322E-03		2.099E-02	3.555E-02	2.184E-03	-0.178
NB-94	8.038E-03		1.598E-02	2.777E-02	1.846E-03	0.289
NB-95	7.978E-02		3.632E-02	6.118E-02	4.578E-03	1.304
ZR-95	3.558E-03		4.687E-02	6.964E-02	5.822E-03	0.051
RU-103	-9.947E-03		2.566E-02	4.355E-02	5.560E-03	-0.228
RH-106	8.652E-02		1.507E-01	2.654E-01	1.636E-02	0.326
RU-106	1.130E-01		1.527E-01	2.701E-01	3.220E-02	0.418
AG-108M	-6.626E-03		1.571E-02	2.684E-02	1.714E-03	-0.247
AG-110M	-2.079E-02		1.741E-02	2.767E-02	1.799E-03	-0.751
SN-113	3.266E-03		2.331E-02	4.091E-02	2.509E-03	0.080
SN-115	4.429E+00	+	3.093E+00	4.265E+00	3.926E-01	1.038
SN-117M	3.004E-03		6.149E-02	1.040E-01	8.455E-03	0.029
TE-123M	-1.095E-03		1.498E-02	2.526E-02	2.069E-03	-0.043
SB-124	-1.665E-02		4.427E-02	7.450E-02	4.849E-03	-0.223
SB-125	2.025E-02		4.487E-02	7.937E-02	4.857E-03	0.255
TE-125M	2.004E+00		5.430E+00	9.399E+00	9.437E-01	0.213
I-126	2.374E-01	+	2.983E-01	3.567E-01	2.211E-02	0.666
SB-126	1.293E-01		1.712E-01	3.017E-01	2.074E-02	0.429

---- Non-Identified Nuclides ----

Nuclide	Key-Line Activity (pCi/GRAM)	K.L. Ided	Act error	MDA (pCi/GRAM)	MDA error	Act/MDA
I-131	-7.250E-02		2.225E-01	3.855E-01	2.817E-02	-0.188
BA-133	1.016E-02		2.185E-02	3.467E-02	4.169E-03	0.293
CS-134	5.475E-02	+	3.125E-02	3.875E-02	3.079E-03	1.413
CS-136	2.304E-03		1.153E-01	2.034E-01	1.770E-02	0.011
BA-137M	2.591E-02		1.833E-02	3.007E-02	1.847E-03	0.862
CS-137	2.740E-02		1.938E-02	3.179E-02	1.960E-03	0.862
CE-139	-2.368E-03		1.606E-02	2.695E-02	2.236E-03	-0.088
BA-140	1.494E-01		2.893E-01	5.050E-01	1.645E-01	0.296
LA-140	3.313E-02		1.028E-01	1.642E-01	1.015E-02	0.202
CE-144	-5.424E-02		1.024E-01	1.713E-01	2.586E-02	-0.317
PM-144	-1.293E-02		1.653E-02	2.684E-02	1.768E-03	-0.482
PM-146	1.822E-02		2.061E-02	3.698E-02	3.228E-03	0.493
ND-147	1.576E-01		7.078E-01	1.237E+00	1.690E-01	0.127
PM-147	-1.244E+03		2.573E+04	4.392E+04	3.406E+03	-0.028
EU-152	-1.389E-03		4.786E-02	7.814E-02	5.915E-03	-0.018
GD-153	-1.513E-02		4.008E-02	6.839E-02	6.241E-03	-0.221
EU-154	8.836E-03		6.629E-02	1.011E-01	9.888E-03	0.087
EU-155	1.312E-02		5.154E-02	8.918E-02	7.615E-03	0.147
TB-160	-6.873E-02		7.733E-02	1.217E-01	1.110E-02	-0.565
TM-171	6.345E+00		1.979E+01	3.146E+01	3.594E+00	0.202
HF-181	-8.638E-03		2.592E-02	4.423E-02	2.666E-03	-0.195
TA-182	-1.023E-01		1.070E-01	1.744E-01	1.166E-02	-0.587
IR-192	2.126E-03		2.209E-02	3.241E-02	2.435E-03	0.066
BI-207	1.974E-02		2.416E-02	4.440E-02	3.613E-03	0.445
BI-210	-5.823E-01		6.765E+00	9.917E+00	1.013E+00	-0.059
PB-210	-5.823E-01		6.765E+00	9.917E+00	1.013E+00	-0.059
PB-211	-9.755E-02		4.599E-01	7.873E-01	4.908E-01	-0.124
RN-219	1.363E-01		1.992E-01	3.543E-01	4.818E-02	0.385
AC-227	-7.112E-02		1.942E-01	3.169E-01	4.845E-02	-0.224
TH-227	-6.991E-02		1.910E-01	3.115E-01	5.570E-02	-0.224
TH-229	-7.977E-02		2.596E-01	4.303E-01	3.598E-02	-0.185
PA-231	2.362E-01		8.728E-01	1.296E+00	1.921E-01	0.182
TH-231	3.712E-01	+	1.684E-01	1.825E-01	1.687E-02	2.034
PA-233	2.331E-02		3.493E-02	5.285E-02	4.146E-03	0.441
PA-234	2.763E-02		1.397E-01	2.496E-01	4.742E-02	0.111
PA-234M	3.020E+00		2.165E+00	4.056E+00	4.069E-01	0.745
NP-239	6.801E-04		9.238E-02	1.581E-01	1.245E-02	0.004
AM-241	-4.492E-02		1.296E-01	2.027E-01	2.745E-02	-0.222
AM-242	6.846E-03		1.037E+00	1.785E+00	1.525E-01	0.004
CM-247	1.447E-02		1.790E-02	3.207E-02	1.855E-03	0.451
CF-249	2.687E-02		1.937E-02	3.536E-02	2.068E-03	0.760
CF-251	4.187E-02		6.188E-02	1.059E-01	8.809E-03	0.395

```

*****
*
*                               General Engineering Labs, LLC
*                               2040 SAVAGE ROAD
*                               CHARLESTON ,SC 29417
*                               GROSS GAMMA REPORT
*
*****
*
* BATCH ID      : 513802                SAMPLE ID   : G158269002
* ANALYST      : MJH1                   DETECTOR    : GAMMA16
* SAMPLE DATE   : 10-MAR-2006 07:55:00.00  COUNT TIME  : 0 06:00:00.00
* ANALYSIS DATE: 10-APR-2006 23:57:35.07  SAMPLE ALQT: 143.550 GRAM
*
*****

```

```

GROSS GAMMA ACTIVITY (pCi/GRAM ) : 8.396E+00
GROSS GAMMA ERROR (pCi/GRAM ) : 1.566E+00
GROSS GAMMA MDA (pCi/GRAM ) : 4.362E+00
GROSS GAMMA DLC (pCi/GRAM ) : 2.134E+00

```

VAX/VMS Nuclide Identification Report Generated 11-APR-2006 10:15:03.91

```

*****
*                               GENERAL ENG. LABS, LLC.                               *
*                               2040 Savage Road                                       *
*                               Charleston, SC 29414                                   *
*****
Configuration : DKA300:[CANBERRA.GAMMA.ARCHIVE.GAMMA]G158269003.CNF;1
Sample date   : 10-MAR-2006 12:00:00 Acquisition date : 11-APR-2006 06:14:36
Sample ID     : G158269003 Sample quantity : 1.29350E+02 GRAM
Detector name : GAMMA16 Detector geometry: CAN
Elapsed live time: 0 04:00:00.00 Elapsed real time: 0 04:00:02.18 0.0%
Energy tolerance : 2.00000 KEV Analyst Initials : MJH1
Abundance limit : 75.00000 Sensitivity : 3.00000
Batch ID       : 513802 Detector SN# : 1922864
Matrix Spike DPM : LCS DPM :
*****

```

Pk	It	Energy	Area	Bkgnd	FWHM	Channel	Left	Pw	Cts/Sec	%Err	Fit
1	0	63.16*	50	599	0.87	124.85	121	8	3.48E-03	89.7	
2	6	72.42*	83	327	1.30	143.36	141	17	5.73E-03	34.4	4.06E+00
3	6	74.79*	527	494	1.03	148.09	141	17	3.66E-02	8.3	
4	6	76.98*	845	583	1.21	152.46	141	17	5.87E-02	6.1	
5	4	84.30*	121	568	1.18	167.10	162	29	8.38E-03	34.2	2.01E+00
6	4	87.22*	340	553	1.14	172.92	162	29	2.36E-02	12.9	
7	4	89.90	244	611	1.34	178.29	162	29	1.69E-02	19.0	
8	4	92.83*	320	660	1.45	184.14	162	29	2.22E-02	16.8	
9	0	99.57	50	369	1.09	197.61	195	6	3.49E-03	62.3	
10	0	105.48*	93	409	1.34	209.42	206	7	6.43E-03	40.1	
11	0	128.70*	69	574	1.27	255.83	252	8	4.77E-03	62.9	
12	0	153.21*	111	506	1.64	304.80	301	8	7.70E-03	37.4	
13	0	185.76*	321	506	1.23	369.87	366	9	2.23E-02	14.6	
14	0	209.07	168	481	1.37	416.44	413	9	1.17E-02	24.7	
15	0	217.19	41	433	1.15	432.68	431	9	2.87E-03	91.5	
16	3	238.46*	2099	324	1.15	475.19	468	23	1.46E-01	2.7	2.11E+00
17	3	241.52*	537	424	1.71	481.31	468	23	3.73E-02	10.2	
18	0	270.11	151	363	1.31	538.46	533	9	1.05E-02	24.1	
19	0	277.33	82	274	0.80	552.89	550	8	5.67E-03	36.7	
20	0	294.94*	790	421	1.14	588.09	582	13	5.49E-02	6.5	
21	0	300.02*	104	323	1.05	598.23	595	9	7.24E-03	33.4	
22	0	327.66	120	455	1.38	653.48	646	14	8.31E-03	38.9	
23	0	337.97*	402	285	1.27	674.09	669	11	2.79E-02	10.0	
24	0	351.56*	1287	336	1.29	701.27	694	14	8.93E-02	4.2	
25	0	408.51*	35	247	1.71	815.12	811	9	2.45E-03	85.0	
26	3	462.50	166	155	2.00	923.03	917	20	1.15E-02	17.4	1.76E+00
27	3	467.48	33	126	2.00	933.01	917	20	2.32E-03	58.2	
28	0	510.46*	176	324	1.79	1018.93	1011	18	1.23E-02	28.8	
29	0	570.73	82	154	2.01	1139.44	1133	14	5.66E-03	34.1	
30	0	582.75*	737	140	1.45	1163.46	1158	13	5.12E-02	5.1	
31	0	608.85*	965	211	1.35	1215.66	1209	15	6.70E-02	4.7	
32	0	643.62	87	188	8.31	1285.18	1274	21	6.03E-03	41.0	
33	3	661.11*	18	72	1.54	1320.16	1317	15	1.22E-03	97.0	4.28E+00
34	3	664.36	46	118	2.20	1326.65	1317	15	3.22E-03	47.9	
35	0	727.09	159	116	2.12	1452.10	1447	13	1.10E-02	16.2	
36	0	762.30	22	69	1.17	1522.50	1520	7	1.56E-03	64.6	
37	2	767.77*	92	112	2.08	1533.46	1527	22	6.37E-03	26.3	1.53E+00
38	2	771.01*	52	94	1.90	1539.94	1527	22	3.60E-03	41.6	

Pk	It	Energy	Area	Bkgnd	FWHM	Channel	Left	Pw	Cts/Sec	%Err	Fit
39	0	784.06	25	98	0.80	1566.03	1564	10	1.74E-03	76.6	
40	0	794.06*	101	78	1.14	1586.03	1581	10	7.03E-03	19.7	
41	0	805.95*	16	91	1.00	1609.82	1605	10	1.14E-03	114.7	
42	0	836.59*	74	149	4.89	1671.10	1663	17	5.13E-03	40.0	
43	0	859.87*	93	78	2.03	1717.65	1712	10	6.43E-03	23.3	
44	0	892.44	25	32	1.24	1782.80	1780	6	1.74E-03	40.7	
45	0	910.30*	426	124	1.65	1818.52	1813	15	2.96E-02	7.7	
46	0	933.75*	51	111	2.01	1865.43	1854	17	3.52E-03	51.0	
47	0	938.25*	15	64	1.33	1874.43	1871	11	1.02E-03	120.1	
48	3	963.71*	58	80	1.96	1925.36	1921	19	4.02E-03	29.9	1.49E+00
49	3	968.02*	267	92	1.86	1933.98	1921	19	1.86E-02	9.6	
50	0	1031.67	54	45	1.44	2061.31	2056	11	3.74E-03	28.0	
51	0	1072.42	50	130	6.57	2142.83	2134	20	3.50E-03	57.2	
52	0	1119.61*	231	96	1.78	2237.23	2231	16	1.60E-02	11.9	
53	0	1176.15	27	38	1.15	2350.37	2347	8	1.90E-03	43.5	
54	0	1236.80	109	52	2.13	2471.73	2467	10	7.55E-03	15.7	
55	0	1240.56	14	37	1.29	2479.25	2476	6	9.49E-04	75.8	
56	0	1376.22	86	36	2.31	2750.71	2740	17	5.96E-03	19.0	
57	0	1408.26*	45	70	3.85	2814.85	2809	26	3.15E-03	53.8	
58	0	1459.35*	1389	39	2.08	2917.09	2908	17	9.65E-02	2.9	
59	0	1471.28	11	17	1.32	2940.98	2934	12	7.37E-04	85.4	
60	0	1508.44*	20	40	1.48	3015.34	3009	14	1.38E-03	74.3	
61	0	1565.51	14	6	1.71	3129.58	3126	8	9.93E-04	39.6	
62	2	1578.66*	18	12	2.60	3155.90	3152	48	1.28E-03	43.8	1.82E+00
63	2	1586.70	25	20	2.15	3172.00	3152	48	1.74E-03	43.7	
64	2	1589.89*	16	24	2.61	3178.38	3152	48	1.11E-03	86.2	
65	0	1619.52*	21	12	2.81	3237.70	3233	11	1.47E-03	44.1	
66	0	1664.75	17	14	3.17	3328.24	3322	14	1.18E-03	52.6	
67	0	1671.55	6	8	0.76	3341.86	3337	12	3.89E-04	114.2	
68	0	1728.90	22	43	1.22	3456.67	3447	16	1.50E-03	72.0	
69	0	1762.79*	179	16	1.59	3524.52	3519	12	1.24E-02	9.2	
70	0	1800.67	24	14	9.20	3600.38	3587	28	1.67E-03	48.6	
71	0	1834.42	16	17	3.93	3667.94	3660	17	1.11E-03	64.1	
72	0	1846.85	29	27	1.90	3692.84	3683	21	1.99E-03	51.9	
73	0	1874.58	14	7	1.55	3748.36	3744	9	1.01E-03	41.6	
74	0	1909.17	6	17	5.19	3817.62	3806	14	4.09E-04	155.8	
75	0	1972.52*	5	2	1.67	3944.49	3942	7	3.70E-04	97.9	

Flag: "*" = Peak area was modified by background subtraction

VAX/VMS Nuclide Identification Report Generated

```

*****
*                               General Eng. Labs, LLC.                               *
*                               2040 Savage Road                                       *
*                               Charleston, SC 29414                                   *
*****
*                               DETECTOR DATA                                       *
*
* Configuration      : DKA300:[CANBERRA.GAMMA.ARCHIVE.GAMMA]G158269003
* Acquisition date   : 11-APR-2006 06:14:36 Detector SN#      : 1922864
* Detector ID        : GAMMA16                      Sensitivity      : 3.000
* Geometry           : CAN                          Energy tolerance: 2.000
* Elapsed live time  : 0 04:00:00.00                Abundance limit : 75.000
* Elapsed real time  : 0 04:00:02.18                Half life ratio  : 8.000
*****
*                               SAMPLE DATA                                         *
*
* Sample date        : 10-MAR-2006 12:00:00 Nuclide Library :
* Sample ID          : G158269003                 Analyst initials: MJH1
* Batch Number       : 513802                     Sample Quantity : 1.2935E+02 GRAM
* Recovery           : 1.00000                     Carrier Weight  : 0.00000
*****
*                               QC DATA                                             *
*
* Standard Weight    : 0.00000
* CALIB. DATE/TIME   : 5-APR-2006 19:34:04 MS Isotope      :
* MSD DPM             : 0.000                      MSD Isotope      :
* LCS DPM             : 0.000                      LCS Isotope      :
* LCSD DPM           : 0.000                      LCSD Isotope     :
*****

```

Combined Activity-MDA Report

---- Identified Nuclides ----

Nuclide	Activity (pCi/GRAM)	Act error	MDA (pCi/GRAM)	
K-40	1.728E+01	1.521E+00	3.301E-01	0.000E+00
MN-54	6.400E-02	5.153E-02	3.889E-02	0.000E+00
CD-109	2.940E+00	8.206E-01	8.573E-01	0.000E+00
SN-126	2.872E-01	8.015E-02	8.442E-02	0.000E+00
CS-135	3.290E-01	1.619E-01	1.701E-01	0.000E+00
BA-137M	1.285E-02	2.494E-02	3.804E-02	0.000E+00
CS-137	1.358E-02	2.636E-02	4.021E-02	0.000E+00
EU-155	1.089E-01	8.885E-02	1.169E-01	0.000E+00
TB-160	-2.436E-03	1.002E-01	1.721E-01	0.000E+00
HG-203	6.010E-02	4.442E-02	5.450E-02	0.000E+00
TL-208	5.379E-01	6.648E-02	3.905E-02	0.000E+00
BI-211	4.139E+00	4.607E-01	2.106E-01	0.000E+00
BI-212	9.906E-01	3.326E-01	3.062E-01	0.000E+00
PB-212	1.552E+00	1.688E-01	6.324E-02	0.000E+00
BI-214	1.283E+00	1.587E-01	6.824E-02	0.000E+00
PB-214	1.440E+00	1.770E-01	7.363E-02	0.000E+00
RA-224	4.525E+00	9.966E-01	7.194E-01	0.000E+00
RA-226	1.283E+00	1.587E-01	6.824E-02	0.000E+00
AC-228	1.354E+00	2.619E-01	1.431E-01	0.000E+00
RA-228	1.354E+00	2.619E-01	1.431E-01	0.000E+00
TH-228	1.552E+00	1.688E-01	6.323E-02	0.000E+00
TH-229	-3.081E-01	3.445E-01	5.780E-01	0.000E+00
TH-230	1.283E+00	1.587E-01	6.824E-02	0.000E+00
TH-232	1.504E+00	1.635E-01	6.126E-02	0.000E+00
TH-234	1.066E+00	1.924E+00	2.129E+00	0.000E+00
U-234	1.520E+00	2.499E-01	1.509E-01	0.000E+00
U-235	7.512E-02	1.345E-01	2.412E-01	0.000E+00
NP-237	8.432E-01	2.927E-01	2.530E-01	0.000E+00
U-238	1.066E+00	1.924E+00	2.129E+00	0.000E+00
AM-242	2.205E+00	1.799E+00	2.354E+00	0.000E+00
ANH-511	9.516E-02	5.504E-02	3.111E-02	0.000E+00

---- Non-Identified Nuclides ----

Nuclide	Key-Line Activity (pCi/GRAM	K.L. Act error) Ided	MDA (pCi/GRAM)	
BE-7	-9.145E-02	2.559E-01	4.466E-01	0.000E+00	NOT IDENT.
NA-22	-3.328E-02	2.903E-02	4.613E-02	0.000E+00	NOT IDENT.
NA-24	0.000E+00	5.642E+13	0.000E+00	0.000E+00	SHORT HLIF
AL-26	-5.810E-03	1.940E-02	2.974E-02	0.000E+00	FAIL ABUN
SC-46	-2.216E-02	3.338E-02	4.589E-02	0.000E+00	FAIL ABUN
V-48	-6.436E-02	9.088E-02	1.547E-01	0.000E+00	NOT IDENT.
CR-51	1.648E-01	3.797E-01	6.567E-01	0.000E+00	NOT IDENT.
CO-56	8.250E-03	2.799E-02	4.932E-02	0.000E+00	FAIL ABUN
MN-56	0.000E+00	3.396E+41	0.000E+00	0.000E+00	SHORT HLIF
CO-57	1.018E-03	1.654E-02	2.966E-02	0.000E+00	NOT IDENT.
CO-58	-9.813E-03	2.779E-02	4.668E-02	0.000E+00	NOT IDENT.
FE-59	-3.243E-02	6.825E-02	1.175E-01	0.000E+00	NOT IDENT.
CO-60	1.036E-02	2.583E-02	4.739E-02	0.000E+00	NOT IDENT.
ZN-65	4.875E-02	6.245E-02	1.044E-01	0.000E+00	NOT IDENT.
SE-75	-2.387E-02	3.244E-02	5.355E-02	0.000E+00	NOT IDENT.
KR-85	4.444E+00	5.050E+00	8.321E+00	0.000E+00	NOT IDENT.
SR-85	2.716E-02	3.085E-02	5.085E-02	0.000E+00	NOT IDENT.
Y-88	2.963E-02	3.804E-02	4.376E-02	0.000E+00	FAIL ABUN
Y-91	-8.296E-03	2.748E-02	4.764E-02	0.000E+00	NOT IDENT.
NB-94	6.406E-03	2.060E-02	3.651E-02	0.000E+00	NOT IDENT.
NB-95	0.000E+00	6.850E-02	8.405E-02	0.000E+00	FAIL ABUN
NB-95M	0.000E+00	3.458E+01	0.000E+00	0.000E+00	SHORT HLIF
ZR-95	3.300E-02	5.076E-02	9.216E-02	0.000E+00	NOT IDENT.
MO-99	0.000E+00	5.057E+01	0.000E+00	0.000E+00	SHORT HLIF
TC-99M	0.000E+00	2.921E+36	0.000E+00	0.000E+00	SHORT HLIF
RU-103	-2.187E-03	3.204E-02	5.689E-02	0.000E+00	FAIL ABUN
RH-106	-1.545E-02	2.067E-01	3.606E-01	0.000E+00	FAIL ABUN
RU-106	1.386E-02	2.088E-01	3.672E-01	0.000E+00	NOT IDENT.
AG-108M	5.032E-03	2.099E-02	3.799E-02	0.000E+00	NOT IDENT.
AG-110M	-2.454E-03	2.456E-02	3.729E-02	0.000E+00	FAIL ABUN
SN-113	-1.848E-02	2.989E-02	5.220E-02	0.000E+00	NOT IDENT.
CD-115	0.000E+00	1.209E+03	0.000E+00	0.000E+00	SHORT HLIF
SN-115	5.572E+00	5.711E+00	5.791E+00	0.000E+00	FAIL ABUN
SN-117M	-3.396E-02	8.480E-02	1.471E-01	0.000E+00	NOT IDENT.
TE-123M	3.137E-03	2.060E-02	3.643E-02	0.000E+00	NOT IDENT.
SB-124	3.659E-02	6.592E-02	1.252E-01	0.000E+00	NOT IDENT.
SB-125	5.061E-03	6.017E-02	1.081E-01	0.000E+00	FAIL ABUN
TE-125M	7.955E+00	6.839E+00	1.271E+01	0.000E+00	NOT IDENT.
I-126	4.199E-01	4.028E-01	4.917E-01	0.000E+00	FAIL ABUN
SB-126	-3.015E-03	2.100E-01	3.656E-01	0.000E+00	FAIL ABUN
SB-127	0.000E+00	1.705E+01	0.000E+00	0.000E+00	SHORT HLIF
I-131	6.362E-02	2.958E-01	5.407E-01	0.000E+00	NOT IDENT.
I-132	0.000E+00	6.145E+41	0.000E+00	0.000E+00	SHORT HLIF
TE-132	0.000E+00	1.589E+01	0.000E+00	0.000E+00	SHORT HLIF
BA-133	-2.372E-03	2.845E-02	4.536E-02	0.000E+00	FAIL ABUN
I-133	0.000E+00	2.248E+09	0.000E+00	0.000E+00	SHORT HLIF
CS-134	0.000E+00	3.775E-02	5.908E-02	0.000E+00	FAIL ABUN
I-135	0.000E+00	5.964E+33	0.000E+00	0.000E+00	SHORT HLIF
CS-136	-5.688E-03	1.633E-01	2.914E-01	0.000E+00	FAIL ABUN
CE-139	-2.402E-03	2.068E-02	3.618E-02	0.000E+00	NOT IDENT.
BA-140	-1.080E-01	3.798E-01	6.591E-01	0.000E+00	NOT IDENT.
LA-140	1.129E-01	1.340E-01	2.611E-01	0.000E+00	FAIL ABUN
CE-141	2.693E-02	5.570E-02	1.001E-01	0.000E+00	NOT IDENT.
CE-143	0.000E+00	2.029E+06	0.000E+00	0.000E+00	SHORT HLIF
CE-144	3.674E-02	1.349E-01	2.419E-01	0.000E+00	NOT IDENT.
PM-144	-3.715E-03	2.266E-02	3.890E-02	0.000E+00	NOT IDENT.
PR-144	0.000E+00	6.100E+41	0.000E+00	0.000E+00	SHORT HLIF
PM-146	2.497E-03	2.600E-02	4.679E-02	0.000E+00	NOT IDENT.
ND-147	7.629E-01	9.939E-01	1.830E+00	0.000E+00	FAIL ABUN
PM-147	-5.193E+03	3.325E+04	5.922E+04	0.000E+00	NOT IDENT.
PM-149	0.000E+00	1.140E+04	0.000E+00	0.000E+00	SHORT HLIF
EU-152	-1.470E-02	6.450E-02	1.074E-01	0.000E+00	FAIL ABUN
GD-153	-5.166E-02	5.638E-02	8.775E-02	0.000E+00	FAIL ABUN
EU-154	-9.230E-02	8.067E-02	1.277E-01	0.000E+00	NOT IDENT.
TM-171	-1.000E+01	2.642E+01	4.321E+01	0.000E+00	NOT IDENT.
HF-181	7.040E-03	3.435E-02	6.189E-02	0.000E+00	NOT IDENT.
TA-182	5.449E-03	1.305E-01	2.305E-01	0.000E+00	FAIL ABUN
IR-192	-4.156E-03	2.656E-02	4.467E-02	0.000E+00	FAIL ABUN
BI-207	1.340E-02	3.180E-02	5.870E-02	0.000E+00	FAIL ABUN
BI-210	-9.069E-02	8.758E+00	1.369E+01	0.000E+00	NOT IDENT.
PB-210	-9.069E-02	8.758E+00	1.369E+01	0.000E+00	NOT IDENT.
PB-211	-9.519E-02	6.717E-01	1.049E+00	0.000E+00	NOT IDENT.
RN-219	9.780E-02	2.561E-01	4.679E-01	0.000E+00	FAIL ABUN
RA-223	-1.751E-01	5.144E-01	7.532E-01	0.000E+00	FAIL ABUN

AC-227	3.043E-02	2.538E-01	4.378E-01	0.000E+00	FAIL	ABUN
TH-227	2.992E-02	2.495E-01	4.303E-01	0.000E+00	FAIL	ABUN
PA-231	2.001E-01	1.011E+00	1.740E+00	0.000E+00	FAIL	ABUN
TH-231	0.000E+00	1.902E-01	2.578E-01	0.000E+00	FAIL	ABUN
PA-233	-1.037E-02	4.079E-02	6.838E-02	0.000E+00	FAIL	ABUN
PA-234	2.683E-02	1.724E-01	3.159E-01	0.000E+00	FAIL	ABUN
PA-234M	2.836E+00	2.939E+00	5.567E+00	0.000E+00	FAIL	ABUN
NP-239	-1.108E-01	1.198E-01	2.075E-01	0.000E+00	FAIL	ABUN
AM-241	-1.337E-01	1.741E-01	2.806E-01	0.000E+00	NOT	IDENT.
CM-247	5.728E-03	2.324E-02	4.222E-02	0.000E+00	FAIL	ABUN
CF-249	1.266E-02	2.451E-02	4.521E-02	0.000E+00	NOT	IDENT.
CF-251	-3.132E-02	8.328E-02	1.437E-01	0.000E+00	NOT	IDENT.

```

*****
*                               GENERAL ENG. LABS, LLC.                               *
*                               2040 Savage Road                                       *
*                               Charleston, SC 29414                                   *
*****
Configuration      : DKA300:[CANBERRA.GAMMA.ARCHIVE.GAMMA]G158269003.CNF;1
Sample date        : 10-MAR-2006 12:00:00 Acquisition date : 11-APR-2006 06:14:36
Sample ID          : G158269003 Sample quantity      : 1.29350E+02 GRAM
Detector name     : GAMMA16 Detector geometry      : CAN
Elapsed live time : 0 04:00:00.00 Elapsed real time: 0 04:00:02.18 0.0%
Energy tolerance  : 2.00000 KEV Analyst Initials   : MJH1
Abundance limit   : 75.00000 Sensitivity       : 3.00000
Batch ID          : 513802 Detector SN#       : 1922864
Matrix Spike DPM  : LCS DPM                          :
*****
    
```

Nuclide Line Activity Report

Nuclide Type:

Nuclide	Energy	Area	%Abn	%Eff	Uncorrected pCi/GRAM	Decay Corr pCi/GRAM	2-Sigma %Error
K-40	1460.81	1389	10.67*	1.093E+00	1.728E+01	1.728E+01	8.80
MN-54	834.83	74	99.83*	1.801E+00	5.964E-02	6.400E-02	80.52
NB-95	765.79	92	99.81*	1.944E+00	6.864E-02	1.288E-01	53.18
CD-109	88.03	340	3.79*	4.645E+00	2.803E+00	2.940E+00	27.91
SN-126	64.28	50	9.60	1.795E+00	4.218E-01	4.218E-01	180.30
	86.94	340	8.90	4.645E+00	1.194E+00	1.194E+00	49.14
	87.57	340	37.00*	4.645E+00	2.872E-01	2.872E-01	27.91
CS-135	268.24	151	16.00*	4.171E+00	3.290E-01	3.290E-01	49.21
BA-137M	661.65	18	89.98*	2.206E+00	1.282E-02	1.285E-02	194.11
CS-137	661.66	18	85.12*	2.206E+00	1.355E-02	1.358E-02	194.11
EU-155	86.54	340	30.90	4.645E+00	3.438E-01	3.481E-01	27.94
	105.31	93	20.70*	5.748E+00	1.128E-01	1.142E-01	80.74
TB-160	86.79	340	13.30	4.645E+00	7.988E-01	1.084E+00	27.91
	298.57	104	27.10	3.883E+00	1.438E-01	1.952E-01	67.18
	879.36	-----	28.50*	1.721E+00	-----	Line Not Found	-----
	962.29	58	9.00	1.580E+00	5.904E-01	8.012E-01	60.40
	966.15	267	24.20	1.574E+00	1.018E+00	1.382E+00	21.16
	1177.93	27	14.40	1.311E+00	2.098E-01	2.847E-01	87.26
HG-203	70.83	83	4.75	3.008E+00	8.380E-01	1.346E+00	70.35
	72.87	83	8.00	3.008E+00	4.975E-01	7.989E-01	70.27
	82.60	121	3.55	4.373E+00	1.128E+00	1.812E+00	70.05
	279.20	82	77.30*	4.097E+00	3.743E-02	6.010E-02	73.91
TL-208	75.00	527	3.43	3.308E+00	6.735E+00	6.952E+00	21.55
	277.35	82	6.80	4.097E+00	4.255E-01	4.392E-01	74.41
	510.84	176	21.60	2.691E+00	4.405E-01	4.547E-01	58.44
	583.14	737	84.20*	2.438E+00	5.212E-01	5.379E-01	12.36
	763.30	22	1.64	1.956E+00	1.015E+00	1.048E+00	129.91
	860.37	93	12.46	1.757E+00	6.134E-01	6.331E-01	47.48
	1093.90	-----	0.37	1.403E+00	-----	Line Not Found	-----
BI-211	351.07	1287	12.94*	3.486E+00	4.139E+00	4.139E+00	11.13
BI-212	727.18	159	11.80*	2.038E+00	9.598E-01	9.906E-01	33.57
PB-212	74.80	527	10.70	3.308E+00	2.159E+00	2.228E+00	21.80

Nuclide Type:

Nuclide	Energy	Area	%Abn	%Eff	Uncorrected pCi/GRAM	Decay Corr pCi/GRAM	2-Sigma %Error
	87.30	340	8.00	4.645E+00	1.328E+00	1.371E+00	29.65
	115.19	-----	0.60	5.993E+00	-----	Line Not Found	-----
	238.63	2099	44.60*	4.541E+00	1.504E+00	1.552E+00	10.87
	300.09	104	3.41	3.883E+00	1.143E+00	1.180E+00	67.43
BI-214	609.31	965	46.30*	2.356E+00	1.283E+00	1.283E+00	12.37
	768.36	92	5.04	1.944E+00	1.359E+00	1.359E+00	53.51
	934.06	51	3.21	1.628E+00	1.407E+00	1.407E+00	102.69
	1120.29	231	15.10	1.373E+00	1.617E+00	1.617E+00	25.90
	1238.11	109	5.94	1.253E+00	2.119E+00	2.119E+00	32.65
	1377.67	86	4.11	1.144E+00	2.650E+00	2.650E+00	39.06
PB-214	74.81	527	6.21	3.308E+00	3.720E+00	3.720E+00	21.04
	77.11	845	10.50	3.575E+00	3.266E+00	3.266E+00	17.85
	87.30	340	4.41	4.645E+00	2.409E+00	2.409E+00	29.08
	241.98	537	7.50	4.502E+00	2.309E+00	2.309E+00	22.72
	295.21	790	19.20	3.928E+00	1.520E+00	1.521E+00	16.44
	351.92	1287	37.20*	3.486E+00	1.440E+00	1.440E+00	12.29
RA-226	295.21	790	19.20	3.928E+00	1.520E+00	1.521E+00	16.44
	351.92	1287	37.20	3.486E+00	1.440E+00	1.440E+00	10.79
	609.31	965	46.30*	2.356E+00	1.283E+00	1.283E+00	12.37
AC-228	209.25	168	4.40	4.954E+00	1.120E+00	1.131E+00	81.00
	338.32	402	11.40	3.580E+00	1.430E+00	1.445E+00	45.57
	463.01	166	4.40	2.887E+00	1.898E+00	1.918E+00	41.91
	794.95	101	4.60	1.887E+00	1.691E+00	1.709E+00	45.73
	911.21	426	27.70*	1.667E+00	1.340E+00	1.354E+00	19.34
	964.77	58	5.20	1.580E+00	1.022E+00	1.033E+00	64.66
	969.11	267	16.60	1.574E+00	1.485E+00	1.500E+00	30.30
RA-228	209.25	168	4.40	4.954E+00	1.120E+00	1.131E+00	81.00
	338.32	402	11.40	3.580E+00	1.430E+00	1.445E+00	45.57
	463.01	166	4.40	2.887E+00	1.898E+00	1.918E+00	41.91
	794.95	101	4.60	1.887E+00	1.691E+00	1.709E+00	45.73
	911.21	426	27.70*	1.667E+00	1.340E+00	1.354E+00	19.34
	964.77	58	5.20	1.580E+00	1.022E+00	1.033E+00	64.66
	969.11	267	16.60	1.574E+00	1.485E+00	1.500E+00	30.30
TH-228	84.40	121	1.21	4.373E+00	3.311E+00	3.417E+00	69.93
	238.60	2099	44.60*	4.541E+00	1.504E+00	1.552E+00	10.87
	300.10	104	3.41	3.883E+00	1.143E+00	1.180E+00	89.18
TH-229	85.43	121	16.50	4.373E+00	2.428E-01	2.428E-01	69.23
	88.47	340	27.10	4.645E+00	3.921E-01	3.921E-01	27.91
	100.00	50	12.40	5.496E+00	1.070E-01	1.070E-01	125.01
	193.63	-----	4.59*	5.199E+00	-----	Line Not Found	-----
	210.97	168	3.26	4.954E+00	1.509E+00	1.509E+00	50.12
TH-230	295.21	790	19.20	3.928E+00	1.520E+00	1.520E+00	16.44
	351.92	1287	37.20	3.486E+00	1.440E+00	1.440E+00	10.79
	609.31	965	46.30*	2.356E+00	1.283E+00	1.283E+00	12.37
TH-232	238.59	2099	44.60*	4.541E+00	1.504E+00	1.504E+00	10.87
	911.20	426	27.70	1.667E+00	1.340E+00	1.340E+00	19.34
	964.40	58	5.20	1.580E+00	1.022E+00	1.022E+00	64.66
	969.11	267	16.60	1.574E+00	1.485E+00	1.485E+00	30.30
TH-234	63.29	50	3.80*	1.795E+00	1.066E+00	1.066E+00	180.56

Nuclide Type:

Nuclide	Energy	Area	%Abn	%Eff	Uncorrected pCi/GRAM	Decay Corr pCi/GRAM	2-Sigma %Error
	92.38	320	5.41	5.090E+00	1.687E+00	1.687E+00	38.47
	112.81	-----	0.24	5.950E+00	-----	Line Not Found	-----
U-234	67.67	-----	0.37	2.385E+00	-----	Line Not Found	-----
	241.98	537	7.49	4.502E+00	2.312E+00	2.312E+00	22.73
	295.21	790	19.20*	3.928E+00	1.520E+00	1.520E+00	16.44
	351.92	1287	37.20	3.486E+00	1.440E+00	1.440E+00	12.29
U-235	89.95	244	2.70	4.871E+00	2.688E+00	2.688E+00	49.26
	93.35	320	4.50	5.090E+00	2.029E+00	2.029E+00	44.03
	105.00	93	2.10	5.748E+00	1.112E+00	1.112E+00	85.64
	143.76	-----	10.50*	5.981E+00	-----	Line Not Found	-----
	163.33	-----	4.70	5.703E+00	-----	Line Not Found	-----
	185.71	321	54.00	5.329E+00	1.616E-01	1.616E-01	30.44
	205.31	-----	5.00	5.012E+00	-----	Line Not Found	-----
NP-237	86.48	340	12.60*	4.645E+00	8.432E-01	8.432E-01	34.71
	95.87	-----	2.60	5.290E+00	-----	Line Not Found	-----
U-238	63.29	50	3.80*	1.795E+00	1.066E+00	1.066E+00	180.56
AM-242	99.55	50	0.63	5.496E+00	2.106E+00	2.107E+00	125.01
	103.70	93	1.01*	5.748E+00	2.313E+00	2.313E+00	80.73
ANH-511	511.00	176	100.00*	2.691E+00	9.516E-02	9.516E-02	57.84

Nuclide Type: NATURAL

Nuclide	Energy	Area	%Abn	%Eff	Uncorrected pCi/GRAM	Decay Corr pCi/GRAM	2-Sigma %Error
RA-224	240.98	537	3.95*	4.502E+00	4.384E+00	4.525E+00	22.02

Flag: "*" = Keyline

Total number of lines in spectrum 75
 Number of unidentified lines 25
 Number of lines tentatively identified by NID 50 66.67%

Nuclide Type :

Nuclide	Hlife	Decay	Uncorrected pCi/GRAM	Decay Corr pCi/GRAM	Decay Corr 2-Sigma Error	2-Sigma %Error	Flags
K-40	1.28E+09Y	1.00	1.728E+01	1.728E+01	0.152E+01	8.80	
MN-54	312.70D	1.07	5.964E-02	6.400E-02	5.153E-02	80.52	
NB-95	35.06D	1.88	6.864E-02	1.288E-01	0.685E-01	53.18	
CD-109	464.00D	1.05	2.803E+00	2.940E+00	0.821E+00	27.91	
SN-126	1.00E+05Y	1.00	2.872E-01	2.872E-01	0.801E-01	27.91	
CS-135	2.30E+06Y	1.00	3.290E-01	3.290E-01	1.619E-01	49.21	
BA-137M	30.17Y	1.00	1.282E-02	1.285E-02	2.494E-02	194.11	
CS-137	30.17Y	1.00	1.355E-02	1.358E-02	2.636E-02	194.11	
EU-155	4.96Y	1.01	1.128E-01	1.142E-01	0.922E-01	80.74	
TB-160	72.30D	1.36	1.438E-01	1.952E-01	1.311E-01	67.18	K
HG-203	46.61D	1.61	3.743E-02	6.010E-02	4.442E-02	73.91	
TL-208	1.91Y	1.03	5.212E-01	5.379E-01	0.665E-01	12.36	
BI-211	7.04E+08Y	1.00	4.139E+00	4.139E+00	0.461E+00	11.13	
BI-212	1.91Y	1.03	9.598E-01	9.906E-01	3.326E-01	33.57	
PB-212	1.91Y	1.03	1.504E+00	1.552E+00	0.169E+00	10.87	
BI-214	1600.00Y	1.00	1.283E+00	1.283E+00	0.159E+00	12.37	
PB-214	1600.00Y	1.00	1.440E+00	1.440E+00	0.177E+00	12.29	
RA-226	1600.00Y	1.00	1.283E+00	1.283E+00	0.159E+00	12.37	
AC-228	5.75Y	1.01	1.340E+00	1.354E+00	0.262E+00	19.34	
RA-228	5.75Y	1.01	1.340E+00	1.354E+00	0.262E+00	19.34	
TH-228	1.91Y	1.03	1.504E+00	1.552E+00	0.169E+00	10.87	
TH-229	7340.00Y	1.00	3.921E-01	3.921E-01	1.094E-01	27.91	K
TH-230	7.70E+04Y	1.00	1.283E+00	1.283E+00	0.159E+00	12.37	
TH-232	1.41E+10Y	1.00	1.504E+00	1.504E+00	0.164E+00	10.87	
TH-234	4.47E+09Y	1.00	1.066E+00	1.066E+00	1.924E+00	180.56	
U-234	2.45E+05Y	1.00	1.520E+00	1.520E+00	0.250E+00	16.44	
U-235	7.04E+08Y	1.00	1.616E-01	1.616E-01	0.492E-01	30.44	K
NP-237	2.14E+06Y	1.00	8.432E-01	8.432E-01	2.927E-01	34.71	
U-238	4.47E+09Y	1.00	1.066E+00	1.066E+00	1.924E+00	180.56	
AM-242	152.00Y	1.00	2.313E+00	2.313E+00	1.868E+00	80.73	
ANH-511	1.00E+09Y	1.00	9.516E-02	9.516E-02	5.504E-02	57.84	
Total Activity :			4.671E+01	4.716E+01			

Nuclide Type : NATURAL

Nuclide	Hlife	Decay	Uncorrected pCi/GRAM	Decay Corr pCi/GRAM	Decay Corr 2-Sigma Error	2-Sigma %Error	Flags
RA-224	1.91Y	1.03	4.384E+00	4.525E+00	0.997E+00	22.02	
Total Activity :			4.384E+00	4.525E+00			

Grand Total Activity : 5.109E+01 5.168E+01

Flags: "K" = Keyline not found "M" = Manually accepted
 "E" = Manually edited "A" = Nuclide specific abn. limit

It	Energy	Area	Bkgnd	FWHM	Channel	Left	Pw	Cts/Sec	%Err	%Eff	Flags
0	128.70	69	574	1.27	255.83	252	8	4.77E-03	****	6.08E+00	
0	153.21	111	506	1.64	304.80	301	8	7.70E-03	74.8	5.86E+00	T
0	217.19	41	433	1.15	432.68	431	9	2.87E-03	****	4.83E+00	
0	327.66	120	455	1.38	653.48	646	14	8.31E-03	77.8	3.66E+00	T
0	408.51	35	247	1.71	815.12	811	9	2.45E-03	****	3.15E+00	
3	467.48	33	126	2.00	933.01	917	20	2.32E-03	****	2.87E+00	T
0	570.73	82	154	2.01	1139.44	1133	14	5.66E-03	68.3	2.48E+00	T
0	643.62	87	188	8.31	1285.18	1274	21	6.03E-03	82.0	2.25E+00	
3	664.36	46	118	2.20	1326.65	1317	15	3.22E-03	95.7	2.20E+00	T
2	771.01	52	94	1.90	1539.94	1527	22	3.60E-03	83.2	1.94E+00	T
0	784.06	25	98	0.80	1566.03	1564	10	1.74E-03	****	1.91E+00	T
0	805.95	16	91	1.00	1609.82	1605	10	1.14E-03	****	1.86E+00	T
0	892.44	25	32	1.24	1782.80	1780	6	1.74E-03	81.4	1.70E+00	
0	938.25	15	64	1.33	1874.43	1871	11	1.02E-03	****	1.62E+00	T
0	1031.67	54	45	1.44	2061.31	2056	11	3.74E-03	56.1	1.48E+00	
0	1072.42	50	130	6.57	2142.83	2134	20	3.50E-03	****	1.43E+00	
0	1240.56	14	37	1.29	2479.25	2476	6	9.49E-04	****	1.25E+00	
0	1408.26	45	70	3.85	2814.85	2809	26	3.15E-03	****	1.12E+00	
0	1471.28	11	17	1.32	2940.98	2934	12	7.37E-04	****	1.09E+00	
0	1508.44	20	40	1.48	3015.34	3009	14	1.38E-03	****	1.07E+00	
0	1565.51	14	6	1.71	3129.58	3126	8	9.93E-04	79.1	1.04E+00	
2	1578.66	18	12	2.60	3155.90	3152	48	1.28E-03	87.5	1.04E+00	
2	1586.70	25	20	2.15	3172.00	3152	48	1.74E-03	87.4	1.03E+00	
2	1589.89	16	24	2.61	3178.38	3152	48	1.11E-03	****	1.03E+00	
0	1619.52	21	12	2.81	3237.70	3233	11	1.47E-03	88.1	1.02E+00	
0	1664.75	17	14	3.17	3328.24	3322	14	1.18E-03	****	1.01E+00	
0	1671.55	6	8	0.76	3341.86	3337	12	3.89E-04	****	1.00E+00	
0	1728.90	22	43	1.22	3456.67	3447	16	1.50E-03	****	9.89E-01	
0	1762.79	179	16	1.59	3524.52	3519	12	1.24E-02	18.3	9.82E-01	
0	1800.67	24	14	9.20	3600.38	3587	28	1.67E-03	97.2	9.75E-01	
0	1834.42	16	17	3.93	3667.94	3660	17	1.11E-03	****	9.70E-01	T
0	1846.85	29	27	1.90	3692.84	3683	21	1.99E-03	****	9.68E-01	
0	1874.58	14	7	1.55	3748.36	3744	9	1.01E-03	83.1	9.65E-01	
0	1909.17	6	17	5.19	3817.62	3806	14	4.09E-04	****	9.63E-01	
0	1972.52	5	2	1.67	3944.49	3942	7	3.70E-04	****	9.60E-01	

Flags: "T" = Tentatively associated

```

*****
*                                     GENERAL ENG. LABS, LLC.                                     *
*                                     2040 Savage Road                                       *
*                                     Charleston, SC 29414                                   *
*****
*                                     DETECTOR DATA                                       *
* Configuration      : DKA300:[CANBERRA.GAMMA.ARCHIVE.GAMMA]G158269003.CNF;1             *
* Acquisition date   : 11-APR-2006 06:14:36  Detector SN#      : 1922864                 *
* Detector ID       : GAMMA16                      Sensitivity   : 3.00000                 *
* Geometry         : CAN                          Energy tolerance: 2.00000                 *
* Elapsed live time: 0 04:00:00.00                Abundance limit  : 75.00000                 *
* Elapsed real time: 0 04:00:02.18                Half life ratio  : 8.00000                 *
*****
*                                     SAMPLE DATA                                       *
* Sample date       : 10-MAR-2006 12:00:00  Nuclide Library   : EPI                       *
* Sample ID        : G158269003              Analyst initials  : MJH1                     *
* Batch Number     : 513802                  Sample Quantity  : 1.29350E+02 GRAM          *
*****
*                                     QC DATA                                           *
* CALIB. DATE/TIME : 5-APR-2006 19:34:04.74MS Isotope      :                      *
* MSD DPM          :                          MSD Isotope    :                      *
* LCS DPM         :                          LCS Isotope     :                      *
*****

```

Combined Activity-MDA Report

---- Identified Nuclides ----

Nuclide	Activity (pCi/GRAM)	Act error	MDA (pCi/GRAM)	MDA error	Act/MDA
K-40	1.728E+01	1.521E+00	3.300E-01	2.178E-02	52.377
MN-54	6.400E-02	5.153E-02	3.852E-02	3.255E-03	1.661
CD-109	2.940E+00	8.206E-01	8.199E-01	8.681E-02	3.586
SN-126	2.872E-01	8.015E-02	8.073E-02	8.530E-03	3.557
CS-135	3.290E-01	1.619E-01	1.654E-01	1.580E-02	1.988
BA-137M	1.285E-02	2.494E-02	3.753E-02	2.305E-03	0.342
CS-137	1.358E-02	2.636E-02	3.968E-02	2.446E-03	0.342
EU-155	1.089E-01	8.885E-02	1.121E-01	9.571E-03	0.972
TB-160	-2.436E-03	1.002E-01	1.706E-01	1.555E-02	-0.014
HG-203	6.010E-02	4.442E-02	5.305E-02	4.397E-03	1.133
TL-208	5.379E-01	6.648E-02	3.846E-02	2.692E-03	13.989
BI-211	4.139E+00	4.607E-01	2.057E-01	1.510E-02	20.119
BI-212	9.906E-01	3.326E-01	3.026E-01	2.609E-02	3.273
PB-212	1.552E+00	1.688E-01	6.141E-02	5.811E-03	25.277
BI-214	1.283E+00	1.587E-01	6.725E-02	5.417E-03	19.080
PB-214	1.440E+00	1.770E-01	7.193E-02	6.467E-03	20.016
RA-224	4.525E+00	9.966E-01	6.987E-01	5.815E-02	6.477
RA-226	1.283E+00	1.587E-01	6.725E-02	5.417E-03	19.080

---- Identified Nuclides ----

Nuclide	Activity (pCi/GRAM)	Act error	MDA (pCi/GRAM)	MDA error	Act/MDA
AC-228	1.354E+00	2.619E-01	1.419E-01	1.675E-02	9.543
RA-228	1.354E+00	2.619E-01	1.419E-01	1.675E-02	9.543
TH-228	1.552E+00	1.688E-01	6.140E-02	5.810E-03	25.279
TH-229	-3.081E-01	3.445E-01	5.595E-01	4.679E-02	-0.551
TH-230	1.283E+00	1.587E-01	6.725E-02	5.417E-03	19.080
TH-232	1.504E+00	1.635E-01	5.949E-02	5.629E-03	25.280
TH-234	1.066E+00	1.924E+00	2.026E+00	4.031E-01	0.526
U-234	1.520E+00	2.499E-01	1.470E-01	1.472E-02	10.342
U-235	7.512E-02	1.345E-01	2.324E-01	3.984E-02	0.323
NP-237	8.432E-01	2.927E-01	2.419E-01	5.602E-02	3.486
U-238	1.066E+00	1.924E+00	2.026E+00	4.031E-01	0.526
AM-242	2.205E+00	1.799E+00	2.257E+00	1.929E-01	0.977
ANH-511	9.516E-02	5.504E-02	3.057E-02	1.860E-03	3.113

---- Non-Identified Nuclides ----

Nuclide	Key-Line Activity (pCi/GRAM)	K.L. Ided	Act error	MDA (pCi/GRAM)	MDA error	Act/MDA
BE-7	-9.145E-02		2.559E-01	4.384E-01	3.042E-02	-0.209
NA-22	-3.328E-02		2.903E-02	4.601E-02	2.990E-03	-0.723
AL-26	-5.810E-03		1.940E-02	2.983E-02	1.716E-03	-0.195
SC-46	-2.216E-02		3.338E-02	4.550E-02	4.216E-03	-0.487
V-48	-6.436E-02		9.088E-02	1.537E-01	1.361E-02	-0.419
CR-51	1.648E-01		3.797E-01	6.406E-01	5.095E-02	0.257
CO-56	8.250E-03		2.799E-02	4.886E-02	4.214E-03	0.169
CO-57	1.018E-03		1.654E-02	2.851E-02	2.209E-03	0.036
CO-58	-9.813E-03		2.779E-02	4.621E-02	3.755E-03	-0.212
FE-59	-3.243E-02		6.825E-02	1.169E-01	9.962E-03	-0.278
CO-60	1.036E-02		2.583E-02	4.730E-02	2.944E-03	0.219
ZN-65	4.875E-02		6.245E-02	1.039E-01	7.868E-03	0.469
SE-75	-2.387E-02		3.244E-02	5.208E-02	4.277E-03	-0.458
KR-85	4.444E+00		5.050E+00	8.178E+00	4.980E-01	0.543
SR-85	2.716E-02		3.085E-02	4.997E-02	3.043E-03	0.543
Y-88	2.963E-02	+	3.804E-02	4.391E-02	2.498E-03	0.675
Y-91	-8.296E-03		2.748E-02	4.688E-02	2.880E-03	-0.177
NB-94	6.406E-03		2.060E-02	3.606E-02	2.397E-03	0.178
NB-95	1.288E-01		6.850E-02	8.313E-02	6.220E-03	1.549
ZR-95	3.300E-02		5.076E-02	9.114E-02	7.620E-03	0.362
RU-103	-2.187E-03		3.204E-02	5.588E-02	7.134E-03	-0.039
RH-106	-1.545E-02		2.067E-01	3.555E-01	2.191E-02	-0.043
RU-106	1.386E-02		2.088E-01	3.620E-01	4.315E-02	0.038
AG-108M	5.032E-03		2.099E-02	3.724E-02	2.378E-03	0.135
AG-110M	-2.454E-03		2.456E-02	3.679E-02	2.392E-03	-0.067
SN-113	-1.848E-02		2.989E-02	5.108E-02	3.133E-03	-0.362
SN-115	5.572E+00	+	5.711E+00	5.746E+00	5.289E-01	0.970
SN-117M	-3.396E-02		8.480E-02	1.420E-01	1.154E-02	-0.239
TE-123M	3.137E-03		2.060E-02	3.516E-02	2.880E-03	0.089
SB-124	3.659E-02		6.592E-02	1.254E-01	8.162E-03	0.292

---- Non-Identified Nuclides ----

Nuclide	Key-Line Activity (pCi/GRAM)	K.L. Ided	Act error	MDA (pCi/GRAM)	MDA error	Act/MDA
SB-125	5.061E-03		6.017E-02	1.059E-01	6.483E-03	0.048
TE-125M	7.955E+00		6.839E+00	1.220E+01	1.225E+00	0.652
I-126	4.199E-01	+	4.028E-01	4.853E-01	3.008E-02	0.865
SB-126	-3.015E-03		2.100E-01	3.613E-01	2.484E-02	-0.008
I-131	6.362E-02		2.958E-01	5.286E-01	3.863E-02	0.120
BA-133	-2.372E-03		2.845E-02	4.432E-02	5.329E-03	-0.054
CS-134	9.381E-02	+	3.775E-02	5.847E-02	4.646E-03	1.604
CS-136	-5.688E-03		1.633E-01	2.897E-01	2.520E-02	-0.020
CE-139	-2.402E-03		2.068E-02	3.493E-02	2.899E-03	-0.069
BA-140	-1.080E-01		3.798E-01	6.482E-01	2.112E-01	-0.167
LA-140	1.129E-01		1.340E-01	2.614E-01	1.616E-02	0.432
CE-141	2.693E-02		5.570E-02	9.646E-02	7.765E-03	0.279
CE-144	3.674E-02		1.349E-01	2.328E-01	3.515E-02	0.158
PM-144	-3.715E-03		2.266E-02	3.842E-02	2.530E-03	-0.097
PM-146	2.497E-03		2.600E-02	4.590E-02	4.006E-03	0.054
ND-147	7.629E-01		9.939E-01	1.799E+00	2.459E-01	0.424
PM-147	-5.193E+03		3.325E+04	5.691E+04	4.413E+03	-0.091
EU-152	-1.470E-02		6.450E-02	1.049E-01	7.941E-03	-0.140
GD-153	-5.166E-02		5.638E-02	8.405E-02	7.670E-03	-0.615
EU-154	-9.230E-02		8.067E-02	1.274E-01	1.246E-02	-0.725
TM-171	-1.000E+01		2.642E+01	4.116E+01	4.702E+00	-0.243
HF-181	7.040E-03		3.435E-02	6.076E-02	3.662E-03	0.116
TA-182	5.449E-03		1.305E-01	2.298E-01	1.535E-02	0.024
IR-192	-4.156E-03		2.656E-02	4.357E-02	3.273E-03	-0.095
BI-207	1.340E-02		3.180E-02	5.837E-02	4.749E-03	0.230
BI-210	-9.069E-02		8.758E+00	1.297E+01	1.324E+00	-0.007
PB-210	-9.069E-02		8.758E+00	1.297E+01	1.324E+00	-0.007
PB-211	-9.519E-02		6.717E-01	1.027E+00	6.403E-01	-0.093
RN-219	9.780E-02		2.561E-01	4.580E-01	6.228E-02	0.214
RA-223	-1.751E-01		5.144E-01	7.349E-01	1.258E-01	-0.238
AC-227	3.043E-02		2.538E-01	4.256E-01	6.507E-02	0.072
TH-227	2.992E-02		2.495E-01	4.183E-01	7.481E-02	0.072
PA-231	2.001E-01		1.011E+00	1.695E+00	2.512E-01	0.118
TH-231	3.870E-01	+	1.902E-01	2.509E-01	2.319E-02	1.543
PA-233	-1.037E-02		4.079E-02	6.668E-02	5.231E-03	-0.156
PA-234	2.683E-02		1.724E-01	3.135E-01	5.957E-02	0.086
PA-234M	2.836E+00		2.939E+00	5.530E+00	5.548E-01	0.513
NP-239	-1.108E-01		1.198E-01	1.993E-01	1.569E-02	-0.556
AM-241	-1.337E-01		1.741E-01	2.668E-01	3.614E-02	-0.501
CM-247	5.728E-03		2.324E-02	4.133E-02	2.391E-03	0.139
CF-249	1.266E-02		2.451E-02	4.423E-02	2.586E-03	0.286
CF-251	-3.132E-02		8.328E-02	1.389E-01	1.155E-02	-0.225

```

*****
*
*                               General Engineering Labs, LLC
*                               2040 SAVAGE ROAD
*                               CHARLESTON ,SC 29417
*                               GROSS GAMMA REPORT
*
*****
*
* BATCH ID      : 513802          SAMPLE ID   : G158269003
* ANALYST      : MJH1            DETECTOR    : GAMMA16
* SAMPLE DATE   : 10-MAR-2006 12:00:00.00  COUNT TIME  : 0 04:00:00.00
* ANALYSIS DATE: 11-APR-2006 06:14:36.24  SAMPLE ALQT: 129.350 GRAM
*
*****

```

```

GROSS GAMMA ACTIVITY (pCi/GRAM ) : 8.756E+00
GROSS GAMMA ERROR   (pCi/GRAM ) : 1.917E+00
GROSS GAMMA MDA     (pCi/GRAM ) : 5.839E+00
GROSS GAMMA DLC     (pCi/GRAM ) : 2.838E+00

```

VAX/VMS Nuclide Identification Report Generated 11-APR-2006 14:23:09.00

```

*****
*                               GENERAL ENG. LABS, LLC.                               *
*                               2040 Savage Road                                       *
*                               Charleston, SC 29414                                   *
*****
Configuration : DKA300:[CANBERRA.GAMMA.ARCHIVE.GAMMA]G158269004.CNF;1
Sample date   : 10-MAR-2006 12:00:00 Acquisition date : 11-APR-2006 10:22:44
Sample ID    : G158269004 Sample quantity : 1.24660E+02 GRAM
Detector name : GAMMA16 Detector geometry: CAN
Elapsed live time: 0 04:00:00.00 Elapsed real time: 0 04:00:02.11 0.0%
Energy tolerance : 2.00000 KEV Analyst Initials : MJH1
Abundance limit : 75.00000 Sensitivity : 3.00000
Batch ID       : 513802 Detector SN# : 1922864
Matrix Spike DPM : LCS DPM :
*****

```

Pk	It	Energy	Area	Bkgnd	FWHM	Channel	Left	Pw	Cts/Sec	%Err	Fit
1	0	63.00*	104	719	0.74	124.52	121	10	7.24E-03	50.5	
2	3	72.72*	108	484	1.31	143.96	141	23	7.52E-03	34.8	8.33E-01
3	3	74.83*	540	552	1.17	148.17	141	23	3.75E-02	8.8	
4	3	77.03*	807	458	1.00	152.57	141	23	5.60E-02	5.7	
5	4	84.15*	108	522	1.20	166.80	163	28	7.47E-03	37.2	1.81E+00
6	4	87.18*	412	581	1.32	172.86	163	28	2.86E-02	11.4	
7	4	89.83	202	355	0.92	178.15	163	28	1.40E-02	15.9	
8	4	92.73*	387	621	1.57	183.94	163	28	2.69E-02	13.8	
9	0	99.13	96	412	1.34	196.74	193	7	6.66E-03	36.6	
10	0	105.15*	92	482	0.85	208.76	205	8	6.38E-03	44.6	
11	0	128.40*	56	552	1.06	255.23	252	8	3.89E-03	75.2	
12	0	143.67*	83	544	1.90	285.75	281	9	5.79E-03	53.6	
13	0	185.87*	328	609	1.12	370.08	365	11	2.28E-02	16.3	
14	0	209.56	213	483	1.09	417.43	413	10	1.48E-02	20.6	
15	3	238.46*	1933	288	1.10	475.20	472	16	1.34E-01	2.8	2.71E+00
16	3	241.54*	581	343	1.71	481.34	472	16	4.04E-02	9.0	
17	0	269.84	161	305	1.33	537.92	535	9	1.12E-02	21.0	
18	0	276.77	56	336	0.66	551.76	547	9	3.88E-03	60.6	
19	0	294.87*	723	273	1.14	587.93	583	10	5.02E-02	5.8	
20	0	299.71*	96	300	1.44	597.61	594	8	6.63E-03	33.9	
21	0	327.05	107	465	1.56	652.27	648	15	7.45E-03	44.6	
22	0	338.15*	365	238	1.17	674.46	671	9	2.54E-02	9.8	
23	0	351.64*	1071	314	1.28	701.42	696	12	7.44E-02	4.6	
24	0	409.29*	44	207	0.63	816.66	813	10	3.07E-03	65.9	
25	0	462.64	123	152	1.27	923.32	919	9	8.56E-03	20.1	
26	0	510.54*	157	223	2.16	1019.09	1012	14	1.09E-02	26.8	
27	0	562.45	48	112	0.84	1122.88	1119	9	3.36E-03	41.7	
28	0	582.86*	667	166	1.62	1163.69	1158	14	4.63E-02	5.8	
29	0	608.83*	789	253	1.33	1215.62	1208	16	5.48E-02	5.9	
30	0	640.44	11	88	1.56	1278.82	1277	9	7.57E-04	158.0	
31	0	656.77	19	80	1.24	1311.47	1309	8	1.32E-03	84.7	
32	0	661.51*	7	66	2.27	1320.95	1318	7	4.67E-04	247.6	
33	0	664.78	33	56	1.10	1327.48	1325	7	2.29E-03	41.4	
34	0	726.48	132	148	1.48	1450.88	1446	13	9.14E-03	20.9	
35	0	741.55	17	57	1.44	1481.01	1478	7	1.15E-03	80.1	
36	0	767.18*	41	157	1.16	1532.27	1529	12	2.82E-03	65.7	
37	0	772.05*	18	71	1.49	1542.02	1540	8	1.25E-03	91.6	
38	0	784.12	27	80	2.29	1566.15	1563	9	1.90E-03	61.7	

Pk	It	Energy	Area	Bkgnd	FWHM	Channel	Left	Pw	Cts/Sec	%Err	Fit
39	0	794.53*	83	136	1.71	1586.97	1582	14	5.75E-03	32.2	
40	0	804.02*	29	54	3.39	1605.95	1602	9	2.03E-03	53.2	
41	0	811.82*	13	38	1.76	1621.55	1619	6	8.77E-04	96.5	
42	0	836.27*	12	71	1.29	1670.44	1664	8	8.19E-04	133.4	
43	0	860.01*	77	88	1.14	1717.93	1713	11	5.32E-03	29.4	
44	0	871.02	32	88	5.76	1739.96	1735	15	2.23E-03	65.6	
45	0	910.53*	419	104	1.65	1818.98	1812	16	2.91E-02	7.7	
46	0	932.76*	50	52	1.15	1863.46	1859	9	3.47E-03	32.0	
47	0	957.89*	34	96	2.50	1913.71	1908	14	2.38E-03	64.8	
48	1	963.85*	61	63	1.66	1925.63	1922	18	4.25E-03	27.4	2.37E+00
49	1	968.21*	256	84	1.88	1934.37	1922	18	1.78E-02	9.5	
50	0	1000.00*	9	76	0.61	1997.96	1994	10	6.48E-04	203.7	
51	0	1042.99	41	51	1.58	2083.94	2080	13	2.88E-03	38.1	
52	0	1077.39	26	68	3.51	2152.77	2146	12	1.82E-03	66.2	
53	0	1119.45*	169	75	1.39	2236.93	2233	12	1.17E-02	13.2	
54	0	1189.34	19	40	1.78	2376.76	2373	8	1.30E-03	64.0	
55	0	1280.59*	26	45	3.21	2559.35	2556	12	1.81E-03	57.1	
56	0	1354.39	15	21	1.39	2707.03	2703	9	1.06E-03	60.7	
57	0	1361.09	39	19	3.83	2720.43	2713	15	2.74E-03	28.7	
58	0	1376.55	35	40	1.72	2751.37	2746	10	2.43E-03	37.8	
59	0	1384.93	42	23	4.03	2768.16	2762	15	2.90E-03	29.2	
60	1	1406.55*	35	19	2.28	2811.41	2804	45	2.41E-03	38.0	1.82E+00
61	1	1408.34*	17	18	2.07	2815.00	2804	45	1.21E-03	68.3	
62	0	1452.24	16	10	1.13	2902.87	2900	7	1.13E-03	40.9	
63	0	1459.53*	1686	80	1.87	2917.45	2910	17	1.17E-01	2.8	
64	1	1587.41	74	23	2.37	3173.43	3166	24	5.12E-03	16.8	5.11E+00
65	1	1590.20*	35	17	2.16	3179.00	3166	24	2.46E-03	35.0	
66	0	1619.47*	13	15	1.97	3237.60	3233	10	9.20E-04	68.3	
67	0	1636.97	28	18	0.60	3272.63	3266	15	1.93E-03	38.9	
68	0	1721.26	12	5	1.91	3441.38	3437	10	8.33E-04	45.3	
69	1	1744.12*	12	7	2.44	3487.14	3483	27	8.32E-04	48.0	6.71E-01
70	1	1748.54	12	5	2.22	3496.00	3483	27	8.59E-04	51.2	
71	0	1762.61*	151	17	2.80	3524.17	3514	22	1.05E-02	11.2	
72	0	1801.11	16	0	0.88	3601.25	3596	12	1.11E-03	25.0	
73	0	1811.71	11	18	0.66	3622.48	3614	12	7.50E-04	84.4	
74	0	1846.37*	19	22	3.08	3691.88	3680	17	1.31E-03	62.8	
75	0	1985.05	6	16	4.93	3969.59	3952	21	4.14E-04	171.8	
76	0	1996.44	11	3	3.28	3992.40	3987	13	7.34E-04	46.9	
77	6	2025.70	21	12	2.34	4051.00	4040	41	1.44E-03	36.4	1.37E+00
78	6	2036.50	16	10	4.15	4072.63	4040	41	1.10E-03	55.4	

Flag: "*" = Peak area was modified by background subtraction

VAX/VMS Nuclide Identification Report Generated

```

*****
*                               General Eng. Labs, LLC.                               *
*                               2040 Savage Road                                       *
*                               Charleston, SC 29414                                   *
*****
*                               DETECTOR DATA                                       *
*
* Configuration      : DKA300:[CANBERRA.GAMMA.ARCHIVE.GAMMA]G158269004
* Acquisition date   : 11-APR-2006 10:22:44 Detector SN#      : 1922864
* Detector ID        : GAMMA16                      Sensitivity    : 3.000
* Geometry           : CAN                          Energy tolerance: 2.000
* Elapsed live time  : 0 04:00:00.00                Abundance limit : 75.000
* Elapsed real time  : 0 04:00:02.11                Half life ratio  : 8.000
*****
*                               SAMPLE DATA                                         *
*
* Sample date        : 10-MAR-2006 12:00:00 Nuclide Library :
* Sample ID          : G158269004                    Analyst initials: MJH1
* Batch Number       : 513802                         Sample Quantity : 1.2466E+02 GRAM
* Recovery           : 1.00000                       Carrier Weight   : 0.00000
*****
*                               QC DATA                                             *
*
* Standard Weight    : 0.00000
* CALIB. DATE/TIME   : 5-APR-2006 19:34:04 MS Isotope      :
* MSD DPM             : 0.000                          MSD Isotope      :
* LCS DPM             : 0.000                          LCS Isotope      :
* LCSD DPM           : 0.000                          LCSD Isotope     :
*****

```

Combined Activity-MDA Report

---- Identified Nuclides ----

Nuclide	Activity (pCi/GRAM)	Act error	MDA (pCi/GRAM)	
K-40	2.177E+01	1.871E+00	4.282E-01	0.000E+00
MN-54	1.060E-02	2.828E-02	4.843E-02	0.000E+00
CO-58	1.413E-02	2.730E-02	5.050E-02	0.000E+00
CD-109	3.696E+00	9.276E-01	8.750E-01	0.000E+00
SN-126	3.609E-01	9.058E-02	8.614E-02	0.000E+00
CS-135	3.635E-01	1.564E-01	1.688E-01	0.000E+00
BA-137M	5.113E-03	2.533E-02	3.109E-02	0.000E+00
CS-137	5.405E-03	2.677E-02	3.287E-02	0.000E+00
CE-141	6.738E-02	7.458E-02	9.497E-02	0.000E+00
GD-153	9.244E-02	6.818E-02	9.491E-02	0.000E+00
EU-155	1.132E-01	1.020E-01	1.238E-01	0.000E+00
TL-208	5.051E-01	6.852E-02	4.006E-02	0.000E+00
BI-211	3.577E+00	4.216E-01	2.311E-01	0.000E+00
BI-212	8.497E-01	3.625E-01	3.136E-01	0.000E+00
PB-212	1.483E+00	1.628E-01	6.663E-02	0.000E+00
BI-214	1.089E+00	1.549E-01	7.307E-02	0.000E+00
PB-214	1.244E+00	1.604E-01	7.857E-02	0.000E+00
RA-224	5.080E+00	1.010E+00	7.389E-01	0.000E+00
RA-226	1.089E+00	1.549E-01	7.307E-02	0.000E+00
AC-228	1.380E+00	2.674E-01	1.497E-01	0.000E+00
RA-228	1.380E+00	2.674E-01	1.497E-01	0.000E+00
TH-228	1.483E+00	1.628E-01	6.662E-02	0.000E+00
TH-229	-2.208E-01	3.338E-01	5.628E-01	0.000E+00
TH-230	1.089E+00	1.549E-01	7.307E-02	0.000E+00
TH-232	1.437E+00	1.577E-01	6.454E-02	0.000E+00
PA-234M	1.089E+00	4.439E+00	4.614E+00	0.000E+00
TH-234	2.328E+00	2.398E+00	2.144E+00	0.000E+00
U-234	1.443E+00	2.211E-01	1.511E-01	0.000E+00
U-235	1.998E-01	2.169E-01	2.534E-01	0.000E+00
NP-237	1.060E+00	3.443E-01	2.581E-01	0.000E+00
U-238	2.328E+00	2.398E+00	2.144E+00	0.000E+00
AM-242	2.294E+00	2.066E+00	2.417E+00	0.000E+00
ANH-511	8.803E-02	4.754E-02	3.324E-02	0.000E+00

---- Non-Identified Nuclides ----

Nuclide	Key-Line Activity (pCi/GRAM	K.L. Act error) Ided	MDA (pCi/GRAM)	
BE-7	9.917E-02	2.540E-01	4.605E-01	0.000E+00	NOT IDENT.
NA-22	-1.468E-02	2.589E-02	4.355E-02	0.000E+00	NOT IDENT.
NA-24	0.000E+00	5.511E+13	0.000E+00	0.000E+00	SHORT HLIF
AL-26	1.399E-02	2.023E-02	3.776E-02	0.000E+00	FAIL ABUN
SC-46	2.460E-04	3.220E-02	5.489E-02	0.000E+00	FAIL ABUN
V-48	5.071E-02	8.968E-02	1.681E-01	0.000E+00	NOT IDENT.
CR-51	9.244E-02	3.855E-01	6.584E-01	0.000E+00	NOT IDENT.
CO-56	2.181E-02	2.915E-02	5.289E-02	0.000E+00	NOT IDENT.
MN-56	0.000E+00	1.336E+41	0.000E+00	0.000E+00	SHORT HLIF
CO-57	2.654E-03	1.637E-02	2.931E-02	0.000E+00	NOT IDENT.
FE-59	-2.244E-02	7.595E-02	1.321E-01	0.000E+00	NOT IDENT.
CO-60	-1.148E-03	2.693E-02	4.744E-02	0.000E+00	NOT IDENT.
ZN-65	-3.007E-02	7.143E-02	1.049E-01	0.000E+00	NOT IDENT.
SE-75	-7.799E-03	3.274E-02	5.519E-02	0.000E+00	NOT IDENT.
KR-85	5.658E+00	4.823E+00	8.139E+00	0.000E+00	NOT IDENT.
SR-85	3.463E-02	2.952E-02	4.982E-02	0.000E+00	NOT IDENT.
Y-88	-2.729E-03	2.340E-02	4.336E-02	0.000E+00	NOT IDENT.
Y-91	-2.774E-04	2.795E-02	4.921E-02	0.000E+00	NOT IDENT.
NB-94	1.307E-02	2.192E-02	3.932E-02	0.000E+00	FAIL ABUN
NB-95	5.919E-02	7.787E-02	8.542E-02	0.000E+00	FAIL ABUN
NB-95M	0.000E+00	3.610E+01	0.000E+00	0.000E+00	SHORT HLIF
ZR-95	8.202E-03	5.333E-02	9.327E-02	0.000E+00	NOT IDENT.
MO-99	0.000E+00	5.963E+01	0.000E+00	0.000E+00	SHORT HLIF
TC-99M	0.000E+00	5.535E+36	0.000E+00	0.000E+00	SHORT HLIF
RU-103	-7.517E-03	3.444E-02	6.030E-02	0.000E+00	FAIL ABUN
RH-106	-7.925E-03	2.025E-01	3.539E-01	0.000E+00	FAIL ABUN
RU-106	-1.806E-02	2.019E-01	3.518E-01	0.000E+00	NOT IDENT.
AG-108M	4.723E-03	2.030E-02	3.673E-02	0.000E+00	NOT IDENT.
AG-110M	1.493E-02	2.531E-02	3.975E-02	0.000E+00	FAIL ABUN
SN-113	3.605E-03	3.307E-02	5.947E-02	0.000E+00	NOT IDENT.
CD-115	0.000E+00	1.279E+03	0.000E+00	0.000E+00	SHORT HLIF
SN-115	5.717E+00	3.695E+00	6.005E+00	0.000E+00	FAIL ABUN
SN-117M	5.354E-02	8.472E-02	1.514E-01	0.000E+00	NOT IDENT.
TE-123M	2.373E-02	2.042E-02	3.704E-02	0.000E+00	NOT IDENT.
SB-124	-1.544E-02	6.117E-02	1.058E-01	0.000E+00	NOT IDENT.
SB-125	-4.650E-03	5.842E-02	1.040E-01	0.000E+00	FAIL ABUN
TE-125M	2.903E+00	7.236E+00	1.310E+01	0.000E+00	NOT IDENT.
I-126	3.131E-01	2.602E-01	4.715E-01	0.000E+00	FAIL ABUN
SB-126	2.653E-02	2.299E-01	4.017E-01	0.000E+00	FAIL ABUN
SB-127	0.000E+00	1.813E+01	0.000E+00	0.000E+00	SHORT HLIF
I-131	-7.754E-02	3.107E-01	5.533E-01	0.000E+00	NOT IDENT.
I-132	0.000E+00	6.310E+41	0.000E+00	0.000E+00	SHORT HLIF
TE-132	0.000E+00	1.688E+01	0.000E+00	0.000E+00	SHORT HLIF
BA-133	-1.176E-02	3.031E-02	4.703E-02	0.000E+00	FAIL ABUN
I-133	0.000E+00	2.763E+09	0.000E+00	0.000E+00	SHORT HLIF
CS-134	0.000E+00	5.169E-02	5.780E-02	0.000E+00	FAIL ABUN
I-135	0.000E+00	9.740E+33	0.000E+00	0.000E+00	SHORT HLIF
CS-136	-1.180E-01	1.906E-01	2.754E-01	0.000E+00	FAIL ABUN
CE-139	-1.319E-02	2.125E-02	3.626E-02	0.000E+00	NOT IDENT.
BA-140	1.189E-01	4.065E-01	7.272E-01	0.000E+00	NOT IDENT.
LA-140	-5.149E-03	1.450E-01	2.231E-01	0.000E+00	FAIL ABUN
CE-143	0.000E+00	2.067E+06	0.000E+00	0.000E+00	SHORT HLIF
CE-144	1.536E-02	1.396E-01	2.477E-01	0.000E+00	NOT IDENT.
PM-144	-2.282E-03	2.199E-02	3.790E-02	0.000E+00	NOT IDENT.
PR-144	0.000E+00	9.635E+41	0.000E+00	0.000E+00	SHORT HLIF
PM-146	2.065E-02	2.813E-02	5.186E-02	0.000E+00	NOT IDENT.
ND-147	3.062E-01	1.051E+00	1.884E+00	0.000E+00	FAIL ABUN
PM-147	-1.432E+04	3.302E+04	5.787E+04	0.000E+00	NOT IDENT.
PM-149	0.000E+00	1.191E+04	0.000E+00	0.000E+00	SHORT HLIF
EU-152	-1.264E-02	6.282E-02	1.045E-01	0.000E+00	FAIL ABUN
EU-154	-3.997E-02	7.183E-02	1.208E-01	0.000E+00	NOT IDENT.
TB-160	7.529E-02	1.066E-01	1.927E-01	0.000E+00	FAIL ABUN
TM-171	5.812E+00	2.678E+01	4.458E+01	0.000E+00	NOT IDENT.
HF-181	-9.127E-03	3.510E-02	6.144E-02	0.000E+00	NOT IDENT.
TA-182	3.498E-02	1.442E-01	2.567E-01	0.000E+00	FAIL ABUN
IR-192	-3.568E-02	2.760E-02	4.313E-02	0.000E+00	FAIL ABUN
HG-203	3.068E-02	4.042E-02	6.370E-02	0.000E+00	FAIL ABUN
BI-207	9.247E-03	3.514E-02	6.370E-02	0.000E+00	NOT IDENT.
BI-210	-3.632E+00	8.927E+00	1.353E+01	0.000E+00	NOT IDENT.
PB-210	-3.632E+00	8.927E+00	1.353E+01	0.000E+00	NOT IDENT.
PB-211	-5.513E-01	6.828E-01	1.007E+00	0.000E+00	NOT IDENT.
RN-219	3.749E-02	2.612E-01	4.709E-01	0.000E+00	FAIL ABUN

RA-223	1.337E-01	4.703E-01	7.198E-01	0.000E+00	FAIL	ABUN
AC-227	1.286E-01	2.655E-01	4.616E-01	0.000E+00	FAIL	ABUN
TH-227	1.264E-01	2.612E-01	4.537E-01	0.000E+00	FAIL	ABUN
PA-231	3.855E-01	1.046E+00	1.804E+00	0.000E+00	FAIL	ABUN
TH-231	0.000E+00	1.837E-01	2.542E-01	0.000E+00	FAIL	ABUN
PA-233	-3.701E-03	4.314E-02	7.261E-02	0.000E+00	FAIL	ABUN
PA-234	-9.575E-02	1.999E-01	3.457E-01	0.000E+00	FAIL	ABUN
NP-239	-7.346E-02	1.182E-01	2.061E-01	0.000E+00	FAIL	ABUN
AM-241	-1.220E-01	1.739E-01	2.792E-01	0.000E+00	NOT	IDENT.
CM-247	-1.469E-02	2.343E-02	4.064E-02	0.000E+00	FAIL	ABUN
CF-249	1.186E-02	2.676E-02	4.885E-02	0.000E+00	NOT	IDENT.
CF-251	-2.651E-02	8.458E-02	1.455E-01	0.000E+00	NOT	IDENT.

```

*****
*                               GENERAL ENG. LABS, LLC.                               *
*                               2040 Savage Road                                   *
*                               Charleston, SC 29414                               *
*****
Configuration      : DKA300:[CANBERRA.GAMMA.ARCHIVE.GAMMA]G158269004.CNF;1
Sample date        : 10-MAR-2006 12:00:00 Acquisition date : 11-APR-2006 10:22:44
Sample ID          : G158269004           Sample quantity  : 1.24660E+02 GRAM
Detector name     : GAMMA16              Detector geometry: CAN
Elapsed live time : 0 04:00:00.00        Elapsed real time: 0 04:00:02.11  0.0%
Energy tolerance  : 2.00000 KEV          Analyst Initials  : MJH1
Abundance limit   : 75.00000             Sensitivity       : 3.00000
Batch ID          : 513802               Detector SN#      : 1922864
Matrix Spike DPM  :                      LCS DPM          :
*****
    
```

Nuclide Line Activity Report

Nuclide Type:

Nuclide	Energy	Area	%Abn	%Eff	Uncorrected pCi/GRAM	Decay Corr pCi/GRAM	2-Sigma %Error
K-40	1460.81	1686	10.67*	1.093E+00	2.177E+01	2.177E+01	8.60
MN-54	834.83	12	99.83*	1.802E+00	9.869E-03	1.060E-02	266.87
CO-58	810.78	13	99.45*	1.851E+00	1.033E-02	1.413E-02	193.19
NB-95	765.79	41	99.81*	1.946E+00	3.143E-02	5.919E-02	131.57
CD-109	88.03	412	3.79*	4.642E+00	3.523E+00	3.696E+00	25.10
SN-126	64.28	104	9.60	1.774E+00	9.214E-01	9.214E-01	102.55
	86.94	412	8.90	4.642E+00	1.500E+00	1.500E+00	47.60
	87.57	412	37.00*	4.642E+00	3.609E-01	3.609E-01	25.10
CS-135	268.24	161	16.00*	4.174E+00	3.635E-01	3.635E-01	43.02
BA-137M	661.65	7	89.98*	2.205E+00	5.103E-03	5.113E-03	495.31
CS-137	661.66	7	85.12*	2.205E+00	5.394E-03	5.405E-03	495.31
CE-141	145.44	83	48.40*	5.982E+00	4.335E-02	8.581E-02	107.47
GD-153	69.67	-----	2.57	2.650E+00	-----	Line Not Found	-----
	83.37	108	0.22	4.359E+00	1.689E+01	1.851E+01	75.09
	97.43	96	31.30*	5.473E+00	8.432E-02	9.244E-02	73.76
	103.18	92	22.20	5.736E+00	1.086E-01	1.191E-01	89.63
EU-155	86.54	412	30.90	4.642E+00	4.321E-01	4.375E-01	25.13
	105.31	92	20.70*	5.736E+00	1.165E-01	1.179E-01	89.64
TL-208	75.00	540	3.43	3.313E+00	7.158E+00	7.390E+00	22.27
	277.35	56	6.80	4.103E+00	3.016E-01	3.113E-01	121.76
	510.84	157	21.60	2.690E+00	4.075E-01	4.207E-01	54.65
	583.14	667	84.20*	2.437E+00	4.893E-01	5.051E-01	13.57
	763.30	-----	1.64	1.954E+00	-----	Line Not Found	-----
	860.37	77	12.46	1.756E+00	5.268E-01	5.439E-01	59.54
	1093.90	-----	0.37	1.403E+00	-----	Line Not Found	-----
BI-211	351.07	1071	12.94*	3.485E+00	3.577E+00	3.577E+00	11.79
BI-212	727.18	132	11.80*	2.039E+00	8.231E-01	8.497E-01	42.66
PB-212	74.80	540	10.70	3.313E+00	2.295E+00	2.369E+00	22.51
	87.30	412	8.00	4.642E+00	1.669E+00	1.723E+00	27.02
	115.19	-----	0.60	5.993E+00	-----	Line Not Found	-----
	238.63	1933	44.60*	4.541E+00	1.437E+00	1.483E+00	10.98
	300.09	96	3.41	3.885E+00	1.086E+00	1.121E+00	68.56

Nuclide Type:

Nuclide	Energy	Area	%Abn	%Eff	Uncorrected pCi/GRAM	Decay Corr pCi/GRAM	2-Sigma %Error
BI-214	609.31	789	46.30*	2.356E+00	1.089E+00	1.089E+00	14.22
	768.36	41	5.04	1.946E+00	6.224E-01	6.225E-01	131.70
	934.06	50	3.21	1.629E+00	1.440E+00	1.440E+00	64.92
	1120.29	169	15.10	1.373E+00	1.228E+00	1.228E+00	28.15
	1238.11	-----	5.94	1.252E+00	-----	Line Not Found	-----
1377.67	35	4.11	1.143E+00	1.121E+00	1.121E+00	76.11	
PB-214	74.81	540	6.21	3.313E+00	3.954E+00	3.954E+00	21.78
	77.11	807	10.50	3.581E+00	3.231E+00	3.231E+00	17.30
	87.30	412	4.41	4.642E+00	3.028E+00	3.028E+00	26.39
	241.98	581	7.50	4.502E+00	2.592E+00	2.592E+00	20.65
	295.21	723	19.20	3.929E+00	1.443E+00	1.443E+00	15.32
RA-226	351.92	1071	37.20*	3.485E+00	1.244E+00	1.244E+00	12.89
	295.21	723	19.20	3.929E+00	1.443E+00	1.443E+00	15.32
	351.92	1071	37.20	3.485E+00	1.244E+00	1.244E+00	11.47
AC-228	609.31	789	46.30*	2.356E+00	1.089E+00	1.089E+00	14.22
	209.25	213	4.40	4.947E+00	1.473E+00	1.488E+00	76.29
	338.32	365	11.40	3.579E+00	1.348E+00	1.362E+00	45.41
	463.01	123	4.40	2.886E+00	1.461E+00	1.476E+00	46.59
	794.95	83	4.60	1.886E+00	1.436E+00	1.452E+00	68.41
	911.21	419	27.70*	1.666E+00	1.365E+00	1.380E+00	19.38
RA-228	964.77	61	5.20	1.580E+00	1.120E+00	1.132E+00	60.05
	969.11	256	16.60	1.573E+00	1.474E+00	1.490E+00	30.25
	209.25	213	4.40	4.947E+00	1.473E+00	1.488E+00	76.29
	338.32	365	11.40	3.579E+00	1.348E+00	1.362E+00	45.41
	463.01	123	4.40	2.886E+00	1.461E+00	1.476E+00	46.59
	794.95	83	4.60	1.886E+00	1.436E+00	1.452E+00	68.41
TH-228	911.21	419	27.70*	1.666E+00	1.365E+00	1.380E+00	19.38
	964.77	61	5.20	1.580E+00	1.120E+00	1.132E+00	60.05
	969.11	256	16.60	1.573E+00	1.474E+00	1.490E+00	30.25
	84.40	108	1.21	4.359E+00	3.070E+00	3.170E+00	75.75
TH-229	238.60	1933	44.60*	4.541E+00	1.437E+00	1.483E+00	10.98
	300.10	96	3.41	3.885E+00	1.086E+00	1.121E+00	90.04
	85.43	108	16.50	4.359E+00	2.252E-01	2.252E-01	75.09
TH-230	88.47	412	27.10	4.642E+00	4.927E-01	4.927E-01	25.10
	100.00	96	12.40	5.473E+00	2.128E-01	2.128E-01	73.76
	193.63	-----	4.59*	5.199E+00	-----	Line Not Found	-----
	210.97	213	3.26	4.947E+00	1.985E+00	1.985E+00	42.09
	295.21	723	19.20	3.929E+00	1.443E+00	1.443E+00	15.32
TH-232	351.92	1071	37.20	3.485E+00	1.244E+00	1.244E+00	11.47
	609.31	789	46.30*	2.356E+00	1.089E+00	1.089E+00	14.22
	238.59	1933	44.60*	4.541E+00	1.437E+00	1.437E+00	10.98
PA-234M	911.20	419	27.70	1.666E+00	1.365E+00	1.365E+00	19.38
	964.40	61	5.20	1.580E+00	1.120E+00	1.120E+00	60.05
	969.11	256	16.60	1.573E+00	1.474E+00	1.474E+00	30.25
TH-234	766.40	41	0.21	1.946E+00	1.494E+01	1.494E+01	152.04
	1001.03	9	0.85*	1.526E+00	1.089E+00	1.089E+00	407.59
	63.29	104	3.80*	1.774E+00	2.328E+00	2.328E+00	103.01
TH-234	92.38	387	5.41	5.083E+00	2.121E+00	2.121E+00	33.27
	112.81	-----	0.24	5.950E+00	-----	Line Not Found	-----

Nuclide Type:

Nuclide	Energy	Area	%Abn	%Eff	Uncorrected pCi/GRAM	Decay Corr pCi/GRAM	2-Sigma %Error
U-234	67.67	-----	0.37	2.385E+00	-----	Line Not Found	-----
	241.98	581	7.49	4.502E+00	2.595E+00	2.595E+00	20.65
	295.21	723	19.20*	3.929E+00	1.443E+00	1.443E+00	15.32
	351.92	1071	37.20	3.485E+00	1.244E+00	1.244E+00	12.89
U-235	89.95	202	2.70	4.865E+00	2.317E+00	2.317E+00	44.59
	93.35	387	4.50	5.083E+00	2.550E+00	2.550E+00	39.57
	105.00	92	2.10	5.736E+00	1.148E+00	1.148E+00	94.07
	143.76	83	10.50*	5.982E+00	1.998E-01	1.998E-01	108.53
	163.33	-----	4.70	5.703E+00	-----	Line Not Found	-----
	185.71	328	54.00	5.327E+00	1.715E-01	1.715E-01	33.67
NP-237	205.31	-----	5.00	5.012E+00	-----	Line Not Found	-----
	86.48	412	12.60*	4.642E+00	1.060E+00	1.060E+00	32.49
	95.87	-----	2.60	5.290E+00	-----	Line Not Found	-----
U-238	63.29	104	3.80*	1.774E+00	2.328E+00	2.328E+00	103.01
AM-242	99.55	96	0.63	5.473E+00	4.189E+00	4.191E+00	73.76
	103.70	92	1.01*	5.736E+00	2.387E+00	2.388E+00	89.63
ANH-511	511.00	157	100.00*	2.690E+00	8.803E-02	8.803E-02	54.01

Nuclide Type: NATURAL

Nuclide	Energy	Area	%Abn	%Eff	Uncorrected pCi/GRAM	Decay Corr pCi/GRAM	2-Sigma %Error
RA-224	240.98	581	3.95*	4.502E+00	4.921E+00	5.080E+00	19.88

Flag: "*" = Keyline

Total number of lines in spectrum 78
 Number of unidentified lines 26
 Number of lines tentatively identified by NID 52 66.67%

Nuclide Type :

Nuclide	Hlife	Decay	Uncorrected pCi/GRAM	Decay Corr pCi/GRAM	Decay Corr 2-Sigma Error	2-Sigma %Error	Flags
K-40	1.28E+09Y	1.00	2.177E+01	2.177E+01	0.187E+01	8.60	
MN-54	312.70D	1.07	9.869E-03	1.060E-02	2.828E-02	266.87	
CO-58	70.80D	1.37	1.033E-02	1.413E-02	2.730E-02	193.19	
NB-95	35.06D	1.88	3.143E-02	5.919E-02	7.787E-02	131.57	
CD-109	464.00D	1.05	3.523E+00	3.696E+00	0.928E+00	25.10	
SN-126	1.00E+05Y	1.00	3.609E-01	3.609E-01	0.906E-01	25.10	
CS-135	2.30E+06Y	1.00	3.635E-01	3.635E-01	1.564E-01	43.02	
BA-137M	30.17Y	1.00	5.103E-03	5.113E-03	25.33E-03	495.31	
CS-137	30.17Y	1.00	5.394E-03	5.405E-03	26.77E-03	495.31	
CE-141	32.50D	1.98	4.335E-02	8.581E-02	9.222E-02	107.47	
GD-153	241.60D	1.10	8.432E-02	9.244E-02	6.818E-02	73.76	
EU-155	4.96Y	1.01	1.165E-01	1.179E-01	1.057E-01	89.64	
TL-208	1.91Y	1.03	4.893E-01	5.051E-01	0.685E-01	13.57	
BI-211	7.04E+08Y	1.00	3.577E+00	3.577E+00	0.422E+00	11.79	
BI-212	1.91Y	1.03	8.231E-01	8.497E-01	3.625E-01	42.66	
PB-212	1.91Y	1.03	1.437E+00	1.483E+00	0.163E+00	10.98	
BI-214	1600.00Y	1.00	1.089E+00	1.089E+00	0.155E+00	14.22	
PB-214	1600.00Y	1.00	1.244E+00	1.244E+00	0.160E+00	12.89	
RA-226	1600.00Y	1.00	1.089E+00	1.089E+00	0.155E+00	14.22	
AC-228	5.75Y	1.01	1.365E+00	1.380E+00	0.267E+00	19.38	
RA-228	5.75Y	1.01	1.365E+00	1.380E+00	0.267E+00	19.38	
TH-228	1.91Y	1.03	1.437E+00	1.483E+00	0.163E+00	10.98	
TH-229	7340.00Y	1.00	4.927E-01	4.927E-01	1.237E-01	25.10	K
TH-230	7.70E+04Y	1.00	1.089E+00	1.089E+00	0.155E+00	14.22	
TH-232	1.41E+10Y	1.00	1.437E+00	1.437E+00	0.158E+00	10.98	
PA-234M	4.47E+09Y	1.00	1.089E+00	1.089E+00	4.439E+00	407.59	
TH-234	4.47E+09Y	1.00	2.328E+00	2.328E+00	2.398E+00	103.01	
U-234	2.45E+05Y	1.00	1.443E+00	1.443E+00	0.221E+00	15.32	
U-235	7.04E+08Y	1.00	1.998E-01	1.998E-01	2.169E-01	108.53	
NP-237	2.14E+06Y	1.00	1.060E+00	1.060E+00	0.344E+00	32.49	
U-238	4.47E+09Y	1.00	2.328E+00	2.328E+00	2.398E+00	103.01	
AM-242	152.00Y	1.00	2.387E+00	2.388E+00	2.140E+00	89.63	
ANH-511	1.00E+09Y	1.00	8.803E-02	8.803E-02	4.754E-02	54.01	
Total Activity :			5.418E+01	5.460E+01			

Nuclide Type : NATURAL

Nuclide	Hlife	Decay	Uncorrected pCi/GRAM	Decay Corr pCi/GRAM	Decay Corr 2-Sigma Error	2-Sigma %Error	Flags
RA-224	1.91Y	1.03	4.921E+00	5.080E+00	1.010E+00	19.88	
Total Activity :			4.921E+00	5.080E+00			

Grand Total Activity : 5.910E+01 5.968E+01

Flags: "K" = Keyline not found "M" = Manually accepted
 "E" = Manually edited "A" = Nuclide specific abn. limit

It	Energy	Area	Bkgnd	FWHM	Channel	Left	Pw	Cts/Sec	%Err	%Eff	Flags
3	72.72	108	484	1.31	143.96	141	23	7.52E-03	69.5	3.05E+00	T
0	128.40	56	552	1.06	255.23	252	8	3.89E-03	****	6.08E+00	
0	327.05	107	465	1.56	652.27	648	15	7.45E-03	89.2	3.66E+00	T
0	409.29	44	207	0.63	816.66	813	10	3.07E-03	****	3.14E+00	
0	562.45	48	112	0.84	1122.88	1119	9	3.36E-03	83.4	2.50E+00	T
0	640.44	11	88	1.56	1278.82	1277	9	7.57E-04	****	2.26E+00	
0	656.77	19	80	1.24	1311.47	1309	8	1.32E-03	****	2.22E+00	T
0	664.78	33	56	1.10	1327.48	1325	7	2.29E-03	82.9	2.20E+00	T
0	741.55	17	57	1.44	1481.01	1478	7	1.15E-03	****	2.00E+00	T
0	772.05	18	71	1.49	1542.02	1540	8	1.25E-03	****	1.93E+00	T
0	784.12	27	80	2.29	1566.15	1563	9	1.90E-03	****	1.91E+00	T
0	804.02	29	54	3.39	1605.95	1602	9	2.03E-03	****	1.87E+00	T
0	871.02	32	88	5.76	1739.96	1735	15	2.23E-03	****	1.74E+00	T
0	957.89	34	96	2.50	1913.71	1908	14	2.38E-03	****	1.59E+00	
0	1042.99	41	51	1.58	2083.94	2080	13	2.88E-03	76.3	1.47E+00	
0	1077.39	26	68	3.51	2152.77	2146	12	1.82E-03	****	1.42E+00	
0	1189.34	19	40	1.78	2376.76	2373	8	1.30E-03	****	1.30E+00	T
0	1280.59	26	45	3.21	2559.35	2556	12	1.81E-03	****	1.22E+00	
0	1354.39	15	21	1.39	2707.03	2703	9	1.06E-03	****	1.16E+00	
0	1361.09	39	19	3.83	2720.43	2713	15	2.74E-03	57.4	1.15E+00	
0	1384.93	42	23	4.03	2768.16	2762	15	2.90E-03	58.5	1.14E+00	T
1	1406.55	35	19	2.28	2811.41	2804	45	2.41E-03	76.0	1.12E+00	
1	1408.34	17	18	2.07	2815.00	2804	45	1.21E-03	****	1.12E+00	
0	1452.24	16	10	1.13	2902.87	2900	7	1.13E-03	81.9	1.10E+00	
1	1587.41	74	23	2.37	3173.43	3166	24	5.12E-03	33.6	1.03E+00	
1	1590.20	35	17	2.16	3179.00	3166	24	2.46E-03	70.0	1.03E+00	
0	1619.47	13	15	1.97	3237.60	3233	10	9.20E-04	****	1.02E+00	
0	1636.97	28	18	0.60	3272.63	3266	15	1.93E-03	77.8	1.02E+00	
0	1721.26	12	5	1.91	3441.38	3437	10	8.33E-04	90.5	9.91E-01	
1	1744.12	12	7	2.44	3487.14	3483	27	8.32E-04	95.9	9.86E-01	
1	1748.54	12	5	2.22	3496.00	3483	27	8.59E-04	****	9.85E-01	
0	1762.61	151	17	2.80	3524.17	3514	22	1.05E-02	22.4	9.82E-01	
0	1801.11	16	0	0.88	3601.25	3596	12	1.11E-03	50.0	9.75E-01	
0	1811.71	11	18	0.66	3622.48	3614	12	7.50E-04	****	9.73E-01	T
0	1846.37	19	22	3.08	3691.88	3680	17	1.31E-03	****	9.68E-01	
0	1985.05	6	16	4.93	3969.59	3952	21	4.14E-04	****	9.61E-01	
0	1996.44	11	3	3.28	3992.40	3987	13	7.34E-04	93.8	9.61E-01	
6	2025.70	21	12	2.34	4051.00	4040	41	1.44E-03	72.8	9.62E-01	
6	2036.50	16	10	4.15	4072.63	4040	41	1.10E-03	****	9.62E-01	

Flags: "T" = Tentatively associated

```

*****
*                                     GENERAL ENG. LABS, LLC.                               *
*                                     2040 Savage Road                                   *
*                                     Charleston, SC 29414                             *
*****
*                                     DETECTOR DATA                                   *
* Configuration      : DKA300:[CANBERRA.GAMMA.ARCHIVE.GAMMA]G158269004.CNF;1          *
* Acquisition date   : 11-APR-2006 10:22:44  Detector SN#      : 1922864             *
* Detector ID       : GAMMA16                      Sensitivity   : 3.00000             *
* Geometry          : CAN                          Energy tolerance: 2.00000             *
* Elapsed live time : 0 04:00:00.00                Abundance limit  : 75.00000             *
* Elapsed real time : 0 04:00:02.11                Half life ratio  : 8.00000             *
*****
*                                     SAMPLE DATA                                   *
* Sample date       : 10-MAR-2006 12:00:00  Nuclide Library   : EPI                   *
* Sample ID        : G158269004              Analyst initials  : MJH1                   *
* Batch Number     : 513802                  Sample Quantity  : 1.24660E+02 GRAM          *
*****
*                                     QC DATA                                       *
* CALIB. DATE/TIME : 5-APR-2006 19:34:04.74MS Isotope       :                   *
* MSD DPM          :                          MSD Isotope     :                   *
* LCS DPM          :                          LCS Isotope     :                   *
*****

```

Combined Activity-MDA Report

---- Identified Nuclides ----

Nuclide	Activity (pCi/GRAM)	Act error	MDA (pCi/GRAM)	MDA error	Act/MDA
K-40	2.177E+01	1.871E+00	4.286E-01	2.829E-02	50.782
MN-54	1.060E-02	2.828E-02	4.809E-02	4.064E-03	0.220
CO-58	1.413E-02	2.730E-02	5.013E-02	4.073E-03	0.282
CD-109	3.696E+00	9.276E-01	8.428E-01	8.923E-02	4.386
SN-126	3.609E-01	9.058E-02	8.296E-02	8.766E-03	4.350
CS-135	3.635E-01	1.564E-01	1.650E-01	1.576E-02	2.203
BA-137M	5.113E-03	2.533E-02	3.078E-02	1.890E-03	0.166
CS-137	5.405E-03	2.677E-02	3.253E-02	2.006E-03	0.166
CE-141	6.738E-02	7.458E-02	9.209E-02	7.413E-03	0.732
GD-153	9.244E-02	6.818E-02	9.154E-02	8.354E-03	1.010
EU-155	1.132E-01	1.020E-01	1.195E-01	1.020E-02	0.948
TL-208	5.051E-01	6.852E-02	3.958E-02	2.771E-03	12.761
BI-211	3.577E+00	4.216E-01	2.268E-01	1.664E-02	15.775
BI-212	8.497E-01	3.625E-01	3.108E-01	2.680E-02	2.734
PB-212	1.483E+00	1.628E-01	6.504E-02	6.155E-03	22.807
BI-214	1.089E+00	1.549E-01	7.225E-02	5.820E-03	15.074
PB-214	1.244E+00	1.604E-01	7.710E-02	6.931E-03	16.140
RA-224	5.080E+00	1.010E+00	7.213E-01	6.003E-02	7.043

---- Identified Nuclides ----

Nuclide	Activity (pCi/GRAM)	Act error	MDA (pCi/GRAM)	MDA error	Act/MDA
RA-226	1.089E+00	1.549E-01	7.225E-02	5.820E-03	15.074
AC-228	1.380E+00	2.674E-01	1.488E-01	1.756E-02	9.271
RA-228	1.380E+00	2.674E-01	1.488E-01	1.756E-02	9.271
TH-228	1.483E+00	1.628E-01	6.503E-02	6.154E-03	22.809
TH-229	-2.208E-01	3.338E-01	5.478E-01	4.581E-02	-0.403
TH-230	1.089E+00	1.549E-01	7.225E-02	5.820E-03	15.074
TH-232	1.437E+00	1.577E-01	6.299E-02	5.961E-03	22.810
PA-234M	1.089E+00	4.439E+00	4.594E+00	4.609E-01	0.237
TH-234	2.328E+00	2.398E+00	2.056E+00	4.092E-01	1.132
U-234	1.443E+00	2.211E-01	1.479E-01	1.481E-02	9.758
U-235	1.998E-01	2.169E-01	2.457E-01	4.211E-02	0.813
NP-237	1.060E+00	3.443E-01	2.485E-01	5.757E-02	4.264
U-238	2.328E+00	2.398E+00	2.056E+00	4.092E-01	1.132
AM-242	2.294E+00	2.066E+00	2.333E+00	1.994E-01	0.983
ANH-511	8.803E-02	4.754E-02	3.278E-02	1.994E-03	2.685

---- Non-Identified Nuclides ----

Nuclide	Key-Line Activity (pCi/GRAM)	K.L. Ided	Act error	MDA (pCi/GRAM)	MDA error	Act/MDA
BE-7	9.917E-02		2.540E-01	4.538E-01	3.149E-02	0.219
NA-22	-1.468E-02		2.589E-02	4.351E-02	2.827E-03	-0.338
AL-26	1.399E-02		2.023E-02	3.791E-02	2.181E-03	0.369
SC-46	2.460E-04		3.220E-02	5.456E-02	5.055E-03	0.005
V-48	5.071E-02		8.968E-02	1.673E-01	1.482E-02	0.303
CR-51	9.244E-02		3.855E-01	6.452E-01	5.131E-02	0.143
CO-56	2.181E-02		2.915E-02	5.253E-02	4.531E-03	0.415
CO-57	2.654E-03		1.637E-02	2.836E-02	2.197E-03	0.094
FE-59	-2.244E-02		7.595E-02	1.317E-01	1.123E-02	-0.170
CO-60	-1.148E-03		2.693E-02	4.742E-02	2.951E-03	-0.024
ZN-65	-3.007E-02		7.143E-02	1.046E-01	7.923E-03	-0.287
SE-75	-7.799E-03		3.274E-02	5.395E-02	4.429E-03	-0.145
KR-85	5.658E+00		4.823E+00	8.029E+00	4.889E-01	0.705
SR-85	3.463E-02		2.952E-02	4.915E-02	2.993E-03	0.705
Y-88	-2.729E-03		2.340E-02	4.354E-02	2.477E-03	-0.063
Y-91	-2.774E-04		2.795E-02	4.860E-02	2.986E-03	-0.006
NB-94	1.307E-02		2.192E-02	3.896E-02	2.590E-03	0.336
NB-95	5.919E-02		7.787E-02	8.473E-02	6.340E-03	0.699
ZR-95	8.202E-03		5.333E-02	9.250E-02	7.734E-03	0.089
RU-103	-7.517E-03		3.444E-02	5.945E-02	7.589E-03	-0.126
RH-106	-7.925E-03		2.025E-01	3.501E-01	2.158E-02	-0.023
RU-106	-1.806E-02		2.019E-01	3.479E-01	4.148E-02	-0.052
AG-108M	4.723E-03		2.030E-02	3.615E-02	2.308E-03	0.131
AG-110M	1.493E-02	+	2.531E-02	3.935E-02	2.558E-03	0.379
SN-113	3.605E-03		3.307E-02	5.844E-02	3.584E-03	0.062
SN-115	5.717E+00	+	3.695E+00	5.973E+00	5.497E-01	0.957
SN-117M	5.354E-02		8.472E-02	1.470E-01	1.195E-02	0.364
TE-123M	2.373E-02		2.042E-02	3.595E-02	2.946E-03	0.660

---- Non-Identified Nuclides ----

Nuclide	Key-Line Activity (pCi/GRAM)	K.L. Ided	Act error	MDA (pCi/GRAM)	MDA error	Act/MDA
SB-124	-1.544E-02		6.117E-02	1.062E-01	6.910E-03	-0.145
SB-125	-4.650E-03		5.842E-02	1.023E-01	6.261E-03	-0.045
TE-125M	2.903E+00		7.236E+00	1.265E+01	1.271E+00	0.229
I-126	3.131E-01	+	2.602E-01	4.667E-01	2.893E-02	0.671
SB-126	2.653E-02		2.299E-01	3.981E-01	2.737E-02	0.067
I-131	-7.754E-02		3.107E-01	5.432E-01	3.971E-02	-0.143
BA-133	-1.176E-02		3.031E-02	4.616E-02	5.550E-03	-0.255
CS-134	7.968E-02	+	5.169E-02	5.736E-02	4.558E-03	1.389
CS-136	-1.180E-01		1.906E-01	2.744E-01	2.387E-02	-0.430
CE-139	-1.319E-02		2.125E-02	3.522E-02	2.922E-03	-0.374
BA-140	1.189E-01		4.065E-01	7.177E-01	2.338E-01	0.166
LA-140	-5.149E-03		1.450E-01	2.236E-01	1.382E-02	-0.023
CE-144	1.536E-02		1.396E-01	2.399E-01	3.621E-02	0.064
PM-144	-2.282E-03		2.199E-02	3.755E-02	2.473E-03	-0.061
PM-146	2.065E-02		2.813E-02	5.107E-02	4.457E-03	0.404
ND-147	3.062E-01		1.051E+00	1.859E+00	2.541E-01	0.165
PM-147	-1.432E+04		3.302E+04	5.598E+04	4.341E+03	-0.256
EU-152	-1.264E-02		6.282E-02	1.025E-01	7.761E-03	-0.123
EU-154	-3.997E-02		7.183E-02	1.207E-01	1.181E-02	-0.331
TB-160	7.529E-02		1.066E-01	1.915E-01	1.745E-02	0.393
TM-171	5.812E+00		2.678E+01	4.278E+01	4.888E+00	0.136
HF-181	-9.127E-03		3.510E-02	6.055E-02	3.649E-03	-0.151
TA-182	3.498E-02		1.442E-01	2.563E-01	1.713E-02	0.136
IR-192	-3.568E-02		2.760E-02	4.226E-02	3.175E-03	-0.844
HG-203	3.068E-02		4.042E-02	6.231E-02	5.164E-03	0.492
BI-207	9.247E-03		3.514E-02	6.348E-02	5.166E-03	0.146
BI-210	-3.632E+00		8.927E+00	1.292E+01	1.320E+00	-0.281
PB-210	-3.632E+00		8.927E+00	1.292E+01	1.320E+00	-0.281
PB-211	-5.513E-01		6.828E-01	9.902E-01	6.173E-01	-0.557
RN-219	3.749E-02		2.612E-01	4.629E-01	6.294E-02	0.081
RA-223	1.337E-01		4.703E-01	7.055E-01	1.208E-01	0.189
AC-227	1.286E-01		2.655E-01	4.510E-01	6.895E-02	0.285
TH-227	1.264E-01		2.612E-01	4.433E-01	7.927E-02	0.285
PA-231	3.855E-01		1.046E+00	1.765E+00	2.617E-01	0.218
TH-231	4.277E-01	+	1.837E-01	2.485E-01	2.298E-02	1.721
PA-233	-3.701E-03		4.314E-02	7.113E-02	5.580E-03	-0.052
PA-234	-9.575E-02		1.999E-01	3.439E-01	6.533E-02	-0.278
NP-239	-7.346E-02		1.182E-01	1.993E-01	1.569E-02	-0.369
AM-241	-1.220E-01		1.739E-01	2.675E-01	3.623E-02	-0.456
CM-247	-1.469E-02		2.343E-02	3.995E-02	2.311E-03	-0.368
CF-249	1.186E-02		2.676E-02	4.800E-02	2.807E-03	0.247
CF-251	-2.651E-02		8.458E-02	1.415E-01	1.177E-02	-0.187

```

*****
*
*                               General Engineering Labs, LLC
*                               2040 SAVAGE ROAD
*                               CHARLESTON ,SC 29417
*                               GROSS GAMMA REPORT
*
*****
*
*   BATCH ID      : 513802                SAMPLE ID   : G158269004
*   ANALYST       : MJH1                  DETECTOR    : GAMMA16
*   SAMPLE DATE   : 10-MAR-2006 12:00:00.00  COUNT TIME  : 0 04:00:00.00
*   ANALYSIS DATE: 11-APR-2006 10:22:44.70  SAMPLE ALQT: 124.660 GRAM
*
*****

```

```

GROSS GAMMA ACTIVITY (pCi/GRAM ) : 9.034E+00
GROSS GAMMA ERROR (pCi/GRAM ) : 2.000E+00
GROSS GAMMA MDA (pCi/GRAM ) : 6.424E+00
GROSS GAMMA DLC (pCi/GRAM ) : 3.121E+00

```


VAX/VMS Nuclide Identification Report Generated 12-APR-2006 03:19:30.80

```

*****
*                               GENERAL ENG. LABS, LLC.                               *
*                               2040 Savage Road                                       *
*                               Charleston, SC 29414                                   *
*****
Configuration   : DKA300:[CANBERRA.GAMMA.ARCHIVE.GAMMA]G1201055607.CNF;1
Sample date     : 21-MAR-2006 00:00:00 Acquisition date : 11-APR-2006 23:19:02
Sample ID      : G1201055607 Sample quantity   : 1.59640E+02 GRAM
Detector name   : GAMMA13 Detector geometry: CAN
Elapsed live time: 0 04:00:00.00 Elapsed real time: 0 04:00:01.66 0.0%
Energy tolerance: 2.00000 KEV Analyst Initials : MJH1
Abundance limit : 75.00000 Sensitivity      : 3.00000
Batch ID       : 513802 Detector SN#      : 37-TN11260A
Matrix Spike DPM : LCS DPM                    :
*****

```

Pk	It	Energy	Area	Bkgnd	FWHM	Channel	Left	Pw	Cts/Sec	%Err	Fit
1	0	113.22*	32	336	1.54	228.82	224	9	2.22E-03	121.6	
2	0	198.19*	8	184	1.18	398.74	397	6	5.66E-04	316.3	
3	0	294.30*	12	172	1.52	590.95	588	8	8.63E-04	234.2	
4	0	352.77*	35	312	4.95	707.86	701	16	2.43E-03	120.2	
5	0	582.97*	2	109	0.66	1168.15	1165	10	1.26E-04	*****	
6	0	608.76*	27	150	4.69	1219.70	1215	15	1.91E-03	108.5	
7	0	643.25*	15	62	1.63	1288.66	1285	7	1.02E-03	103.6	
8	0	703.07	54	84	3.04	1408.24	1404	11	3.77E-03	35.2	
9	0	765.28*	46	77	3.17	1532.62	1526	14	3.18E-03	48.8	
10	0	818.63*	23	35	3.44	1639.26	1635	9	1.58E-03	67.8	
11	0	874.03	17	54	0.61	1749.99	1744	9	1.21E-03	79.4	
12	0	933.36	38	27	1.92	1868.59	1865	8	2.61E-03	29.3	
13	0	937.50*	1	41	1.48	1876.86	1872	8	5.09E-05	*****	
14	0	965.10*	69	95	10.23	1932.04	1918	27	4.76E-03	45.3	
15	0	999.49*	2	72	1.17	2000.76	1994	12	1.27E-04	*****	
16	0	1127.73	39	50	4.18	2257.06	2249	18	2.72E-03	45.0	
17	0	1135.11	20	49	1.36	2271.81	2267	12	1.41E-03	71.8	
18	0	1282.85	47	54	10.78	2567.05	2555	25	3.24E-03	45.6	
19	0	1334.94	84	22	8.49	2671.14	2660	28	5.83E-03	18.9	
20	0	1383.32	14	6	1.44	2767.82	2765	8	9.44E-04	41.6	
21	0	1467.01	11	17	0.80	2935.02	2931	10	7.59E-04	77.5	
22	0	1580.26	30	16	3.25	3161.30	3153	16	2.08E-03	35.0	
23	0	1602.84	14	20	1.56	3206.40	3198	16	9.89E-04	75.0	
24	0	1647.67	38	80	26.70	3295.96	3259	64	2.65E-03	98.1	
25	0	1898.96*	5	9	3.54	3797.94	3786	18	3.29E-04	172.8	

Flag: "*" = Peak area was modified by background subtraction

VAX/VMS Nuclide Identification Report Generated

```

*****
*                               General Eng. Labs, LLC.                               *
*                               2040 Savage Road                                       *
*                               Charleston, SC 29414                                   *
*****
*                               DETECTOR DATA                                       *
*
* Configuration      : DKA300:[CANBERRA.GAMMA.ARCHIVE.GAMMA]G1201055607
* Acquisition date   : 11-APR-2006 23:19:02 Detector SN#      : 37-TN11260
* Detector ID       : GAMMA13                      Sensitivity    : 3.000
* Geometry          : CAN                          Energy tolerance: 2.000
* Elapsed live time : 0 04:00:00.00              Abundance limit : 75.000
* Elapsed real time : 0 04:00:01.66              Half life ratio  : 8.000
*****
*                               SAMPLE DATA                                         *
*
* Sample date       : 21-MAR-2006 00:00:00 Nuclide Library  : FERMC
* Sample ID        : G1201055607                 Analyst initials: MJH1
* Batch Number     : 513802                       Sample Quantity : 1.5964E+02 GRAM
* Recovery         : 1.00000                      Carrier Weight  : 0.00000
*****
*                               QC DATA                                             *
*
* Standard Weight  : 0.00000
* CALIB. DATE/TIME : 20-JUN-2005 11:56:42 MS Isotope      : TOPLOADER
* MSD DPM          : 5.440                        MSD Isotope     : TOPLOADER
* LCS DPM          : 0.000                        LCS Isotope     : TOPLOADER
* LCSD DPM        : 0.000                        LCSD Isotope   : TOPLOADER
*****

```

Combined Activity-MDA Report

---- Identified Nuclides ----

Nuclide	Activity (pCi/GRAM)	Act error	MDA (pCi/GRAM)	
NB-95	4.909E-02	4.795E-02	4.642E-02	0.000E+00
BI-211	9.822E-02	2.361E-01	1.907E-01	0.000E+00
RA-226	3.374E-02	7.324E-02	6.634E-02	0.000E+00
TH-230	3.374E-02	7.324E-02	6.633E-02	0.000E+00
PA-234M	1.870E-01	4.104E+00	3.771E+00	0.000E+00
U-234	2.045E-02	9.579E-02	1.004E-01	0.000E+00

---- Non-Identified Nuclides ----

Nuclide	Key-Line Activity (pCi/GRAM)	K.L. Act error) Ided	MDA (pCi/GRAM)	
BE-7	-3.952E-02	1.799E-01	3.155E-01	0.000E+00 NOT IDENT.
NA-22	4.183E-03	2.520E-02	4.034E-02	0.000E+00 NOT IDENT.
NA-24	0.000E+00	7.783E+08	0.000E+00	0.000E+00 SHORT HLIF
AL-26	1.591E-02	1.653E-02	3.476E-02	0.000E+00 NOT IDENT.
K-40	4.848E-02	1.898E-01	3.542E-01	0.000E+00 NOT IDENT.
SC-46	5.289E-03	2.247E-02	4.099E-02	0.000E+00 NOT IDENT.
V-48	3.080E-02	5.213E-02	9.698E-02	0.000E+00 NOT IDENT.
CR-51	-3.677E-02	2.213E-01	4.010E-01	0.000E+00 NOT IDENT.
MN-54	1.550E-02	2.056E-02	3.879E-02	0.000E+00 NOT IDENT.
CO-56	1.003E-02	2.305E-02	4.267E-02	0.000E+00 NOT IDENT.
MN-56	0.000E+00	2.000E+41	0.000E+00	0.000E+00 SHORT HLIF
CO-57	-2.823E-04	1.021E-02	1.862E-02	0.000E+00 NOT IDENT.
CO-58	7.486E-03	2.212E-02	4.096E-02	0.000E+00 NOT IDENT.
FE-59	1.833E-02	4.863E-02	8.909E-02	0.000E+00 NOT IDENT.
CO-60	3.411E-02	2.174E-02	4.179E-02	0.000E+00 NOT IDENT.
ZN-65	-3.833E-02	5.179E-02	8.462E-02	0.000E+00 NOT IDENT.
SE-75	1.527E-02	2.106E-02	4.035E-02	0.000E+00 FAIL ABUN
KR-85	-2.064E+01	5.181E+00	7.134E+00	0.000E+00 NOT IDENT.
SR-85	-1.138E-01	2.856E-02	3.933E-02	0.000E+00 NOT IDENT.
Y-88	-5.980E-03	1.830E-02	3.204E-02	0.000E+00 NOT IDENT.
Y-91	-1.052E-02	2.249E-02	3.810E-02	0.000E+00 NOT IDENT.

NB-94	3.486E-02	2.456E-02	3.617E-02	0.000E+00	FAIL ABUN
NB-95M	-6.537E+00	3.197E+00	5.443E+00	0.000E+00	NOT IDENT.
ZR-95	-3.811E-03	3.943E-02	7.104E-02	0.000E+00	NOT IDENT.
MO-99	-1.077E+00	3.016E+00	5.352E+00	0.000E+00	NOT IDENT.
TC-99M	0.000E+00	3.487E+24	0.000E+00	0.000E+00	SHORT HLIF
RU-103	6.648E-03	2.441E-02	4.403E-02	0.000E+00	FAIL ABUN
RH-106	-1.106E-01	1.702E-01	2.999E-01	0.000E+00	NOT IDENT.
RU-106	-1.758E-01	1.735E-01	2.979E-01	0.000E+00	NOT IDENT.
AG-108M	-7.572E-03	1.712E-02	2.979E-02	0.000E+00	NOT IDENT.
CD-109	-2.750E-01	2.615E-01	4.117E-01	0.000E+00	NOT IDENT.
AG-110M	-1.014E-03	1.797E-02	3.284E-02	0.000E+00	FAIL ABUN
SN-113	2.691E-03	2.349E-02	4.263E-02	0.000E+00	NOT IDENT.
CD-115	0.000E+00	5.109E+01	0.000E+00	0.000E+00	SHORT HLIF
SN-115	3.248E+00	1.904E+00	3.810E+00	0.000E+00	FAIL ABUN
SN-117M	3.545E-02	3.370E-02	6.325E-02	0.000E+00	NOT IDENT.
TE-123M	6.797E-03	1.295E-02	2.372E-02	0.000E+00	NOT IDENT.
SB-124	-6.315E-02	4.794E-02	7.007E-02	0.000E+00	NOT IDENT.
SB-125	-2.028E-03	4.858E-02	8.674E-02	0.000E+00	NOT IDENT.
TE-125M	-1.838E-01	5.600E+00	7.229E+00	0.000E+00	NOT IDENT.
I-126	-6.753E-02	1.369E-01	2.421E-01	0.000E+00	NOT IDENT.
SB-126	1.152E-01	1.106E-01	2.149E-01	0.000E+00	NOT IDENT.
SN-126	-1.842E-02	2.572E-02	4.126E-02	0.000E+00	NOT IDENT.
SB-127	-1.022E+00	2.501E+00	4.439E+00	0.000E+00	NOT IDENT.
I-131	4.343E-02	1.062E-01	1.967E-01	0.000E+00	NOT IDENT.
I-132	0.000E+00	1.618E+41	0.000E+00	0.000E+00	SHORT HLIF
TE-132	-5.012E-01	1.262E+00	2.324E+00	0.000E+00	NOT IDENT.
BA-133	1.929E-02	2.372E-02	4.016E-02	0.000E+00	NOT IDENT.
I-133	0.000E+00	8.239E+05	0.000E+00	0.000E+00	SHORT HLIF
CS-134	1.491E-02	2.321E-02	4.351E-02	0.000E+00	NOT IDENT.
CS-135	-2.658E-02	6.948E-02	1.264E-01	0.000E+00	NOT IDENT.
I-135	0.000E+00	9.176E+22	0.000E+00	0.000E+00	SHORT HLIF
CS-136	3.548E-03	8.191E-02	1.453E-01	0.000E+00	FAIL ABUN
BA-137M	5.064E-03	1.860E-02	3.461E-02	0.000E+00	NOT IDENT.
CS-137	5.401E-03	1.966E-02	3.660E-02	0.000E+00	NOT IDENT.
CE-139	2.792E-03	1.326E-02	2.390E-02	0.000E+00	NOT IDENT.
BA-140	-2.343E-02	2.120E-01	3.697E-01	0.000E+00	NOT IDENT.
LA-140	-4.377E-02	7.419E-02	1.026E-01	0.000E+00	NOT IDENT.
CE-141	-2.600E-03	3.163E-02	5.669E-02	0.000E+00	NOT IDENT.
CE-143	0.000E+00	2.949E+03	0.000E+00	0.000E+00	SHORT HLIF
CE-144	9.216E-03	8.697E-02	1.584E-01	0.000E+00	NOT IDENT.
PM-144	1.046E-02	1.906E-02	3.579E-02	0.000E+00	NOT IDENT.
PR-144	0.000E+00	1.823E+41	0.000E+00	0.000E+00	SHORT HLIF
PM-146	-2.202E-02	2.334E-02	3.909E-02	0.000E+00	NOT IDENT.
ND-147	4.117E-01	4.819E-01	8.955E-01	0.000E+00	NOT IDENT.
PM-147	-9.748E+03	2.060E+04	3.685E+04	0.000E+00	NOT IDENT.
PM-149	0.000E+00	3.723E+02	0.000E+00	0.000E+00	SHORT HLIF
EU-152	1.112E-02	4.881E-02	8.977E-02	0.000E+00	FAIL ABUN
GD-153	1.955E-02	2.989E-02	5.137E-02	0.000E+00	NOT IDENT.
EU-154	1.140E-02	7.012E-02	1.122E-01	0.000E+00	FAIL ABUN
EU-155	-4.995E-04	4.366E-02	7.193E-02	0.000E+00	NOT IDENT.
TB-160	4.243E-02	7.499E-02	1.415E-01	0.000E+00	FAIL ABUN
TM-171	1.414E+00	5.720E+00	9.861E+00	0.000E+00	NOT IDENT.
HF-181	-6.123E-03	2.447E-02	4.277E-02	0.000E+00	NOT IDENT.
TA-182	-7.710E-02	7.996E-02	1.332E-01	0.000E+00	NOT IDENT.
IR-192	3.086E-03	1.852E-02	3.414E-02	0.000E+00	FAIL ABUN
HG-203	-3.884E-03	2.071E-02	3.791E-02	0.000E+00	NOT IDENT.
BI-207	2.415E-03	2.709E-02	4.823E-02	0.000E+00	NOT IDENT.
TL-208	1.211E-03	3.128E-02	4.117E-02	0.000E+00	FAIL ABUN
BI-210	0.000E+00	2.761E-01	5.586E-01	0.000E+00	NOT IDENT.
PB-210	0.000E+00	2.761E-01	5.586E-01	0.000E+00	NOT IDENT.
PB-211	2.109E-01	4.645E-01	8.575E-01	0.000E+00	NOT IDENT.
BI-212	5.737E-02	1.515E-01	2.821E-01	0.000E+00	NOT IDENT.
PB-212	0.000E+00	2.778E-02	5.577E-02	0.000E+00	FAIL ABUN
BI-214	3.374E-02	7.324E-02	7.466E-02	0.000E+00	FAIL ABUN
PB-214	3.417E-02	8.212E-02	7.031E-02	0.000E+00	FAIL ABUN
RN-219	-4.492E-02	2.004E-01	3.563E-01	0.000E+00	NOT IDENT.
RA-223	4.352E-02	3.246E-01	5.965E-01	0.000E+00	NOT IDENT.
RA-224	-5.810E-01	3.129E-01	5.372E-01	0.000E+00	NOT IDENT.
AC-227	1.377E-01	1.777E-01	3.417E-01	0.000E+00	NOT IDENT.
TH-227	1.355E-01	1.748E-01	3.362E-01	0.000E+00	NOT IDENT.
AC-228	5.687E-03	7.768E-02	1.386E-01	0.000E+00	FAIL ABUN
RA-228	5.687E-03	7.768E-02	1.386E-01	0.000E+00	FAIL ABUN
TH-228	0.000E+00	2.775E-02	5.569E-02	0.000E+00	NOT IDENT.
TH-229	-8.712E-02	2.358E-01	4.078E-01	0.000E+00	NOT IDENT.
PA-231	-4.463E-01	7.170E-01	1.283E+00	0.000E+00	NOT IDENT.
TH-231	1.242E-02	7.922E-02	1.481E-01	0.000E+00	FAIL ABUN
TH-232	0.000E+00	2.714E-02	5.446E-02	0.000E+00	FAIL ABUN
PA-233	1.183E-02	3.076E-02	5.750E-02	0.000E+00	NOT IDENT.

PA-234	-8.174E-02	1.735E-01	2.962E-01	0.000E+00	FAIL	ABUN
TH-234	0.000E+00	3.258E-01	7.071E-01	0.000E+00	FAIL	ABUN
U-235	1.086E-01	9.222E-02	1.741E-01	0.000E+00	NOT	IDENT.
NP-237	2.595E-02	7.304E-02	1.242E-01	0.000E+00	NOT	IDENT.
U-238	0.000E+00	3.258E-01	7.071E-01	0.000E+00	NOT	IDENT.
NP-239	4.407E-02	8.418E-02	1.417E-01	0.000E+00	NOT	IDENT.
AM-241	-1.661E-02	2.585E-02	4.286E-02	0.000E+00	NOT	IDENT.
AM-242	-4.898E-01	8.837E-01	1.411E+00	0.000E+00	NOT	IDENT.
CM-247	9.358E-04	1.849E-02	3.337E-02	0.000E+00	NOT	IDENT.
CF-249	-8.714E-03	1.960E-02	3.447E-02	0.000E+00	NOT	IDENT.
CF-251	-8.250E-03	5.452E-02	9.624E-02	0.000E+00	NOT	IDENT.
ANH-511	0.000E+00	2.329E-02	4.977E-02	0.000E+00	NOT	IDENT.

```

*****
*                               GENERAL ENG. LABS, LLC.                               *
*                               2040 Savage Road                                       *
*                               Charleston, SC 29414                                   *
*****
Configuration      : DKA300:[CANBERRA.GAMMA.ARCHIVE.GAMMA]G1201055607.CNF;1
Sample date        : 21-MAR-2006 00:00:00 Acquisition date : 11-APR-2006 23:19:02
Sample ID          : G1201055607 Sample quantity      : 1.59640E+02 GRAM
Detector name     : GAMMA13 Detector geometry      : CAN
Elapsed live time : 0 04:00:00.00 Elapsed real time: 0 04:00:01.66 0.0%
Energy tolerance  : 2.00000 KEV Analyst Initials   : MJH1
Abundance limit   : 75.00000 Sensitivity       : 3.00000
Batch ID          : 513802 Detector SN#       : 37-TN11260A
Matrix Spike DPM  : LCS DPM                       :
*****

```

Nuclide Line Activity Report

Nuclide Type:

Nuclide	Energy	Area	%Abn	%Eff	Uncorrected pCi/GRAM	Decay Corr pCi/GRAM	2-Sigma %Error
NB-95	765.79	46	99.81*	1.702E+00	3.174E-02	4.909E-02	97.69
BI-211	351.07	35	12.94*	3.237E+00	9.822E-02	9.822E-02	240.37
RA-226	295.21	12	19.20	3.722E+00	2.045E-02	2.045E-02	468.38
	351.92	35	37.20	3.237E+00	3.416E-02	3.417E-02	240.37
	609.31	27	46.30*	2.066E+00	3.374E-02	3.374E-02	217.07
TH-230	295.21	12	19.20	3.722E+00	2.045E-02	2.045E-02	468.38
	351.92	35	37.20	3.237E+00	3.416E-02	3.416E-02	240.37
	609.31	27	46.30*	2.066E+00	3.374E-02	3.374E-02	217.07
PA-234M	766.40	46	0.21	1.702E+00	1.509E+01	1.509E+01	97.69
	1001.03	2	0.85*	1.359E+00	1.870E-01	1.870E-01	2194.93
U-234	67.67	-----	0.37	7.024E+00	-----	Line Not Found	-----
	241.98	-----	7.49	4.293E+00	-----	Line Not Found	-----
	295.21	12	19.20*	3.722E+00	2.045E-02	2.045E-02	468.38
	351.92	35	37.20	3.237E+00	3.416E-02	3.416E-02	240.37

Flag: "*" = Keyline

Total number of lines in spectrum 25
 Number of unidentified lines 9
 Number of lines tentatively identified by NID 16 64.00%

Nuclide Type :

Nuclide	Hlife	Decay	Uncorrected pCi/GRAM	Decay Corr pCi/GRAM	Decay Corr 2-Sigma Error	2-Sigma %Error	Flags
NB-95	35.06D	1.55	3.174E-02	4.909E-02	4.795E-02	97.69	
BI-211	7.04E+08Y	1.00	9.822E-02	9.822E-02	23.61E-02	240.37	
RA-226	1600.00Y	1.00	3.374E-02	3.374E-02	7.324E-02	217.07	
TH-230	7.70E+04Y	1.00	3.374E-02	3.374E-02	7.324E-02	217.07	
PA-234M	4.47E+09Y	1.00	1.870E-01	1.870E-01	41.04E-01	2194.93	
U-234	2.45E+05Y	1.00	2.045E-02	2.045E-02	9.579E-02	468.38	
Total Activity :			4.048E-01	4.222E-01			

Grand Total Activity : 4.048E-01 4.222E-01

Flags: "K" = Keyline not found "M" = Manually accepted
 "E" = Manually edited "A" = Nuclide specific abn. limit

It	Energy	Area	Bkgnd	FWHM	Channel	Left	Pw	Cts/Sec	%Err	%Eff	Flags
0	113.22	32	336	1.54	228.82	224	9	2.22E-03	****	6.53E+00	T
0	198.19	8	184	1.18	398.74	397	6	5.66E-04	****	4.91E+00	T
0	582.97	2	109	0.66	1168.15	1165	10	1.26E-04	****	2.14E+00	T
0	643.25	15	62	1.63	1288.66	1285	7	1.02E-03	****	1.97E+00	
0	703.07	54	84	3.04	1408.24	1404	11	3.77E-03	70.5	1.83E+00	T
0	818.63	23	35	3.44	1639.26	1635	9	1.58E-03	****	1.61E+00	T
0	874.03	17	54	0.61	1749.99	1744	9	1.21E-03	****	1.52E+00	T
0	933.36	38	27	1.92	1868.59	1865	8	2.61E-03	58.6	1.44E+00	T
0	937.50	1	41	1.48	1876.86	1872	8	5.09E-05	****	1.43E+00	T
0	965.10	69	95	10.23	1932.04	1918	27	4.76E-03	90.5	1.40E+00	T
0	1127.73	39	50	4.18	2257.06	2249	18	2.72E-03	90.0	1.23E+00	
0	1135.11	20	49	1.36	2271.81	2267	12	1.41E-03	****	1.22E+00	T
0	1282.85	47	54	10.78	2567.05	2555	25	3.24E-03	91.2	1.11E+00	
0	1334.94	84	22	8.49	2671.14	2660	28	5.83E-03	37.9	1.08E+00	
0	1383.32	14	6	1.44	2767.82	2765	8	9.44E-04	83.2	1.05E+00	T
0	1467.01	11	17	0.80	2935.02	2931	10	7.59E-04	****	1.00E+00	
0	1580.26	30	16	3.25	3161.30	3153	16	2.08E-03	69.9	9.45E-01	
0	1602.84	14	20	1.56	3206.40	3198	16	9.89E-04	****	9.35E-01	
0	1647.67	38	80	26.70	3295.96	3259	64	2.65E-03	****	9.17E-01	
0	1898.96	5	9	3.54	3797.94	3786	18	3.29E-04	****	8.30E-01	

Flags: "T" = Tentatively associated

```

*****
*                                     GENERAL ENG. LABS, LLC.                               *
*                                     2040 Savage Road                                   *
*                                     Charleston, SC 29414                             *
*****
*                                     DETECTOR DATA                                   *
* Configuration      : DKA300:[CANBERRA.GAMMA.ARCHIVE.GAMMA]G1201055607.CNF;1         *
* Acquisition date   : 11-APR-2006 23:19:02  Detector SN#      : 37-TN11260A         *
* Detector ID       : GAMMA13                Sensitivity       : 3.00000             *
* Geometry         : CAN                     Energy tolerance   : 2.00000             *
* Elapsed live time: 0 04:00:00.00          Abundance limit     : 75.00000             *
* Elapsed real time: 0 04:00:01.66          Half life ratio    : 8.00000             *
*****
*                                     SAMPLE DATA                                   *
* Sample date       : 21-MAR-2006 00:00:00  Nuclide Library   : EPI                   *
* Sample ID        : G1201055607           Analyst initials  : MJH1                   *
* Batch Number     : 513802                Sample Quantity   : 1.59640E+02 GRAM          *
*****
*                                     QC DATA                                       *
* CALIB. DATE/TIME : 20-JUN-2005 11:56:42.9MS Isotope       : TOPLOADER             *
* MSD DPM          :                       MSD Isotope       :                       *
* LCS DPM          :                       LCS Isotope       :                       *
*****

```

Combined Activity-MDA Report

---- Identified Nuclides ----

Nuclide	Activity (pCi/GRAM)	Act error	MDA (pCi/GRAM)	MDA error	Act/MDA
NB-95	4.909E-02	4.795E-02	4.509E-02	0.000E+00	1.089
BI-211	9.822E-02	2.361E-01	1.812E-01	0.000E+00	0.542
RA-226	3.374E-02	7.324E-02	6.402E-02	0.000E+00	0.527
TH-230	3.374E-02	7.324E-02	6.402E-02	0.000E+00	0.527
PA-234M	1.870E-01	4.104E+00	3.692E+00	0.000E+00	0.051
U-234	2.045E-02	9.579E-02	9.491E-02	0.000E+00	0.215

---- Non-Identified Nuclides ----

Nuclide	Key-Line Activity (pCi/GRAM)	K.L. Ided	Act error	MDA (pCi/GRAM)	MDA error	Act/MDA
BE-7	-3.952E-02		1.799E-01	3.024E-01	0.000E+00	-0.131
NA-22	4.183E-03		2.520E-02	3.979E-02	0.000E+00	0.105
AL-26	1.591E-02		1.653E-02	3.465E-02	0.000E+00	0.459
K-40	4.848E-02		1.898E-01	3.507E-01	0.000E+00	0.138
SC-46	5.289E-03		2.247E-02	4.000E-02	0.000E+00	0.132
V-48	3.080E-02		5.213E-02	9.492E-02	0.000E+00	0.324

---- Non-Identified Nuclides ----

Nuclide	Key-Line Activity (pCi/GRAM)	K.L. Ided	Act error	MDA (pCi/GRAM)	MDA error	Act/MDA
CR-51	-3.677E-02		2.213E-01	3.801E-01	0.000E+00	-0.097
MN-54	1.550E-02		2.056E-02	3.778E-02	0.000E+00	0.410
CO-56	1.003E-02		2.305E-02	4.158E-02	0.000E+00	0.241
CO-57	-2.823E-04		1.021E-02	1.720E-02	0.000E+00	-0.016
CO-58	7.486E-03		2.212E-02	3.986E-02	0.000E+00	0.188
FE-59	1.833E-02		4.863E-02	8.748E-02	0.000E+00	0.210
CO-60	3.411E-02		2.174E-02	4.127E-02	0.000E+00	0.827
ZN-65	-3.833E-02		5.179E-02	8.313E-02	0.000E+00	-0.461
SE-75	1.527E-02		2.106E-02	3.804E-02	0.000E+00	0.401
KR-85	-2.064E+01		5.181E+00	6.852E+00	0.000E+00	-3.012
SR-85	-1.138E-01		2.856E-02	3.778E-02	0.000E+00	-3.012
Y-88	-5.980E-03		1.830E-02	3.195E-02	0.000E+00	-0.187
Y-91	-1.052E-02		2.249E-02	3.668E-02	0.000E+00	-0.287
NB-94	3.486E-02	+	2.456E-02	3.505E-02	0.000E+00	0.995
NB-95M	-6.537E+00		3.197E+00	5.116E+00	0.000E+00	-1.278
ZR-95	-3.811E-03		3.943E-02	6.899E-02	0.000E+00	-0.055
MO-99	-1.077E+00		3.016E+00	4.961E+00	0.000E+00	-0.217
RU-103	6.648E-03		2.441E-02	4.225E-02	0.000E+00	0.157
RH-106	-1.106E-01		1.702E-01	2.896E-01	0.000E+00	-0.382
RU-106	-1.758E-01		1.735E-01	2.877E-01	0.000E+00	-0.611
AG-108M	-7.572E-03		1.712E-02	2.847E-02	0.000E+00	-0.266
CD-109	-2.750E-01		2.615E-01	3.770E-01	0.000E+00	-0.729
AG-110M	-1.014E-03		1.797E-02	3.176E-02	0.000E+00	-0.032
SN-113	2.691E-03		2.349E-02	4.063E-02	0.000E+00	0.066
SN-115	3.248E+00	+	1.904E+00	3.723E+00	0.000E+00	0.872
SN-117M	3.545E-02		3.370E-02	5.881E-02	0.000E+00	0.603
TE-123M	6.797E-03		1.295E-02	2.206E-02	0.000E+00	0.308
SB-124	-6.315E-02		4.794E-02	6.969E-02	0.000E+00	-0.906
SB-125	-2.028E-03		4.858E-02	8.288E-02	0.000E+00	-0.024
TE-125M	-1.838E-01		5.600E+00	6.657E+00	0.000E+00	-0.028
I-126	-6.753E-02		1.369E-01	2.343E-01	0.000E+00	-0.288
SB-126	1.152E-01		1.106E-01	2.084E-01	0.000E+00	0.553
SN-126	-1.842E-02		2.572E-02	3.778E-02	0.000E+00	-0.488
SB-127	-1.022E+00		2.501E+00	4.299E+00	0.000E+00	-0.238
I-131	4.343E-02		1.062E-01	1.871E-01	0.000E+00	0.232
TE-132	-5.012E-01		1.262E+00	2.182E+00	0.000E+00	-0.230
BA-133	1.929E-02		2.372E-02	3.818E-02	0.000E+00	0.505
CS-134	1.491E-02		2.321E-02	4.232E-02	0.000E+00	0.352
CS-135	-2.658E-02		6.948E-02	1.192E-01	0.000E+00	-0.223
CS-136	3.548E-03		8.191E-02	1.424E-01	0.000E+00	0.025
BA-137M	5.064E-03		1.860E-02	3.348E-02	0.000E+00	0.151
CS-137	5.401E-03		1.966E-02	3.541E-02	0.000E+00	0.153
CE-139	2.792E-03		1.326E-02	2.226E-02	0.000E+00	0.125
BA-140	-2.343E-02		2.120E-01	3.555E-01	0.000E+00	-0.066
LA-140	-4.377E-02		7.419E-02	1.019E-01	0.000E+00	-0.430
CE-141	-2.600E-03		3.163E-02	5.259E-02	0.000E+00	-0.049
CE-144	9.216E-03		8.697E-02	1.466E-01	0.000E+00	0.063
PM-144	1.046E-02		1.906E-02	3.468E-02	0.000E+00	0.302

---- Non-Identified Nuclides ----

Nuclide	Key-Line Activity (pCi/GRAM)	K.L. Ided	Act error	MDA (pCi/GRAM)	MDA error	Act/MDA
PM-146	-2.202E-02		2.334E-02	3.741E-02	0.000E+00	-0.588
ND-147	4.117E-01		4.819E-01	8.609E-01	0.000E+00	0.478
PM-147	-9.748E+03		2.060E+04	3.403E+04	0.000E+00	-0.286
EU-152	1.112E-02		4.881E-02	8.525E-02	0.000E+00	0.130
GD-153	1.955E-02		2.989E-02	4.717E-02	0.000E+00	0.415
EU-154	1.140E-02		7.012E-02	1.107E-01	0.000E+00	0.103
EU-155	-4.995E-04		4.366E-02	6.617E-02	0.000E+00	-0.008
TB-160	4.243E-02		7.499E-02	1.380E-01	0.000E+00	0.308
TM-171	1.414E+00		5.720E+00	8.966E+00	0.000E+00	0.158
HF-181	-6.123E-03		2.447E-02	4.101E-02	0.000E+00	-0.149
TA-182	-7.710E-02		7.996E-02	1.312E-01	0.000E+00	-0.588
IR-192	3.086E-03		1.852E-02	3.235E-02	0.000E+00	0.095
HG-203	-3.884E-03		2.071E-02	3.580E-02	0.000E+00	-0.108
BI-207	2.415E-03		2.709E-02	4.731E-02	0.000E+00	0.051
TL-208	1.211E-03	+	3.128E-02	3.969E-02	0.000E+00	0.031
BI-210	1.103E+00		2.761E-01	5.033E-01	0.000E+00	2.192
PB-210	1.103E+00		2.761E-01	5.033E-01	0.000E+00	2.192
PB-211	2.109E-01		4.645E-01	8.181E-01	0.000E+00	0.258
BI-212	5.737E-02		1.515E-01	2.737E-01	0.000E+00	0.210
PB-212	5.978E-02		2.778E-02	5.244E-02	0.000E+00	1.140
BI-214	3.374E-02	+	7.324E-02	7.205E-02	0.000E+00	0.468
PB-214	3.417E-02	+	8.212E-02	6.682E-02	0.000E+00	0.511
RN-219	-4.492E-02		2.004E-01	3.398E-01	0.000E+00	-0.132
RA-223	4.352E-02		3.246E-01	5.656E-01	0.000E+00	0.077
RA-224	-5.810E-01		3.129E-01	5.052E-01	0.000E+00	-1.150
AC-227	1.377E-01		1.777E-01	3.219E-01	0.000E+00	0.428
TH-227	1.355E-01		1.748E-01	3.167E-01	0.000E+00	0.428
AC-228	5.687E-03		7.768E-02	1.353E-01	0.000E+00	0.042
RA-228	5.687E-03		7.768E-02	1.353E-01	0.000E+00	0.042
TH-228	5.921E-02		2.775E-02	5.236E-02	0.000E+00	1.131
TH-229	-8.712E-02		2.358E-01	3.813E-01	0.000E+00	-0.228
PA-231	-4.463E-01		7.170E-01	1.212E+00	0.000E+00	-0.368
TH-231	1.242E-02		7.922E-02	1.397E-01	0.000E+00	0.089
TH-232	5.774E-02		2.714E-02	5.120E-02	0.000E+00	1.128
PA-233	1.183E-02		3.076E-02	5.446E-02	0.000E+00	0.217
PA-234	-8.174E-02		1.735E-01	2.896E-01	0.000E+00	-0.282
TH-234	2.816E+00		3.258E-01	6.421E-01	0.000E+00	4.386
U-235	1.086E-01		9.222E-02	1.615E-01	0.000E+00	0.673
NP-237	2.595E-02		7.304E-02	1.136E-01	0.000E+00	0.228
U-238	2.816E+00		3.258E-01	6.421E-01	0.000E+00	4.386
NP-239	4.407E-02		8.418E-02	1.308E-01	0.000E+00	0.337
AM-241	-1.661E-02		2.585E-02	3.886E-02	0.000E+00	-0.427
AM-242	-4.898E-01		8.837E-01	1.298E+00	0.000E+00	-0.377
CM-247	9.358E-04		1.849E-02	3.183E-02	0.000E+00	0.029
CF-249	-8.714E-03		1.960E-02	3.284E-02	0.000E+00	-0.265
CF-251	-8.250E-03		5.452E-02	8.974E-02	0.000E+00	-0.092
ANH-511	1.364E-01		2.329E-02	4.780E-02	0.000E+00	2.854

```

*****
*
*                               General Engineering Labs, LLC
*                               2040 SAVAGE ROAD
*                               CHARLESTON ,SC 29417
*                               GROSS GAMMA REPORT
*
*****
*
*  BATCH ID      : 513802                SAMPLE ID   : G1201055607
*  ANALYST       : MJH1                  DETECTOR    : GAMMA13
*  SAMPLE DATE   : 21-MAR-2006 00:00:00.00  COUNT TIME  : 0 04:00:00.00
*  ANALYSIS DATE: 11-APR-2006 23:19:02.61  SAMPLE ALQT: 159.640 GRAM
*
*****

```

```

GROSS GAMMA ACTIVITY (pCi/GRAM ) : 5.741E-01
GROSS GAMMA ERROR   (pCi/GRAM ) : 7.801E-01
GROSS GAMMA MDA     (pCi/GRAM ) : 1.911E+00
GROSS GAMMA DLC     (pCi/GRAM ) : 9.280E-01

```

VAX/VMS Nuclide Identification Report Generated 12-APR-2006 03:20:09.58

```

*****
*                               GENERAL ENG. LABS, LLC.                               *
*                               2040 Savage Road                                       *
*                               Charleston, SC 29414                                 *
*****
Configuration   : DKA300:[CANBERRA.GAMMA.ARCHIVE.GAMMA]G1201055608.CNF;1
Sample date     : 10-MAR-2006 07:46:00 Acquisition date : 11-APR-2006 23:19:39
Sample ID      : G1201055608 Sample quantity   : 1.59640E+02 GRAM
Detector name   : GAMMA16 Detector geometry: CAN
Elapsed live time: 0 04:00:00.00 Elapsed real time: 0 04:00:02.78 0.0%
Energy tolerance: 2.00000 KEV Analyst Initials : MJH1
Abundance limit : 75.00000 Sensitivity      : 3.00000
Batch ID       : 513802 Detector SN#      : 1922864
Matrix Spike DPM : LCS DPM                  :
*****

```

Pk	It	Energy	Area	Bkgnd	FWHM	Channel	Left	Pw	Cts/Sec	%Err	Fit
1	0	58.85	35	660	1.02	116.24	113	7	2.44E-03	121.9	
2	0	63.22*	91	797	1.33	124.96	121	8	6.30E-03	56.7	
3	3	74.70*	761	823	1.20	147.91	141	19	5.28E-02	7.3	2.20E+00
4	3	77.02*	1096	637	1.05	152.54	141	19	7.61E-02	5.0	
5	3	79.04*	96	584	1.06	156.58	141	19	6.65E-03	50.9	
6	6	84.35*	226	595	1.58	167.19	164	26	1.57E-02	18.7	1.85E+00
7	6	87.23*	594	986	1.60	172.94	164	26	4.12E-02	11.0	
8	6	89.80	314	589	1.05	178.08	164	26	2.18E-02	13.7	
9	6	92.76*	502	975	1.64	183.99	164	26	3.48E-02	13.2	
10	0	99.15	134	736	0.66	196.77	193	8	9.27E-03	36.2	
11	0	105.20*	133	834	1.95	208.86	205	9	9.21E-03	41.1	
12	0	115.07	123	642	1.10	228.59	226	7	8.52E-03	35.4	
13	0	128.81*	178	889	1.04	256.05	252	9	1.24E-02	31.4	
14	0	153.49	104	604	1.14	305.36	302	7	7.19E-03	40.5	
15	0	185.67*	378	1012	1.21	369.68	364	12	2.62E-02	18.1	
16	0	202.08	53	530	1.23	402.48	400	7	3.68E-03	73.4	
17	0	209.08	257	632	1.09	416.47	413	8	1.79E-02	18.0	
18	5	238.48*	3374	418	1.12	475.24	468	18	2.34E-01	2.0	1.24E+00
19	5	241.36*	795	430	1.76	480.99	468	18	5.52E-02	6.6	
20	0	270.00	267	522	1.60	538.24	533	11	1.85E-02	17.7	
21	0	277.23	75	436	1.28	552.68	548	8	5.20E-03	49.6	
22	0	287.36	29	382	0.94	572.92	570	8	2.05E-03	116.0	
23	0	295.03*	733	440	1.12	588.26	584	10	5.09E-02	6.6	
24	0	299.86*	201	383	1.09	597.93	595	8	1.40E-02	18.6	
25	0	312.52	42	253	1.70	623.22	620	7	2.92E-03	64.8	
26	0	328.00	149	350	1.26	654.16	650	9	1.04E-02	24.0	
27	0	338.18*	753	464	1.39	674.52	669	13	5.23E-02	7.1	
28	0	351.62*	1231	454	1.23	701.37	695	13	8.55E-02	4.6	
29	0	409.11*	70	342	1.12	816.30	811	11	4.89E-03	53.6	
30	0	462.64	186	230	1.64	923.32	918	10	1.29E-02	16.9	
31	0	469.18	61	175	1.46	936.39	932	9	4.26E-03	41.1	
32	0	510.38*	296	436	1.85	1018.76	1011	18	2.06E-02	19.4	
33	0	582.76*	1034	213	1.49	1163.48	1158	12	7.18E-02	4.3	
34	0	608.82*	893	276	1.39	1215.60	1209	13	6.20E-02	5.2	
35	0	678.37*	23	89	1.57	1354.67	1352	7	1.60E-03	75.5	
36	0	726.78	240	176	1.49	1451.47	1445	12	1.66E-02	12.8	
37	0	767.50*	120	109	2.50	1532.92	1528	10	8.32E-03	19.8	
38	0	771.97*	91	89	1.70	1541.86	1538	10	6.35E-03	22.4	

Pk	It	Energy	Area	Bkgnd	FWHM	Channel	Left	Pw	Cts/Sec	%Err	Fit
39	0	785.10	94	104	1.36	1568.11	1563	10	6.52E-03	23.0	
40	0	793.83*	149	109	1.49	1585.56	1581	10	1.04E-02	15.8	
41	0	805.73*	31	96	0.93	1609.37	1607	8	2.16E-03	59.3	
42	0	823.79*	24	93	1.48	1645.50	1641	10	1.65E-03	82.8	
43	0	835.06*	58	115	1.62	1668.04	1663	10	3.99E-03	38.1	
44	0	839.29*	48	93	1.80	1676.49	1673	8	3.33E-03	39.4	
45	0	860.17*	153	211	1.58	1718.26	1709	18	1.06E-02	24.6	
46	0	882.30	26	45	1.39	1762.52	1760	6	1.79E-03	46.5	
47	0	910.38*	722	132	1.56	1818.68	1813	13	5.01E-02	5.1	
48	0	932.39*	59	154	1.74	1862.72	1855	15	4.12E-03	48.5	
49	4	963.95*	114	92	1.91	1925.85	1921	20	7.93E-03	18.0	2.02E+00
50	4	968.18*	417	101	1.82	1934.31	1921	20	2.89E-02	6.9	
51	0	1118.99*	224	110	1.53	2236.00	2228	14	1.56E-02	12.3	
52	0	1154.56	29	56	1.37	2307.16	2304	7	1.98E-03	47.3	
53	0	1197.75	9	113	0.93	2393.59	2393	9	5.90E-04	227.6	
54	0	1237.61	83	144	1.65	2473.35	2468	13	5.77E-03	31.9	
55	0	1264.72	20	52	1.40	2527.58	2525	7	1.37E-03	65.7	
56	0	1311.32	26	41	1.87	2620.84	2618	7	1.78E-03	45.7	
57	0	1367.23	21	30	2.05	2732.73	2730	8	1.49E-03	49.1	
58	0	1376.59	63	31	1.54	2751.46	2747	10	4.34E-03	21.2	
59	2	1406.92*	43	24	2.51	2812.16	2807	20	2.96E-03	27.8	1.47E+00
60	2	1411.31	40	22	2.51	2820.94	2807	20	2.80E-03	29.7	
61	0	1419.04	30	15	2.13	2836.42	2833	9	2.06E-03	30.2	
62	0	1459.46*	2692	62	1.93	2917.32	2906	20	1.87E-01	2.1	
63	0	1472.94	30	16	6.30	2944.30	2937	16	2.08E-03	35.0	
64	0	1479.58	22	11	1.65	2957.59	2953	11	1.53E-03	36.1	
65	0	1507.84*	9	30	1.59	3014.15	3010	10	6.36E-04	121.8	
66	0	1577.14*	20	15	4.74	3152.87	3147	12	1.40E-03	48.4	
67	0	1588.33*	72	76	1.71	3175.26	3167	18	4.99E-03	31.6	
68	0	1608.45	9	17	0.96	3215.53	3211	11	5.90E-04	98.7	
69	3	1619.39*	48	16	2.89	3237.43	3232	36	3.32E-03	21.9	1.14E+00
70	3	1629.38*	23	7	2.89	3257.44	3232	36	1.61E-03	49.9	
71	0	1636.32*	16	7	2.26	3271.32	3268	11	1.08E-03	44.9	
72	0	1659.95*	8	14	0.75	3318.64	3316	8	5.88E-04	94.8	
73	6	1678.64	23	4	3.89	3356.04	3346	40	1.62E-03	39.3	8.20E-01
74	6	1690.59	14	10	2.93	3379.98	3346	40	9.73E-04	45.7	
75	0	1728.10	65	11	2.62	3455.07	3450	13	4.50E-03	16.0	
76	0	1749.49	24	11	3.82	3497.90	3491	15	1.69E-03	36.2	
77	0	1763.28*	142	40	2.38	3525.50	3518	18	9.86E-03	14.3	
78	0	1846.54*	26	23	2.44	3692.22	3683	15	1.81E-03	46.0	
79	0	1976.75	10	10	1.50	3952.97	3950	9	7.19E-04	61.3	

Flag: "*" = Peak area was modified by background subtraction

VAX/VMS Nuclide Identification Report Generated

```

*****
*                               General Eng. Labs, LLC.                               *
*                               2040 Savage Road                                       *
*                               Charleston, SC 29414                                   *
*****
*                               DETECTOR DATA                                       *
*
* Configuration      : DKA300:[CANBERRA.GAMMA.ARCHIVE.GAMMA]G1201055608
* Acquisition date   : 11-APR-2006 23:19:39 Detector SN#      : 1922864
* Detector ID        : GAMMA16                      Sensitivity    : 3.000
* Geometry           : CAN                          Energy tolerance: 2.000
* Elapsed live time  : 0 04:00:00.00                Abundance limit : 75.000
* Elapsed real time  : 0 04:00:02.78                Half life ratio  : 8.000
*****
*                               SAMPLE DATA                                         *
*
* Sample date        : 10-MAR-2006 07:46:00 Nuclide Library :
* Sample ID          : G1201055608                    Analyst initials: MJH1
* Batch Number       : 513802                          Sample Quantity : 1.5964E+02 GRAM
* Recovery           : 1.00000                          Carrier Weight   : 0.00000
*****
*                               QC DATA                                             *
*
* Standard Weight    : 0.00000
* CALIB. DATE/TIME   : 5-APR-2006 19:34:04 MS Isotope      :
* MSD DPM             : 0.000                          MSD Isotope      :
* LCS DPM             : 0.000                          LCS Isotope      :
* LCSD DPM            : 0.000                          LCSD Isotope     :
*****

```

Combined Activity-MDA Report

---- Identified Nuclides ----

Nuclide	Activity (pCi/GRAM)	Act error	MDA (pCi/GRAM)	
K-40	2.714E+01	2.114E+00	3.342E-01	0.000E+00
MN-54	4.038E-02	3.097E-02	4.072E-02	0.000E+00
NB-95	1.054E-02	6.228E-02	7.382E-02	0.000E+00
CD-109	4.164E+00	1.014E+00	8.717E-01	0.000E+00
SN-126	4.062E-01	9.887E-02	8.573E-02	0.000E+00
CS-135	4.701E-01	1.721E-01	1.629E-01	0.000E+00
EU-155	1.283E-01	1.067E-01	1.213E-01	0.000E+00
TL-208	6.118E-01	6.749E-02	3.914E-02	0.000E+00
BI-211	3.209E+00	3.797E-01	2.197E-01	0.000E+00
BI-212	1.211E+00	3.278E-01	2.796E-01	0.000E+00
PB-212	2.024E+00	2.085E-01	6.231E-02	0.000E+00
BI-214	9.629E-01	1.263E-01	7.467E-02	0.000E+00
PB-214	1.116E+00	1.444E-01	7.560E-02	0.000E+00
RA-224	5.431E+00	8.500E-01	7.087E-01	0.000E+00
RA-226	9.629E-01	1.263E-01	7.467E-02	0.000E+00
AC-228	1.858E+00	2.904E-01	1.452E-01	0.000E+00
RA-228	1.858E+00	2.904E-01	1.452E-01	0.000E+00
TH-228	2.024E+00	2.085E-01	6.230E-02	0.000E+00
TH-229	1.128E-01	3.149E-01	5.709E-01	0.000E+00
TH-230	9.628E-01	1.263E-01	7.467E-02	0.000E+00
TH-232	1.959E+00	2.019E-01	6.030E-02	0.000E+00
PA-233	3.387E-02	4.394E-02	6.507E-02	0.000E+00
TH-234	1.557E+00	1.793E+00	2.079E+00	0.000E+00
U-234	1.143E+00	1.900E-01	1.455E-01	0.000E+00
U-235	7.566E-02	1.261E-01	2.336E-01	0.000E+00
NP-237	1.193E+00	3.806E-01	2.569E-01	0.000E+00
U-238	1.557E+00	1.793E+00	2.079E+00	0.000E+00
AM-241	9.090E-02	2.220E-01	2.847E-01	0.000E+00
AM-242	2.599E+00	2.159E+00	2.402E+00	0.000E+00
ANH-511	1.295E-01	5.091E-02	3.044E-02	0.000E+00

---- Non-Identified Nuclides ----

Key-Line

Nuclide	Activity (pCi/GRAM	K.L. Act error) Ided	MDA (pCi/GRAM)	
BE-7	-5.889E-02	2.341E-01	4.194E-01	0.000E+00	NOT IDENT.
NA-22	1.190E-02	2.655E-02	4.839E-02	0.000E+00	NOT IDENT.
NA-24	0.000E+00	1.219E+14	0.000E+00	0.000E+00	SHORT HLIF
AL-26	-4.252E-04	1.487E-02	2.811E-02	0.000E+00	FAIL ABUN
SC-46	-2.036E-03	2.793E-02	4.795E-02	0.000E+00	FAIL ABUN
V-48	7.159E-03	8.339E-02	1.523E-01	0.000E+00	FAIL ABUN
CR-51	-6.690E-02	3.532E-01	6.075E-01	0.000E+00	NOT IDENT.
CO-56	-1.146E-02	2.838E-02	4.778E-02	0.000E+00	FAIL ABUN
MN-56	0.000E+00	2.473E+41	0.000E+00	0.000E+00	SHORT HLIF
CO-57	3.794E-03	1.624E-02	3.028E-02	0.000E+00	NOT IDENT.
CO-58	1.657E-02	2.793E-02	5.038E-02	0.000E+00	NOT IDENT.
FE-59	-2.786E-02	6.985E-02	1.218E-01	0.000E+00	NOT IDENT.
CO-60	-4.847E-03	2.278E-02	3.982E-02	0.000E+00	NOT IDENT.
ZN-65	2.321E-02	6.080E-02	9.752E-02	0.000E+00	NOT IDENT.
SE-75	-1.701E-02	3.018E-02	5.180E-02	0.000E+00	NOT IDENT.
KR-85	4.689E+00	4.415E+00	7.468E+00	0.000E+00	NOT IDENT.
SR-85	2.892E-02	2.723E-02	4.606E-02	0.000E+00	NOT IDENT.
Y-88	9.943E-03	2.066E-02	4.088E-02	0.000E+00	NOT IDENT.
Y-91	-6.564E-03	2.620E-02	4.635E-02	0.000E+00	NOT IDENT.
NB-94	5.217E-03	2.118E-02	3.755E-02	0.000E+00	NOT IDENT.
NB-95M	0.000E+00	3.995E+01	0.000E+00	0.000E+00	SHORT HLIF
ZR-95	-1.050E-02	5.223E-02	9.008E-02	0.000E+00	NOT IDENT.
MO-99	0.000E+00	5.932E+01	0.000E+00	0.000E+00	SHORT HLIF
TC-99M	0.000E+00	3.407E+37	0.000E+00	0.000E+00	SHORT HLIF
RU-103	1.752E-02	3.217E-02	5.958E-02	0.000E+00	FAIL ABUN
RH-106	-2.534E-02	1.981E-01	3.492E-01	0.000E+00	FAIL ABUN
RU-106	-2.935E-02	1.980E-01	3.486E-01	0.000E+00	NOT IDENT.
AG-108M	-1.677E-02	1.924E-02	3.369E-02	0.000E+00	NOT IDENT.
AG-110M	-1.022E-02	2.251E-02	3.871E-02	0.000E+00	FAIL ABUN
SN-113	3.072E-03	2.856E-02	5.273E-02	0.000E+00	NOT IDENT.
CD-115	0.000E+00	1.483E+03	0.000E+00	0.000E+00	SHORT HLIF
SN-115	5.348E+00	5.211E+00	5.529E+00	0.000E+00	FAIL ABUN
SN-117M	2.310E-02	8.173E-02	1.499E-01	0.000E+00	NOT IDENT.
TE-123M	-7.396E-03	1.917E-02	3.445E-02	0.000E+00	NOT IDENT.
SB-124	4.907E-02	4.496E-02	8.497E-02	0.000E+00	FAIL ABUN
SB-125	-1.027E-02	5.446E-02	9.866E-02	0.000E+00	FAIL ABUN
TE-125M	2.108E+00	6.892E+00	1.297E+01	0.000E+00	NOT IDENT.
I-126	1.559E-01	2.753E-01	5.004E-01	0.000E+00	NOT IDENT.
SB-126	1.611E-01	2.324E-01	4.226E-01	0.000E+00	NOT IDENT.
SB-127	0.000E+00	1.942E+01	0.000E+00	0.000E+00	SHORT HLIF
I-131	-7.708E-02	3.051E-01	5.582E-01	0.000E+00	NOT IDENT.
I-132	0.000E+00	8.314E+41	0.000E+00	0.000E+00	SHORT HLIF
TE-132	0.000E+00	1.865E+01	0.000E+00	0.000E+00	SHORT HLIF
BA-133	4.842E-03	2.762E-02	4.562E-02	0.000E+00	FAIL ABUN
I-133	0.000E+00	4.502E+09	0.000E+00	0.000E+00	SHORT HLIF
CS-134	0.000E+00	2.910E-02	5.321E-02	0.000E+00	NOT IDENT.
I-135	0.000E+00	5.807E+34	0.000E+00	0.000E+00	SHORT HLIF
CS-136	-6.548E-02	1.542E-01	2.699E-01	0.000E+00	FAIL ABUN
BA-137M	-3.842E-03	2.226E-02	3.885E-02	0.000E+00	NOT IDENT.
CS-137	-4.117E-03	2.353E-02	4.106E-02	0.000E+00	NOT IDENT.
CE-139	-3.407E-03	2.045E-02	3.688E-02	0.000E+00	NOT IDENT.
BA-140	7.979E-02	4.030E-01	7.292E-01	0.000E+00	NOT IDENT.
LA-140	-1.443E-01	1.301E-01	2.006E-01	0.000E+00	FAIL ABUN
CE-141	1.954E-03	5.483E-02	1.004E-01	0.000E+00	NOT IDENT.
CE-143	0.000E+00	2.421E+06	0.000E+00	0.000E+00	SHORT HLIF
CE-144	-4.692E-02	1.282E-01	2.333E-01	0.000E+00	NOT IDENT.
PM-144	-2.397E-02	2.174E-02	3.566E-02	0.000E+00	NOT IDENT.
PR-144	0.000E+00	9.068E+40	0.000E+00	0.000E+00	SHORT HLIF
PM-146	2.392E-02	2.666E-02	5.016E-02	0.000E+00	NOT IDENT.
ND-147	-6.095E-01	1.002E+00	1.740E+00	0.000E+00	FAIL ABUN
PM-147	-1.149E+04	3.311E+04	6.074E+04	0.000E+00	NOT IDENT.
PM-149	0.000E+00	1.855E+04	0.000E+00	0.000E+00	SHORT HLIF
EU-152	-2.285E-02	6.199E-02	1.050E-01	0.000E+00	FAIL ABUN
GD-153	0.000E+00	7.350E-02	9.386E-02	0.000E+00	FAIL ABUN
EU-154	3.174E-02	7.345E-02	1.337E-01	0.000E+00	NOT IDENT.
TB-160	-5.704E-04	1.106E-01	1.669E-01	0.000E+00	FAIL ABUN
TM-171	5.877E+00	2.262E+01	4.379E+01	0.000E+00	FAIL ABUN
HF-181	2.556E-02	3.414E-02	6.383E-02	0.000E+00	FAIL ABUN
TA-182	-4.914E-02	1.429E-01	2.458E-01	0.000E+00	FAIL ABUN
IR-192	-2.720E-03	2.478E-02	4.284E-02	0.000E+00	FAIL ABUN
HG-203	4.518E-02	4.501E-02	6.058E-02	0.000E+00	FAIL ABUN
BI-207	-2.518E-02	3.194E-02	5.431E-02	0.000E+00	NOT IDENT.
BI-210	2.358E+00	8.060E+00	1.338E+01	0.000E+00	NOT IDENT.
PB-210	2.358E+00	8.060E+00	1.338E+01	0.000E+00	NOT IDENT.
PB-211	1.723E-02	6.353E-01	1.027E+00	0.000E+00	NOT IDENT.

RN-219	1.598E-02	2.476E-01	4.547E-01	0.000E+00	FAIL	ABUN
RA-223	2.124E-01	4.061E-01	7.171E-01	0.000E+00	FAIL	ABUN
AC-227	-4.839E-02	2.469E-01	4.312E-01	0.000E+00	FAIL	ABUN
TH-227	-4.756E-02	2.427E-01	4.238E-01	0.000E+00	FAIL	ABUN
PA-231	4.884E-01	9.626E-01	1.713E+00	0.000E+00	FAIL	ABUN
TH-231	0.000E+00	2.021E-01	2.457E-01	0.000E+00	FAIL	ABUN
PA-234	-1.029E-01	1.822E-01	3.173E-01	0.000E+00	FAIL	ABUN
PA-234M	3.830E+00	2.709E+00	5.234E+00	0.000E+00	FAIL	ABUN
NP-239	0.000E+00	1.548E-01	2.139E-01	0.000E+00	FAIL	ABUN
CM-247	1.123E-02	2.230E-02	4.163E-02	0.000E+00	FAIL	ABUN
CF-249	-1.035E-02	2.307E-02	4.163E-02	0.000E+00	NOT IDENT.	
CF-251	3.288E-03	7.966E-02	1.440E-01	0.000E+00	NOT IDENT.	


```

*****
*                               GENERAL ENG. LABS, LLC.                               *
*                               2040 Savage Road                                       *
*                               Charleston, SC 29414                                   *
*****
Configuration      : DKA300:[CANBERRA.GAMMA.ARCHIVE.GAMMA]G1201055608.CNF;1
Sample date        : 10-MAR-2006 07:46:00 Acquisition date : 11-APR-2006 23:19:39
Sample ID          : G1201055608           Sample quantity  : 1.59640E+02 GRAM
Detector name     : GAMMA16                Detector geometry: CAN
Elapsed live time : 0 04:00:00.00          Elapsed real time : 0 04:00:02.78  0.0%
Energy tolerance  : 2.00000 KEV           Analyst Initials  : MJH1
Abundance limit   : 75.00000              Sensitivity       : 3.00000
Batch ID          : 513802                 Detector SN#      : 1922864
Matrix Spike DPM  :                       LCS DPM         :
*****
    
```

Nuclide Line Activity Report

Nuclide Type:

Nuclide	Energy	Area	%Abn	%Eff	Uncorrected pCi/GRAM	Decay Corr pCi/GRAM	2-Sigma %Error
K-40	1460.81	2692	10.67*	1.093E+00	2.714E+01	2.714E+01	7.79
MN-54	834.83	58	99.83*	1.804E+00	3.755E-02	4.038E-02	76.70
NB-95	765.79	120	99.81*	1.945E+00	7.255E-02	1.386E-01	40.29
CD-109	88.03	594	3.79*	4.646E+00	3.966E+00	4.164E+00	24.34
SN-126	64.28	91	9.60	1.802E+00	6.162E-01	6.162E-01	114.80
	86.94	594	8.90	4.646E+00	1.689E+00	1.689E+00	47.21
	87.57	594	37.00*	4.646E+00	4.062E-01	4.062E-01	24.34
CS-135	268.24	267	16.00*	4.173E+00	4.701E-01	4.701E-01	36.61
EU-155	86.54	594	30.90	4.646E+00	4.864E-01	4.925E-01	24.37
	105.31	133	20.70*	5.738E+00	1.313E-01	1.330E-01	82.74
HG-203	70.83	-----	4.75	2.802E+00	-----	Line Not Found	-----
	72.87	761	8.00	3.297E+00	3.391E+00	5.517E+00	20.57
	82.60	226	3.55	4.378E+00	1.712E+00	2.785E+00	40.22
	279.20	75	77.30*	4.098E+00	2.777E-02	4.518E-02	99.61
TL-208	75.00	761	3.43	3.297E+00	7.909E+00	8.170E+00	19.99
	277.35	75	6.80	4.098E+00	3.157E-01	3.261E-01	99.98
	510.84	296	21.60	2.691E+00	5.996E-01	6.194E-01	40.19
	583.14	1034	84.20*	2.438E+00	5.922E-01	6.118E-01	11.03
	763.30	-----	1.64	1.954E+00	-----	Line Not Found	-----
	860.37	153	12.46	1.756E+00	8.220E-01	8.492E-01	50.08
	1093.90	-----	0.37	1.403E+00	-----	Line Not Found	-----
BI-211	351.07	1231	12.94*	3.485E+00	3.209E+00	3.209E+00	11.83
BI-212	727.18	240	11.80*	2.039E+00	1.172E+00	1.211E+00	27.08
PB-212	74.80	761	10.70	3.297E+00	2.535E+00	2.619E+00	20.26
	87.30	594	8.00	4.646E+00	1.879E+00	1.941E+00	26.32
	115.19	123	0.60	5.991E+00	4.001E+00	4.134E+00	71.32
	238.63	3374	44.60*	4.541E+00	1.959E+00	2.024E+00	10.30
	300.09	201	3.41	3.884E+00	1.788E+00	1.847E+00	38.45
BI-214	609.31	893	46.30*	2.356E+00	9.628E-01	9.629E-01	13.12
	768.36	120	5.04	1.945E+00	1.437E+00	1.437E+00	40.73
	934.06	59	3.21	1.630E+00	1.332E+00	1.332E+00	97.65
	1120.29	224	15.10	1.373E+00	1.271E+00	1.271E+00	26.57

Nuclide Type:

Nuclide	Energy	Area	%Abn	%Eff	Uncorrected pCi/GRAM	Decay Corr pCi/GRAM	2-Sigma %Error
	1238.11	83	5.94	1.252E+00	1.312E+00	1.312E+00	64.44
	1377.67	63	4.11	1.143E+00	1.565E+00	1.565E+00	43.26
PB-214	74.81	761	6.21	3.297E+00	4.368E+00	4.369E+00	19.44
	77.11	1096	10.50	3.580E+00	3.429E+00	3.429E+00	16.41
	87.30	594	4.41	4.646E+00	3.408E+00	3.408E+00	25.67
	241.98	795	7.50	4.504E+00	2.769E+00	2.769E+00	16.62
	295.21	733	19.20	3.927E+00	1.143E+00	1.143E+00	16.62
RA-226	351.92	1231	37.20*	3.485E+00	1.116E+00	1.116E+00	12.93
	295.21	733	19.20	3.927E+00	1.143E+00	1.143E+00	16.62
	351.92	1231	37.20	3.485E+00	1.116E+00	1.116E+00	11.52
AC-228	609.31	893	46.30*	2.356E+00	9.628E-01	9.629E-01	13.12
	209.25	257	4.40	4.954E+00	1.388E+00	1.403E+00	73.61
	338.32	753	11.40	3.579E+00	2.170E+00	2.194E+00	43.37
	463.01	186	4.40	2.886E+00	1.720E+00	1.739E+00	41.23
	794.95	149	4.60	1.888E+00	2.020E+00	2.042E+00	39.08
	911.21	722	27.70*	1.667E+00	1.838E+00	1.858E+00	15.63
	964.77	114	5.20	1.580E+00	1.634E+00	1.652E+00	43.75
RA-228	969.11	417	16.60	1.574E+00	1.875E+00	1.896E+00	27.25
	209.25	257	4.40	4.954E+00	1.388E+00	1.403E+00	73.61
	338.32	753	11.40	3.579E+00	2.170E+00	2.194E+00	43.37
	463.01	186	4.40	2.886E+00	1.720E+00	1.739E+00	41.23
	794.95	149	4.60	1.888E+00	2.020E+00	2.042E+00	39.08
	911.21	722	27.70*	1.667E+00	1.838E+00	1.858E+00	15.63
	964.77	114	5.20	1.580E+00	1.634E+00	1.652E+00	43.75
	969.11	417	16.60	1.574E+00	1.875E+00	1.896E+00	27.25
TH-228	84.40	226	1.21	4.378E+00	5.022E+00	5.188E+00	40.02
	238.60	3374	44.60*	4.541E+00	1.959E+00	2.024E+00	10.30
	300.10	201	3.41	3.884E+00	1.788E+00	1.847E+00	69.89
TH-229	85.43	226	16.50	4.378E+00	3.683E-01	3.683E-01	38.77
	88.47	594	27.10	4.646E+00	5.546E-01	5.546E-01	24.34
	100.00	134	12.40	5.474E+00	2.313E-01	2.313E-01	73.02
	193.63	-----	4.59*	5.199E+00	-----	Line Not Found	-----
	210.97	257	3.26	4.954E+00	1.871E+00	1.871E+00	37.00
TH-230	295.21	733	19.20	3.927E+00	1.143E+00	1.143E+00	16.62
	351.92	1231	37.20	3.485E+00	1.116E+00	1.116E+00	11.52
	609.31	893	46.30*	2.356E+00	9.628E-01	9.628E-01	13.12
TH-232	238.59	3374	44.60*	4.541E+00	1.959E+00	1.959E+00	10.30
	911.20	722	27.70	1.667E+00	1.838E+00	1.838E+00	15.63
	964.40	114	5.20	1.580E+00	1.634E+00	1.634E+00	43.75
	969.11	417	16.60	1.574E+00	1.875E+00	1.875E+00	27.25
PA-233	75.28	761	1.26	3.297E+00	2.153E+01	2.153E+01	22.01
	86.59	594	1.89	4.646E+00	7.952E+00	7.952E+00	35.18
	300.12	201	6.60	3.884E+00	9.238E-01	9.238E-01	39.89
	311.98	42	38.60*	3.776E+00	3.387E-02	3.387E-02	129.74
	340.50	-----	4.50	3.562E+00	-----	Line Not Found	-----
	398.62	-----	1.27	3.200E+00	-----	Line Not Found	-----
	415.76	-----	1.62	3.109E+00	-----	Line Not Found	-----
TH-234	63.29	91	3.80*	1.802E+00	1.557E+00	1.557E+00	115.20
	92.38	502	5.41	5.085E+00	2.144E+00	2.144E+00	32.25

Nuclide Type:

Nuclide	Energy	Area	%Abn	%Eff	Uncorrected pCi/GRAM	Decay Corr pCi/GRAM	2-Sigma %Error
	112.81	-----	0.24	5.950E+00	-----	Line Not Found	-----
U-234	67.67	-----	0.37	2.385E+00	-----	Line Not Found	-----
	241.98	795	7.49	4.504E+00	2.772E+00	2.772E+00	16.63
	295.21	733	19.20*	3.927E+00	1.143E+00	1.143E+00	16.62
	351.92	1231	37.20	3.485E+00	1.116E+00	1.116E+00	12.93
U-235	89.95	314	2.70	4.862E+00	2.812E+00	2.812E+00	41.66
	93.35	502	4.50	5.085E+00	2.577E+00	2.577E+00	38.71
	105.00	133	2.10	5.738E+00	1.295E+00	1.295E+00	87.52
	143.76	-----	10.50*	5.981E+00	-----	Line Not Found	-----
	163.33	-----	4.70	5.703E+00	-----	Line Not Found	-----
	185.71	378	54.00	5.330E+00	1.542E-01	1.542E-01	37.22
	205.31	-----	5.00	5.012E+00	-----	Line Not Found	-----
NP-237	86.48	594	12.60*	4.646E+00	1.193E+00	1.193E+00	31.91
	95.87	-----	2.60	5.290E+00	-----	Line Not Found	-----
U-238	63.29	91	3.80*	1.802E+00	1.557E+00	1.557E+00	115.20
NP-239	99.55	134	14.70	5.474E+00	1.951E-01	1.951E-01	73.02
	117.00	123	11.10*	5.991E+00	2.170E-01	2.170E-01	71.32
	209.75	257	3.24	4.954E+00	1.885E+00	1.885E+00	37.00
	228.18	-----	10.70	4.677E+00	-----	Line Not Found	-----
	277.60	75	14.10	4.098E+00	1.522E-01	1.522E-01	99.59
	334.31	-----	2.04	3.607E+00	-----	Line Not Found	-----
AM-241	59.54	35	35.90*	1.268E+00	9.088E-02	9.090E-02	244.28
AM-242	99.55	134	0.63	5.474E+00	4.553E+00	4.554E+00	73.02
	103.70	133	1.01*	5.738E+00	2.692E+00	2.693E+00	82.73
ANH-511	511.00	296	100.00*	2.691E+00	1.295E-01	1.295E-01	39.31

Nuclide Type: NATURAL

Nuclide	Energy	Area	%Abn	%Eff	Uncorrected pCi/GRAM	Decay Corr pCi/GRAM	2-Sigma %Error
RA-224	240.98	795	3.95*	4.504E+00	5.257E+00	5.431E+00	15.65

Flag: "*" = Keyline

Total number of lines in spectrum 79
 Number of unidentified lines 26
 Number of lines tentatively identified by NID 53 67.09%

Nuclide Type :

Nuclide	Hlife	Decay	Uncorrected pCi/GRAM	Decay Corr pCi/GRAM	Decay Corr 2-Sigma Error	2-Sigma %Error	Flags
K-40	1.28E+09Y	1.00	2.714E+01	2.714E+01	0.211E+01	7.79	
MN-54	312.70D	1.08	3.755E-02	4.038E-02	3.097E-02	76.70	
NB-95	35.06D	1.91	7.255E-02	1.386E-01	0.558E-01	40.29	
CD-109	464.00D	1.05	3.966E+00	4.164E+00	1.014E+00	24.34	
SN-126	1.00E+05Y	1.00	4.062E-01	4.062E-01	0.989E-01	24.34	
CS-135	2.30E+06Y	1.00	4.701E-01	4.701E-01	1.721E-01	36.61	
EU-155	4.96Y	1.01	1.313E-01	1.330E-01	1.100E-01	82.74	
HG-203	46.61D	1.63	2.777E-02	4.518E-02	4.501E-02	99.61	
TL-208	1.91Y	1.03	5.922E-01	6.118E-01	0.675E-01	11.03	
BI-211	7.04E+08Y	1.00	3.209E+00	3.209E+00	0.380E+00	11.83	
BI-212	1.91Y	1.03	1.172E+00	1.211E+00	0.328E+00	27.08	
PB-212	1.91Y	1.03	1.959E+00	2.024E+00	0.209E+00	10.30	
BI-214	1600.00Y	1.00	9.628E-01	9.629E-01	1.263E-01	13.12	
PB-214	1600.00Y	1.00	1.116E+00	1.116E+00	0.144E+00	12.93	
RA-226	1600.00Y	1.00	9.628E-01	9.629E-01	1.263E-01	13.12	
AC-228	5.75Y	1.01	1.838E+00	1.858E+00	0.290E+00	15.63	
RA-228	5.75Y	1.01	1.838E+00	1.858E+00	0.290E+00	15.63	
TH-228	1.91Y	1.03	1.959E+00	2.024E+00	0.209E+00	10.30	
TH-229	7340.00Y	1.00	5.546E-01	5.546E-01	1.350E-01	24.34	K
TH-230	7.70E+04Y	1.00	9.628E-01	9.628E-01	1.263E-01	13.12	
TH-232	1.41E+10Y	1.00	1.959E+00	1.959E+00	0.202E+00	10.30	
PA-233	2.14E+06Y	1.00	3.387E-02	3.387E-02	4.394E-02	129.74	
TH-234	4.47E+09Y	1.00	1.557E+00	1.557E+00	1.793E+00	115.20	
U-234	2.45E+05Y	1.00	1.143E+00	1.143E+00	0.190E+00	16.62	
U-235	7.04E+08Y	1.00	1.542E-01	1.542E-01	0.574E-01	37.22	K
NP-237	2.14E+06Y	1.00	1.193E+00	1.193E+00	0.381E+00	31.91	
U-238	4.47E+09Y	1.00	1.557E+00	1.557E+00	1.793E+00	115.20	
NP-239	7380.00Y	1.00	2.170E-01	2.170E-01	1.548E-01	71.32	
AM-241	432.20Y	1.00	9.088E-02	9.090E-02	22.20E-02	244.28	
AM-242	152.00Y	1.00	2.692E+00	2.693E+00	2.228E+00	82.73	
ANH-511	1.00E+09Y	1.00	1.295E-01	1.295E-01	0.509E-01	39.31	
Total Activity :			6.010E+01	6.062E+01			

Nuclide Type : NATURAL

Nuclide	Hlife	Decay	Uncorrected pCi/GRAM	Decay Corr pCi/GRAM	Decay Corr 2-Sigma Error	2-Sigma %Error	Flags
RA-224	1.91Y	1.03	5.257E+00	5.431E+00	0.850E+00	15.65	
Total Activity :			5.257E+00	5.431E+00			

Grand Total Activity : 6.536E+01 6.605E+01

Flags: "K" = Keyline not found "M" = Manually accepted
 "E" = Manually edited "A" = Nuclide specific abn. limit

It	Energy	Area	Bkgnd	FWHM	Channel	Left	Pw	Cts/Sec	%Err	%Eff	Flags
0	128.81	178	889	1.04	256.05	252	9	1.24E-02	62.9	6.08E+00	
0	153.49	104	604	1.14	305.36	302	7	7.19E-03	81.1	5.85E+00	T
0	202.08	53	530	1.23	402.48	400	7	3.68E-03	****	5.06E+00	
0	287.36	29	382	0.94	572.92	570	8	2.05E-03	****	4.00E+00	T
0	328.00	149	350	1.26	654.16	650	9	1.04E-02	48.0	3.65E+00	T
0	409.11	70	342	1.12	816.30	811	11	4.89E-03	****	3.14E+00	
0	469.18	61	175	1.46	936.39	932	9	4.26E-03	82.2	2.86E+00	T
0	678.37	23	89	1.57	1354.67	1352	7	1.60E-03	****	2.16E+00	T
0	771.97	91	89	1.70	1541.86	1538	10	6.35E-03	44.9	1.93E+00	T
0	785.10	94	104	1.36	1568.11	1563	10	6.52E-03	46.0	1.91E+00	T
0	805.73	31	96	0.93	1609.37	1607	8	2.16E-03	****	1.86E+00	T
0	823.79	24	93	1.48	1645.50	1641	10	1.65E-03	****	1.83E+00	
0	839.29	48	93	1.80	1676.49	1673	8	3.33E-03	78.7	1.80E+00	
0	882.30	26	45	1.39	1762.52	1760	6	1.79E-03	93.0	1.72E+00	T
0	1154.56	29	56	1.37	2307.16	2304	7	1.98E-03	94.7	1.33E+00	
0	1197.75	9	113	0.93	2393.59	2393	9	5.90E-04	****	1.29E+00	
0	1264.72	20	52	1.40	2527.58	2525	7	1.37E-03	****	1.23E+00	
0	1311.32	26	41	1.87	2620.84	2618	7	1.78E-03	91.4	1.19E+00	T
0	1367.23	21	30	2.05	2732.73	2730	8	1.49E-03	98.3	1.15E+00	T
2	1406.92	43	24	2.51	2812.16	2807	20	2.96E-03	55.5	1.12E+00	
2	1411.31	40	22	2.51	2820.94	2807	20	2.80E-03	59.4	1.12E+00	
0	1419.04	30	15	2.13	2836.42	2833	9	2.06E-03	60.3	1.12E+00	
0	1472.94	30	16	6.30	2944.30	2937	16	2.08E-03	69.9	1.09E+00	
0	1479.58	22	11	1.65	2957.59	2953	11	1.53E-03	72.3	1.08E+00	
0	1507.84	9	30	1.59	3014.15	3010	10	6.36E-04	****	1.07E+00	
0	1577.14	20	15	4.74	3152.87	3147	12	1.40E-03	96.7	1.04E+00	
0	1588.33	72	76	1.71	3175.26	3167	18	4.99E-03	63.2	1.03E+00	
0	1608.45	9	17	0.96	3215.53	3211	11	5.90E-04	****	1.03E+00	
3	1619.39	48	16	2.89	3237.43	3232	36	3.32E-03	43.8	1.02E+00	
3	1629.38	23	7	2.89	3257.44	3232	36	1.61E-03	99.8	1.02E+00	
0	1636.32	16	7	2.26	3271.32	3268	11	1.08E-03	99.7	1.02E+00	
0	1659.95	8	14	0.75	3318.64	3316	8	5.88E-04	****	1.01E+00	
6	1678.64	23	4	3.89	3356.04	3346	40	1.62E-03	78.7	1.00E+00	T
6	1690.59	14	10	2.93	3379.98	3346	40	9.73E-04	91.4	9.99E-01	T
0	1728.10	65	11	2.62	3455.07	3450	13	4.50E-03	32.0	9.89E-01	
0	1749.49	24	11	3.82	3497.90	3491	15	1.69E-03	72.4	9.84E-01	
0	1763.28	142	40	2.38	3525.50	3518	18	9.86E-03	28.6	9.82E-01	
0	1846.54	26	23	2.44	3692.22	3683	15	1.81E-03	91.9	9.68E-01	
0	1976.75	10	10	1.50	3952.97	3950	9	7.19E-04	****	9.60E-01	

Flags: "T" = Tentatively associated

```

*****
*                                     GENERAL ENG. LABS, LLC.                               *
*                                     2040 Savage Road                                   *
*                                     Charleston, SC 29414                             *
*****
*                                     DETECTOR DATA                                   *
*
* Configuration      : DKA300:[CANBERRA.GAMMA.ARCHIVE.GAMMA]G1201055608.CNF;1
* Acquisition date   : 11-APR-2006 23:19:39  Detector SN#      : 1922864
* Detector ID        : GAMMA16                Sensitivity       : 3.00000
* Geometry           : CAN                    Energy tolerance: 2.00000
* Elapsed live time  : 0 04:00:00.00          Abundance limit  : 75.00000
* Elapsed real time  : 0 04:00:02.78          Half life ratio  : 8.00000
*****
*                                     SAMPLE DATA                                   *
*
* Sample date        : 10-MAR-2006 07:46:00  Nuclide Library   : EPI
* Sample ID          : G1201055608           Analyst initials    : MJH1
* Batch Number       : 513802                Sample Quantity    : 1.59640E+02 GRAM
*****
*                                     QC DATA                                       *
*
* CALIB. DATE/TIME  : 5-APR-2006 19:34:04.74MS Isotope         :
* MSD DPM            :                       MSD Isotope        :
* LCS DPM            :                       LCS Isotope         :
*****

```

Combined Activity-MDA Report

---- Identified Nuclides ----

Nuclide	Activity (pCi/GRAM)	Act error	MDA (pCi/GRAM)	MDA error	Act/MDA
K-40	2.714E+01	2.114E+00	3.309E-01	2.185E-02	81.998
MN-54	4.038E-02	3.097E-02	3.966E-02	3.351E-03	1.018
NB-95	1.054E-02	6.228E-02	7.172E-02	5.367E-03	0.147
CD-109	4.164E+00	1.014E+00	7.982E-01	8.452E-02	5.217
SN-126	4.062E-01	9.887E-02	7.850E-02	8.294E-03	5.175
CS-135	4.701E-01	1.721E-01	1.537E-01	1.468E-02	3.059
EU-155	1.283E-01	1.067E-01	1.116E-01	9.533E-03	1.150
TL-208	6.118E-01	6.749E-02	3.773E-02	2.641E-03	16.215
BI-211	3.209E+00	3.797E-01	2.088E-01	1.532E-02	15.369
BI-212	1.211E+00	3.278E-01	2.712E-01	2.338E-02	4.463
PB-212	2.024E+00	2.085E-01	5.858E-02	5.544E-03	34.547
BI-214	9.629E-01	1.263E-01	7.207E-02	5.805E-03	13.360
PB-214	1.116E+00	1.444E-01	7.185E-02	6.459E-03	15.538
RA-224	5.431E+00	8.500E-01	6.665E-01	5.547E-02	8.148
RA-226	9.629E-01	1.263E-01	7.207E-02	5.805E-03	13.360
AC-228	1.858E+00	2.904E-01	1.417E-01	1.672E-02	13.106
RA-228	1.858E+00	2.904E-01	1.417E-01	1.672E-02	13.106
TH-228	2.024E+00	2.085E-01	5.858E-02	5.543E-03	34.550

---- Identified Nuclides ----

Nuclide	Activity (pCi/GRAM)	Act error	MDA (pCi/GRAM)	MDA error	Act/MDA
TH-229	1.128E-01	3.149E-01	5.338E-01	4.464E-02	0.211
TH-230	9.628E-01	1.263E-01	7.207E-02	5.805E-03	13.360
TH-232	1.959E+00	2.019E-01	5.670E-02	5.365E-03	34.551
PA-233	3.387E-02	4.394E-02	6.164E-02	4.835E-03	0.549
TH-234	1.557E+00	1.793E+00	1.888E+00	3.757E-01	0.825
U-234	1.143E+00	1.900E-01	1.376E-01	1.378E-02	8.307
U-235	7.566E-02	1.261E-01	2.167E-01	3.715E-02	0.349
NP-237	1.193E+00	3.806E-01	2.352E-01	5.447E-02	5.072
U-238	1.557E+00	1.793E+00	1.888E+00	3.757E-01	0.825
AM-241	9.090E-02	2.220E-01	2.582E-01	3.496E-02	0.352
AM-242	2.599E+00	2.159E+00	2.209E+00	1.888E-01	1.176
ANH-511	1.295E-01	5.091E-02	2.923E-02	1.779E-03	4.430

---- Non-Identified Nuclides ----

Nuclide	Key-Line Activity (pCi/GRAM)	K.L. Ided	Act error	MDA (pCi/GRAM)	MDA error	Act/MDA
BE-7	-5.889E-02		2.341E-01	4.020E-01	2.790E-02	-0.146
NA-22	1.190E-02		2.655E-02	4.772E-02	3.101E-03	0.249
AL-26	-4.252E-04		1.487E-02	2.802E-02	1.612E-03	-0.015
SC-46	-2.036E-03		2.793E-02	4.679E-02	4.336E-03	-0.044
V-48	7.159E-03		8.339E-02	1.491E-01	1.320E-02	0.048
CR-51	-6.690E-02		3.532E-01	5.758E-01	4.580E-02	-0.116
CO-56	-1.146E-02		2.838E-02	4.655E-02	4.015E-03	-0.246
CO-57	3.794E-03		1.624E-02	2.797E-02	2.167E-03	0.136
CO-58	1.657E-02		2.793E-02	4.903E-02	3.983E-03	0.338
FE-59	-2.786E-02		6.985E-02	1.196E-01	1.019E-02	-0.233
CO-60	-4.847E-03		2.278E-02	3.932E-02	2.447E-03	-0.123
ZN-65	2.321E-02		6.080E-02	9.579E-02	7.255E-03	0.242
SE-75	-1.701E-02		3.018E-02	4.884E-02	4.010E-03	-0.348
KR-85	4.689E+00		4.415E+00	7.173E+00	4.367E-01	0.654
SR-85	2.892E-02		2.723E-02	4.424E-02	2.694E-03	0.654
Y-88	9.943E-03		2.066E-02	4.076E-02	2.319E-03	0.244
Y-91	-6.564E-03		2.620E-02	4.462E-02	2.741E-03	-0.147
NB-94	5.217E-03		2.118E-02	3.639E-02	2.419E-03	0.143
ZR-95	-1.050E-02		5.223E-02	8.748E-02	7.314E-03	-0.120
RU-103	1.752E-02		3.217E-02	5.717E-02	7.298E-03	0.306
RH-106	-2.534E-02		1.981E-01	3.372E-01	2.079E-02	-0.075
RU-106	-2.935E-02		1.980E-01	3.367E-01	4.013E-02	-0.087
AG-108M	-1.677E-02		1.924E-02	3.220E-02	2.057E-03	-0.521
AG-110M	-1.022E-02		2.251E-02	3.745E-02	2.434E-03	-0.273
SN-113	3.072E-03		2.856E-02	5.026E-02	3.082E-03	0.061
SN-115	5.348E+00	+	5.211E+00	5.403E+00	4.973E-01	0.990
SN-117M	2.310E-02		8.173E-02	1.394E-01	1.133E-02	0.166
TE-123M	-7.396E-03		1.917E-02	3.204E-02	2.625E-03	-0.231
SB-124	4.907E-02	+	4.496E-02	8.452E-02	5.501E-03	0.581
SB-125	-1.027E-02		5.446E-02	9.427E-02	5.769E-03	-0.109
TE-125M	2.108E+00		6.892E+00	1.194E+01	1.200E+00	0.177

---- Non-Identified Nuclides ----

Nuclide	Key-Line Activity (pCi/GRAM)	K.L. Ided	Act error	MDA (pCi/GRAM)	MDA error	Act/MDA
I-126	1.559E-01		2.753E-01	4.842E-01	3.001E-02	0.322
SB-126	1.611E-01		2.324E-01	4.098E-01	2.818E-02	0.393
I-131	-7.708E-02		3.051E-01	5.309E-01	3.889E-02	-0.145
BA-133	4.842E-03		2.762E-02	4.336E-02	5.214E-03	0.112
CS-134	8.632E-02		2.910E-02	5.176E-02	4.113E-03	1.668
CS-136	-6.548E-02		1.542E-01	2.646E-01	2.302E-02	-0.247
BA-137M	-3.842E-03		2.226E-02	3.759E-02	2.308E-03	-0.102
CS-137	-4.117E-03		2.353E-02	3.972E-02	2.449E-03	-0.104
CE-139	-3.407E-03		2.045E-02	3.434E-02	2.849E-03	-0.099
BA-140	7.979E-02		4.030E-01	7.013E-01	2.285E-01	0.114
LA-140	-1.443E-01		1.301E-01	1.992E-01	1.231E-02	-0.724
CE-141	1.954E-03		5.483E-02	9.319E-02	7.502E-03	0.021
CE-144	-4.692E-02		1.282E-01	2.160E-01	3.261E-02	-0.217
PM-144	-2.397E-02		2.174E-02	3.455E-02	2.276E-03	-0.694
PM-146	2.392E-02		2.666E-02	4.800E-02	4.190E-03	0.498
ND-147	-6.095E-01		1.002E+00	1.673E+00	2.286E-01	-0.364
PM-147	-1.149E+04		3.311E+04	5.609E+04	4.349E+03	-0.205
EU-152	-2.285E-02		6.199E-02	9.970E-02	7.548E-03	-0.229
GD-153	1.007E-01	+	7.350E-02	8.618E-02	7.864E-03	1.168
EU-154	3.174E-02		7.345E-02	1.318E-01	1.290E-02	0.241
TB-160	-5.704E-04		1.106E-01	1.628E-01	1.484E-02	-0.004
TM-171	5.877E+00		2.262E+01	3.981E+01	4.548E+00	0.148
HF-181	2.556E-02		3.414E-02	6.119E-02	3.688E-03	0.418
TA-182	-4.914E-02		1.429E-01	2.421E-01	1.618E-02	-0.203
IR-192	-2.720E-03		2.478E-02	4.059E-02	3.050E-03	-0.067
HG-203	4.518E-02		4.501E-02	5.721E-02	4.741E-03	0.790
BI-207	-2.518E-02		3.194E-02	5.327E-02	4.335E-03	-0.473
BI-210	2.358E+00		8.060E+00	1.206E+01	1.231E+00	0.196
PB-210	2.358E+00		8.060E+00	1.206E+01	1.231E+00	0.196
PB-211	1.723E-02		6.353E-01	9.799E-01	6.109E-01	0.018
RN-219	1.598E-02		2.476E-01	4.337E-01	5.897E-02	0.037
RA-223	2.124E-01		4.061E-01	6.799E-01	1.164E-01	0.312
AC-227	-4.839E-02		2.469E-01	4.062E-01	6.211E-02	-0.119
TH-227	-4.756E-02		2.427E-01	3.993E-01	7.140E-02	-0.119
PA-231	4.884E-01		9.626E-01	1.618E+00	2.399E-01	0.302
TH-231	5.530E-01	+	2.021E-01	2.318E-01	2.143E-02	2.386
PA-234	-1.029E-01		1.822E-01	3.101E-01	5.892E-02	-0.332
PA-234M	3.830E+00		2.709E+00	5.125E+00	5.141E-01	0.747
NP-239	2.170E-01	+	1.548E-01	1.973E-01	1.553E-02	1.100
CM-247	1.123E-02		2.230E-02	3.971E-02	2.297E-03	0.283
CF-249	-1.035E-02		2.307E-02	3.967E-02	2.319E-03	-0.261
CF-251	3.288E-03		7.966E-02	1.343E-01	1.117E-02	0.024


```

*****
*
*                               General Engineering Labs, LLC
*                               2040 SAVAGE ROAD
*                               CHARLESTON ,SC 29417
*                               GROSS GAMMA REPORT
*
*****
*
*   BATCH ID      : 513802                SAMPLE ID   : G1201055608
*   ANALYST       : MJH1                  DETECTOR    : GAMMA16
*   SAMPLE DATE   : 10-MAR-2006 07:46:00.00  COUNT TIME  : 0 04:00:00.00
*   ANALYSIS DATE: 11-APR-2006 23:19:39.16  SAMPLE ALQT: 159.640 GRAM
*
*****

```

```

GROSS GAMMA ACTIVITY (pCi/GRAM ) : 1.038E+01
GROSS GAMMA ERROR (pCi/GRAM ) : 2.012E+00
GROSS GAMMA MDA (pCi/GRAM ) : 6.021E+00
GROSS GAMMA DLC (pCi/GRAM ) : 2.940E+00

```

VAX/VMS Nuclide Identification Report Generated 11-APR-2006 15:32:01.09

```

*****
*                               GENERAL ENG. LABS, LLC.                               *
*                               2040 Savage Road                                       *
*                               Charleston, SC 29414                                   *
*****
Configuration   : DKA300:[CANBERRA.GAMMA.ARCHIVE.GAMMA]G1201055609.CNF;1
Sample date     : 21-MAR-2006 00:00:00 Acquisition date : 11-APR-2006 14:31:28
Sample ID      : G1201055609 Sample quantity   : 1.00000E+02 GRAM
Detector name   : WELL Detector geometry     : CAN
Elapsed live time: 0 01:00:00.00 Elapsed real time: 0 01:00:02.86 0.1%
Energy tolerance: 2.00000 KEV Analyst Initials  : MJH1
Abundance limit : 75.00000 Sensitivity     : 3.00000
Batch ID       : 513802 Detector SN#     : 3941466
Matrix Spike DPM : LCS DPM                   :
*****

```

Pk	It	Energy	Area	Bkgnd	FWHM	Channel	Left	Pw	Cts/Sec	%Err	Fit
1	0	33.21*	246	769	1.48	65.39	63	7	6.83E-02	19.9	
2	0	36.87*	129	814	2.01	72.65	70	8	3.57E-02	39.7	
3	0	59.65	4879	1697	1.38	117.92	111	13	1.36E+00	2.2	
4	0	88.24*	4854	1204	1.32	174.71	167	14	1.35E+00	2.1	
5	0	92.77*	5	335	1.31	183.70	181	8	1.28E-03	727.5	
6	0	122.41*	1614	701	1.40	242.60	235	14	4.48E-01	4.3	
7	0	136.67	239	369	1.49	270.92	266	11	6.63E-02	16.9	
8	0	166.12	873	343	1.41	329.44	323	14	2.43E-01	5.6	
9	0	186.07*	17	276	0.71	369.08	364	9	4.61E-03	187.6	
10	0	373.86*	30	92	0.62	742.25	738	8	8.31E-03	59.1	
11	0	391.75*	387	190	1.47	777.80	770	14	1.08E-01	9.1	
12	0	410.36*	59	137	4.23	814.78	810	12	1.65E-02	41.9	
13	0	511.35*	15	201	2.67	1015.50	1008	17	4.29E-03	219.8	
14	0	661.63*	1454	187	1.72	1314.21	1307	17	4.04E-01	3.4	
15	0	682.32	20	44	1.31	1355.35	1352	7	5.51E-03	59.8	
16	0	689.00*	18	28	0.67	1368.62	1367	5	4.98E-03	50.8	
17	0	753.51*	15	50	1.43	1496.87	1494	8	4.25E-03	84.5	
18	0	813.97	54	196	11.04	1617.07	1607	29	1.49E-02	76.0	
19	0	897.75	370	187	1.84	1783.64	1775	19	1.03E-01	10.2	
20	0	920.03	18	90	1.01	1827.95	1821	10	5.10E-03	100.4	
21	0	1018.81*	16	89	1.35	2024.35	2020	11	4.36E-03	121.1	
22	0	1044.16	24	57	1.55	2074.77	2071	9	6.80E-03	58.8	
23	0	1133.39	91	120	11.57	2252.21	2235	37	2.52E-02	40.1	
24	0	1173.08*	1432	88	1.98	2331.15	2321	21	3.98E-01	3.1	
25	0	1332.22*	1308	39	2.24	2647.68	2638	22	3.63E-01	3.0	
26	0	1411.26	24	4	7.43	2804.91	2797	19	6.73E-03	29.3	
27	0	1574.30*	18	6	0.92	3129.28	3123	13	4.88E-03	38.4	
28	0	1629.15	18	4	4.66	3238.42	3233	14	5.00E-03	32.5	
29	0	1689.48	18	15	11.99	3358.46	3346	29	4.86E-03	66.9	
30	0	1835.85	237	9	2.87	3649.73	3641	19	6.60E-02	7.2	

Flag: "*" = Peak area was modified by background subtraction

VAX/VMS Nuclide Identification Report Generated

```

*****
*                               General Eng. Labs, LLC.                               *
*                               2040 Savage Road                                       *
*                               Charleston, SC 29414                                   *
*****
*                               DETECTOR DATA                                         *
*
* Configuration      : DKA300:[CANBERRA.GAMMA.ARCHIVE.GAMMA]G1201055609
* Acquisition date   : 11-APR-2006 14:31:28 Detector SN#      : 3941466
* Detector ID        : WELL                               Sensitivity      : 3.000
* Geometry           : CAN                               Energy tolerance: 2.000
* Elapsed live time  : 0 01:00:00.00                   Abundance limit  : 75.000
* Elapsed real time  : 0 01:00:02.86                   Half life ratio  : 8.000
*****
*                               SAMPLE DATA                                           *
*
* Sample date        : 21-MAR-2006 00:00:00 Nuclide Library  : FERMC
* Sample ID          : G1201055609                   Analyst initials: MJH1
* Batch Number       : 513802                         Sample Quantity  : 1.0000E+02 GRAM
* Recovery           : 1.00000                        Carrier Weight   : 0.00000
*****
*                               QC DATA                                              *
*
* Standard Weight    : 0.00000
* CALIB. DATE/TIME   : 14-DEC-2005 17:16:53 MS Isotope      :
* MSD DPM             : *****                      MSD Isotope       :
* LCS DPM             : 0.000                         LCS Isotope       :
* LCSD DPM           : 0.000                         LCSD Isotope      :
*****

```

Combined Activity-MDA Report

---- Identified Nuclides ----

Nuclide	Activity (pCi/GRAM)	Act error	MDA (pCi/GRAM)	
CO-57	2.962E+00	2.541E-01	1.602E-01	0.000E+00
CO-60	1.366E+01	8.254E-01	2.748E-01	0.000E+00
Y-88	3.785E+00	5.440E-01	2.499E-01	0.000E+00
CD-109	1.960E+02	8.169E+00	4.653E+00	0.000E+00
SN-113	2.320E+00	4.228E-01	3.431E-01	0.000E+00
SN-126	1.943E+01	8.102E-01	4.620E-01	0.000E+00
BA-137M	9.115E+00	6.215E-01	2.690E-01	0.000E+00
CS-137	9.635E+00	6.570E-01	2.844E-01	0.000E+00
CE-139	2.037E+00	2.299E-01	1.609E-01	0.000E+00
NP-237	5.707E+01	2.379E+00	1.360E+00	0.000E+00
AM-241	2.514E+01	1.131E+00	7.162E-01	0.000E+00
ANH-511	6.821E-02	2.998E-01	2.295E-01	0.000E+00

---- Non-Identified Nuclides ----

Nuclide	Key-Line Activity (pCi/GRAM)	K.L. Act error) Ided	MDA (pCi/GRAM)	
BE-7	-1.212E+00	1.813E+00	2.925E+00	0.000E+00 NOT IDENT.
NA-22	-9.751E-02	1.206E-01	1.893E-01	0.000E+00 NOT IDENT.
NA-24	0.000E+00	2.821E+09	0.000E+00	0.000E+00 SHORT HLIF
AL-26	3.999E-02	1.045E-01	2.233E-01	0.000E+00 FAIL ABUN
K-40	7.812E-02	1.178E+00	2.256E+00	0.000E+00 NOT IDENT.
SC-46	1.213E-01	2.475E-01	4.425E-01	0.000E+00 NOT IDENT.
V-48	-1.408E-01	5.440E-01	9.221E-01	0.000E+00 NOT IDENT.
CR-51	1.442E+00	1.676E+00	3.009E+00	0.000E+00 NOT IDENT.
MN-54	6.027E-04	2.085E-01	3.623E-01	0.000E+00 NOT IDENT.
CO-56	-2.890E-02	2.393E-01	4.125E-01	0.000E+00 NOT IDENT.
MN-56	0.000E+00	2.000E+41	0.000E+00	0.000E+00 SHORT HLIF
CO-58	-3.886E-02	2.440E-01	3.649E-01	0.000E+00 NOT IDENT.
FE-59	-3.310E-01	5.463E-01	8.951E-01	0.000E+00 NOT IDENT.
ZN-65	2.347E-01	4.725E-01	8.431E-01	0.000E+00 NOT IDENT.
SE-75	-1.478E-02	1.643E-01	2.819E-01	0.000E+00 FAIL ABUN

KR-85	2.958E+01	3.745E+01	5.876E+01	0.000E+00	NOT IDENT.
SR-85	1.623E-01	2.055E-01	3.225E-01	0.000E+00	NOT IDENT.
Y-91	5.549E-02	1.840E-01	3.170E-01	0.000E+00	NOT IDENT.
NB-94	1.014E-01	1.464E-01	2.715E-01	0.000E+00	NOT IDENT.
NB-95	-4.520E-02	2.425E-01	4.212E-01	0.000E+00	NOT IDENT.
NB-95M	-1.102E+01	2.193E+01	3.697E+01	0.000E+00	NOT IDENT.
ZR-95	2.777E-02	3.797E-01	5.891E-01	0.000E+00	NOT IDENT.
MO-99	-1.303E+01	2.069E+01	3.089E+01	0.000E+00	NOT IDENT.
TC-99M	0.000E+00	8.198E+24	0.000E+00	0.000E+00	SHORT HLIF
RU-103	1.536E-01	2.240E-01	3.939E-01	0.000E+00	NOT IDENT.
RH-106	1.304E+00	1.494E+00	2.795E+00	0.000E+00	FAIL ABUN
RU-106	1.750E+00	1.528E+00	2.896E+00	0.000E+00	NOT IDENT.
AG-108M	-5.856E-02	1.646E-01	2.720E-01	0.000E+00	NOT IDENT.
AG-110M	9.996E-02	2.200E-01	3.485E-01	0.000E+00	NOT IDENT.
CD-115	0.000E+00	3.871E+02	0.000E+00	0.000E+00	SHORT HLIF
SN-115	-5.335E+00	2.286E+01	3.886E+01	0.000E+00	NOT IDENT.
SN-117M	8.848E-02	2.480E-01	4.390E-01	0.000E+00	NOT IDENT.
TE-123M	5.940E-02	9.603E-02	1.717E-01	0.000E+00	NOT IDENT.
SB-124	5.839E-01	7.814E-01	6.100E-01	0.000E+00	FAIL ABUN
SB-125	-1.697E-01	4.356E-01	7.198E-01	0.000E+00	NOT IDENT.
TE-125M	6.479E-02	3.519E+01	5.763E+01	0.000E+00	NOT IDENT.
I-126	4.939E-01	1.257E+00	2.019E+00	0.000E+00	FAIL ABUN
SB-126	7.103E-03	9.462E-01	1.671E+00	0.000E+00	NOT IDENT.
SB-127	1.759E+01	2.943E+01	3.478E+01	0.000E+00	FAIL ABUN
I-131	1.598E-01	8.962E-01	1.540E+00	0.000E+00	NOT IDENT.
I-132	0.000E+00	1.980E+41	0.000E+00	0.000E+00	SHORT HLIF
TE-132	-1.316E+00	9.531E+00	1.636E+01	0.000E+00	NOT IDENT.
BA-133	2.602E-02	1.805E-01	3.103E-01	0.000E+00	NOT IDENT.
I-133	0.000E+00	4.933E+06	0.000E+00	0.000E+00	SHORT HLIF
CS-134	6.189E-02	2.042E-01	3.655E-01	0.000E+00	NOT IDENT.
CS-135	-3.873E-01	5.605E-01	9.308E-01	0.000E+00	NOT IDENT.
I-135	0.000E+00	1.618E+23	0.000E+00	0.000E+00	SHORT HLIF
CS-136	3.815E-01	9.761E-01	1.517E+00	0.000E+00	FAIL ABUN
BA-140	1.149E+00	1.753E+00	3.088E+00	0.000E+00	NOT IDENT.
LA-140	-7.316E-02	5.259E-01	9.584E-01	0.000E+00	FAIL ABUN
CE-141	2.065E-01	2.091E-01	3.818E-01	0.000E+00	NOT IDENT.
CE-143	0.000E+00	1.228E+04	0.000E+00	0.000E+00	SHORT HLIF
CE-144	3.181E-01	7.160E-01	1.139E+00	0.000E+00	NOT IDENT.
PM-144	-8.859E-03	1.518E-01	2.675E-01	0.000E+00	NOT IDENT.
PR-144	0.000E+00	2.000E+41	0.000E+00	0.000E+00	SHORT HLIF
PM-146	-8.325E-02	2.296E-01	3.782E-01	0.000E+00	NOT IDENT.
ND-147	9.074E-01	3.908E+00	6.709E+00	0.000E+00	FAIL ABUN
PM-147	0.000E+00	5.220E+05	7.620E+05	0.000E+00	FAIL ABUN
PM-149	0.000E+00	2.522E+03	0.000E+00	0.000E+00	SHORT HLIF
EU-152	-8.067E-03	3.816E-01	6.521E-01	0.000E+00	FAIL ABUN
GD-153	1.060E-01	2.532E-01	4.240E-01	0.000E+00	NOT IDENT.
EU-154	-3.320E-01	3.468E-01	5.274E-01	0.000E+00	FAIL ABUN
EU-155	1.283E-01	3.826E-01	6.353E-01	0.000E+00	FAIL ABUN
TB-160	2.393E-01	8.738E-01	1.543E+00	0.000E+00	FAIL ABUN
TM-171	6.076E+01	7.596E+01	1.283E+02	0.000E+00	FAIL ABUN
HF-181	2.032E-01	2.461E-01	4.337E-01	0.000E+00	FAIL ABUN
TA-182	-1.008E-01	6.469E-01	1.124E+00	0.000E+00	NOT IDENT.
IR-192	-1.369E-01	1.418E-01	2.298E-01	0.000E+00	NOT IDENT.
HG-203	2.506E-01	1.706E-01	3.130E-01	0.000E+00	NOT IDENT.
BI-207	-9.199E-02	2.988E-01	5.024E-01	0.000E+00	FAIL ABUN
TL-208	3.872E-02	1.778E-01	3.029E-01	0.000E+00	FAIL ABUN
BI-210	-7.908E+00	4.826E+00	7.666E+00	0.000E+00	NOT IDENT.
PB-210	-7.908E+00	4.826E+00	7.666E+00	0.000E+00	NOT IDENT.
BI-211	6.338E-02	7.888E-01	1.355E+00	0.000E+00	NOT IDENT.
PB-211	-1.111E+00	4.078E+00	6.810E+00	0.000E+00	NOT IDENT.
BI-212	-1.218E-02	1.279E+00	2.261E+00	0.000E+00	NOT IDENT.
PB-212	8.160E-02	1.980E-01	3.479E-01	0.000E+00	FAIL ABUN
BI-214	3.714E-02	3.081E-01	5.498E-01	0.000E+00	NOT IDENT.
PB-214	-9.536E-02	2.803E-01	4.694E-01	0.000E+00	FAIL ABUN
RN-219	3.045E-01	1.858E+00	3.181E+00	0.000E+00	NOT IDENT.
RA-223	-1.836E+00	2.553E+00	4.195E+00	0.000E+00	FAIL ABUN
RA-224	-1.716E+00	2.277E+00	3.786E+00	0.000E+00	NOT IDENT.
RA-226	3.714E-02	3.081E-01	5.498E-01	0.000E+00	NOT IDENT.
AC-227	-8.429E-02	1.464E+00	2.513E+00	0.000E+00	NOT IDENT.
TH-227	-8.293E-02	1.441E+00	2.472E+00	0.000E+00	FAIL ABUN
AC-228	1.208E-01	8.064E-01	1.405E+00	0.000E+00	NOT IDENT.
RA-228	1.208E-01	8.064E-01	1.405E+00	0.000E+00	NOT IDENT.
TH-228	8.308E-02	1.980E-01	3.481E-01	0.000E+00	NOT IDENT.
TH-229	-1.091E+00	1.607E+00	2.709E+00	0.000E+00	FAIL ABUN
TH-230	3.714E-02	3.081E-01	5.498E-01	0.000E+00	NOT IDENT.
PA-231	-3.053E-01	5.623E+00	9.646E+00	0.000E+00	NOT IDENT.
TH-231	-2.289E-02	6.492E-01	1.116E+00	0.000E+00	NOT IDENT.
TH-232	8.180E-02	1.938E-01	3.407E-01	0.000E+00	NOT IDENT.

PA-233	1.676E-01	2.444E-01	4.351E-01	0.000E+00	FAIL	ABUN
PA-234	1.112E+00	1.916E+00	3.418E+00	0.000E+00	FAIL	ABUN
PA-234M	-6.186E+00	2.510E+01	4.257E+01	0.000E+00	NOT	IDENT.
TH-234	-2.839E+00	3.428E+00	4.874E+00	0.000E+00	FAIL	ABUN
U-234	-3.309E-02	4.879E-01	8.349E-01	0.000E+00	NOT	IDENT.
U-235	1.838E-01	6.321E-01	1.121E+00	0.000E+00	FAIL	ABUN
U-238	-2.839E+00	3.428E+00	4.874E+00	0.000E+00	NOT	IDENT.
NP-239	1.236E-01	8.598E-01	1.254E+00	0.000E+00	NOT	IDENT.
AM-242	2.713E+00	7.612E+00	1.267E+01	0.000E+00	NOT	IDENT.
CM-247	-3.816E-03	1.667E-01	2.823E-01	0.000E+00	NOT	IDENT.
CF-249	-2.508E-02	2.041E-01	3.003E-01	0.000E+00	NOT	IDENT.
CF-251	4.912E-01	3.962E-01	7.271E-01	0.000E+00	NOT	IDENT.

```

*****
*                               GENERAL ENG. LABS, LLC.                               *
*                               2040 Savage Road                                       *
*                               Charleston, SC 29414                                   *
*****
Configuration      : DKA300:[CANBERRA.GAMMA.ARCHIVE.GAMMA]G1201055609.CNF;1
Sample date        : 21-MAR-2006 00:00:00 Acquisition date : 11-APR-2006 14:31:28
Sample ID          : G1201055609 Sample quantity      : 1.00000E+02 GRAM
Detector name      : WELL Detector geometry          : CAN
Elapsed live time  : 0 01:00:00.00 Elapsed real time: 0 01:00:02.86 0.1%
Energy tolerance   : 2.00000 KEV Analyst Initials    : MJH1
Abundance limit    : 75.00000 Sensitivity         : 3.00000
Batch ID           : 513802 Detector SN#          : 3941466
Matrix Spike DPM   : LCS DPM                          :
*****

```

Nuclide Line Activity Report

Nuclide Type:

Nuclide	Energy	Area	%Abn	%Eff	Uncorrected pCi/GRAM	Decay Corr pCi/GRAM	2-Sigma %Error
CO-57	122.06	1614	85.51*	5.056E+00	2.803E+00	2.962E+00	8.58
	136.47	239	10.47	4.892E+00	3.496E+00	3.695E+00	33.76
CO-60	1173.24	1432	99.90	8.068E-01	1.334E+01	1.344E+01	6.23
	1332.50	1308	99.98*	7.246E-01	1.356E+01	1.366E+01	6.04
Y-88	898.02	370	93.40	1.014E+00	2.934E+00	3.377E+00	20.49
	1836.01	237	99.38*	5.454E-01	3.289E+00	3.785E+00	14.37
CD-109	88.03	4854	3.79*	5.068E+00	1.897E+02	1.960E+02	4.17
SN-113	391.69	387	64.90*	2.198E+00	2.037E+00	2.320E+00	18.22
SN-126	64.28	-----	9.60	4.325E+00	-----	Line Not Found	-----
	86.94	4854	8.90	5.068E+00	8.080E+01	8.080E+01	4.17
	87.57	4854	37.00*	5.068E+00	1.943E+01	1.943E+01	4.17
BA-137M	661.65	1454	89.98*	1.332E+00	9.103E+00	9.115E+00	6.82
CS-137	661.66	1454	85.12*	1.332E+00	9.622E+00	9.635E+00	6.82
CE-139	165.85	873	80.35*	4.466E+00	1.826E+00	2.037E+00	11.29
PM-147	121.30	1614	0.00*	5.056E+00	5.991E+06	6.086E+06	8.58
NP-237	86.48	4854	12.60*	5.068E+00	5.707E+01	5.707E+01	4.17
	95.87	-----	2.60	5.140E+00	-----	Line Not Found	-----
AM-241	59.54	4879	35.90*	4.059E+00	2.514E+01	2.514E+01	4.50
ANH-511	511.00	15	100.00*	1.699E+00	6.821E-02	6.821E-02	439.53

Flag: "*" = Keyline

Total number of lines in spectrum 30
 Number of unidentified lines 10
 Number of lines tentatively identified by NID 20 66.67%

Nuclide Type :

Nuclide	Hlife	Decay	Uncorrected pCi/GRAM	Decay Corr pCi/GRAM	Decay Corr 2-Sigma Error	2-Sigma %Error	Flags
CO-57	270.90D	1.06	2.803E+00	2.962E+00	0.254E+00	8.58	
CO-60	5.27Y	1.01	1.356E+01	1.366E+01	0.083E+01	6.04	
Y-88	106.60D	1.15	3.289E+00	3.785E+00	0.544E+00	14.37	
CD-109	464.00D	1.03	1.897E+02	1.960E+02	0.082E+02	4.17	
SN-113	115.10D	1.14	2.037E+00	2.320E+00	0.423E+00	18.22	
SN-126	1.00E+05Y	1.00	1.943E+01	1.943E+01	0.081E+01	4.17	
BA-137M	30.17Y	1.00	9.103E+00	9.115E+00	0.622E+00	6.82	
CS-137	30.17Y	1.00	9.622E+00	9.635E+00	0.657E+00	6.82	
CE-139	137.66D	1.12	1.826E+00	2.037E+00	0.230E+00	11.29	
PM-147	2.62Y	1.02	5.991E+06	6.086E+06	0.522E+06	8.58	
NP-237	2.14E+06Y	1.00	5.707E+01	5.707E+01	0.238E+01	4.17	
AM-241	432.20Y	1.00	2.514E+01	2.514E+01	0.113E+01	4.50	
ANH-511	1.00E+09Y	1.00	6.821E-02	6.821E-02	29.98E-02	439.53	
Total Activity :			5.991E+06	6.086E+06			

Grand Total Activity : 5.991E+06 6.086E+06

Flags: "K" = Keyline not found "M" = Manually accepted
 "E" = Manually edited "A" = Nuclide specific abn. limit

It	Energy	Area	Bkgnd	FWHM	Channel	Left	Pw	Cts/Sec	%Err	%Eff	Flags
0	33.21	246	769	1.48	65.39	63	7	6.83E-02	39.7	1.69E+00	
0	36.87	129	814	2.01	72.65	70	8	3.57E-02	79.3	2.08E+00	
0	92.77	5	335	1.31	183.70	181	8	1.28E-03	****	5.12E+00	T
0	186.07	17	276	0.71	369.08	364	9	4.61E-03	****	4.17E+00	T
0	373.86	30	92	0.62	742.25	738	8	8.31E-03	****	2.30E+00	
0	410.36	59	137	4.23	814.78	810	12	1.65E-02	83.8	2.10E+00	T
0	682.32	20	44	1.31	1355.35	1352	7	5.51E-03	****	1.30E+00	
0	689.00	18	28	0.67	1368.62	1367	5	4.98E-03	****	1.28E+00	
0	753.51	15	50	1.43	1496.87	1494	8	4.25E-03	****	1.18E+00	T
0	813.97	54	196	11.04	1617.07	1607	29	1.49E-02	****	1.10E+00	T
0	920.03	18	90	1.01	1827.95	1821	10	5.10E-03	****	9.92E-01	T
0	1018.81	16	89	1.35	2024.35	2020	11	4.36E-03	****	9.09E-01	
0	1044.16	24	57	1.55	2074.77	2071	9	6.80E-03	****	8.90E-01	
0	1133.39	91	120	11.57	2252.21	2235	37	2.52E-02	80.2	8.31E-01	T
0	1411.26	24	4	7.43	2804.91	2797	19	6.73E-03	58.7	6.90E-01	
0	1574.30	18	6	0.92	3129.28	3123	13	4.88E-03	76.7	6.27E-01	
0	1629.15	18	4	4.66	3238.42	3233	14	5.00E-03	65.0	6.09E-01	
0	1689.48	18	15	11.99	3358.46	3346	29	4.86E-03	****	5.89E-01	T

Flags: "T" = Tentatively associated


```

*****
*                                     GENERAL ENG. LABS, LLC.                               *
*                                     2040 Savage Road                                   *
*                                     Charleston, SC 29414                             *
*****
*                                     DETECTOR DATA                                   *
*
* Configuration      : DKA300:[CANBERRA.GAMMA.ARCHIVE.GAMMA]G1201055609.CNF;1
* Acquisition date   : 11-APR-2006 14:31:28  Detector SN#      : 3941466
* Detector ID        : WELL                      Sensitivity       : 3.00000
* Geometry           : CAN                      Energy tolerance: 2.00000
* Elapsed live time  : 0 01:00:00.00           Abundance limit  : 75.00000
* Elapsed real time  : 0 01:00:02.86           Half life ratio  : 8.00000
*****
*                                     SAMPLE DATA                                   *
*
* Sample date        : 21-MAR-2006 00:00:00  Nuclide Library   : EPI
* Sample ID          : G1201055609           Analyst initials   : MJH1
* Batch Number       : 513802                Sample Quantity   : 1.00000E+02 GRAM
*****
*                                     QC DATA                                       *
*
* CALIB. DATE/TIME  : 14-DEC-2005 17:16:53.5MS Isotope       :
* MSD DPM           :                          MSD Isotope     :
* LCS DPM           :                          LCS Isotope     :
*****

```

Combined Activity-MDA Report

---- Identified Nuclides ----

Nuclide	Activity (pCi/GRAM)	Act error	MDA (pCi/GRAM)	MDA error	Act/MDA
CO-57	2.962E+00	2.541E-01	1.605E-01	0.000E+00	18.450
CO-60	1.366E+01	8.254E-01	2.771E-01	0.000E+00	49.311
Y-88	3.785E+00	5.440E-01	2.523E-01	0.000E+00	15.004
CD-109	1.960E+02	8.169E+00	4.660E+00	0.000E+00	42.052
SN-113	2.320E+00	4.228E-01	3.449E-01	0.000E+00	6.726
SN-126	1.943E+01	8.102E-01	4.626E-01	0.000E+00	42.011
BA-137M	9.115E+00	6.215E-01	2.708E-01	0.000E+00	33.660
CS-137	9.635E+00	6.570E-01	2.863E-01	0.000E+00	33.660
CE-139	2.037E+00	2.299E-01	1.614E-01	0.000E+00	12.615
NP-237	5.707E+01	2.379E+00	1.362E+00	0.000E+00	41.904
AM-241	2.514E+01	1.131E+00	7.165E-01	0.000E+00	35.090
ANH-511	6.821E-02	2.998E-01	2.309E-01	0.000E+00	0.295

---- Non-Identified Nuclides ----

Nuclide	Key-Line Activity (pCi/GRAM)	K.L. Ided	Act error	MDA (pCi/GRAM)	MDA error	Act/MDA
BE-7	-1.212E+00		1.813E+00	2.942E+00	0.000E+00	-0.412

---- Non-Identified Nuclides ----

Nuclide	Key-Line Activity (pCi/GRAM)	K.L. Ided	Act error	MDA (pCi/GRAM)	MDA error	Act/MDA
NA-22	-9.751E-02		1.206E-01	1.909E-01	0.000E+00	-0.511
AL-26	3.999E-02		1.045E-01	2.254E-01	0.000E+00	0.177
K-40	7.812E-02		1.178E+00	2.276E+00	0.000E+00	0.034
SC-46	1.213E-01		2.475E-01	4.458E-01	0.000E+00	0.272
V-48	-1.408E-01		5.440E-01	9.292E-01	0.000E+00	-0.151
CR-51	1.442E+00		1.676E+00	3.024E+00	0.000E+00	0.477
MN-54	6.027E-04		2.085E-01	3.650E-01	0.000E+00	0.002
CO-56	-2.890E-02		2.393E-01	4.155E-01	0.000E+00	-0.070
CO-58	-3.886E-02		2.440E-01	3.675E-01	0.000E+00	-0.106
FE-59	-3.310E-01		5.463E-01	9.023E-01	0.000E+00	-0.367
ZN-65	2.347E-01		4.725E-01	8.499E-01	0.000E+00	0.276
SE-75	-1.478E-02		1.643E-01	2.831E-01	0.000E+00	-0.052
KR-85	2.958E+01		3.745E+01	5.912E+01	0.000E+00	0.500
SR-85	1.623E-01		2.055E-01	3.244E-01	0.000E+00	0.500
Y-91	5.549E-02		1.840E-01	3.189E-01	0.000E+00	0.174
NB-94	1.014E-01		1.464E-01	2.734E-01	0.000E+00	0.371
NB-95	-4.520E-02		2.425E-01	4.241E-01	0.000E+00	-0.107
NB-95M	-1.102E+01		2.193E+01	3.711E+01	0.000E+00	-0.297
ZR-95	2.777E-02		3.797E-01	5.932E-01	0.000E+00	0.047
MO-99	-1.303E+01		2.069E+01	3.097E+01	0.000E+00	-0.421
RU-103	1.536E-01		2.240E-01	3.963E-01	0.000E+00	0.388
RH-106	1.304E+00		1.494E+00	2.813E+00	0.000E+00	0.464
RU-106	1.750E+00		1.528E+00	2.915E+00	0.000E+00	0.600
AG-108M	-5.856E-02		1.646E-01	2.735E-01	0.000E+00	-0.214
AG-110M	9.996E-02		2.200E-01	3.508E-01	0.000E+00	0.285
SN-115	-5.335E+00		2.286E+01	3.915E+01	0.000E+00	-0.136
SN-117M	8.848E-02		2.480E-01	4.403E-01	0.000E+00	0.201
TE-123M	5.940E-02		9.603E-02	1.722E-01	0.000E+00	0.345
SB-124	5.839E-01	+	7.814E-01	6.155E-01	0.000E+00	0.949
SB-125	-1.697E-01		4.356E-01	7.238E-01	0.000E+00	-0.234
TE-125M	6.479E-02		3.519E+01	5.775E+01	0.000E+00	0.001
I-126	4.939E-01		1.257E+00	2.032E+00	0.000E+00	0.243
SB-126	7.103E-03		9.462E-01	1.683E+00	0.000E+00	0.004
SB-127	1.759E+01		2.943E+01	3.502E+01	0.000E+00	0.502
I-131	1.598E-01		8.962E-01	1.548E+00	0.000E+00	0.103
TE-132	-1.316E+00		9.531E+00	1.642E+01	0.000E+00	-0.080
BA-133	2.602E-02		1.805E-01	3.118E-01	0.000E+00	0.083
CS-134	6.189E-02		2.042E-01	3.681E-01	0.000E+00	0.168
CS-135	-3.873E-01		5.605E-01	9.348E-01	0.000E+00	-0.414
CS-136	3.815E-01		9.761E-01	1.529E+00	0.000E+00	0.250
BA-140	1.149E+00		1.753E+00	3.106E+00	0.000E+00	0.370
LA-140	-7.316E-02		5.259E-01	9.670E-01	0.000E+00	-0.076
CE-141	2.065E-01		2.091E-01	3.828E-01	0.000E+00	0.539
CE-144	3.181E-01		7.160E-01	1.142E+00	0.000E+00	0.279
PM-144	-8.859E-03		1.518E-01	2.693E-01	0.000E+00	-0.033
PM-146	-8.325E-02		2.296E-01	3.803E-01	0.000E+00	-0.219
ND-147	9.074E-01		3.908E+00	6.750E+00	0.000E+00	0.134
PM-147	6.086E+06		5.220E+05	7.637E+05	0.000E+00	7.969

---- Non-Identified Nuclides ----

Nuclide	Key-Line Activity (pCi/GRAM)	K.L. Ided	Act error	MDA (pCi/GRAM)	MDA error	Act/MDA
EU-152	-8.067E-03		3.816E-01	6.553E-01	0.000E+00	-0.012
GD-153	1.060E-01		2.532E-01	4.247E-01	0.000E+00	0.250
EU-154	-3.320E-01		3.468E-01	5.318E-01	0.000E+00	-0.624
EU-155	1.283E-01		3.826E-01	6.365E-01	0.000E+00	0.202
TB-160	2.393E-01		8.738E-01	1.555E+00	0.000E+00	0.154
TM-171	6.076E+01		7.596E+01	1.284E+02	0.000E+00	0.473
HF-181	2.032E-01		2.461E-01	4.362E-01	0.000E+00	0.466
TA-182	-1.008E-01		6.469E-01	1.133E+00	0.000E+00	-0.089
IR-192	-1.369E-01		1.418E-01	2.309E-01	0.000E+00	-0.593
HG-203	2.506E-01		1.706E-01	3.143E-01	0.000E+00	0.797
BI-207	-9.199E-02		2.988E-01	5.063E-01	0.000E+00	-0.182
TL-208	3.872E-02		1.778E-01	3.048E-01	0.000E+00	0.127
BI-210	-7.908E+00		4.826E+00	7.664E+00	0.000E+00	-1.032
PB-210	-7.908E+00		4.826E+00	7.664E+00	0.000E+00	-1.032
BI-211	6.338E-02		7.888E-01	1.362E+00	0.000E+00	0.047
PB-211	-1.111E+00		4.078E+00	6.847E+00	0.000E+00	-0.162
BI-212	-1.218E-02		1.279E+00	2.276E+00	0.000E+00	-0.005
PB-212	8.160E-02		1.980E-01	3.493E-01	0.000E+00	0.234
BI-214	3.714E-02		3.081E-01	5.534E-01	0.000E+00	0.067
PB-214	-9.536E-02		2.803E-01	4.717E-01	0.000E+00	-0.202
RN-219	3.045E-01		1.858E+00	3.198E+00	0.000E+00	0.095
RA-223	-1.836E+00		2.553E+00	4.215E+00	0.000E+00	-0.436
RA-224	-1.716E+00		2.277E+00	3.802E+00	0.000E+00	-0.451
RA-226	3.714E-02		3.081E-01	5.534E-01	0.000E+00	0.067
AC-227	-8.429E-02		1.464E+00	2.523E+00	0.000E+00	-0.033
TH-227	-8.293E-02		1.441E+00	2.483E+00	0.000E+00	-0.033
AC-228	1.208E-01		8.064E-01	1.415E+00	0.000E+00	0.085
RA-228	1.208E-01		8.064E-01	1.415E+00	0.000E+00	0.085
TH-228	8.308E-02		1.980E-01	3.495E-01	0.000E+00	0.238
TH-229	-1.091E+00		1.607E+00	2.718E+00	0.000E+00	-0.401
TH-230	3.714E-02		3.081E-01	5.533E-01	0.000E+00	0.067
PA-231	-3.053E-01		5.623E+00	9.689E+00	0.000E+00	-0.032
TH-231	-2.289E-02		6.492E-01	1.121E+00	0.000E+00	-0.020
TH-232	8.180E-02		1.938E-01	3.421E-01	0.000E+00	0.239
PA-233	1.676E-01		2.444E-01	4.371E-01	0.000E+00	0.383
PA-234	1.112E+00		1.916E+00	3.444E+00	0.000E+00	0.323
PA-234M	-6.186E+00		2.510E+01	4.290E+01	0.000E+00	-0.144
TH-234	-2.839E+00		3.428E+00	4.877E+00	0.000E+00	-0.582
U-234	-3.309E-02		4.879E-01	8.387E-01	0.000E+00	-0.039
U-235	1.838E-01		6.321E-01	1.124E+00	0.000E+00	0.164
U-238	-2.839E+00		3.428E+00	4.877E+00	0.000E+00	-0.582
NP-239	1.236E-01		8.598E-01	1.256E+00	0.000E+00	0.098
AM-242	2.713E+00		7.612E+00	1.269E+01	0.000E+00	0.214
CM-247	-3.816E-03		1.667E-01	2.838E-01	0.000E+00	-0.013
CF-249	-2.508E-02		2.041E-01	3.019E-01	0.000E+00	-0.083
CF-251	4.912E-01		3.962E-01	7.294E-01	0.000E+00	0.673

```

*****
*
*                               General Engineering Labs, LLC
*                               2040 SAVAGE ROAD
*                               CHARLESTON ,SC 29417
*                               GROSS GAMMA REPORT
*
*****
*
* BATCH ID      : 513802                SAMPLE ID   : G1201055609
* ANALYST      : MJH1                   DETECTOR    : WELL
* SAMPLE DATE   : 21-MAR-2006 00:00:00.00  COUNT TIME  : 0 01:00:00.00
* ANALYSIS DATE: 11-APR-2006 14:31:28.48  SAMPLE ALQT: 100.000 GRAM
*
*****

```

```

GROSS GAMMA ACTIVITY (pCi/GRAM ) : 6.532E+01
GROSS GAMMA ERROR (pCi/GRAM ) : 1.219E+01
GROSS GAMMA MDA (pCi/GRAM ) : 2.310E+01
GROSS GAMMA DLC (pCi/GRAM ) : 1.130E+01

```

Radiochemistry Batch Checklist, Rev 4

Batch# 517517 Product: PG-210 Date: 4/10/06

Criteria:	Yes	No	Comments
Sample Solids are less than 100 mg for GAB.	NA		
If activity less 10* MDA, error is 150% or less of sample activity. If greater 10* MDA, error is 40% or less. If below the MDA, error is okay.	✓		
Instrument source check is within limits.	✓		
Instrument bkg check is within limits.	✓		
Method RDL has been met.	✓		
If duplicate activities are less 5* MDA, then rpd is 100% or less. If greater 5* MDA, then rpd 20% or less. If below the MDA, the rpd is 0%.			
Or meets the client's required RER acceptance criteria.	✓		
Tracer yield is 15-125% . Carrier yield 25-125%.			
Or meets the client's contract acceptance criteria.	✓		
Method blank is less than the RDL. (If rad samples, < 5% of lowest activity)	✓		
Sample was run within hold time.	✓		
Special requirements page checked	✓		
Sample was correctly preserved if required.	✓		
Smears Taken for Radioactive batches.	NA		
Method Spike and LCS are within 75-125% or meets the client's contract acceptance criteria.	✓		
No blank spaces on data forms. All lineouts initialed and dated. No transcription errors are apparent.	✓		
QC data entered into QC database.	✓		
Batch entered into Case Narrative.	✓		
Batch non-conformances completed If applicable.	NA		

General Engineering Laboratories

2/22/2005
Primary Review Performed By: J. Park 4/10/06

Secondary Review Performed By: KO 4/10/06

4/6 - 4/13
MWH
Page 160 of 587

Pb-210 Que Sheet

04/04/06

Batch #: 517517 Analyst: BXF1 Minimum Due Date 04/06/2006
 Spike Isotope: Pb210 Spike Code: ET491E Expiration Date: 11-11-06 Vol: 0.1-1 Bi Separation Date/Time: 4-5-06 / 1350
 LCS Isotope: Pb210 LCS Code: ET491E Expiration Date: 11-11-06 Vol: 0.1-1 Std Wt: 13.88
 Carrier: Pb Carrier Code: 1006364 Expiration Date: 1-19-03 Vol: 1ml Analytical Scale #: 38110047
 Prep Date: 4-4-06 Initials: BXF Pipet #: 449263 Balance #: 50410272 Witness: 5 x 54

Sample ID	Client Description	Type	Hazard Code	RDL	Client	Matrix	Collection Date & Time	Bkr#	Aliquot (mL or g)	Det	Initial Pb Weight (g)	Final Pb Weight (g)	Net Pb Weight (mg)
158048001	2603090024	SAMPLE	3 pCi/g	MWHL002	SOIL	07-MAR-06	1	2.507	1A		.0749	.0818	6.9
158048002	2603090027	SAMPLE	3 pCi/g	MWHL002	SOIL	07-MAR-06	2	2.317	1B		.0747	.0839	9.2
158048003	2603090028	SAMPLE	3 pCi/g	MWHL002	SOIL	07-MAR-06	3	2.603	1C		.0747	.0838	9.1
158048004	2603090026	SAMPLE	3 pCi/g	MWHL002	SOIL	07-MAR-06	4	2.328	1D		.0750	.0821	7.1
158048005	2603090029	SAMPLE	3 pCi/g	MWHL002	SOIL	07-MAR-06	5	2.438	2A		.0794	.0873	7.9
158269001	2603140361 M121-0.5	SAMPLE	3 pCi/g	MWHL002	SOIL	10-MAR-06	6	2.226	2B		.0799	.0891	9.2
158269002	2603140362 M121-5	SAMPLE	3 pCi/g	MWHL002	SOIL	10-MAR-06	7	2.494	2C		.0821	.0907	10.6
158269003	2603140364 M121-5D	SAMPLE	3 pCi/g	MWHL002	SOIL	10-MAR-06	8	2.318	2D		.0739	.0842	10.3
158269004	2603140365 M121-80	SAMPLE	3 pCi/g	MWHL002	SOIL	10-MAR-06	9	2.207	3B		.0763	.0826	6.3
1201063764	MB for batch 517517	MB	3 pCi/g	QC ACCOUNT	SOIL	07-MAR-06	10	2.603	3C		.0729	.0819	9
1201063765	2603090029(158048005DUP)	DUP	3 pCi/g	QC ACCOUNT	SOIL	07-MAR-06	11	2.266	3D		.0801	.0897	9.6
1201063766	2603090029(158048005MS)	MS	3 pCi/g	QC ACCOUNT	SOIL	07-MAR-06	12	2.391	4A		.0802	.0886	8.4
1201063767	LCS for batch 517517	LCS	3 pCi/g	QC ACCOUNT	SOIL	07-MAR-06	13	2.603	4B		.0762	.0871	10.9

hah

UP

Data Reviewed By:

Page 1 of 1

PIC S/N: 10751-4

Instrument Used (circle one): LB4100 S/N 8219

4/10/06



Weight/Loss Aliquot Correction Report



Select What to Correct Aliquot to

Dry Weight Wet Weight

Submit

Batch ID: 517517

Calculate Corrected Aliquot

Aliquot Correction to Dry Weight for Batch 517517

Sample Id	Aliquot (G)	Sample Type	Parent Sample Id	Loss (Dec)	Corrected Aliquot (G)
158048001	2.452	SAMPLE	NA	.0220	2.50741242
158048002	2.259	SAMPLE	NA	.0248	2.31651343
158048003	2.539	SAMPLE	NA	.0246	2.60313088
158048004	2.284	SAMPLE	NA	.0189	2.32803515
158048005	2.165	SAMPLE	NA	.1118	2.43753272
158269001	2.169	SAMPLE	NA	.0257	2.22623919
158269002	2.398	SAMPLE	NA	.0386	2.49436476
158269003	2.227	SAMPLE	NA	.0392	2.31803780
158269004	2.129	SAMPLE	NA	.0352	2.20686422
1201063764		MB	NA	NA	
1201063765	2.013	DUP	158048005	.1118	2.26639879
1201063766	2.124	MS	158048005	.1118	2.39137160
1201063767		LCS	NA	NA	

General Engineering Laboratories, LLC

JFD
4/10/06

Lead-210 Soil

Filename : PB210.XLS
 File type : Excel
 Version # : 1

Spike S/N : ET491-E
 Spike Exp Date : 11/11/2006
 Spike Activity (dpm/ml): 405.94
 Spike Volume Added: 0.1

Pipet, 0.1 ml Stdev : +/- 0.000701 ml
 Pipet, 0.5 ml Stdev : +/- 0.002564 ml
 Pipet, 1 ml Stdev : +/- 0.005480 ml

Procedure Code : GFC_PBS
 Parmname : Lead-210
 Required MDA: 3 pCi/G
 Halflife of Pb-210 : 22.26 years
 Halflife of Bi-210 : 5.013 days
 Batch counted on : PIC
 BKG Count time : 500 min

Batch : 517517
 Analyst : BXF1
 Prep Date : 4/4/2006
 Pb-210 Abundance : 1

Carrier S/N : 1006864
 Carrier Exp Date : 1/19/2008
 Carrier Volume Added: 1.0
 Carrier Weight (mg/ml): 13.88
 Carrier Weight StDev.: 0.05

Sample Characteristics			Carrier Calculations					
Sample ID	Sample Aliquot G	Sample Aliquot StDev.	Sample Date/Time	Carrier Weight (Standard)	Net Weight (Sample)	Net Weight StDev.	Carrier Aliquot (mL)	Carrier Aliquot StDev.
158048001	2.507	3.4796E-03	3/7/2006 9:10	13.88	6.90	0.036986	1.0	0.005480
158048002	2.317	3.4600E-03	3/7/2006 10:10	13.88	9.20	0.046872	1.0	0.005480
158048003	2.603	3.4895E-03	3/7/2006 11:45	13.88	9.10	0.046442	1.0	0.005480
158048004	2.328	3.4611E-03	3/7/2006 9:30	13.88	7.10	0.037846	1.0	0.005480
158048005	2.438	3.4725E-03	3/7/2006 12:45	13.88	7.90	0.041284	1.0	0.005480
158269001	2.226	3.4505E-03	3/10/2006 7:46	13.88	9.20	0.046872	1.0	0.005480
158269002	2.494	3.4782E-03	3/10/2006 7:55	13.88	10.60	0.052889	1.0	0.005480
158269003	2.318	3.4601E-03	3/10/2006 12:00	13.88	10.30	0.051599	1.0	0.005480
158269004	2.207	3.4486E-03	3/10/2006 12:00	13.88	6.30	0.034407	1.0	0.005480
1201063764	2.603	3.4895E-03	4/4/2006 0:00	13.88	9.00	0.046012	1.0	0.005480
1201063765	2.266	3.4547E-03	3/7/2006 12:45	13.88	9.60	0.048591	1.0	0.005480
1201063766	2.391	3.4676E-03	3/7/2006 12:45	13.88	8.40	0.043433	1.0	0.005480
1201063767	2.603	3.4895E-03	4/4/2006 0:00	13.88	10.90	0.054178	1.0	0.005480

Handwritten notes: 5/1/06, 7/04/10/06

Count Raw Data														
Detector ID	Counting Time	Gross Counts		Gross Beta CPM	Weekly Bkg		Detector Efficiency	Detector Error	Count Start Date/Time	Bi-210 Separation Date/Time	Bi-210 Ingrowth	Pb-210 Decay	Sample Recovery %	Sample Recovery Error %
		Alpha	Beta		CPM	Count Time								
1A	60	7	37	0.617	0.422	500	0.3697	0.00600	4/9/2006 9:57	4/5/2006 13:50	0.414	0.997	49.71%	1.00%
1B	60	3	20	0.333	0.362	500	0.3436	0.00409	4/9/2006 9:57	4/5/2006 13:50	0.414	0.997	66.28%	0.97%
1C	60	1	27	0.450	0.434	500	0.3483	0.00344	4/9/2006 9:57	4/5/2006 13:50	0.414	0.997	65.56%	0.98%
1D	60	3	23	0.383	0.354	500	0.3660	0.00511	4/9/2006 9:57	4/5/2006 13:50	0.414	0.997	51.15%	1.00%
2A	60	5	39	0.650	0.406	500	0.3604	0.00349	4/9/2006 9:57	4/5/2006 13:50	0.414	0.997	56.92%	0.99%
2B	60	2	31	0.517	0.242	500	0.3492	0.00383	4/9/2006 9:57	4/5/2006 13:50	0.414	0.997	66.28%	0.97%
2C	60	2	19	0.317	0.350	500	0.3335	0.00575	4/9/2006 9:58	4/5/2006 13:50	0.414	0.997	76.37%	0.96%
2D	60	8	33	0.550	0.458	500	0.3416	0.00479	4/9/2006 9:58	4/5/2006 13:50	0.414	0.997	74.21%	0.97%
3B	60	9	24	0.400	0.382	500	0.3655	0.00655	4/9/2006 9:58	4/5/2006 13:50	0.414	0.997	45.39%	1.01%
3C	60	3	29	0.483	0.434	500	0.3441	0.00535	4/9/2006 9:57	4/5/2006 13:50	0.414	1.000	64.84%	0.98%
3D	60	1	27	0.450	0.416	500	0.3403	0.00464	4/9/2006 9:57	4/5/2006 13:50	0.414	0.997	69.16%	0.97%
4A	60	4	207	3.450	0.392	500	0.3535	0.00744	4/9/2006 9:57	4/5/2006 13:50	0.414	0.997	60.52%	0.98%
4B	60	6	231	3.850	0.454	500	0.3363	0.00196	4/9/2006 9:57	4/5/2006 13:50	0.414	1.000	78.53%	0.96%

Handwritten signature

Results		MDA	Sample Act. Conc.	Sample Act. Error	Net Count Rate	Net Count Rate Error	2 SIGMA Counting Uncertainty	2 SIGMA Total Prop. Uncertainty	Sample QC	Sample Type	RPD	RER	Nominal	Recovery
Decision Level pCi/G	Critical Level pCi/G	pCi/G			Rate	Rate Error	Uncertainty	Uncertainty						
0.6553	0.4626	1.0322	0.4616	0.5419	0.1947	0.1055	0.4901	0.4902		SAMPLE				
0.5299	0.3741	0.8416	-0.0593	2.7643	-0.0287	0.0792	0.3216	0.3216		SAMPLE				
0.5150	0.3636	0.8100	0.0294	5.7173	0.0160	0.0915	0.3295	0.3295		SAMPLE				
0.6343	0.4478	1.0086	0.0735	2.8719	0.0293	0.0842	0.4138	0.4138		SAMPLE				
0.5921	0.4180	0.9345	0.5330	0.4424	0.2440	0.1079	0.4620	0.4621		SAMPLE				
0.4436	0.3132	0.7220	0.5822	0.3474	0.2747	0.0954	0.3962	0.3964		SAMPLE				
0.4327	0.3055	0.6884	-0.0573	2.3195	-0.0333	0.0773	0.2605	0.2605		SAMPLE				
0.5350	0.3777	0.8392	0.1710	1.0915	0.0920	0.1004	0.3657	0.3658		SAMPLE				
0.7841	0.5536	1.2417	0.0537	4.7890	0.0180	0.0862	0.5039	0.5039		SAMPLE				
0.5259	0.3713	0.8272	0.0926	1.9149	0.0493	0.0945	0.3474	0.3475		MB				
0.5620	0.3967	0.8859	0.0696	2.6847	0.0340	0.0913	0.3664	0.3664	158048005	DUP	0.0%		7.67	85.2%
0.5688	0.4016	0.8994	6.5304	0.0799	3.0580	0.2414	1.0105	1.0229	158048005	MS			7.02	76.6%
0.4544	0.3208	0.7132	5.3840	0.0758	3.3960	0.2551	0.7927	0.7995		LCS				

5/4/10
H/F

SampleID	Instr	Time	Alpha	Beta	Count Start Time	Count End Time
158048001	1A	60	7	37	4/9/2006 9:57	4/9/2006 10:57
158048002	1B	60	3	20	4/9/2006 9:57	4/9/2006 10:57
158048003	1C	60	1	27	4/9/2006 9:57	4/9/2006 10:57
158048004	1D	60	3	23	4/9/2006 9:57	4/9/2006 10:57
158048005	2A	60	5	39	4/9/2006 9:57	4/9/2006 10:57
158269001	2B	60	2	31	4/9/2006 9:57	4/9/2006 10:57
158269002	2C	60	2	19	4/9/2006 9:58	4/9/2006 10:58
158269003	2D	60	8	33	4/9/2006 9:58	4/9/2006 10:58
158269004	3B	60	9	24	4/9/2006 9:58	4/9/2006 10:58
1201063764	3C	60	3	29	4/9/2006 9:57	4/9/2006 10:57
1201063765	3D	60	1	27	4/9/2006 9:57	4/9/2006 10:57
1201063766	4A	60	4	207	4/9/2006 9:57	4/9/2006 10:57
1201063767	4B	60	6	231	4/9/2006 9:57	4/9/2006 10:57

off
4/10/06

Batch#: 521637

Client: MWHL

Date: 4/21/06

Criteria:	Yes	No	Comments
Calibration percent discrepancy is less than or equal to 10% (positive or negative).	✓		
Calibration R2 is greater than or equal to 0.99.	✓		
All calibration standard and sample lifetimes are 150-350us.	✓	✓	see narrative
All calibration standard and sample R2s are greater than or equal to 0.96.	✓		
All reference intensity ratios are between 0.8 and 1.2.	✓		
All reference lifetimes are 150-350us.	✓		
CRDL has been met.	✓		
All CCVs are 90-110% of known value.	✓		
One of the CCVs is a concentration used during calibration, and the other is not.	✓		
Method blank activity is less than the CRDL.	✓		
LCS, LCSD, and method spike (if applicable) recovery is 75-125%.	✓		
Special requirements page has been reviewed.	✓		
No blank spaces on data forms. All lineouts initialed and dated. No transcription errors are apparent.	✓		
Batch entered into a case narrative.	✓		
Batch entered into an NCR (if applicable).	MA		

Primary Review Performed By: [Signature] 4/21/06

Secondary Review Performed By: [Signature] 4/21/06

Total Uranium Que Sheet

Batch #: 521637
 Analyst: DRS1
 Spike Isotope: Natural U Spike Code: 0873 4/17/06
 LCS Isotope: Natural U LCS Code: 0873 4/17/06
 LCS Code: 0873 4/17/06
 Minimum Due Date: 04/08/2006
 Expiration Date: 06/17/07
 Vol: 2.0
 Nom Conc: 9.43
 Nom Conc: 10.0 / 1.0
 Comments:

Witness: 4/14/06 KD
 Initials: DRS Pipet ID: 56228507/1007205
(C-2)

Sample I	Client Description	Type	Hazard Code	Min CRDL	Matrix	Client	Bkr#	Sample Aliquot (g or mL)	Aliquot for Analysis (mL)
158269001	2603140361 M121-0.5	SAMPLE		1 ug/g	SOIL	MWHL002	1	0.105 : 50	(
158269002	2603140362 M121-5	SAMPLE		1 ug/g	SOIL	MWHL002	2	0.104 : 50	(
158269003	2603140364 M121-5D	SAMPLE		1 ug/g	SOIL	MWHL002	3	0.106 : 50	(
158269004	2603140365 M121-80	SAMPLE		1 ug/g	SOIL	MWHL002	4	0.107 : 50	(
158270001	2603100106 M118-0.5	SAMPLE		1 ug/g	SOIL	MWHL002	5	0.104 : 50	(
158270002	2603100107 M118-5	SAMPLE		1 ug/g	SOIL	MWHL002	6	0.107 : 50	(
158437001	2603150347 M119-0.5	SAMPLE		1 ug/g	SOIL	MWHL002	7	0.107 : 50	(
158437002	2603150349 M119-0.5D	SAMPLE		1 ug/g	SOIL	MWHL002	8	0.105 : 50	(
158437003	2603150350 M119-5	SAMPLE		1 ug/g	SOIL	MWHL002	9	0.104 : 50 <u>4/17/06</u>	(
158437004	2603150352 M119-50	SAMPLE		1 ug/g	SOIL	MWHL002	10	0.104 : 50 100	(
158438001	2603150303 M116-0.5	SAMPLE		1 ug/g	SOIL	MWHL002	11	0.105 : 50 100	(
158438002	2603150304 M116-0.5D	SAMPLE		1 ug/g	SOIL	MWHL002	12	0.105 : 50 100	(
158438003	2603150305 M116-5	SAMPLE		1 ug/g	SOIL	MWHL002	13	0.107 : 50	(
158438004	2603150307 M117-0.5	SAMPLE		1 ug/g	SOIL	MWHL002	14	0.105 : 50 <u>4/17/06</u>	(
158438005	2603150308 M117-5	SAMPLE		1 ug/g	SOIL	MWHL002	15	0.107 : 50 100	(
1201073174	MB for batch 521637	MB		1 ug/g	SOIL	QC ACCOUNT	16	0.100 : 50 <u>4/17/06</u>	(
1201073175	2603140361 M121-0.5(158269001)DDUP	DDUP		1 ug/g	SOIL	QC ACCOUNT	17	0.105 : 50 100	(
1201073176	2603140361 M121-0.5(158269001)MMS	MMS		1 ug/g	SOIL	QC ACCOUNT	18	0.106 : 50 100	(
1201073177	LCS for batch 521637	LCS		1 ug/g	SOIL	QC ACCOUNT	19	0.100 : 50	(
1201073178	LCS for batch 521637	LCS		1 ug/g	SOIL	QC ACCOUNT	20	0.100 : 50	(

Instrument Used (circle one): KPA-10 S/N 89-05050-0035, KPA-10A S/N 89-05040-025, KPA-11 S/N 94-45050-064
 Data Reviewed By: [Signature]
 Page 1 of 1
 General Engineering Laboratories, Radiochemistry Division



Weight/Loss Aliquot Correction Report



Select What to Correct Aliquot to

Dry Weight Wet Weight

Submit

Batch ID: 521637

Calculate Corrected Aliquot

Aliquot Correction to Dry Weight for Batch 521637

Sample Id	Aliquot (G)	Sample Type	Parent Sample Id	Loss (Dec)	Corrected Aliquot (G)
158269001	0.102	SAMPLE	NA	.0257	0.10469174
158269002	0.100	SAMPLE	NA	.0386	0.10401854
158269003	0.102	SAMPLE	NA	.0392	0.10616967
158269004	0.103	SAMPLE	NA	.0352	0.10676703
158270001	0.101	SAMPLE	NA	.0280	0.10391292
158270002	0.104	SAMPLE	NA	.0280	0.10700680
158437001	0.104	SAMPLE	NA	.0244	0.10660661
158437002	0.102	SAMPLE	NA	.0279	0.10492749
158437003	0.101	SAMPLE	NA	.0274	0.10384607
158437004	0.101	SAMPLE	NA	.0304	0.10416666
158438001	0.103	SAMPLE	NA	.0227	0.10539777
158438002	0.102	SAMPLE	NA	.0263	0.10476009
158438003	0.103	SAMPLE	NA	.0328	0.10650055
158438004	0.103	SAMPLE	NA	.0213	0.10525201
158438005	0.104	SAMPLE	NA	.0253	0.10670074
1201073174		MB	NA	NA	
1201073175	0.102	DUP	158269001	.0257	0.10469174
1201073176	0.103	MS	158269001	.0257	0.10571813
1201073177		LCS	NA	NA	
1201073178		LCSD	NA	NA	

MPK

[Signature]

General Engineering Laboratories, LLC

Uranium Soil

Filename : TOTU.XLS
 File type : Excel
 Version # : 1

Spike S/N : 0873
 Spike Exp Date : 6/17/2007
 Spike Activity (ug/L): 500.00
 Spike Volume Added(mL): 2.0

LCS S/N : 0873
 LCS Exp Date : 6/17/2007
 LCS Activity (ug/L): 500.00
 LCS Volume Added(mL): 2.0

Batch : 521637

Analyst : DRS1

Prep Date : 4/14/2006

Nat-U Abundance : 1

Procedure Code : KPATOTUS
 Parmname : Total Uranium

Calibration Date : 4/21/2006 10:36:21

Calibration Due Date : 4/22/2006 10:36:21

Pipet, 0.1 ml Stdev : +/- 0.000701 ml
 Pipet, 0.5 ml Stdev : +/- 0.002564 ml
 Pipet, 1.0 ml Stdev : +/- 0.005480 ml
 Pipet, 5.0 ml Stdev : +/- 0.025729 ml

Batch counted on : KPA11AUTO1

Sample Characteristics

KPA Raw Data

Sample ID	Initial Aliquot G	Initial Sample StDev	Final Aliquot L	Final Aliquot StDev	Sample Counted mL	Sample Counted StDev	Sample Date/Time	Analysis Range	Intensity	Lifetime (us)	R^2
158269001	0.105	3.2300E-03	0.050	2.2223E-04	1.000	5.4802E-03	3/10/2006 7:46	Low	28614.670	151.5168	0.9939
158269002	0.104	3.2299E-03	0.050	2.2223E-04	1.000	5.4802E-03	3/10/2006 7:55	Low	34701.800	161.5325	0.9988
158269003	0.106	3.2301E-03	0.050	2.2223E-04	1.000	5.4802E-03	3/10/2006 12:00	Low	30768.590	156.9704	0.9988
158269004	0.107	3.2302E-03	0.050	2.2223E-04	1.000	5.4802E-03	3/10/2006 12:00	Low	30057.580	152.0697	0.9982
158270001	0.104	3.2299E-03	0.050	2.2223E-04	1.000	5.4802E-03	3/8/2006 11:10	Low	23422.450	161.8889	0.9931
158270002	0.107	3.2302E-03	0.050	2.2223E-04	1.000	5.4802E-03	3/8/2006 11:20	Low	29697.340	163.0796	0.9936
158437001	0.107	3.2302E-03	0.050	2.2223E-04	1.000	5.4802E-03	3/14/2006 7:30	Low	20928.610	168.3646	0.9869
158437002	0.105	3.2300E-03	0.050	2.2223E-04	1.000	5.4802E-03	3/14/2006 12:00	Low	27183.960	150.7522	0.9962
158437003	0.104	3.2299E-03	0.050	2.2223E-04	1.000	5.4802E-03	3/14/2006 7:35	Low	24490.810	163.1401	0.9925
158437004	0.104	3.2299E-03	0.100	4.3713E-04	1.000	5.4802E-03	3/14/2006 9:00	Low	48143.040	177.4590	0.9999
158438001	0.105	3.2300E-03	0.100	4.3713E-04	1.000	5.4802E-03	3/11/2006 11:55	Low	27306.000	168.7448	0.9993
158438002	0.105	3.2300E-03	0.100	4.3713E-04	1.000	5.4802E-03	3/11/2006 12:05	Low	26756.080	177.7031	0.9996
158438003	0.107	3.2302E-03	0.050	2.2223E-04	1.000	5.4802E-03	3/11/2006 12:05	Low	26025.400	151.7966	0.9986
158438004	0.105	3.2300E-03	0.050	2.2223E-04	1.000	5.4802E-03	3/11/2006 7:38	Low	17226.710	183.7544	0.9691
158438005	0.107	3.2302E-03	0.100	4.3713E-04	1.000	5.4802E-03	3/11/2006 7:48	Low	23974.620	180.5077	0.9997
1201073174	0.100	4.3713E-04	0.050	2.2223E-04	1.000	5.4802E-03	4/14/2006 0:00	Low	728.844	312.1344	0.9892
1201073175	0.105	3.2300E-03	0.100	4.3713E-04	1.000	5.4802E-03	3/10/2006 7:46	Low	28723.490	178.3609	0.9997
1201073176	0.106	3.2301E-03	0.100	4.3713E-04	1.000	5.4802E-03	3/10/2006 7:46	Low	99722.360	169.4966	0.9987
1201073177	0.100	4.3713E-04	0.050	2.2223E-04	1.000	5.4802E-03	4/14/2006 0:00	High	1061.044	292.8112	0.9986
1201073178	0.100	4.3713E-04	0.050	2.2223E-04	1.000	5.4802E-03	4/14/2006 0:00	Low	10101.030	305.5775	0.9998

Ref Ratio	Results (ug/L)	Error (ug/L)	Count Date/Time	Dilution Corrected Results			Results (pCi)				pCi/ug= 0.67			1 SIGMA	
				KPA Result ug/G	KPA Error ug/G	MDA pCi/G	Decision Level pCi/G	Critical Level pCi/G	Sample Act. Conc. pCi/G	Sample Act. Error pCi/G	Counting Uncertainty	Total Prop. Uncertainty			
0.9835	5.1510	0.1688	4/19/2006 10:06	2.4528	0.0804	0.0726	0.0514	0.0363	1.6434	0.0220	0.1056	0.4687			
0.9676	6.2798	0.1069	4/19/2006 10:08	3.0191	0.0514	0.0738	0.0519	0.0366	2.0228	0.0114	0.0675	0.5688			
0.9653	5.5504	0.0972	4/19/2006 10:10	2.6181	0.0458	0.0719	0.0509	0.0360	1.7541	0.0117	0.0602	0.4889			
0.9649	5.4185	0.1095	4/19/2006 10:12	2.5320	0.0512	0.0712	0.0504	0.0356	1.6965	0.0135	0.0672	0.4719			
0.9740	4.1881	0.1367	4/19/2006 10:14	2.0135	0.0657	0.0733	0.0519	0.0366	1.3491	0.0219	0.0863	0.3864			
0.9750	5.3517	0.1678	4/19/2006 10:16	2.5008	0.0784	0.0712	0.0504	0.0356	1.6755	0.0210	0.1030	0.4727			
0.9829	3.7256	0.1570	4/19/2006 10:18	1.7410	0.0734	0.0726	0.0504	0.0356	1.1664	0.0282	0.0963	0.3353			
0.9864	4.8857	0.1307	4/19/2006 10:21	2.3265	0.0622	0.0726	0.0514	0.0363	1.5588	0.0179	0.0817	0.4408			
0.9854	4.3862	0.1472	4/19/2006 10:23	2.1088	0.0708	0.0733	0.0519	0.0366	1.4129	0.0225	0.0929	0.4053			
0.9240	6.6969	0.0786	4/20/2006 15:03	6.4393	0.0756	0.1466	0.1038	0.0733	4.3143	0.0079	0.0992	1.2140			
0.9236	3.8265	0.0543	4/20/2006 15:06	3.6443	0.0518	0.1452	0.1028	0.0726	2.4417	0.0095	0.0680	0.6850			
0.9274	3.7508	0.0484	4/20/2006 15:08	3.5722	0.0461	0.1452	0.1028	0.0726	2.3933	0.0086	0.0606	0.6708			
0.9914	4.6708	0.0860	4/19/2006 10:31	2.1826	0.0402	0.0712	0.0504	0.0356	1.4624	0.0123	0.0528	0.4060			
0.9870	3.0392	0.1787	4/19/2006 10:33	1.4472	0.0851	0.0726	0.0514	0.0363	0.9696	0.0394	0.1117	0.2917			
0.9312	3.3676	0.0417	4/20/2006 15:11	3.1473	0.0390	0.1425	0.1009	0.0712	2.1087	0.0083	0.0512	0.5855			
0.9901	-0.0203	-0.0005	4/19/2006 10:37	-0.0101	-0.0002	0.0762	0.0540	0.0381	-0.0068	0.0153	0.0003	0.0004			
0.9340	4.0218	0.0498	4/20/2006 15:13	3.8303	0.0474	0.1452	0.1028	0.0726	2.5663	0.0083	0.0623	0.7191			
0.9343	13.8022	0.2222	4/20/2006 15:15	13.0209	0.2096	0.1438	0.1018	0.0719	8.7240	0.0108	0.2753	2.4397			
1.0093	16.0709	0.5189	4/19/2006 10:46	8.0355	0.2594	0.0762	0.0540	0.0381	5.3838	0.0216	0.3407	0.4289			
0.9904	1.7177	0.0201	4/19/2006 10:48	0.8589	0.0100	0.0762	0.0540	0.0381	0.5754	0.0078	0.0132	0.0308			

Handwritten signature

MDA Study Information

Effective Date: 4/1/2006

Expiration Date: 7/1/2006

Average: 1.040000000

StDev.: 0.048900000

Results (ug) Decision Level ug/G	Critical Level ug/G	MDA ug/G	Sample Act. Conc. ug/G	Sample Act. Error ug/G	2 SIGMA Counting Uncertainty	2 SIGMA Total Prop. Uncertainty	Sample QC	Sample Type	RPD	RER	Nominal	Recovery
0.0767	0.0542	0.1083	2.4528	0.0328	0.1576	0.6996		SAMPLE				
0.0775	0.0547	0.1094	3.0191	0.0170	0.1007	0.8489		SAMPLE				
0.0760	0.0537	0.1073	2.6181	0.0175	0.0898	0.7297		SAMPLE				
0.0753	0.0532	0.1063	2.5320	0.0202	0.1003	0.7043		SAMPLE				
0.0775	0.0547	0.1094	2.0135	0.0326	0.1289	0.5767		SAMPLE				
0.0753	0.0532	0.1063	2.5008	0.0314	0.1537	0.7054		SAMPLE				
0.0753	0.0532	0.1063	1.7410	0.0421	0.1438	0.5004		SAMPLE				
0.0767	0.0542	0.1083	2.3265	0.0267	0.1219	0.6579		SAMPLE				
0.0775	0.0547	0.1094	2.1088	0.0336	0.1387	0.6049		SAMPLE				
0.1549	0.1094	0.2188	6.4393	0.0117	0.1481	1.8120		SAMPLE				
0.1535	0.1083	0.2167	3.6443	0.0142	0.1014	1.0223		SAMPLE				
0.1535	0.1083	0.2167	3.5722	0.0129	0.0904	1.0012		SAMPLE				
0.0753	0.0532	0.1063	2.1826	0.0184	0.0788	0.6060		SAMPLE				
0.0767	0.0542	0.1083	1.4472	0.0588	0.1668	0.4353		SAMPLE				
0.1506	0.1063	0.2126	3.1473	0.0124	0.0764	0.8739		SAMPLE				
0.0806	0.0569	0.1138	-0.0101	0.0229	0.0005	0.0007		MB				
0.1535	0.1063	0.2167	3.8303	0.0124	0.0930	1.0732	158269001	DUP	43.8%	2.1073	9.43	112.0%
0.1520	0.1073	0.2146	13.0209	0.0161	0.4109	3.6413	158269001	MS			10.00	80.4%
0.0806	0.0569	0.1138	8.0355	0.0323	0.5085	0.6402		LCS			1.00	85.9%
0.0806	0.0569	0.1138	0.8589	0.0117	0.0197	0.0460		LCS	161.4%	21.9166	1.00	85.9%

Handwritten signature

Sample-ID 1.0 ug/L	Sample-Description ConcTst	Reference-ReferenceRatio	Sample-Lifetime	Sample-RV2	Sample-AnalysisDate	Analysis-Range	Sample-Intercept	Result-AnalyticalResult	Result-AnalyticalUncertainty	Standard 1.0 ug/L	Recovery #VAL/UEI
2	CChkStd	1.015179	304.8153	0.999527	4/19/2006 8:00	Low	5791.411	1.970959	0	2	99%
5	CChkStd	0.9863993	305.553	0.9998211	4/19/2006 9:20	Low	11466.49	2.29E-02	2.99E-02	2	99%
50	CChkStd	0.9877033	312.284	0.999953	4/19/2006 9:23	Low	28480.97	5.126175	5.84E-02	5	103%
250	CChkStd	0.9964994	323.7815	0.9996001	4/19/2006 9:25	High	3221.531	48.97681	1.546921	50	98%
158269001	CChkStd	0.996206	304.4304	0.9998451	4/19/2006 9:27	High	16614.59	253.6043	7.979593	250	101%
158269002	5216371	0.9834651	151.5168	0.9938796	4/19/2006 10:06	Low	28614.67	5.15097	0.1688437		
158269003	5216372	0.9675801	161.5325	0.9988071	4/19/2006 10:08	Low	34701.8	6.279786	0.1068649		
158269004	5216373	0.9653266	156.9704	0.9987552	4/19/2006 10:10	Low	30768.59	5.550398	9.72E-02		
158270001	5216374	0.9649115	152.0697	0.9981679	4/19/2006 10:12	Low	30057.58	5.418547	0.1094643		
158270002	5216375	0.9739848	161.6889	0.9930981	4/19/2006 10:14	Low	23422.45	4.188107	0.1367392		
158437001	5216376	0.9749774	163.0796	0.9935971	4/19/2006 10:16	Low	29697.34	5.351743	0.1677889		
158437002	5216377	0.962896	168.3646	0.9869373	4/19/2006 10:18	Low	20928.61	3.725644	0.1569821		
158437003	5216378	0.985447	150.7522	0.9962325	4/19/2006 10:21	Low	27183.96	4.885654	0.1306657		
158438001	5216379	0.985447	163.1401	0.9925245	4/19/2006 10:23	Low	24490.81	4.386229	0.1472173		
158438002	52163710	0.9913704	149.8335	0.9903251	4/19/2006 10:25	Low	53639.21	9.791595	0.2623931		
158438003	52163711	1.000688	144.22	0.996124	4/19/2006 10:27	Low	25219.65	4.521387	0.1844021		
158438004	52163712	0.9913979	151.7966	0.9986246	4/19/2006 10:29	Low	28284.46	5.089734	0.1428854		
158438005	52163713	0.9869763	183.7544	0.9691334	4/19/2006 10:31	Low	26025.4	4.670806	8.60E-02		
1201073174	52163714	0.993068	225.6618	0.9724522	4/19/2006 10:33	Low	17226.71	3.039151	0.1786634		
1201073175	52163715	0.9900799	312.1344	0.9892274	4/19/2006 10:35	Low	25613.02	4.594334	0.2100728		
1201073176	52163716	0.9936023	148.5711	0.9934931	4/19/2006 10:37	Low	728.8437	-2.03E-04	-4.63E-04		
1201073177	52163717	1.015951	146.188	0.989579	4/19/2006 10:39	Low	27978	5.032904	0.1725128		
1201073178	52163718	1.009287	292.8112	0.9895875	4/19/2006 10:41	High	1003.69	15.19803	0.8081281		
2	CChkStd	0.9904416	305.5775	0.9997729	4/19/2006 10:43	High	1061.044	16.07093	0.5188541	2	90%
5	CChkStd	0.9925501	298.7238	0.9995536	4/19/2006 10:44	Low	10101.03	1.717743	2.01E-02	5	99%
250	CChkStd	0.9982696	290.7059	0.9998528	4/19/2006 10:50	Low	10496.49	1.791078	2.07E-02	50	100%
158269001	CChkStd	1.001619	304.9433	0.9993668	4/19/2006 10:56	High	27489.66	4.942344	5.73E-02	250	100%
158269002	CChkStd	0.9966449	300.1391	0.999854	4/19/2006 10:58	High	3301.338	50.1918	1.593677		
158269003	5216371	0.9868905	153.5851	0.9943186	4/19/2006 11:39	Low	16400.49	30345.37	0.1715336		
158269004	5216372	0.9656691	152.1669	0.9991096	4/19/2006 11:41	Low	35390.99	6.407591	0.1040891		
158269005	5216373	0.9621575	154.0736	0.9983983	4/19/2006 11:43	Low	31791.73	5.740133	0.1098937		
158269006	5216374	0.9632051	149.8885	0.9975623	4/19/2006 11:45	Low	30907.78	5.57621	0.1261546		
158270001	5216375	0.973178	158.43	0.9931245	4/19/2006 11:47	Low	28288.64	4.077991	0.1353255		
158437001	5216376	0.9833986	162.3149	0.9933005	4/19/2006 11:50	Low	28089.76	5.053627	0.1622427		
158437002	5216377	0.9877269	172.3907	0.9854	4/19/2006 11:52	Low	20826.23	3.706658	0.1610164		
158437003	5216379	0.9914905	150.9297	0.9963481	4/19/2006 11:54	Low	28912.91	4.835389	0.1275451		
158437004	52163710	1.005836	162.6	0.992139	4/19/2006 11:56	High	24287.18	4.348466	0.1497161		
158438001	52163711	0.9936714	145.9376	0.9939824	4/19/2006 12:01	Low	1017.159	15.40178	0.6865477		
158438002	52163712	1.006081	149.1253	0.9899911	4/19/2006 12:05	Low	24942.62	4.470014	0.1945381		
158438003	52163713	0.9918972	143.1666	0.9952648	4/19/2006 12:06	High	780.3599	11.79672	0.5009188		
158438004	52163714	0.9851436	152.5361	0.9974464	4/19/2006 12:06	Low	25946.24	4.656128	0.1057968		
158438005	52163715	0.9944347	185.4472	0.9649491	4/19/2006 12:08	Low	16692.4	2.940067	0.1825326		
1201073175	52163716	0.9946537	145.9422	0.997261	4/19/2006 12:11	Low	26836.61	4.82124	0.1164142		
1201073176	52163717	1.008086	148.6045	0.9948929	4/19/2006 12:13	Low	64918.8	11.86332	0.3659206		
2	CChkStd	0.9989305	145.4348	0.9910215	4/19/2006 12:17	High	1289.896	19.55413	0.9767898	2	95%
5	CChkStd	0.9962268	293.2501	0.9997929	4/19/2006 12:18	Low	11052.63	1.894212	2.21E-02	5	100%
50	CChkStd	0.9998017	298.5897	0.9998721	4/19/2006 12:22	Low	27811.13	5.001958	5.77E-02	5	102%
250	CChkStd	0.9990258	319.0769	0.9995897	4/19/2006 12:26	High	3358.041	51.05692	1.613235	50	99%
5	CChkStd	0.9998021	323.0347	0.9999397	4/19/2006 12:26	High	16238.22	247.8379	7.783497	250	109%
50	CChkStd	0.9968954	333.9677	0.9989975	4/20/2006 14:26	Low	15385.69	2.185819	2.48E-02	5	108%
250	CChkStd	0.9974557	327.5624	0.9994638	4/20/2006 14:32	High	6300.261	5.403488	6.17E-02	5	108%
158437004	521637	0.9348087	322.7957	0.9989881	4/20/2006 14:35	High	34320.84	49.40655	1.567117	50	98%
158438001	521637	0.9239793	177.459	0.9998775	4/20/2006 15:03	Low	48143.04	273.675	8.62856	250	109%
		0.9235593	168.7448	0.9992825	4/20/2006 15:06	Low	27306	3.826512	0.0543412		

W. C. ...

W. C. ...

158438002	521637	0.9273942	177.7031	0.9995724	4/20/2006 15:08	Low	26756.08	3.750758	0.0484198	2	109%
158438005	521637	0.9311544	180.5077	0.9997067	4/20/2006 15:11	Low	23974.62	3.367601	4.17E-02	5	108%
1201073175	521637	0.9340066	176.3609	0.999713	4/20/2006 15:13	Low	28723.49	4.021776	4.98E-02	5	107%
1201073176	521637	0.9342846	169.4966	0.9987264	4/20/2006 15:15	Low	99722.36	13.80215	0.2222143	250	107%
	CChkStd	0.9280117	321.3094	0.9996265	4/20/2006 15:18	Low	15407.13	2.187395	2.56E-02	2	106%
	CChkStd	0.9386966	333.2115	0.9999149	4/20/2006 15:22	Low	38698.71	5.395902	6.11E-02	5	97%
	CChkStd	0.9482937	327.9472	0.9994354	4/20/2006 15:23	High	6803.558	53.33803	1.692242	250	107%
	CChkStd	0.9393737	333.9432	0.9999226	4/20/2006 15:26	High	33464.57	266.651	8.402281	2	106%
	CChkStd	0.977299	317.4226	0.9998281	4/20/2006 16:36	Low	15173.23	2.112619	2.31E-02	5	97%
	CChkStd	0.9846466	339.9385	0.9999489	4/20/2006 16:39	Low	36037.84	4.86291	5.24E-02	5	91%
	CChkStd	1.004076	323.4604	0.9998722	4/20/2006 16:41	High	5843.935	45.60827	1.429597	250	90%
158437004	521637	0.9997197	318.5651	0.9999002	4/20/2006 16:47	High	28654.95	225.0568	6.990772	250	90%
158438001	521637	0.9846579	181.0665	0.9998722	4/20/2006 16:54	Low	42953.87	5.774553	0.084913	2	104%
158438002	521637	0.9873068	170.7912	0.9996775	4/20/2006 16:56	Low	24561.12	3.350094	4.07E-02	5	99%
158438005	521637	0.9895955	177.224	0.9997618	4/20/2006 16:59	Low	24070.27	3.285392	3.85E-02	5	99%
1210173175	521637	0.9935957	180.9698	0.9997128	4/20/2006 17:01	Low	22926.21	3.134587	3.72E-02	50	100%
1210173176	521637	0.988754	171.9204	0.9996576	4/20/2006 17:03	Low	26187.88	3.564527	4.36E-02	2	104%
	CChkStd	0.9821866	161.5261	0.9995993	4/20/2006 17:06	Low	95773.55	12.73703	0.1615019	2	104%
	CChkStd	0.9714403	319.4821	0.9997946	4/20/2006 17:08	Low	14996.8	2.089231	0.0229534	5	99%
	CChkStd	0.9778636	332.5217	0.9998664	4/20/2006 17:11	Low	36592.72	4.936051	5.37E-02	50	99%
	CChkStd	0.9919038	326.8352	0.9995726	4/20/2006 17:13	High	6363.198	49.67219	1.550157	250	100%
	CChkStd	0.9894531	320.705	0.9999521	4/20/2006 17:15	High	31737.35	249.4475	7.742156	250	100%

KPAWIN® (Version 1.2.8) Multiple Sample Report

Laboratory:

ANALYTE: Uranium

ANALYST:

Salina

Sample Identification

Sample ID	Proc ID	Sample Type	Description	Date / Time	SpA	SpG	Atomic Mass	Basis Sample	Customer ID
2.0	None	CChkStd	CChkStd	04/19/2006 09:20 AM	25000	1	238.0289	None	None
5.0	None	CChkStd	CChkStd	04/19/2006 09:23 AM	25000	1	238.0289	None	None
50.0	None	CChkStd	CChkStd	04/19/2006 09:25 AM	25000	1	238.0289	None	None
250.0	None	CChkStd	CChkStd	04/19/2006 09:27 AM	25000	1	238.0289	None	None
1.0 ug/L	None	ConfTst	ConfTst	04/19/2006 08:00 AM	25000	1	238.0289	None	None
158269001	None	Sample	521637'	04/19/2006 10:06 AM	25000	1	238.0289	None	None
158269002	None	Sample	521637'1	04/19/2006 10:08 AM	25000	1	238.0289	None	None
158269003	None	Sample	521637'2	04/19/2006 10:10 AM	25000	1	238.0289	None	None
158269004	None	Sample	521637'3	04/19/2006 10:12 AM	25000	1	238.0289	None	None
158270001	None	Sample	521637'4	04/19/2006 10:14 AM	25000	1	238.0289	None	None
158270002	None	Sample	521637'5	04/19/2006 10:16 AM	25000	1	238.0289	None	None
158437001	None	Sample	521637'6	04/19/2006 10:18 AM	25000	1	238.0289	None	None
158437002	None	Sample	521637'7	04/19/2006 10:21 AM	25000	1	238.0289	None	None
158437003	None	Sample	521637'8	04/19/2006 10:23 AM	25000	1	238.0289	None	None
158437004	None	Sample	521637'9	04/19/2006 10:25 AM	25000	1	238.0289	None	None
158438001	None	Sample	521637'10	04/19/2006 10:27 AM	25000	1	238.0289	None	None
158438002	None	Sample	521637'11	04/19/2006 10:29 AM	25000	1	238.0289	None	None

Handwritten signature

Handwritten signature

KPAWIN® (Version 1.2.8) Multiple Sample Report

Laboratory:

ANALYTE: Uranium

ANALYST:

Salina

Sample Identification

Sample ID	Proc ID	Sample Type	Description	Date / Time	SpA	SpG	Atomic Mass	Basis Sample	Customer ID
158438003	None	Sample	521637'12	04/19/2006 10:31 AM	25000	1	238.0289	None	None
158438004	None	Sample	521637'13	04/19/2006 10:33 AM	25000	1	238.0289	None	None
158438005	None	Sample	521637'14	04/19/2006 10:35 AM	25000	1	238.0289	None	None
1201073174	None	Sample	521637'15	04/19/2006 10:37 AM	25000	1	238.0289	None	None
1201073175	None	Sample	521637'16	04/19/2006 10:39 AM	25000	1	238.0289	None	None
1201073176	None	Sample	521637'17	04/19/2006 10:43 AM	25000	1	238.0289	None	None
1201073177	None	Sample	521637'18	04/19/2006 10:46 AM	25000	1	238.0289	None	None
1201073178	None	Sample	521637'19	04/19/2006 10:48 AM	25000	1	238.0289	None	None
2.0	None	CChkStd	CChkStd	04/19/2006 10:50 AM	25000	1	238.0289	None	None
5.	None	CChkStd	CChkStd	04/19/2006 10:54 AM	25000	1	238.0289	None	None
50.	None	CChkStd	CChkStd	04/19/2006 10:56 AM	25000	1	238.0289	None	None
250.	None	CChkStd	CChkStd	04/19/2006 10:58 AM	25000	1	238.0289	None	None
158269001	None	Sample	521637'1	04/19/2006 11:39 AM	25000	1	238.0289	None	None
158269002	None	Sample	521637'2	04/19/2006 11:41 AM	25000	1	238.0289	None	None
158269003	None	Sample	521637'3	04/19/2006 11:43 AM	25000	1	238.0289	None	None
158269004	None	Sample	521637'4	04/19/2006 11:45 AM	25000	1	238.0289	None	None
158270001	None	Sample	521637'5	04/19/2006 11:47 AM	25000	1	238.0289	None	None

Handwritten signature/initials

KPAWin® (Version 1.2.8) Multiple Sample Report

Laboratory:

ANALYTE: Uranium

ANALYST: Salina

Sample Identification

Sample ID	Proc ID	Sample Type	Description	Date / Time	SpA	SpG	Atomic Mass	Basis Sample	Customer ID
158270002	None	Sample	521637'6	04/19/2006 11:50 AM	25000	1	238.0289	None	None
158437001	None	Sample	521637'7	04/19/2006 11:52 AM	25000	1	238.0289	None	None
158437002	None	Sample	521637'8	04/19/2006 11:54 AM	25000	1	238.0289	None	None
158437003	None	Sample	521637'9	04/19/2006 11:56 AM	25000	1	238.0289	None	None
158437004	None	Sample	521637'10	04/19/2006 12:00 PM	25000	1	238.0289	None	None
158438001	None	Sample	521637'11	04/19/2006 12:01 PM	25000	1	238.0289	None	None
158438002	None	Sample	521637'12	04/19/2006 12:05 PM	25000	1	238.0289	None	None
158438003	None	Sample	521637'13	04/19/2006 12:06 PM	25000	1	238.0289	None	None
158438004	None	Sample	521637'14	04/19/2006 12:08 PM	25000	1	238.0289	None	None
158438005	None	Sample	521637'15	04/19/2006 12:11 PM	25000	1	238.0289	None	None
1201073175	None	Sample	521637'16	04/19/2006 12:13 PM	25000	1	238.0289	None	None
1201073176	None	Sample	521637'17	04/19/2006 12:17 PM	25000	1	238.0289	None	None
2.0	None	CChkStd	CChkStd	04/19/2006 12:18 PM	25000	1	238.0289	None	None
5.	None	CChkStd	CChkStd	04/19/2006 12:22 PM	25000	1	238.0289	None	None
50.	None	CChkStd	CChkStd	04/19/2006 12:24 PM	25000	1	238.0289	None	None
250.	None	CChkStd	CChkStd	04/19/2006 12:26 PM	25000	1	238.0289	None	None

Page 3 of 57

Handwritten signature/initials

KPAWIN® (Version 1.2.8) Multiple Sample Report

Laboratory: ANALYTE: Uranium ANALYST: sa101078

Sample Identification

Sample ID	Proc ID	Sample Type	Description	Date / Time	SPA	SPG	Atomic Mass	Basis Sample	Customer ID
2.0	None	CChkStd	CChkStd	04/20/2006 02:26	PM 2.5E+04	1	238.0289	None	None
5.0	None	CChkStd	CChkStd	04/20/2006 02:31	PM 2.5E+04	1	238.0289	None	None
50.0	None	CChkStd	CChkStd	04/20/2006 02:32	PM 2.5E+04	1	238.0289	None	None
250.0	None	CChkStd	CChkStd	04/20/2006 02:35	PM 2.5E+04	1	238.0289	None	None
158437004	None	Sample	521637	04/20/2006 03:03	PM 2.5E+04	1	238.0289	None	None
158438001	None	Sample	521637	04/20/2006 03:06	PM 2.5E+04	1	238.0289	None	None
158438002	None	Sample	521637	04/20/2006 03:08	PM 2.5E+04	1	238.0289	None	None
158438005	None	Sample	521637	04/20/2006 03:11	PM 2.5E+04	1	238.0289	None	None
1201073175	None	Sample	521637	04/20/2006 03:13	PM 2.5E+04	1	238.0289	None	None
1201073176	None	Sample	521637	04/20/2006 03:15	PM 2.5E+04	1	238.0289	None	None
2.0	None	CChkStd	CChkStd	04/20/2006 03:18	PM 2.5E+04	1	238.0289	None	None
5.0	None	CChkStd	CChkStd	04/20/2006 03:22	PM 2.5E+04	1	238.0289	None	None
50.0	None	CChkStd	CChkStd	04/20/2006 03:23	PM 2.5E+04	1	238.0289	None	None
250.0	None	CChkStd	CChkStd	04/20/2006 03:26	PM 2.5E+04	1	238.0289	None	None
2.0	None	CChkStd	CChkStd	04/20/2006 04:36	PM 2.5E+04	1	238.0289	None	None
5.0	None	CChkStd	CChkStd	04/20/2006 04:39	PM 2.5E+04	1	238.0289	None	None
50.0	None	CChkStd	CChkStd	04/20/2006 04:41	PM 2.5E+04	1	238.0289	None	None

Page 78 of 587

[Handwritten Signature]

KPAWin® (Version 1.2.8) Multiple Sample Report

Laboratory:

ANALYTE: Uranium

ANALYST:

sal01078

Sample Identification

Sample ID	Proc ID	Sample Type	Description	Date / Time	SpA	SpG	Atomic Mass	Basis Sample	Customer ID
250.0	None	CChkStd	CChkStd	04/20/2006 04:47 PM	2.5E+04	1	238.0289	None	None
158437004	None	Sample	521637	04/20/2006 04:54 PM	2.5E+04	1	238.0289	None	None
158438001	None	Sample	521637	04/20/2006 04:56 PM	2.5E+04	1	238.0289	None	None
158438002	None	Sample	521637	04/20/2006 04:59 PM	2.5E+04	1	238.0289	None	None
158438005	None	Sample	521637	04/20/2006 05:01 PM	2.5E+04	1	238.0289	None	None
1210173175	None	Sample	521637	04/20/2006 05:03 PM	2.5E+04	1	238.0289	None	None
1210173176	None	Sample	521638	04/20/2006 05:06 PM	2.5E+04	1	238.0289	None	None
2.0	None	CChkStd	CChkStd	04/20/2006 05:08 PM	2.5E+04	1	238.0289	None	None
5.0	None	CChkStd	CChkStd	04/20/2006 05:11 PM	2.5E+04	1	238.0289	None	None
50.0	None	CChkStd	CChkStd	04/20/2006 05:13 PM	2.5E+04	1	238.0289	None	None
250.0	None	CChkStd	CChkStd	04/20/2006 05:15 PM	2.5E+04	1	238.0289	None	None

Page 2 of 5

af

KPAWIN® (Version 1.2.8) Multiple Sample Report

Laboratory: **ANALYTE:** Uranium **ANALYST:** Salina

Analytical Results

Sample ID	Range	Time Gates	Sample Units	Analytical Result	Total Dilution	Sample Type	Final Result	Pulses	Calibration ID	Uncertainty
1802.0	Low	5 -49	µg/l	1.971		CChkStd		1000	041906	.023
55.0	Low	5 -49	µg/l	5.126		CChkStd		1000	041906	.058
50.0	High	5 -49	µg/l	48.977		CChkStd		1000	041906	1.547
250.0	High	5 -49	µg/l	253.604		CChkStd		1000	041906	7.980
1.0 ug/L	Low	5 -49	µg/l	.000		ConfTst	.000	1000	041906	.000
158269001	Low	5 -49	µg/l	5.151	1	Sample	5.151	1000	041906	.169
158269002	Low	5 -49	µg/l	6.280	1	Sample	6.280	1000	041906	.107
158269003	Low	5 -49	µg/l	5.550	1	Sample	5.550	1000	041906	.097
158269004	Low	5 -49	µg/l	5.419	1	Sample	5.419	1000	041906	.109
158270001	Low	5 -49	µg/l	4.188	1	Sample	4.188	1000	041906	.137
158270002	Low	5 -49	µg/l	5.352	1	Sample	5.352	1000	041906	.168
158437001	Low	5 -49	µg/l	3.726	1	Sample	3.726	1000	041906	.157
158437002	Low	5 -49	µg/l	4.886	1	Sample	4.886	1000	041906	.131
158437003	Low	5 -49	µg/l	4.386	1	Sample	4.386	1000	041906	.147
158437004	Low	5 -49	µg/l	9.792	1	Sample	9.792	1000	041906	.262
158438001	Low	5 -49	µg/l	4.521	1	Sample	4.521	1000	041906	.184
158438002	Low	5 -49	µg/l	5.090	1	Sample	5.090	1000	041906	.143

Handwritten signature

Handwritten signature

KPAWIN® (Version 1.2.8) Multiple Sample Report

Laboratory:

ANALYTE: Uranium

ANALYST:

Salina

Analytical Results

Sample ID	Range	Time Gates	Sample Units	Analytical Result	Total Dilution	Sample Type	Final Result	Pulses	Calibration ID	Uncertainty
158438003	Low	5 -49	µg/l	4.671	1	Sample	4.671	1000	041906	.086
158438004	Low	5 -49	µg/l	3.039	1	Sample	3.039	1000	041906	.179
158438005	Low	5 -49	µg/l	4.594	1	Sample	4.594	1000	041906	.210
1201073174	Low	5 -49	µg/l	-.020	1	Sample	-.020	1000	041906	.000
1201073175	Low	5 -49	µg/l	5.033	1	Sample	5.033	1000	041906	.173
1201073176	High	5 -49	µg/l	15.198	1	Sample	15.198	1000	041906	.808
1201073177	High	5 -49	µg/l	16.071	1	Sample	16.071	1000	041906	.519
1201073178	Low	5 -49	µg/l	1.718	1	Sample	1.718	1000	041906	.020
2.0	Low	5 -49	µg/l	1.791		CChkStd		1000	041906	.021
5.	Low	5 -49	µg/l	4.942		CChkStd		1000	041906	.057
50.	High	5 -49	µg/l	50.192		CChkStd		1000	041906	1.594
250.	High	5 -49	µg/l	250.324		CChkStd		1000	041906	7.876
158269001	Low	5 -49	µg/l	5.472	1	Sample	5.472	1000	041906	.172
158269002	Low	5 -49	µg/l	6.408	1	Sample	6.408	1000	041906	.104
158269003	Low	5 -49	µg/l	5.740	1	Sample	5.740	1000	041906	.110
158269004	Low	5 -49	µg/l	5.576	1	Sample	5.576	1000	041906	.126
158270001	Low	5 -49	µg/l	4.078	1	Sample	4.078	1000	041906	.135

Page 181 of 277

Handwritten signature

KPAWin® (Version 1.2.8) Multiple Sample Report

Laboratory: ANALYTE: Uranium ANALYST: Salina

Analytical Results

Sample ID	Range	Time Gates	Sample Units	Analytical Result	Total Dilution	Sample Type	Final Result	Pulses	Calibration ID	Uncertainty
158270002	Low	5 -49	µg/l	5.054	1	Sample	5.054	1000	041906	.162
158437001	Low	5 -49	µg/l	3.707	1	Sample	3.707	1000	041906	.161
158437002	Low	5 -49	µg/l	4.835	1	Sample	4.835	1000	041906	.128
158437003	Low	5 -49	µg/l	4.348	1	Sample	4.348	1000	041906	.150
158437004	High	5 -49	µg/l	15.402	1	Sample	15.402	1000	041906 Default	.687
158438001	Low	5 -49	µg/l	4.470	1	Sample	4.470	1000	041906	.195
158438002	High	5 -49	µg/l	11.797	1	Sample	11.797	1000	041906 Default	.501
158438003	Low	5 -49	µg/l	4.656	1	Sample	4.656	1000	041906	.106
158438004	Low	5 -49	µg/l	2.940	1	Sample	2.940	1000	041906	.183
158438005	Low	5 -49	µg/l	4.821	1	Sample	4.821	1000	041906	.116
1201073175	Low	5 -49	µg/l	11.883	1	Sample	11.883	1000	041906	.366
1201073176	High	5 -49	µg/l	19.554	1	Sample	19.554	1000	041906 Default	.977
2.0	Low	5 -49	µg/l	1.894		CChkStd		1000	041906	.022
5.	Low	5 -49	µg/l	5.002		CChkStd		1000	041906	.058
50.	High	5 -49	µg/l	51.057		CChkStd		1000	041906 Default	1.613
250.	High	5 -49	µg/l	247.838		CChkStd		1000	041906 Default	7.783

KPAWIN® (Version 1.2.8) Multiple Sample Report

Laboratory:

ANALYTE:

Uranium

ANALYST:

sal01078

Analytical Results

Sample ID	Range	Time Gates	Sample Units	Analytical Result	Total Dilution	Sample Type	Final Result	Pulses	Calibration ID	Uncertainty
22.0	Low	5 -39	µg/l	2.19E+00		CChkStd		1000	042006	2.48E-02
55.0	Low	5 -39	µg/l	5.40E+00		CChkStd		1000	042006	6.17E-02
50.0	High	5 -39	µg/l	4.94E+01		CChkStd		1000	042006	1.57E+00
250.0	High	5 -39	µg/l	2.74E+02		CChkStd		1000	042006	8.63E+00
158437004	Low	5 -39	µg/l	6.70E+00	1	Sample	6.70E+00	1000	042006	7.86E-02
158438001	Low	5 -39	µg/l	3.83E+00	1	Sample	3.83E+00	1000	042006	5.43E-02
158438002	Low	5 -39	µg/l	3.75E+00	1	Sample	3.75E+00	1000	042006	4.84E-02
158438005	Low	5 -39	µg/l	3.37E+00	1	Sample	3.37E+00	1000	042006	4.17E-02
1201073175	Low	5 -39	µg/l	4.02E+00	1	Sample	4.02E+00	1000	042006	4.98E-02
1201073176	Low	5 -39	µg/l	1.38E+01	1	Sample	1.38E+01	1000	042006	2.22E-01
2.0	Low	5 -39	µg/l	2.19E+00		CChkStd		1000	042006	2.56E-02
5.0	Low	5 -39	µg/l	5.40E+00		CChkStd		1000	042006	6.11E-02
50.0	High	5 -39	µg/l	5.33E+01		CChkStd		1000	042006	1.69E+00
250.0	High	5 -39	µg/l	2.67E+02		CChkStd		1000	042006	8.40E+00
2.0	Low	5 -39	µg/l	2.11E+00		CChkStd		1000	Default	2.31E-02
5.0	Low	5 -39	µg/l	4.86E+00		CChkStd		1000	Default	5.24E-02
50.0	High	5 -39	µg/l	4.56E+01		CChkStd		1000	Default	1.43E+00

KPAWin® (Version 1.2.8) Multiple Sample Report

Laboratory: ANALYTE: Uranium ANALYST: sa101078

Analytical Results

Sample ID	Range	Time Gates	Sample Units	Analytical Result	Total Dilution	Sample Type	Final Result	Pulses	Calibration ID	Uncertainty
250.0	High	5 -39	µg/l	2.25E+02		CChkStd		1000	Default	6.99E+00
158437004	Low	5 -39	µg/l	5.77E+00	1	Sample	5.77E+00	1000	Default	6.49E-02
158438001	Low	5 -39	µg/l	3.35E+00	1	Sample	3.35E+00	1000	Default	4.07E-02
158438002	Low	5 -39	µg/l	3.29E+00	1	Sample	3.29E+00	1000	Default	3.85E-02
158438005	Low	5 -39	µg/l	3.13E+00	1	Sample	3.13E+00	1000	Default	3.72E-02
1210173175	Low	5 -39	µg/l	3.56E+00	1	Sample	3.56E+00	1000	Default	4.36E-02
1210173176	Low	5 -39	µg/l	1.27E+01	1	Sample	1.27E+01	1000	Default	1.62E-01
2.0	Low	5 -39	µg/l	2.09E+00		CChkStd		1000	Default	2.30E-02
5.0	Low	5 -39	µg/l	4.94E+00		CChkStd		1000	Default	5.37E-02
50.0	High	5 -39	µg/l	4.97E+01		CChkStd		1000	Default	1.55E+00
250.0	High	5 -39	µg/l	2.49E+02		CChkStd		1000	Default	7.74E+00

KPAWin® (Version 1.2.8) Multiple Sample Report

Laboratory:

ANALYTE:

Uranium

ANALYST:

Salina

Quality Control

Sample ID	Basis Sample	Reference Lifetime	R ² Intensity	Reference Ratio	Sample Lifetime	Sample Intercept	IDL / MDL	Recovery (%)	RPD (%)	AW Flags
188	None	317	.9998	.98634	306	11466	0E+00/ 0E+00	98.55		
189	None	316	1.0000	.98870	312	28481	0E+00/ 0E+00	102.52		
190	None	316	.9996	.99650	324	3222	0E+00/ 0E+00	97.95		
250.0	None	317	.9998	.99692	304	16615	0E+00/ 0E+00	101.44		
1.0 ug/L	None	325	.9995	1.01518	305	5791	0E+00/ 0E+00			
158269001	None	316	.9939	.98347	152	28615	0E+00/ 0E+00			
158269002	None	317	.9988	.96758	162	34702	0E+00/ 0E+00			
158269003	None	316	.9988	.96533	157	30769	0E+00/ 0E+00			
158269004	None	317	.9982	.96491	152	30058	0E+00/ 0E+00			
158270001	None	318	.9931	.97398	162	23422	0E+00/ 0E+00			
158270002	None	319	.9936	.97498	163	29697	0E+00/ 0E+00			
158437001	None	318	.9869	.98290	168	20929	0E+00/ 0E+00			
158437002	None	319	.9962	.98639	151	27184	0E+00/ 0E+00			
158437003	None	320	.9925	.98545	163	24491	0E+00/ 0E+00			
158437004	None	320	.9963	.98703	149	53639	0E+00/ 0E+00			A9
158438001	None	318	.9903	.99137	150	25220	0E+00/ 0E+00			A9
158438002	None	316	.9961	1.00069	144	28284	0E+00/ 0E+00			A9

KPAWIN® (Version 1.2.8) Multiple Sample Report

Laboratory: ANALYTE: Uranium ANALYST: Salina

Quality Control

Sample ID	Basis Sample	Reference Lifetime	R ² Intensity	Reference Ratio	Sample Lifetime	Sample Intercept	IDL / MDL	Recovery (%)	RPD (%)	AW Flags
158438003	None	318	.9986	.99140	152	26025	0E+00 / 0E+00			
158438004	None	319	.9691	.98698	184	17227	0E+00 / 0E+00			
158438005	None	317	.9725	.99307	226	25613	0E+00 / 0E+00			
1201073174	None	317	.9892	.99008	312	729	0E+00 / 0E+00			
1201073175	None	316	.9935	.99360	149	27978	0E+00 / 0E+00			A9
1201073176	None	315	.9890	1.01595	146	1004	0E+00 / 0E+00			A9
1201073177	None	316	.9986	1.00929	293	1061	0E+00 / 0E+00			
1201073178	None	318	.9998	.99044	306	10101	0E+00 / 0E+00			
2.0	None	316	.9999	.99255	299	10496	0E+00 / 0E+00	89.55		
5.	None	317	.9999	.99827	291	27490	0E+00 / 0E+00	98.85		
50.	None	316	.9994	1.00162	305	3301	0E+00 / 0E+00	100.38		
250.	None	318	.9999	.99664	300	16400	0E+00 / 0E+00	100.13		
158269001	None	315	.9943	.98683	154	30345	0E+00 / 0E+00			
158269002	None	316	.9991	.96567	152	35391	0E+00 / 0E+00			
158269003	None	316	.9984	.96216	154	31792	0E+00 / 0E+00			
158269004	None	317	.9976	.96321	150	30908	0E+00 / 0E+00			A9
158270001	None	316	.9931	.97118	158	22829	0E+00 / 0E+00			

Handwritten signature/initials

KPAWIN® (Version 1.2.8) Multiple Sample Report

Laboratory: ANALYTE: Uranium ANALYST: Salina

Quality Control

Sample ID	Basis Sample	Reference Lifetime	R ² Intensity	Reference Ratio	Sample Lifetime	Sample Intercept	IDL / MDL	Recovery (%)	RPD (%)	AW Flags
158270002	None	317	.9933	.97318	162	28090	0E+00 / 0E+00			
158437001	None	317	.9854	.98340	172	20826	0E+00 / 0E+00			
158437002	None	316	.9963	.98773	151	26913	0E+00 / 0E+00			
158437003	None	317	.9921	.99149	163	24287	0E+00 / 0E+00			
158437004	None	319	.9940	1.00584	146	1017	0E+00 / 0E+00			A9
158438001	None	317	.9890	.99367	149	24943	0E+00 / 0E+00			A9
158438002	None	317	.9953	1.00608	143	780	0E+00 / 0E+00			A9
158438003	None	318	.9974	.99190	153	25946	0E+00 / 0E+00			
158438004	None	317	.9649	.98514	185	16692	0E+00 / 0E+00			
158438005	None	314	.9973	.99443	146	26837	0E+00 / 0E+00			A9
1201073175	None	315	.9949	.99465	149	64919	0E+00 / 0E+00			A9
1201073176	None	315	.9910	1.00809	145	1290	0E+00 / 0E+00			A9
2.0	None	314	.9998	.99893	293	11053	0E+00 / 0E+00	94.71		
5.	None	316	.9999	.99623	299	27811	0E+00 / 0E+00	100.04		
50.	None	315	.9996	.99980	319	3358	0E+00 / 0E+00	102.11		
250.	None	315	.9999	.99903	313	16238	0E+00 / 0E+00	99.14		

Page 187 of 507

Handwritten signature

KPAWin® (Version 1.2.8) Multiple Sample Report

Laboratory:

ANALYTE:

Uranium

ANALYST:

sal01078

Quality Control

Sample ID	Basis Sample	Reference Lifetime	R ² Intensity	Reference Ratio	Sample Lifetime	Sample Intercept	IDL / MDL	Recovery (%)	RPD (%)	AW Flags
2.0	None	283	.9999	.92980	323	15396	0E+00 / 0E+00	109.29		
5.0	None	281	.9998	.93690	334	38754	0E+00 / 0E+00	108.07		
50.0	None	282	.9995	.93746	328	6300	0E+00 / 0E+00	98.81		
250.0	None	281	.9999	.93481	323	34321	0E+00 / 0E+00	109.47		
158437004	None	281	.9999	.92397	177	48143	0E+00 / 0E+00			
158438001	None	281	.9993	.92356	169	27306	0E+00 / 0E+00			
158438002	None	281	.9996	.92739	178	26756	0E+00 / 0E+00			
158438005	None	282	.9997	.93115	181	23975	0E+00 / 0E+00			
1201073175	None	281	.9997	.93401	178	28723	0E+00 / 0E+00			
1201073176	None	282	.9987	.93428	169	99722	0E+00 / 0E+00			A18
2.0	None	282	.9996	.92801	321	15407	0E+00 / 0E+00	109.37		
5.0	None	282	.9999	.93870	333	38699	0E+00 / 0E+00	107.92		
50.0	None	281	.9994	.94829	328	6804	0E+00 / 0E+00	106.68		
250.0	None	282	.9999	.93937	334	33465	0E+00 / 0E+00	106.66		
2.0	None	280	.9998	.97730	317	15173	0E+00 / 0E+00	105.63		
5.0	None	281	.9999	.98465	340	36038	0E+00 / 0E+00	97.26		
50.0	None	281	.9993	1.00408	323	5844	0E+00 / 0E+00	91.22		

Handwritten signature and date: 4/20/06

KPAWin® (Version 1.2.8) Multiple Sample Report

Laboratory: ANALYTE: Uranium ANALYST: sa101078

Quality Control

Sample ID	Basis Sample	Reference Lifetime	R ² Intensity	Reference Ratio	Sample Lifetime	Sample Intercept	IDL / MDL	Recovery (%)	RPD (%)	AW Flags
250.0	None	281	.9999	.99972	319	28655	0E+00 / 0E+00	90.02		
158437004	None	281	.9999	.98466	181	42954	0E+00 / 0E+00			
158438001	None	280	.9997	.98731	171	24561	0E+00 / 0E+00			
158438002	None	279	.9998	.98960	177	24070	0E+00 / 0E+00			
158438005	None	280	.9997	.99360	181	22926	0E+00 / 0E+00			
1210173175	None	280	.9997	.98875	172	26188	0E+00 / 0E+00			
1210173176	None	281	.9996	.98219	162	95774	0E+00 / 0E+00			A18
2.0	None	282	.9998	.97144	319	14996	0E+00 / 0E+00	104.46		
5.0	None	281	.9999	.97788	333	36593	0E+00 / 0E+00	98.72		
50.0	None	279	.9996	.99190	327	6363	0E+00 / 0E+00	99.34		
250.0	None	279	1.0000	.98945	321	31737	0E+00 / 0E+00	99.78		

KPAWIN® (Version 1.2.8) Multiple Sample Report

Laboratory: ANALYTE: Uranium ANALYST: Salina

Calibration Report Results

Low Calibration ID - 041906 High Calibration ID - Default
 Batch ID - 2180
 Date - 4/19/2006 9:08:50 AM

Calibration Report Results

Range	Used	Sample ID	Std Conc	Std ID	Intercept	Uncert	Percent Discrep	Time Reference Gates	Ratio	Lifetime	R ²	AW Flags
Low	+	BckGnd	0.000		342	18	.000	5-49	1.0000	358	.9556	
Low	+	1.0 ug/L	1.000	0914	6063	78	-3.101	5-49	.9896	305	.9995	
Low	+	3.0 ug/L	3.000	0872	17112	131	.594	5-49	.9850	305	.9999	
Low	+	5.0 ug/L	5.000	0898	27967	167	.618	5-49	.9884	312	.9999	
Low	+	10.0 ug/L	10.000	0840	54668	234	-.177	5-49	.9956	297	.9999	

High	+	BckGnd	0.000		4	3	.000	5-29	1.0000	346	.4817	
High	+	10.0 ug/L	10.000	0840	662	26	-.003	5-49	.9898	288	.9982	
High	+	250 ug/L	250.000	0876	16379	128	.000	5-49	.9919	312	.9998	
High	+	500 ug/L	500.000	0842	32645	181	.000	5-49	.9935	302	1.0000	

Signature

Signature

KPAWin Detailed Calibration Report

Laboratory:

Calibration Details

Laboratory ID	KPA11AUTO1	Customer ID	None
Analyst	Salina	Procedure ID	None
Calibration Config ID	1000 Release	Calibration Date	4/19/2006 9:08:50 AM
Calibration Batch ID	2180		

Low Range Details

High Range Details

User Calibration	True	None
Calibration Id	041906	Default
Minimum Number of Standards	3	3
Calibration Alarms	0.99999431	1
Calibration R ²	8.27E+02	3.36E-10
Variance	Y= +5392.492X +838.109	Y= -0.001X ² +65.713X +5.223
Calibration Equation		

AS
4/21/06

KPAWin® (Version 1.2.8) Multiple Sample Report

Laboratory: **ANALYTE:** Uranium **ANALYST:** sal01078

Calibration Report Results

Low Calibration ID - 042006 High Calibration ID - 042006
 Batch ID - 1539
 Date - 4/20/2006 8:46:28 AM

Calibration Report Results

Range	Used	Sample ID	Std Conc	Std ID	Intercept	Uncert	Percent Time Reference			R ²	AW Flags
							Discrep	Gates	Lifetime		
Low	+	BckGnd	0.000		649	25	.000	5-39	1.0000	306	.9748
Low	+	1.0 ug/L	1.000	0836	7002	84	2.959	5-39	.9965	312	.9993
Low	+	3.0 ug/L	3.000	0838	20871	144	-1.997	5-39	.9969	315	.9999
Low	+	5.0 ug/L	5.000	0839	36047	190	.612	5-39	1.0026	338	.9999
Low	+	10.0 ug/L	10.000	0840	72119	269	-.003	5-39	1.0069	303	1.0000

High	+	BckGnd	0.000		5	3	.000	5-37	1.0000	334	.3543
High	+	10.0 ug/L	10.000	0840	1232	35	.001	5-39	1.0189	308	.9972
High	+	250 ug/L	250.000	0856	31429	177	.000	5-39	1.0209	329	.9999
High	+	500 ug/L	500.000	0842	61174	247	.000	5-39	1.0219	314	1.0000

W. J. [Signature]

A. [Signature]

KPAWin Detailed Calibration Report

Laboratory:

Calibration Details

Laboratory ID KPA11AUTO2 Customer ID None
Analyst sal01078 Procedure ID None
Calibration Config ID 1001 Config Calibration Date - 4/20/2006 8:46:28 AM
Calibration Batch ID 1539

Low Range Details

User Calibration True
Calibration Id 042006
Minimum Number of Standards 3
Calibration Alarms 1
Calibration R² 0.9998794
Variance 3.18E+03
Calibration Equation Y= +7259.319X -471.868 Y= -0.014X² +129.455X -61.57

High Range Details

User Calibration True
Calibration Id 042006
Minimum Number of Standards 3
Calibration Alarms 1
Calibration R² 0.9998794
Variance 3.18E+03
Calibration Equation Y= +7259.319X -471.868 Y= -0.014X² +129.455X -61.57



KPAWin© (Version 1.2.8) Multiple Sample Report

Laboratory: **ANALYTE:** Uranium **ANALYST:** sal01078

Calibration Report Results

Low Calibration ID - Default High Calibration ID - Default
 Batch ID - 1650
 Date - 4/20/2006 4:21:53 PM

Calibration Report Results

Range	Used	Sample ID	Std Conc	Std ID	Intercept	Uncert	Discrep	Percent Time Reference	Ratio	Lifetime	R ²	AW Flags
Low	+	BckGnd	0.000		574	24	.000	5-39	1.0000	325	.9701	
Low	+	1.0 ug/L	1.000	0836	7393	86	8.712	5-39	.9905	314	.9998	
Low	+	3.0 ug/L	3.000	0838	21525	147	-1.672	5-39	.9925	312	.9998	
Low	+	5.0 ug/L	5.000	0839	36421	191	-1.732	5-39	.9901	335	.9999	
Low	+	10.0 ug/L	10.000	0840	75386	275	.496	5-39	.9900	301	.9999	

High	+	BckGnd	0.000		5	3	.000	5-28	1.0000	227	.6017	
High	+	10.0 ug/L	10.000	0840	1290	36	.004	5-39	1.0060	298	.9983	
High	+	250 ug/L	250.000	0856	31807	178	.000	5-39	.9994	319	.9999	
High	+	500 ug/L	500.000	0842	63151	251	.000	5-39	.9974	306	.9999	

Handwritten signature

Handwritten initials

KPAWin Detailed Calibration Report

Laboratory:

Calibration Details

Laboratory ID	KPA11AUTO2	Customer ID	None
Analyst	sal01078	Procedure ID	None
Calibration Config ID	1001 Config	Calibration Date	4/20/2006 4:21:53 PM
Calibration Batch ID	1539		

Low Range Details

User Calibration
 Calibration Id None
 Minimum Number of Standards Default
 Calibration Alarms 3
 Calibration R ² 0.9995518
 Variance 1.29E+04
 Calibration Equation Y= +7586.331X -853.799

High Range Details

 None
 Default
 3
 1
 2.69E-09
 Y= -0.004X² +128.101X +9.047

Handwritten signature and date: 4/20/06

METHOD CALIBRATION DATA


General Engineering Laboratories

2040 Savage Road, Charleston, SC 29414
(843)556-8171


Gas Flow Proportional Counter Calibration Package

Method: Pb-210

	YES	NO	Comments
1) Is all calibration standard information enclosed for: primary standard certificate? secondard standard(s) documentation? standard preparation information? standard < 1 Year old or verified?	<input checked="" type="checkbox"/>		
	<input checked="" type="checkbox"/>		
	<input checked="" type="checkbox"/>		
	<input checked="" type="checkbox"/>		
2) Are the detector graphs included? beta absorption curves? beta plateau?	<input checked="" type="checkbox"/>		
	<input checked="" type="checkbox"/>		
3) Is the raw count data included for: the plateau generation? the absorption curve generation? the calibration verification? the crosstalk calculations?	<input checked="" type="checkbox"/>		
	<input checked="" type="checkbox"/>		
	<input checked="" type="checkbox"/>		
	<input checked="" type="checkbox"/>		
4) Are the calibration verification calculations included? are verification recoveries 100% +/- 25%	<input checked="" type="checkbox"/>		
	<input checked="" type="checkbox"/>		

Prepared By: 

Date: 7/29/05

Reviewed By: 

Date: 7/30/05

Effective Date: 7/29/05

0356

DEUTSCHER KALIBRIERDIENST **DKD**

Kalibrierlaboratorium für Meßgrößen der Radioaktivität
Calibration laboratory for measurements of radioactivity

AKKREDITIERT DURCH DIE
PHYSIKALISCH-TECHNISCHE BUNDESANSTALT (PTB)



AEA Technology QSA GmbH
Postfach 58 42 Gieselweg 1
D-38049 Braunschweig D-38110 Braunschweig

Tel. +49 (0) 5307 932-0
Fax +49 (0) 5307 932-194

Source no. FX 248

08640
DKD-K-06501
01-01

Kalibrierschein
Calibration Certificate

Kalibrierzeichen
Calibration mark

Gegenstand
Object

Reference Solution

Dieser Kalibrierschein dokumentiert die Rückführung auf nationale Normale zur Darstellung der Einheiten in Übereinstimmung mit dem Internationalen Einheitensystem (SI).

Hersteller
Manufacturer

AEA Technology QSA GmbH

Der Deutsche Kalibrierdienst ist Unterzeichner des multilateralen Übereinkommens der European co-operation for Accreditation (EA) zur gegenseitigen Anerkennung der Kalibrierscheine.

Typ
Type

RBZB44

Für die Einhaltung einer angemessenen Frist zur Wiederholung der Kalibrierung ist der Benutzer verantwortlich.

Strahler-Nr.
Source number

FX 248

Auftraggeber
Customer

AEA TECHNOLOGY QSA, INC.
USA-BURLINGTON MA 01803

This calibration certificate documents the traceability to national standards, which realize the units of measurement according to the International System of Units (SI).

Auftragsnummer
Order No.

CO 34622

The Deutscher Kalibrierdienst is signatory to the multilateral agreement of the European co-operation for (EA) for the mutual recognition of calibration certificates.

Anzahl der Seiten des Kalibrierscheines
Number of pages of the certificate

2

The user is obliged to have the object recalibrated at appropriate intervals.

Referenzdatum
Reference date

1 January 2001

Dieser Kalibrierschein darf nur vollständig und unverändert weiterverbreitet werden. Auszüge oder Änderungen bedürfen der Genehmigung sowohl der Physikalisch-Technischen Bundesanstalt als auch des ausstellenden Kalibrierlaboratoriums. Kalibrierscheine ohne Unterschrift und Stempel haben keine Gültigkeit.

This calibration certificate may not be reproduced other than in full except with the permission of both the Physikalisch-Technische Bundesanstalt and the issuing laboratory. Calibration certificates without signature and seal are not valid.

Stempel
Seal



Datum
Date

31 January 2001

Leiter des Kalibrierlaboratoriums
Head of the calibration laboratory

Dr. Thieme

Stellvertreter
Deputy

Schott

Bearbeiter
Person in charge

Linke / Schott / Schüler

mm 7/29/05

Reference Solution

Solution no.	FX 248
Drawing	VZ-2058/1
Nuclide	Lead-210
Radioactive concentration	34.2 kBq/g
Reference date	1 January 20001 at 12.00 GMT
Mass of solution	(5.182 ± 0.001) g
Volume of solution	approx. 5 ml
Contamination test	Wipe test according to ISO 9978.
Date of wipe test	30 January 2001
Chemical composition	Solution in 1.2 M HNO ₃ ; Carrier: Pb(NO ₃) ₂ , Bi(NO ₃) ₃ ; each 20 mg/l of the corresponding element.
Measuring method	The activity was determined by comparison with a reference solution by measurement with a Ge-detector with MCA.
Traceability	Additional to the direct traceability to the PTB through the DKD this product complies with the requirements for traceability to NIST specified in the American National Standard "Traceability of Radioactive Sources to the NIST and Associated Instrument Quality Control (ANSI N42.22-1995)". As a requirement of the ANSI N42.22-1995 AEA Technology QSA GmbH participates in the NEI/NIST Measurements Assurance Program of the Nuclear Power Industry.
Uncertainty	The relative uncertainty of the activity is 3 %. The reported uncertainty is based on a standard uncertainty multiplied by a coverage factor k = 2, providing a level of confidence of approximately 95 %. (Ref. NIST Technical Note 1297/"Guide to the Expression of Uncertainty in Measurement" ISO Guide, 1995)
Radioactive impurities	Related to Pb-210 (equal 100 %) the following radioactive impurities were detected: Ra-226: 0.003 %
Quality assurance system	The quality assurance system of AEA Technology QSA GmbH was certified by Lloyd's Register Quality Assurance (LRQA) according to ISO 9001, issue 1994. Isotrak products meet the requirements of 10CFR50 Appendix B in the USA.
Remark	

1297/29/02

Explanations for Certificates (Page 2 of Certificates)

Overall uncertainty

The reported uncertainty is based on standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95 %. (ISO Guide, 1995)

Traceability

This certificate documents the traceability of measurement results to national standards, standard measuring equipment and methods for the realisation of physical units of measurement according to the International System of Units (SI). Traceability is defined as 'the property of a result of a measurement whereby it can be related to appropriate standards, generally International or national standards, through an unbroken chain of comparisons'.

AEA Technology QSA GmbH has been accredited as DKD (Deutscher Kalibrierdienst) calibration laboratory by the Physikalisch-Technische Bundesanstalt (PTB) and is authorized to issue reference sources which are traceable to national standards held at the PTB in Germany. Because of the European co-operation for Accreditation (EA) mutual recognition agreement the certificates are also accepted by all EA-members (e. g. NAMAS, UK).

This product complies with the requirements for traceability to NIST specified in the American National Standard 'Traceability of Radioactive Sources to the NIST and Associated Instrument Quality Control (ANSI N42.22-1995)'. As a requirement for the ANSI N42.22-1995 AEA Technology QSA participates in the NEVNIST Measurements Assurance Program of the Nuclear Power Industry.

Leakage and contamination tests

Stringent tests for leakage are an essential feature of radioactive sources production. They are based on ISO 9978. Some standard methods used for testing radiation sources are listed below.

Wipe test I

The source is wiped with a swab or tissue, moistened with ethanol or water, the activity removed is measured. Limit: 185 Bq

Immersion test II

The source is immersed in a suitable liquid at 50 °C for at least 4 hours and the activity removed is measured. Limit: 185 Bq

Bubble test III

The source is immersed in water or a suitable liquid and the pressure in the vessel reduced to 13 kPa (100 mm Hg). No bubbles must be observed. (This test conforms to ISO 9978 except that for some sources, the 100 mm³ free volume requirement is not met.)

Emanation test IV

The source is placed in a gas tight enclosure with activated carbon as absorber and is left there for at least 3 h. The source is considered leak tight when not more than 185 Bq Radon related to a collection time of 12 h can be measured afterwards.

ISO classification

The International Organization for Standardization (ISO) has proposed a system of classification of sealed radioactive sources based on safety requirements for typical uses (see ISO 2919). This system provides a manufacturer of sealed radioactive sources with a set of tests to evaluate the safety of his products. It also assists a user of such sealed sources to select types which suit the application he has in mind. The tests to which specimen sources are subjected are listed in the following table.

Classification of sealed source performance standard according to ISO 2919

	Class 1	2	3	4	5	6
Temperature	No test	- 40 °C (20 min) + 80 °C (1 h)	- 40 °C (20 min) + 180 °C (1 h)	- 40 °C (20 min) + 400 °C (1 h) and thermal shock 400 °C to 20 °C	- 40 °C (20 min) + 600 °C (1 h) and thermal shock 600 °C to 20 °C	- 40 °C (20 min) + 800 °C (1 h) and thermal shock 800 °C to 20 °C
External Pressure	No test	25 kPa absolute	25 kPa absolute to 2 MPa absolute	25 kPa absolute to 7 MPa absolute	25 kPa absolute to 70 MPa absolute	25 kPa absolute to 170 MPa absolute
Impact	No test	50 g from 1 m	200 g from 1 m	2 kg from 1 m	5 kg from 1 m	20 kg from 1 m
Vibration	No test	3 x 10 min 25 - 500 Hz at 5 g peak amplitude	3 x 10 min 25 - 50 Hz at 5 g peak amplitude and 50 - 90 Hz at 0.635 mm amplitude peak to peak and 90 - 500 Hz at 10 g peak amplitude	3 x 30 min 25 - 80 Hz at 1.5 mm amplitude peak to peak and 80 - 2000 Hz at 20 g peak amplitude		
Puncture	No test	1 g from 1 m	10 g from 1 m	50 g from 1 m	300 g from 1 m	1 kg from 1 m

Special applications

No test programme can cover all possible combinations of environments to which a source may be exposed. Users should therefore consult our experts before using sources in potentially adverse environments.

IAEA Special Form

'Special Form' is a test specification for sealed sources given in the IAEA transport regulations (IAEA Safety Series No. 6, 1985, revised edition). It is used in determining the maximum acceptable activities for various types of transport containers.

Quality assurance system

The quality assurance system of AEA Technology QSA GmbH was certified by Lloyd's Register Quality Assurance (LRQA) according to ISO 9001, issue 1994. Isotrak products meet the requirements of 10CFR50 Appendix B.



ms/ector





Standard Traceability Log Rad

Source Material Info	
Parent Code:	0356
Prepared By:	Angela Albee
Carrier Conc:	1.2M HNO3
Reference Date:	01/01/2001
Ampoule Mass (g):	5.182 g
Uncertainty:	+/- 3 %
LogBook No:	RC S 034 16b

A Solution Material Info	
Isotope:	Lead-210
Prepared By:	Angela Albee
Prep Date:	04/03/2001
Verification Date:	07/12/2005
Expiration Date:	07/12/2006
Primary Code:	0356-A
Dilution(mL):	100 mL
Mass of Parent(g):	4.275 g
Density(g/mL):	1.0290

Calculations Converting parent activity to dpm/mL/dpm/g

$(\text{Mass of parent(g)}) * (\text{Parm Activity (kBq/g)}) * (\text{conversion dpm to kBq}) / (\text{Dilution Vol}) = \text{Parent Activity (dpm/mL)}$
$(\text{Mass of parent(g)}) * (\text{Parm Activity (kBq/g)}) * (\text{conversion dpm to kBq}) / \text{Density (g/mL)} / (\text{Dilution Vol}) = \text{Parent Activity (dpm/g)}$
$(4.275 \text{ g}) * (34.2 \text{ kBq/g}) * (60000 \text{ dpm/kBq}) / (100 \text{ mL}) = 87723.0000 \text{ dpm/mL}$
$(4.275 \text{ g}) * (34.2 \text{ kBq/g}) * (60000 \text{ dpm/kBq}) / (1.0290 \text{ g/mL}) / (100 \text{ mL}) = 85250.5630 \text{ dpm/g}$

Secondary Standards

Prep Date	Preparer	Mass Primary	Dilution (mL)	Code	Conc dpm/mL	Verification Date	Expiration Date
-----------	----------	--------------	---------------	------	-------------	-------------------	-----------------

General Engineering Laboratories, LLC
Version 1.0 9/18/2000

Angela Albee

Verification for Pb-210 Standard 0356-A

A.Fehr 7/12/2005		Standard			
Isotope	Detector CPM	BKG CPM	NET CPM	Detector Eff Mass. Used (mL)	Source DPM/mL
0356-A N1	20294.0000	21.7000	20294.0000	0.1000	76051.19747
0356-A N2	20276.6000	21.7000	20276.6000	0.1000	75985.99146
0356-A N3	20079.7000	21.7000	20079.7000	0.1000	75248.11421
Mean Value (Counting) =			99.4402909	Average =	
Stdev =			0.00588727	75761.76771	

Mean Value (Counting) = 75761.76771 dpm/g Pass
 Stdev = 446.03015 dpm/g Rule 3 (Pass/Fail)

Certificate Value = 76188.2 dpm/g
 Lower Limit = 74869.70741 dpm/g
 Upper Limit = 76653.82801 dpm/g
 Rule 1 Pass/Fail Pass
 Two sigma = 892.0603001
 10 % of Mean = 7576.176771
 Rule 2 (Pass/Fail) Pass

Verification Rules

- Rule 1 = The certificate value (NOT including any uncertainty) shall lie within the 95% confidence interval determined from the mean and two sigma standard deviation of the three measurements
- Rule 2 = The two sigma value used for the 95% confidence interval shall not exceed 10% of the mean value of the three verification measurements.
- Rule 3 = The determined mean value shall be within 10% of the certificate value.

The analyst prepared three calibration sources for source 0356-A by transferring portions of the standard to tared glass liquid scintillation vials. Ten mL of Ready Gel liquid scintillation cocktail was added to each vial and the vials were shaken to mix. A Blank vial was prepared in a similar fashion using 1 mL of DI water and 10 mL of Ready Gel cocktail. The calibration vials and background source were dark adapted for two hours and counted on LSC Yellow (Wallac) using Protocol 31 for Pb-210 standard verification. The efficiency calibration which was used for verification calculations was performed on 7/12/05 using source ET491-A (Pb-210). Each verification source calculation was performed as follows:

$$\text{Source dpm/g} = (A - B)/(C)(D)$$

where:

- A = Ver. source cpm,
- B = BKG cpm,
- C = System efficiency, (cpm/dpm), and
- D = mass used for standard verification.

mm/halor

Angela D. Johnson 7/29/05

PROTOCOL : 31 Pb-210 Verification
DATE : 2005/07/12
TIME : 05:29
ID : P31AS005


Wallac 1414 WinSpectral v1.40 S/N 4140127
Counting mode : CPM
Isotope(s) : Pb210
Pb210 = 5- 520,21.00 y
Protocol name : Pb-210 Verification
Counting time : 300
Repeats : 1
Cycles : 1
Replicates : 1
2 sigma % : 0.01
Minimum cpm : 0.00 Checking time: 10
Advanced modes : Chemilum,PSA
PSA level : 35
Output to Display :
POS,CTIME,DATE,TIME,RACKPOS,CPMw1,CPM,SQPI,CPM1
Additions to Display : Spectrum,Header,Listing
Spectrum : Alpha,Beta
Window 1 : 685- 745 /Alpha
Window 2 : 1-1024 /Beta
Window 3 : 1-1024 /Beta
Window 4 : 1-1024 /Beta
Window 5 : 1-1024 /Beta
Window 6 : 1-1024 /Beta
FNCT1 = FNCT1 :
FNCT2 = FNCT2 :
FNCT3 = FNCT3 :
FNCT4 = FNCT4 :

Total count rate:
Pb210 72372.3 CPM

per 1/2/05
Oct 7/12/05

AAQ
7/29/05

POS	CTIME	DATE	TIME	RACKPOS	CPM
1	300	7/12/2005	5:29 AM	1	20.20

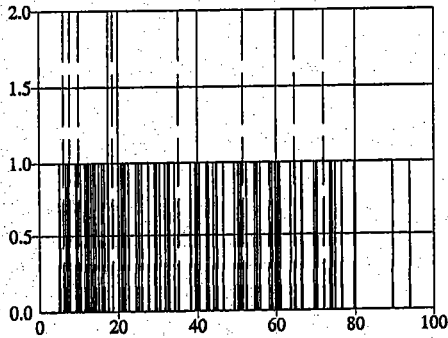


Counts Alpha

Counts Beta

Bkg

2	300	7/12/2005	5:35 AM	2	22785.60
---	-----	-----------	---------	---	----------

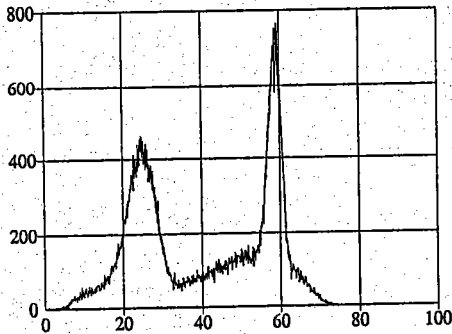


Counts Alpha

Counts Beta

ET491-A

3	300	7/12/2005	5:41 AM	3	22178.60
---	-----	-----------	---------	---	----------

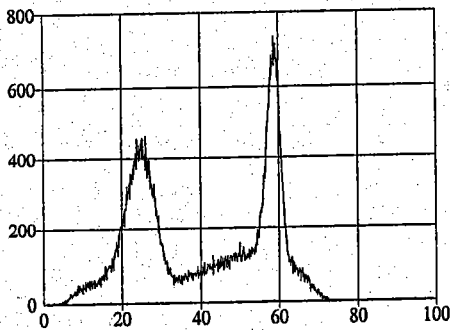

Counts Alpha

Counts Beta


ET491-A

ms 7/29/05

ALF 7/12/05

AdQ
7/29/05

POS	CTIME	DATE	TIME	RACKPOS	CPM
4	300	7/12/2005	5:46 AM	4	22065.70

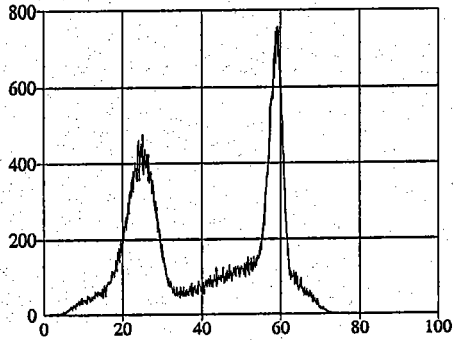


Counts Alpha

Counts Beta

ET491-A

5	300	7/12/2005	5:52 AM	5	21.70
---	-----	-----------	---------	---	-------

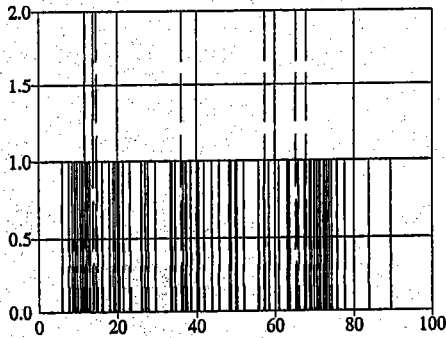


Counts Alpha

Counts Beta

Bkg

6	300	7/12/2005	5:58 AM	6	20294.00
---	-----	-----------	---------	---	----------

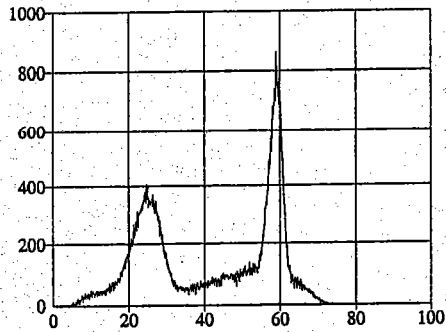

Counts Alpha

Counts Beta


0356-A

ms/rales

ALF7/12/05

ms/rales
7/29/05

POS	CTIME	DATE	TIME	RACKPOS	CPM
7	300	7/12/2005	6:04 AM	7	20276.60

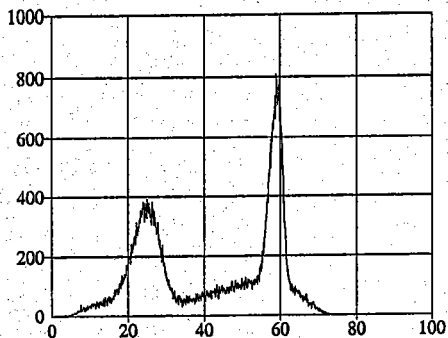


Counts Alpha

Counts Beta

0356-A

8	300	7/12/2005	6:09 AM	8	20079.70
---	-----	-----------	---------	---	----------

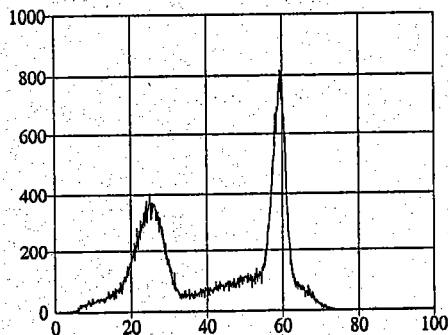

Counts Alpha

Counts Beta

0356-A

pm 7/29/05
ALF 7/12/05

ALF
7/29/05

**General Engineering Laboratories
Calibration Source Preparation Sheet**

Applicable SOP Number GL-RAD-A-018 Isotope Pb-210
 Date Standards Prepared 7/14/05 Cocktail Type Used NA
 Standard ID 0356-A Matrix of Vial/Planchett Lead chromate precipitate on Tuffryn filter
 Amount Used (g or ml) 0.5 Type of Scintillation Vial N/A
 Standard Activity (DPM/g or ml) 87723 Pipette ID Used 2440913
 Reference Date 11/1/05 Balance ID Used R 12/1/04
 Expiration Date 7/12/06 Residue/Carrier Agent Lead Carrier 14.65 μ g/ml Quenching Agent N/A

Separation Date / Time: 7/14/05 0800

Standard Number	Quenching Vol (uL)/ Residue Volume(mL)	Initial Wt. (g)	Final Wt. (g)	Net Wt. (mg)
C1	0.1	0.0844	0.0850	0.6
C2	0.2	0.0851	0.0865	1.4
C3	0.3	0.0845	0.0880	3.5
C4	0.4	0.0849	0.0913	6.4
C5	0.5	0.0847	0.0926	7.9
C6	0.6	0.0874	0.0975	10.1
C7	0.7	0.0860	0.0950	9.0
C8	0.8	0.0879	0.1000	12.1
C9	0.9	0.0846	0.0966	12.0
C10	1.0	0.0852	0.1000	14.8
C11	1.1	0.0841	0.1010	16.9
C12	1.3	0.0865	0.1033	18.8
		0.0850	0.1053	
		7/13/05		

0.0854 1.0
0.0875 2.4

Prepared By: [Signature] Date 7/22/05
 Reviewed By: [Signature] Date 7/26/05

INSTR_ID	SAMPLE_ID	CNT_TIME	A	B	TIME	USER2	BATCH_ID
Instrument 1 - A	1	2	84	22018	7/28/2005 7:55	1575	PbCal705
Instrument 1 - A	2	2	84	22854	7/28/2005 8:20	1575	PbCal705
Instrument 1 - A	3	2	102	20935	7/28/2005 8:05	1575	PbCal705
Instrument 1 - A	4	2	99	22720	7/28/2005 8:01	1575	PbCal705
Instrument 1 - A	5	2	95	22892	7/28/2005 10:09	1575	PbCal705
Instrument 1 - A	6	2	83	23217	7/28/2005 10:25	1575	PbCal705
Instrument 1 - A	7	2	63	19193	7/28/2005 10:20	1575	PbCal705
Instrument 1 - A	8	2	78	20620	7/28/2005 10:16	1575	PbCal705
Instrument 1 - A	9	2	65	18730	7/28/2005 9:35	1575	PbCal705
Instrument 1 - A	10	2	73	20335	7/28/2005 10:06	1575	PbCal705
Instrument 1 - A	11	2	81	19694	7/28/2005 10:02	1575	PbCal705
Instrument 1 - A	12	2	89	20801	7/28/2005 9:43	1575	PbCal705
Instrument 1 - B	1	2	56	21763	7/28/2005 8:01	1575	PbCal705
Instrument 1 - B	2	2	78	22474	7/28/2005 7:55	1575	PbCal705
Instrument 1 - B	3	2	73	20359	7/28/2005 8:20	1575	PbCal705
Instrument 1 - B	4	2	58	22111	7/28/2005 8:05	1575	PbCal705
Instrument 1 - B	5	2	71	23056	7/28/2005 10:16	1575	PbCal705
Instrument 1 - B	6	2	72	22905	7/28/2005 10:09	1575	PbCal705
Instrument 1 - B	7	2	62	18664	7/28/2005 10:25	1575	PbCal705
Instrument 1 - B	8	2	56	20619	7/28/2005 10:21	1575	PbCal705
Instrument 1 - B	9	2	62	18705	7/28/2005 9:43	1575	PbCal705
Instrument 1 - B	10	2	45	19770	7/28/2005 9:35	1575	PbCal705
Instrument 1 - B	11	2	42	19125	7/28/2005 10:06	1575	PbCal705
Instrument 1 - B	12	2	56	20230	7/28/2005 10:02	1575	PbCal705
Instrument 1 - C	1	2	132	22038	7/28/2005 8:06	1575	PbCal705
Instrument 1 - C	2	2	151	22700	7/28/2005 8:01	1575	PbCal705
Instrument 1 - C	3	2	161	20552	7/28/2005 7:55	1575	PbCal705
Instrument 1 - C	4	2	179	22690	7/28/2005 8:20	1575	PbCal705
Instrument 1 - C	5	2	149	23030	7/28/2005 10:21	1575	PbCal705
Instrument 1 - C	6	2	163	22975	7/28/2005 10:16	1575	PbCal705
Instrument 1 - C	7	2	137	19131	7/28/2005 10:09	1575	PbCal705
Instrument 1 - C	8	2	136	20712	7/28/2005 10:25	1575	PbCal705
Instrument 1 - C	9	2	132	19007	7/28/2005 10:02	1575	PbCal705
Instrument 1 - C	10	2	129	20055	7/28/2005 9:43	1575	PbCal705
Instrument 1 - C	11	2	110	19004	7/28/2005 9:35	1575	PbCal705
Instrument 1 - C	12	2	125	20586	7/28/2005 10:06	1575	PbCal705
Instrument 1 - D	1	2	314	21985	7/28/2005 8:20	1575	PbCal705
Instrument 1 - D	2	2	339	22577	7/28/2005 8:06	1575	PbCal705
Instrument 1 - D	3	2	302	20759	7/28/2005 8:01	1575	PbCal705
Instrument 1 - D	4	2	337	22777	7/28/2005 7:55	1575	PbCal705
Instrument 1 - D	5	2	299	23052	7/28/2005 10:25	1575	PbCal705
Instrument 1 - D	6	2	273	22954	7/28/2005 10:21	1575	PbCal705
Instrument 1 - D	7	2	234	19018	7/28/2005 10:16	1575	PbCal705
Instrument 1 - D	8	2	275	20545	7/28/2005 10:09	1575	PbCal705
Instrument 1 - D	9	2	253	18798	7/28/2005 10:06	1575	PbCal705
Instrument 1 - D	10	2	272	20117	7/28/2005 10:02	1575	PbCal705
Instrument 1 - D	11	2	259	19117	7/28/2005 9:43	1575	PbCal705
Instrument 1 - D	12	2	229	20856	7/28/2005 9:35	1575	PbCal705
Instrument 2 - A	1	2	225	21853	7/28/2005 8:42	1575	PbCal705
Instrument 2 - A	2	2	264	22781	7/28/2005 9:21	1575	PbCal705
Instrument 2 - A	3	2	246	20682	7/28/2005 8:52	1575	PbCal705

Instrument 2 - A	4	2	230	22878	7/28/2005 8:49	1575	PbCal705
Instrument 2 - A	5	2	266	23137	7/28/2005 7:55	1575	PbCal705
Instrument 2 - A	6	2	231	23217	7/28/2005 8:20	1575	PbCal705
Instrument 2 - A	7	2	172	19166	7/28/2005 8:06	1575	PbCal705
Instrument 2 - A	8	2	193	20672	7/28/2005 8:01	1575	PbCal705
Instrument 2 - A	9	2	201	19025	7/28/2005 10:09	1575	PbCal705
Instrument 2 - A	10	2	188	20237	7/28/2005 10:25	1575	PbCal705
Instrument 2 - A	11	2	194	19477	7/28/2005 10:21	1575	PbCal705
Instrument 2 - A	12	2	193	20724	7/28/2005 10:17	1575	PbCal705
Instrument 2 - B	1	2	9	22048	7/28/2005 8:49	1575	PbCal705
Instrument 2 - B	2	2	15	23045	7/28/2005 8:42	1575	PbCal705
Instrument 2 - B	3	2	16	20750	7/28/2005 9:21	1575	PbCal705
Instrument 2 - B	4	2	9	22958	7/28/2005 8:52	1575	PbCal705
Instrument 2 - B	5	2	12	23347	7/28/2005 8:01	1575	PbCal705
Instrument 2 - B	6	2	12	22888	7/28/2005 7:55	1575	PbCal705
Instrument 2 - B	7	2	12	19018	7/28/2005 8:20	1575	PbCal705
Instrument 2 - B	8	2	9	20774	7/28/2005 8:06	1575	PbCal705
Instrument 2 - B	9	2	12	18915	7/28/2005 10:17	1575	PbCal705
Instrument 2 - B	10	2	10	20157	7/28/2005 10:10	1575	PbCal705
Instrument 2 - B	11	2	14	19263	7/28/2005 10:25	1575	PbCal705
Instrument 2 - B	12	2	8	20483	7/28/2005 10:21	1575	PbCal705
Instrument 2 - C	1	2	280	21996	7/28/2005 8:52	1575	PbCal705
Instrument 2 - C	2	2	292	22508	7/28/2005 8:49	1575	PbCal705
Instrument 2 - C	3	2	244	20689	7/28/2005 8:42	1575	PbCal705
Instrument 2 - C	4	2	283	22518	7/28/2005 9:21	1575	PbCal705
Instrument 2 - C	5	2	264	23133	7/28/2005 8:06	1575	PbCal705
Instrument 2 - C	6	2	268	22568	7/28/2005 8:01	1575	PbCal705
Instrument 2 - C	7	2	240	18943	7/28/2005 7:55	1575	PbCal705
Instrument 2 - C	8	2	239	20584	7/28/2005 8:20	1575	PbCal705
Instrument 2 - C	9	2	222	18740	7/28/2005 10:21	1575	PbCal705
Instrument 2 - C	10	2	222	19943	7/28/2005 10:17	1575	PbCal705
Instrument 2 - C	11	2	221	19199	7/28/2005 10:10	1575	PbCal705
Instrument 2 - C	12	2	234	20523	7/28/2005 10:25	1575	PbCal705
Instrument 2 - D	1	2	280	22194	7/28/2005 9:21	1575	PbCal705
Instrument 2 - D	2	2	338	23021	7/28/2005 8:53	1575	PbCal705
Instrument 2 - D	3	2	288	20861	7/28/2005 8:49	1575	PbCal705
Instrument 2 - D	4	2	282	22714	7/28/2005 8:42	1575	PbCal705
Instrument 2 - D	5	2	254	23276	7/28/2005 8:20	1575	PbCal705
Instrument 2 - D	6	2	282	23097	7/28/2005 8:06	1575	PbCal705
Instrument 2 - D	7	2	232	19264	7/28/2005 8:02	1575	PbCal705
Instrument 2 - D	8	2	274	21105	7/28/2005 7:55	1575	PbCal705
Instrument 2 - D	9	2	221	19341	7/28/2005 10:25	1575	PbCal705
Instrument 2 - D	10	2	250	20334	7/28/2005 10:21	1575	PbCal705
Instrument 2 - D	11	2	210	19513	7/28/2005 10:17	1575	PbCal705
Instrument 2 - D	12	2	241	20672	7/28/2005 10:10	1575	PbCal705
Instrument 3 - A	1	2	151	21669	7/28/2005 9:34	1575	PbCal705
Instrument 3 - A	2	2	140	21967	7/28/2005 10:05	1575	PbCal705
Instrument 3 - A	3	2	151	20088	7/28/2005 10:01	1575	PbCal705
Instrument 3 - A	4	2	162	21796	7/28/2005 9:42	1575	PbCal705
Instrument 3 - A	5	2	165	22294	7/28/2005 8:42	1575	PbCal705
Instrument 3 - A	6	2	180	22353	7/28/2005 9:21	1575	PbCal705
Instrument 3 - A	7	2	95	18346	7/28/2005 8:53	1575	PbCal705

M 7/29/05


Instrument 3 - A	8	2	136	19841	7/28/2005 8:49	1575	PbCal705
Instrument 3 - A	9	2	104	18127	7/28/2005 7:56	1575	PbCal705
Instrument 3 - A	10	2	176	19341	7/28/2005 8:20	1575	PbCal705
Instrument 3 - A	11	2	120	18537	7/28/2005 8:06	1575	PbCal705
Instrument 3 - A	12	2	142	20233	7/28/2005 8:02	1575	PbCal705
Instrument 3 - B	1	2	236	21613	7/28/2005 9:42	1575	PbCal705
Instrument 3 - B	2	2	219	22011	7/28/2005 9:34	1575	PbCal705
Instrument 3 - B	3	2	220	20493	7/28/2005 10:05	1575	PbCal705
Instrument 3 - B	4	2	235	22109	7/28/2005 10:01	1575	PbCal705
Instrument 3 - B	5	2	244	22536	7/28/2005 8:49	1575	PbCal705
Instrument 3 - B	6	2	221	22658	7/28/2005 8:42	1575	PbCal705
Instrument 3 - B	7	2	207	18626	7/28/2005 9:21	1575	PbCal705
Instrument 3 - B	8	2	216	20102	7/28/2005 8:53	1575	PbCal705
Instrument 3 - B	9	2	188	18433	7/28/2005 8:02	1575	PbCal705
Instrument 3 - B	10	2	228	19517	7/28/2005 7:56	1575	PbCal705
Instrument 3 - B	11	2	189	19126	7/28/2005 8:20	1575	PbCal705
Instrument 3 - B	12	2	205	20505	7/28/2005 8:06	1575	PbCal705
Instrument 3 - C	1	2	322	21556	7/28/2005 10:01	1575	PbCal705
Instrument 3 - C	2	2	360	22173	7/28/2005 9:43	1575	PbCal705
Instrument 3 - C	3	2	329	20388	7/28/2005 9:34	1575	PbCal705
Instrument 3 - C	4	2	326	22168	7/28/2005 10:05	1575	PbCal705
Instrument 3 - C	5	2	338	23046	7/28/2005 8:53	1575	PbCal705
Instrument 3 - C	6	2	378	22957	7/28/2005 8:49	1575	PbCal705
Instrument 3 - C	7	2	283	18866	7/28/2005 8:42	1575	PbCal705
Instrument 3 - C	8	2	308	20233	7/28/2005 9:21	1575	PbCal705
Instrument 3 - C	9	2	291	18650	7/28/2005 8:06	1575	PbCal705
Instrument 3 - C	10	2	305	19515	7/28/2005 8:02	1575	PbCal705
Instrument 3 - C	11	2	290	19302	7/28/2005 7:56	1575	PbCal705
Instrument 3 - C	12	2	318	20119	7/28/2005 8:20	1575	PbCal705
Instrument 3 - D	1	2	244	21693	7/28/2005 10:05	1575	PbCal705
Instrument 3 - D	2	2	239	22623	7/28/2005 10:01	1575	PbCal705
Instrument 3 - D	3	2	241	20563	7/28/2005 9:43	1575	PbCal705
Instrument 3 - D	4	2	244	22484	7/28/2005 9:34	1575	PbCal705
Instrument 3 - D	5	2	258	23049	7/28/2005 9:21	1575	PbCal705
Instrument 3 - D	6	2	262	22650	7/28/2005 8:53	1575	PbCal705
Instrument 3 - D	7	2	196	19014	7/28/2005 8:50	1575	PbCal705
Instrument 3 - D	8	2	234	20041	7/28/2005 8:42	1575	PbCal705
Instrument 3 - D	9	2	213	18822	7/28/2005 8:20	1575	PbCal705
Instrument 3 - D	10	2	239	19800	7/28/2005 8:06	1575	PbCal705
Instrument 3 - D	11	2	221	18990	7/28/2005 8:02	1575	PbCal705
Instrument 3 - D	12	2	234	20049	7/28/2005 7:56	1575	PbCal705
Instrument 4 - A	1	2	179	22048	7/28/2005 10:09	1575	PbCal705
Instrument 4 - A	2	2	167	22217	7/28/2005 10:24	1575	PbCal705
Instrument 4 - A	3	2	149	20830	7/28/2005 10:20	1575	PbCal705
Instrument 4 - A	4	2	133	22551	7/28/2005 10:16	1575	PbCal705
Instrument 4 - A	5	2	137	23240	7/28/2005 9:34	1575	PbCal705
Instrument 4 - A	6	2	164	22718	7/28/2005 10:05	1575	PbCal705
Instrument 4 - A	7	2	130	19096	7/28/2005 10:01	1575	PbCal705
Instrument 4 - A	8	2	139	20375	7/28/2005 9:43	1575	PbCal705
Instrument 4 - A	9	2	126	18833	7/28/2005 8:42	1575	PbCal705
Instrument 4 - A	10	2	128	20217	7/28/2005 9:21	1575	PbCal705
Instrument 4 - A	11	2	149	19209	7/28/2005 8:53	1575	PbCal705

Instrument 4 - A	12	2	141	20634	7/28/2005 8:50	1575	PbCal705
Instrument 4 - B	1	2	19	22035	7/28/2005 10:16	1575	PbCal705
Instrument 4 - B	2	2	17	22750	7/28/2005 10:09	1575	PbCal705
Instrument 4 - B	3	2	21	21081	7/28/2005 10:24	1575	PbCal705
Instrument 4 - B	4	2	19	22859	7/28/2005 10:20	1575	PbCal705
Instrument 4 - B	5	2	19	23403	7/28/2005 9:43	1575	PbCal705
Instrument 4 - B	6	2	24	23177	7/28/2005 9:34	1575	PbCal705
Instrument 4 - B	7	2	13	19259	7/28/2005 10:05	1575	PbCal705
Instrument 4 - B	8	2	16	20883	7/28/2005 10:01	1575	PbCal705
Instrument 4 - B	9	2	12	19153	7/28/2005 8:50	1575	PbCal705
Instrument 4 - B	10	2	15	20262	7/28/2005 8:42	1575	PbCal705
Instrument 4 - B	11	2	23	19727	7/28/2005 9:21	1575	PbCal705
Instrument 4 - B	12	2	23	20878	7/28/2005 8:53	1575	PbCal705
Instrument 4 - C	1	2	249	22116	7/28/2005 10:20	1575	PbCal705
Instrument 4 - C	2	2	278	22252	7/28/2005 10:16	1575	PbCal705
Instrument 4 - C	3	2	254	20864	7/28/2005 10:09	1575	PbCal705
Instrument 4 - C	4	2	272	22535	7/28/2005 10:24	1575	PbCal705
Instrument 4 - C	5	2	272	23428	7/28/2005 10:02	1575	PbCal705
Instrument 4 - C	6	2	262	23097	7/28/2005 9:43	1575	PbCal705
Instrument 4 - C	7	2	208	19113	7/28/2005 9:35	1575	PbCal705
Instrument 4 - C	8	2	217	20633	7/28/2005 10:05	1575	PbCal705
Instrument 4 - C	9	2	233	18843	7/28/2005 8:53	1575	PbCal705
Instrument 4 - C	10	2	209	20281	7/28/2005 8:50	1575	PbCal705
Instrument 4 - C	11	2	244	19412	7/28/2005 8:43	1575	PbCal705
Instrument 4 - C	12	2	239	20691	7/28/2005 9:21	1575	PbCal705
Instrument 4 - D	1	2	522	21545	7/28/2005 10:25	1575	PbCal705
Instrument 4 - D	2	2	521	22295	7/28/2005 10:20	1575	PbCal705
Instrument 4 - D	3	2	520	20598	7/28/2005 10:16	1575	PbCal705
Instrument 4 - D	4	2	528	22522	7/28/2005 10:09	1575	PbCal705
Instrument 4 - D	5	2	519	23125	7/28/2005 10:05	1575	PbCal705
Instrument 4 - D	6	2	539	23225	7/28/2005 10:02	1575	PbCal705
Instrument 4 - D	7	2	422	18621	7/28/2005 9:43	1575	PbCal705
Instrument 4 - D	8	2	490	20410	7/28/2005 9:35	1575	PbCal705
Instrument 4 - D	9	2	450	18857	7/28/2005 9:21	1575	PbCal705
Instrument 4 - D	10	2	477	20057	7/28/2005 8:53	1575	PbCal705
Instrument 4 - D	11	2	424	19123	7/28/2005 8:50	1575	PbCal705
Instrument 4 - D	12	2	484	20501	7/28/2005 8:43	1575	PbCal705

Pb-210 Efficiency Curve 7/05

Instrument 1

+ 1-A Δ 1-B ○ 1-C + 1-D

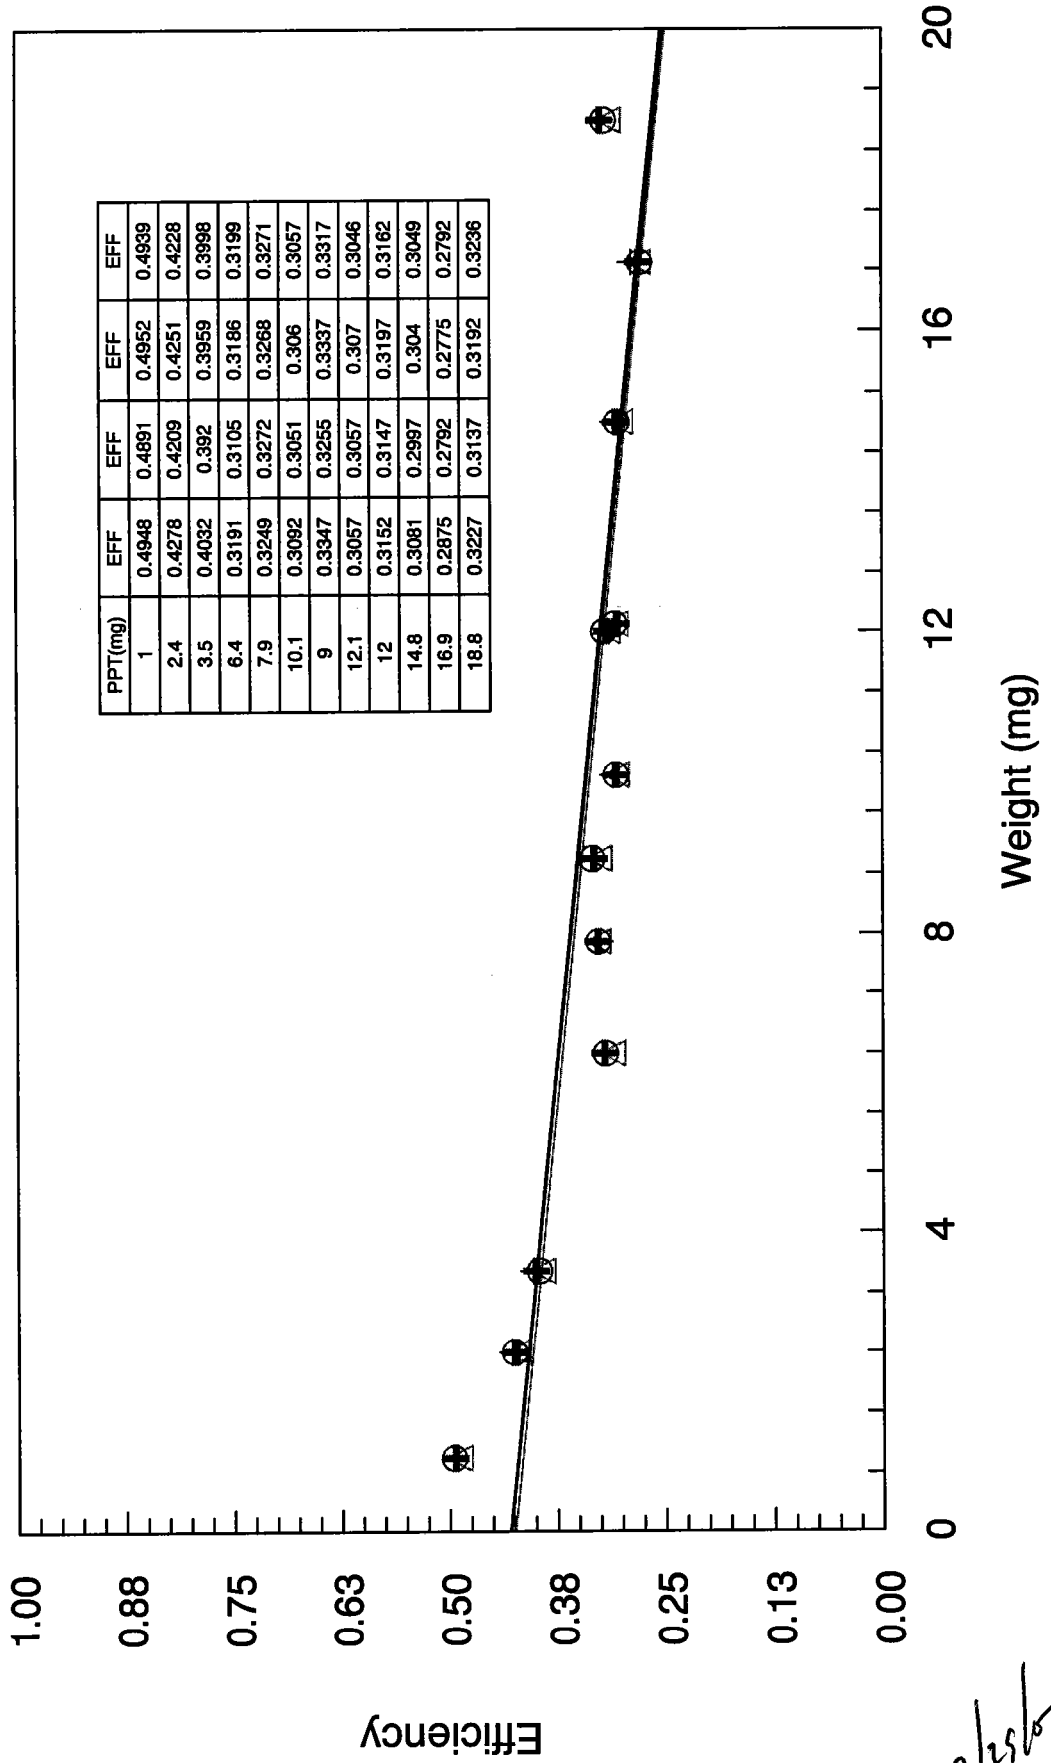


Handwritten signature/initials

Pb-210 Efficiency Curve 7/05

Instrument 2

+ 2-A △ 2-B ○ 2-C + 2-D

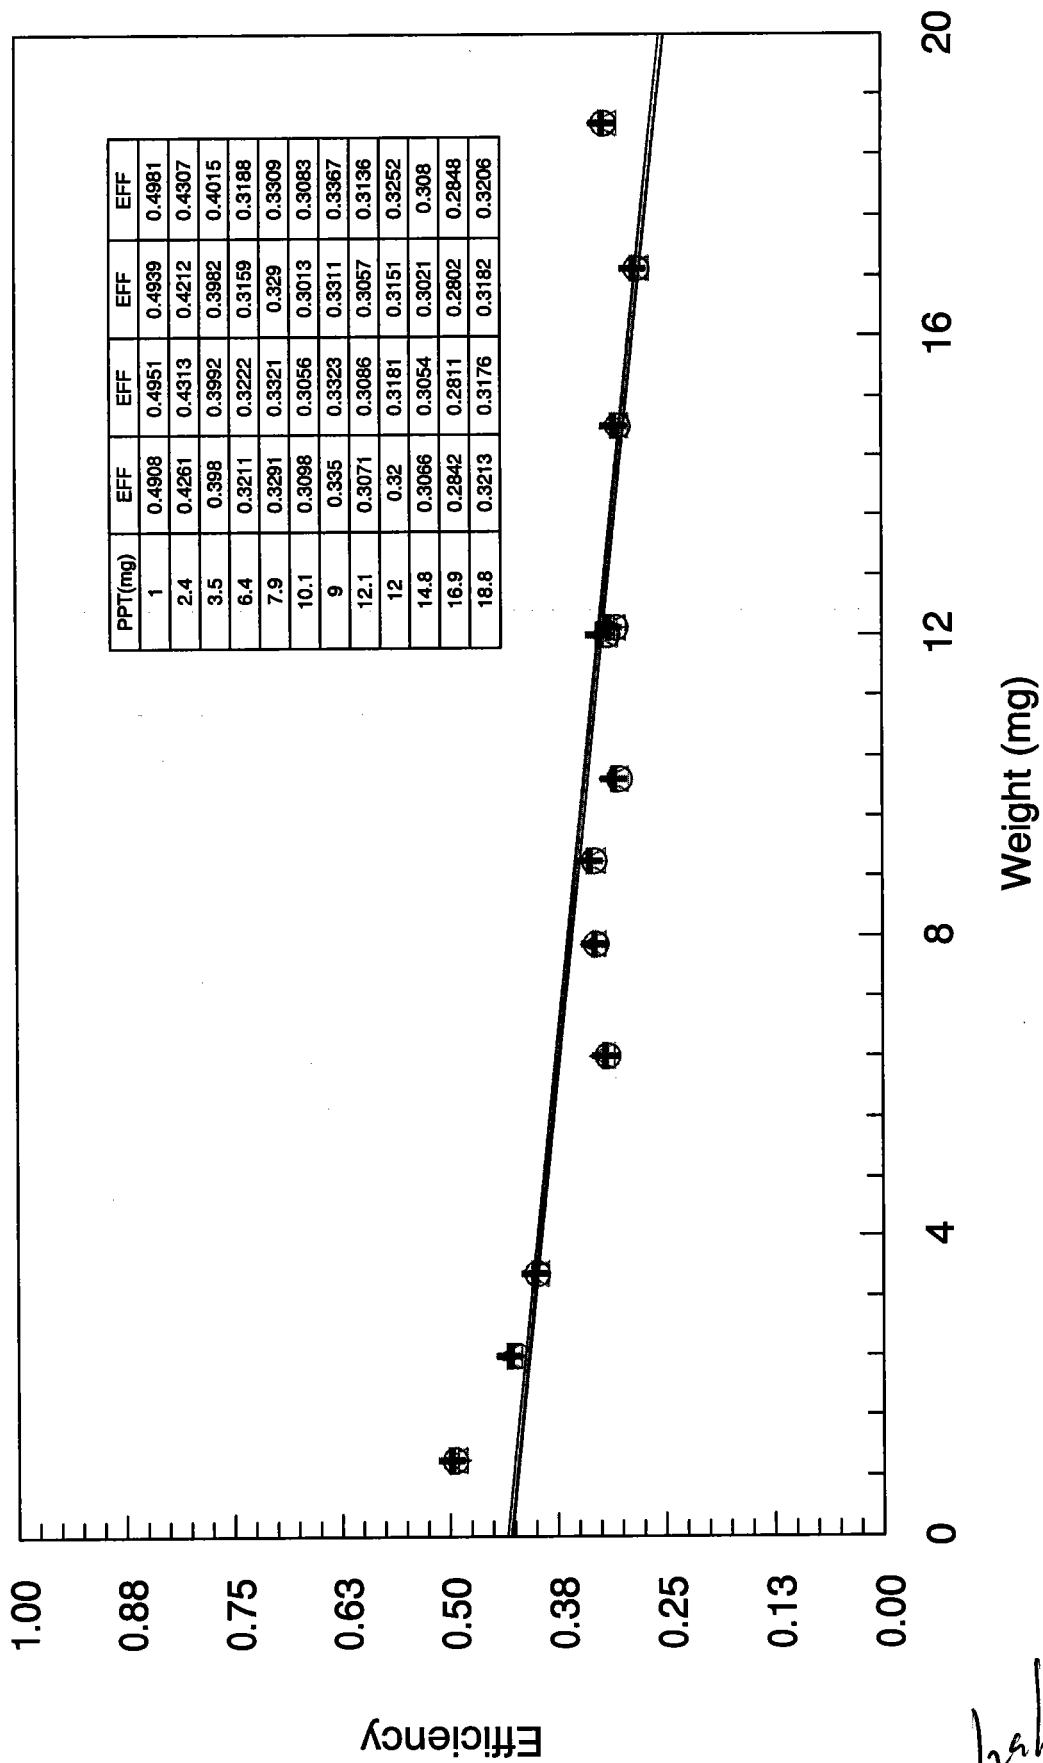


Handwritten signature

Pb-210 Efficiency Curve 7/05

Instrument 3

+ 3-A Δ 3-B ○ 3-C + 3-D

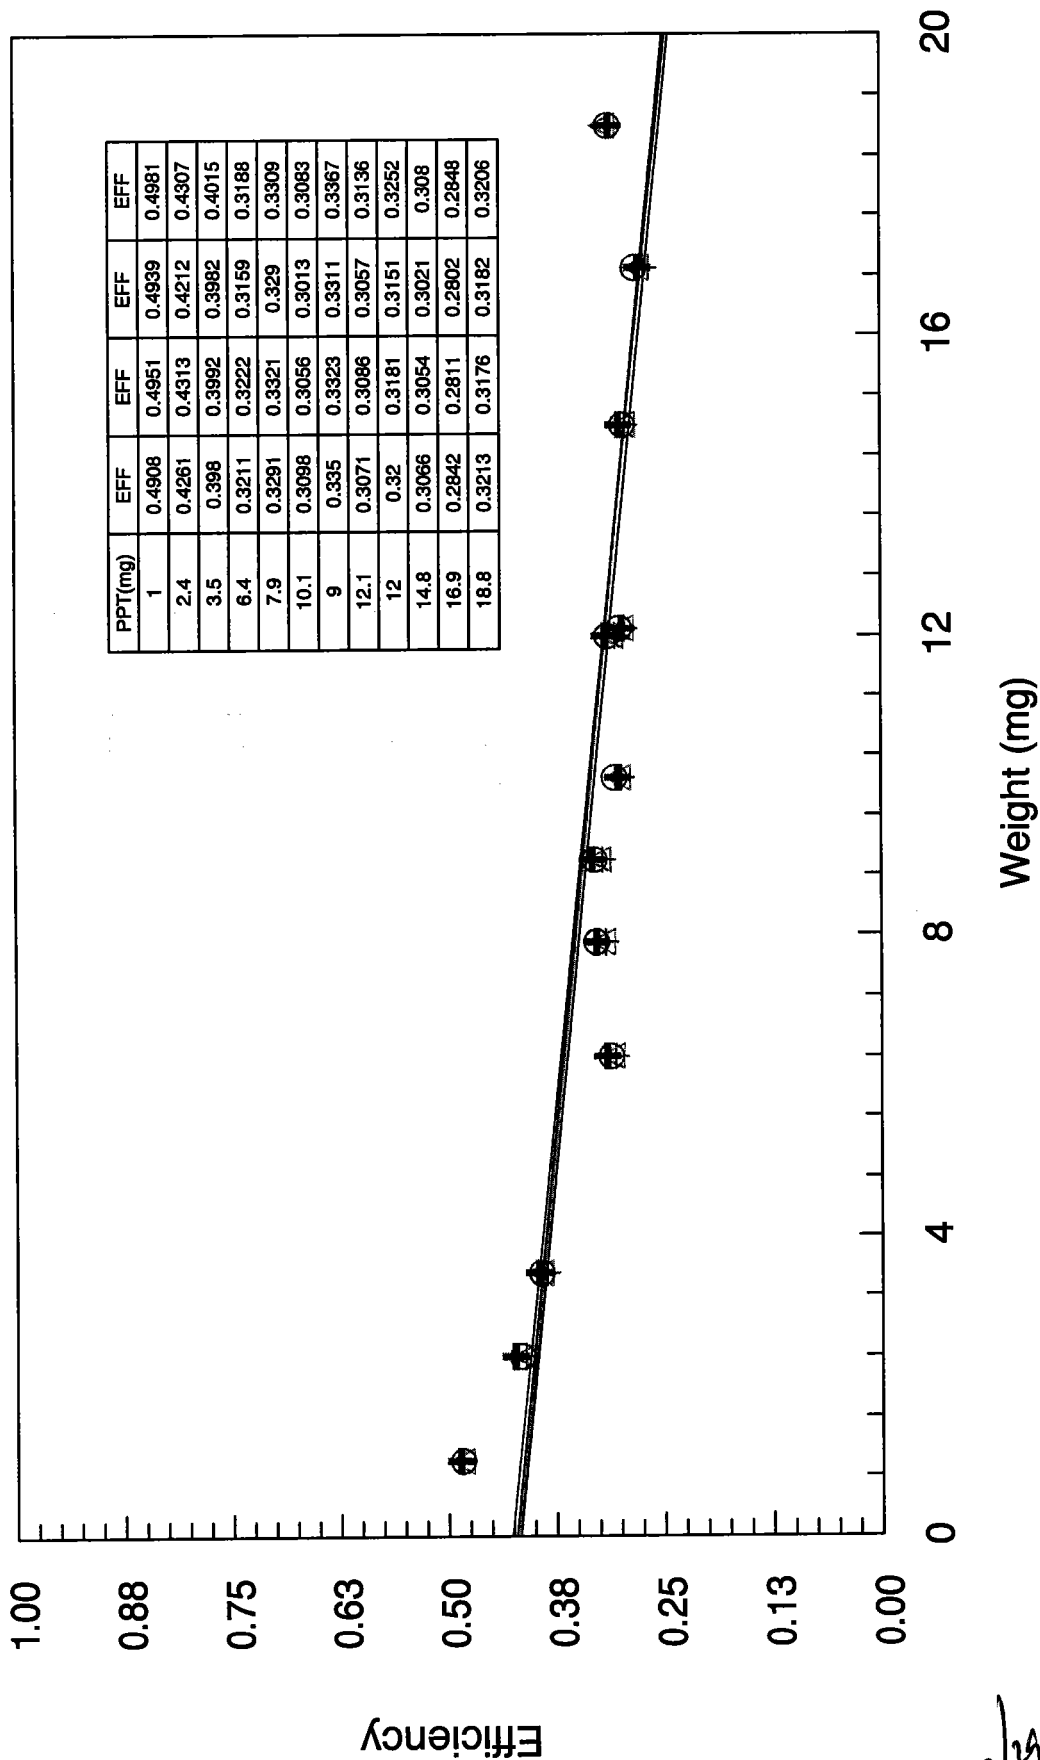


Handwritten signature


Pb-210 Efficiency Curve 7/05

Instrument 4

+ 4-A Δ 4-B ○ 4-C + 4-D

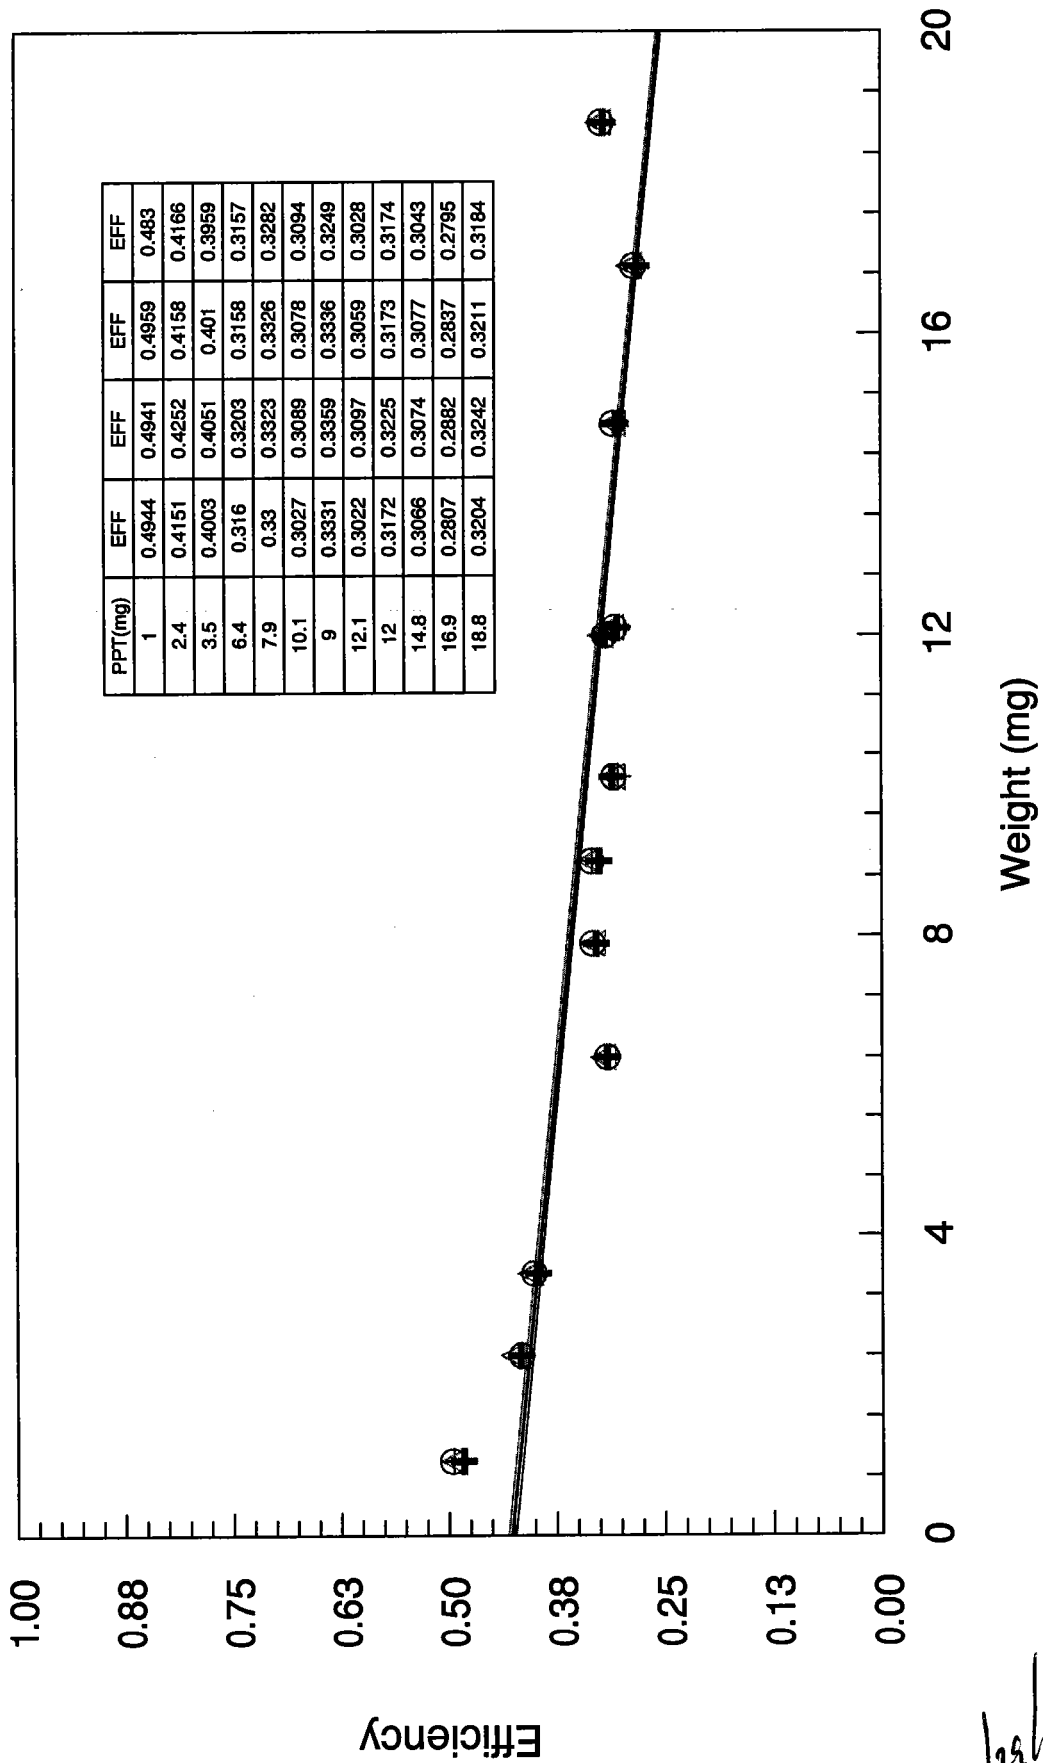


7/2/05

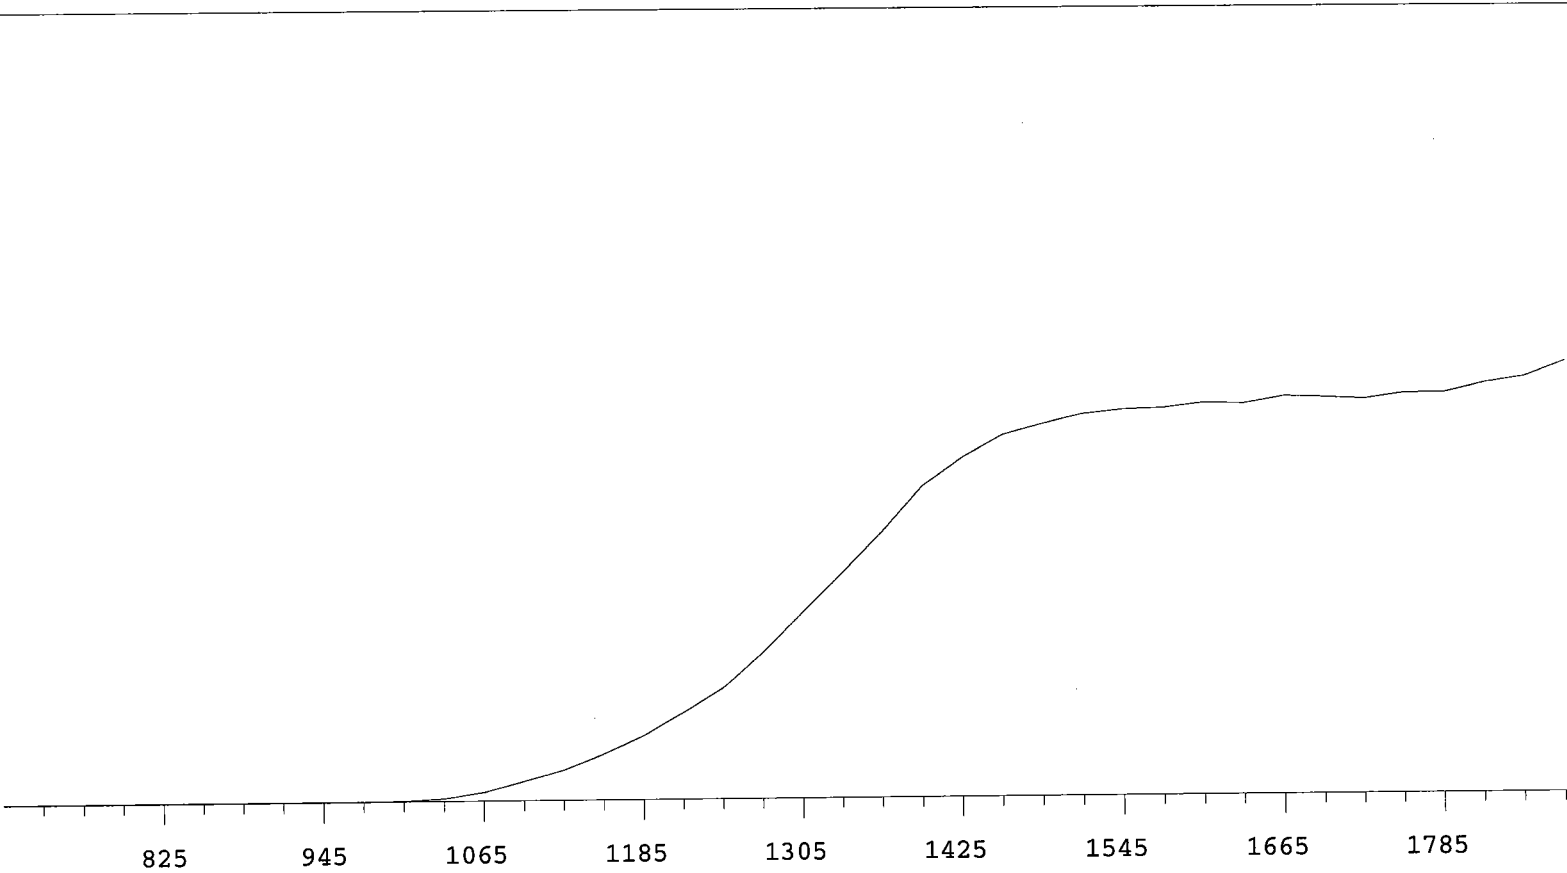


VOLTS	COUNTS	%/100 Volts	VOLTS	COUNTS	%/100 Volts
705	3		1305	16206	+70.03
735	1		1335	19739	+60.77
765	1	-18.52	1365	23317	+49.57
795	2	>100	1395	27238	+38.47
825	2	+76.92	1425	29745	+26.87
855	6	+0.00	1455	31733	+16.81
885	2	+0.00	1485	32738	+10.51
915	2	+0.00	1515	33561	+5.83
945	4	>100	1545	33929	+3.90
975	5	>100	1575	34042	+2.13
1005	45	>100	1605	34473	+2.40
1035	260	>100	1635	34376	+2.14
1065	800	>100	1665	34998	+0.99
1095	1706	>100	1695	34891	+1.35
1125	2681	>100	1725	34732	+0.78
1155	4043	>100	1755	35214	+2.68
1185	5606	+98.69	1785	35247	+4.20
1215	7546	+90.11	1815	36051	+6.12
1245	9680	+84.91	1845	36556	
1275	12706	+78.21	1875	37879	

Yurkalo

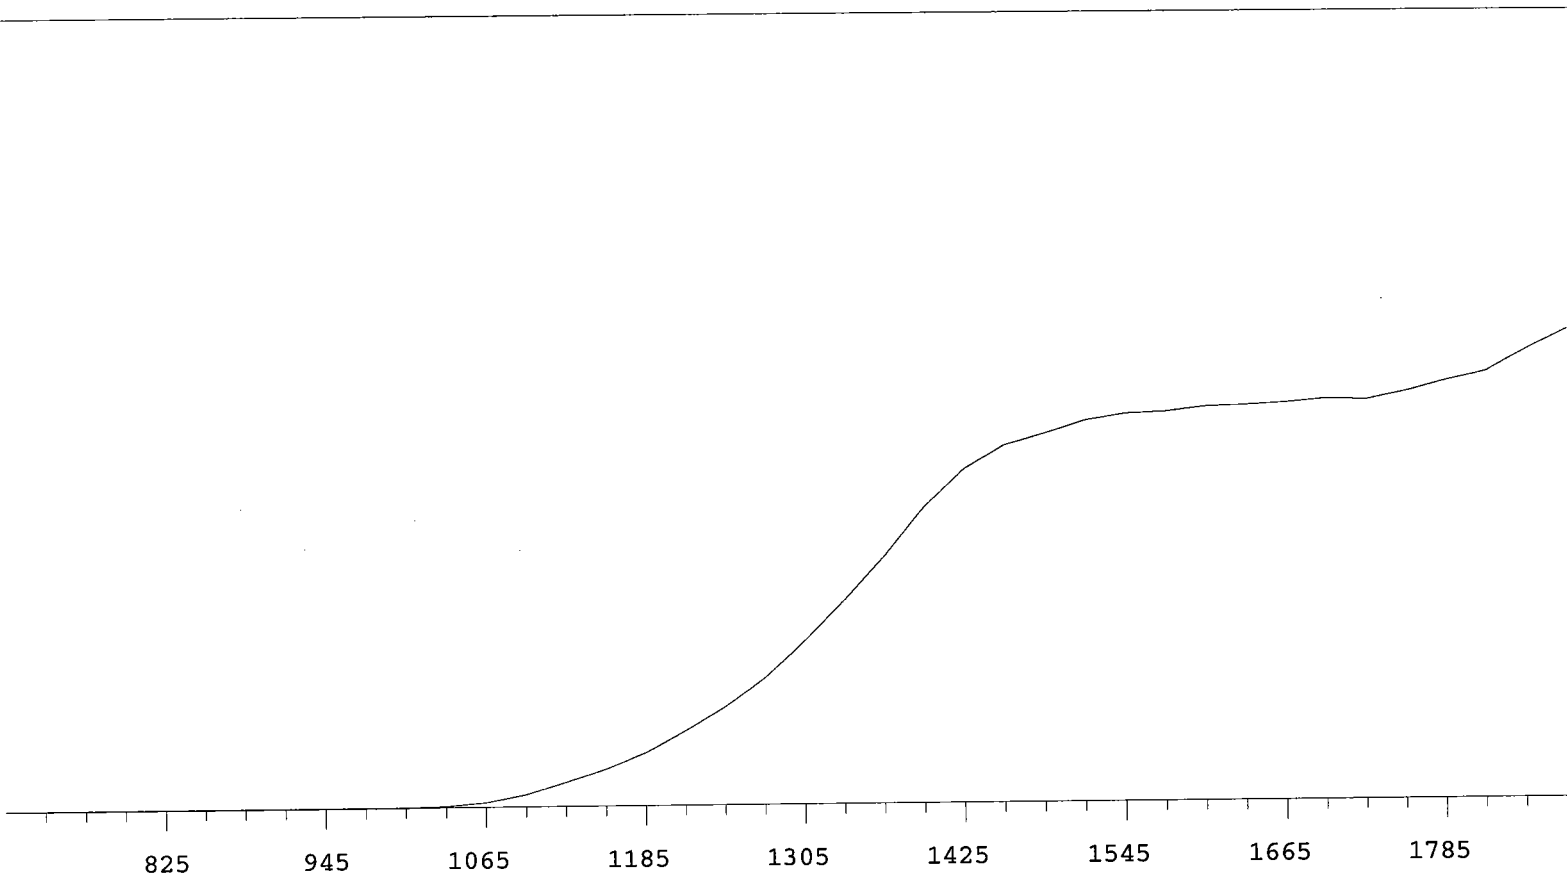


VOLTS	COUNTS	%/100 Volts	VOLTS	COUNTS	%/100 Volts
705	1		1305	16022	+74.49
735	2		1335	19934	+67.06
765	3	+33.33	1365	24065	+57.27
795	2	-15.15	1395	28750	+45.17
825	2	-30.30	1425	32437	+31.43
855	2	+0.00	1455	34703	+19.63
885	2	+55.56	1485	35773	+11.94
915	2	+71.43	1515	37013	+7.34
945	4	>100	1545	37643	+5.08
975	4	>100	1575	37795	+2.85
1005	7	>100	1605	38223	+2.11
1035	115	>100	1635	38341	+2.22
1065	458	>100	1665	38578	+1.47
1095	1190	>100	1695	38896	+2.28
1125	2315	>100	1725	38794	+3.94
1155	3550	>100	1755	39562	+5.68
1185	5136	>100	1785	40569	+9.25
1215	7197	+97.45	1815	41402	+11.70
1245	9511	+89.47	1845	43531	
1275	12416	+81.91	1875	45470	

Handwritten signature
7/18/05

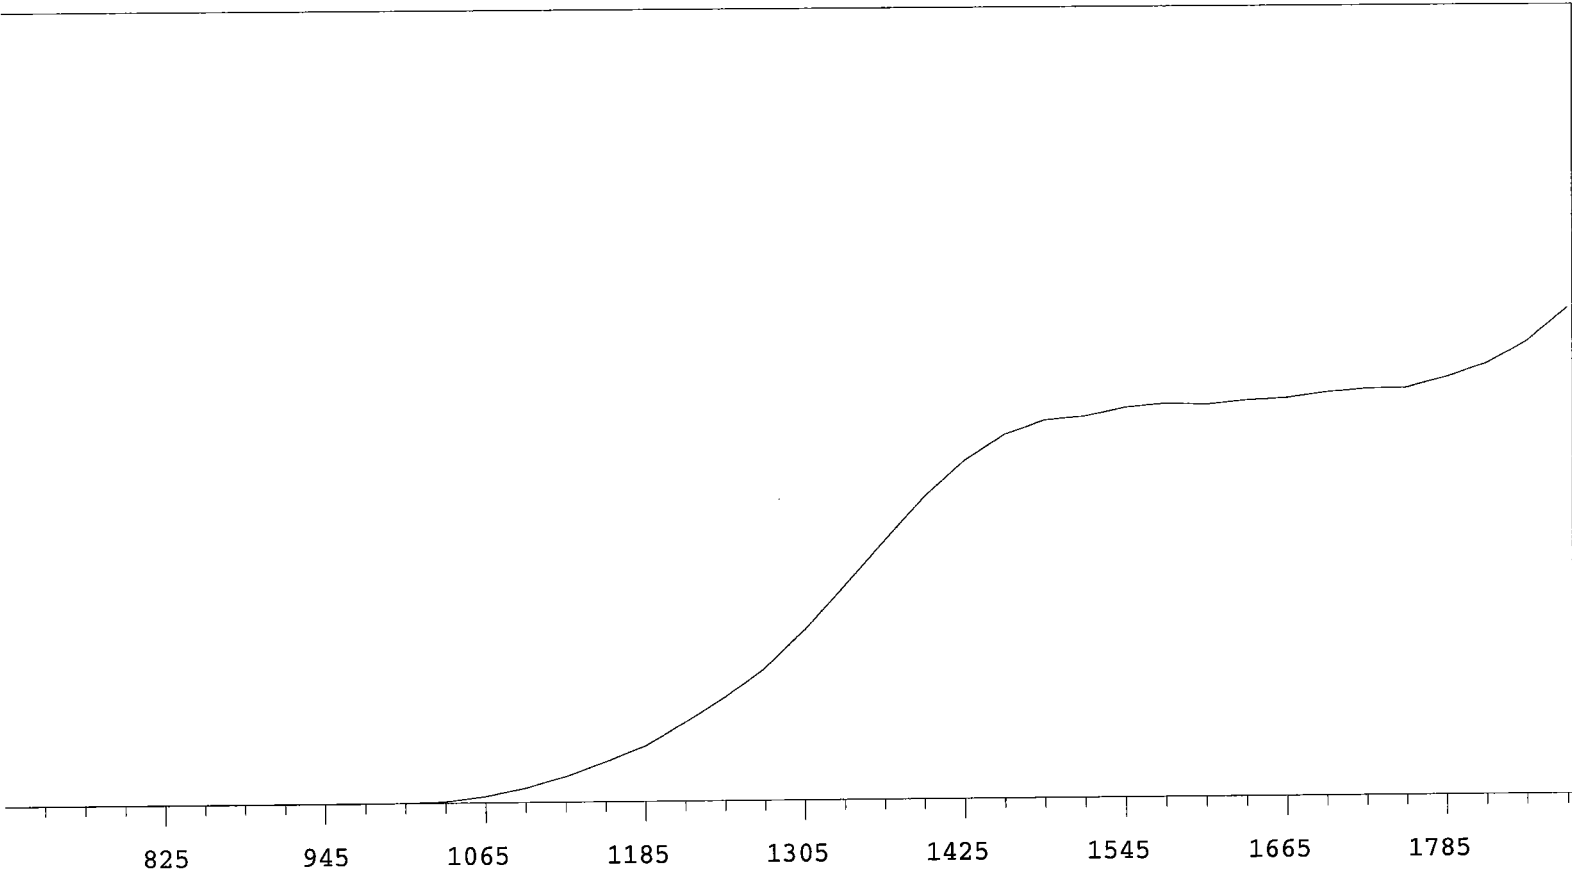


VOLTS	COUNTS	%/100 Volts	VOLTS	COUNTS	%/100 Volts
705	0		1305	16230	+74.23
735	0		1335	20402	+66.21
765	0		1365	24668	+55.06
795	1	>100	1395	28808	+42.90
825	0	>100	1425	32235	+30.71
855	2	+95.24	1455	34745	+19.08
885	2	>100	1485	36123	+11.26
915	2	+64.10	1515	36502	+6.50
945	3	>100	1545	37333	+3.68
975	4	>100	1575	37699	+2.82
1005	17	>100	1605	37570	+1.69
1035	154	>100	1635	37966	+2.25
1065	602	>100	1665	38158	+3.13
1095	1390	>100	1695	38687	+2.67
1125	2520	>100	1725	39009	+3.61
1155	3909	>100	1755	39083	+5.36
1185	5395	>100	1785	40069	+9.12
1215	7579	+92.75	1815	41344	+14.50
1245	9892	+86.09	1845	43429	
1275	12623	+79.89	1875	46557	

perkins

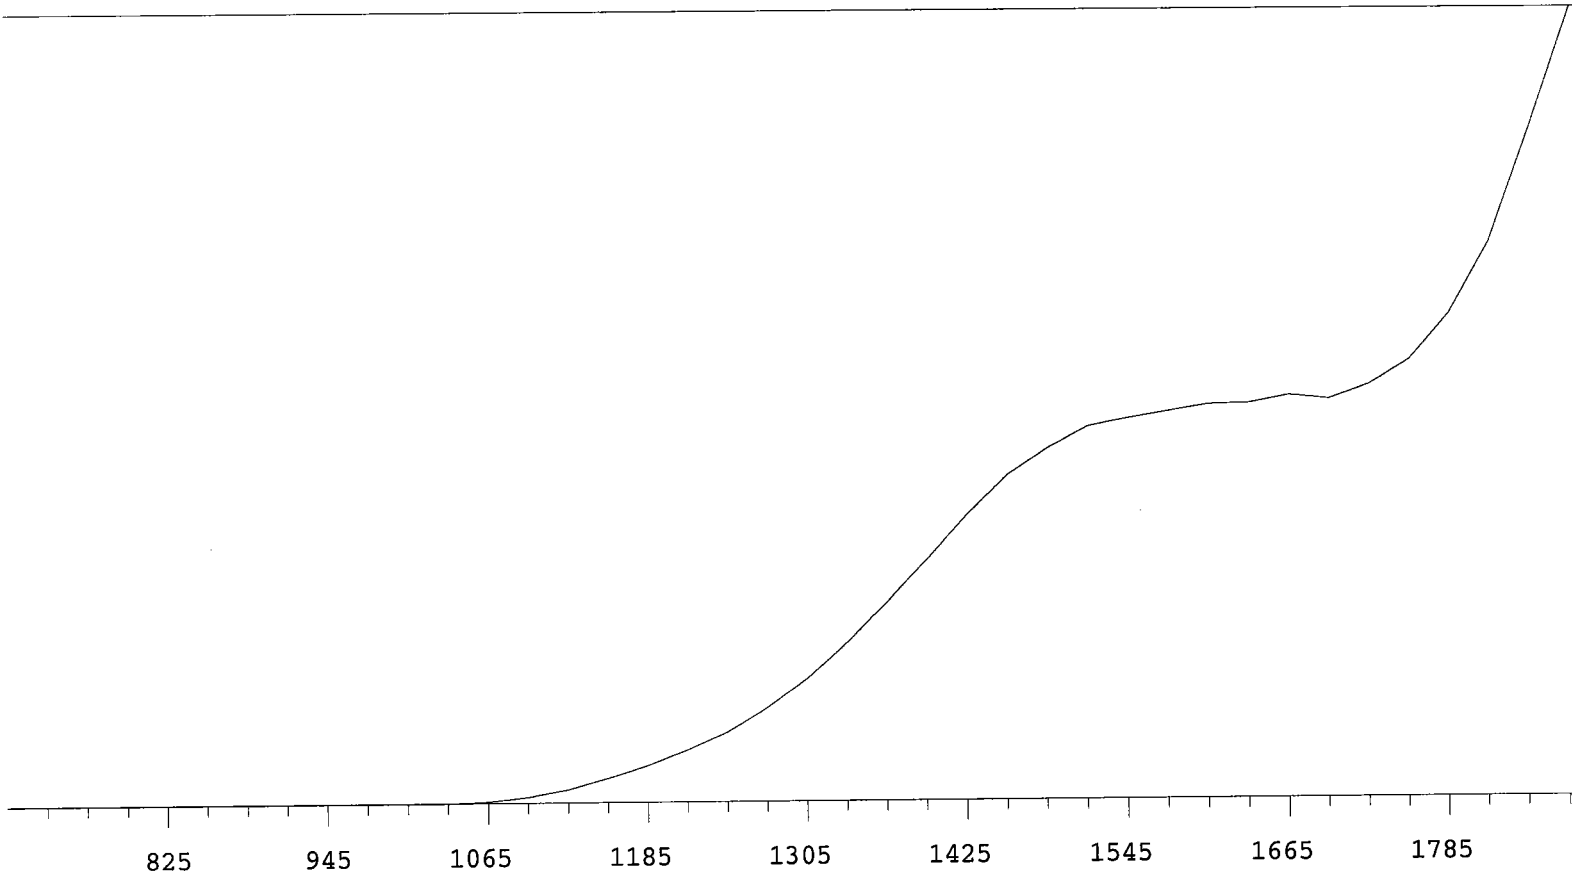


VOLTS	COUNTS	%/100 Volts	VOLTS	COUNTS	%/100 Volts
705	0		1305	10971	+84.34
735	1		1335	14097	+75.14
765	2	+0.00	1365	17622	+66.59
795	1	-66.67	1395	21247	+57.12
825	0	>100	1425	25202	+45.74
855	1	+0.00	1455	28604	+34.50
885	0	+0.00	1485	30899	+22.78
915	1	+83.33	1515	32756	+13.99
945	0	>100	1545	33437	+8.81
975	2	>100	1575	34038	+5.07
1005	1	>100	1605	34638	+4.42
1035	13	>100	1635	34735	+2.60
1065	134	>100	1665	35372	+3.37
1095	511	>100	1695	35026	+7.70
1125	1129	>100	1725	36274	+15.84
1155	2134	>100	1755	38436	+28.19
1185	3197	>100	1785	42586	+41.27
1215	4542	>100	1815	48885	+52.29
1245	6086	+97.20	1845	58919	
1275	8291	+90.92	1875	71030	

Y 7/25/05

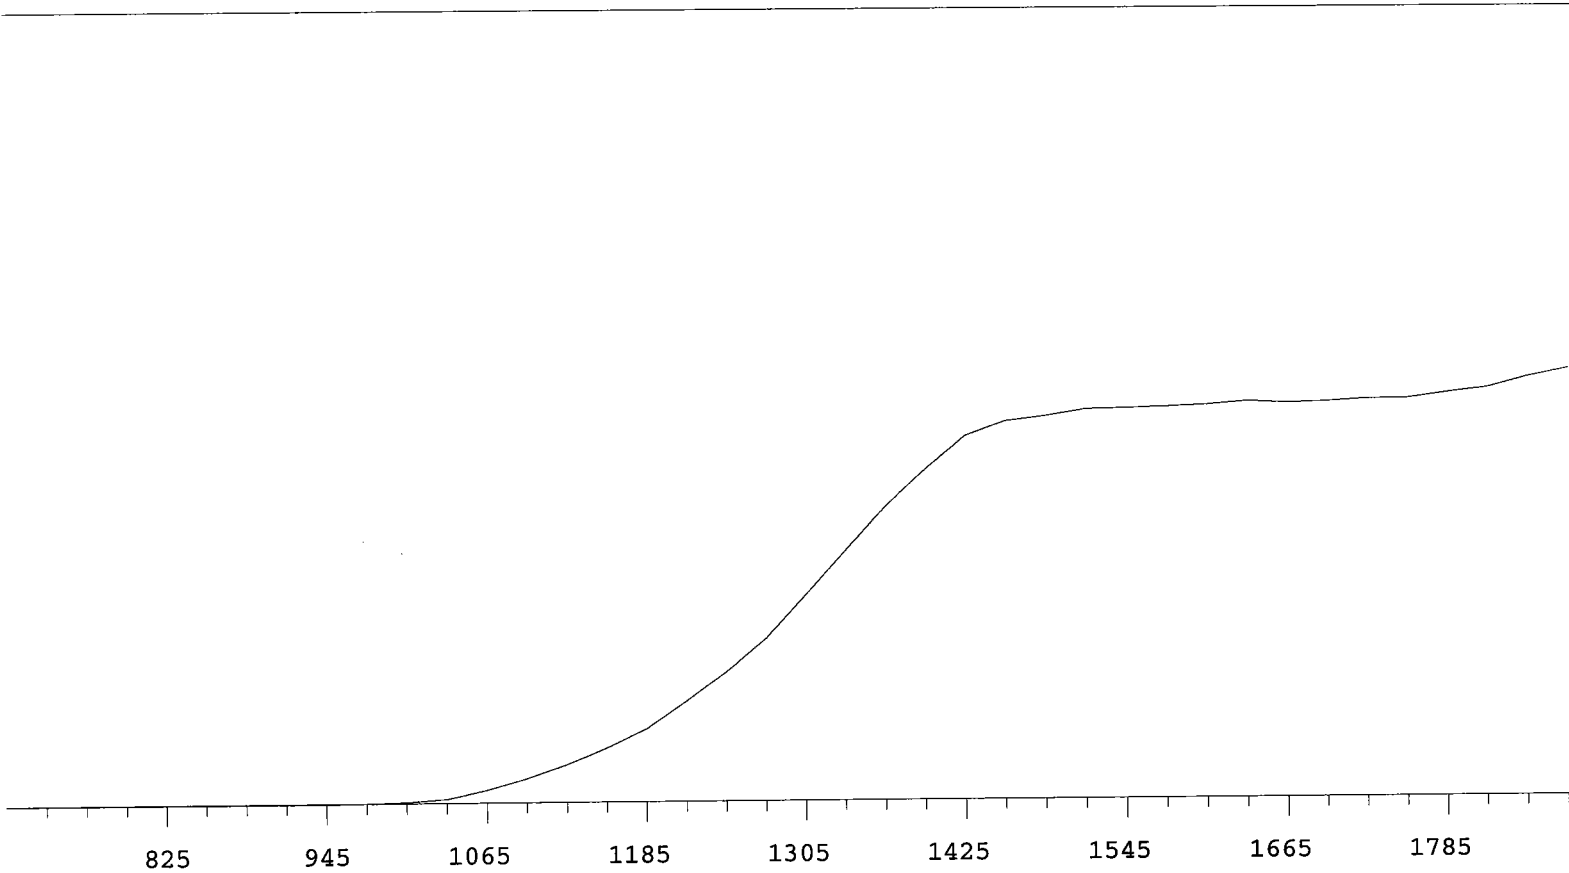


VOLTS	COUNTS	%/100 Volts	VOLTS	COUNTS	%/100 Volts
705	0		1305	22314	+66.02
735	0		1335	27016	+56.65
765	0		1365	31730	+46.09
795	0	>100	1395	35861	+34.20
825	0	>100	1425	39521	+21.96
855	0	>100	1455	41096	+12.55
885	4	+33.33	1485	41618	+5.70
915	1	>100	1515	42360	+2.97
945	0	>100	1545	42428	+1.93
975	25	>100	1575	42562	+1.42
1005	123	>100	1605	42743	+1.15
1035	462	>100	1635	43108	+0.84
1065	1382	>100	1665	42891	+0.79
1095	2620	>100	1695	43031	+0.67
1125	4094	>100	1725	43288	+1.82
1155	5833	>100	1755	43345	+2.62
1185	7915	+97.20	1785	43916	+4.27
1215	10844	+88.32	1815	44430	+5.91
1245	14050	+81.59	1845	45569	
1275	17692	+73.63	1875	46488	

Handwritten signature

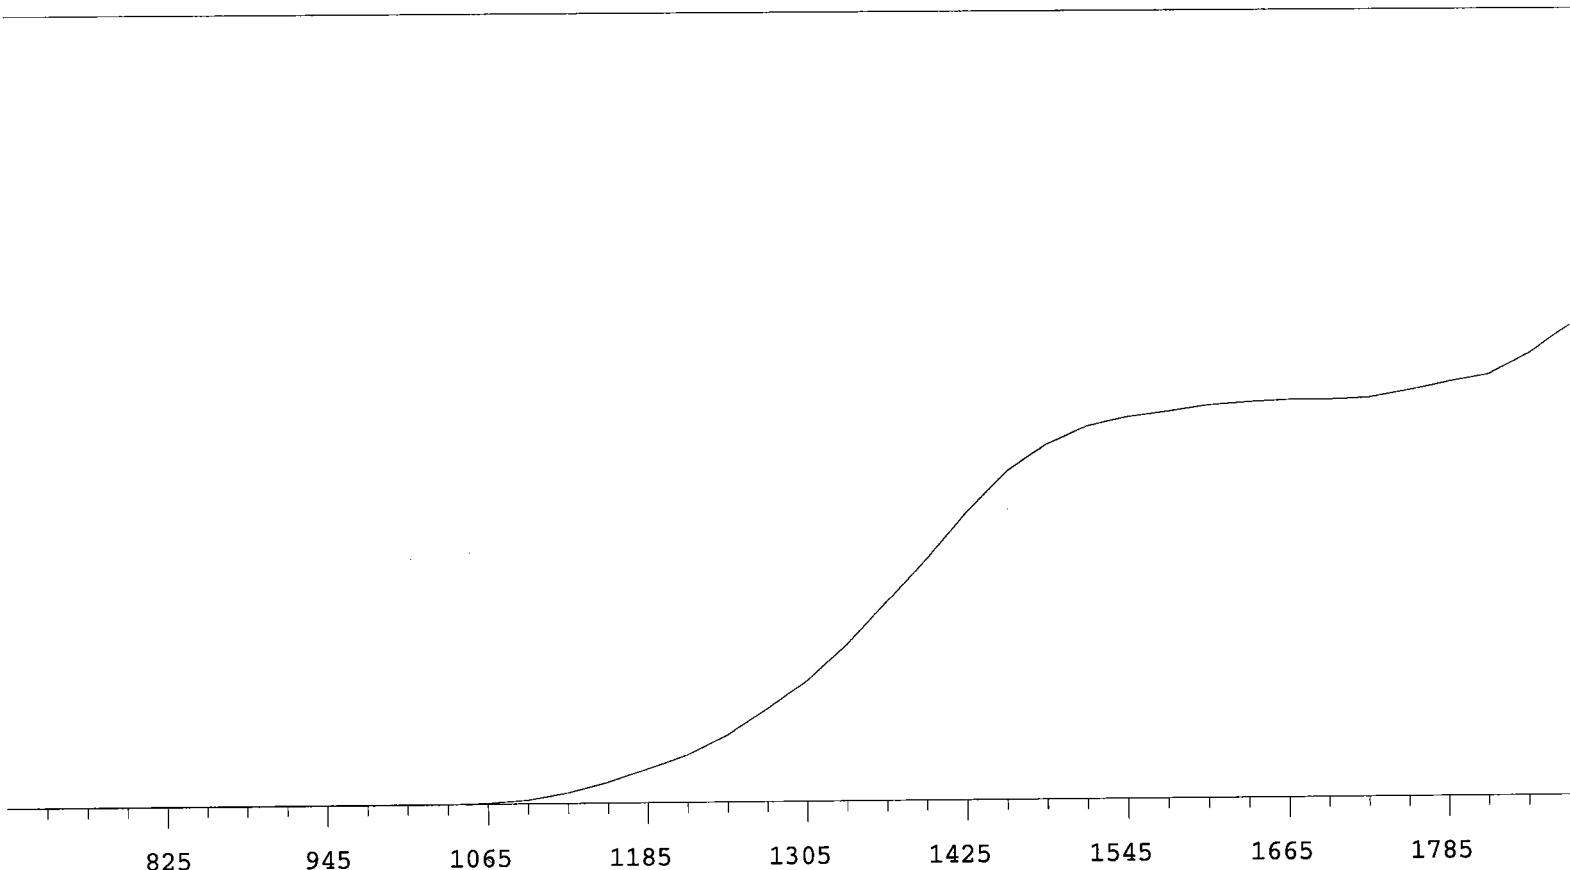


VOLTS	COUNTS	%/100 Volts	VOLTS	COUNTS	%/100 Volts
705	0		1305	11504	+85.43
735	1		1335	14849	+76.81
765	2	+66.67	1365	18861	+68.80
795	1	-27.78	1395	22846	+58.63
825	1	+0.00	1425	27157	+46.27
855	1	>100	1455	30851	+34.04
885	2	+74.07	1485	33326	+22.12
915	3	+0.00	1515	34995	+13.15
945	2	+51.28	1545	35846	+7.97
975	1	>100	1575	36351	+4.94
1005	5	>100	1605	36888	+3.44
1035	11	>100	1635	37159	+2.18
1065	76	>100	1665	37334	+1.21
1095	354	>100	1695	37337	+1.96
1125	989	>100	1725	37477	+3.64
1155	1937	>100	1755	38192	+5.29
1185	3197	>100	1785	38972	+8.13
1215	4514	>100	1815	39629	+11.94
1245	6395	>100	1845	41535	
1275	8812	+93.25	1875	44161	

gmk/ab

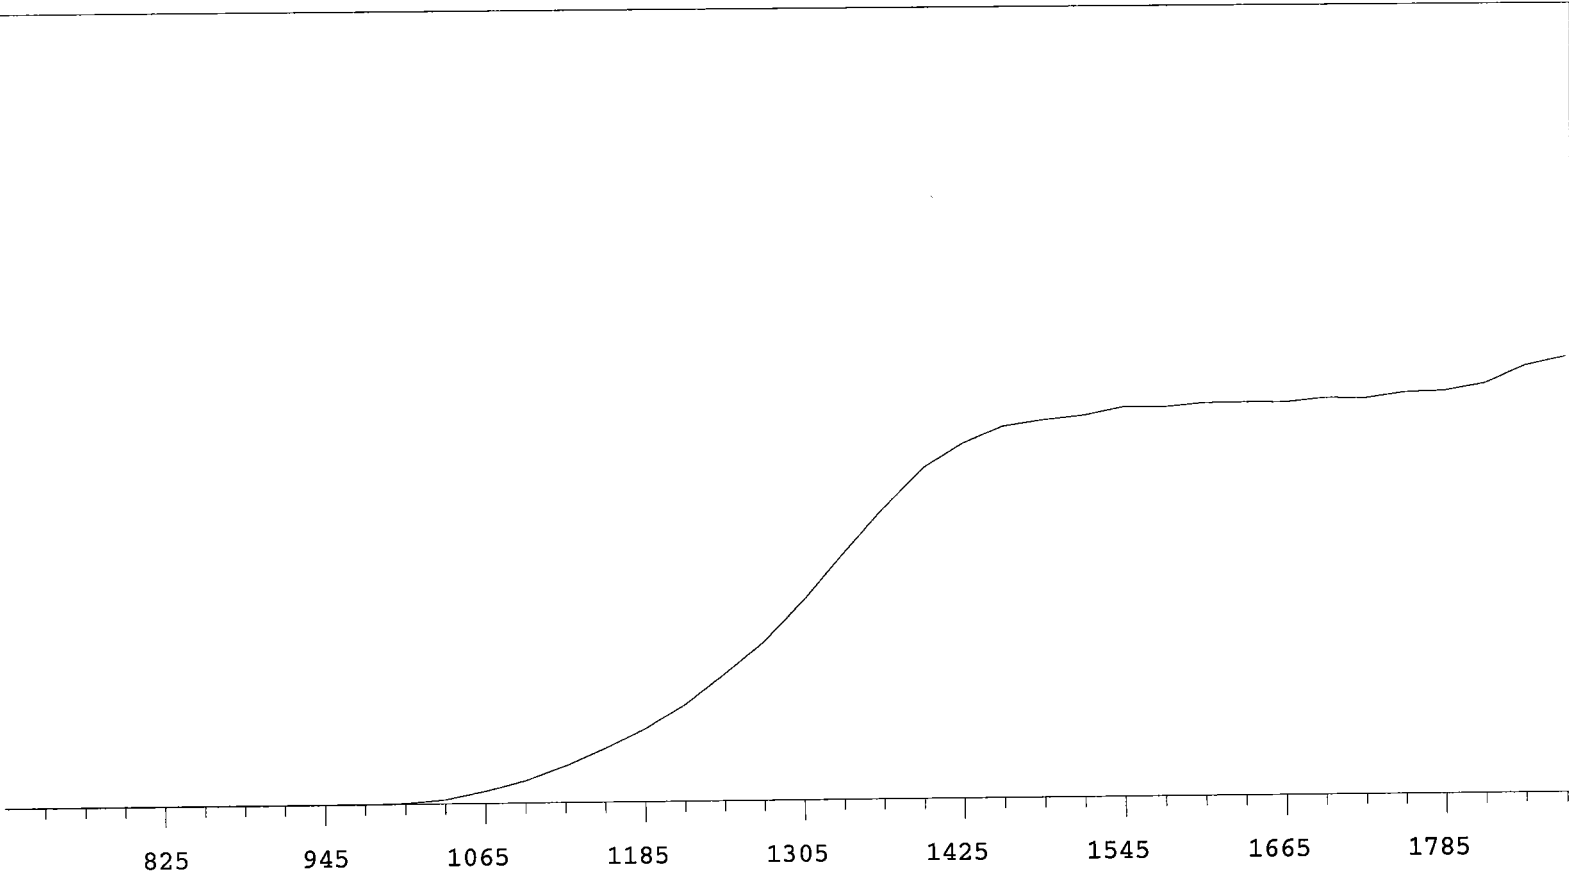


VOLTS	COUNTS	%/100 Volts	VOLTS	COUNTS	%/100 Volts
705	2		1305	16352	+67.34
735	6		1335	20077	+59.09
765	3	-20.83	1365	23789	+46.51
795	2	-58.82	1395	27076	+33.20
825	3	-41.67	1425	29091	+20.71
855	3	-66.67	1455	30421	+11.33
885	1	-30.30	1485	30894	+6.95
915	1	>100	1515	31231	+4.14
945	3	>100	1545	31889	+3.39
975	9	>100	1575	31864	+2.37
1005	87	>100	1605	32186	+0.96
1035	349	>100	1635	32217	+1.30
1065	1009	>100	1665	32174	+0.81
1095	1793	>100	1695	32499	+1.72
1125	2982	>100	1725	32437	+2.17
1155	4367	>100	1755	32922	+2.82
1185	5942	+97.04	1785	33023	+5.92
1215	7886	+87.16	1815	33599	+7.59
1245	10422	+80.66	1845	35066	
1275	13013	+74.57	1875	35778	

pm 7/29/05

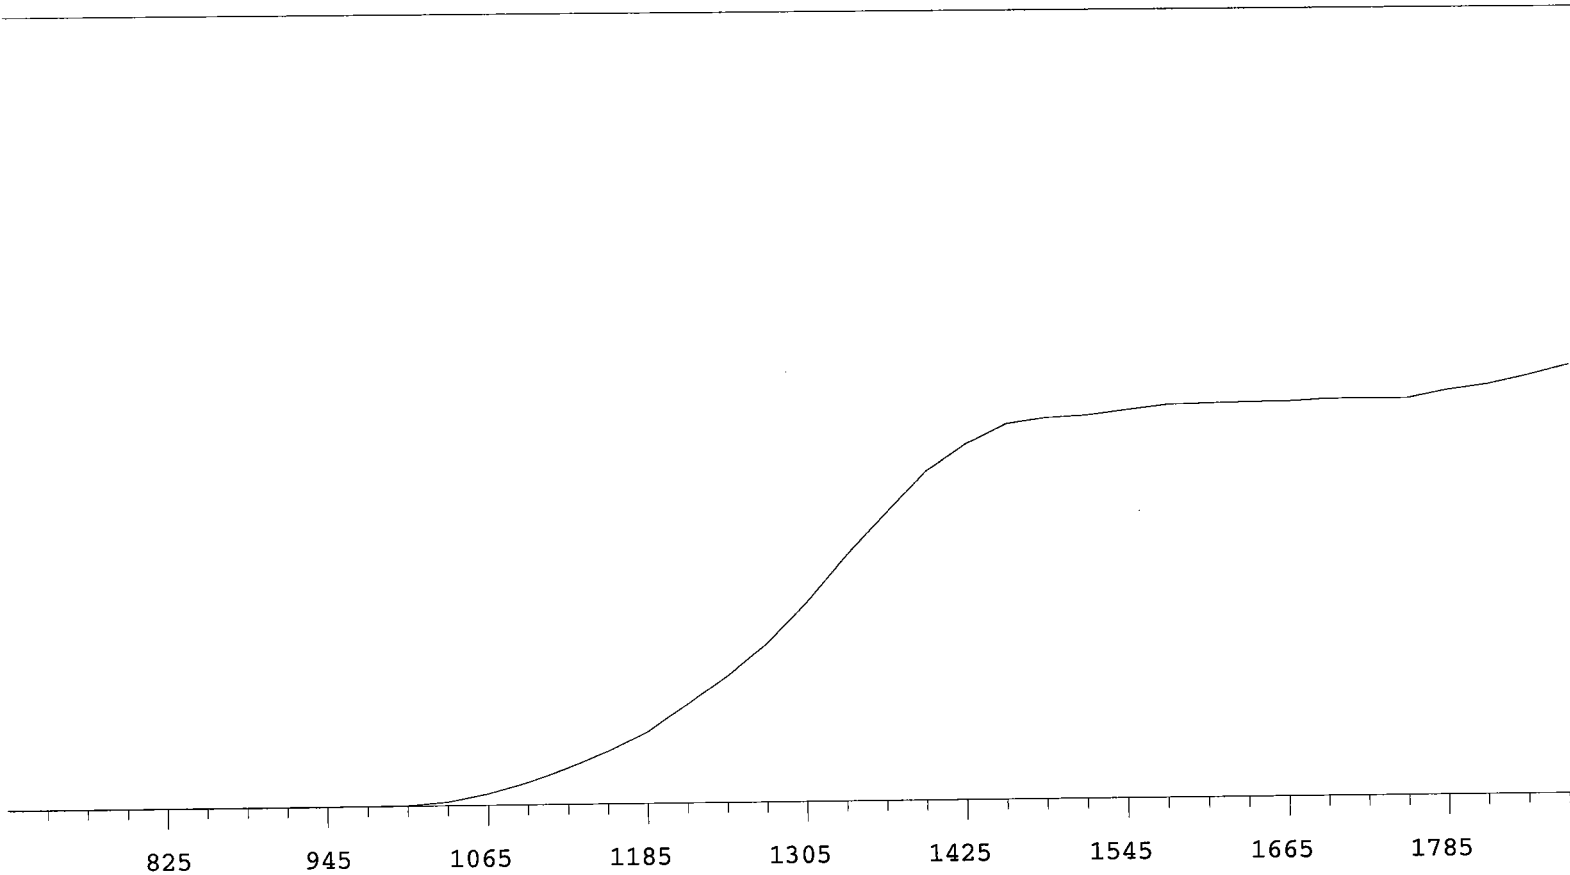


VOLTS	COUNTS	%/100 Volts	VOLTS	COUNTS	%/100 Volts
705	3		1305	22754	+66.54
735	1		1335	27979	+58.16
765	3	-55.56	1365	32713	+46.35
795	0	-23.81	1395	37461	+34.14
825	2	>100	1425	40450	+22.38
855	1	>100	1455	42675	+12.11
885	0	+66.67	1485	43308	+6.46
915	5	>100	1515	43568	+3.76
945	2	>100	1545	44157	+3.14
975	19	>100	1575	44714	+2.51
1005	86	>100	1605	44814	+1.32
1035	451	>100	1635	44910	+0.82
1065	1295	>100	1665	44945	+0.82
1095	2525	>100	1695	45204	+0.66
1125	4114	>100	1725	45222	+1.70
1155	5953	>100	1755	45215	+2.80
1185	8113	+98.45	1785	46095	+4.67
1215	11136	+88.70	1815	46688	+6.29
1245	14448	+81.12	1845	47723	
1275	18173	+74.07	1875	48829	

Handwritten signature

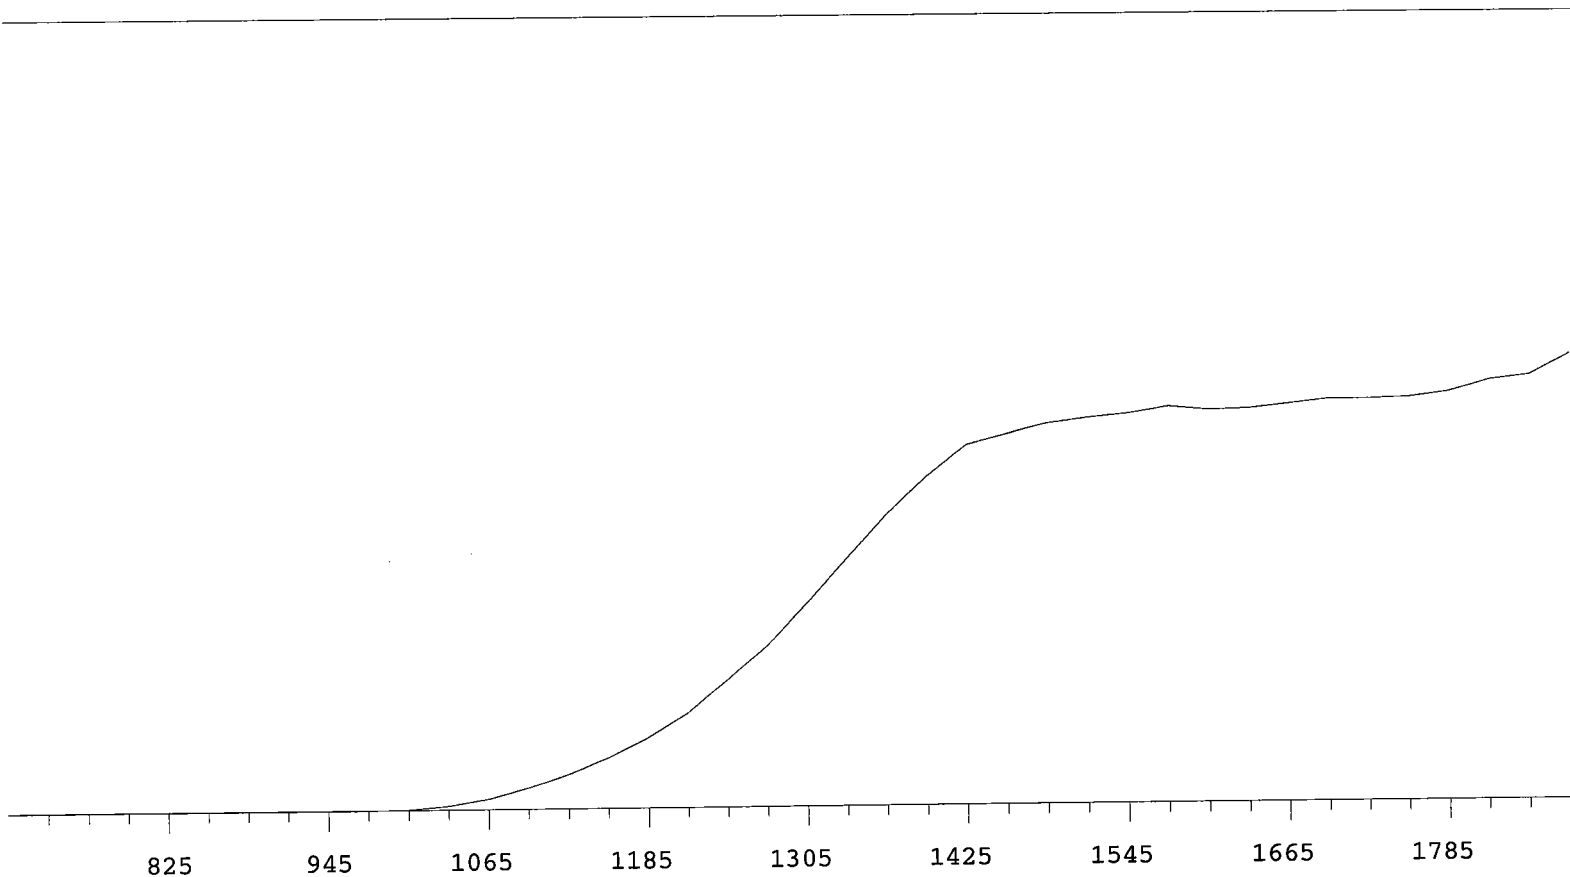

VOLTS	COUNTS	%/100 Volts	VOLTS	COUNTS	%/100 Volts
705	4		1305	19958	+67.03
735	4		1335	24246	+57.28
765	0		1365	28539	+46.21
795	0	+18.52	1395	32266	+33.26
825	1	>100	1425	35414	+21.60
855	4	+100.00	1455	36466	+12.52
885	3	-30.30	1485	37462	+6.66
915	2	+20.83	1515	37985	+5.29
945	1	>100	1545	38363	+3.02
975	6	>100	1575	39020	+1.64
1005	71	>100	1605	38677	+1.19
1035	402	>100	1635	38778	+1.48
1065	1048	>100	1665	39179	+2.33
1095	2130	>100	1695	39636	+2.03
1125	3384	>100	1725	39616	+1.90
1155	4976	>100	1755	39758	+3.40
1185	6855	>100	1785	40252	+4.91
1215	9208	+92.12	1815	41367	+7.87
1245	12454	+85.04	1845	41801	
1275	15798	+76.70	1875	43872	

msk

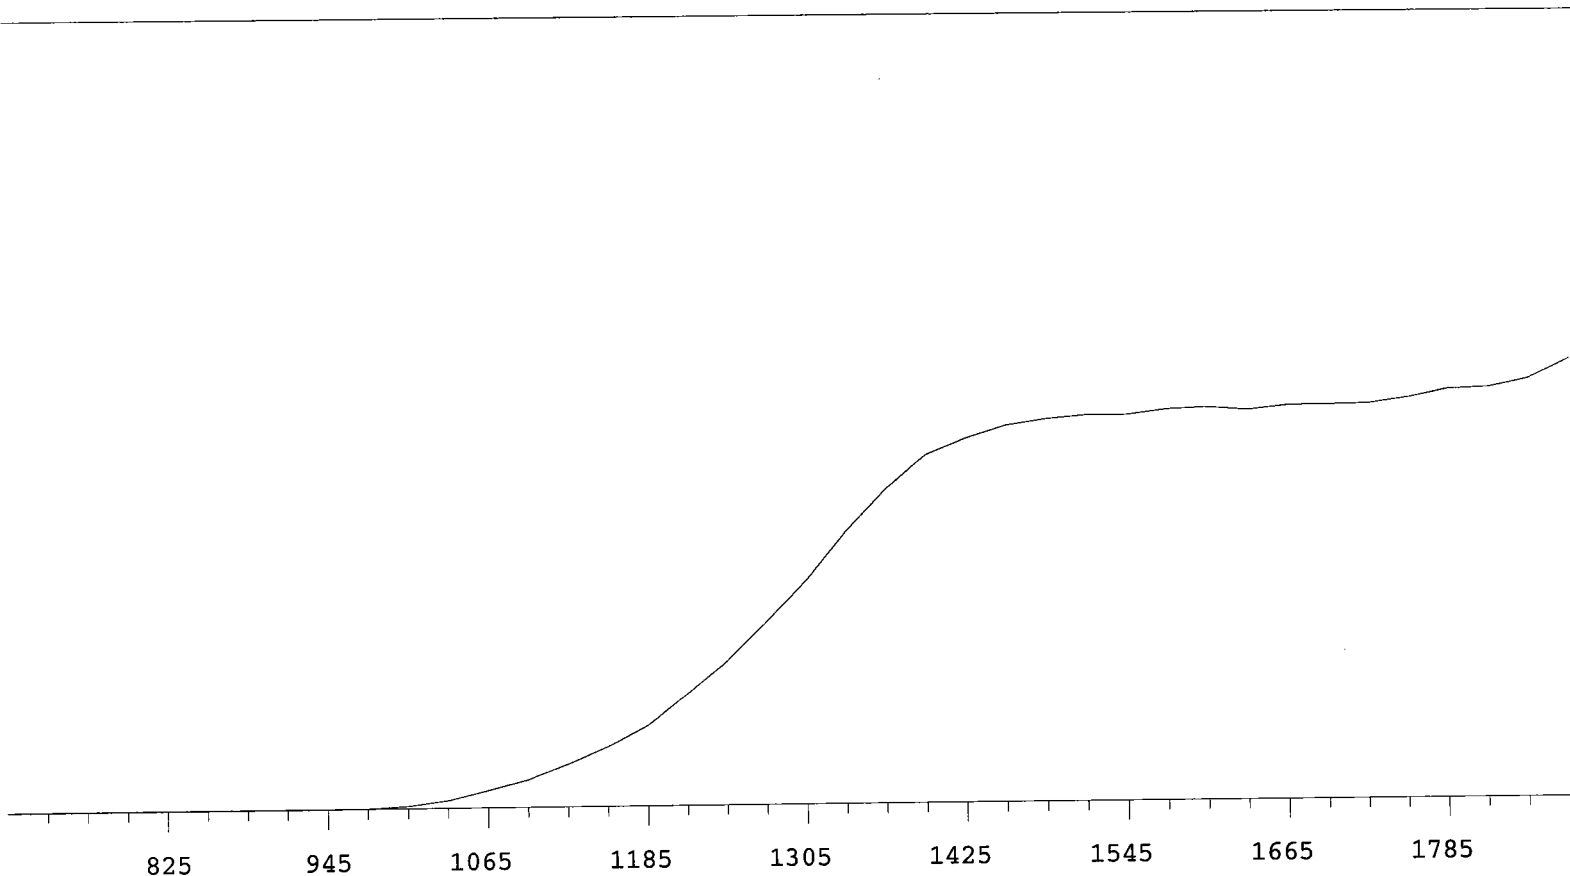


VOLTS	COUNTS	%/100 Volts
-------	--------	-------------

VOLTS	COUNTS	%/100 Volts
-------	--------	-------------

705	1	
735	0	
765	1	
795	2	>100
825	3	+0.00
855	2	-33.33
885	1	-33.33
915	2	>100
945	2	>100
975	23	>100
1005	188	>100
1035	628	>100
1065	1402	>100
1095	2202	>100
1125	3405	>100
1155	4734	>100
1185	6329	+95.04
1215	8730	+88.10
1245	11220	+79.46
1275	14252	+70.70


1305	17371	+61.82
1335	21059	+51.03
1365	24146	+38.17
1395	26716	+25.34
1425	27972	+15.55
1455	28941	+8.73
1485	29433	+4.91
1515	29724	+2.97
1545	29727	+2.22
1575	30112	+1.21
1605	30235	+1.21
1635	30012	+0.64
1665	30324	+0.75
1695	30358	+1.95
1725	30404	+3.02
1755	30862	+3.77
1785	31464	+4.62
1815	31575	+6.76
1845	32217	
1875	33728	

mshab

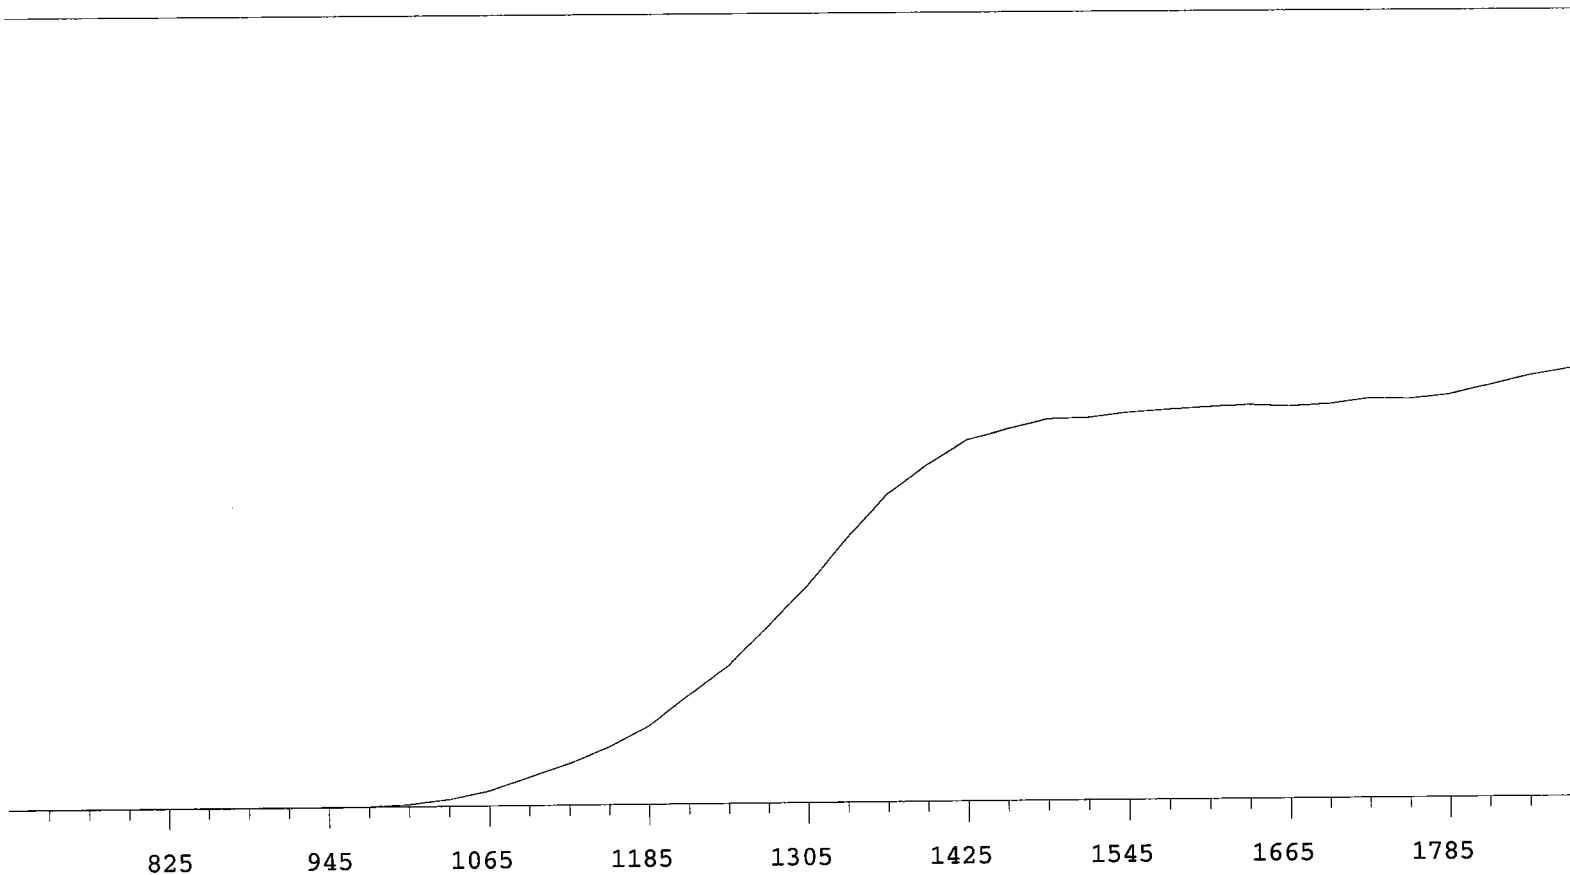


VOLTS	COUNTS	%/100 Volts	VOLTS	COUNTS	%/100 Volts
705	0		1305	19992	+64.10
735	1		1335	24434	+52.32
765	2	-55.56	1365	28341	+40.24
795	0	-83.33	1395	31016	+27.00
825	0	>100	1425	33244	+17.26
855	1	>100	1455	34234	+10.11
885	0	>100	1485	35116	+5.57
915	1	>100	1515	35198	+3.72
945	7	>100	1545	35658	+2.57
975	26	>100	1575	35928	+2.43
1005	201	>100	1605	36121	+1.20
1035	622	>100	1635	36271	+0.67
1065	1395	>100	1665	36135	+1.26
1095	2589	>100	1695	36285	+1.47
1125	3807	>100	1725	36799	+2.20
1155	5311	>100	1755	36745	+3.29
1185	7258	+96.60	1785	37112	+4.71
1215	10100	+88.77	1815	37953	+6.34
1245	12793	+79.49	1845	38842	
1275	16338	+71.46	1875	39499	

Jan 12 2006

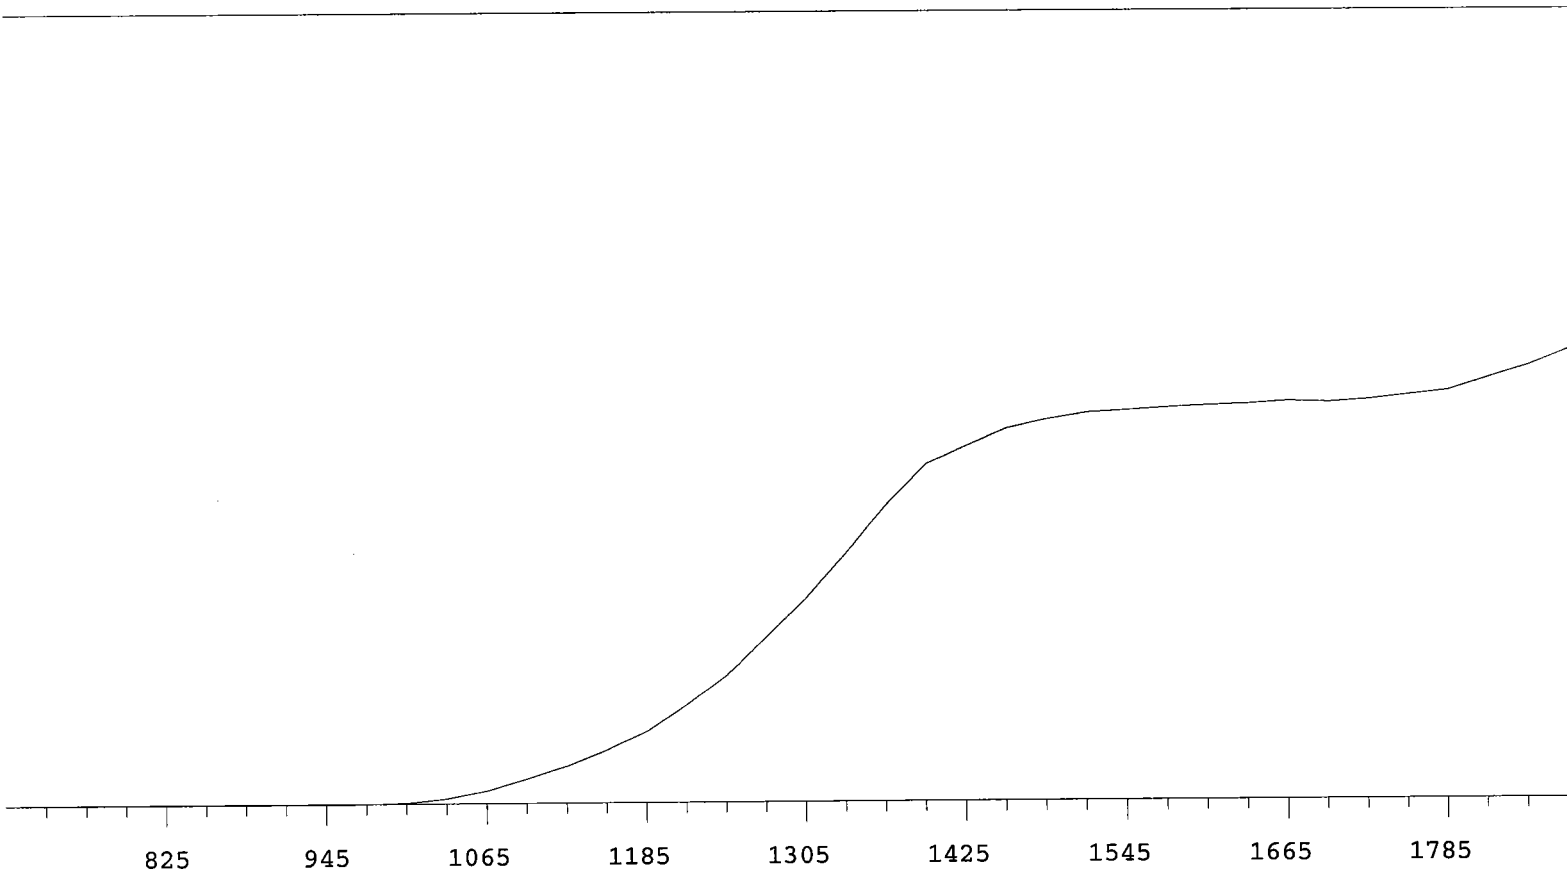


VOLTS	COUNTS	%/100 Volts	VOLTS	COUNTS	%/100 Volts
705	3		1305	20823	+66.52
735	0		1335	25209	+57.37
765	0	-27.78	1365	30058	+44.75
795	1	>100	1395	34207	+31.58
825	2	+41.67	1425	35961	+19.48
855	0	+27.78	1455	37712	+11.46
885	1	+0.00	1485	38621	+7.54
915	2	>100	1515	39266	+4.27
945	1	>100	1545	39505	+2.69
975	12	>100	1575	39765	+1.77
1005	101	>100	1605	39960	+1.71
1035	505	>100	1635	40095	+1.10
1065	1271	>100	1665	40363	+0.99
1095	2435	>100	1695	40227	+1.48
1125	3717	>100	1725	40494	+2.25
1155	5349	>100	1755	40925	+4.61
1185	7264	+98.50	1785	41387	+6.78
1215	9948	+91.79	1815	42624	+9.20
1245	13035	+83.57	1845	43902	
1275	16927	+74.29	1875	45583	

m7/25/05

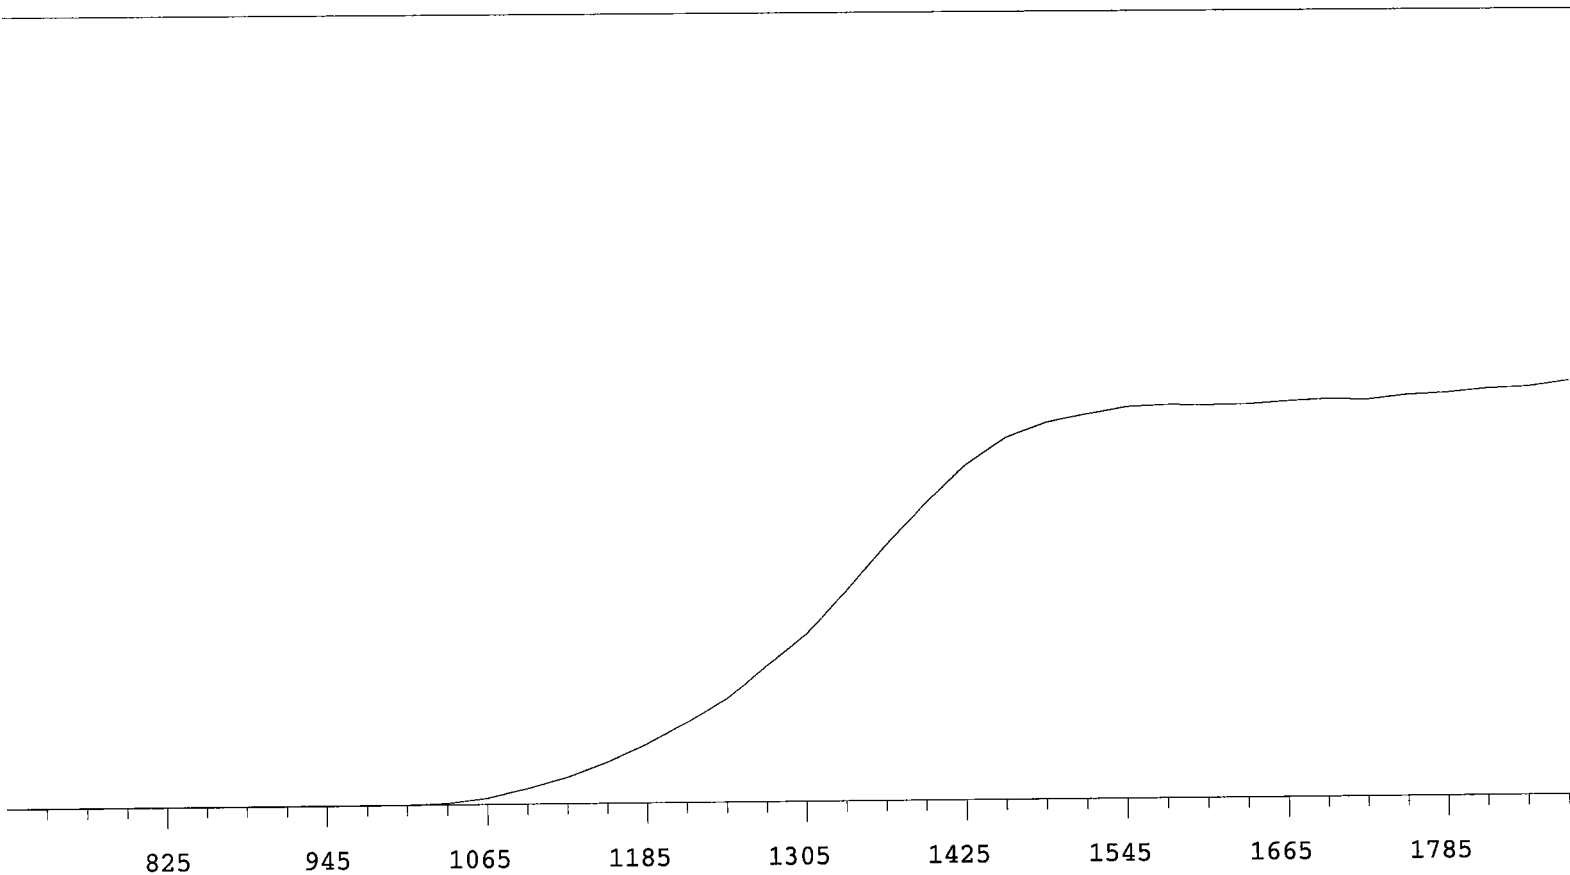


VOLTS	COUNTS	%/100 Volts	VOLTS	COUNTS	%/100 Volts
705	2		1305	18669	+72.76
735	0		1335	23370	+64.55
765	0	+66.67	1365	28550	+55.91
795	0	>100	1395	33260	+43.78
825	3	+83.33	1425	37418	+31.11
855	0	-83.33	1455	40334	+20.16
885	1	>100	1485	41951	+12.02
915	0	>100	1515	42838	+6.74
945	1	>100	1545	43602	+3.50
975	3	>100	1575	43809	+1.61
1005	34	>100	1605	43735	+0.82
1035	190	>100	1635	43823	+1.13
1065	725	>100	1665	44134	+1.17
1095	1724	>100	1695	44358	+1.41
1125	2937	>100	1725	44239	+1.42
1155	4543	>100	1755	44705	+1.95
1185	6429	>100	1785	44909	+2.35
1215	8789	+94.33	1815	45328	+2.52
1245	11443	+85.00	1845	45509	
1275	15155	+78.33	1875	46116	

mm/2005

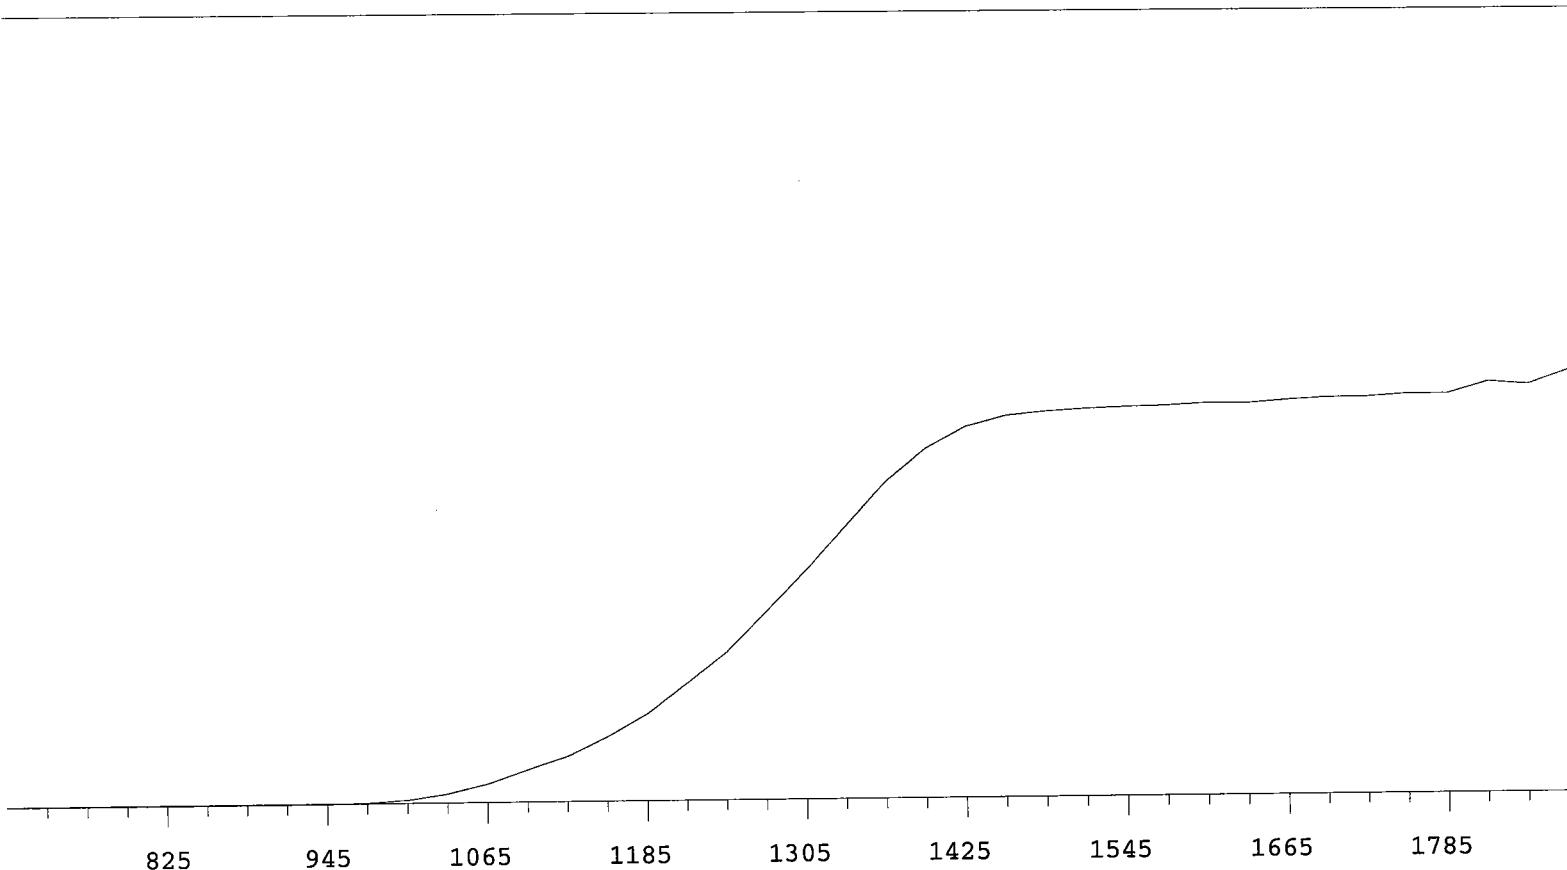


VOLTS	COUNTS	%/100 Volts	VOLTS	COUNTS	%/100 Volts
705	3		1305	17564	+61.34
735	2		1335	20983	+50.92
765	1	-66.67	1365	24340	+39.30
795	4	+45.45	1395	26885	+26.88
825	0	+30.30	1425	28563	+15.81
855	4	+0.00	1455	29365	+8.25
885	2	>100	1485	29683	+3.89
915	3	>100	1515	29898	+2.00
945	6	>100	1545	30019	+1.51
975	42	>100	1575	30093	+1.01
1005	244	>100	1605	30263	+1.18
1035	697	>100	1635	30232	+1.46
1065	1429	>100	1665	30485	+1.36
1095	2487	>100	1695	30648	+1.63
1125	3483	>100	1725	30678	+1.10
1155	4980	>100	1755	30883	+2.70
1185	6683	+92.69	1785	30876	+2.89
1215	8988	+84.24	1815	31805	+4.51
1245	11345	+76.74	1845	31569	
1275	14366	+68.74	1875	32673	

Handwritten signature

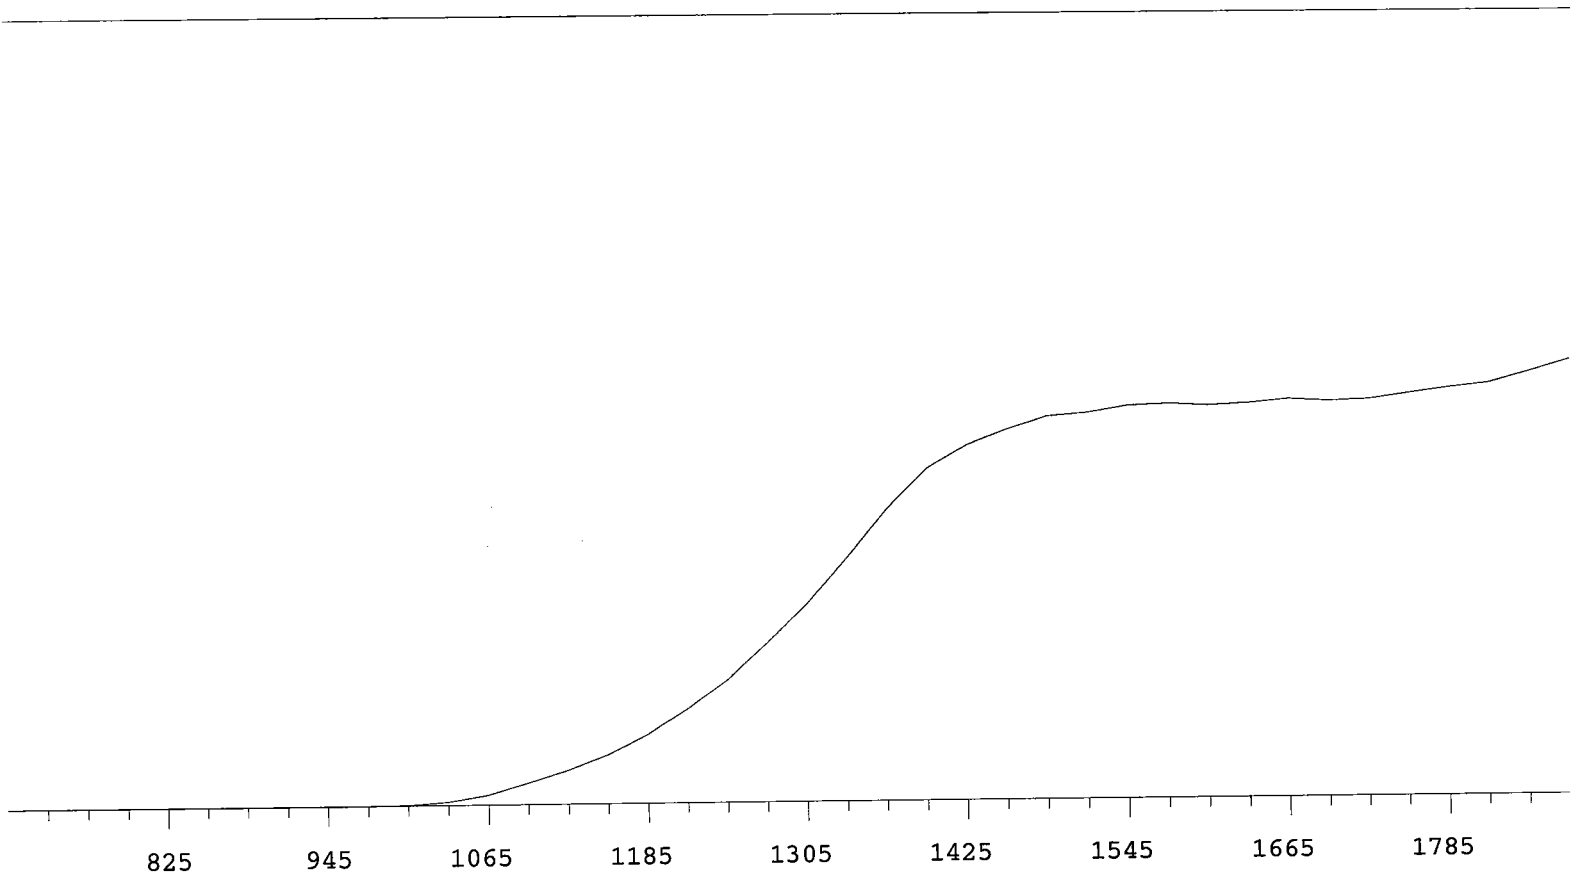

VOLTS	COUNTS	%/100 Volts	VOLTS	COUNTS	%/100 Volts
705	1		1305	17606	+68.88
735	0		1335	21599	+59.41
765	0		1365	25809	+47.05
795	0	>100	1395	29372	+33.37
825	2	>100	1425	31486	+21.76
855	0	+100.00	1455	32894	+12.91
885	1	>100	1485	34077	+8.33
915	2	>100	1515	34357	+5.14
945	4	>100	1545	34948	+2.35
975	10	>100	1575	35100	+1.39
1005	53	>100	1605	34930	+0.94
1035	327	>100	1635	35093	+0.78
1065	902	>100	1665	35444	+1.03
1095	1970	>100	1695	35257	+1.49
1125	3079	>100	1725	35393	+2.34
1155	4435	>100	1755	35908	+3.77
1185	6202	+99.16	1785	36373	+5.15
1215	8385	+91.20	1815	36800	+6.47
1245	10930	+83.12	1845	37764	
1275	14132	+75.94	1875	38815	

Handwritten signature/initials

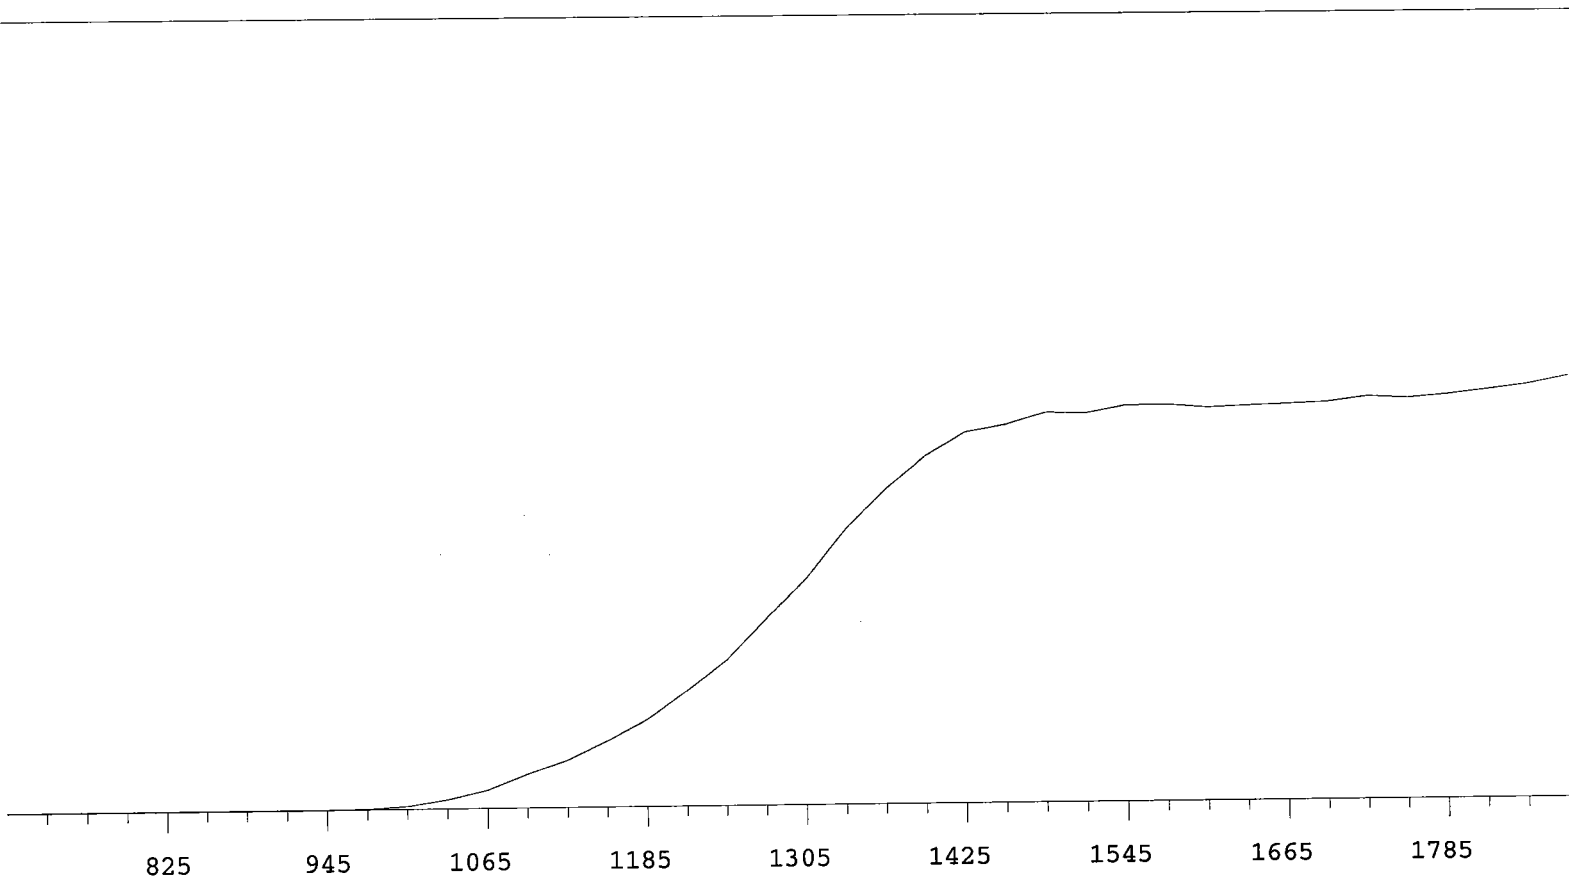

VOLTS	COUNTS	%/100 Volts	VOLTS	COUNTS	%/100 Volts
705	4		1305	21893	+61.23
735	3		1335	26615	+50.22
765	1		1365	30345	+39.18
795	1	>100	1395	33570	+25.90
825	0	>100	1425	35845	+16.79
855	1	>100	1455	36520	+8.95
885	5	>100	1485	37628	+5.26
915	3	>100	1515	37539	+3.72
945	14	>100	1545	38268	+1.30
975	77	>100	1575	38301	+0.80
1005	298	>100	1605	37985	-0.13
1035	932	>100	1635	38135	+0.48
1065	1829	>100	1665	38276	+1.84
1095	3311	>100	1695	38429	+1.51
1125	4603	>100	1725	38899	+1.48
1155	6424	+96.24	1755	38695	+1.85
1185	8451	+88.86	1785	39003	+2.37
1215	11201	+83.16	1815	39457	+4.14
1245	14170	+76.31	1845	39914	
1275	18128	+69.83	1875	40696	

mu 9/29/05

Pb-210 WATER

Batch : CALVER
 Analyst : JMJ
 Date : 7/28/2005

Procedure Code : GFC_PBL
 Parmname : Lead-210
 Batch Counted On : PIC
 Lead Carrier Weight : 14.65 mg/mL

Required MDA : 5.00 pCi/L
 Bkg Count Time : 500 min

Sample ID	Sample Aliquot L	Sample Date/Time	Prep Date	Carrier Weight mg	Bi-210 Start Time	Bi-210 Ingrowth Factor	Detector Number#	Count Time min
V1	1.000	7/14/2005 0:00	7/14/2005	1.30	7/14/2005 8:00	0.858	1A	10
V2	1.000	7/14/2005 0:00	7/14/2005	2.10	7/14/2005 8:00	0.858	1B	10
V3	1.000	7/14/2005 0:00	7/14/2005	3.60	7/14/2005 8:00	0.858	1C	10
V4	1.000	7/14/2005 0:00	7/14/2005	5.00	7/14/2005 8:00	0.858	1D	10
V5	1.000	7/14/2005 0:00	7/14/2005	7.00	7/14/2005 8:00	0.858	2A	10
V6	1.000	7/14/2005 0:00	7/14/2005	8.80	7/14/2005 8:00	0.858	2B	10
V7	1.000	7/14/2005 0:00	7/14/2005	11.70	7/14/2005 8:00	0.858	2C	10
V8	1.000	7/14/2005 0:00	7/14/2005	13.40	7/14/2005 8:00	0.858	2D	10
V9	1.000	7/14/2005 0:00	7/14/2005	12.90	7/14/2005 8:00	0.858	3A	10
V10	1.000	7/14/2005 0:00	7/14/2005	15.30	7/14/2005 8:00	0.858	3B	10
V11	1.000	7/14/2005 0:00	7/14/2005	15.70	7/14/2005 8:00	0.858	3C	10
V12	1.000	7/14/2005 0:00	7/14/2005	19.80	7/14/2005 8:00	0.858	3D	10
V1	1.000	7/14/2005 0:00	7/14/2005	1.30	7/14/2005 8:00	0.858	4A	10
V2	1.000	7/14/2005 0:00	7/14/2005	2.10	7/14/2005 8:00	0.858	4B	10
V3	1.000	7/14/2005 0:00	7/14/2005	3.60	7/14/2005 8:00	0.858	4C	10
V4	1.000	7/14/2005 0:00	7/14/2005	5.00	7/14/2005 8:00	0.858	4D	10

Handwritten signature
 7/25/05

Pb-210 0.1 ML
 ET491-A 80900.6 DPM
 3644.17 pCi/L

Total Beta Counts	Raw cpm	Detector Efficiency dec	BKG cpm	Counted Time	Sample Decay Factor	Test Rec. dec	Pb-210 MDA pCi/L	Pb-210 RESULT pCi/L	Pb-210 Recovery (%)
22806	2280.60	0.4191	0.362	7/28/2005 10:51	0.999	0.8874	1.636	3223.022	88.44%
23555	2355.50	0.4061	0.296	7/28/2005 10:51	0.999	0.7167	1.937	4252.948	116.71%
25567	2556.70	0.3977	0.36	7/28/2005 10:51	0.999	0.8191	1.864	4124.728	113.19%
23587	2358.70	0.3846	0.338	7/28/2005 10:51	0.999	0.8532	1.806	3777.228	103.65%
26230	2623.00	0.3682	0.348	7/28/2005 10:52	0.999	0.9556	1.703	3917.583	107.50%
25997	2599.70	0.3528	0.386	7/28/2005 10:52	0.999	1.0011	1.766	3868.023	106.14%
26435	2643.50	0.3237	0.42	7/28/2005 10:52	0.999	1.1409	1.745	3762.025	103.23%
26101	2610.10	0.3139	0.414	7/28/2005 10:52	0.999	1.1433	1.786	3822.424	104.89%
22288	2228.80	0.3046	0.32	7/28/2005 10:52	0.999	0.9784	1.948	3930.475	107.86%
24112	2411.20	0.2889	0.366	7/28/2005 10:52	0.999	1.0444	2.025	4199.302	115.23%
22831	2283.10	0.2864	0.402	7/28/2005 10:52	0.999	0.9742	2.271	4300.541	118.01%
21369	2136.90	0.2483	0.384	7/28/2005 10:53	0.999	1.0396	2.411	4349.436	119.35%
22530	2253.00	0.4156	0.334	7/28/2005 11:09	0.999	0.8874	1.600	3210.006	88.09%
24318	2431.80	0.4129	0.32	7/28/2005 11:09	0.999	0.7167	1.961	4317.153	118.47%
25689	2568.90	0.3967	0.35	7/28/2005 11:09	0.999	0.8191	1.848	4153.294	113.97%
23412	2341.20	0.3802	0.394	7/28/2005 11:09	0.999	0.8532	1.937	3791.786	104.05%

VERRAW.XLS

INSTR_ID	SAMPLE_ID	CNT_TIME	A	B	TIME	USER2
Instrument 1 - A	1	10	112	22806	7/28/2005 10:51	1575
Instrument 1 - B	2	10	88	23555	7/28/2005 10:51	1575
Instrument 1 - C	3	10	212	25567	7/28/2005 10:51	1575
Instrument 1 - D	4	10	331	23587	7/28/2005 10:51	1575
Instrument 2 - A	5	10	310	26230	7/28/2005 10:52	1575
Instrument 2 - B	6	10	14	25997	7/28/2005 10:52	1575
Instrument 2 - C	7	10	357	26435	7/28/2005 10:52	1575
Instrument 2 - D	8	10	314	26101	7/28/2005 10:52	1575
Instrument 3 - A	9	10	192	22288	7/28/2005 10:52	1575
Instrument 3 - B	10	10	240	24112	7/28/2005 10:52	1575
Instrument 3 - C	11	10	308	22831	7/28/2005 10:52	1575
Instrument 3 - D	12	10	276	21369	7/28/2005 10:53	1575
Instrument 4 - A	1	10	183	22530	7/28/2005 11:09	1575
Instrument 4 - B	2	10	30	24318	7/28/2005 11:09	1575
Instrument 4 - C	3	10	273	25689	7/28/2005 11:09	1575
Instrument 4 - D	4	10	602	23412	7/28/2005 11:09	1575

for 2/2/06

**General Engineering Laboratories
Verification Source Preparation Sheet**

Applicable SOP Number GL-RAD-A-018 Isotope Pb-210
 Date Standards Prepared 7/14/05 Cocktail Type Used N/A
 Standard ID ET491-A Matrix of Vial/Planchett Lead chromate precipitate on Tuffryn filter
 Amount Used (g or ml) 0.1 Type of Scintillation Vial N/A
 Standard Activity (DPM/g or ml) 112301.8 Pipette ID Used 1429303
 Reference Date 1/1/95 Balance ID Used N/A
 Expiration Date 11/1/05 Quenching Agent N/A
 Residue/Carrier Agent Lead Carrier 14.65 ^{ug}/ml

Separation Date/Time: 7/14/05 0800

Standard Number	Quenching Vol (uL)/ Residue Volume (mL)	Initial Wt. (g)	Final Wt. (g)	Net Wt. (mg)
V1	0.1	0.0839	0.0843	0.49 0.0852
V2	0.2	0.0841	0.0856	1.5 0.0862
V3	0.3	0.0840	0.0876	3.6
V4	0.4	0.0856	0.0906	5.0
V5	0.5	0.0846	0.0916	7.0
V6	0.6	0.0844	0.0932	8.8
V7	0.7	0.0839	0.0956	11.7
V8	0.8	0.0859	0.0993	13.4
V9	0.9	0.0879	0.1008	12.9
V10	1.0	0.0844	0.0997	15.3
V11	1.1	0.0867	0.1024	13.7
V12	1.3	0.0840	0.1038	19.8

1.3
2.1

Prepared By: [Signature]

Date

7/29/05

Reviewed By: [Signature]

Date

2/20/08

Rev 1 RLM 9/10/97

DEUTSCHER KALIBRIERDIENST (DKD)

Kalibrierlaboratorium für Meßgrößen der Radioaktivität
 Calibration laboratory for measurements of radioactivity

AKKREDITIERT DURCH DIE PHYSIKALISCH-TECHNISCHE BUNDESANSTALT (PTB)



Amersham Buchler GmbH & Co KG
 Postfach 11 49 Gieselweg 1
 D-38001 Braunschweig D-38110 Braunschweig

Telefon (05307) 930-0
 Telefax (05307) 930-293
 Telefax-Zentrale 930-237

Kalibrierschein Calibration Certificate

Kalibrierzeichen
 Calibration mark

02628
DKD-K- 06501
95-10

Gegenstand <i>Object</i>	Radioactive Reference Solution
Hersteller <i>Manufacturer</i>	Amersham Buchler GmbH & Co KG Postfach 11 49 Gieselweg 1 D-38001 Braunschweig D-38110 Braunschweig
Typ <i>Type</i>	RBZB44
Strahler-Nr. <i>Source number</i>	ET 491
Auftraggeber <i>Customer</i>	Amersham Corporation 2636 S. Clearbrook Drive Arlington Heights, IL 60005 USA-Arlington Heights, IL
Auftragsnummer <i>Work order number</i>	112116
Anzahl der Seiten des Kalibrierscheines <i>Number of pages of the certificate</i>	2
Referenzdatum <i>Reference date</i>	1 January 1995

Der Deutsche Kalibrierdienst ist Unterzeichner des multilateralen Übereinkommens der Western European Calibration Cooperation (WECC) zur gegenseitigen Anerkennung der Kalibrierscheine. Die Kalibrierung erfolgt auf der Grundlage des zwischen der Physikalisch-Technischen Bundesanstalt und dem Träger abgeschlossenen Vertrages. Dieser Kalibrierschein dokumentiert die Rückführbarkeit auf nationale Normale zur Darstellung der physikalischen Einheiten in Übereinstimmung mit dem Internationalen Einheitensystem (SI). Für die Einhaltung einer angemessenen Frist zur Wiederholung der Kalibrierung ist der Benutzer verantwortlich. *The Deutscher Kalibrierdienst is signatory to the multilateral agreement of the Western European Calibration Cooperation (WECC) for the mutual recognition of calibration certificates. The calibration is performed according to the stipulations of the contract between the Physikalisch-Technische Bundesanstalt and the holder of the calibration laboratory. This calibration certificate documents the traceability to national standards, which realize the physical units of measurement according to the International System of Units (SI). The user is obliged to have the object recalibrated at appropriate intervals.*

Dieser Kalibrierschein darf nur vollständig und unverändert weiterverbreitet werden. Auszüge oder Änderungen bedürfen der Genehmigung sowohl der Physikalisch-Technischen Bundesanstalt als auch des ausstellenden Kalibrierlaboratoriums. Kalibrierscheine ohne Unterschrift und Stempel haben keine Gültigkeit. *This calibration certificate may not be reproduced other than in full except with the permission of both the Physikalisch-Technische Bundesanstalt and the issuing laboratory. Calibration certificates without signature and seal are not valid.*

Stempel <i>Seal</i>	Datum <i>Date</i>	Leiter des Kalibrierlaboratoriums <i>Head of the calibration laboratory</i>	Stellvertreter <i>Deputy</i>	Bearbeiter <i>Person responsible</i>
	18 October 1995	Dr. Dornhöfer	Dr. Thieme	E. Schuber PC-5-013-4



DEUTSCHER KALIBRIERDIENST (DKD)

PAGE 2 OF CALIBRATION CERTIFICATE FROM 18 October 1995

02628
DKD-K-06501
95-10

Radioactive Reference Solution

Solution No.: ET 491

Drawing No.: VZ-2058

Nuclide: Lead-210

Radioactive concentration: 38.1 kBq/g

Reference date: 1 January 1995 at 12.00 GMT

Mass of solution: (5.182 ± 0.001) g

Volume of solution: approx. 5 ml

Chemical composition: Solution in 1.2 M HNO₃
Carrier: Pb (NO₃)₂, Bi (NO₃)₃; each 20 mg/l of the corresponding element.

Measuring method: The activity was determined by comparison with a reference solution by measurement with a Ge-detector with MCA.

Traceability: Additional to the direct traceability to the PTB through the DKD this product satisfies the quality assurance requirements of USNRC Regulatory Guide 4.15 Revision 1, February 1979, for achieving NIST traceability through Amersham's participation in the NEI-NIST Measurements Assurance Program of the Nuclear Power Industry.

Uncertainty: The relative uncertainty of the activity is ± 3 %.

The declared uncertainty U is an expanded uncertainty $U = k \cdot u_c$ with a coverage factor of $k = 3$. The combined uncertainty u_c is the sum of all uncertainties which can be evaluated by statistical means (uncertainty type A, u_A) and all other uncertainties (uncertainty type B, u_B) whereby $u_c^2 = u_A^2 + u_B^2$.
(Ref.: NIST Technical Note 1297 / WECC-Doc. 19-1990)

Radioactive impurities: Related to Pb-210 (equal 100 %) the following radioactive impurities were detected:
Ra-226: 0.003 %



Handwritten signature and date: 18/10/95
Handwritten reference: LC-5-013-4A



TRACEABILITY TO NIST

Amersham Corporation
2636 S. Clearbrook Drive
Arlington Heights, IL 60005
tel (708) 593-6300
fax (708) 593-8091



Traceability is the ability to relate the accuracy of measurement of radionuclides to the National Institute of Standards and Technology (NIST). Traceability is achieved by participation in a Measurements Assurance Program linked to NIST and production of certified materials in accordance with a quality assurance program.

Amersham participates in measurement assurance programs conducted by NIST in cooperation with the Nuclear Energy Institute (NEI, formerly USCEA). Additionally, our production facilities and measurement laboratories operate under routinely audited quality assurance programs.

Therefore, Amersham certified standardized products meet or exceed, the NRC requirements for measurements traceable to NIST.

278004C

mu 7/25/06

RC-S-013-4B



Standard Traceability Log Rad

Source Material Info		A Solution Material Info	
Parent Code:	ET491	Isotope:	Lead-210
Prepared By:	Garret Ray	Prepared By:	Garret Ray
Carrier Conc:	1.2M HNO3	Prep Date:	03/01/1996
Reference Date:	01/01/1995	Verification Date:	07/12/2005
Ampoule Mass (g):	5.182 g	Expiration Date:	07/12/2006
Uncertainty:	+/- 3 %	Primary Code:	ET491-A
LogBook No:	RC S 014 004	Dilution(mL):	100 mL
		Mass of Parent(g):	5.0547 g
		Density(g/mL):	1.0000

Calculations Converting parent activity to dpm/mL|dpm/g

$(\text{Mass of parent(g)}) * (\text{Parm Activity (kBq/g)}) * (\text{conversion dpm to kBq}) / (\text{Dilution Vol}) = \text{Parent Activity (dpm/mL)}$
$(\text{Mass of parent(g)}) * (\text{Parm Activity (kBq/g)}) * (\text{conversion dpm to kBq}) / \text{Density (g/mL)} / (\text{Dilution Vol}) = \text{Parent Activity (dpm/g)}$
$(5.0547 \text{ g}) * (38.1 \text{ kBq/g}) * (60000 \text{ dpm/kBq}) / (100 \text{ mL}) = 115550.4420 \text{ dpm/mL}$
$(5.0547 \text{ g}) * (38.1 \text{ kBq/g}) * (60000 \text{ dpm/kBq}) / (1.0000 \text{ g/mL}) / (100 \text{ mL}) = 115550.4420 \text{ dpm/g}$

Secondary Standards

Prep Date	Preparer	Mass Primary	Dilution (mL)	Code	Conc dpm/mL	Verification Date	Expiration Date
10/20/1997	Richard Kinney	.467	100	ET491-B	524.45 dpm/ml	03/01/1997	03/01/1998
10/29/1997	Richard Kinney	3.0992	500	ET491-C	696.09 dpm/mL	10/29/1998	10/29/1999
04/03/2001	Angela Albee	.5184	100	ET491-D	582.17 dpm/mL	04/16/2003	04/16/2004
09/15/2003	Angela Albee	.5132	100	ET491-E	576.33 dpm/mL	11/11/2004	11/11/2005

General Engineering Laboratories, LLC
Version 1.0 9/18/2000

m 7/29/05

Verification for Pb-210 Standard ET491-A

A. Fehr
7/12/2005

JAG
7/29/05

Isotope	Detector CPM	BKG CPM	NET CPM	Detector Eff	Mass. Used (g)	Standard	Source DPM/ μ rc ⁻² g
ET491-E N1	22785.6000	20.2000	22785.6000	2.63365	0.1038		83349.97114
ET491-E N2	22178.6000	20.2000	22178.6000	2.63365	0.1033		81522.24763
ET491-E N3	22065.7000	20.2000	22065.7000	2.63365	0.1031		81264.5963
						Average =	82045.60502

Mean Value (Counting) = 82045.60502 101.400909 Pass
 Stdev = 1136.936355 0.01385737 Rule 3 (Pass/Fail)

Certificate Value = 80912.1
 Lower Limit = 79771.73231
 Upper Limit = 84319.47773
 Rule 1 Pass/Fail Pass
 Two sigma = 2273.872711
 10 % of Mean = 8204.560502
 Rule 2 (Pass/Fail) Pass

Verification Rules

- Rule 1 = The certificate value (NOT including any uncertainty) shall lie within the 95% confidence interval determined from the mean and two sigma standard deviation of the three measurements
- Rule 2 = The two sigma value used for the 95% confidence interval shall not exceed 10% of the mean value of the three verification measurements.
- Rule 3 = The determined mean value shall be within 10% of the certificate value.

The analyst prepared three calibration sources for source ET491-A by transferring 0.1 mL portions of the standard to glass liquid scintillation vials. Ten mL of Ready Gel liquid scintillation cocktail was added to each vial and the vials were shaken to mix. A Blank vial was prepared in a similar fashion using 1 mL of DI water and 10 mL of Ready Gel cocktail. The calibration vials and background source were dark adapted for two hours and counted on LSC Yellow (Wallac) using Protocol 31 for Pb-210 standard verification. The efficiency calibration which was used for verification calculations was performed on 7/12/05 using source 0356-A (Pb-210). Each verification source calculation was performed as follows:

$$\text{Source dpm/g} = (A - B)/(C/D)$$

where:

- A = Ver. source cpm,
- B = BKG cpm,
- C = System efficiency, (cpm/dpm), and
- D = mass used for standard verification.

Reference RAD SOP M-001

Margaret A. Johnson
7/29/05

PROTOCOL : 31 Pb-210 Verification
DATE : 2005/07/12
TIME : 05:29
ID : P31AS005

Wallac 1414 WinSpectral v1.40 S/N 4140127

Counting mode : CPM
Isotope(s) : Pb210
Pb210 = 5- 520,21.00 y
Protocol name : Pb-210 Verification
Counting time : 300
Repeats : 1
Cycles : 1
Replicates : 1
2 sigma % : 0.01
Minimum cpm : 0.00 Checking time: 10
Advanced modes : Chemilum,PSA
PSA level : 35
Output to Display :
POS,CTIME,DATE,TIME,RACKPOS,CPMw1,CPM,SQPI,CPM1
Additions to Display : Spectrum,Header,Listing
Spectrum : Alpha,Beta
Window 1 : 685- 745 /Alpha
Window 2 : 1-1024 /Beta
Window 3 : 1-1024 /Beta
Window 4 : 1-1024 /Beta
Window 5 : 1-1024 /Beta
Window 6 : 1-1024 /Beta
FNCT1 = FNCT1 :
FNCT2 = FNCT2 :
FNCT3 = FNCT3 :
FNCT4 = FNCT4 :


Total count rate:
Pb210 72372.3 CPM

ast 7/12/05

Handwritten signatures and dates:
7/29/05
7/29/05

POS CTIME DATE TIME RACKPOS CPM

1 300 7/12/2005 5:29 AM 1 20.20

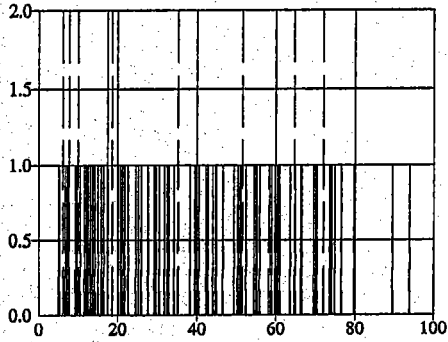


Counts Alpha

Counts Beta

Bkg

2 300 7/12/2005 5:35 AM 2 22785.60

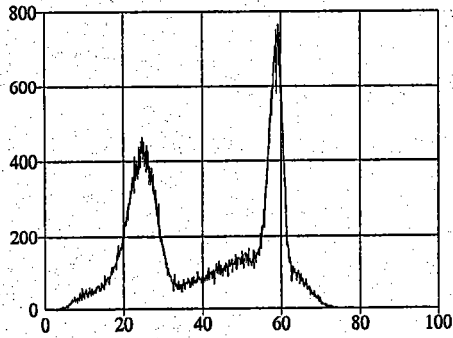


Counts Alpha

Counts Beta

ET491-A

3 300 7/12/2005 5:41 AM 3 22178.60

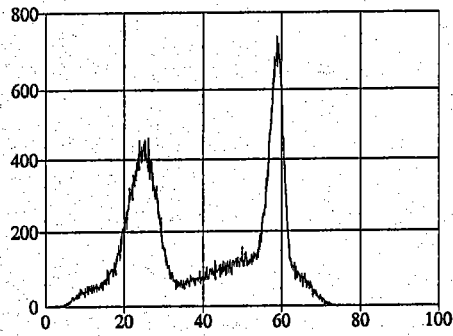

Counts Alpha


Counts Beta

ET491-A

ALF 7/12/05

m 7/24/05
7/29/05


POS	CTIME	DATE	TIME	RACKPOS	CPM
4	300	7/12/2005	5:46 AM	4	22065.70

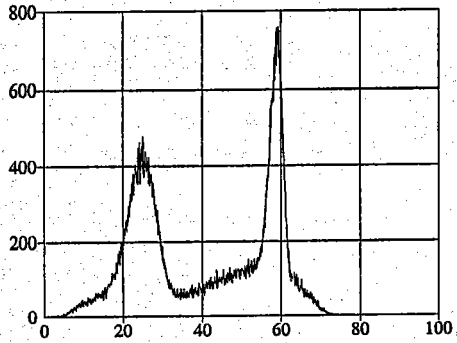

Counts Alpha
Counts Beta

ET491-A


5	300	7/12/2005	5:52 AM	5	21.70
---	-----	-----------	---------	---	-------

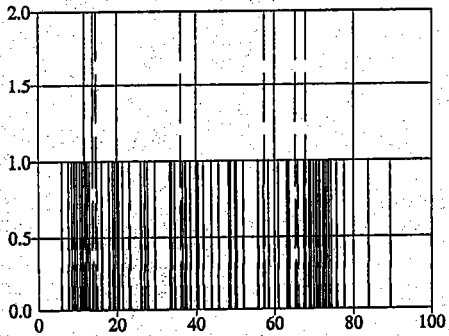

Counts Alpha
Counts Beta

Bkg

6	300	7/12/2005	5:58 AM	6	20294.00
---	-----	-----------	---------	---	----------

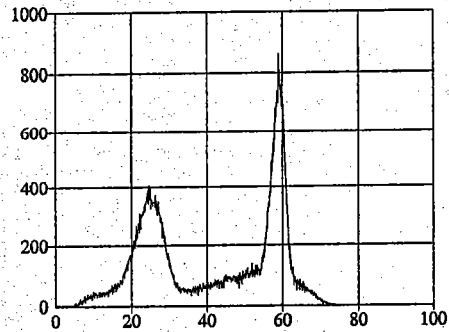

Counts Alpha
Counts Beta

0356-A


awf7/12/05

Handwritten signature

Handwritten initials and date
JLQ
7/29/05

POS CTIME DATE TIME RACKPOS CPM

7 300 7/12/2005 6:04 AM 7 20276.60

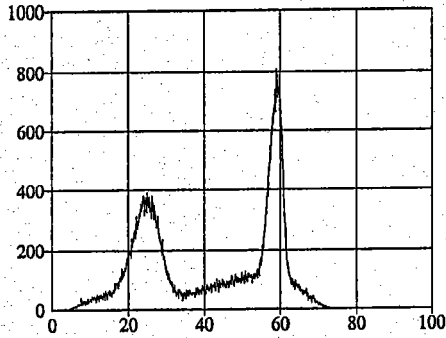


Counts Alpha

Counts Beta

0356-A

8 300 7/12/2005 6:09 AM 8 20079.70

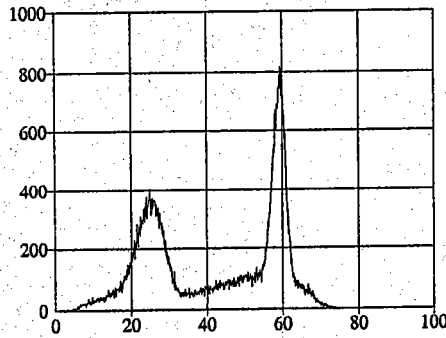

Counts Alpha

Counts Beta

0356-A

AWF 7/12/05

AWF 7/12/05
AWF
7/29/05

Alpha Spectroscopy Calibration Sources

The following is a summary of the procedure performed for preparing mixed alpha calibration standards:

A calibration stock solution was prepared by combining the following in a volumetric flask and diluting to 50 ml (51.4561 grams). These individual standards were first verified by direct precipitation of small aliquots of each standard (as described in Attachment I).

Isotope	Serial #	amount used (g)	dpm (note 1)
Gd-148	64445-278	0.2471	212.159287
Np-237	4341	1.8075	204.438594
Cm-244	4320A	7.2704	240.144737

Note 1: Dpm values are decay corrected to 2/7/2003.

Forty one weighted aliquots were then directly precipitated using Neodymium Flouride /HF system. The sources were then mounted on 0.1Poly-propylene filters and taped securely to 1 inch stainless steel planchettes for counting in an Alpha Spectroscopy system. The liquid fraction that passes through the filter is collected, traced with Am-241 and prepared for counting using the identical procedure. These samples are counted to ensure there is no more than 1% loss in the filtering processes. All sources pass this requirement. The DPM information for each source is listed in attachment II.

Certificate files were then created on the Alpha system used for acquisition and processing of data. Each source is assigned a name (AESS-001 through AESS-041). The information for the source activities is entered into the certificate files appropriate for the detector being used.

For example: If source AESS-001 is used for calibrating detector 25, the source data is entered into the certificate file name [env_alpha.cer]U025.cer.

The computer software uses these certificate files to calculate an energy calibration and determine the efficiency of the detector after counting the source.

Ante Hill
4/1/03

2002 Alpha Eff Source Stock Verification

Curium-244

Isotope	Value pCi/g
SSTOCK2002A2_AM	106.000
SSTOCK2002B2_AM	106.000
SSTOCK2002C2_AM	106.000

Mean Value (Counting) = 106.000 98.04%
 Stdev = 0 pCi/g

Target = 108.1230
 Lower Limit = 106
 Upper Limit = 106
 Rule 1 Pass/Fail Pass
 Two sigma = 0
 10 % of Mean = 10.6
 Rule 2 (Pass/Fail) Pass

PASS
 Fair 3/2/0

Neptunium-237

Isotope	Value pCi/g
SSTOCK2002A2_AM	90.100
SSTOCK2002B2_AM	87.200
SSTOCK2002C2_AM	93.500

Mean Value (Counting) = 90.267 98.02%
 Stdev = 3.153305144 pCi/g

Target = 92.0900
 Lower Limit = 83.96005638
 Upper Limit = 96.57327696
 Rule 1 Pass/Fail Pass
 Two sigma = 6.306610289
 10 % of Mean = 9.026666667
 Rule 2 (Pass/Fail) Pass

Gadolinium-148

Isotope	Value pCi/g
SSTOCK2002A2_AM	95.080
SSTOCK2002B2_AM	93.750
SSTOCK2002C2_AM	96.560

Mean Value (Counting) = 95.463 99.81%
 Stdev = 1.503074627 pCi/g

Target = 95.6460
 Lower Limit = 92.45718408
 Upper Limit = 98.46948259
 Rule 1 Pass/Fail Pass
 Two sigma = 3.006148253
 10 % of Mean = 9.546333333
 Rule 2 (Pass/Fail) Pass

The analyst prepared three standard verification sources for the mixed alpha stock standard using 0.1030 g for source #1, 0.1035 g for source #2 and 0.1028 g for source #3. Each standard was combined with 1.0 mL of Am-243 standard 0454-A and 0.1 mL of Nd carrier in a disposable centrifuge tube. Four mL of 2 M HCl was added to each standard and then diluted with 4 mL of DI water. 5 mL of ascorbic acid was added to each sample then one mL of 48% HF was added to precipitate Nd (and Curium) fluoride. After 30 minutes, each sample was filtered following routine procedures for alpha spectroscopy source preparation. Each source was counted using routine alpha spec procedures. pCi/L values for the Mixed Alpha Stock were calculated and compared to Am-243 certified values.

① The rule failed because the 3 results from 3 sources were the same. Therefore, the stdev was zero. The intent of this rule is to ensure an appropriate amount of counts are achieved for proper determinations. ~~Since~~ For each standard the # of counts achieved was just under 10000 which has a counting error of nearly 1%. Because the standard's bias is < 2% from the known value the standard is acceptable.

Robertson 02/20/03

Attachment II

Mixed alpha isotope	Reference date = Source	Stock Dpm/g	Reference date	Half-life (years)	amount used for mixed	Dpm/g mixed	Decay corr dpm/g
Gd-148	64445-278 (0502)	44354.59289	9/5/2002	74.60	0.2471	212.9974853	212.159287
Np-237	Srm 4341 (0493)	5820	3/1/1992	2.14E+06	1.8075	204.4393182	204.438594
Cm-244	SRM 4320a (0490)	2223.6	2/1/1996	18.1	7.2704	314.1796879	240.144737
Source	Amount of standard used	dpm Gd-148	dpm Np-237	dpm Cm-244	dps Gd-148	dps Np-237	dps Cm-244
AESS-001	1.0362	219.839	211.839	248.838	3.664	3.531	4.147
AESS-002	1.0344	219.458	211.471	248.406	3.658	3.525	4.140
AESS-003	1.034	219.373	211.390	248.310	3.656	3.523	4.138
AESS-004	1.0331	219.182	211.206	248.094	3.653	3.520	4.135
AESS-005	1.0353	219.649	211.655	248.622	3.661	3.528	4.144
AESS-006	1.0331	219.182	211.206	248.094	3.653	3.520	4.135
AESS-007	1.0348	219.542	211.553	248.502	3.659	3.526	4.142
AESS-008	1.0363	219.861	211.860	248.862	3.664	3.531	4.148
AESS-009	1.0352	219.627	211.635	248.598	3.660	3.527	4.143
AESS-010	1.0346	219.500	211.512	248.454	3.658	3.525	4.141
AESS-011	1.0353	219.649	211.655	248.622	3.661	3.528	4.144
AESS-012	1.0367	219.946	211.941	248.958	3.666	3.532	4.149
AESS-013	1.0396	220.561	212.534	249.654	3.676	3.542	4.161
AESS-014	1.0368	219.967	211.962	248.982	3.666	3.533	4.150
AESS-015	1.0363	219.861	211.860	248.862	3.664	3.531	4.148
AESS-016	1.0353	219.649	211.655	248.622	3.661	3.528	4.144
AESS-017	1.0356	219.712	211.717	248.694	3.662	3.529	4.145
AESS-018	1.0359	219.776	211.778	248.766	3.663	3.530	4.146
AESS-019	1.0349	219.564	211.574	248.526	3.659	3.526	4.142
AESS-020	1.0361	219.818	211.819	248.814	3.664	3.530	4.147
AESS-021	1.0348	219.542	211.553	248.502	3.659	3.526	4.142
AESS-022	1.0353	219.649	211.655	248.622	3.661	3.528	4.144
AESS-023	1.0353	219.649	211.655	248.622	3.661	3.528	4.144
AESS-024	1.0343	219.436	211.451	248.382	3.657	3.524	4.140
AESS-025	1.0364	219.882	211.880	248.886	3.665	3.531	4.148
AESS-026	1.0336	219.288	211.308	248.214	3.655	3.522	4.137
AESS-027	1.0353	219.649	211.655	248.622	3.661	3.528	4.144
AESS-028	1.0366	219.924	211.921	248.934	3.665	3.532	4.149

Attachment II

AESS-029	1.0355	219.691	211.696	248.670	3.662	3.528	4.144
AESS-030	1.0349	219.564	211.574	248.526	3.659	3.526	4.142
AESS-031	1.0343	219.436	211.451	248.382	3.657	3.524	4.140
AESS-032	1.0326	219.076	211.103	247.973	3.651	3.518	4.133
AESS-033	1.0308	218.694	210.735	247.541	3.645	3.512	4.126
AESS-034	1.0314	218.821	210.858	247.685	3.647	3.514	4.128
AESS-035	1.0303	218.588	210.633	247.421	3.643	3.511	4.124
AESS-036	1.0343	219.436	211.451	248.382	3.657	3.524	4.140
AESS-037	1.0353	219.649	211.655	248.622	3.661	3.528	4.144
AESS-038	1.0373	220.073	212.064	249.102	3.668	3.534	4.152
AESS-039	1.0334	219.245	211.267	248.166	3.654	3.521	4.136
AESS-040	1.0346	219.500	211.512	248.454	3.658	3.525	4.141
AESS-041	1.0352	219.627	211.635	248.598	3.660	3.527	4.143



0490
0491

National Institute of Standards & Technology

Certificate

Standard Reference Material 4320A Curium-244 Radioactivity Standard

This Standard Reference Material (SRM) consists of radioactive curium-244 nitrate and nitric acid dissolved in 5 mL of distilled water. The solution is contained in a flame-sealed NIST borosilicate-glass ampoule. The SRM is intended for the calibration of alpha-particle counting instruments and for the monitoring of radiochemical procedures.

Radiological Hazard

The SRM ampoule contains curium-244 with a total activity of approximately 200 Bq. Curium-244 decays by alpha-particle emission to plutonium-240, which also decays by alpha-particle emission. None of the alpha particles escape from the SRM ampoule. During the decay process X-rays and gamma rays with energies from 40 keV to 1100 keV are also emitted. Most of these photons escape from the SRM ampoule but their intensities are so small that they do not represent a radiation hazard. Approximate unshielded dose rates at several distances (as of the reference time) are given in note [a]*. The SRM should be used only by persons qualified to handle radioactive material.

Chemical Hazard

The SRM ampoule contains nitric acid (HNO_3) with a concentration of 1 mole per liter of water. The solution is corrosive and represents a health hazard if it comes in contact with eyes or skin. If the ampoule is to be opened to transfer the solution, the recommended procedure is given on page 2. The ampoule should be opened only by persons qualified to handle both radioactive material and strong acid solution.

Storage and Handling

The SRM should be stored and used at a temperature between 5 and 65 °C. The solution in an unopened ampoule should remain stable and homogeneous until at least February 2006.

The ampoule (or any subsequent container) should always be clearly marked as containing radioactive material. If the ampoule is transported it should be packed, marked, labeled, and shipped in accordance with the applicable national, international, and carrier regulations. The solution in the ampoule is a dangerous good (hazardous material) both because of the radioactivity and because of the strong acid.

Preparation

This Standard Reference Material was prepared in the Physics Laboratory, Ionizing Radiation Division, Radioactivity Group, J.M.R. Hutchinson, Group Leader. The overall technical direction and physical measurements leading to certification were provided by L.L. Lucas of the Radioactivity Group.

The support aspects involved in the preparation, certification, and issuance of this SRM were coordinated through the Standard Reference Materials Program by N.M. Trahey.

Gaithersburg, Maryland 20899
February 1996 (Text only revised November 1997)

Thomas E. Gills, Chief
Standard Reference Materials Program

Recommended Procedure for Opening the SRM Ampoule

- 1) If the SRM solution is to be diluted, it is recommended that the diluting solution have a composition comparable to that of the SRM solution.
- 2) Wear eye protection, gloves, and protective clothing and work over a tray with absorbent paper in it. Work in a fume hood. In addition to the radioactive material, the solution contains strong acid and is corrosive.
- 3) Shake the ampoule to wet all of the inside surface of the ampoule. Return the ampoule to the upright position.
- 4) Check that all of the liquid has drained out of the neck of the ampoule. If necessary, gently tap the neck to speed the process.
- 5) Holding the ampoule upright, score the narrowest part of the neck with a scribe or diamond pencil.
- 6) Lightly wet the scored line. This reduces the crack propagation velocity and makes for a cleaner break.
- 7) Hold the ampoule upright with a paper towel, a wiper, or a support jig. Position the scored line away from you. Using a paper towel or wiper to avoid contamination, snap off the top of the ampoule by pressing the narrowest part of the neck away from you while pulling the tip of the ampoule towards you.
- 8) Transfer the solution from the ampoule using a pycnometer or a pipet with dispenser handle.
NEVER PIPETTE BY MOUTH
- 9) Seal any unused SRM solution in a flame-sealed glass ampoule, if possible, to minimize the evaporation loss.

See also reference [4]*.

PROPERTIES OF SRM 4320A
(Certified values are shown in bold type)

Source identification number	NIST SRM 4320A		
Physical Properties:			
Source description	Liquid in flame-sealed NIST borosilicate-glass ampoule		
Ampoule specifications	Body outside diameter	(16.5 ± 0.5) mm	
	Wall Thickness	(0.60 ± 0.04) mm	
	Barium content	Less than 2.5%	
	Lead-oxide content	Less than 0.02%	
	Other heavy elements	Trace quantities	
Solution density	(1.030 ± 0.002) g·mL ⁻¹ at 22.8 °C [b]*		
Solution mass	Approximately 5.15 g		
Chemical Properties:			
Solution composition	Chemical Formula	Concentration (mol·L ⁻¹)	Mass Fraction (g·g ⁻¹)
	H ₂ O	54	0.94
	HNO ₃	1.0	0.06
	HCl	<0.001	<4 × 10 ⁻⁵
	²⁴⁴ Cm +3	5 × 10 ⁻¹¹	1 × 10 ⁻¹¹
Radiological Properties:			
Radionuclide	Curium-244		
Reference time	1230 EST, 1 February 1996 [c]		
Massic activity of the solution [d]	37.06 Bq·g ⁻¹ 24.12 Bq·g ⁻¹		
Relative expanded uncertainty (k=2)	0.68% [e] [f]		
Alpha-particle-emitting daughters	Plutonium-240: (0.22 ± 0.11) Bq·g ⁻¹ [b] [c]		
Alpha-particle-emitting impurities	Curium-243: (0.005 ± 0.004) Bq·g ⁻¹ [b] [g]		
Photon-emitting impurities	None detected [h]		
Half lives used in the decay corrections	Curium-244: (18.10 ± 0.02) a [i] Plutonium-240: (6563 ± 7) a [i]		
Calibration method	Two 4π liquid-scintillation counting systems		

- [i] The stated uncertainty is the standard uncertainty. See reference [5].
- [j] Relative standard uncertainty of the input quantity x_i .
- [k] The relative change in the output quantity y divided by the relative change in the input quantity x_i . If $|\partial y/\partial x_i| \cdot (x_i/y) = 1.0$, then a 1% change in x_i results in a 1% change in y . If $|\partial y/\partial x_i| \cdot (x_i/y) = 0.05$, then a 1% change in x_i results in a 0.05% change in y .
- [m] Relative component of combined standard uncertainty of output quantity y , rounded to two significant figures or less. The relative component of combined standard uncertainty of y is given by $u_i(y)/y = |\partial y/\partial x_i| \cdot u(x_i)/y = |\partial y/\partial x_i| \cdot (x_i/y) \cdot u(x_i)/x_i$. The numerical values of $u(x_i)/x_i$, $|\partial y/\partial x_i| \cdot (x_i/y)$, and $u_i(y)/y$, all dimensionless quantities, are listed in columns 3, 4, and 5, respectively. Thus, the value in column 5 is equal to the value in column 4 multiplied by the value in column 3. The input quantities are independent, or very nearly so. Hence the covariances are zero or negligible.
- [n] The relative standard uncertainty of $\lambda \cdot t$ is determined by the relative standard uncertainty of λ (i.e., of the half life). The relative standard uncertainty of t is negligible.
- [p] $|\partial y/\partial x_i| \cdot (x_i/y) = |\lambda \cdot t|$
- [q] The live time is determined by counting the pulses from a gated oscillator.
- [r] The standard uncertainty given is for the detected Cm-243 impurity. $|\partial y/\partial x_i| \cdot (x_i/y) = \{(\text{response per Bq of impurity})/(\text{response per Bq of Cm-244})\} \cdot \{(\text{Bq of impurity})/(\text{Bq of Cm-244})\}$.
- [s] The standard uncertainty for each undetected impurity that might reasonably be expected to be present is estimated to be equal to the estimated limit of detection for that impurity, i.e. $u(x_i)/x_i = 100\%$. $|\partial y/\partial x_i| \cdot (x_i/y) = \{(\text{response per Bq of impurity})/(\text{response per Bq of Cm-244})\} \cdot \{(\text{Bq of impurity})/(\text{Bq of Cm-244})\}$. Thus $u_i(y)/y$ is the relative change in y if the impurity were present with a massic activity equal to the estimated limit of detection.

REFERENCES

- [1] International Organization for Standardization (ISO), *ISO Standards Handbook - Quantities and Units*, 1993. Available from the American National Standards Institute, 11 West 42nd Street, New York, NY 10036, U.S.A. 1-212-642-4900.
- [2] International Organization for Standardization (ISO), *Guide to the Expression of Uncertainty in Measurement*, 1993. Available from the American National Standards Institute, 11 West 42nd Street, New York, NY 10036, U.S.A. 1-212-642-4900. (Listed under ISO miscellaneous publications as "ISO Guide to the Expression 1993".)
- [3] B. N. Taylor and C. E. Kuyatt, *Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Results*, NIST Technical Note 1297, 1994. Available from the Superintendent of Documents, U.S. Government Printing Office, Washington, DC 20407, U.S.A.
- [4] National Council on Radiation Protection and Measurements Report No. 58, *A Handbook of Radioactivity Measurements Procedures*, Second Edition, 1985. Available from the National Council on Radiation Protection and Measurements, 7910 Woodmont Avenue, Bethesda, MD 20814 U.S.A.
- [5] Evaluated Nuclear Structure Data File (ENSDF), February 1996.



CERTIFICATE OF CALIBRATION

Standard Radionuclide Source

64445-278

Gd-148 5 mL Liquid in Flame Sealed Vial

This standard radionuclide source was prepared gravimetrically from a calibrated master liquid radionuclide solution source. The master source was calibrated by liquid scintillation counting.

ANALYTICS maintains traceability to the National Institute of Standards and Technology through Measurements Assurance Programs as described in USNRC Reg. Guide 4.15, Revision 1.

Radionuclide purity and calibration were checked using a germanium gamma spectrometer system. The nuclear decay rate and assay date for this source are given below.

ISOTOPE:	Gd-148
ACTIVITY (dps):	<u>3.759 E3</u>
HALF-LIFE:	<u>74.6 years</u>
CALIBRATION DATE:	September 5, 2002 12:00 EST
TOTAL UNCERTAINTY*:	2.7%
SYSTEMATIC:	1.9%
RANDOM:	0.8%

99% confidence level.

5.08493 grams 0.1M HCl solution.

P O NUMBER 3207RD, Item 1

SOURCE PREPARED BY:

M.D. Currie
M.D. Currie, Radiochemist

Q A APPROVED:

100. [Signature] 9-6-02

25
31
30
31
31
7

0493



National Institute of Standards & Technology

Certificate

Standard Reference Material 4341 Radioactivity Standard

Radionuclide	Neptunium-237
Source identification	SRM 4341
Source description	Liquid in flame-sealed NIST borosilicate-glass ampoule ⁽¹⁾ *
Solution mass	Approximately 5 grams
Solution composition	Neptunium-237 in 2 mol·L ⁻¹ nitric acid
Reference time	March 1992
Radioactivity concentration	97.0 Bq·g ⁻¹
Overall uncertainty	1.28 percent ⁽²⁾
Photon-emitting impurities	None detected ⁽³⁾
Alpha-particle-emitting impurities	None detected ⁽⁴⁾
Half life	(2.14 ± 0.11) × 10 ⁶ years ⁽⁵⁾
Measuring instrument	NIST "0.8π" α defined-solid-angle counter with scintillation detector

This standard reference material was prepared in the Physics Laboratory, Ionizing Radiation Division, Radioactivity Group, J.M. Robin Hutchinson, Acting Group Leader.

Gaithersburg, MD
January 1993

William P. Reed, Chief
Standard Reference Materials Program

*Notes on back

PC 5 075 000

NOTES

(1) Approximately five milliliters of solution. Ampoule specifications:

body diameter	16.5 ± 0.5 mm
wall thickness	0.60 ± 0.04 mm
barium content	less than 2.5 percent
lead oxide content	less than 0.02 percent
other heavy elements	trace quantities

(2) The overall uncertainty was formed by taking three times the quadratic combination of the standard deviations of the mean, or approximations thereof, for the following:

a) alpha-particle-emission-rate measurements	0.34 percent
b) background	0.01 percent
c) livetime	0.10 percent
d) detection efficiency	0.16 percent
e) count-rate-vs-energy extrapolation to zero energy	0.10 percent
f) half life	0.00 percent
g) gravimetric measurements	0.10 percent
h) alpha-emitting impurities	0.10 percent

(3) The protactinium-233 daughter of neptunium-237 is approximately in equilibrium.
The limit of detection for photon-emitting impurities is

$0.19 \text{ } \gamma \cdot \text{s}^{-1} \cdot \text{g}^{-1}$ for energies between 30 and 307 keV and
 $0.01 \text{ } \gamma \cdot \text{s}^{-1} \cdot \text{g}^{-1}$ for energies between 317 and 1750 keV,

provided that the impurity photons are separated in energy by 5 keV or more from photons emitted in the decay of neptunium-237 and progeny.

(4) The limit of detection for alpha-particle-emitting impurities is

$0.10 \text{ } \alpha \cdot \text{s}^{-1} \cdot \text{g}^{-1}$ for energies between 1.0 and 4.3 MeV and
 $0.05 \text{ } \alpha \cdot \text{s}^{-1} \cdot \text{g}^{-1}$ for energies between 4.9 and 10 MeV.

(5) Evaluated Nuclear Structure Data File (ENSDF), February 1990.

For further information please contact Dr. J.M. Robin Hutchinson at NIST.
Telephone: (301) 975-5532
FAX: (301) 926-7416

Subsection 1: Energy Calibration

The Energy Calibration energy=Cal_Zero+(e1*C)+(e2*C^2)

where : Cal_Zero = Energy Calibration Zero
 e1 = Energy Calibration Slope
 e2 = Energy Calibration Quadratic
 C = Channel

Instrument : CHAMBER 001
 Detector : 33088
 Calibration Date/Time : 3-APR-2006 16:30:52
 Calibration Source Id : AESS-001

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3182.589
NP-237	4341	2/28/06	4768.800	4768.498
CM-244	4320A	2/28/06	5795.020	5794.859

Energy/Channel Equation : see above
 Energy Calibration Zero : 2394.447
 Energy Calibration Slope : 4.976289
 Energy Calibration Quadratic : 2.7050270E-04
 Energy Calibration Range : 7774.000

Instrument : CHAMBER 003
 Detector : 20659
 Calibration Date/Time : 3-APR-2006 16:32:34
 Calibration Source Id : AESS-003

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3182.813
NP-237	4341	2/28/06	4768.800	4768.688
CM-244	4320A	2/28/06	5795.020	5795.021

Energy/Channel Equation : see above
 Energy Calibration Zero : 2371.253
 Energy Calibration Slope : 5.028544
 Energy Calibration Quadratic : 2.5955989E-04
 Energy Calibration Range : 7793.000

Instrument : CHAMBER 004
 Detector : 33077
 Calibration Date/Time : 3-APR-2006 16:32:51
 Calibration Source Id : AESS-004

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3181.835
NP-237	4341	2/28/06	4768.800	4768.419
CM-244	4320A	2/28/06	5795.020	5794.571

Energy/Channel Equation : see above
 Energy Calibration Zero : 2409.653
 Energy Calibration Slope : 4.949907
 Energy Calibration Quadratic : 2.7518670E-04
 Energy Calibration Range : 7767.000

Instrument : CHAMBER 005
 Detector : 28642
 Calibration Date/Time : 3-APR-2006 16:33:05
 Calibration Source Id : AESS-005

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3183.000
NP-237	4341	2/28/06	4768.800	4768.800
CM-244	4320A	2/28/06	5795.020	5794.893

Energy/Channel Equation : see above
 Energy Calibration Zero : 2356.725
 Energy Calibration Slope : 4.952652
 Energy Calibration Quadratic : 3.0983411E-04
 Energy Calibration Range : 7753.000

Instrument : CHAMBER 007
 Detector : 30416
 Calibration Date/Time : 3-APR-2006 16:35:21
 Calibration Source Id : AESS-007

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3183.000
NP-237	4341	2/28/06	4768.800	4768.624
CM-244	4320A	2/28/06	5795.020	5795.021

Energy/Channel Equation : see above
 Energy Calibration Zero : 2382.813
 Energy Calibration Slope : 4.944474
 Energy Calibration Quadratic : 3.1966669E-04
 Energy Calibration Range : 7781.000

Instrument : CHAMBER 009
 Detector : 13285
 Calibration Date/Time : 3-APR-2006 16:39:51
 Calibration Source Id : AESS-009

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3182.700
NP-237	4341	2/28/06	4768.800	4768.800
CM-244	4320A	2/28/06	5795.020	5794.917

Energy/Channel Equation : see above
 Energy Calibration Zero : 2406.029
 Energy Calibration Slope : 4.889740
 Energy Calibration Quadratic : 3.3907106E-04
 Energy Calibration Range : 7769.000

Instrument : CHAMBER 010
 Detector : 33083
 Calibration Date/Time : 3-APR-2006 16:40:04
 Calibration Source Id : AESS-010
 Cal. Isotopes Source Id Expiration Date Standard Energy Actual Energy
 GD-148 6445-278 2/28/06 3183.000 3182.328
 NP-237 4341 2/28/06 4768.800 4768.118
 CM-244 4320A 2/28/06 5795.020 5795.011
 Energy/Channel Equation : see above
 Energy Calibration Zero : 2382.230
 Energy Calibration Slope : 4.964393
 Energy Calibration Quadratic : 2.9206229E-04
 Energy Calibration Range : 7772.000

Instrument : CHAMBER 011
 Detector : 9537
 Calibration Date/Time : 3-APR-2006 16:40:58
 Calibration Source Id : AESS-011
 Cal. Isotopes Source Id Expiration Date Standard Energy Actual Energy
 GD-148 6445-278 2/28/06 3183.000 3182.722
 NP-237 4341 2/28/06 4768.800 4768.758
 CM-244 4320A 2/28/06 5795.020 5794.941
 Energy/Channel Equation : see above
 Energy Calibration Zero : 2401.574
 Energy Calibration Slope : 4.894418
 Energy Calibration Quadratic : 3.3610439E-04
 Energy Calibration Range : 7766.000

Instrument : CHAMBER 012
 Detector : 33085
 Calibration Date/Time : 3-APR-2006 16:41:13
 Calibration Source Id : AESS-012
 Cal. Isotopes Source Id Expiration Date Standard Energy Actual Energy
 GD-148 6445-278 2/28/06 3183.000 3183.000
 NP-237 4341 2/28/06 4768.800 4768.403
 CM-244 4320A 2/28/06 5795.020 5794.958
 Energy/Channel Equation : see above
 Energy Calibration Zero : 2403.072
 Energy Calibration Slope : 4.959775
 Energy Calibration Quadratic : 2.8419620E-04
 Energy Calibration Range : 7780.000

Instrument : CHAMBER 013
 Detector : 21084
 Calibration Date/Time : 3-APR-2006 16:41:26
 Calibration Source Id : AESS-013
 Cal. Isotopes Source Id Expiration Date Standard Energy Actual Energy
 GD-148 6445-278 2/28/06 3183.000 3183.603
 NP-237 4341 2/28/06 4768.800 4769.678
 CM-244 4320A 2/28/06 5795.020 5795.297
 Energy/Channel Equation : see above
 Energy Calibration Zero : 2372.215
 Energy Calibration Slope : 4.879492
 Energy Calibration Quadratic : 3.3235765E-04
 Energy Calibration Range : 7717.000

Instrument : CHAMBER 016
 Detector : 21086
 Calibration Date/Time : 3-APR-2006 16:45:33
 Calibration Source Id : AESS-016
 Cal. Isotopes Source Id Expiration Date Standard Energy Actual Energy
 GD-148 6445-278 2/28/06 3183.000 3182.993
 NP-237 4341 2/28/06 4768.800 4768.792
 CM-244 4320A 2/28/06 5795.020 5794.887
 Energy/Channel Equation : see above
 Energy Calibration Zero : 2373.788
 Energy Calibration Slope : 4.866085
 Energy Calibration Quadratic : 3.4461656E-04
 Energy Calibration Range : 7718.000

Instrument : CHAMBER 017
 Detector : 33203
 Calibration Date/Time : 3-APR-2006 16:45:52
 Calibration Source Id : AESS-017
 Cal. Isotopes Source Id Expiration Date Standard Energy Actual Energy
 GD-148 6445-278 2/28/06 3183.000 3182.753
 NP-237 4341 2/28/06 4768.800 4768.686
 CM-244 4320A 2/28/06 5795.020 5795.002
 Energy/Channel Equation : see above
 Energy Calibration Zero : 2381.283
 Energy Calibration Slope : 4.983909
 Energy Calibration Quadratic : 2.9758285E-04
 Energy Calibration Range : 7797.000

Instrument : CHAMBER 018
 Detector : 21063
 Calibration Date/Time : 3-APR-2006 16:46:43
 Calibration Source Id : AESS-018
 Cal. Isotopes Source Id Expiration Date Standard Energy Actual Energy
 GD-148 6445-278 2/28/06 3183.000 3182.678
 NP-237 4341 2/28/06 4768.800 4768.731
 CM-244 4320A 2/28/06 5795.020 5795.019
 Energy/Channel Equation : see above
 Energy Calibration Zero : 2340.789
 Energy Calibration Slope : 4.900531
 Energy Calibration Quadratic : 3.0987556E-04
 Energy Calibration Range : 7684.000

Instrument : CHAMBER 019
 Detector : 23882
 Calibration Date/Time : 3-APR-2006 16:46:59
 Calibration Source Id : AESS-019
 Cal. Isotopes Source Id Expiration Date Standard Energy Actual Energy
 GD-148 6445-278 2/28/06 3183.000 3183.344
 NP-237 4341 2/28/06 4768.800 4769.286
 CM-244 4320A 2/28/06 5795.020 5795.346
 Energy/Channel Equation : see above
 Energy Calibration Zero : 2328.678
 Energy Calibration Slope : 5.011906
 Energy Calibration Quadratic : 2.4903595E-04
 Energy Calibration Range : 7722.000

Instrument : CHAMBER 020
 Detector : 33093
 Calibration Date/Time : 3-APR-2006 16:47:46
 Calibration Source Id : AESS-020
 Cal. Isotopes Source Id Expiration Date Standard Energy Actual Energy
 GD-148 6445-278 2/28/06 3183.000 3183.000
 NP-237 4341 2/28/06 4768.800 4768.523
 CM-244 4320A 2/28/06 5795.020 5795.020
 Energy/Channel Equation : see above
 Energy Calibration Zero : 2351.189
 Energy Calibration Slope : 4.985672
 Energy Calibration Quadratic : 2.7204608E-04
 Energy Calibration Range : 7742.000

Instrument : CHAMBER 021
 Detector : 33893
 Calibration Date/Time : 3-APR-2006 16:48:06
 Calibration Source Id : AESS-021

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3182.276
NP-237	4341	2/28/06	4768.800	4768.355
CM-244	4320A	2/28/06	5795.020	5794.907

Energy/Channel Equation : see above
 Energy Calibration Zero : 2374.427
 Energy Calibration Slope : 4.951159
 Energy Calibration Quadratic : 3.0070700E-04
 Energy Calibration Range : 7760.000

Instrument : CHAMBER 023
 Detector : 22873
 Calibration Date/Time : 3-APR-2006 16:49:38
 Calibration Source Id : AESS-023

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3180.453
NP-237	4341	2/28/06	4768.800	4764.511
CM-244	4320A	2/28/06	5795.020	5793.157

Energy/Channel Equation : see above
 Energy Calibration Zero : 2403.611
 Energy Calibration Slope : 4.972397
 Energy Calibration Quadratic : 2.1793865E-04
 Energy Calibration Range : 7724.000

Instrument : CHAMBER 026
 Detector : 34427
 Calibration Date/Time : 4-APR-2006 12:02:00
 Calibration Source Id : AESS-002

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3182.743
NP-237	4341	2/28/06	4768.800	4768.458
CM-244	4320A	2/28/06	5795.020	5794.860

Energy/Channel Equation : see above
 Energy Calibration Zero : 2367.357
 Energy Calibration Slope : 4.926605
 Energy Calibration Quadratic : 3.3364003E-04
 Energy Calibration Range : 7762.000

Instrument : CHAMBER 027
 Detector : 31436
 Calibration Date/Time : 4-APR-2006 12:02:17
 Calibration Source Id : AESS-003

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3183.368
NP-237	4341	2/28/06	4768.800	4769.435
CM-244	4320A	2/28/06	5795.020	5795.142

Energy/Channel Equation : see above
 Energy Calibration Zero : 2385.802
 Energy Calibration Slope : 4.966618
 Energy Calibration Quadratic : 2.6491811E-04
 Energy Calibration Range : 7749.000

Instrument : CHAMBER 028
 Detector : 21056
 Calibration Date/Time : 4-APR-2006 12:02:41
 Calibration Source Id : AESS-004

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3183.000
NP-237	4341	2/28/06	4768.800	4768.801
CM-244	4320A	2/28/06	5795.020	5795.020

Energy/Channel Equation : see above
 Energy Calibration Zero : 2320.544
 Energy Calibration Slope : 4.935237
 Energy Calibration Quadratic : 2.7769944E-04
 Energy Calibration Range : 7665.000

Instrument : CHAMBER 029
 Detector : 30419
 Calibration Date/Time : 4-APR-2006 12:02:56
 Calibration Source Id : AESS-005

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3183.690
NP-237	4341	2/28/06	4768.800	4770.051
CM-244	4320A	2/28/06	5795.020	5795.380

Energy/Channel Equation : see above
 Energy Calibration Zero : 2360.631
 Energy Calibration Slope : 4.932264
 Energy Calibration Quadratic : 2.8612607E-04
 Energy Calibration Range : 7711.000

Instrument : CHAMBER 030
 Detector : 30420
 Calibration Date/Time : 4-APR-2006 12:03:11
 Calibration Source Id : AESS-006

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3183.000
NP-237	4341	2/28/06	4768.800	4768.638
CM-244	4320A	2/28/06	5795.020	5794.905

Energy/Channel Equation : see above
 Energy Calibration Zero : 2379.492
 Energy Calibration Slope : 4.942307
 Energy Calibration Quadratic : 3.2948688E-04
 Energy Calibration Range : 7786.000

Instrument : CHAMBER 032
 Detector : 33207
 Calibration Date/Time : 4-APR-2006 12:04:09
 Calibration Source Id : AESS-008

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3183.162
NP-237	4341	2/28/06	4768.800	4769.075
CM-244	4320A	2/28/06	5795.020	5795.066

Energy/Channel Equation : see above
 Energy Calibration Zero : 2332.264
 Energy Calibration Slope : 4.962142
 Energy Calibration Quadratic : 2.9673061E-04
 Energy Calibration Range : 7725.000

Instrument : CHAMBER 033
 Detector : 28647
 Calibration Date/Time : 4-APR-2006 12:04:20
 Calibration Source Id : AESS-009

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3183.000
NP-237	4341	2/28/06	4768.800	4768.737
CM-244	4320A	2/28/06	5795.020	5794.927

Energy/Channel Equation : see above
 Energy Calibration Zero : 2371.926
 Energy Calibration Slope : 4.915609
 Energy Calibration Quadratic : 3.0408576E-04
 Energy Calibration Range : 7724.000

Instrument : CHAMBER 034
 Detector : 32697
 Calibration Date/Time : 4-APR-2006 12:04:32
 Calibration Source Id : AESS-010
 Cal. Isotopes Source Id Expiration Date Standard Energy Actual Energy
 GD-148 6445-278 2/28/06 3183.000 3182.670
 NP-237 4341 2/28/06 4768.800 4768.840
 CM-244 4320A 2/28/06 5795.020 5795.021

Energy/Channel Equation : see above
 Energy Calibration Zero : 2340.410
 Energy Calibration Slope : 4.974835
 Energy Calibration Quadratic : 3.3510773E-04
 Energy Calibration Range : 7786.000

Instrument : CHAMBER 035
 Detector : 29271
 Calibration Date/Time : 4-APR-2006 12:04:44
 Calibration Source Id : AESS-011
 Cal. Isotopes Source Id Expiration Date Standard Energy Actual Energy
 GD-148 6445-278 2/28/06 3183.000 3183.000
 NP-237 4341 2/28/06 4768.800 4768.800
 CM-244 4320A 2/28/06 5795.020 5795.020

Energy/Channel Equation : see above
 Energy Calibration Zero : 2347.646
 Energy Calibration Slope : 4.986292
 Energy Calibration Quadratic : 2.8726328E-04
 Energy Calibration Range : 7755.000

Instrument : CHAMBER 036
 Detector : 29275
 Calibration Date/Time : 4-APR-2006 12:04:58
 Calibration Source Id : AESS-012
 Cal. Isotopes Source Id Expiration Date Standard Energy Actual Energy
 GD-148 6445-278 2/28/06 3183.000 3181.797
 NP-237 4341 2/28/06 4768.800 4767.041
 CM-244 4320A 2/28/06 5795.020 5793.387

Energy/Channel Equation : see above
 Energy Calibration Zero : 2388.490
 Energy Calibration Slope : 5.017391
 Energy Calibration Quadratic : 3.2070087E-04
 Energy Calibration Range : 7863.000

Instrument : CHAMBER 037
 Detector : 32690
 Calibration Date/Time : 4-APR-2006 12:05:37
 Calibration Source Id : AESS-013

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3183.000
NP-237	4341	2/28/06	4768.800	4768.312
CM-244	4320A	2/28/06	5795.020	5794.990

Energy/Channel Equation : see above
 Energy Calibration Zero : 2422.263
 Energy Calibration Slope : 4.994318
 Energy Calibration Quadratic : 2.9049869E-04
 Energy Calibration Range : 7841.000

Instrument : CHAMBER 038
 Detector : 19323
 Calibration Date/Time : 4-APR-2006 12:05:48
 Calibration Source Id : AESS-014

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3183.338
NP-237	4341	2/28/06	4768.800	4769.033
CM-244	4320A	2/28/06	5795.020	5795.267

Energy/Channel Equation : see above
 Energy Calibration Zero : 2386.917
 Energy Calibration Slope : 4.961154
 Energy Calibration Quadratic : 3.4057652E-04
 Energy Calibration Range : 7824.000

Instrument : CHAMBER 040
 Detector : 30446
 Calibration Date/Time : 4-APR-2006 12:06:33
 Calibration Source Id : AESS-016

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3182.744
NP-237	4341	2/28/06	4768.800	4768.729
CM-244	4320A	2/28/06	5795.020	5794.990

Energy/Channel Equation : see above
 Energy Calibration Zero : 2361.522
 Energy Calibration Slope : 4.912026
 Energy Calibration Quadratic : 3.2777814E-04
 Energy Calibration Range : 7735.000

Instrument : CHAMBER 041
 Detector : 22834
 Calibration Date/Time : 4-APR-2006 12:06:46
 Calibration Source Id : AESS-017
 Cal. Isotopes Source Id Expiration Date Standard Energy Actual Energy
 GD-148 6445-278 2/28/06 3183.000 3183.000
 NP-237 4341 2/28/06 4768.800 4769.004
 CM-244 4320A 2/28/06 5795.020 5795.141
 Energy/Channel Equation : see above
 Energy Calibration Zero : 2357.184
 Energy Calibration Slope : 4.881192
 Energy Calibration Quadratic : 3.4815943E-04
 Energy Calibration Range : 7721.000

Instrument : CHAMBER 042
 Detector : 32695
 Calibration Date/Time : 4-APR-2006 12:07:02
 Calibration Source Id : AESS-018
 Cal. Isotopes Source Id Expiration Date Standard Energy Actual Energy
 GD-148 6445-278 2/28/06 3183.000 3183.000
 NP-237 4341 2/28/06 4768.800 4769.104
 CM-244 4320A 2/28/06 5795.020 5795.107
 Energy/Channel Equation : see above
 Energy Calibration Zero : 2418.706
 Energy Calibration Slope : 4.890110
 Energy Calibration Quadratic : 3.4867792E-04
 Energy Calibration Range : 7792.000

Instrument : CHAMBER 043
 Detector : 42470
 Calibration Date/Time : 4-APR-2006 12:07:20
 Calibration Source Id : AESS-019
 Cal. Isotopes Source Id Expiration Date Standard Energy Actual Energy
 GD-148 6445-278 2/28/06 3183.000 3183.000
 NP-237 4341 2/28/06 4768.800 4769.388
 CM-244 4320A 2/28/06 5795.020 5795.759
 Energy/Channel Equation : see above
 Energy Calibration Zero : 2363.161
 Energy Calibration Slope : 5.010756
 Energy Calibration Quadratic : 2.3886505E-04
 Energy Calibration Range : 7745.000

Instrument : CHAMBER 044
 Detector : 34433
 Calibration Date/Time : 4-APR-2006 12:07:31
 Calibration Source Id : AESS-020

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3183.000
NP-237	4341	2/28/06	4768.800	4768.800
CM-244	4320A	2/28/06	5795.020	5795.020

Energy/Channel Equation : see above
 Energy Calibration Zero : 2381.287
 Energy Calibration Slope : 4.986757
 Energy Calibration Quadratic : 2.9497029E-04
 Energy Calibration Range : 7797.000

Instrument : CHAMBER 045
 Detector : 34430
 Calibration Date/Time : 4-APR-2006 12:07:49
 Calibration Source Id : AESS-021

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3183.000
NP-237	4341	2/28/06	4768.800	4768.799
CM-244	4320A	2/28/06	5795.020	5795.021

Energy/Channel Equation : see above
 Energy Calibration Zero : 2396.370
 Energy Calibration Slope : 4.975925
 Energy Calibration Quadratic : 2.7766536E-04
 Energy Calibration Range : 7783.000

Instrument : CHAMBER 046
 Detector : 42471
 Calibration Date/Time : 4-APR-2006 12:08:03
 Calibration Source Id : AESS-022

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3181.981
NP-237	4341	2/28/06	4768.800	4768.475
CM-244	4320A	2/28/06	5795.020	5794.831

Energy/Channel Equation : see above
 Energy Calibration Zero : 2370.690
 Energy Calibration Slope : 4.938850
 Energy Calibration Quadratic : 3.0132200E-04
 Energy Calibration Range : 7744.000

Instrument : CHAMBER 047
 Detector : 30449
 Calibration Date/Time : 4-APR-2006 12:08:14
 Calibration Source Id : AESS-023

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3183.000
NP-237	4341	2/28/06	4768.800	4768.801
CM-244	4320A	2/28/06	5795.020	5795.020

Energy/Channel Equation : see above
 Energy Calibration Zero : 2367.885
 Energy Calibration Slope : 4.977801
 Energy Calibration Quadratic : 2.7243813E-04
 Energy Calibration Range : 7751.000

Instrument : CHAMBER 048
 Detector : 42483
 Calibration Date/Time : 4-APR-2006 12:08:24
 Calibration Source Id : AESS-024

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3183.000
NP-237	4341	2/28/06	4768.800	4768.800
CM-244	4320A	2/28/06	5795.020	5795.020

Energy/Channel Equation : see above
 Energy Calibration Zero : 2379.919
 Energy Calibration Slope : 5.011742
 Energy Calibration Quadratic : 2.4467456E-04
 Energy Calibration Range : 7769.000

Instrument : CHAMBER 065
 Detector : 21087
 Calibration Date/Time : 3-APR-2006 12:05:24
 Calibration Source Id : AESS-001

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3182.701
NP-237	4341	2/28/06	4768.800	4768.799
CM-244	4320A	2/28/06	5795.020	5795.020

Energy/Channel Equation : see above
 Energy Calibration Zero : 2381.709
 Energy Calibration Slope : 4.966328
 Energy Calibration Quadratic : 3.2913609E-04
 Energy Calibration Range : 7812.000

Instrument : CHAMBER 066
 Detector : 38159
 Calibration Date/Time : 3-APR-2006 12:05:41
 Calibration Source Id : AESS-002

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3183.194
NP-237	4341	2/28/06	4768.800	4769.460
CM-244	4320A	2/28/06	5795.020	5795.202

Energy/Channel Equation : see above
 Energy Calibration Zero : 2361.937
 Energy Calibration Slope : 4.956664
 Energy Calibration Quadratic : 3.0704346E-04
 Energy Calibration Range : 7760.000

Instrument : CHAMBER 068
 Detector : 33204
 Calibration Date/Time : 3-APR-2006 12:06:11
 Calibration Source Id : AESS-004

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3182.734
NP-237	4341	2/28/06	4768.800	4768.288
CM-244	4320A	2/28/06	5795.020	5794.885

Energy/Channel Equation : see above
 Energy Calibration Zero : 2340.602
 Energy Calibration Slope : 4.952214
 Energy Calibration Quadratic : 2.9989655E-04
 Energy Calibration Range : 7726.000

Instrument : CHAMBER 069
 Detector : 39172
 Calibration Date/Time : 3-APR-2006 12:06:22
 Calibration Source Id : AESS-005

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3182.678
NP-237	4341	2/28/06	4768.800	4768.439
CM-244	4320A	2/28/06	5795.020	5794.953

Energy/Channel Equation : see above
 Energy Calibration Zero : 2383.433
 Energy Calibration Slope : 4.992626
 Energy Calibration Quadratic : 3.0025930E-04
 Energy Calibration Range : 7811.000

Instrument : CHAMBER 070
 Detector : 33207
 Calibration Date/Time : 3-APR-2006 12:06:32
 Calibration Source Id : AESS-006
 Cal. Isotopes Source Id Expiration Date Standard Energy Actual Energy
 GD-148 6445-278 2/28/06 3183.000 3182.583
 NP-237 4341 2/28/06 4768.800 4768.687
 CM-244 4320A 2/28/06 5795.020 5794.788
 Energy/Channel Equation : see above
 Energy Calibration Zero : 2397.668
 Energy Calibration Slope : 4.915377
 Energy Calibration Quadratic : 3.6479929E-04
 Energy Calibration Range : 7814.000

Instrument : CHAMBER 072
 Detector : 33210
 Calibration Date/Time : 3-APR-2006 12:07:20
 Calibration Source Id : AESS-008
 Cal. Isotopes Source Id Expiration Date Standard Energy Actual Energy
 GD-148 6445-278 2/28/06 3183.000 3185.797
 NP-237 4341 2/28/06 4768.800 4771.520
 CM-244 4320A 2/28/06 5795.020 5795.709
 Energy/Channel Equation : see above
 Energy Calibration Zero : 2429.633
 Energy Calibration Slope : 4.970463
 Energy Calibration Quadratic : 2.6446831E-04
 Energy Calibration Range : 7797.000

Instrument : CHAMBER 073
 Detector : 33211
 Calibration Date/Time : 3-APR-2006 12:07:31
 Calibration Source Id : AESS-009
 Cal. Isotopes Source Id Expiration Date Standard Energy Actual Energy
 GD-148 6445-278 2/28/06 3183.000 3182.651
 NP-237 4341 2/28/06 4768.800 4768.479
 CM-244 4320A 2/28/06 5795.020 5794.623
 Energy/Channel Equation : see above
 Energy Calibration Zero : 2374.705
 Energy Calibration Slope : 4.961344
 Energy Calibration Quadratic : 3.4754534E-04
 Energy Calibration Range : 7820.000

Instrument : CHAMBER 075
 Detector : 29976
 Calibration Date/Time : 3-APR-2006 12:07:53
 Calibration Source Id : AESS-011

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3182.693
NP-237	4341	2/28/06	4768.800	4768.668
CM-244	4320A	2/28/06	5795.020	5794.923

Energy/Channel Equation : see above
 Energy Calibration Zero : 2362.553
 Energy Calibration Slope : 4.960943
 Energy Calibration Quadratic : 3.2853242E-04
 Energy Calibration Range : 7787.000

Instrument : CHAMBER 076
 Detector : 33213
 Calibration Date/Time : 3-APR-2006 12:08:02
 Calibration Source Id : AESS-012

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3182.644
NP-237	4341	2/28/06	4768.800	4768.760
CM-244	4320A	2/28/06	5795.020	5794.972

Energy/Channel Equation : see above
 Energy Calibration Zero : 2372.898
 Energy Calibration Slope : 4.983890
 Energy Calibration Quadratic : 3.3487112E-04
 Energy Calibration Range : 7828.000

Instrument : CHAMBER 077
 Detector : 28239
 Calibration Date/Time : 3-APR-2006 12:08:16
 Calibration Source Id : AESS-013

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3183.346
NP-237	4341	2/28/06	4768.800	4769.262
CM-244	4320A	2/28/06	5795.020	5795.317

Energy/Channel Equation : see above
 Energy Calibration Zero : 2368.874
 Energy Calibration Slope : 4.931313
 Energy Calibration Quadratic : 3.2203639E-04
 Energy Calibration Range : 7756.000

Instrument : CHAMBER 078
 Detector : 34425
 Calibration Date/Time : 3-APR-2006 12:08:26
 Calibration Source Id : AESS-014
 Cal. Isotopes Source Id Expiration Date Standard Energy Actual Energy
 GD-148 6445-278 2/28/06 3183.000 3182.993
 NP-237 4341 2/28/06 4768.800 4768.645
 CM-244 4320A 2/28/06 5795.020 5794.911
 Energy/Channel Equation : see above
 Energy Calibration Zero : 2393.754
 Energy Calibration Slope : 4.904502
 Energy Calibration Quadratic : 3.5731806E-04
 Energy Calibration Range : 7791.000

Instrument : CHAMBER 079
 Detector : 28408
 Calibration Date/Time : 3-APR-2006 12:08:37
 Calibration Source Id : AESS-015
 Cal. Isotopes Source Id Expiration Date Standard Energy Actual Energy
 GD-148 6445-278 2/28/06 3183.000 3182.266
 NP-237 4341 2/28/06 4768.800 4768.567
 CM-244 4320A 2/28/06 5795.020 5794.887
 Energy/Channel Equation : see above
 Energy Calibration Zero : 2383.558
 Energy Calibration Slope : 4.929332
 Energy Calibration Quadratic : 3.0991141E-04
 Energy Calibration Range : 7756.000

Instrument : CHAMBER 080
 Detector : 29269
 Calibration Date/Time : 3-APR-2006 12:08:46
 Calibration Source Id : AESS-016
 Cal. Isotopes Source Id Expiration Date Standard Energy Actual Energy
 GD-148 6445-278 2/28/06 3183.000 3182.363
 NP-237 4341 2/28/06 4768.800 4768.345
 CM-244 4320A 2/28/06 5795.020 5794.711
 Energy/Channel Equation : see above
 Energy Calibration Zero : 2360.141
 Energy Calibration Slope : 5.008783
 Energy Calibration Quadratic : 2.6339359E-04
 Energy Calibration Range : 7765.000

Instrument : CHAMBER 081
 Detector : 28243
 Calibration Date/Time : 5-APR-2006 14:20:00
 Calibration Source Id : AESS-017
 Cal. Isotopes Source Id Expiration Date Standard Energy Actual Energy
 GD-148 6445-278 2/28/06 3183.000 3183.000
 NP-237 4341 2/28/06 4768.800 4769.124
 CM-244 4320A 2/28/06 5795.020 5795.316
 Energy/Channel Equation : see above
 Energy Calibration Zero : 2423.205
 Energy Calibration Slope : 4.974538
 Energy Calibration Quadratic : 2.3569762E-04
 Energy Calibration Range : 7764.000

Instrument : CHAMBER 083
 Detector : 34436
 Calibration Date/Time : 3-APR-2006 12:09:35
 Calibration Source Id : AESS-019
 Cal. Isotopes Source Id Expiration Date Standard Energy Actual Energy
 GD-148 6445-278 2/28/06 3183.000 3183.000
 NP-237 4341 2/28/06 4768.800 4768.144
 CM-244 4320A 2/28/06 5795.020 5794.581
 Energy/Channel Equation : see above
 Energy Calibration Zero : 2370.701
 Energy Calibration Slope : 5.018431
 Energy Calibration Quadratic : 2.5893620E-04
 Energy Calibration Range : 7781.000

Instrument : CHAMBER 084
 Detector : 29953
 Calibration Date/Time : 3-APR-2006 12:09:48
 Calibration Source Id : AESS-020
 Cal. Isotopes Source Id Expiration Date Standard Energy Actual Energy
 GD-148 6445-278 2/28/06 3183.000 3182.067
 NP-237 4341 2/28/06 4768.800 4768.425
 CM-244 4320A 2/28/06 5795.020 5794.511
 Energy/Channel Equation : see above
 Energy Calibration Zero : 2368.562
 Energy Calibration Slope : 5.005028
 Energy Calibration Quadratic : 3.0593007E-04
 Energy Calibration Range : 7815.000

Instrument : CHAMBER 085
 Detector : 30451
 Calibration Date/Time : 3-APR-2006 12:10:02
 Calibration Source Id : AESS-021
 Cal. Isotopes Source Id Expiration Date Standard Energy Actual Energy
 GD-148 6445-278 2/28/06 3183.000 3182.503
 NP-237 4341 2/28/06 4768.800 4768.802
 CM-244 4320A 2/28/06 5795.020 5795.019
 Energy/Channel Equation : see above
 Energy Calibration Zero : 2385.228
 Energy Calibration Slope : 4.990182
 Energy Calibration Quadratic : 3.0125739E-04
 Energy Calibration Range : 7811.000

Instrument : CHAMBER 086
 Detector : 29278
 Calibration Date/Time : 3-APR-2006 12:10:24
 Calibration Source Id : AESS-022
 Cal. Isotopes Source Id Expiration Date Standard Energy Actual Energy
 GD-148 6445-278 2/28/06 3183.000 3183.000
 NP-237 4341 2/28/06 4768.800 4768.313
 CM-244 4320A 2/28/06 5795.020 5794.889
 Energy/Channel Equation : see above
 Energy Calibration Zero : 2367.011
 Energy Calibration Slope : 5.001186
 Energy Calibration Quadratic : 2.4593988E-04
 Energy Calibration Range : 7746.000

Instrument : CHAMBER 087
 Detector : 34430
 Calibration Date/Time : 3-APR-2006 12:10:36
 Calibration Source Id : AESS-023
 Cal. Isotopes Source Id Expiration Date Standard Energy Actual Energy
 GD-148 6445-278 2/28/06 3183.000 3182.326
 NP-237 4341 2/28/06 4768.800 4768.556
 CM-244 4320A 2/28/06 5795.020 5794.574
 Energy/Channel Equation : see above
 Energy Calibration Zero : 2363.815
 Energy Calibration Slope : 5.009631
 Energy Calibration Quadratic : 2.4977388E-04
 Energy Calibration Range : 7756.000

Instrument : CHAMBER 088
 Detector : 30434
 Calibration Date/Time : 3-APR-2006 12:10:54
 Calibration Source Id : AESS-024

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3182.313
NP-237	4341	2/28/06	4768.800	4767.746
CM-244	4320A	2/28/06	5795.020	5794.659

Energy/Channel Equation : see above
 Energy Calibration Zero : 2334.709
 Energy Calibration Slope : 4.874549
 Energy Calibration Quadratic : 2.1355411E-04
 Energy Calibration Range : 7550.000

Instrument : CHAMBER 089
 Detector : 21087
 Calibration Date/Time : 3-APR-2006 23:05:32
 Calibration Source Id : AESS-001

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3182.451
NP-237	4341	2/28/06	4768.800	4768.626
CM-244	4320A	2/28/06	5795.020	5794.917

Energy/Channel Equation : see above
 Energy Calibration Zero : 2349.260
 Energy Calibration Slope : 4.948930
 Energy Calibration Quadratic : 3.2322409E-04
 Energy Calibration Range : 7756.000

Instrument : CHAMBER 090
 Detector : 38159
 Calibration Date/Time : 3-APR-2006 23:06:16
 Calibration Source Id : AESS-002

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3183.000
NP-237	4341	2/28/06	4768.800	4768.800
CM-244	4320A	2/28/06	5795.020	5794.866

Energy/Channel Equation : see above
 Energy Calibration Zero : 2386.311
 Energy Calibration Slope : 4.986774
 Energy Calibration Quadratic : 3.3244080E-04
 Energy Calibration Range : 7841.000

Instrument : CHAMBER 091
 Detector : 33205
 Calibration Date/Time : 4-APR-2006 21:06:36
 Calibration Source Id : AESS-003

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3183.391
NP-237	4341	2/28/06	4768.800	4769.357
CM-244	4320A	2/28/06	5795.020	5795.305

Energy/Channel Equation : see above
 Energy Calibration Zero : 2363.386
 Energy Calibration Slope : 4.961743
 Energy Calibration Quadratic : 3.2066394E-04
 Energy Calibration Range : 7780.000

Instrument : CHAMBER 092
 Detector : 33204
 Calibration Date/Time : 3-APR-2006 23:08:02
 Calibration Source Id : AESS-004

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3183.000
NP-237	4341	2/28/06	4768.800	4768.867
CM-244	4320A	2/28/06	5795.020	5795.175

Energy/Channel Equation : see above
 Energy Calibration Zero : 2358.222
 Energy Calibration Slope : 4.950097
 Energy Calibration Quadratic : 3.0710385E-04
 Energy Calibration Range : 7749.000

Instrument : CHAMBER 093
 Detector : 33206
 Calibration Date/Time : 3-APR-2006 23:08:14
 Calibration Source Id : AESS-005

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3183.000
NP-237	4341	2/28/06	4768.800	4769.063
CM-244	4320A	2/28/06	5795.020	5795.298

Energy/Channel Equation : see above
 Energy Calibration Zero : 2375.739
 Energy Calibration Slope : 4.926612
 Energy Calibration Quadratic : 3.1170124E-04
 Energy Calibration Range : 7747.000

Instrument : CHAMBER 094
 Detector : 33207
 Calibration Date/Time : 3-APR-2006 23:08:34
 Calibration Source Id : AESS-006

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3182.993
NP-237	4341	2/28/06	4768.800	4768.799
CM-244	4320A	2/28/06	5795.020	5795.021

Energy/Channel Equation : see above
 Energy Calibration Zero : 2369.583
 Energy Calibration Slope : 4.936423
 Energy Calibration Quadratic : 3.2235958E-04
 Energy Calibration Range : 7762.000

Instrument : CHAMBER 096
 Detector : 30429
 Calibration Date/Time : 3-APR-2006 23:09:48
 Calibration Source Id : AESS-008

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3182.677
NP-237	4341	2/28/06	4768.800	4768.561
CM-244	4320A	2/28/06	5795.020	5794.869

Energy/Channel Equation : see above
 Energy Calibration Zero : 2346.092
 Energy Calibration Slope : 4.863141
 Energy Calibration Quadratic : 3.1486651E-04
 Energy Calibration Range : 7656.000

Instrument : CHAMBER 098
 Detector : 30431
 Calibration Date/Time : 3-APR-2006 23:10:26
 Calibration Source Id : AESS-010

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3182.647
NP-237	4341	2/28/06	4768.800	4768.514
CM-244	4320A	2/28/06	5795.020	5794.903

Energy/Channel Equation : see above
 Energy Calibration Zero : 2380.759
 Energy Calibration Slope : 4.922705
 Energy Calibration Quadratic : 3.2662629E-04
 Energy Calibration Range : 7764.000

Instrument : CHAMBER 099
 Detector : 30432
 Calibration Date/Time : 4-APR-2006 21:07:16
 Calibration Source Id : AESS-011

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3183.000
NP-237	4341	2/28/06	4768.800	4769.171
CM-244	4320A	2/28/06	5795.020	5795.241

Energy/Channel Equation : see above
 Energy Calibration Zero : 2411.170
 Energy Calibration Slope : 4.859684
 Energy Calibration Quadratic : 3.3678240E-04
 Energy Calibration Range : 7741.000

Instrument : CHAMBER 101
 Detector : 31696
 Calibration Date/Time : 3-APR-2006 23:11:17
 Calibration Source Id : AESS-013

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3181.759
NP-237	4341	2/28/06	4768.800	4767.478
CM-244	4320A	2/28/06	5795.020	5793.923

Energy/Channel Equation : see above
 Energy Calibration Zero : 2397.165
 Energy Calibration Slope : 4.939373
 Energy Calibration Quadratic : 2.7448736E-04
 Energy Calibration Range : 7743.000

Instrument : CHAMBER 102
 Detector : 30438
 Calibration Date/Time : 3-APR-2006 23:11:38
 Calibration Source Id : AESS-014

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3183.000
NP-237	4341	2/28/06	4768.800	4768.799
CM-244	4320A	2/28/06	5795.020	5795.021

Energy/Channel Equation : see above
 Energy Calibration Zero : 2390.065
 Energy Calibration Slope : 4.967123
 Energy Calibration Quadratic : 3.3759646E-04
 Energy Calibration Range : 7830.000

Instrument : CHAMBER 103
 Detector : 30437
 Calibration Date/Time : 3-APR-2006 23:11:50
 Calibration Source Id : AESS-015

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3182.632
NP-237	4341	2/28/06	4768.800	4768.780
CM-244	4320A	2/28/06	5795.020	5795.021

Energy/Channel Equation : see above
 Energy Calibration Zero : 2378.634
 Energy Calibration Slope : 4.949142
 Energy Calibration Quadratic : 3.4029011E-04
 Energy Calibration Range : 7803.000

Instrument : CHAMBER 104
 Detector : 30436
 Calibration Date/Time : 3-APR-2006 23:12:05
 Calibration Source Id : AESS-016

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3182.656
NP-237	4341	2/28/06	4768.800	4768.710
CM-244	4320A	2/28/06	5795.020	5794.893

Energy/Channel Equation : see above
 Energy Calibration Zero : 2402.033
 Energy Calibration Slope : 4.941638
 Energy Calibration Quadratic : 3.3733863E-04
 Energy Calibration Range : 7816.000

Instrument : CHAMBER 106
 Detector : 45382
 Calibration Date/Time : 3-APR-2006 23:13:35
 Calibration Source Id : AESS-018

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3183.390
NP-237	4341	2/28/06	4768.800	4768.938
CM-244	4320A	2/28/06	5795.020	5795.081

Energy/Channel Equation : see above
 Energy Calibration Zero : 2377.948
 Energy Calibration Slope : 4.942991
 Energy Calibration Quadratic : 3.4093895E-04
 Energy Calibration Range : 7797.000

Instrument : CHAMBER 107
 Detector : 31697
 Calibration Date/Time : 3-APR-2006 23:13:46
 Calibration Source Id : AESS-019

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3183.000
NP-237	4341	2/28/06	4768.800	4768.800
CM-244	4320A	2/28/06	5795.020	5795.020

Energy/Channel Equation : see above
 Energy Calibration Zero : 2398.373
 Energy Calibration Slope : 4.985534
 Energy Calibration Quadratic : 2.7872290E-04
 Energy Calibration Range : 7796.000

Instrument : CHAMBER 109
 Detector : 31693
 Calibration Date/Time : 3-APR-2006 23:14:12
 Calibration Source Id : AESS-021

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3183.000
NP-237	4341	2/28/06	4768.800	4769.000
CM-244	4320A	2/28/06	5795.020	5795.208

Energy/Channel Equation : see above
 Energy Calibration Zero : 2387.754
 Energy Calibration Slope : 4.924148
 Energy Calibration Quadratic : 3.0788378E-04
 Energy Calibration Range : 7753.000

Instrument : CHAMBER 110
 Detector : 30447
 Calibration Date/Time : 4-APR-2006 21:08:36
 Calibration Source Id : AESS-022

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3183.635
NP-237	4341	2/28/06	4768.800	4768.800
CM-244	4320A	2/28/06	5795.020	5795.020

Energy/Channel Equation : see above
 Energy Calibration Zero : 2419.221
 Energy Calibration Slope : 4.999035
 Energy Calibration Quadratic : 2.2320703E-04
 Energy Calibration Range : 7772.000

Instrument : CHAMBER 111
 Detector : 30448
 Calibration Date/Time : 3-APR-2006 23:15:36
 Calibration Source Id : AESS-023

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3182.627
NP-237	4341	2/28/06	4768.800	4768.799
CM-244	4320A	2/28/06	5795.020	5795.021

Energy/Channel Equation : see above
 Energy Calibration Zero : 2388.052
 Energy Calibration Slope : 4.962283
 Energy Calibration Quadratic : 2.9634466E-04
 Energy Calibration Range : 7780.000

Instrument : CHAMBER 112
 Detector : 30449
 Calibration Date/Time : 3-APR-2006 23:15:47
 Calibration Source Id : AESS-024

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3183.000
NP-237	4341	2/28/06	4768.800	4768.664
CM-244	4320A	2/28/06	5795.020	5795.019

Energy/Channel Equation : see above
 Energy Calibration Zero : 2375.519
 Energy Calibration Slope : 4.935473
 Energy Calibration Quadratic : 2.8306872E-04
 Energy Calibration Range : 7726.000

Instrument : CHAMBER 113
 Detector : 45-111B4
 Calibration Date/Time : 4-APR-2006 17:02:58
 Calibration Source Id : AESS-001

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3182.303
NP-237	4341	2/28/06	4768.800	4767.615
CM-244	4320A	2/28/06	5795.020	5794.404

Energy/Channel Equation : see above
 Energy Calibration Zero : 2393.614
 Energy Calibration Slope : 4.990646
 Energy Calibration Quadratic : 3.0610454E-04
 Energy Calibration Range : 7825.000

Instrument : CHAMBER 114
 Detector : 45-111B5
 Calibration Date/Time : 4-APR-2006 17:03:22
 Calibration Source Id : AESS-007

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3181.771
NP-237	4341	2/28/06	4768.800	4767.996
CM-244	4320A	2/28/06	5795.020	5794.695

Energy/Channel Equation : see above
 Energy Calibration Zero : 2391.292
 Energy Calibration Slope : 4.957956
 Energy Calibration Quadratic : 3.2139214E-04
 Energy Calibration Range : 7805.000

Instrument : CHAMBER 115
 Detector : 45-132EE5
 Calibration Date/Time : 4-APR-2006 17:03:37
 Calibration Source Id : AESS-002

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3183.000
NP-237	4341	2/28/06	4768.800	4768.468
CM-244	4320A	2/28/06	5795.020	5794.664

Energy/Channel Equation : see above
 Energy Calibration Zero : 2372.417
 Energy Calibration Slope : 4.988519
 Energy Calibration Quadratic : 2.9488039E-04
 Energy Calibration Range : 7790.000

Instrument : CHAMBER 116
 Detector : 45-132FF2
 Calibration Date/Time : 4-APR-2006 17:03:51
 Calibration Source Id : AESS-008

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3181.985
NP-237	4341	2/28/06	4768.800	4767.986
CM-244	4320A	2/28/06	5795.020	5794.612

Energy/Channel Equation : see above
 Energy Calibration Zero : 2377.594
 Energy Calibration Slope : 4.965635
 Energy Calibration Quadratic : 3.1974592E-04
 Energy Calibration Range : 7798.000

Instrument : CHAMBER 117
 Detector : 45-132FF3
 Calibration Date/Time : 4-APR-2006 17:04:04
 Calibration Source Id : AESS-003

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3181.825
NP-237	4341	2/28/06	4768.800	4767.294
CM-244	4320A	2/28/06	5795.020	5794.289

Energy/Channel Equation : see above
 Energy Calibration Zero : 2399.138
 Energy Calibration Slope : 4.995797
 Energy Calibration Quadratic : 2.8692893E-04
 Energy Calibration Range : 7816.000

Instrument : CHAMBER 118
 Detector : 45-132FF4
 Calibration Date/Time : 4-APR-2006 17:04:21
 Calibration Source Id : AESS-009

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3181.738
NP-237	4341	2/28/06	4768.800	4767.705
CM-244	4320A	2/28/06	5795.020	5794.733

Energy/Channel Equation : see above
 Energy Calibration Zero : 2382.726
 Energy Calibration Slope : 4.977871
 Energy Calibration Quadratic : 3.1087140E-04
 Energy Calibration Range : 7806.000

Instrument : CHAMBER 119
 Detector : 45-132FF5
 Calibration Date/Time : 4-APR-2006 17:04:33
 Calibration Source Id : AESS-004

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3181.725
NP-237	4341	2/28/06	4768.800	4768.406
CM-244	4320A	2/28/06	5795.020	5794.422

Energy/Channel Equation : see above
 Energy Calibration Zero : 2394.460
 Energy Calibration Slope : 4.945233
 Energy Calibration Quadratic : 3.2115451E-04
 Energy Calibration Range : 7795.000

Instrument : CHAMBER 120
 Detector : 45-142F1
 Calibration Date/Time : 4-APR-2006 17:05:08
 Calibration Source Id : AESS-010

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3181.702
NP-237	4341	2/28/06	4768.800	4767.716
CM-244	4320A	2/28/06	5795.020	5794.385

Energy/Channel Equation : see above
 Energy Calibration Zero : 2370.954
 Energy Calibration Slope : 4.969444
 Energy Calibration Quadratic : 2.9560321E-04
 Energy Calibration Range : 7770.000

Instrument : CHAMBER 121
 Detector : 45-142J4
 Calibration Date/Time : 4-APR-2006 17:05:19
 Calibration Source Id : AESS-005

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3181.854
NP-237	4341	2/28/06	4768.800	4767.926
CM-244	4320A	2/28/06	5795.020	5794.359

Energy/Channel Equation : see above
 Energy Calibration Zero : 2388.517
 Energy Calibration Slope : 4.957601
 Energy Calibration Quadratic : 3.2604721E-04
 Energy Calibration Range : 7807.000

Instrument : CHAMBER 122
 Detector : 45-142J5
 Calibration Date/Time : 4-APR-2006 17:05:33
 Calibration Source Id : AESS-011

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3181.708
NP-237	4341	2/28/06	4768.800	4767.643
CM-244	4320A	2/28/06	5795.020	5794.644

Energy/Channel Equation : see above
 Energy Calibration Zero : 2379.562
 Energy Calibration Slope : 4.966173
 Energy Calibration Quadratic : 3.1077259E-04
 Energy Calibration Range : 7791.000

Instrument : CHAMBER 123
 Detector : 45-142V1
 Calibration Date/Time : 4-APR-2006 17:05:57
 Calibration Source Id : AESS-006

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3180.927
NP-237	4341	2/28/06	4768.800	4767.132
CM-244	4320A	2/28/06	5795.020	5794.117

Energy/Channel Equation : see above
 Energy Calibration Zero : 2393.486
 Energy Calibration Slope : 4.981727
 Energy Calibration Quadratic : 2.8783656E-04
 Energy Calibration Range : 7797.000

Instrument : CHAMBER 124
 Detector : 45-142V2
 Calibration Date/Time : 4-APR-2006 17:06:12
 Calibration Source Id : AESS-012

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3181.329
NP-237	4341	2/28/06	4768.800	4767.124
CM-244	4320A	2/28/06	5795.020	5794.622

Energy/Channel Equation : see above
 Energy Calibration Zero : 2394.312
 Energy Calibration Slope : 4.963425
 Energy Calibration Quadratic : 3.1662040E-04
 Energy Calibration Range : 7809.000

Instrument : CHAMBER 125
 Detector : 45-142V3
 Calibration Date/Time : 4-APR-2006 17:06:28
 Calibration Source Id : AESS-013

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3181.749
NP-237	4341	2/28/06	4768.800	4766.709
CM-244	4320A	2/28/06	5795.020	5794.138

Energy/Channel Equation : see above
 Energy Calibration Zero : 2389.743
 Energy Calibration Slope : 4.991052
 Energy Calibration Quadratic : 2.6156937E-04
 Energy Calibration Range : 7775.000

Instrument : CHAMBER 126
 Detector : 45-142V5
 Calibration Date/Time : 4-APR-2006 17:06:44
 Calibration Source Id : AESS-019

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3181.536
NP-237	4341	2/28/06	4768.800	4766.676
CM-244	4320A	2/28/06	5795.020	5794.299

Energy/Channel Equation : see above
 Energy Calibration Zero : 2392.589
 Energy Calibration Slope : 5.019009
 Energy Calibration Quadratic : 2.5404955E-04
 Energy Calibration Range : 7798.000

Instrument : CHAMBER 127
 Detector : 45-142W1
 Calibration Date/Time : 4-APR-2006 17:07:12
 Calibration Source Id : AESS-014

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3181.047
NP-237	4341	2/28/06	4768.800	4767.379
CM-244	4320A	2/28/06	5795.020	5794.462

Energy/Channel Equation : see above
 Energy Calibration Zero : 2390.982
 Energy Calibration Slope : 4.949072
 Energy Calibration Quadratic : 3.2237647E-04
 Energy Calibration Range : 7797.000

Instrument : CHAMBER 128
 Detector : 45-142W2
 Calibration Date/Time : 4-APR-2006 17:07:27
 Calibration Source Id : AESS-020

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3181.794
NP-237	4341	2/28/06	4768.800	4767.351
CM-244	4320A	2/28/06	5795.020	5794.426

Energy/Channel Equation : see above
 Energy Calibration Zero : 2376.436
 Energy Calibration Slope : 4.990520
 Energy Calibration Quadratic : 2.8923506E-04
 Energy Calibration Range : 7790.000

Instrument : CHAMBER 129
 Detector : 45-142W3
 Calibration Date/Time : 4-APR-2006 17:07:43
 Calibration Source Id : AESS-015
 Cal. Isotopes Source Id Expiration Date Standard Energy Actual Energy
 GD-148 6445-278 2/28/06 3183.000 3181.920
 NP-237 4341 2/28/06 4768.800 4767.431
 CM-244 4320A 2/28/06 5795.020 5794.286

Energy/Channel Equation : see above
 Energy Calibration Zero : 2397.947
 Energy Calibration Slope : 4.950837
 Energy Calibration Quadratic : 3.2286491E-04
 Energy Calibration Range : 7806.000

Instrument : CHAMBER 130
 Detector : 45-142W5
 Calibration Date/Time : 4-APR-2006 17:07:58
 Calibration Source Id : AESS-021
 Cal. Isotopes Source Id Expiration Date Standard Energy Actual Energy
 GD-148 6445-278 2/28/06 3183.000 3181.779
 NP-237 4341 2/28/06 4768.800 4767.779
 CM-244 4320A 2/28/06 5795.020 5794.289

Energy/Channel Equation : see above
 Energy Calibration Zero : 2390.948
 Energy Calibration Slope : 5.005381
 Energy Calibration Quadratic : 2.9957382E-04
 Energy Calibration Range : 7831.000

Instrument : CHAMBER 131
 Detector : 45-145K1
 Calibration Date/Time : 4-APR-2006 17:08:16
 Calibration Source Id : AESS-016
 Cal. Isotopes Source Id Expiration Date Standard Energy Actual Energy
 GD-148 6445-278 2/28/06 3183.000 3181.832
 NP-237 4341 2/28/06 4768.800 4767.927
 CM-244 4320A 2/28/06 5795.020 5794.474

Energy/Channel Equation : see above
 Energy Calibration Zero : 2383.200
 Energy Calibration Slope : 4.971618
 Energy Calibration Quadratic : 3.1435001E-04
 Energy Calibration Range : 7804.000

Instrument : CHAMBER 132
 Detector : 45-145K2
 Calibration Date/Time : 4-APR-2006 17:08:32
 Calibration Source Id : AESS-022

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3181.897
NP-237	4341	2/28/06	4768.800	4767.248
CM-244	4320A	2/28/06	5795.020	5794.594

Energy/Channel Equation : see above
 Energy Calibration Zero : 2374.090
 Energy Calibration Slope : 5.015432
 Energy Calibration Quadratic : 2.7181130E-04
 Energy Calibration Range : 7795.000

Instrument : CHAMBER 133
 Detector : 45-145K3
 Calibration Date/Time : 4-APR-2006 17:09:47
 Calibration Source Id : AESS-017

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3181.967
NP-237	4341	2/28/06	4768.800	4767.767
CM-244	4320A	2/28/06	5795.020	5794.419

Energy/Channel Equation : see above
 Energy Calibration Zero : 2364.883
 Energy Calibration Slope : 4.958282
 Energy Calibration Quadratic : 2.8459914E-04
 Energy Calibration Range : 7741.000

Instrument : CHAMBER 134
 Detector : 45-145K4
 Calibration Date/Time : 4-APR-2006 17:11:02
 Calibration Source Id : AESS-023

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3181.715
NP-237	4341	2/28/06	4768.800	4767.525
CM-244	4320A	2/28/06	5795.020	5794.621

Energy/Channel Equation : see above
 Energy Calibration Zero : 2384.888
 Energy Calibration Slope : 4.989409
 Energy Calibration Quadratic : 2.7175582E-04
 Energy Calibration Range : 7779.000

Instrument : CHAMBER 135
 Detector : 45-145K5
 Calibration Date/Time : 4-APR-2006 17:11:53
 Calibration Source Id : AESS-018

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3181.833
NP-237	4341	2/28/06	4768.800	4768.171
CM-244	4320A	2/28/06	5795.020	5794.435

Energy/Channel Equation : see above
 Energy Calibration Zero : 2394.605
 Energy Calibration Slope : 4.968740
 Energy Calibration Quadratic : 2.9795556E-04
 Energy Calibration Range : 7795.000

Instrument : CHAMBER 136
 Detector : 45-145L1
 Calibration Date/Time : 4-APR-2006 17:12:12
 Calibration Source Id : AESS-024

Cal. Isotopes	Source Id	Expiration Date	Standard Energy	Actual Energy
GD-148	6445-278	2/28/06	3183.000	3181.493
NP-237	4341	2/28/06	4768.800	4767.151
CM-244	4320A	2/28/06	5795.020	5794.044

Energy/Channel Equation : see above
 Energy Calibration Zero : 2384.309
 Energy Calibration Slope : 5.003936
 Energy Calibration Quadratic : 2.5798104E-04
 Energy Calibration Range : 7779.000

Subsection 2: Background Calibration

Instrument : CHAMBER 001
 Detector : 33088
 Background Analysis Date/Time : 2-APR-2006 11:38:32
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2990.456	3298.943	2.000000	0.4799997	70.71068	95.00000
NP-237	4433.436	4903.018	13.00000	3.119998	27.73501	95.00000
CM-244	5530.638	5887.374	28.00000	6.719995	18.89822	95.00000

Instrument : CHAMBER 003
 Detector : 20659
 Background Analysis Date/Time : 2-APR-2006 11:38:32
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2988.599	3300.169	5.000000	1.199999	44.72136	95.00000
NP-237	4434.674	4902.844	22.00000	5.279996	21.32007	95.00000
CM-244	5535.248	5883.783	33.00000	7.919994	17.40777	95.00000

Instrument : CHAMBER 004
 Detector : 33077
 Background Analysis Date/Time : 2-APR-2006 11:38:32
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2987.545	3299.456	0.000000E+00	0.000000E+00	0.000000E+00	95.00000
NP-237	4433.646	4906.400	4.000000	0.9599993	50.00000	95.00000
CM-244	5531.494	5886.867	18.00000	4.319997	23.57022	95.00000

Instrument : CHAMBER 005
 Detector : 28642
 Background Analysis Date/Time : 2-APR-2006 11:38:32
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2990.709	3298.775	3.000000	0.7199995	57.73503	95.00000
NP-237	4434.190	4905.248	19.00000	4.559997	22.94157	95.00000
CM-244	5530.463	5883.921	31.00000	7.439995	17.96053	95.00000

Instrument : CHAMBER 007
 Detector : 30416
 Background Analysis Date/Time : 2-APR-2006 11:38:33
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2990.797	3298.358	1.000000	0.2399998	100.0000	95.00000
NP-237	4432.556	4903.394	25.00000	5.999996	20.00000	95.00000
CM-244	5533.897	5887.491	49.00000	11.75999	14.28572	95.00000

Instrument : CHAMBER 009
 Detector : 13285
 Background Analysis Date/Time : 2-APR-2006 11:38:33
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2987.740	3302.180	3.000000	0.7199995	57.73503	95.00000
NP-237	4436.826	4904.306	10.00000	2.399998	31.62278	95.00000
CM-244	5530.853	5882.488	30.00000	7.199995	18.25742	95.00000

Instrument : CHAMBER 010
 Detector : 33083
 Background Analysis Date/Time : 2-APR-2006 11:38:33
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2992.233	3300.495	1.000000	0.2399998	100.0000	95.00000
NP-237	4435.514	4905.914	11.00000	2.639998	30.15113	95.00000
CM-244	5535.151	5882.345	27.00000	6.479995	19.24501	95.00000

Instrument : CHAMBER 011
 Detector : 9537
 Background Analysis Date/Time : 2-APR-2006 11:38:33
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2988.769	3298.475	1.000000	0.2399998	100.0000	95.00000
NP-237	4433.776	4901.438	2.000000	0.4799997	70.71068	95.00000
CM-244	5533.457	5885.193	35.00000	8.399994	16.90309	95.00000

Instrument : CHAMBER 012
 Detector : 33085
 Background Analysis Date/Time : 2-APR-2006 11:38:33
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2992.283	3299.978	1.000000	0.2399998	100.0000	95.00000
NP-237	4432.454	4901.598	3.000000	0.7199995	57.73503	95.00000
CM-244	5534.285	5885.751	13.00000	3.119998	27.73501	95.00000

Instrument : CHAMBER 013
 Detector : 21084
 Background Analysis Date/Time : 2-APR-2006 11:38:34
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2992.308	3301.307	1.000000	0.2399998	100.0000	95.00000
NP-237	4433.829	4905.476	4.000000	0.9599993	50.00000	95.00000
CM-244	5530.551	5886.625	27.00000	6.479995	19.24501	95.00000

Instrument : CHAMBER 016
 Detector : 21086
 Background Analysis Date/Time : 2-APR-2006 11:38:34
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2992.386	3300.792	3.000000	0.7199995	57.73503	95.00000
NP-237	4437.111	4903.407	9.000000	2.159998	33.33334	95.00000
CM-244	5533.819	5884.776	38.00000	9.119993	16.22214	95.00000

Instrument : CHAMBER 017
 Detector : 33203
 Background Analysis Date/Time : 2-APR-2006 11:38:34
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2988.693	3298.212	1.000000	0.2399998	100.0000	95.00000
NP-237	4432.905	4905.400	9.000000	2.159998	33.33334	95.00000
CM-244	5532.198	5886.394	44.00000	10.55999	15.07557	95.00000

Instrument : CHAMBER 018
 Detector : 21063
 Background Analysis Date/Time : 2-APR-2006 11:38:34
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2988.076	3298.134	1.000000	0.2399998	100.0000	95.00000
NP-237	4433.036	4905.011	4.000000	0.9599993	50.00000	95.00000
CM-244	5535.243	5885.674	34.00000	8.159994	17.14986	95.00000

Instrument : CHAMBER 019
 Detector : 23882
 Background Analysis Date/Time : 2-APR-2006 11:38:35
 Background Count Time : 59999.99

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2989.511	3300.144	16916.00	4059.841	0.7688669	95.00000
NP-237	4435.855	4902.151	5184.000	1244.160	1.388889	95.00000
CM-244	5531.789	5884.041	1897.000	455.2801	2.295970	95.00000

Instrument : CHAMBER 020
 Detector : 33093
 Background Analysis Date/Time : 2-APR-2006 11:38:35
 Background Count Time : 59999.99

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2988.758	3298.111	2.000000	0.4800001	70.71068	95.00000
NP-237	4435.838	4901.523	7.000000	1.680000	37.79645	95.00000
CM-244	5530.915	5883.311	45.00000	10.80000	14.90712	95.00000

Instrument : CHAMBER 021
 Detector : 33893
 Background Analysis Date/Time : 2-APR-2006 11:38:35
 Background Count Time : 59999.99

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2987.969	3300.683	1.000000	0.2400001	100.0000	95.00000
NP-237	4434.165	4904.181	5.000000	1.200000	44.72136	95.00000
CM-244	5533.125	5885.623	21.00000	5.040001	21.82179	95.00000

Instrument : CHAMBER 023
 Detector : 22873
 Background Analysis Date/Time : 2-APR-2006 11:38:35
 Background Count Time : 59999.99

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2988.365	3300.653	2.000000	0.4800001	70.71068	95.00000
NP-237	4432.587	4902.786	9.000000	2.160001	33.33334	95.00000
CM-244	5533.585	5885.616	41.00000	9.840002	15.61738	95.00000

Instrument : CHAMBER 026
 Detector : 34427
 Background Analysis Date/Time : 2-APR-2006 11:38:36
 Background Count Time : 59999.99

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2988.396	3300.299	1.000000	0.2400001	100.0000	95.00000
NP-237	4432.951	4903.551	14.00000	3.360001	26.72612	95.00000
CM-244	5534.085	5882.486	27.00000	6.480001	19.24501	95.00000

Instrument : CHAMBER 027
 Detector : 31436
 Background Analysis Date/Time : 2-APR-2006 11:38:36
 Background Count Time : 59999.99

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2990.641	3298.501	0.0000000E+00	0.0000000E+00	0.0000000E+00	95.00000
NP-237	4435.554	4903.960	9.000000	2.160001	33.33334	95.00000
CM-244	5535.178	5885.600	13.00000	3.120001	27.73501	95.00000

Instrument : CHAMBER 028
 Detector : 21056
 Background Analysis Date/Time : 2-APR-2006 11:38:36
 Background Count Time : 59999.99

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2991.862	3298.519	1.000000	0.2400001	100.0000	95.00000
NP-237	4437.162	4904.527	5.000000	1.200000	44.72136	95.00000
CM-244	5534.678	5884.670	3.000000	0.7200001	57.73503	95.00000

Instrument : CHAMBER 029
 Detector : 30419
 Background Analysis Date/Time : 2-APR-2006 11:38:36
 Background Count Time : 59999.99

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2991.643	3298.009	4.000000	0.9600002	50.00000	95.00000
NP-237	4436.124	4903.513	4.000000	0.9600002	50.00000	95.00000
CM-244	5533.909	5884.139	20.00000	4.800001	22.36068	95.00000

Instrument : CHAMBER 030
 Detector : 30420
 Background Analysis Date/Time : 2-APR-2006 11:38:36
 Background Count Time : 59999.99

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2992.381	3300.032	2.000000	0.4800001	70.71068	95.00000
NP-237	4435.171	4901.399	1.000000	0.2400001	100.0000	95.00000
CM-244	5532.938	5887.226	28.00000	6.720002	18.89822	95.00000

Instrument : CHAMBER 032
 Detector : 33207
 Background Analysis Date/Time : 2-APR-2006 11:38:36
 Background Count Time : 59999.99

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2992.438	3301.011	4.000000	0.9599994	50.00000	95.00000
NP-237	4437.450	4903.298	8.000000	1.919999	35.35534	95.00000
CM-244	5533.518	5886.674	40.00000	9.599994	15.81139	95.00000

Instrument : CHAMBER 033
 Detector : 28647
 Background Analysis Date/Time : 2-APR-2006 11:38:36
 Background Count Time : 59999.99

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2991.128	3301.778	10.00000	2.399998	31.62278	95.00000
NP-237	4433.277	4905.752	9.000000	2.159999	33.33334	95.00000
CM-244	5531.202	5887.135	39.00000	9.359994	16.01282	95.00000

Instrument : CHAMBER 034
 Detector : 32697
 Background Analysis Date/Time : 2-APR-2006 11:38:36
 Background Count Time : 59999.99

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2987.740	3297.727	18.00000	4.319997	23.57022	95.00000
NP-237	4436.424	4906.295	31.00000	7.439995	17.96053	95.00000
CM-244	5532.067	5883.683	33.00000	7.919995	17.40777	95.00000

Instrument : CHAMBER 035
 Detector : 29271
 Background Analysis Date/Time : 2-APR-2006 11:38:36
 Background Count Time : 59999.99

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2990.597	3300.316	1.000000	0.2399998	100.0000	95.00000
NP-237	4435.093	4902.062	25.00000	5.999996	20.00000	95.00000
CM-244	5533.546	5887.289	24.00000	5.759996	20.41241	95.00000

Instrument : CHAMBER 036
 Detector : 29275
 Background Analysis Date/Time : 2-APR-2006 11:38:36
 Background Count Time : 59999.99

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2990.101	3302.011	0.0000000E+00	0.0000000E+00	0.0000000E+00	95.00000
NP-237	4436.212	4902.690	21.00000	5.039997	21.82179	95.00000
CM-244	5530.586	5883.211	28.00000	6.719995	18.89822	95.00000

Instrument : CHAMBER 037
 Detector : 32690
 Background Analysis Date/Time : 2-APR-2006 11:38:37
 Background Count Time : 59999.99

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2990.331	3300.070	3.000000	0.7200001	57.73503	95.00000
NP-237	4435.120	4902.289	15.00000	3.600001	25.81989	95.00000
CM-244	5534.121	5882.713	34.00000	8.160002	17.14986	95.00000

Instrument : CHAMBER 038
 Detector : 19323
 Background Analysis Date/Time : 2-APR-2006 11:38:37
 Background Count Time : 59999.99

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2992.203	3301.129	4.000000	0.9600002	50.00000	95.00000
NP-237	4436.340	4904.950	11.00000	2.640001	30.15113	95.00000
CM-244	5534.574	5885.451	22.00000	5.280001	21.32007	95.00000

Instrument : CHAMBER 040
 Detector : 30446
 Background Analysis Date/Time : 2-APR-2006 11:38:37
 Background Count Time : 59999.99

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2990.636	3301.603	3.000000	0.7200001	57.73503	95.00000
NP-237	4435.733	4904.719	11.00000	2.640001	30.15113	95.00000
CM-244	5532.976	5885.423	19.00000	4.560001	22.94157	95.00000

Instrument : CHAMBER 041
 Detector : 22834
 Background Analysis Date/Time : 2-APR-2006 11:38:37
 Background Count Time : 59999.99

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2987.681	3302.193	2.000000	0.4800001	70.71068	95.00000
NP-237	4432.502	4905.743	8.000000	1.920000	35.35534	95.00000
CM-244	5533.298	5885.604	23.00000	5.520001	20.85144	95.00000

Instrument : CHAMBER 042
 Detector : 32695
 Background Analysis Date/Time : 2-APR-2006 11:38:37
 Background Count Time : 59999.99

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2990.651	3300.194	4.000000	0.9600002	50.00000	95.00000
NP-237	4435.708	4903.810	19.00000	4.560001	22.94157	95.00000
CM-244	5531.417	5883.758	26.00000	6.240001	19.61161	95.00000

Instrument : CHAMBER 043
 Detector : 42470
 Background Analysis Date/Time : 2-APR-2006 11:38:38
 Background Count Time : 59999.99

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2988.168	3298.326	1.000000	0.2399998	100.0000	95.00000
NP-237	4436.901	4902.013	2.000000	0.4799997	70.71068	95.00000
CM-244	5535.121	5886.262	19.00000	4.559997	22.94157	95.00000

Instrument : CHAMBER 044
 Detector : 34433
 Background Analysis Date/Time : 2-APR-2006 11:38:38
 Background Count Time : 59999.99

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2989.004	3298.648	28.00000	6.719995	18.89822	95.00000
NP-237	4433.632	4906.174	35.00000	8.399995	16.90309	95.00000
CM-244	5532.967	5887.129	38.00000	9.119994	16.22214	95.00000

Instrument : CHAMBER 045
 Detector : 34430
 Background Analysis Date/Time : 2-APR-2006 11:38:38
 Background Count Time : 59999.99

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2992.438	3301.033	4.000000	0.9599994	50.00000	95.00000
NP-237	4436.365	4906.490	17.00000	4.079998	24.25356	95.00000
CM-244	5535.004	5886.982	17.00000	4.079998	24.25356	95.00000

Instrument : CHAMBER 046
 Detector : 42471
 Background Analysis Date/Time : 2-APR-2006 11:38:38
 Background Count Time : 59999.99

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2987.741	3299.741	14.00000	3.359998	26.72612	95.00000
NP-237	4435.900	4904.967	49.00000	11.75999	14.28572	95.00000
CM-244	5532.671	5884.488	25.00000	5.999996	20.00000	95.00000

Instrument : CHAMBER 047
 Detector : 30449
 Background Analysis Date/Time : 2-APR-2006 11:38:38
 Background Count Time : 59999.99

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2989.322	3298.103	0.000000E+00	0.000000E+00	0.000000E+00	95.00000
NP-237	4433.780	4903.899	14.00000	3.359998	26.72612	95.00000
CM-244	5532.276	5884.114	29.00000	6.959996	18.56953	95.00000

Instrument : CHAMBER 048
 Detector : 42483
 Background Analysis Date/Time : 2-APR-2006 11:38:38
 Background Count Time : 59999.99

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2989.922	3300.161	1.000000	0.2399998	100.0000	95.00000
NP-237	4434.180	4904.923	20.00000	4.799997	22.36068	95.00000
CM-244	5533.436	5885.010	24.00000	5.759996	20.41241	95.00000

Instrument : CHAMBER 065
 Detector : 21087
 Background Analysis Date/Time : 2-APR-2006 11:38:39
 Background Count Time : 59999.99

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2992.500	3301.569	5.000000	1.199999	44.72136	95.00000
NP-237	4436.593	4904.814	10.00000	2.399998	31.62278	95.00000
CM-244	5533.641	5883.942	18.00000	4.319997	23.57022	95.00000

Instrument : CHAMBER 066
 Detector : 38159
 Background Analysis Date/Time : 2-APR-2006 11:38:39
 Background Count Time : 59999.99

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2991.351	3299.570	1.000000	0.2399998	100.0000	95.00000
NP-237	4435.367	4906.503	12.00000	2.879998	28.86751	95.00000
CM-244	5531.751	5885.195	19.00000	4.559997	22.94157	95.00000

Instrument : CHAMBER 068
 Detector : 33204
 Background Analysis Date/Time : 2-APR-2006 11:38:39
 Background Count Time : 59999.99

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2989.458	3302.482	2.000000	0.4799997	70.71068	95.00000
NP-237	4437.019	4902.188	5.000000	1.199999	44.72136	95.00000
CM-244	5531.579	5884.315	15.00000	3.599998	25.81989	95.00000

Instrument : CHAMBER 069
 Detector : 39172
 Background Analysis Date/Time : 2-APR-2006 11:38:39
 Background Count Time : 59999.99

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2991.937	3302.037	1.000000	0.2399998	100.0000	95.00000
NP-237	4433.758	4901.912	5.000000	1.199999	44.72136	95.00000
CM-244	5535.302	5884.863	13.00000	3.119998	27.73501	95.00000

Instrument : CHAMBER 070
 Detector : 33207
 Background Analysis Date/Time : 2-APR-2006 11:38:39
 Background Count Time : 59999.99

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2987.764	3299.302	3.000000	0.7199996	57.73503	95.00000
NP-237	4432.603	4904.338	13.00000	3.119998	27.73501	95.00000
CM-244	5531.790	5887.167	12.00000	2.879998	28.86751	95.00000

Instrument : CHAMBER 072
 Detector : 33210
 Background Analysis Date/Time : 2-APR-2006 11:38:40
 Background Count Time : 59999.99

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2989.642	3302.500	4.000000	0.9599994	50.00000	95.00000
NP-237	4434.229	4902.517	7.000000	1.679999	37.79645	95.00000
CM-244	5533.565	5883.889	14.00000	3.359998	26.72612	95.00000

Instrument : CHAMBER 073
 Detector : 33211
 Background Analysis Date/Time : 2-APR-2006 11:38:40
 Background Count Time : 59999.99

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2990.209	3299.359	1.000000	0.2399998	100.0000	95.00000
NP-237	4435.813	4905.119	6.000000	1.439999	40.82483	95.00000
CM-244	5530.447	5887.394	15.00000	3.599998	25.81989	95.00000

Instrument : CHAMBER 075
 Detector : 29976
 Background Analysis Date/Time : 2-APR-2006 11:38:40
 Background Count Time : 59999.99

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2987.804	3301.738	1.000000	0.2399998	100.0000	95.00000
NP-237	4436.078	4904.005	18.00000	4.319997	23.57022	95.00000
CM-244	5532.428	5882.500	16.00000	3.839998	25.00000	95.00000

Instrument : CHAMBER 076
 Detector : 33213
 Background Analysis Date/Time : 2-APR-2006 11:38:40
 Background Count Time : 59999.99

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2990.982	3301.271	1.000000	0.2399998	100.0000	95.00000
NP-237	4435.792	4906.032	9.000000	2.159999	33.33334	95.00000
CM-244	5532.284	5884.164	16.00000	3.839998	25.00000	95.00000

Instrument : CHAMBER 077
 Detector : 28239
 Background Analysis Date/Time : 2-APR-2006 11:38:41
 Background Count Time : 59999.99

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2990.320	3302.291	3.000000	0.7200001	57.73503	95.00000
NP-237	4434.458	4904.534	18.00000	4.320001	23.57022	95.00000
CM-244	5534.090	5887.188	14.00000	3.360001	26.72612	95.00000

Instrument : CHAMBER 078
 Detector : 34425
 Background Analysis Date/Time : 2-APR-2006 11:38:41
 Background Count Time : 59999.99

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2992.430	3298.209	2.000000	0.4800001	70.71068	95.00000
NP-237	4433.493	4903.776	8.000000	1.920000	35.35534	95.00000
CM-244	5534.483	5883.260	14.00000	3.360001	26.72612	95.00000

Instrument : CHAMBER 079
 Detector : 28408
 Background Analysis Date/Time : 2-APR-2006 11:38:41
 Background Count Time : 59999.99

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2989.549	3301.048	4.000000	0.9600002	50.00000	95.00000
NP-237	4435.951	4904.750	7.000000	1.680000	37.79645	95.00000
CM-244	5532.313	5884.158	23.00000	5.520001	20.85144	95.00000

Instrument : CHAMBER 080
 Detector : 29269
 Background Analysis Date/Time : 2-APR-2006 11:38:41
 Background Count Time : 59999.99

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2990.355	3300.887	0.0000000E+00	0.0000000E+00	0.0000000E+00	95.00000
NP-237	4437.124	4904.027	11.00000	2.640001	30.15113	95.00000
CM-244	5534.833	5882.541	24.00000	5.760001	20.41241	95.00000

Instrument : CHAMBER 081
 Detector : 28243
 Background Analysis Date/Time : 2-APR-2006 11:38:41
 Background Count Time : 59999.99

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2988.337	3300.967	0.0000000E+00	0.0000000E+00	0.0000000E+00	95.00000
NP-237	4435.244	4901.705	5.000000	1.199999	44.72136	95.00000
CM-244	5534.853	5883.115	9.000000	2.159999	33.33334	95.00000

Instrument : CHAMBER 083
 Detector : 34436
 Background Analysis Date/Time : 2-APR-2006 11:38:42
 Background Count Time : 59999.99

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2991.885	3297.745	2.000000	0.4799997	70.71068	95.00000
NP-237	4435.182	4902.448	13.00000	3.119998	27.73501	95.00000
CM-244	5533.629	5886.856	19.00000	4.559997	22.94157	95.00000

Instrument : CHAMBER 084
 Detector : 29953
 Background Analysis Date/Time : 2-APR-2006 11:38:42
 Background Count Time : 59999.99

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2988.809	3299.845	2.000000	0.4799997	70.71068	95.00000
NP-237	4435.274	4905.090	36.00000	8.639995	16.66667	95.00000
CM-244	5535.465	5886.345	11.00000	2.639998	30.15113	95.00000

Instrument : CHAMBER 085
 Detector : 30451
 Background Analysis Date/Time : 2-APR-2006 11:38:42
 Background Count Time : 59999.99

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2988.388	3298.321	0.000000E+00	0.000000E+00	0.000000E+00	95.00000
NP-237	4434.734	4902.750	2.000000	0.4799997	70.71068	95.00000
CM-244	5530.623	5885.465	16.00000	3.839998	25.00000	95.00000

Instrument : CHAMBER 086
 Detector : 29278
 Background Analysis Date/Time : 2-APR-2006 11:38:42
 Background Count Time : 59999.99

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2990.939	3300.647	0.000000E+00	0.000000E+00	0.000000E+00	95.00000
NP-237	4432.832	4902.859	8.000000	1.919999	35.35534	95.00000
CM-244	5530.458	5886.876	7.000000	1.679999	37.79645	95.00000

Instrument : CHAMBER 087
 Detector : 34430
 Background Analysis Date/Time : 2-APR-2006 11:38:42
 Background Count Time : 59999.99

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2988.850	3299.145	8.000000	1.919999	35.35534	95.00000
NP-237	4433.685	4904.783	101.0000	24.23998	9.950372	95.00000
CM-244	5533.892	5885.860	3.000000	0.7199996	57.73503	95.00000

Instrument : CHAMBER 088
 Detector : 30434
 Background Analysis Date/Time : 2-APR-2006 11:38:42
 Background Count Time : 59999.99

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2991.733	3298.324	1.000000	0.2399998	100.0000	95.00000
NP-237	4434.854	4901.741	3.000000	0.7199996	57.73503	95.00000
CM-244	5531.597	5882.583	6.000000	1.439999	40.82483	95.00000

Instrument : CHAMBER 089
 Detector : 21087
 Background Analysis Date/Time : 2-APR-2006 11:38:43
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2988.018	3301.225	0.000000E+00	0.000000E+00	0.000000E+00	95.00000
NP-237	4432.655	4904.531	3.000000	0.7199995	57.73503	95.00000
CM-244	5531.146	5885.550	1.000000	0.2399998	100.0000	95.00000

Instrument : CHAMBER 090
 Detector : 38159
 Background Analysis Date/Time : 2-APR-2006 11:38:43
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2989.511	3299.809	0.000000E+00	0.000000E+00	0.000000E+00	95.00000
NP-237	4434.211	4904.337	4.000000	0.9599993	50.00000	95.00000
CM-244	5530.381	5887.548	0.000000E+00	0.000000E+00	0.000000E+00	95.00000

Instrument : CHAMBER 091
 Detector : 33205
 Background Analysis Date/Time : 2-APR-2006 11:38:43
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2988.614	3302.446	1.000000	0.2399998	100.0000	95.00000
NP-237	4435.933	4903.299	6.000000	1.439999	40.82483	95.00000
CM-244	5530.786	5885.646	0.0000000E+00	0.0000000E+00	0.0000000E+00	95.00000

Instrument : CHAMBER 092
 Detector : 33204
 Background Analysis Date/Time : 2-APR-2006 11:38:43
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2991.837	3299.694	0.0000000E+00	0.0000000E+00	0.0000000E+00	95.00000
NP-237	4434.184	4904.789	3.000000	0.7199995	57.73503	95.00000
CM-244	5534.672	5882.398	1.000000	0.2399998	100.0000	95.00000

Instrument : CHAMBER 093
 Detector : 33206
 Background Analysis Date/Time : 2-APR-2006 11:38:43
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2991.432	3297.831	1.000000	0.2399998	100.0000	95.00000
NP-237	4432.503	4906.496	4.000000	0.9599993	50.00000	95.00000
CM-244	5534.120	5886.021	0.0000000E+00	0.0000000E+00	0.0000000E+00	95.00000

Instrument : CHAMBER 094
 Detector : 33207
 Background Analysis Date/Time : 2-APR-2006 11:38:43
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2991.673	3298.910	1.000000	0.2399998	100.0000	95.00000
NP-237	4437.305	4902.611	3.000000	0.7199995	57.73503	95.00000
CM-244	5532.741	5886.161	1.000000	0.2399998	100.0000	95.00000

Instrument : CHAMBER 096
 Detector : 30429
 Background Analysis Date/Time : 2-APR-2006 11:38:44
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2988.567	3301.392	2.000000	0.4800001	70.71068	95.00000
NP-237	4433.899	4903.007	4.000000	0.9600002	50.00000	95.00000
CM-244	5534.841	5883.364	8.000000	1.920000	35.35534	95.00000

Instrument : CHAMBER 098
 Detector : 30431
 Background Analysis Date/Time : 2-APR-2006 11:38:44
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2991.193	3297.595	2.000000	0.4800001	70.71068	95.00000
NP-237	4433.217	4902.776	10.00000	2.400000	31.62278	95.00000
CM-244	5531.761	5884.598	1.000000	0.2400000	100.0000	95.00000

Instrument : CHAMBER 099
 Detector : 30432
 Background Analysis Date/Time : 2-APR-2006 11:38:44
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2989.302	3301.806	0.0000000E+00	0.0000000E+00	0.0000000E+00	95.00000
NP-237	4434.583	4904.427	0.0000000E+00	0.0000000E+00	0.0000000E+00	95.00000
CM-244	5532.529	5887.439	1.000000	0.2399998	100.0000	95.00000

Instrument : CHAMBER 101
 Detector : 31696
 Background Analysis Date/Time : 2-APR-2006 11:38:45
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2988.838	3300.184	2.000000	0.4800001	70.71068	95.00000
NP-237	4437.473	4904.200	4.000000	0.9600002	50.00000	95.00000
CM-244	5533.420	5882.862	1.000000	0.2400000	100.0000	95.00000

Instrument : CHAMBER 102
 Detector : 30438
 Background Analysis Date/Time : 2-APR-2006 11:38:45
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2990.981	3300.175	0.000000E+00	0.000000E+00	0.000000E+00	95.00000
NP-237	4436.167	4905.013	14.00000	3.360001	26.72612	95.00000
CM-244	5534.874	5885.847	0.000000E+00	0.000000E+00	0.000000E+00	95.00000

Instrument : CHAMBER 103
 Detector : 30437
 Background Analysis Date/Time : 2-APR-2006 11:38:45
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2987.494	3300.797	2.000000	0.4800001	70.71068	95.00000
NP-237	4433.628	4906.553	4.000000	0.9600002	50.00000	95.00000
CM-244	5534.963	5885.168	3.000000	0.7200001	57.73503	95.00000

Instrument : CHAMBER 104
 Detector : 30436
 Background Analysis Date/Time : 2-APR-2006 11:38:45
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2989.844	3302.458	1.000000	0.2400000	100.0000	95.00000
NP-237	4432.663	4904.432	2.000000	0.4800001	70.71068	95.00000
CM-244	5531.252	5885.942	1.000000	0.2400000	100.0000	95.00000

Instrument : CHAMBER 106
 Detector : 45382
 Background Analysis Date/Time : 2-APR-2006 11:38:45
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2991.094	3299.001	2.000000	0.4800001	70.71068	95.00000
NP-237	4435.781	4902.986	7.000000	1.680000	37.79645	95.00000
CM-244	5530.755	5886.020	0.000000E+00	0.000000E+00	0.000000E+00	95.00000

Instrument : CHAMBER 107
 Detector : 31697
 Background Analysis Date/Time : 2-APR-2006 11:38:46
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2990.547	3299.714	1.000000	0.2400000	100.0000	95.00000
NP-237	4437.183	4902.948	1.000000	0.2400000	100.0000	95.00000
CM-244	5532.612	5885.240	6.000000	1.440000	40.82483	95.00000

Instrument : CHAMBER 109
 Detector : 31693
 Background Analysis Date/Time : 2-APR-2006 11:38:46
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2988.084	3299.184	3.000000	0.7200001	57.73503	95.00000
NP-237	4432.535	4905.875	1.000000	0.2400000	100.0000	95.00000
CM-244	5532.554	5883.883	2.000000	0.4800001	70.71068	95.00000

Instrument : CHAMBER 110
 Detector : 30447
 Background Analysis Date/Time : 2-APR-2006 11:38:46
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2992.012	3300.888	1.000000	0.2400000	100.0000	95.00000
NP-237	4433.842	4901.474	1.000000	0.2400000	100.0000	95.00000
CM-244	5530.607	5884.669	1.000000	0.2400000	100.0000	95.00000

Instrument : CHAMBER 111
 Detector : 30448
 Background Analysis Date/Time : 2-APR-2006 11:38:46
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2987.793	3301.004	3.000000	0.7200001	57.73503	95.00000
NP-237	4435.981	4906.484	6.000000	1.440000	40.82483	95.00000
CM-244	5530.639	5883.341	2.000000	0.4800001	70.71068	95.00000

Instrument : CHAMBER 112
 Detector : 30449
 Background Analysis Date/Time : 2-APR-2006 11:38:46
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2991.870	3298.269	1.000000	0.2400000	100.0000	95.00000
NP-237	4436.313	4903.586	3.000000	0.7200001	57.73503	95.00000
CM-244	5533.752	5883.818	0.0000000E+00	0.0000000E+00	0.0000000E+00	95.00000

Instrument : CHAMBER 113
 Detector : 45-111B4
 Background Analysis Date/Time : 2-APR-2006 10:57:16
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2991.835	3301.848	1.000000	0.2400000	100.0000	95.00000
NP-237	4433.613	4901.946	2.000000	0.4800001	70.71068	95.00000
CM-244	5530.358	5885.560	2.000000	0.4800001	70.71068	95.00000

Instrument : CHAMBER 114
 Detector : 45-111B5
 Background Analysis Date/Time : 2-APR-2006 10:57:20
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2990.875	3299.211	0.0000000E+00	0.0000000E+00	0.0000000E+00	95.00000
NP-237	4436.329	4903.130	1.000000	0.2400000	100.0000	95.00000
CM-244	5535.235	5884.346	0.0000000E+00	0.0000000E+00	0.0000000E+00	95.00000

Instrument : CHAMBER 115
 Detector : 45-132EE5
 Background Analysis Date/Time : 2-APR-2006 10:57:23
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2990.466	3300.287	0.0000000E+00	0.0000000E+00	0.0000000E+00	95.00000
NP-237	4435.908	4903.427	1.000000	0.2400000	100.0000	95.00000
CM-244	5530.487	5884.796	0.0000000E+00	0.0000000E+00	0.0000000E+00	95.00000

Instrument : CHAMBER 116
 Detector : 45-132FF2
 Background Analysis Date/Time : 2-APR-2006 10:57:26
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2988.161	3302.097	1.000000	0.2400000	100.0000	95.00000
NP-237	4435.898	4903.366	0.0000000E+00	0.0000000E+00	0.0000000E+00	95.00000
CM-244	5530.965	5885.878	1.000000	0.2400000	100.0000	95.00000

Instrument : CHAMBER 117
 Detector : 45-132FF3
 Background Analysis Date/Time : 2-APR-2006 10:57:29
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2987.574	3297.481	2.000000	0.4800001	70.71068	95.00000
NP-237	4432.916	4905.417	3.000000	0.7200001	57.73503	95.00000
CM-244	5531.962	5885.886	2.000000	0.4800001	70.71068	95.00000

Instrument : CHAMBER 118
 Detector : 45-132FF4
 Background Analysis Date/Time : 2-APR-2006 10:57:33
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2989.600	3298.996	1.000000	0.2400000	100.0000	95.00000
NP-237	4434.069	4901.807	2.000000	0.4800001	70.71068	95.00000
CM-244	5534.903	5884.430	0.0000000E+00	0.0000000E+00	0.0000000E+00	95.00000

Instrument : CHAMBER 119
 Detector : 45-132FF5
 Background Analysis Date/Time : 2-APR-2006 10:57:36
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2987.490	3300.068	0.0000000E+00	0.0000000E+00	0.0000000E+00	95.00000
NP-237	4434.344	4905.254	0.0000000E+00	0.0000000E+00	0.0000000E+00	95.00000
CM-244	5530.554	5884.197	0.0000000E+00	0.0000000E+00	0.0000000E+00	95.00000

Instrument : CHAMBER 120
 Detector : 45-142F1
 Background Analysis Date/Time : 2-APR-2006 10:57:39
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2991.710	3300.418	0.000000E+00	0.000000E+00	0.000000E+00	95.00000
NP-237	4437.274	4903.259	1.000000	0.2400000	100.0000	95.00000
CM-244	5533.634	5886.862	1.000000	0.2400000	100.0000	95.00000

Instrument : CHAMBER 121
 Detector : 45-142J4
 Background Analysis Date/Time : 2-APR-2006 10:57:42
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2988.124	3301.600	1.000000	0.2400000	100.0000	95.00000
NP-237	4434.163	4906.581	1.000000	0.2400000	100.0000	95.00000
CM-244	5533.976	5883.453	2.000000	0.4800001	70.71068	95.00000

Instrument : CHAMBER 122
 Detector : 45-142J5
 Background Analysis Date/Time : 2-APR-2006 10:57:46
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2990.061	3298.780	1.000000	0.2400000	100.0000	95.00000
NP-237	4436.620	4903.419	1.000000	0.2400000	100.0000	95.00000
CM-244	5535.258	5884.098	1.000000	0.2400000	100.0000	95.00000

Instrument : CHAMBER 123
 Detector : 45-142V1
 Background Analysis Date/Time : 2-APR-2006 10:57:49
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2990.387	3299.522	2.000000	0.4800001	70.71068	95.00000
NP-237	4437.442	4903.641	1.000000	0.2400000	100.0000	95.00000
CM-244	5534.110	5887.297	1.000000	0.2400000	100.0000	95.00000

Instrument : CHAMBER 124
 Detector : 45-142V2
 Background Analysis Date/Time : 2-APR-2006 10:57:52
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2989.443	3297.987	2.000000	0.4800001	70.71068	95.00000
NP-237	4435.559	4902.411	2.000000	0.4800001	70.71068	95.00000
CM-244	5534.467	5883.494	1.000000	0.2400000	100.0000	95.00000

Instrument : CHAMBER 125
 Detector : 45-142V3
 Background Analysis Date/Time : 2-APR-2006 10:57:55
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2992.436	3301.693	1.000000	0.2400000	100.0000	95.00000
NP-237	4433.216	4903.410	2.000000	0.4800001	70.71068	95.00000
CM-244	5531.615	5883.226	2.000000	0.4800001	70.71068	95.00000

Instrument : CHAMBER 126
 Detector : 45-142V5
 Background Analysis Date/Time : 2-APR-2006 10:57:59
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2988.369	3299.131	0.0000000E+00	0.0000000E+00	0.0000000E+00	95.00000
NP-237	4435.618	4902.366	1.000000	0.2400000	100.0000	95.00000
CM-244	5532.732	5885.449	3.000000	0.7200001	57.73503	95.00000

Instrument : CHAMBER 127
 Detector : 45-142W1
 Background Analysis Date/Time : 2-APR-2006 10:58:02
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2989.513	3302.392	0.0000000E+00	0.0000000E+00	0.0000000E+00	95.00000
NP-237	4432.606	4903.961	1.000000	0.2400000	100.0000	95.00000
CM-244	5535.216	5883.874	1.000000	0.2400000	100.0000	95.00000

Instrument : CHAMBER 128
 Detector : 45-142W2
 Background Analysis Date/Time : 2-APR-2006 10:58:05
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2989.584	3299.388	0.000000E+00	0.000000E+00	0.000000E+00	95.00000
NP-237	4434.590	4901.786	0.000000E+00	0.000000E+00	0.000000E+00	95.00000
CM-244	5533.622	5887.583	2.000000	0.4800001	70.71068	95.00000

Instrument : CHAMBER 129
 Detector : 45-142W3
 Background Analysis Date/Time : 2-APR-2006 10:58:09
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2991.668	3299.558	0.000000E+00	0.000000E+00	0.000000E+00	95.00000
NP-237	4435.149	4901.376	2.000000	0.4800001	70.71068	95.00000
CM-244	5532.751	5886.867	2.000000	0.4800001	70.71068	95.00000

Instrument : CHAMBER 130
 Detector : 45-142W5
 Background Analysis Date/Time : 2-APR-2006 10:58:13
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2990.831	3301.623	0.000000E+00	0.000000E+00	0.000000E+00	95.00000
NP-237	4435.787	4904.916	0.000000E+00	0.000000E+00	0.000000E+00	95.00000
CM-244	5534.223	5884.439	1.000000	0.2400000	100.0000	95.00000

Instrument : CHAMBER 131
 Detector : 45-145K1
 Background Analysis Date/Time : 2-APR-2006 10:58:17
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2989.369	3298.448	1.000000	0.2400000	100.0000	95.00000
NP-237	4432.591	4905.330	0.000000E+00	0.000000E+00	0.000000E+00	95.00000
CM-244	5532.857	5887.665	1.000000	0.2400000	100.0000	95.00000

Instrument : CHAMBER 132
 Detector : 45-145K2
 Background Analysis Date/Time : 2-APR-2006 10:58:20
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2990.018	3301.016	0.000000E+00	0.000000E+00	0.000000E+00	95.00000
NP-237	4434.219	4902.195	2.000000	0.4800001	70.71068	95.00000
CM-244	5534.644	5883.351	4.000000	0.9600002	50.00000	95.00000

Instrument : CHAMBER 133
 Detector : 45-145K3
 Background Analysis Date/Time : 2-APR-2006 10:58:23
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2989.115	3302.033	0.000000E+00	0.000000E+00	0.000000E+00	95.00000
NP-237	4435.237	4904.688	0.000000E+00	0.000000E+00	0.000000E+00	95.00000
CM-244	5532.486	5884.151	1.000000	0.2400000	100.0000	95.00000

Instrument : CHAMBER 134
 Detector : 45-145K4
 Background Analysis Date/Time : 2-APR-2006 10:58:26
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2987.530	3301.962	1.000000	0.2400000	100.0000	95.00000
NP-237	4434.547	4905.459	0.000000E+00	0.000000E+00	0.000000E+00	95.00000
CM-244	5534.869	5887.271	0.000000E+00	0.000000E+00	0.000000E+00	95.00000

Instrument : CHAMBER 135
 Detector : 45-145K5
 Background Analysis Date/Time : 2-APR-2006 10:58:30
 Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2990.104	3298.632	1.000000	0.2400000	100.0000	95.00000
NP-237	4434.981	4906.088	0.000000E+00	0.000000E+00	0.000000E+00	95.00000
CM-244	5531.074	5884.261	0.000000E+00	0.000000E+00	0.000000E+00	95.00000

Instrument : CHAMBER 136
Detector : 45-145L1
Background Analysis Date/Time : 2-APR-2006 10:58:33
Background Count Time : 60000.00

Cal. Isotopes	Start Energy	End Energy	Counts in 1000 min	Counts during Cal	% Error	Confidence
GD-148	2988.496	3298.473	0.000000E+00	0.000000E+00	0.000000E+00	95.00000
NP-237	4437.582	4903.436	1.000000	0.240000	100.0000	95.00000
CM-244	5532.704	5884.860	0.000000E+00	0.000000E+00	0.000000E+00	95.00000

Subsection 3: Efficiency Calibration

Instrument : CHAMBER 001
 Detector : 33088
 Standard ID : AESS-001
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 12:02:15
 Calibration Count Time : 239.9998
 Efficiency Calibration Date/Time : 3-APR-2006 16:30:52
 Average Efficiency : 0.2781914
 Average Efficiency Error : 7.6626688E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.8400	28-FEB-2006	2990.456	3298.943	14076.00	0.2746735	1.1824497E-02	65.35928
NP-237	211.8600	28-FEB-2006	4433.436	4903.018	14340.00	0.2819934	1.4295015E-02	71.99430
CM-244	248.8200	28-FEB-2006	5530.638	5887.374	14794.00	0.2795064	1.4163047E-02	64.69388

Instrument : CHAMBER 003
 Detector : 20659
 Standard ID : AESS-003
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 12:02:15
 Calibration Count Time : 239.9998
 Efficiency Calibration Date/Time : 3-APR-2006 16:32:34
 Average Efficiency : 0.2880620
 Average Efficiency Error : 7.9304650E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.3600	28-FEB-2006	2988.599	3300.169	14554.00	0.2846224	1.2245077E-02	49.78555
NP-237	211.3800	28-FEB-2006	4434.674	4902.844	14694.00	0.2895928	1.4675476E-02	61.61686
CM-244	248.2800	28-FEB-2006	5535.248	5883.783	15396.00	0.2915129	1.4763834E-02	53.23063

Instrument : CHAMBER 004
 Detector : 33077
 Standard ID : AESS-004
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 12:02:15
 Calibration Count Time : 239.9998
 Efficiency Calibration Date/Time : 3-APR-2006 16:32:51
 Average Efficiency : 0.3098668
 Average Efficiency Error : 8.5239913E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.1800	28-FEB-2006	2987.545	3299.456	15401.00	0.3014340	1.2955099E-02	59.94693
NP-237	211.2000	28-FEB-2006	4433.646	4906.400	15919.00	0.3140544	1.5898786E-02	66.99142
CM-244	248.1000	28-FEB-2006	5531.494	5886.867	16816.00	0.3186174	1.6119311E-02	64.44215

Instrument : CHAMBER 005
 Detector : 28642
 Standard ID : AESS-005
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 12:02:15
 Calibration Count Time : 239.9998
 Efficiency Calibration Date/Time : 3-APR-2006 16:33:05
 Average Efficiency : 0.3158097
 Average Efficiency Error : 8.6822659E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.6600	28-FEB-2006	2990.709	3298.775	16078.00	0.3139968	1.3485039E-02	54.11107
NP-237	211.6800	28-FEB-2006	4434.190	4905.248	16264.00	0.3200765	1.6199514E-02	58.77632
CM-244	248.6400	28-FEB-2006	5530.463	5883.921	16620.00	0.3142197	1.5898999E-02	55.82949

Instrument : CHAMBER 007
 Detector : 30416
 Standard ID : AESS-007
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 12:02:16
 Calibration Count Time : 239.9998
 Efficiency Calibration Date/Time : 3-APR-2006 16:35:21
 Average Efficiency : 0.3047189
 Average Efficiency Error : 8.3812820E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.5400	28-FEB-2006	2990.797	3298.358	15695.00	0.3066845	1.3176420E-02	50.85197
NP-237	211.5600	28-FEB-2006	4432.556	4903.394	15403.00	0.3033007	1.5360770E-02	59.57014
CM-244	248.5200	28-FEB-2006	5533.897	5887.491	16043.00	0.3034657	1.5361345E-02	53.08852

Instrument : CHAMBER 009
 Detector : 13285
 Standard ID : AESS-009
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 12:02:16
 Calibration Count Time : 239.9998
 Efficiency Calibration Date/Time : 3-APR-2006 16:39:51
 Average Efficiency : 0.3341929
 Average Efficiency Error : 9.1806399E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.6000	28-FEB-2006	2987.740	3302.180	16955.00	0.3312147	1.4212075E-02	53.77267
NP-237	211.6200	28-FEB-2006	4436.826	4904.306	17080.00	0.3362575	1.7008657E-02	68.28894
CM-244	248.5800	28-FEB-2006	5530.853	5882.488	17788.00	0.3363935	1.7007809E-02	56.00669

Instrument : CHAMBER 010
 Detector : 33083
 Standard ID : AESS-010
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 12:02:16
 Calibration Count Time : 239.9998
 Efficiency Calibration Date/Time : 3-APR-2006 16:40:04
 Average Efficiency : 0.3340436
 Average Efficiency Error : 9.1786785E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.4800	28-FEB-2006	2992.233	3300.495	16676.00	0.3259426	1.3989601E-02	68.92194
NP-237	211.5000	28-FEB-2006	4435.514	4905.914	17301.00	0.3408116	1.7236479E-02	78.65460
CM-244	248.4600	28-FEB-2006	5535.151	5882.345	17946.00	0.3395274	1.7164614E-02	63.81354

Instrument : CHAMBER 011
 Detector : 9537
 Standard ID : AESS-011
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 12:02:16
 Calibration Count Time : 239.9998
 Efficiency Calibration Date/Time : 3-APR-2006 16:40:58
 Average Efficiency : 0.3105724
 Average Efficiency Error : 8.5400529E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.6600	28-FEB-2006	2988.769	3298.475	15819.00	0.3089387	1.3271471E-02	48.37308
NP-237	211.6800	28-FEB-2006	4433.776	4901.438	15834.00	0.3116739	1.5779305E-02	60.99158
CM-244	248.6400	28-FEB-2006	5533.457	5885.193	16490.00	0.3117799	1.5776988E-02	49.82006

Instrument : CHAMBER 012
 Detector : 33085
 Standard ID : AESS-012
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 12:02:16
 Calibration Count Time : 239.9998
 Efficiency Calibration Date/Time : 3-APR-2006 16:41:13
 Average Efficiency : 0.2681623
 Average Efficiency Error : 7.3903115E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.9600	28-FEB-2006	2992.283	3299.978	13668.00	0.2665664	1.1482058E-02	61.90531
NP-237	211.9200	28-FEB-2006	4432.454	4901.598	13787.00	0.2710549	1.3747970E-02	71.13239
CM-244	248.9400	28-FEB-2006	5534.285	5885.751	14169.00	0.2675734	1.3566247E-02	62.43946

Instrument : CHAMBER 013
 Detector : 21084
 Standard ID : AESS-013
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 12:02:17
 Calibration Count Time : 239.9998
 Efficiency Calibration Date/Time : 3-APR-2006 16:41:26
 Average Efficiency : 0.3412675
 Average Efficiency Error : 9.3716113E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	220.5600	28-FEB-2006	2992.308	3301.307	17507.00	0.3405094	1.4603521E-02	45.62738
NP-237	212.5200	28-FEB-2006	4433.829	4905.476	17346.00	0.3400816	1.7199026E-02	62.98444
CM-244	249.6600	28-FEB-2006	5530.551	5886.625	18245.00	0.3435482	1.7364752E-02	51.62660

Instrument : CHAMBER 016
 Detector : 21086
 Standard ID : AESS-016
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 12:02:17
 Calibration Count Time : 239.9998
 Efficiency Calibration Date/Time : 3-APR-2006 16:45:33
 Average Efficiency : 0.3303408
 Average Efficiency Error : 9.0769110E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.6600	28-FEB-2006	2992.386	3300.792	16669.00	0.3255388	1.3972365E-02	50.42868
NP-237	211.6800	28-FEB-2006	4437.111	4903.407	16820.00	0.3310585	1.6748626E-02	58.68690
CM-244	248.6400	28-FEB-2006	5533.819	5884.776	17810.00	0.3367283	1.7024504E-02	54.94007

Instrument : CHAMBER 017
 Detector : 33203
 Standard ID : AESS-017
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 12:02:17
 Calibration Count Time : 239.9998
 Efficiency Calibration Date/Time : 3-APR-2006 16:45:52
 Average Efficiency : 0.2902693
 Average Efficiency Error : 7.9895537E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.7200	28-FEB-2006	2988.693	3298.212	15015.00	0.2931568	1.2605052E-02	49.49680
NP-237	211.7400	28-FEB-2006	4432.905	4905.400	14650.00	0.2882629	1.4608623E-02	61.60561
CM-244	248.7000	28-FEB-2006	5532.198	5886.394	15257.00	0.2883977	1.4607739E-02	50.89099

Instrument : CHAMBER 018
 Detector : 21063
 Standard ID : AESS-018
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 12:02:17
 Calibration Count Time : 239.9998
 Efficiency Calibration Date/Time : 3-APR-2006 16:46:43
 Average Efficiency : 0.2559204
 Average Efficiency Error : 7.0582652E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.7800	28-FEB-2006	2988.076	3298.134	13144.00	0.2565568	1.1059588E-02	50.10976
NP-237	211.8000	28-FEB-2006	4433.036	4905.011	12933.00	0.2544221	1.2916340E-02	58.60687
CM-244	248.7600	28-FEB-2006	5535.243	5885.674	13576.00	0.2565605	1.3015677E-02	54.43167

Instrument : CHAMBER 019
 Detector : 23882
 Standard ID : AESS-019
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 12:02:18
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 3-APR-2006 16:46:59
 Average Efficiency : 0.2848921
 Average Efficiency Error : 7.8617986E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.5400	28-FEB-2006	2989.511	3300.144	15017.00	0.2934360	1.2617028E-02	46.50811
NP-237	211.5600	28-FEB-2006	4435.855	4902.151	15150.00	0.2626681	1.3361575E-02	61.07557
CM-244	248.5200	28-FEB-2006	5531.789	5884.041	15932.00	0.3013749	1.5256786E-02	50.77583

Instrument : CHAMBER 020
 Detector : 33093
 Standard ID : AESS-020
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 12:02:18
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 3-APR-2006 16:47:46
 Average Efficiency : 0.3374673
 Average Efficiency Error : 9.2702135E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.8400	28-FEB-2006	2988.758	3298.111	16991.00	0.3315554	1.4226208E-02	58.22562
NP-237	211.8000	28-FEB-2006	4435.838	4901.523	17420.00	0.3426790	1.7329575E-02	71.40521
CM-244	248.8200	28-FEB-2006	5530.915	5883.311	18048.00	0.3409902	1.7237470E-02	64.18688

Instrument : CHAMBER 021
 Detector : 33893
 Standard ID : AESS-021
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 12:02:18
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 3-APR-2006 16:48:06
 Average Efficiency : 0.3097920
 Average Efficiency Error : 8.5189342E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.5400	28-FEB-2006	2987.969	3300.683	16019.00	0.3130153	1.3443721E-02	48.52213
NP-237	211.5600	28-FEB-2006	4434.165	4904.181	15665.00	0.3085031	1.5620876E-02	57.03367
CM-244	248.5200	28-FEB-2006	5533.125	5885.623	16217.00	0.3067660	1.5526365E-02	49.52942

Instrument : CHAMBER 023
 Detector : 22873
 Standard ID : AESS-023
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 12:02:18
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 3-APR-2006 16:49:38
 Average Efficiency : 0.2765626
 Average Efficiency Error : 7.6345578E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.6600	28-FEB-2006	2988.365	3300.653	13199.00	0.2577709	1.1110976E-02	64.03100
NP-237	211.6800	28-FEB-2006	4432.587	4902.786	15014.00	0.2955187	1.4971492E-02	68.68533
CM-244	248.6400	28-FEB-2006	5533.585	5885.616	15406.00	0.2912842	1.4752124E-02	67.86546

Instrument : CHAMBER 026
 Detector : 34427
 Standard ID : AESS-002
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 07:45:51
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 4-APR-2006 12:02:00
 Average Efficiency : 0.3111628
 Average Efficiency Error : 5.9400578E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.4800	28-FEB-2006	2988.396	3300.299	15946.00	0.3116805	7.0337788E-03	55.54451
NP-237	211.5000	28-FEB-2006	4432.951	4903.551	15774.00	0.3107190	1.5731754E-02	60.78556
CM-244	248.4000	28-FEB-2006	5534.085	5882.486	16328.00	0.3090416	1.5640259E-02	54.94981

Instrument : CHAMBER 027
 Detector : 31436
 Standard ID : AESS-003
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 07:45:51
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 4-APR-2006 12:02:17
 Average Efficiency : 0.2851310
 Average Efficiency Error : 5.4681562E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.3600	28-FEB-2006	2990.641	3298.501	14516.00	0.2838850	6.4452491E-03	62.80336
NP-237	211.3800	28-FEB-2006	4435.554	4903.960	14590.00	0.2875520	1.4573419E-02	61.53238
CM-244	248.2800	28-FEB-2006	5535.178	5885.600	15268.00	0.2891185	1.4644115E-02	66.27240

Instrument : CHAMBER 028
 Detector : 21056
 Standard ID : AESS-004
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 07:45:51
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 4-APR-2006 12:02:41
 Average Efficiency : 0.2688177
 Average Efficiency Error : 5.1718531E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.1800	28-FEB-2006	2991.862	3298.519	13660.00	0.2673638	6.0955230E-03	60.48663
NP-237	211.2000	28-FEB-2006	4437.162	4904.527	13850.00	0.2732216	1.3856977E-02	78.59827
CM-244	248.1000	28-FEB-2006	5534.678	5884.670	14348.00	0.2718943	1.3782959E-02	69.00627

Instrument : CHAMBER 029
 Detector : 30419
 Standard ID : AESS-005
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 07:45:51
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 4-APR-2006 12:02:56
 Average Efficiency : 0.2803768
 Average Efficiency Error : 5.3804033E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.6600	28-FEB-2006	2991.643	3298.009	14347.00	0.2801967	6.3665169E-03	50.13651
NP-237	211.6800	28-FEB-2006	4436.124	4903.513	14180.00	0.2791024	1.4150602E-02	62.17907
CM-244	248.6400	28-FEB-2006	5533.909	5884.139	14945.00	0.2825924	1.4317507E-02	55.61591

Instrument : CHAMBER 030
 Detector : 30420
 Standard ID : AESS-006
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 07:45:51
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 4-APR-2006 12:03:11
 Average Efficiency : 0.3032622
 Average Efficiency Error : 5.7966388E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.1800	28-FEB-2006	2992.381	3300.032	15532.00	0.3040040	6.8717906E-03	53.70943
NP-237	211.2000	28-FEB-2006	4435.171	4901.399	15235.00	0.3005646	1.5224237E-02	63.92149
CM-244	248.1000	28-FEB-2006	5532.938	5887.226	15953.00	0.3023090	1.5303830E-02	56.83110

Instrument : CHAMBER 032
 Detector : 33207
 Standard ID : AESS-008
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 07:45:53
 Calibration Count Time : 239.9998
 Efficiency Calibration Date/Time : 4-APR-2006 12:04:09
 Average Efficiency : 0.3210600
 Average Efficiency Error : 9.3805837E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.8400	28-FEB-2006	2992.438	3301.011	16394.00	0.3199127	1.6193897E-02	48.92264
NP-237	211.8600	28-FEB-2006	4437.450	4903.298	16174.00	0.3180676	1.6098870E-02	62.34297
CM-244	248.8800	28-FEB-2006	5533.518	5886.674	17224.00	0.3253718	1.6456470E-02	58.56594

Instrument : CHAMBER 033
 Detector : 28647
 Standard ID : AESS-009
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 07:45:53
 Calibration Count Time : 239.9998
 Efficiency Calibration Date/Time : 4-APR-2006 12:04:20
 Average Efficiency : 0.3189350
 Average Efficiency Error : 9.3192765E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.6000	28-FEB-2006	2991.128	3301.778	16210.00	0.3166678	1.6031807E-02	50.20483
NP-237	211.6200	28-FEB-2006	4433.277	4905.752	16119.00	0.3173501	1.6063211E-02	65.81153
CM-244	248.5800	28-FEB-2006	5531.202	5887.135	17074.00	0.3229274	1.6334468E-02	56.14278

Instrument : CHAMBER 034
 Detector : 32697
 Standard ID : AESS-010
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 07:45:53
 Calibration Count Time : 239.9998
 Efficiency Calibration Date/Time : 4-APR-2006 12:04:32
 Average Efficiency : 0.3285644
 Average Efficiency Error : 9.5973080E-03
 Confidence : 95.00000

Cal. Isteps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.4800	28-FEB-2006	2987.740	3297.727	16717.00	0.3267508	1.6536236E-02	46.19645
NP-237	211.5000	28-FEB-2006	4436.424	4906.295	16590.00	0.3267619	1.6533978E-02	65.57603
CM-244	248.4600	28-FEB-2006	5532.067	5883.683	17561.00	0.3322987	1.6803153E-02	52.60378

Instrument : CHAMBER 035
 Detector : 29271
 Standard ID : AESS-011
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 07:45:53
 Calibration Count Time : 239.9998
 Efficiency Calibration Date/Time : 4-APR-2006 12:04:44
 Average Efficiency : 0.3070081
 Average Efficiency Error : 8.9746779E-03
 Confidence : 95.00000

Cal. Isteps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.6600	28-FEB-2006	2990.597	3300.316	15823.00	0.3090232	1.5649391E-02	58.07399
NP-237	211.6800	28-FEB-2006	4435.093	4902.062	15491.00	0.3048278	1.5437050E-02	77.73704
CM-244	248.6400	28-FEB-2006	5533.546	5887.289	16248.00	0.3072308	1.5549533E-02	61.23973

Instrument : CHAMBER 036
 Detector : 29275
 Standard ID : AESS-012
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 07:45:53
 Calibration Count Time : 239.9998
 Efficiency Calibration Date/Time : 4-APR-2006 12:04:58
 Average Efficiency : 0.3204660
 Average Efficiency Error : 9.3638916E-03
 Confidence : 95.00000

Cal. Isteps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.9600	28-FEB-2006	2990.101	3302.011	16111.00	0.3142187	1.5908994E-02	70.87608
NP-237	211.9200	28-FEB-2006	4436.212	4902.690	16497.00	0.3243046	1.6410707E-02	86.38094
CM-244	248.9400	28-FEB-2006	5530.586	5883.211	17117.00	0.3232544	1.6350558E-02	83.27386

Instrument : CHAMBER 037
 Detector : 32690
 Standard ID : AESS-013
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 07:45:55
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 4-APR-2006 12:05:37
 Average Efficiency : 0.3298278
 Average Efficiency Error : 6.2852711E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	220.5600	28-FEB-2006	2990.331	3300.070	16648.00	0.3238085	7.2884769E-03	65.32179
NP-237	212.5200	28-FEB-2006	4435.120	4902.289	17586.00	0.3447773	1.7433835E-02	73.49030
CM-244	249.6600	28-FEB-2006	5534.121	5882.713	18584.00	0.3498755	1.7681209E-02	65.58303

Instrument : CHAMBER 038
 Detector : 19323
 Standard ID : AESS-014
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 07:45:55
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 4-APR-2006 12:05:48
 Average Efficiency : 0.3550652
 Average Efficiency Error : 6.7386958E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.9600	28-FEB-2006	2992.203	3301.129	18140.00	0.3537907	7.9244133E-03	44.64486
NP-237	211.9800	28-FEB-2006	4436.340	4904.950	18294.00	0.3595673	1.8173877E-02	68.25054
CM-244	249.0000	28-FEB-2006	5534.574	5885.451	18924.00	0.3572362	1.8049749E-02	49.98671

Instrument : CHAMBER 040
 Detector : 30446
 Standard ID : AESS-016
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 07:45:55
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 4-APR-2006 12:06:33
 Average Efficiency : 0.3232525
 Average Efficiency Error : 6.1597549E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.6600	28-FEB-2006	2990.636	3301.603	16579.00	0.3237876	7.2898054E-03	47.52289
NP-237	211.6800	28-FEB-2006	4435.733	4904.719	16163.00	0.3181213	1.6101720E-02	60.46703
CM-244	248.6400	28-FEB-2006	5532.976	5885.423	17235.00	0.3258936	1.6482741E-02	51.53939

Instrument : CHAMBER 041
 Detector : 22834
 Standard ID : AESS-017
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 07:45:55
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 4-APR-2006 12:06:46
 Average Efficiency : 0.3322699
 Average Efficiency Error : 6.3254358E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.7200	28-FEB-2006	2987.681	3302.193	16913.00	0.3302204	7.4258945E-03	49.34238
NP-237	211.7400	28-FEB-2006	4432.502	4905.743	17206.00	0.3385508	1.7123217E-02	64.06297
CM-244	248.7000	28-FEB-2006	5533.298	5885.604	17818.00	0.3368361	1.7029859E-02	51.09551

Instrument : CHAMBER 042
 Detector : 32695
 Standard ID : AESS-018
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 07:45:55
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 4-APR-2006 12:07:02
 Average Efficiency : 0.3361240
 Average Efficiency Error : 6.3955071E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.7800	28-FEB-2006	2990.651	3300.194	17115.00	0.3340732	7.5073489E-03	62.01425
NP-237	211.8000	28-FEB-2006	4435.708	4903.810	17181.00	0.3379442	1.7092843E-02	71.83335
CM-244	248.7600	28-FEB-2006	5531.417	5883.758	18276.00	0.3453112	1.7453661E-02	58.83952

Instrument : CHAMBER 043
 Detector : 42470
 Standard ID : AESS-019
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 07:45:57
 Calibration Count Time : 239.9998
 Efficiency Calibration Date/Time : 4-APR-2006 12:07:20
 Average Efficiency : 0.3229622
 Average Efficiency Error : 6.1558355E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.5400	28-FEB-2006	2988.168	3298.326	16460.00	0.3216395	7.2445576E-03	53.07267
NP-237	211.5600	28-FEB-2006	4436.901	4902.013	16611.00	0.3271490	1.6553231E-02	63.02407
CM-244	248.5200	28-FEB-2006	5535.121	5886.262	17214.00	0.3256539	1.6470846E-02	50.82504

Instrument : CHAMBER 044
 Detector : 34433
 Standard ID : AESS-020
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 07:45:57
 Calibration Count Time : 239.9998
 Efficiency Calibration Date/Time : 4-APR-2006 12:07:31
 Average Efficiency : 0.3240791
 Average Efficiency Error : 6.1765807E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.8400	28-FEB-2006	2989.004	3298.648	16495.00	0.3218836	7.2491337E-03	50.22718
NP-237	211.8000	28-FEB-2006	4433.632	4906.174	16705.00	0.3285425	1.6622754E-02	66.23325
CM-244	248.8200	28-FEB-2006	5532.967	5887.129	17532.00	0.3312699	1.6751442E-02	56.69666

Instrument : CHAMBER 045
 Detector : 34430
 Standard ID : AESS-021
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 07:45:57
 Calibration Count Time : 239.9998
 Efficiency Calibration Date/Time : 4-APR-2006 12:07:49
 Average Efficiency : 0.2941546
 Average Efficiency Error : 5.6320531E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.5400	28-FEB-2006	2992.438	3301.033	14988.00	0.2928756	6.6353632E-03	49.71279
NP-237	211.5600	28-FEB-2006	4436.365	4906.490	15086.00	0.2970952	1.5050440E-02	64.58119
CM-244	248.5200	28-FEB-2006	5535.004	5886.982	15743.00	0.2978074	1.5078431E-02	59.00225

Instrument : CHAMBER 046
 Detector : 42471
 Standard ID : AESS-022
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 07:45:57
 Calibration Count Time : 239.9998
 Efficiency Calibration Date/Time : 4-APR-2006 12:08:03
 Average Efficiency : 0.3344716
 Average Efficiency Error : 6.3659614E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.6600	28-FEB-2006	2987.741	3299.741	16999.00	0.3319905	7.4634906E-03	48.96851
NP-237	211.6800	28-FEB-2006	4435.900	4904.967	17273.00	0.3399139	1.7191468E-02	65.78371
CM-244	248.6400	28-FEB-2006	5532.671	5884.488	18104.00	0.3422939	1.7302830E-02	53.33138

Instrument : CHAMBER 047
 Detector : 30449
 Standard ID : AESS-023
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 07:45:57
 Calibration Count Time : 239.9998
 Efficiency Calibration Date/Time : 4-APR-2006 12:08:14
 Average Efficiency : 0.2966904
 Average Efficiency Error : 5.6765815E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.6600	28-FEB-2006	2989.322	3298.103	15222.00	0.2972857	6.7285444E-03	49.84683
NP-237	211.6800	28-FEB-2006	4433.780	4903.899	15016.00	0.2955441	1.4972775E-02	59.65280
CM-244	248.6400	28-FEB-2006	5532.276	5884.114	15597.00	0.2948985	1.4932883E-02	51.68388

Instrument : CHAMBER 048
 Detector : 42483
 Standard ID : AESS-024
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 07:45:57
 Calibration Count Time : 239.9998
 Efficiency Calibration Date/Time : 4-APR-2006 12:08:24
 Average Efficiency : 0.3119769
 Average Efficiency Error : 5.9553082E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.4200	28-FEB-2006	2989.922	3300.161	15954.00	0.3119224	7.0390208E-03	55.83012
NP-237	211.4400	28-FEB-2006	4434.180	4904.923	15787.00	0.3110589	1.5748808E-02	72.44879
CM-244	248.4000	28-FEB-2006	5533.436	5885.010	16547.00	0.3131823	1.5847316E-02	61.06746

Instrument : CHAMBER 065
 Detector : 21087
 Standard ID : AESS-001
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 06:54:10
 Calibration Count Time : 239.9998
 Efficiency Calibration Date/Time : 3-APR-2006 12:05:24
 Average Efficiency : 0.3027465
 Average Efficiency Error : 5.7869283E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.8400	28-FEB-2006	2992.500	3301.569	15511.00	0.3026739	6.8422910E-03	49.27271
NP-237	211.8600	28-FEB-2006	4436.593	4904.814	15341.00	0.3016613	1.5278513E-02	63.47648
CM-244	248.8200	28-FEB-2006	5533.641	5883.942	16102.00	0.3042169	1.5398668E-02	52.45229

Instrument : CHAMBER 066
 Detector : 38159
 Standard ID : AESS-002
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 06:54:10
 Calibration Count Time : 239.9998
 Efficiency Calibration Date/Time : 3-APR-2006 12:05:41
 Average Efficiency : 0.2898386
 Average Efficiency Error : 5.5523221E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.4800	28-FEB-2006	2991.351	3299.570	14848.00	0.2902116	6.5790205E-03	54.22055
NP-237	211.5000	28-FEB-2006	4435.367	4906.503	14731.00	0.2901337	1.4702437E-02	64.20898
CM-244	248.4000	28-FEB-2006	5531.751	5885.195	15203.00	0.2877176	1.4573953E-02	57.41096

Instrument : CHAMBER 068
 Detector : 33204
 Standard ID : AESS-004
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 06:54:10
 Calibration Count Time : 239.9998
 Efficiency Calibration Date/Time : 3-APR-2006 12:06:11
 Average Efficiency : 0.2982503
 Average Efficiency Error : 5.7051168E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.1800	28-FEB-2006	2989.458	3302.482	15312.00	0.2996904	6.7803976E-03	66.72219
NP-237	211.2000	28-FEB-2006	4437.019	4902.188	15036.00	0.2966104	1.5026535E-02	82.73407
CM-244	248.1000	28-FEB-2006	5531.579	5884.315	15461.00	0.2929541	1.4836024E-02	72.39137

Instrument : CHAMBER 069
 Detector : 39172
 Standard ID : AESS-005
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 06:54:10
 Calibration Count Time : 239.9998
 Efficiency Calibration Date/Time : 3-APR-2006 12:06:22
 Average Efficiency : 0.2872442
 Average Efficiency Error : 5.5063334E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.6600	28-FEB-2006	2991.937	3302.037	14638.00	0.2858726	6.4867456E-03	52.69576
NP-237	211.6800	28-FEB-2006	4433.758	4901.912	14877.00	0.2928176	1.4836427E-02	60.78927
CM-244	248.6400	28-FEB-2006	5535.302	5884.863	15275.00	0.2888012	1.4627955E-02	53.21272

Instrument : CHAMBER 070
 Detector : 33207
 Standard ID : AESS-006
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 06:54:10
 Calibration Count Time : 239.9998
 Efficiency Calibration Date/Time : 3-APR-2006 12:06:32
 Average Efficiency : 0.3410026
 Average Efficiency Error : 6.4845588E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.1800	28-FEB-2006	2987.764	3299.302	17333.00	0.3392459	7.6180245E-03	53.32024
NP-237	211.2000	28-FEB-2006	4432.603	4904.338	17596.00	0.3470635	1.7549409E-02	63.32718
CM-244	248.1000	28-FEB-2006	5531.790	5887.167	18166.00	0.3442082	1.7398918E-02	55.68260

Instrument : CHAMBER 072
 Detector : 33210
 Standard ID : AESS-008
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 06:54:11
 Calibration Count Time : 239.9998
 Efficiency Calibration Date/Time : 3-APR-2006 12:07:20
 Average Efficiency : 0.2718624
 Average Efficiency Error : 5.2260533E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.8400	28-FEB-2006	2989.642	3302.500	13882.00	0.2708864	6.1688591E-03	78.20691
NP-237	211.8600	28-FEB-2006	4434.229	4902.517	13764.00	0.2706604	1.3728318E-02	68.85778
CM-244	248.8800	28-FEB-2006	5533.565	5883.889	14730.00	0.2782284	1.4099089E-02	58.98390

Instrument : CHAMBER 073
 Detector : 33211
 Standard ID : AESS-009
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 06:54:11
 Calibration Count Time : 239.9998
 Efficiency Calibration Date/Time : 3-APR-2006 12:07:31
 Average Efficiency : 0.3248378
 Average Efficiency Error : 6.1892127E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.6000	28-FEB-2006	2990.209	3299.359	16628.00	0.3248250	7.3118629E-03	52.98417
NP-237	211.6200	28-FEB-2006	4435.813	4905.119	16178.00	0.3184740	1.6119437E-02	62.15504
CM-244	248.5800	28-FEB-2006	5530.447	5887.394	17545.00	0.3317996	1.6778087E-02	56.17911

Instrument : CHAMBER 075
 Detector : 29976
 Standard ID : AESS-011
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 06:54:11
 Calibration Count Time : 239.9998
 Efficiency Calibration Date/Time : 3-APR-2006 12:07:53
 Average Efficiency : 0.3238373
 Average Efficiency Error : 6.1713755E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.6600	28-FEB-2006	2987.804	3301.738	16526.00	0.3227443	7.2676861E-03	50.99773
NP-237	211.6800	28-FEB-2006	4436.078	4904.005	16602.00	0.3267108	1.6531264E-02	64.22369
CM-244	248.6400	28-FEB-2006	5532.428	5882.500	17275.00	0.3266147	1.6518781E-02	59.07774

Instrument : CHAMBER 076
 Detector : 33213
 Standard ID : AESS-012
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 06:54:11
 Calibration Count Time : 239.9998
 Efficiency Calibration Date/Time : 3-APR-2006 12:08:02
 Average Efficiency : 0.3136021
 Average Efficiency Error : 5.9847333E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.9600	28-FEB-2006	2990.982	3301.271	16036.00	0.3127477	7.0554069E-03	52.31974
NP-237	211.9200	28-FEB-2006	4435.792	4906.032	16070.00	0.3159233	1.5991600E-02	63.89199
CM-244	248.9400	28-FEB-2006	5532.284	5884.164	16716.00	0.3156649	1.5971025E-02	56.41280

Instrument : CHAMBER 077
 Detector : 28239
 Standard ID : AESS-013
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 06:54:12
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 3-APR-2006 12:08:16
 Average Efficiency : 0.3282876
 Average Efficiency Error : 6.2494567E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	220.5600	28-FEB-2006	2990.320	3302.291	16964.00	0.3299461	7.4184034E-03	49.98071
NP-237	212.5200	28-FEB-2006	4434.458	4904.534	16485.00	0.3231252	1.6351206E-02	66.72607
CM-244	249.6600	28-FEB-2006	5534.090	5887.188	17279.00	0.3253554	1.6455045E-02	48.65668

Instrument : CHAMBER 078
 Detector : 34425
 Standard ID : AESS-014
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 06:54:12
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 3-APR-2006 12:08:26
 Average Efficiency : 0.3266231
 Average Efficiency Error : 6.2230360E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.9600	28-FEB-2006	2992.430	3298.209	16615.00	0.3240396	7.2945217E-03	49.76765
NP-237	211.9800	28-FEB-2006	4433.493	4903.776	16900.00	0.3321434	1.6802609E-02	62.23470
CM-244	249.0000	28-FEB-2006	5534.483	5883.260	17741.00	0.3349401	1.6934805E-02	53.02275

Instrument : CHAMBER 079
 Detector : 28408
 Standard ID : AESS-015
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 06:54:12
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 3-APR-2006 12:08:37
 Average Efficiency : 0.3381511
 Average Efficiency Error : 6.4334050E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.8400	28-FEB-2006	2989.549	3301.048	17162.00	0.3348904	7.5245029E-03	58.89482
NP-237	211.8600	28-FEB-2006	4435.951	4904.750	17588.00	0.3458672	1.7488951E-02	69.24126
CM-244	248.8800	28-FEB-2006	5532.313	5884.158	18433.00	0.3481725	1.7596556E-02	62.07035

Instrument : CHAMBER 080
 Detector : 29269
 Standard ID : AESS-016
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 06:54:12
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 3-APR-2006 12:08:46
 Average Efficiency : 0.3413618
 Average Efficiency Error : 6.4887921E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.6600	28-FEB-2006	2990.355	3300.887	17518.00	0.3421173	7.6778606E-03	54.84035
NP-237	211.6800	28-FEB-2006	4437.124	4904.027	17076.00	0.3360595	1.6998719E-02	70.53491
CM-244	248.6400	28-FEB-2006	5534.833	5882.541	18143.00	0.3430255	1.7339373E-02	59.19316

Instrument : CHAMBER 081
 Detector : 28243
 Standard ID : AESS-017
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 5-APR-2006 09:52:15
 Calibration Count Time : 239.9998
 Efficiency Calibration Date/Time : 5-APR-2006 14:20:00
 Average Efficiency : 0.2709154
 Average Efficiency Error : 5.2182535E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.7200	28-FEB-2006	2988.337	3300.967	13526.00	0.2640979	6.0252789E-03	74.73094
NP-237	211.7400	28-FEB-2006	4435.244	4901.705	14659.00	0.2884400	1.4617478E-02	76.53771
CM-244	248.7000	28-FEB-2006	5534.853	5883.115	15575.00	0.2944268	1.4909291E-02	67.72768

Instrument : CHAMBER 083
 Detector : 34436
 Standard ID : AESS-019
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 06:54:13
 Calibration Count Time : 239.9998
 Efficiency Calibration Date/Time : 3-APR-2006 12:09:35
 Average Efficiency : 0.3063384
 Average Efficiency Error : 5.8566006E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.5400	28-FEB-2006	2991.885	3297.745	15476.00	0.3024036	6.8371557E-03	53.97715
NP-237	211.5600	28-FEB-2006	4435.182	4902.448	16168.00	0.3183721	1.6114395E-02	65.19810
CM-244	248.5200	28-FEB-2006	5533.629	5886.856	16706.00	0.3160093	1.5988560E-02	59.26429

Instrument : CHAMBER 084
 Detector : 29953
 Standard ID : AESS-020
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 06:54:13
 Calibration Count Time : 239.9998
 Efficiency Calibration Date/Time : 3-APR-2006 12:09:48
 Average Efficiency : 0.3377420
 Average Efficiency Error : 6.4240936E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.8400	28-FEB-2006	2988.809	3299.845	17241.00	0.3364322	7.5571463E-03	45.28139
NP-237	211.8000	28-FEB-2006	4435.274	4905.090	17241.00	0.3390163	1.7146526E-02	64.38337
CM-244	248.8200	28-FEB-2006	5535.465	5886.345	18173.00	0.3433445	1.7355187E-02	52.99788

Instrument : CHAMBER 085
 Detector : 30451
 Standard ID : AESS-021
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 06:54:13
 Calibration Count Time : 239.9998
 Efficiency Calibration Date/Time : 3-APR-2006 12:10:02
 Average Efficiency : 0.2997026
 Average Efficiency Error : 5.7319975E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.5400	28-FEB-2006	2988.388	3298.321	15330.00	0.2995507	6.7767296E-03	51.54943
NP-237	211.5600	28-FEB-2006	4434.734	4902.750	15266.00	0.3006592	1.5228639E-02	59.35664
CM-244	248.5200	28-FEB-2006	5530.623	5885.465	15834.00	0.2995146	1.5163762E-02	54.82895

Instrument : CHAMBER 086
 Detector : 29278
 Standard ID : AESS-022
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 06:54:13
 Calibration Count Time : 239.9998
 Efficiency Calibration Date/Time : 3-APR-2006 12:10:24
 Average Efficiency : 0.2629639
 Average Efficiency Error : 5.0652758E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.6600	28-FEB-2006	2990.939	3300.647	13365.00	0.2610116	5.9599294E-03	51.29673
NP-237	211.6800	28-FEB-2006	4432.832	4902.859	13621.00	0.2680805	1.3599468E-02	59.09101
CM-244	248.6400	28-FEB-2006	5530.458	5886.876	14175.00	0.2680037	1.3587984E-02	51.32809

Instrument : CHAMBER 087
 Detector : 34430
 Standard ID : AESS-023
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 06:54:13
 Calibration Count Time : 239.9998
 Efficiency Calibration Date/Time : 3-APR-2006 12:10:36
 Average Efficiency : 0.2783446
 Average Efficiency Error : 5.3436500E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.6600	28-FEB-2006	2988.850	3299.145	14228.00	0.2778656	6.3170986E-03	45.75569
NP-237	211.6800	28-FEB-2006	4433.685	4904.783	14271.00	0.2804829	1.4219985E-02	56.29552
CM-244	248.6400	28-FEB-2006	5533.892	5885.860	14737.00	0.2786293	1.4119316E-02	52.11374

Instrument : CHAMBER 088
 Detector : 30434
 Standard ID : AESS-024
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 06:54:13
 Calibration Count Time : 239.9998
 Efficiency Calibration Date/Time : 3-APR-2006 12:10:54
 Average Efficiency : 0.2708718
 Average Efficiency Error : 5.2093272E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.4200	28-FEB-2006	2991.733	3298.324	13762.00	0.2690588	6.1309491E-03	70.44978
NP-237	211.4400	28-FEB-2006	4434.854	4901.741	13876.00	0.2734241	1.3866881E-02	84.52332
CM-244	248.4000	28-FEB-2006	5531.597	5882.583	14679.00	0.2778009	1.4078071E-02	70.46585

Instrument : CHAMBER 089
 Detector : 21087
 Standard ID : AESS-001
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 18:48:42
 Calibration Count Time : 239.9998
 Efficiency Calibration Date/Time : 3-APR-2006 23:05:32
 Average Efficiency : 0.2906057
 Average Efficiency Error : 8.5010817E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.8400	28-FEB-2006	2988.018	3301.225	14810.00	0.2889985	1.4647639E-02	48.13472
NP-237	211.8600	28-FEB-2006	4432.655	4904.531	14711.00	0.2893088	1.4660804E-02	59.05686
CM-244	248.8200	28-FEB-2006	5531.146	5885.550	15539.00	0.2935953	1.4867556E-02	51.89399

Instrument : CHAMBER 090
 Detector : 38159
 Standard ID : AESS-002
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 18:48:42
 Calibration Count Time : 239.9998
 Efficiency Calibration Date/Time : 3-APR-2006 23:06:16
 Average Efficiency : 0.3262078
 Average Efficiency Error : 9.5290253E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.4800	28-FEB-2006	2989.511	3299.809	16611.00	0.3246745	1.6432377E-02	43.47319
NP-237	211.5000	28-FEB-2006	4434.211	4904.337	16570.00	0.3264199	1.6516838E-02	66.74939
CM-244	248.4000	28-FEB-2006	5530.381	5887.548	17307.00	0.3275529	1.6565884E-02	47.20604

Instrument : CHAMBER 091
 Detector : 33205
 Standard ID : AESS-003
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 16:38:39
 Calibration Count Time : 239.9998
 Efficiency Calibration Date/Time : 4-APR-2006 21:06:36
 Average Efficiency : 0.3295136
 Average Efficiency Error : 9.6244970E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.3600	28-FEB-2006	2988.614	3302.446	16877.00	0.3300617	1.6701948E-02	49.16127
NP-237	211.3800	28-FEB-2006	4435.933	4903.299	16753.00	0.3302219	1.6707057E-02	67.62949
CM-244	248.2800	28-FEB-2006	5530.786	5885.646	17335.00	0.3282727	1.6601983E-02	54.15368

Instrument : CHAMBER 092
 Detector : 33204
 Standard ID : AESS-004
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 18:48:42
 Calibration Count Time : 239.9998
 Efficiency Calibration Date/Time : 3-APR-2006 23:08:02
 Average Efficiency : 0.3230760
 Average Efficiency Error : 9.4387615E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.1800	28-FEB-2006	2991.837	3299.694	16466.00	0.3222808	1.6312918E-02	54.19599
NP-237	211.2000	28-FEB-2006	4434.184	4904.789	16328.00	0.3221140	1.6301801E-02	61.31636
CM-244	248.1000	28-FEB-2006	5534.672	5882.398	17144.00	0.3248603	1.6431469E-02	53.39663

Instrument : CHAMBER 093
 Detector : 33206
 Standard ID : AESS-005
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 18:48:42
 Calibration Count Time : 239.9998
 Efficiency Calibration Date/Time : 3-APR-2006 23:08:14
 Average Efficiency : 0.3278230
 Average Efficiency Error : 9.5757600E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.6600	28-FEB-2006	2991.432	3297.831	16618.00	0.3245451	1.6425749E-02	53.44844
NP-237	211.6800	28-FEB-2006	4432.503	4906.496	16789.00	0.3304530	1.6718345E-02	71.37048
CM-244	248.6400	28-FEB-2006	5534.120	5886.021	17378.00	0.3285792	1.6617021E-02	55.20338

Instrument : CHAMBER 094
 Detector : 33207
 Standard ID : AESS-006
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 18:48:42
 Calibration Count Time : 239.9998
 Efficiency Calibration Date/Time : 3-APR-2006 23:08:34
 Average Efficiency : 0.3064194
 Average Efficiency Error : 8.9583928E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.1800	28-FEB-2006	2991.673	3298.910	15769.00	0.3086388	1.5630580E-02	47.47134
NP-237	211.2000	28-FEB-2006	4437.305	4902.611	15693.00	0.3095863	1.5675372E-02	59.32807
CM-244	248.1000	28-FEB-2006	5532.741	5886.161	15901.00	0.3013068	1.5253706E-02	48.40099

Instrument : CHAMBER 096
 Detector : 30429
 Standard ID : AESS-008
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 18:48:43
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 3-APR-2006 23:09:48
 Average Efficiency : 0.3211957
 Average Efficiency Error : 9.3840715E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.8400	28-FEB-2006	2988.567	3301.392	16420.00	0.3204154	1.6219035E-02	48.33763
NP-237	211.8600	28-FEB-2006	4433.899	4903.007	16366.00	0.3218482	1.6287910E-02	62.84891
CM-244	248.8800	28-FEB-2006	5534.841	5883.364	17011.00	0.3213297	1.6254338E-02	53.34020

Instrument : CHAMBER 098
 Detector : 30431
 Standard ID : AESS-010
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 18:48:43
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 3-APR-2006 23:10:26
 Average Efficiency : 0.3423861
 Average Efficiency Error : 9.9960957E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.4800	28-FEB-2006	2991.193	3297.595	17461.00	0.3412881	1.7263338E-02	48.27054
NP-237	211.5000	28-FEB-2006	4433.217	4902.776	17377.00	0.3422896	1.7310398E-02	71.89059
CM-244	248.4600	28-FEB-2006	5531.761	5884.598	18159.00	0.3435947	1.7367978E-02	56.75472

Instrument : CHAMBER 099
 Detector : 30432
 Standard ID : AESS-011
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 16:38:43
 Calibration Count Time : 239.9998
 Efficiency Calibration Date/Time : 4-APR-2006 21:07:16
 Average Efficiency : 0.3424250
 Average Efficiency Error : 9.9976454E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.6600	28-FEB-2006	2989.302	3301.806	17277.00	0.3374230	1.7069872E-02	61.73035
NP-237	211.6800	28-FEB-2006	4434.583	4904.427	17554.00	0.3455301	1.7472234E-02	70.83485
CM-244	248.6400	28-FEB-2006	5532.529	5887.439	18221.00	0.3445468	1.7415471E-02	58.75341

Instrument : CHAMBER 101
 Detector : 31696
 Standard ID : AESS-013
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 18:48:44
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 3-APR-2006 23:11:17
 Average Efficiency : 0.3289411
 Average Efficiency Error : 6.2637404E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	220.5600	28-FEB-2006	2988.838	3300.184	16815.00	0.3270522	7.3571443E-03	74.97670
NP-237	212.5200	28-FEB-2006	4437.473	4904.200	16905.00	0.3314256	1.6766205E-02	82.64299
CM-244	249.6600	28-FEB-2006	5533.420	5882.862	17869.00	0.3364823	1.7011438E-02	82.36337

Instrument : CHAMBER 102
 Detector : 30438
 Standard ID : AESS-014
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 18:48:44
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 3-APR-2006 23:11:38
 Average Efficiency : 0.3398052
 Average Efficiency Error : 6.4618774E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.9600	28-FEB-2006	2990.981	3300.175	17329.00	0.3379689	7.5894571E-03	50.78636
NP-237	211.9800	28-FEB-2006	4436.167	4905.013	17442.00	0.3427780	1.7334390E-02	60.55743
CM-244	249.0000	28-FEB-2006	5534.874	5885.847	18355.00	0.3465500	1.7515350E-02	55.09371

Instrument : CHAMBER 103
 Detector : 30437
 Standard ID : AESS-015
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 18:48:44
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 3-APR-2006 23:11:50
 Average Efficiency : 0.3428698
 Average Efficiency Error : 6.5169050E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.8400	28-FEB-2006	2987.494	3300.797	17526.00	0.3419976	7.6749846E-03	52.55986
NP-237	211.8600	28-FEB-2006	4433.628	4906.553	17575.00	0.3456304	1.7477097E-02	70.84139
CM-244	248.8800	28-FEB-2006	5534.963	5885.168	18244.00	0.3446204	1.7418953E-02	56.82663

Instrument : CHAMBER 104
 Detector : 30436
 Standard ID : AESS-016
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 18:48:44
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 3-APR-2006 23:12:05
 Average Efficiency : 0.3178734
 Average Efficiency Error : 6.0614208E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.6600	28-FEB-2006	2989.844	3302.458	16342.00	0.3191546	7.1916869E-03	48.79966
NP-237	211.6800	28-FEB-2006	4432.663	4904.432	16000.00	0.3149317	1.5942214E-02	61.83171
CM-244	248.6400	28-FEB-2006	5531.252	5885.942	16635.00	0.3145305	1.5914533E-02	54.39241

Instrument : CHAMBER 106
 Detector : 45382
 Standard ID : AESS-018
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 18:48:44
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 3-APR-2006 23:13:35
 Average Efficiency : 0.3366815
 Average Efficiency Error : 6.4043794E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.7800	28-FEB-2006	2991.094	3299.001	17214.00	0.3360010	7.5481492E-03	67.49383
NP-237	211.8000	28-FEB-2006	4435.781	4902.986	17151.00	0.3373776	1.7064495E-02	78.07959
CM-244	248.7600	28-FEB-2006	5530.755	5886.020	17964.00	0.3394951	1.7162759E-02	66.37016

Instrument : CHAMBER 107
 Detector : 31697
 Standard ID : AESS-019
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 18:48:45
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 3-APR-2006 23:13:46
 Average Efficiency : 0.3279476
 Average Efficiency Error : 6.2480466E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.5400	28-FEB-2006	2990.547	3299.714	16632.00	0.3249958	7.3156110E-03	56.35443
NP-237	211.5600	28-FEB-2006	4437.183	4902.948	17025.00	0.3353024	1.6960930E-02	65.36469
CM-244	248.5200	28-FEB-2006	5532.612	5885.240	17789.00	0.3365124	1.7013798E-02	57.27279

Instrument : CHAMBER 109
 Detector : 31693
 Standard ID : AESS-021
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 18:48:45
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 3-APR-2006 23:14:12
 Average Efficiency : 0.3172656
 Average Efficiency Error : 6.0536368E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.5400	28-FEB-2006	2988.084	3299.184	16099.00	0.3145808	7.0950659E-03	55.32108
NP-237	211.5600	28-FEB-2006	4432.535	4905.875	16551.00	0.3259623	1.6493894E-02	66.04156
CM-244	248.5200	28-FEB-2006	5532.554	5883.883	17073.00	0.3229679	1.6336529E-02	53.16661

Instrument : CHAMBER 110
 Detector : 30447
 Standard ID : AESS-022
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 16:38:46
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 4-APR-2006 21:08:36
 Average Efficiency : 0.2903691
 Average Efficiency Error : 5.5707125E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.6600	28-FEB-2006	2992.012	3300.888	14540.00	0.2839686	6.4464426E-03	65.21424
NP-237	211.6800	28-FEB-2006	4433.842	4901.474	15514.00	0.3053748	1.5464325E-02	67.45113
CM-244	248.6400	28-FEB-2006	5530.607	5884.669	16569.00	0.3133079	1.5853422E-02	61.19852

Instrument : CHAMBER 111
 Detector : 30448
 Standard ID : AESS-023
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 18:48:45
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 3-APR-2006 23:15:36
 Average Efficiency : 0.3388006
 Average Efficiency Error : 6.4431382E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.6600	28-FEB-2006	2987.793	3301.004	17314.00	0.3381375	7.5936201E-03	56.34806
NP-237	211.6800	28-FEB-2006	4435.981	4906.484	17500.00	0.3444386	1.7417673E-02	71.36749
CM-244	248.6400	28-FEB-2006	5530.639	5883.341	17810.00	0.3367471	1.7025441E-02	55.06728

Instrument : CHAMBER 112
 Detector : 30449
 Standard ID : AESS-024
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 3-APR-2006 18:48:45
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 3-APR-2006 23:15:47
 Average Efficiency : 0.3139323
 Average Efficiency Error : 5.9938701E-03
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.4200	28-FEB-2006	2991.870	3298.269	15891.00	0.3106862	7.0128250E-03	50.73674
NP-237	211.4400	28-FEB-2006	4436.313	4903.586	16308.00	0.3213587	1.6263809E-02	62.04948
CM-244	248.4000	28-FEB-2006	5533.752	5883.818	17126.00	0.3241271	1.6394578E-02	52.78824

Instrument : CHAMBER 113
 Detector : 45-111B4
 Standard ID : AESS-001
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 12:00:36
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 4-APR-2006 17:02:58
 Average Efficiency : 0.3703099
 Average Efficiency Error : 1.0161426E-02
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.8400	28-FEB-2006	2991.835	3301.848	18597.00	0.3629034	1.5549773E-02	64.50990
NP-237	211.8600	28-FEB-2006	4433.613	4901.946	18886.00	0.3714283	1.8767057E-02	90.91785
CM-244	248.8200	28-FEB-2006	5530.358	5885.560	20134.00	0.3804419	1.9210188E-02	71.11305

Instrument : CHAMBER 114
 Detector : 45-111B5
 Standard ID : AESS-007
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 12:00:40
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 4-APR-2006 17:03:22
 Average Efficiency : 0.3901447
 Average Efficiency Error : 1.0698882E-02
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.5400	28-FEB-2006	2990.875	3299.211	19570.00	0.3824124	1.6373768E-02	64.95810
NP-237	211.5600	28-FEB-2006	4436.329	4903.130	20139.00	0.3966328	2.0027624E-02	80.48977
CM-244	248.5200	28-FEB-2006	5535.235	5884.346	20889.00	0.3951845	1.9947579E-02	69.68978

Instrument : CHAMBER 115
 Detector : 45-132EE5
 Standard ID : AESS-002
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 12:00:44
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 4-APR-2006 17:03:37
 Average Efficiency : 0.3799683
 Average Efficiency Error : 1.0422695E-02
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.4800	28-FEB-2006	2990.466	3300.287	19152.00	0.3743467	1.6033292E-02	67.16986
NP-237	211.5000	28-FEB-2006	4435.908	4903.427	19268.00	0.3795908	1.9175535E-02	85.64700
CM-244	248.4000	28-FEB-2006	5530.487	5884.796	20541.00	0.3887886	1.9627862E-02	69.09605

Instrument : CHAMBER 116
 Detector : 45-132FF2
 Standard ID : AESS-008
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 12:00:47
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 4-APR-2006 17:03:51
 Average Efficiency : 0.3906634
 Average Efficiency Error : 1.0711731E-02
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.8400	28-FEB-2006	2988.161	3302.097	19763.00	0.3856568	1.6510434E-02	61.93254
NP-237	211.8600	28-FEB-2006	4435.898	4903.366	20060.00	0.3945222	1.9921809E-02	83.61416
CM-244	248.8800	28-FEB-2006	5530.965	5885.878	20861.00	0.3940839	1.9892277E-02	67.87167

Instrument : CHAMBER 117
 Detector : 45-132FF3
 Standard ID : AESS-003
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 12:00:52
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 4-APR-2006 17:04:04
 Average Efficiency : 0.3838457
 Average Efficiency Error : 1.0529065E-02
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.3600	28-FEB-2006	2987.574	3297.481	19157.00	0.3746493	1.6046192E-02	69.46350
NP-237	211.3800	28-FEB-2006	4432.916	4905.417	19746.00	0.3892191	1.9657088E-02	87.03203
CM-244	248.2800	28-FEB-2006	5531.962	5885.886	20722.00	0.3924041	1.9808734E-02	73.89016

Instrument : CHAMBER 118
 Detector : 45-132FF4
 Standard ID : AESS-009
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 12:00:56
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 4-APR-2006 17:04:21
 Average Efficiency : 0.3946549
 Average Efficiency Error : 1.0820382E-02
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.6000	28-FEB-2006	2989.600	3298.996	19935.00	0.3894384	1.6670343E-02	63.05709
NP-237	211.6200	28-FEB-2006	4434.069	4901.807	20060.00	0.3949601	1.9943934E-02	82.03598
CM-244	248.5800	28-FEB-2006	5534.903	5884.430	21258.00	0.4020683	2.0291740E-02	65.29355

Instrument : CHAMBER 119
 Detector : 45-132FF5
 Standard ID : AESS-004
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 12:00:59
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 4-APR-2006 17:04:33
 Average Efficiency : 0.3958072
 Average Efficiency Error : 1.0851006E-02
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.1800	28-FEB-2006	2987.490	3300.068	20085.00	0.3931205	1.6826242E-02	64.97130
NP-237	211.2000	28-FEB-2006	4434.344	4905.254	20104.00	0.3966229	2.0027457E-02	79.50690
CM-244	248.1000	28-FEB-2006	5530.554	5884.197	21046.00	0.3988287	2.0130115E-02	68.84389

Instrument : CHAMBER 120
 Detector : 45-142F1
 Standard ID : AESS-010
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 12:01:03
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 4-APR-2006 17:05:08
 Average Efficiency : 0.3892356
 Average Efficiency Error : 1.0674394E-02
 Confidence : 95.00000

Cal. Isteps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.4800	28-FEB-2006	2991.710	3300.418	19511.00	0.3813637	1.6329555E-02	65.80540
NP-237	211.5000	28-FEB-2006	4437.274	4903.259	19969.00	0.3933960	1.9865829E-02	87.35593
CM-244	248.4600	28-FEB-2006	5533.634	5886.862	20972.00	0.3968505	2.0030931E-02	68.58372

Instrument : CHAMBER 121
 Detector : 45-142J4
 Standard ID : AESS-005
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 12:01:07
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 4-APR-2006 17:05:19
 Average Efficiency : 0.3879517
 Average Efficiency Error : 1.0639026E-02
 Confidence : 95.00000

Cal. Isteps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.6600	28-FEB-2006	2988.124	3301.600	19515.00	0.3811294	1.6319472E-02	66.81467
NP-237	211.6800	28-FEB-2006	4434.163	4906.581	19891.00	0.3915263	1.9772179E-02	83.76527
CM-244	248.6400	28-FEB-2006	5533.976	5883.453	20862.00	0.3944832	1.9912424E-02	67.69315

Instrument : CHAMBER 122
 Detector : 45-142J5
 Standard ID : AESS-011
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 12:01:10
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 4-APR-2006 17:05:33
 Average Efficiency : 0.3964319
 Average Efficiency Error : 1.0868002E-02
 Confidence : 95.00000

Cal. Isteps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.6600	28-FEB-2006	2990.061	3298.780	20106.00	0.3926716	1.6806791E-02	65.77823
NP-237	211.6800	28-FEB-2006	4436.620	4903.419	20147.00	0.3965701	2.0024376E-02	83.48605
CM-244	248.6400	28-FEB-2006	5535.258	5884.098	21247.00	0.4017632	2.0276442E-02	70.88770

Instrument : CHAMBER 123
 Detector : 45-142V1
 Standard ID : AESS-006
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 12:01:15
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 4-APR-2006 17:05:57
 Average Efficiency : 0.3805304
 Average Efficiency Error : 1.0439763E-02
 Confidence : 95.00000

Cal. Isteps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.1800	28-FEB-2006	2990.387	3299.522	18959.00	0.3710815	1.5895747E-02	68.66263
NP-237	211.2000	28-FEB-2006	4437.442	4903.641	19446.00	0.3836367	1.9378122E-02	86.99185
CM-244	248.1000	28-FEB-2006	5534.110	5887.297	20682.00	0.3919307	1.9785201E-02	66.84405

Instrument : CHAMBER 124
 Detector : 45-142V2
 Standard ID : AESS-012
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 12:01:18
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 4-APR-2006 17:06:12
 Average Efficiency : 0.3873872
 Average Efficiency Error : 1.0623961E-02
 Confidence : 95.00000

Cal. Isteps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.9600	28-FEB-2006	2989.443	3297.987	19472.00	0.3797709	1.6261807E-02	64.41782
NP-237	211.9200	28-FEB-2006	4435.559	4902.411	19887.00	0.3909993	1.9745609E-02	86.15575
CM-244	248.9400	28-FEB-2006	5534.467	5883.494	20923.00	0.3951599	1.9946033E-02	70.30408

Instrument : CHAMBER 125
 Detector : 45-142V3
 Standard ID : AESS-013
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 12:01:21
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 4-APR-2006 17:06:28
 Average Efficiency : 0.3867655
 Average Efficiency Error : 1.0609177E-02
 Confidence : 95.00000

Cal. Isteps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	220.5600	28-FEB-2006	2992.436	3301.693	19282.00	0.3750422	1.6061539E-02	55.83823
NP-237	212.5200	28-FEB-2006	4433.216	4903.410	20074.00	0.3935665	1.9873424E-02	88.64875
CM-244	249.6600	28-FEB-2006	5531.615	5883.226	21143.00	0.3981633	2.0095672E-02	68.92764

Instrument : CHAMBER 126
 Detector : 45-142V5
 Standard ID : AESS-019
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 12:01:25
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 4-APR-2006 17:06:44
 Average Efficiency : 0.3776715
 Average Efficiency Error : 1.0360188E-02
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.5400	28-FEB-2006	2988.369	3299.131	19021.00	0.3716846	1.5920833E-02	61.61137
NP-237	211.5600	28-FEB-2006	4435.618	4902.366	19293.00	0.3799706	1.9194474E-02	87.82700
CM-244	248.5200	28-FEB-2006	5532.732	5885.449	20309.00	0.3842119	1.9398922E-02	63.11655

Instrument : CHAMBER 127
 Detector : 45-142W1
 Standard ID : AESS-014
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 12:01:29
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 4-APR-2006 17:07:12
 Average Efficiency : 0.3934290
 Average Efficiency Error : 1.0787830E-02
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.9600	28-FEB-2006	2989.513	3302.392	19757.00	0.3853294	1.6496489E-02	64.47871
NP-237	211.9800	28-FEB-2006	4432.606	4903.961	20292.00	0.3988588	2.0138543E-02	84.68309
CM-244	249.0000	28-FEB-2006	5535.216	5883.874	21190.00	0.4001061	2.0193312E-02	70.60645

Instrument : CHAMBER 128
 Detector : 45-142W2
 Standard ID : AESS-020
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 12:01:34
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 4-APR-2006 17:07:27
 Average Efficiency : 0.3859246
 Average Efficiency Error : 1.0586893E-02
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.8400	28-FEB-2006	2989.584	3299.388	19162.00	0.3739288	1.6015276E-02	59.93734
NP-237	211.8000	28-FEB-2006	4434.590	4901.786	20058.00	0.3945944	1.9925477E-02	79.19832
CM-244	248.8200	28-FEB-2006	5533.622	5887.583	20951.00	0.3958796	1.9982109E-02	66.89229

Instrument : CHAMBER 129
 Detector : 45-142W3
 Standard ID : AESS-015
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 12:01:38
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 4-APR-2006 17:07:43
 Average Efficiency : 0.3895081
 Average Efficiency Error : 1.0681822E-02
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.8400	28-FEB-2006	2991.668	3299.558	19525.00	0.3810124	1.6314350E-02	61.82140
NP-237	211.8600	28-FEB-2006	4435.149	4901.376	20156.00	0.3964100	2.0016206E-02	81.45658
CM-244	248.8800	28-FEB-2006	5532.751	5886.867	20929.00	0.3953595	1.9956063E-02	71.15770

Instrument : CHAMBER 130
 Detector : 45-142W5
 Standard ID : AESS-021
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 12:01:42
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 4-APR-2006 17:07:58
 Average Efficiency : 0.3877107
 Average Efficiency Error : 1.0633443E-02
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.5400	28-FEB-2006	2990.831	3301.623	19394.00	0.3789733	1.6228566E-02	61.42154
NP-237	211.5600	28-FEB-2006	4435.787	4904.916	20099.00	0.3958496	1.9988457E-02	82.39708
CM-244	248.5200	28-FEB-2006	5534.223	5884.439	20760.00	0.3927440	1.9825550E-02	67.39270

Instrument : CHAMBER 131
 Detector : 45-145K1
 Standard ID : AESS-016
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 12:01:46
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 4-APR-2006 17:08:16
 Average Efficiency : 0.3897060
 Average Efficiency Error : 1.0686211E-02
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.6600	28-FEB-2006	2989.369	3298.448	19647.00	0.3837073	1.6428316E-02	64.42750
NP-237	211.6800	28-FEB-2006	4432.591	4905.330	20018.00	0.3940307	1.9897401E-02	82.42314
CM-244	248.6400	28-FEB-2006	5532.857	5887.665	20846.00	0.3941807	1.9897297E-02	71.83934

Instrument : CHAMBER 132
 Detector : 45-145K2
 Standard ID : AESS-022
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 12:01:49
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 4-APR-2006 17:08:32
 Average Efficiency : 0.3905833
 Average Efficiency Error : 1.0710652E-02
 Confidence : 95.00000

Cal. Isteps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.6600	28-FEB-2006	2990.018	3301.016	19613.00	0.3830433	1.6400279E-02	65.20789
NP-237	211.6800	28-FEB-2006	4434.219	4902.195	20056.00	0.3947787	1.9934803E-02	89.44299
CM-244	248.6400	28-FEB-2006	5534.644	5883.351	21028.00	0.3976221	2.0069377E-02	68.53607

Instrument : CHAMBER 133
 Detector : 45-145K3
 Standard ID : AESS-017
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 12:01:52
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 4-APR-2006 17:09:47
 Average Efficiency : 0.3868218
 Average Efficiency Error : 1.0608377E-02
 Confidence : 95.00000

Cal. Isteps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.7200	28-FEB-2006	2989.115	3302.033	19459.00	0.3799319	1.6268853E-02	67.58065
NP-237	211.7400	28-FEB-2006	4435.237	4904.688	19979.00	0.3931513	1.9853372E-02	78.76342
CM-244	248.7000	28-FEB-2006	5532.486	5884.151	20667.00	0.3907017	1.9723292E-02	68.61700

Instrument : CHAMBER 134
 Detector : 45-145K4
 Standard ID : AESS-023
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 12:01:56
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 4-APR-2006 17:11:02
 Average Efficiency : 0.3909511
 Average Efficiency Error : 1.0721575E-02
 Confidence : 95.00000

Cal. Isteps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.6600	28-FEB-2006	2987.530	3301.962	19533.00	0.3814809	1.6334314E-02	58.87649
NP-237	211.6800	28-FEB-2006	4434.547	4905.459	20169.00	0.3970030	2.0046022E-02	84.02620
CM-244	248.6400	28-FEB-2006	5534.869	5887.271	21114.00	0.3992483	2.0150691E-02	67.90365

Instrument : CHAMBER 135
 Detector : 45-145K5
 Standard ID : AESS-018
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 12:01:59
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 4-APR-2006 17:11:53
 Average Efficiency : 0.3932157
 Average Efficiency Error : 1.0781703E-02
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.7800	28-FEB-2006	2990.104	3298.632	19831.00	0.3870894	1.6570982E-02	66.57359
NP-237	211.8000	28-FEB-2006	4434.981	4906.088	20001.00	0.3934731	1.9869408E-02	92.58358
CM-244	248.7600	28-FEB-2006	5531.074	5884.261	21277.00	0.4021365	2.0295015E-02	73.11333

Instrument : CHAMBER 136
 Detector : 45-145L1
 Standard ID : AESS-024
 Standard Reference Date : 7-FEB-2003 00:00:00
 Calibration Analysis Date/Time : 4-APR-2006 12:02:04
 Calibration Count Time : 240.0000
 Efficiency Calibration Date/Time : 4-APR-2006 17:12:12
 Average Efficiency : 0.3798372
 Average Efficiency Error : 1.0422947E-02
 Confidence : 95.00000

Cal. Istps	DPM	Exp. Date	Start Engy	End Engy	Counts	EFF.	EFF Err	Resolution
GD-148	219.4200	28-FEB-2006	2988.496	3298.473	18764.00	0.3668631	1.5717393E-02	63.35145
NP-237	211.4400	28-FEB-2006	4437.582	4903.436	19751.00	0.3892161	1.9656880E-02	93.25786
CM-244	248.4000	28-FEB-2006	5532.704	5884.860	20649.00	0.3908328	1.9730078E-02	69.15901

General Engineering Laboratories, LLC

2040 Savage Road, Charleston, SC 29414
(803)556-8171

Gamma Spectrometer Geometry Calibration Package

Detector: Gamma 13

Geometry: Co

	YES	NO	Comments
1) Is all calibration standard information enclosed for: the primary standard certificate? the secondard standard(s) documentation? the nuclide library used? the VMS certificate file?	/		
	NA		
	/		
	/		
2) Is the detector efficiency curve printout included?		/	
3) Is the efficiency calibration report included and reviewed?	/		
4) Is the raw count data included for: the calibration peak report? the calibration verification PEAK report? the calibration verification NID report? the last instrument background?	/		
	/		
	/		
	/		
5) Are the calibration verification calculations included?	/		
6) Are the instrument settings included: amp, HVPS, ADC settings?	/		

Prepared By: [Signature]
Reviewed By: [Signature]

Date: 6/22/05
Date: 6/22/05

EFF: 6/22/05

General Engineering Laboratories, LLC

2040 Savage Road, Charleston, SC 29414
(803)556-8171

Gamma Spectrometer Front End Electronics Setup **Detector: Gamma 13**

Date Performed: 6/22/2005

Performed By: Kinsey Boehl

<p>High Voltage Power Supply</p> <p>Model No. <u>TC 950</u> High Voltage <u>3.00 KeV</u></p>	<p>Spectroscopy Amplifier</p> <p>Model No. <u>2026</u> Course Gain <u>50</u> Fine Gain <u>0.643</u> Time Constant <u>6us</u> Input polarity <u>Neg</u> BSLR rate <u>N/A</u> BSLR mode <u>N/A</u> Threshold <u>N/A</u></p>
<p>ADC</p> <p>Model No. <u>ND579</u> Gain <u>4K</u></p>	
<p>AIM Module</p> <p>Model No. <u>ND556</u> Address <u>NIC1:1</u></p>	

Gamma Spectroscopy Calibration Verification

Instrument: Gamma 13

Calibration Date: 6/22/2005

Geometry: CAN

Standard Id: 70530-278

Isotope		CALIBRATED ACTIVITY (PCI)	MEASURED ACTIVITY (PCI)	DIFFERENCE %
Am-241		6.2283E+04	6.206E+04	-0.36
Cd-109		8.2222E+05	8.060E+05	-1.97
Co-57		1.8996E+04	2.007E+04	5.65
Ce-139		2.8853E+04	2.820E+04	-2.26
Sn-113		4.8141E+04	4.847E+04	0.68
Cs-137		2.4217E+04	2.512E+04	3.73
Y-88	1836.06	8.5829E+04	8.662E+04	0.92
Co-60	1832.5	3.8655E+04	3.877E+04	0.30
Pb-210		8.1682E+05	8.833E+05	8.14

Prepared By: [Signature]

Date: 6/22/05

Reviewed By: [Signature]

Date: 6/21/05

Verified:

QA filename : DKA300:[CANBERRA.GAMMA]QC_BKG_GAMMA13.QAF;2


Sample ID : BKG_GAMMA13 Sample quantity : 1.80 LITER
Sample date : 17-JUN-2005 00:00:00 Acquisition date : 17-JUN-2005 13:51:45
Elapsed live time: 0 16:40:00.00 Elapsed real time: 0 16:40:06.98

Out-of-range Test: BOUNDARY

Parameter Description	Lower	Upper	Value	Flag
BACKGROUND (GROSS COUNTS)	1.86E+05	2.14E+05	1.92E+05	
BACKGROUND (CPS)	3.08	3.54	3.19	

Flags: "*" means the out-of-range test is parameter-dependent

Approved by:

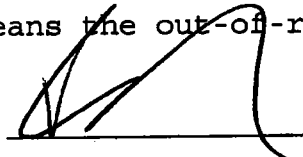

Approval Date:

6/20/05

 * GENERAL ENG. LABS, LLC. *
 * 2040 Savage Road *
 * Charleston, SC 29414 *

Configuration : DKA300:[CANBERRA.GAMMA.ARCHIVE.GAMMA]VER_GAMMA13_CAN.CNF;1
 Sample date : 1-APR-2005 12:00:00. Acquisition date : 20-JUN-2005 11:57:47
 Sample ID : VER_GAMMA13_CAN Sample quantity : 1.00000E+00 LITER
 Detector name : GAMMA13 Detector geometry: CAN
 Elapsed live time: 0 01:00:00.00 Elapsed real time: 0 01:01:46.67 2.9%
 Energy tolerance : 2.00000 KEV Analyst Initials : AKB
 Abundance limit : 75.00000 Sensitivity : 3.00000
 Batch ID : Detector SN# : 37-TN11260A
 Matrix Spike DPM : LCS DPM :

Pk	It	Energy	Area	Bkgnd	FWHM	Channel	Left	Pw	Cts/Sec	%Err	Fit
1	6	36.39	2783	8446	1.25	75.14	74	31	7.73E-01	3.7	1.45E+03
2	6	37.84	18612	58770	1.85	78.05	74	31	5.17E+00	2.2	
3	6	40.63	18755	91164	1.86	83.62	74	31	5.21E+00	3.3	
4	6	42.67	14388	65776	1.41	87.70	74	31	4.00E+00	3.3	
5	6	46.51*	291224	63194	1.38	95.40	74	31	8.09E+01	0.2	
6	6	49.31	9810	60706	1.59	100.99	74	31	2.73E+00	5.0	
7	0	59.60	203523	89035	1.15	121.58	115	14	5.65E+01	0.4	
8	7	66.77	6121	51907	2.10	135.90	131	24	1.70E+00	7.5	5.24E+00
9	7	68.76	5754	62281	2.11	139.89	131	24	1.60E+00	9.3	
10	7	70.80	9162	38851	1.32	143.97	131	24	2.55E+00	4.0	
11	7	72.85*	11278	34516	1.21	148.06	131	24	3.13E+00	3.0	
12	0	78.66*	663	30594	1.63	159.69	157	6	1.84E-01	41.9	
13	8	81.38	619	35702	1.15	165.14	162	26	1.72E-01	49.1	6.26E+02
14	8	82.73*	8116	65086	2.42	167.83	162	26	2.25E+00	6.3	
15	8	85.49*	10092	66260	2.38	173.35	162	26	2.80E+00	7.1	
16	8	88.05*	251500	28643	1.20	178.47	162	26	6.99E+01	0.2	
17	0	122.12	118333	41393	1.19	246.61	240	14	3.29E+01	0.5	
18	0	136.52*	13884	29268	1.18	275.41	270	12	3.86E+00	2.6	
19	0	165.89*	110255	32147	1.22	334.16	327	14	3.06E+01	0.5	
20	0	199.19*	4412	18983	1.44	400.75	396	11	1.23E+00	6.2	
21	0	203.88*	1130	13186	1.13	410.13	407	8	3.14E-01	17.9	
22	0	237.71*	488	11187	1.78	477.78	475	8	1.35E-01	37.9	
23	0	255.11	3100	12868	1.31	512.58	508	10	8.61E-01	7.1	
24	0	279.23*	77338	19722	1.32	560.82	553	16	2.15E+01	0.5	
25	0	300.16	269	7521	1.42	602.67	600	8	7.48E-02	56.1	
26	0	329.76	152	5892	1.05	661.85	659	7	4.22E-02	84.4	
27	0	391.72	77055	14956	1.45	785.75	778	16	2.14E+01	0.5	
28	0	510.86*	1768	8495	2.61	1023.97	1017	14	4.91E-01	11.3	
29	0	661.68*	54548	15066	1.72	1325.50	1316	20	1.52E+01	0.7	
30	0	701.75	209	4527	1.71	1405.61	1403	8	5.81E-02	56.3	
31	0	813.93*	1557	5852	2.32	1629.87	1623	15	4.33E-01	11.0	
32	0	898.03	93818	11753	1.87	1797.98	1788	20	2.61E+01	0.4	
33	0	1036.67	126	2387	1.19	2075.07	2073	7	3.51E-02	64.8	
34	0	1057.53	59	3009	1.30	2116.77	2113	9	1.64E-02	168.0	
35	0	1173.18*	60125	6828	2.13	2347.89	2336	24	1.67E+01	0.5	
36	5	1326.28	2286	3256	3.75	2653.84	2642	40	6.35E-01	8.4	4.00E+01
37	5	1332.50*	54024	2519	2.62	2666.27	2642	40	1.50E+01	0.5	
38	0	1356.32	62	906	1.39	2713.86	2712	6	1.73E-02	77.6	

Pk	It	Energy	Area	Bkgnd	FWHM	Channel	Left	Pw	Cts/Sec	%Err	Fit
39	0	1836.00	57861	2032	2.69	3672.16	3659	27	1.61E+01	0.5	
40	0	1966.22*	44	141	2.25	3932.28	3929	8	1.22E-02	49.7	
41	0	2032.54	41	345	8.17	4064.73	4054	20	1.14E-02	111.5	

Flag: "*" = Peak area was modified by background subtraction

VAX/VMS Nuclide Identification Report Generated

```
*****
*                                     General Eng. Labs, LLC.                               *
*                                     2040 Savage Road                                   *
*                                     Charleston, SC 29414                               *
*****
```

DETECTOR DATA

```
* Configuration      : DKA300:[CANBERRA.GAMMA.ARCHIVE.GAMMA]VER_GAMMA13_
* Acquisition date   : 20-JUN-2005 11:57:47 Detector SN#      : 37-TN11260
* Detector ID        : GAMMA13          Sensitivity           : 3.000
* Geometry           : CAN              Energy tolerance     : 2.000
* Elapsed live time  : 0 01:00:00.00   Abundance limit      : 75.000
* Elapsed real time  : 0 01:01:46.67   Half life ratio      : 8.000
*****
```

SAMPLE DATA

```
* Sample date       : 1-APR-2005 12:00:00 Nuclide Library :
* Sample ID         : VER_GAMMA13_CAN       Analyst initials  : AKB
* Batch Number      :                      Sample Quantity  : 1.0000E+00 LITER
* Recovery          : 1.00000              Carrier Weight    : 0.00000
*****
```

QC DATA

```
* Standard Weight   : 0.00000
* CALIB. DATE/TIME : 20-JUN-2005 11:56:42 MS Isotope      :
* MSD DPM           : 0.000              MSD Isotope       :
* LCS DPM           : 0.000              LCS Isotope       :
* LCSD DPM          : 0.000              LCSD Isotope      :
*****
```

Combined Activity-MDA Report

---- Identified Nuclides ----

Nuclide	Activity (pCi/LITER)	Act error	MDA (pCi/LITER)	
CO-57	2.007E+04	2.282E+03	1.048E+02	0.000E+00
CO-60	3.877E+04	2.187E+03	1.444E+02	0.000E+00
Y-88	8.662E+04	4.686E+03	2.130E+02	0.000E+00
CD-109	8.060E+05	7.920E+04	2.349E+03	0.000E+00
SN-113	4.847E+04	2.878E+03	2.434E+02	0.000E+00
CS-137	2.512E+04	2.165E+03	1.767E+02	0.000E+00
CE-139	2.820E+04	2.057E+03	1.416E+02	0.000E+00
HG-203	6.379E+04	4.820E+03	3.566E+02	0.000E+00
PB-210	8.833E+05	6.433E+04	2.856E+03	0.000E+00
AM-241	6.206E+04	4.332E+03	2.647E+02	0.000E+00

---- Non-Identified Nuclides ----

Nuclide	Key-Line Activity (pCi/LITER)	K.L. Act error) Ided	MDA (pCi/LITER)	
---------	--------------------------------------	--------------------------	---------------------	--

```

*****
*                                     GENERAL ENG. LABS, LLC.                               *
*                                     2040 Savage Road                               *
*                                     Charleston, SC 29414                          *
*****
Configuration      : DKA300:[CANBERRA.GAMMA.ARCHIVE.GAMMA]VER_GAMMA13_CAN.CNF;1
Sample date        : 1-APR-2005 12:00:00. Acquisition date : 20-JUN-2005 11:57:47
Sample ID          : VER_GAMMA13_CAN          Sample quantity  : 1.00000E+00 LITER
Detector name     : GAMMA13                 Detector geometry: CAN
Elapsed live time : 0 01:00:00.00          Elapsed real time: 0 01:01:46.67  2.9%
Energy tolerance  : 2.00000 KEV            Analyst Initials   : AKB
Abundance limit   : 75.00000              Sensitivity        : 3.00000
Batch ID          :                        Detector SN#       : 37-TN11260A
Matrix Spike DPM  :                        LCS DPM         :
*****

```

Nuclide Line Activity Report

Nuclide Type:

Nuclide	Energy	Area	%Abn	%Eff	Uncorrected pCi/LITER	Decay Corr pCi/LITER	2-Sigma %Error
CO-57	122.06	118333	85.51*	6.347E+00	1.637E+04	2.007E+04	11.37
	136.47	13884	10.47	6.046E+00	1.647E+04	2.019E+04	11.89
CO-60	1173.24	60125	99.90	1.192E+00	3.791E+04	3.902E+04	6.36
	1332.50	54024	99.98*	1.077E+00	3.767E+04	3.877E+04	5.64
Y-88	898.04	93818	93.40	1.487E+00	5.072E+04	8.533E+04	6.48
	1836.06	57861	99.38*	8.490E-01	5.149E+04	8.662E+04	5.41
CD-109	88.03	251500	3.79*	6.971E+00	7.147E+05	8.060E+05	9.83
SN-113	391.70	77055	64.90*	2.978E+00	2.994E+04	4.847E+04	5.94
CS-137	661.66	54548	85.12*	1.925E+00	2.499E+04	2.512E+04	8.62
CE-139	165.85	110255	80.35*	5.465E+00	1.885E+04	2.820E+04	7.29
HG-203	70.83	9162	4.75	7.051E+00	2.054E+04	6.752E+04	14.77
	72.87	11278	8.00	7.060E+00	1.499E+04	4.929E+04	13.46
	82.60	8116	3.55	7.027E+00	2.443E+04	8.031E+04	18.11
	279.20	77338	77.30*	3.872E+00	1.940E+04	6.379E+04	7.56
PB-210	46.50	291224	4.05*	6.154E+00	8.773E+05	8.833E+05	7.28
AM-241	59.54	203523	35.90*	6.861E+00	6.204E+04	6.206E+04	6.98

Flag: "*" = Keyline

Total number of lines in spectrum 41
 Number of unidentified lines 25
 Number of lines tentatively identified by NID 16 39.02%

Nuclide Type :

Nuclide	Hlife	Decay	Uncorrected pCi/LITER	Decay Corr pCi/LITER	Decay Corr 2-Sigma Error	2-Sigma %Error	Flags
CO-57	271.74D	1.23	1.637E+04	2.007E+04	0.228E+04	11.37	
CO-60	5.27Y	1.03	3.767E+04	3.877E+04	0.219E+04	5.64	
Y-88	106.63D	1.68	5.149E+04	8.662E+04	0.469E+04	5.41	
CD-109	461.40D	1.13	7.147E+05	8.060E+05	0.792E+05	9.83	
SN-113	115.09D	1.62	2.994E+04	4.847E+04	0.288E+04	5.94	
CS-137	30.00Y	1.01	2.499E+04	2.512E+04	0.217E+04	8.62	
CE-139	137.64D	1.50	1.885E+04	2.820E+04	0.206E+04	7.29	
HG-203	46.60D	3.29	1.940E+04	6.379E+04	0.482E+04	7.56	
PB-210	22.26Y	1.01	8.773E+05	8.833E+05	0.643E+05	7.28	
AM-241	432.20Y	1.00	6.204E+04	6.206E+04	0.433E+04	6.98	
Total Activity :			1.853E+06	2.062E+06			

Grand Total Activity : 1.853E+06 2.062E+06

Flags: "K" = Keyline not found
 "E" = Manually edited

"M" = Manually accepted
 "A" = Nuclide specific abn. limit

It	Energy	Area	Bkgnd	FWHM	Channel	Left	Pw	Cts/Sec	%Err	%Eff	Flags
6	36.39	2783	8446	1.25	75.14	74	31	7.73E-01	7.4	5.00E+00	
6	37.84	18612	58770	1.85	78.05	74	31	5.17E+00	4.5	5.21E+00	
6	40.63	18755	91164	1.86	83.62	74	31	5.21E+00	6.6	5.57E+00	
6	42.67	14388	65776	1.41	87.70	74	31	4.00E+00	6.7	5.79E+00	
6	49.31	9810	60706	1.59	100.99	74	31	2.73E+00	10.0	6.37E+00	
7	66.77	6121	51907	2.10	135.90	131	24	1.70E+00	14.9	7.01E+00	
7	68.76	5754	62281	2.11	139.89	131	24	1.60E+00	18.6	7.04E+00	
0	78.66	663	30594	1.63	159.69	157	6	1.84E-01	83.9	7.05E+00	
8	81.38	619	35702	1.15	165.14	162	26	1.72E-01	98.1	7.04E+00	
8	85.49	10092	66260	2.38	173.35	162	26	2.80E+00	14.1	7.00E+00	
0	199.19	4412	18983	1.44	400.75	396	11	1.23E+00	12.5	4.89E+00	
0	203.88	1130	13186	1.13	410.13	407	8	3.14E-01	35.7	4.82E+00	
0	237.71	488	11187	1.78	477.78	475	8	1.35E-01	75.8	4.35E+00	
0	255.11	3100	12868	1.31	512.58	508	10	8.61E-01	14.2	4.14E+00	
0	300.16	269	7521	1.42	602.67	600	8	7.48E-02	****	3.67E+00	
0	329.76	152	5892	1.05	661.85	659	7	4.22E-02	****	3.41E+00	
0	510.86	1768	8495	2.61	1023.97	1017	14	4.91E-01	22.7	2.39E+00	
0	701.75	209	4527	1.71	1405.61	1403	8	5.81E-02	****	1.83E+00	
0	813.93	1557	5852	2.32	1629.87	1623	15	4.33E-01	22.0	1.62E+00	
0	1036.67	126	2387	1.19	2075.07	2073	7	3.51E-02	****	1.32E+00	
0	1057.53	59	3009	1.30	2116.77	2113	9	1.64E-02	****	1.30E+00	
5	1326.28	2286	3256	3.75	2653.84	2642	40	6.35E-01	16.8	1.08E+00	
0	1356.32	62	906	1.39	2713.86	2712	6	1.73E-02	****	1.06E+00	
0	1966.22	44	141	2.25	3932.28	3929	8	1.22E-02	99.5	8.11E-01	
0	2032.54	41	345	8.17	4064.73	4054	20	1.14E-02	****	7.93E-01	

Flags: "T" = Tentatively associated

 * GENERAL ENG. LABS, LLC. *
 * 2040 Savage Road *
 * Charleston, SC 29414 *

DETECTOR DATA

* Configuration : DKA300:[CANBERRA.GAMMA.ARCHIVE.GAMMA]VER_GAMMA13_CAN.CNF;1*
 * Acquisition date : 20-JUN-2005 11:57:47 Detector SN# : 37-TN11260A *
 * Detector ID : GAMMA13 Sensitivity : 3.00000 *
 * Geometry : CAN Energy tolerance: 2.00000 *
 * Elapsed live time: 0 01:00:00.00 Abundance limit : 75.00000 *
 * Elapsed real time: 0 01:01:46.67 Half life ratio : 8.00000 *

SAMPLE DATA

* Sample date : 1-APR-2005 12:00:00. Nuclide Library : CAL *
 * Sample ID : VER_GAMMA13_CAN Analyst initials: AKB *
 * Batch Number : Sample Quantity : 1.00000E+00 LITER *

QC DATA

* CALIB. DATE/TIME : 20-JUN-2005 11:56:42.9MS Isotope : *
 * MSD DPM : MSD Isotope : *
 * LCS DPM : LCS Isotope : *

Combined Activity-MDA Report

---- Identified Nuclides ----

Nuclide	Activity (pCi/LITER)	Act error	MDA (pCi/LITER)	MDA error	Act/MDA
CO-57	2.007E+04	2.282E+03	1.048E+02	1.188E+01	191.531
CO-60	3.877E+04	2.187E+03	1.444E+02	8.024E+00	268.588
Y-88	8.662E+04	4.686E+03	2.130E+02	1.135E+01	406.596
CD-109	8.060E+05	7.920E+04	2.349E+03	2.306E+02	343.066
SN-113	4.847E+04	2.878E+03	2.434E+02	1.424E+01	199.110
CS-137	2.512E+04	2.165E+03	1.767E+02	1.503E+01	142.118
CE-139	2.820E+04	2.057E+03	1.416E+02	1.024E+01	199.174
HG-203	6.379E+04	4.820E+03	3.566E+02	2.667E+01	178.896
PB-210	8.833E+05	6.433E+04	2.856E+03	2.075E+02	309.321
AM-241	6.206E+04	4.332E+03	2.647E+02	1.836E+01	234.421

```

*****
*                               GENERAL ENG. LABS, LLC.                               *
*                               2040 Savage Road                                       *
*                               Charleston, SC 29414                                   *
*****
Configuration      : DKA300:[CANBERRA.GAMMA.ARCHIVE.GAMMA]CAL_GAMMA13_CAN.CNF;2
Sample date        : 1-APR-2005 12:00:00. Acquisition date : 20-JUN-2005 10:31:08
Sample ID          : CAL_GAMMA13_CAN          Sample quantity : 1.00000E+00 LITER
Detector name     : GAMMA13                 Detector geometry: CAN
Elapsed live time : 0 01:00:00.00          Elapsed real time: 0 01:01:46.29  2.9%
Energy tolerance  : 2.00000 KEV            Analyst Initials  : AKB
Abundance limit   : 75.00000              Sensitivity       : 3.00000
Batch ID          :                        Detector SN#    : 37-TN11260A
Matrix Spike DPM  :                        LCS DPM       :
*****

```

Pk	It	Energy	Area	Bkgnd	FWHM	Channel	Left	Pw	Cts/Sec	%Err	Fit
1	3	37.98	14226	66957	1.39	78.32	74	31	3.95E+00	3.3	1.01E+03
2	3	40.66	13900	66344	1.40	83.70	74	31	3.86E+00	3.4	
3	3	46.55*	270184	55457	1.18	95.46	74	31	7.51E+01	0.2	
4	0	59.62	203384	86985	1.16	121.61	115	14	5.65E+01	0.4	
5	10	67.51	10402	66137	2.93	137.39	131	24	2.89E+00	5.4	1.09E+01
6	10	70.87	11085	48443	1.70	144.12	131	24	3.08E+00	3.9	
7	10	72.88*	10648	34619	1.12	148.14	131	24	2.96E+00	3.1	
8	4	82.65*	5848	49936	1.71	167.67	162	30	1.62E+00	6.9	5.13E+02
9	4	84.86*	8784	48471	1.72	172.09	162	30	2.44E+00	4.7	
10	4	88.03*	250811	27618	1.23	178.44	162	30	6.97E+01	0.2	
11	0	98.52*	294	17314	0.91	199.42	197	6	8.17E-02	70.9	
12	0	122.14	117267	41659	1.20	246.65	240	14	3.26E+01	0.5	
13	0	136.50*	14278	28684	1.20	275.38	270	12	3.97E+00	2.5	
14	0	165.90*	110209	31714	1.22	334.16	327	14	3.06E+01	0.5	
15	0	199.08*	4349	17263	1.37	400.52	396	10	1.21E+00	5.9	
16	0	203.74*	1356	14612	2.02	409.85	406	9	3.77E-01	16.3	
17	0	255.05	3567	12417	1.31	512.46	508	10	9.91E-01	6.1	
18	0	279.21*	77702	19412	1.33	560.78	553	16	2.16E+01	0.5	
19	0	313.65	224	5932	1.83	629.65	627	7	6.21E-02	57.6	
20	0	381.04	360	6102	2.43	764.39	761	8	9.99E-02	38.0	
21	0	391.69	76049	14994	1.44	785.68	778	16	2.11E+01	0.5	
22	0	510.72*	1708	8588	3.46	1023.69	1017	14	4.75E-01	11.8	
23	0	661.59*	54080	14331	1.70	1325.33	1316	19	1.50E+01	0.7	
24	0	813.72*	1287	5129	2.24	1629.44	1623	13	3.57E-01	11.8	
25	0	876.55*	84	2974	1.30	1755.03	1751	7	2.33E-02	108.5	
26	0	897.94	94388	12282	1.91	1797.78	1787	22	2.62E+01	0.4	
27	0	918.50	106	4210	1.04	1838.89	1836	9	2.94E-02	111.2	
28	0	1015.43	103	2128	0.99	2032.62	2029	6	2.87E-02	71.4	
29	0	1173.10*	59829	6655	2.17	2347.73	2337	23	1.66E+01	0.5	
30	0	1227.66	195	1798	3.41	2456.77	2451	12	5.43E-02	44.0	
31	0	1232.68	77	1027	0.95	2466.79	2462	7	2.14E-02	70.0	
32	0	1270.94	94	1695	1.09	2543.26	2538	12	2.62E-02	87.8	
33	6	1325.83	2620	3105	4.12	2652.94	2643	39	7.28E-01	6.7	3.29E+01
34	6	1332.34*	53359	2360	2.55	2665.96	2643	39	1.48E+01	0.5	
35	0	1457.66	40	1260	1.37	2916.35	2913	8	1.11E-02	155.1	
36	0	1570.74*	104	2203	2.09	3142.28	3137	10	2.89E-02	85.1	
37	0	1597.33	177	2304	1.20	3195.40	3190	10	4.91E-02	51.5	
38	0	1718.78*	56	511	1.74	3438.02	3435	8	1.54E-02	72.0	

Pk	It	Energy	Area	Bkgnd	FWHM	Channel	Left	Pw	Cts/Sec	%Err	Fit
39	0	1723.78	139	897	5.46	3448.01	3442	15	3.87E-02	47.6	
40	0	1753.06	37	321	1.37	3506.51	3503	7	1.03E-02	82.0	
41	0	1835.79	57460	2307	2.70	3671.74	3659	28	1.60E+01	0.5	
42	0	1857.38	94	478	2.25	3714.88	3710	10	2.60E-02	45.1	
43	0	1993.41	29	113	0.98	3986.58	3984	6	8.18E-03	59.6	

Flag: "*" = Peak area was modified by background subtraction

Configuration : MCA0:[GAMMA]GAMMA13\$1
 Analyses by : CALIBRATE V1.7, PEAK V16.4
 Detector Name : GAMMA13 Energy Calib Time: 17-JUN-2005 12:54:40
 Efficiency type : Empirical Effncy Calib Time: 20-JUN-2005 11:56:42
 Detector Geometry: GAMMA13 Shelf :

Energy Calibration Report

$$\text{Energy} = -1.182 + 0.5000 * \text{Channel} + 9.1833\text{E-}08 * (\text{Channel} ** 2)$$

Nbr	Centroid Channel	True Energy	Computed Energy	Difference
1	95.32	46.50	46.48	0.023
2	121.43	59.54	59.53	0.007
3	178.42	88.03	88.02	0.011
4	246.57	122.06	122.10	-0.039
5	334.10	165.85	165.87	-0.013
6	785.72	391.70	391.70	0.000
7	1325.46	661.66	661.66	0.005
8	1797.97	898.04	898.03	0.015
9	2347.97	1173.24	1173.22	0.024
10	2666.35	1332.50	1332.54	-0.040
11	3672.28	1836.06	1836.06	0.008

FWHM Calibration Report

$$\text{FWHM} = 0.7849 + 4.2344\text{E-}02 * (\text{Energy} ** 1/2)$$

Nbr	Energy	True FWHM	Computed FWHM	Difference
1	46.50	1.30	1.07	0.225
2	59.54	1.14	1.11	0.032
3	88.03	1.26	1.18	0.077
4	122.06	1.19	1.25	-0.062
5	165.85	1.24	1.33	-0.088
6	391.70	1.46	1.62	-0.166
7	661.66	1.73	1.87	-0.145
8	898.04	1.92	2.05	-0.135
9	1173.24	2.15	2.24	-0.085
10	1332.50	2.58	2.33	0.250
11	1836.06	2.70	2.60	0.097

Efficiency Calibration Report

$$\text{Eff} = \exp(a2 + a3 * x + a4 * x ** 2 + a5 * x ** 3 + a6 * x ** 4 + a7 * x ** 5), \quad x = \ln(a1 / \text{energy})$$

a1 a2 a3 a4 a5 a6 a7
 941.3 -4.248 0.8364 4.2377E-02 -5.4519E-02 1.1469E-02 -3.6336E-03


Average Deviation = 1.62 % Reduced Chi-Square = 1.05

Nbr	Energy (KEV)	Measured Efficiency	Efficiency Error	Computed Efficiency	Diff/ Error	% Diff
-----	--------------	---------------------	------------------	---------------------	-------------	--------

1	46.50	6.17E-02	1.86E-03	6.15E-02	0.12	0.36
---	-------	----------	----------	----------	------	------

Nbr	Energy (KEV)	Measured Efficiency	Efficiency Error	Computed Efficiency	Diff/ /Error	% Diff
2	59.54	6.83E-02	2.07E-03	6.86E-02	-0.13	-0.40
3	88.03	6.81E-02	2.25E-03	6.97E-02	-0.71	-2.34
4	122.06	6.65E-02	2.02E-03	6.35E-02	1.47	4.48
5	165.85	5.34E-02	1.51E-03	5.47E-02	-0.84	-2.38
6	391.70	2.96E-02	7.84E-04	2.98E-02	-0.26	-0.68
7	661.66	1.98E-02	6.09E-04	1.93E-02	0.89	2.75
8	898.04	1.46E-02	3.85E-04	1.49E-02	-0.71	-1.88
9	1173.24	1.21E-02	3.33E-04	1.19E-02	0.51	1.40
10	1332.50	1.07E-02	2.82E-04	1.08E-02	-0.35	-0.94
11	1836.06	8.51E-03	2.25E-04	8.49E-03	0.07	0.19

Approved by: _____

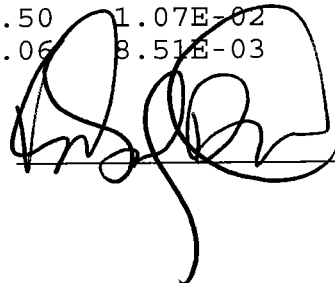

Approval Date: 6/20/05

for 6/20/05

```

Library Title      :
Library file name : DKA300:[CANBERRA.GAMMA]CAL.NLB;1
Date printed      : 6-DEC-2004 10:31:17.67
Number of nuclides : 10
Number of lines   : 17

```

Nuclide Name	Half-Life	Nuclide Type	Key Line	Energy	Abundance
CO-57	271.74D		*	122.06 keV	85.51 %
				136.47 keV	10.47 %
CO-60	5.27Y		*	1173.24 keV	99.90 %
				1332.50 keV	99.98 %
Y-88	106.63D		*	898.04 keV	93.40 %
				1836.06 keV	99.38 %
				88.03 keV	3.79 %
CD-109	461.40D		*	391.70 keV	64.90 %
SN-113	115.09D		*	661.66 keV	85.12 %
CS-137	30.00Y		*	165.85 keV	80.35 %
CE-139	137.64D		*	70.83 keV	4.75 %
				72.87 keV	8.00 %
				82.60 keV	3.55 %
				279.20 keV	77.30 %
HG-203	46.60D		*	46.50 keV	4.05 %
				59.54 keV	35.90 %
PB-210	22.26Y		*		
AM-241	432.20Y		*		

Print Time : 14-JUN-2005 17:43:24.41
 Certificate file name : DKA300:[CANBERRA.GAMMA]70530-278.CER;1
 Certificate title : CAN
 Certificate date : 1-APR-2005 12:00:00.00
 Certificate quantity : 1.00000E+00

Rcd	Nuclide	Halflife	CAL/ INIT	Energy	Rate	%Abun	Activity (uCi)
1	AM-241	432.20Y	Yes	59.54	8.2730E+02	35.90	6.2283E-02
2	CD-109	462.60D	No	88.03	1.1530E+03	3.79	8.2222E-01
3	Co-57	271.79D	No	122.06	6.0100E+02	85.51	1.8996E-02
4	CE-139	137.60D	No	165.85	8.5780E+02	80.35	2.8853E-02
5	SN-113	115.10D	No	391.70	1.1560E+03	64.90	4.8141E-02
6	CS-137	30.07Y	Yes	661.66	7.6270E+02	85.12	2.4217E-02
7	Y-88	106.60D	No	898.04	3.0220E+03	93.40	8.7447E-02
8	Y-88	106.60D	Yes	1836.06	3.1560E+03	99.38	8.5829E-02
9	Co-60	5.27Y	Yes	1173.24	1.4150E+03	99.90	3.8282E-02
10	CO-60	5.27Y	No	1332.50	1.4300E+03	99.98	3.8655E-02
11	PB-210	22.30Y	No	46.50	1.2240E+03	4.05	8.1682E-01





CERTIFICATE OF CALIBRATION
Standard Radionuclide Source

70530-278

100 mL Solid in 100 mL Aluminum Can

This standard radionuclide source was prepared using aliquots measured gravimetrically from master radionuclide solution sources. The Am-241 and Pb-210 were calibrated by 4 pi alpha liquid scintillation counting. All other radionuclides were calibrated using a germanium gamma spectrometer system. Calibration and purity were checked using a germanium gamma spectrometer system. At the time of calibration no interfering gamma-ray emitting impurities were detected. The gamma ray emission rates for the most intense gamma-ray lines are given. Analytical maintains traceability to the National Institute of Standards and Technology through a Measurements Assurance Program as described in US NRC Regulatory Guide 4.15, Revision 1, February 1979.

US Patent 4,430,258; UK Patent GB2,149,194B; CA Patent 1,196,776.
Density of solid matrix 1.15 g/cc.

Calibration Date: April 1, 2005 12:00 EST

ISOTOPE	GAMMA ENERGY	HALF-LIFE	GAMMA-RAYS PER SECOND	TOTAL UNCERTAINTY %
Pb-210	46.5	22.3 y	1224	3.0
Am-241	59.5	432.2 y	827.3	3.0
Cd-109	88	462.6 d	1153	3.3
Co-57	122	271.79 d	601.0	3.0
Ce-139	166	137.6 d	857.8	2.8
Hg-203	279	46.61 d	1856	2.7
Sn-113	392	115.1 d	1156	2.6
Cs-137	662	30.07 y	762.7	3.0
Y-88	898	106.6 d	3022	2.6
Co-60	1173	5.271 y	1415	2.7
Co-60	1332	5.271 y	1430	2.6
Y-88	1836	106.6 d	3156	2.6

P O NUMBER 2832RD, Item 3

SOURCE PREPARED BY: M. Dimitrova
M. Dimitrova, Radiochemist

Q A APPROVED: M. M. 5-12-05

This standard will expire one year after the calibration date.

General Engineering Laboratories, LLC

2040 Savage Road, Charleston, SC 29414
(843)556-8171

Gamma Spectrometer Geometry Calibration Package

Detector: GAMMA 16

Geometry: CAN

	YES	NO	Comments
1) Is all calibration standard information enclosed for: the primary standard certificate? the second standard(s) documentation? the nuclide library used? the VMS certificate file?	<input checked="" type="checkbox"/>		
			N/A
	<input checked="" type="checkbox"/>		
	<input checked="" type="checkbox"/>		
2) Is the detector efficiency curve printout included?		<input checked="" type="checkbox"/>	
3) Is the efficiency calibration report included and reviewed?	<input checked="" type="checkbox"/>		
4) Is the raw count data included for: the calibration peak report? the calibration verification PEAK report? the calibration verification NID report? the last instrument background?	<input checked="" type="checkbox"/>		
	<input checked="" type="checkbox"/>		
	<input checked="" type="checkbox"/>		
	<input checked="" type="checkbox"/>		
5) Are the calibration verification calculations included?	<input checked="" type="checkbox"/>		
6) Are the instrument settings included: amp, HVPS, ADC settings?	<input checked="" type="checkbox"/>		

Prepared By: Michael Hinton

Date: 4/5/06

Reviewed By: Th J Austin

Date: 4/6/2006

Effective Date: 3/22/06



CERTIFICATE OF CALIBRATION
Standard Radionuclide Source

70530-278

100 mL Solid in 100 mL Aluminum Can

This standard radionuclide source was prepared using aliquots measured gravimetrically from master radionuclide solution sources. The Am-241 and Pb-210 were calibrated by 4 pi alpha liquid scintillation counting. All other radionuclides were calibrated using a germanium gamma spectrometer system. Calibration and purity were checked using a germanium gamma spectrometer system. At the time of calibration no interfering gamma-ray emitting impurities were detected. The gamma ray emission rates for the most intense gamma-ray lines are given. Analytical maintains traceability to the National Institute of Standards and Technology through a Measurements Assurance Program as described in US NRC Regulatory Guide 4.15, Revision 1, February 1979.

US Patent 4,430,258; UK Patent GB2,149,194B; CA Patent 1,196,776.
Density of solid matrix 1.15 g/cc.

Calibration Date: April 1, 2005 12:00 EST

ISOTOPE	GAMMA ENERGY	HALF-LIFE		GAMMA-RAYS PER SECOND	TOTAL UNCERTAINTY %
Pb-210	46.5	22.3	Y	1224	3.0
Am-241	59.5	432.2	Y	827.3	3.0
Cd-109	88	462.6	d	1153	3.3
Co-57	122	271.79	d	601.0	3.0
Ce-139	166	137.6	d	857.8	2.8
Hg-203	279	46.61	d	1856	2.7
Sn-113	392	115.1	d	1156	2.6
Cs-137	662	30.07	Y	762.7	3.0
Y-88	898	106.6	d	3022	2.6
Co-60	1173	5.271	Y	1415	2.7
Co-60	1332	5.271	Y	1430	2.6
Y-88	1836	106.6	d	3156	2.6

P O NUMBER 2832RD, Item 3

SOURCE PREPARED BY:

M. Dimitrova
M. Dimitrova, Radiochemist

Q A APPROVED:

SM. mfg 5-12-05

This standard will expire one year after the calibration date.

Library Title :
 Library file name : DKA300:[CANBERRA.GAMMA]CAL.NLB;1
 Date printed : 8-JUL-2005 17:13:45.13
 Number of nuclides : 10
 Number of lines : 17

Nuclide		Nuclide	Key	Energy		Abundance
Name	Half-Life	Type	Line			
CO-57	271.74D		*	122.06	keV	85.51 %
				136.47	keV	10.47 %
CO-60	5.27Y		*	1173.24	keV	99.90 %
				1332.50	keV	99.98 %
Y-88	106.63D		*	898.04	keV	93.40 %
				1836.06	keV	99.38 %
CD-109	461.40D		*	88.03	keV	3.79 %
SN-113	115.09D		*	391.70	keV	64.90 %
CS-137	30.00Y		*	661.66	keV	85.12 %
CE-139	137.64D		*	165.85	keV	80.35 %
HG-203	46.60D			70.83	keV	4.75 %
				72.87	keV	8.00 %
				82.60	keV	3.55 %
				279.20	keV	77.30 %
PB-210	22.26Y		*	46.50	keV	4.05 %
AM-241	432.20Y		*	59.54	keV	35.90 %

Print Time : 14-JUN-2005 17:43:24.41
 Certificate file name : DKA300:[CANBERRA.GAMMA]70530-278.CER;1
 Certificate title : CAN
 Certificate date : 1-APR-2005 12:00:00.00
 Certificate quantity : 1.00000E+00

Rcd	Nuclide	Halflife	CAL/ INIT	Energy	Rate	%Abun	Activity (uCi)
1	AM-241	432.20Y	Yes	59.54	8.2730E+02	35.90	6.2283E-02
2	CD-109	462.60D	No	88.03	1.1530E+03	3.79	8.2222E-01
3	Co-57	271.79D	No	122.06	6.0100E+02	85.51	1.8996E-02
4	CE-139	137.60D	No	165.85	8.5780E+02	80.35	2.8853E-02
5	SN-113	115.10D	No	391.70	1.1560E+03	64.90	4.8141E-02
6	CS-137	30.07Y	Yes	661.66	7.6270E+02	85.12	2.4217E-02
7	Y-88	106.60D	No	898.04	3.0220E+03	93.40	8.7447E-02
8	Y-88	106.60D	Yes	1836.06	3.1560E+03	99.38	8.5829E-02
9	Co-60	5.27Y	Yes	1173.24	1.4150E+03	99.90	3.8282E-02
10	CO-60	5.27Y	No	1332.50	1.4300E+03	99.98	3.8655E-02
11	PB-210	22.30Y	No	46.50	1.2240E+03	4.05	8.1682E-01

Configuration : MCA0:[GAMMA]GAMMA16\$1
 Analyses by : CALIBRATE V1.7,PEAK V16.4,ENBACK V1.5
 Detector Name : GAMMA16 Energy Calib Time: 16-MAR-2006 18:45:26
 Efficiency type : Empirical Effncy Calib Time: 5-APR-2006 19:34:04
 Detector Geometry: GAMMA16 Shelf :

Energy Calibration Report

$$\text{Energy} = 0.6806 + 0.5005 * \text{Channel} + -1.4110\text{E-}07 * (\text{Channel} ** 2)$$

Nbr	Centroid Channel	True Energy	Computed Energy	Difference
1	91.61	46.50	46.52	-0.024
2	117.43	59.54	59.44	0.092
3	174.63	88.03	88.07	-0.039
4	242.39	122.06	121.98	0.086
5	330.14	165.85	165.88	-0.032
6	781.66	391.70	391.78	-0.077
7	1321.43	661.66	661.75	-0.087
8	1794.10	898.04	898.09	-0.046
9	2344.40	1173.24	1173.17	0.070
10	2662.97	1332.50	1332.37	0.126
11	3671.38	1836.06	1836.13	-0.069

FWHM Calibration Report

$$\text{FWHM} = 0.7322 + 3.5683\text{E-}02 * (\text{Energy} ** 1/2)$$

Nbr	Energy	True FWHM	Computed FWHM	Difference
1	46.50	1.10	0.98	0.123
2	59.54	1.11	1.01	0.100
3	88.03	1.11	1.07	0.039
4	122.06	1.05	1.13	-0.077
5	165.85	1.13	1.19	-0.060
6	391.70	1.32	1.44	-0.119
7	661.66	1.54	1.65	-0.108
8	898.04	1.71	1.80	-0.087
9	1173.24	1.90	1.95	-0.056
10	1332.50	2.22	2.03	0.190
11	1836.06	2.32	2.26	0.056

Efficiency Calibration Report

$$\text{Eff} = \exp(a2 + a3 * x + a4 * x ** 2 + a5 * x ** 3 + a6 * x ** 4 + a7 * x ** 5), \quad x = \ln(a1 / \text{energy})$$

a1 a2 a3 a a5 a6 a7
 941.3 -4.125 0.9352 -8.5206E-02 -0.2798 0.2907 -8.1774E-02

Average Deviation = 2.55 % Reduced Chi-Square = 2.12

Nbr	Energy (KEV)	Measured Efficiency	Efficiency Error	Computed Efficiency	Diff/ Error	% Diff
-----	--------------	---------------------	------------------	---------------------	-------------	--------

1	46.50	2.32E-03	8.34E-05	2.39E-03	-0.91	-3.27
---	-------	----------	----------	----------	-------	-------

Nbr	Energy (KEV)	Measured Efficiency	Efficiency Error	Computed Efficiency	Diff/ /Error	% Diff
2	59.54	1.42E-02	4.36E-04	1.35E-02	1.76	5.40
3	88.03	4.52E-02	1.50E-03	4.72E-02	-1.33	-4.42
4	122.06	5.92E-02	1.80E-03	6.07E-02	-0.84	-2.55
5	165.85	5.83E-02	1.68E-03	5.66E-02	0.98	2.82
6	391.70	3.26E-02	9.08E-04	3.24E-02	0.22	0.61
7	661.66	2.21E-02	6.69E-04	2.20E-02	0.15	0.46
8	898.04	1.62E-02	4.46E-04	1.69E-02	-1.47	-4.04
9	1173.24	1.34E-02	3.65E-04	1.31E-02	0.72	1.95
10	1332.50	1.19E-02	3.13E-04	1.17E-02	0.61	1.59
11	1836.06	9.61E-03	2.60E-04	9.70E-03	-0.34	-0.93

Approved by: *Mahmud Sultan*

Approval Date: 4 / 5 / 06

 * GENERAL ENG. LABS, LLC. *
 * 2040 Savage Road *
 * Charleston, SC 29414 *

Configuration : DKA300:[CANBERRA.GAMMA.ARCHIVE.GAMMA]CAL_GAMMA16_CAN.CNF;1
 Sample date : 1-APR-2005 12:00:00. Acquisition date : 22-MAR-2006 05:47:44
 Sample ID : CAL_GAMMA16_CAN Sample quantity : 1.00000E+00 LITER
 Detector name : GAMMA16 Detector geometry: 2L_MB
 Elapsed live time: 0 02:00:00.00 Elapsed real time: 0 02:01:11.57 1.0%
 Energy tolerance : 2.00000 KEV Analyst Initials : MJH1
 Abundance limit : 75.00000 Sensitivity : 3.00000
 Batch ID : Detector SN# : 1922864
 Matrix Spike DPM : LCS DPM :

Pk	It	Energy	Area	Bkgnd	FWHM	Channel	Left	Pw	Cts/Sec	%Err	Fit
1	0	46.36*	19828	35947	1.10	91.28	86	11	2.75E+00	2.0	
2	0	59.46*	84725	44271	1.12	117.45	111	13	1.18E+01	0.6	
3	0	66.70*	372	19791	0.84	131.92	130	6	5.17E-02	59.8	
4	0	88.03	220337	54455	1.12	174.54	168	14	3.06E+01	0.3	
5	0	102.87*	421	14597	0.62	204.21	202	6	5.85E-02	45.7	
6	0	122.06*	103595	32707	1.13	242.56	236	14	1.44E+01	0.5	
7	0	136.46	12668	18212	1.12	271.33	267	10	1.76E+00	2.2	
8	0	165.86	60247	22999	1.14	330.08	323	14	8.37E+00	0.7	
9	0	194.99	314	8684	1.62	388.30	386	6	4.36E-02	47.3	
10	0	198.38*	315	8583	1.71	395.09	393	6	4.37E-02	46.9	
11	0	255.20*	1285	10182	1.17	508.64	506	8	1.78E-01	13.9	
12	0	279.21	2423	10411	1.21	556.65	553	9	3.36E-01	7.9	
13	0	367.79	244	6774	1.39	733.71	731	7	3.38E-02	56.3	
14	0	391.66*	32015	14974	1.31	781.42	774	15	4.45E+00	1.0	
15	0	511.05*	561	6489	3.07	1020.11	1016	9	7.79E-02	26.4	
16	0	661.58*	118936	12322	1.52	1321.09	1312	18	1.65E+01	0.4	
17	0	683.72	197	4393	1.20	1365.37	1362	8	2.73E-02	58.9	
18	0	813.55	402	4936	1.63	1625.00	1622	9	5.58E-02	31.9	
19	0	835.59	98	4442	0.51	1669.10	1667	8	1.36E-02	118.7	
20	0	897.89	35146	11702	1.66	1793.69	1785	18	4.88E+00	0.9	
21	0	940.22	134	3492	0.96	1878.38	1877	5	1.86E-02	66.7	
22	0	1151.03	103	2374	1.62	2300.10	2298	8	1.43E-02	82.7	
23	0	1172.96	120184	6723	1.86	2343.98	2334	20	1.67E+01	0.3	
24	0	1302.66	84	1532	4.86	2603.50	2600	15	1.17E-02	101.5	
25	1	1325.10	598	1599	2.23	2648.41	2638	46	8.31E-02	14.3	5.08E+01
26	1	1332.09*	108135	1401	2.11	2662.41	2638	46	1.50E+01	0.3	
27	0	1459.87*	63	738	2.23	2918.14	2911	10	8.69E-03	82.6	
28	0	1761.02	104	354	4.95	3520.97	3516	14	1.45E-02	39.4	
29	1	1808.14*	86	337	2.47	3615.32	3609	15	1.19E-02	45.6	2.47E+00
30	1	1810.70*	62	181	2.03	3620.45	3609	15	8.59E-03	41.5	
31	0	1835.77	21735	799	2.31	3670.66	3659	25	3.02E+00	0.8	
32	0	1938.46	50	197	3.50	3876.28	3872	11	6.95E-03	56.0	
33	0	1951.96*	27	162	2.53	3903.32	3901	8	3.74E-03	84.2	

Flag: "*" = Peak area was modified by background subtraction

```

*****
*                               GENERAL ENG. LABS, LLC.                               *
*                               2040 Savage Road                                   *
*                               Charleston, SC 29414                               *
*****
Configuration      : DKA300:[CANBERRA.GAMMA.ARCHIVE.GAMMA]VER_GAMMA16_CAN.CNF;1
Sample date        : 1-APR-2005 12:00:00. Acquisition date : 22-MAR-2006 08:28:37
Sample ID          : VER_GAMMA16_CAN      Sample quantity   : 1.00000E+00 LITER
Detector name      : GAMMA16             Detector geometry:  CAN
Elapsed live time  : 0 02:00:00.00       Elapsed real time: 0 02:01:11.69  1.0%
Energy tolerance   : 2.00000 KEV         Analyst Initials  : MJH1
Abundance limit   : 75.00000            Sensitivity       : 3.00000
Batch ID          :                      Detector SN#      : 1922864
Matrix Spike DPM  :                      LCS DPM         :
*****

```

Pk	It	Energy	Area	Bkgnd	FWHM	Channel	Left	Pw	Cts/Sec	%Err	Fit
1	0	46.39*	19766	29516	1.08	91.34	87	9	2.75E+00	1.7	
2	0	59.49*	84360	43432	1.11	117.51	112	13	1.17E+01	0.6	
3	0	65.64*	283	15476	1.03	129.81	128	5	3.93E-02	65.9	
4	0	67.95*	260	17276	1.20	134.42	133	5	3.61E-02	75.9	
5	0	88.03	218470	50747	1.12	174.55	169	13	3.03E+01	0.3	
6	0	102.37*	175	12102	1.31	203.21	202	5	2.44E-02	94.4	
7	0	122.06*	103554	33091	1.14	242.56	236	14	1.44E+01	0.5	
8	0	136.46	12388	18242	1.10	271.34	267	10	1.72E+00	2.2	
9	0	165.87	59667	21967	1.13	330.11	324	13	8.29E+00	0.7	
10	0	214.63	198	7817	0.63	427.56	426	5	2.75E-02	67.4	
11	0	255.06*	1423	11624	1.32	508.36	504	9	1.98E-01	13.9	
12	0	279.10	2310	10580	1.31	556.42	552	9	3.21E-01	8.3	
13	0	310.72	217	7410	1.41	619.63	617	7	3.02E-02	66.0	
14	0	391.73*	32540	13768	1.31	781.56	776	14	4.52E+00	0.9	
15	0	444.62*	214	5644	1.54	887.30	885	6	2.97E-02	56.0	
16	0	510.88*	630	8712	2.91	1019.78	1014	12	8.76E-02	30.0	
17	0	603.63*	204	3438	1.75	1205.22	1203	6	2.84E-02	46.1	
18	0	610.37*	67	4196	1.33	1218.70	1217	7	9.30E-03	161.2	
19	0	661.65*	119483	12267	1.53	1321.24	1312	18	1.66E+01	0.4	
20	0	772.08	148	3436	0.91	1542.08	1540	7	2.05E-02	66.4	
21	0	814.16	321	4978	1.55	1626.24	1623	9	4.45E-02	40.1	
22	0	897.99	34326	11689	1.72	1793.89	1786	17	4.77E+00	0.9	
23	0	936.84*	85	5672	1.43	1871.60	1870	8	1.18E-02	154.1	
24	0	950.16*	79	5860	1.37	1898.25	1895	8	1.10E-02	167.7	
25	0	958.16*	103	5782	1.36	1914.25	1910	8	1.42E-02	128.9	
26	0	1036.88	70	3495	1.20	2071.72	2069	7	9.72E-03	140.5	
27	0	1110.97*	77	2459	0.89	2219.96	2218	5	1.06E-02	97.8	
28	0	1120.83*	146	2590	1.73	2239.69	2237	7	2.03E-02	58.5	
29	0	1173.10	120543	6551	1.88	2344.26	2334	20	1.67E+01	0.3	
30	6	1325.96	1292	2409	3.60	2650.13	2639	39	1.79E-01	12.6	5.30E+01
31	6	1332.31*	109158	1304	2.17	2662.84	2639	39	1.52E+01	0.3	
32	0	1526.89	66	565	1.79	3052.27	3050	7	9.22E-03	60.5	
33	0	1552.16*	46	587	0.71	3102.86	3099	7	6.34E-03	89.3	
34	0	1687.25	94	368	2.62	3373.30	3370	8	1.30E-02	36.8	
35	0	1706.74	93	576	3.57	3412.30	3406	14	1.29E-02	55.8	
36	0	1765.06*	28	136	0.98	3529.08	3527	5	3.95E-03	65.5	
37	0	1771.14*	59	283	2.41	3541.25	3536	10	8.24E-03	55.0	
38	0	1792.79*	20	196	1.32	3584.59	3581	7	2.72E-03	121.2	

Pk	It	Energy	Area	Bkgnd	FWHM	Channel	Left	Pw	Cts/Sec	%Err	Fit
39	0	1835.99	21386	851	2.27	3671.08	3661	22	2.97E+00	0.8	
40	4	1992.72*	46	117	1.91	3984.95	3981	15	6.37E-03	41.7	2.31E+00
41	4	1996.33	54	122	2.28	3992.16	3981	15	7.55E-03	38.2	

Flag: "*" = Peak area was modified by background subtraction

VAX/VMS Nuclide Identification Report Generated

 * General Eng. Labs, LLC. *
 * 2040 Savage Road *
 * Charleston, SC 29414 *

DETECTOR DATA

* Configuration : DKA300:[CANBERRA.GAMMA.ARCHIVE.GAMMA]VER_GAMMA16_ *
 * Acquisition date : 22-MAR-2006 08:28:37 Detector SN# : 1922864 *
 * Detector ID : GAMMA16 Sensitivity : 3.000 *
 * Geometry : CAN Energy tolerance: 2.000 *
 * Elapsed live time: 0 02:00:00.00 Abundance limit : 75.000 *
 * Elapsed real time: 0 02:01:11.69 Half life ratio : 8.000 *

SAMPLE DATA

* Sample date : 1-APR-2005 12:00:00 Nuclide Library : *
 * Sample ID : VER_GAMMA16_CAN Analyst initials: MJH1 *
 * Batch Number : Sample Quantity : 1.0000E+00 LITER *
 * Recovery : 1.00000 Carrier Weight : 0.00000 *

QC DATA

* Standard Weight : 0.00000 *
 * CALIB. DATE/TIME : 5-APR-2006 19:34:04 MS Isotope : *
 * MSD DPM : 0.000 MSD Isotope : *
 * LCS DPM : 0.000 LCS Isotope : *
 * LCSD DPM : 0.000 LCSD Isotope : *

Combined Activity-MDA Report

---- Identified Nuclides ----

Nuclide	Activity (pCi/LITER)	Act error	MDA (pCi/LITER)	
CO-57	1.852E+04	1.448E+03	9.493E+01	0.000E+00
CO-60	3.965E+04	2.480E+03	5.609E+01	0.000E+00
Y-88	8.368E+04	4.934E+03	3.796E+02	0.000E+00
CD-109	7.820E+05	9.456E+04	2.400E+03	0.000E+00
SN-113	4.927E+04	3.209E+03	5.930E+02	0.000E+00
CS-137	2.444E+04	1.517E+03	6.997E+01	0.000E+00
CE-139	2.941E+04	2.472E+03	2.269E+02	0.000E+00
HG-203	5.395E+04	1.002E+04	9.723E+03	0.000E+00
PB-210	8.052E+05	8.949E+04	2.365E+04	0.000E+00
AM-241	6.584E+04	8.964E+03	4.690E+02	0.000E+00

---- Non-Identified Nuclides ----

Nuclide	Key-Line Activity (pCi/LITER)	K.L. Act error) Ided	MDA (pCi/LITER)
---------	--------------------------------------	--------------------------	---------------------

```

*****
*                               GENERAL ENG. LABS, LLC.                               *
*                               2040 Savage Road                                       *
*                               Charleston, SC 29414                                   *
*****
Configuration      : DKA300:[CANBERRA.GAMMA.ARCHIVE.GAMMA]VER_GAMMA16_CAN.CNF;1
Sample date        : 1-APR-2005 12:00:00. Acquisition date : 22-MAR-2006 08:28:37
Sample ID          : VER_GAMMA16_CAN          Sample quantity : 1.00000E+00 LITER
Detector name     : GAMMA16                  Detector geometry: CAN
Elapsed live time : 0 02:00:00.00           Elapsed real time: 0 02:01:11.69  1.0%
Energy tolerance  : 2.00000 KEV             Analyst Initials  : MJH1
Abundance limit   : 75.00000                Sensitivity       : 3.00000
Batch ID          :                          Detector SN#     : 1922864
Matrix Spike DPM  :                          LCS DPM      :
*****

```

Nuclide Line Activity Report

Nuclide Type:

Nuclide	Energy	Area	%Abn	%Eff	Uncorrected pCi/LITER	Decay Corr pCi/LITER	2-Sigma %Error
CO-57	122.06	103554	85.51*	6.068E+00	7.492E+03	1.852E+04	7.82
	136.47	12388	10.47	6.049E+00	7.343E+03	1.816E+04	9.60
CO-60	1173.24	120543	99.90	1.314E+00	3.446E+04	3.916E+04	6.86
	1332.50	109158	99.98*	1.175E+00	3.489E+04	3.965E+04	6.26
Y-88	898.04	34326	93.40	1.688E+00	8.173E+03	8.209E+04	9.61
	1836.06	21386	99.38*	9.696E-01	8.331E+03	8.368E+04	5.90
CD-109	88.03	218470	3.79*	4.716E+00	4.589E+05	7.820E+05	12.09
SN-113	391.70	32540	64.90*	3.238E+00	5.812E+03	4.927E+04	6.51
CS-137	661.66	119483	85.12*	2.205E+00	2.390E+04	2.444E+04	6.21
CE-139	165.85	59667	80.35*	5.662E+00	4.923E+03	2.941E+04	8.41
HG-203	70.83	-----	4.75	2.802E+00	-----	Line Not Found	-----
	72.87	-----	8.00	3.066E+00	-----	Line Not Found	-----
	82.60	-----	3.55	4.202E+00	-----	Line Not Found	-----
	279.20	2310	77.30*	4.079E+00	2.751E+02	5.395E+04	18.58
PB-210	46.50	19766	4.05*	2.345E-01	7.812E+05	8.052E+05	11.11
AM-241	59.54	84360	35.90*	1.342E+00	6.574E+04	6.584E+04	13.61

Flag: "*" = Keyline

Total number of lines in spectrum 41
 Number of unidentified lines 28
 Number of lines tentatively identified by NID 13 31.71%

Nuclide Type :

Nuclide	Hlife	Decay	Uncorrected pCi/LITER	Decay Corr pCi/LITER	Decay Corr 2-Sigma Error	2-Sigma %Error	Flags
CO-57	271.74D	2.47	7.492E+03	1.852E+04	0.145E+04	7.82	
CO-60	5.27Y	1.14	3.489E+04	3.965E+04	0.248E+04	6.26	
Y-88	106.63D	10.0	8.331E+03	8.368E+04	0.493E+04	5.90	
CD-109	461.40D	1.70	4.589E+05	7.820E+05	0.946E+05	12.09	
SN-113	115.09D	8.48	5.812E+03	4.927E+04	0.321E+04	6.51	
CS-137	30.00Y	1.02	2.390E+04	2.444E+04	0.152E+04	6.21	
CE-139	137.64D	5.97	4.923E+03	2.941E+04	0.247E+04	8.41	
HG-203	46.60D	196.	2.751E+02	5.395E+04	1.002E+04	18.58	
PB-210	22.26Y	1.03	7.812E+05	8.052E+05	0.895E+05	11.11	
AM-241	432.20Y	1.00	6.574E+04	6.584E+04	0.896E+04	13.61	
Total Activity :			1.391E+06	1.952E+06			

Grand Total Activity : 1.391E+06 1.952E+06

Flags: "K" = Keyline not found
 "E" = Manually edited

"M" = Manually accepted
 "A" = Nuclide specific abn. limit

It	Energy	Area	Bkgnd	FWHM	Channel	Left	Pw	Cts/Sec	%Err	%Eff	Flags
0	65.64	283	15476	1.03	129.81	128	5	3.93E-02	****	2.12E+00	
0	67.95	260	17276	1.20	134.42	133	5	3.61E-02	****	2.42E+00	
0	102.37	175	12102	1.31	203.21	202	5	2.44E-02	****	5.63E+00	
0	214.63	198	7817	0.63	427.56	426	5	2.75E-02	****	4.87E+00	
0	255.06	1423	11624	1.32	508.36	504	9	1.98E-01	27.9	4.34E+00	
0	310.72	217	7410	1.41	619.63	617	7	3.02E-02	****	3.79E+00	
0	444.62	214	5644	1.54	887.30	885	6	2.97E-02	****	2.97E+00	
0	510.88	630	8712	2.91	1019.78	1014	12	8.76E-02	60.0	2.69E+00	
0	603.63	204	3438	1.75	1205.22	1203	6	2.84E-02	92.2	2.37E+00	
0	610.37	67	4196	1.33	1218.70	1217	7	9.30E-03	****	2.35E+00	
0	772.08	148	3436	0.91	1542.08	1540	7	2.05E-02	****	1.93E+00	
0	814.16	321	4978	1.55	1626.24	1623	9	4.45E-02	80.2	1.85E+00	
0	936.84	85	5672	1.43	1871.60	1870	8	1.18E-02	****	1.62E+00	
0	950.16	79	5860	1.37	1898.25	1895	8	1.10E-02	****	1.60E+00	
0	958.16	103	5782	1.36	1914.25	1910	8	1.42E-02	****	1.59E+00	
0	1036.88	70	3495	1.20	2071.72	2069	7	9.72E-03	****	1.48E+00	
0	1110.97	77	2459	0.89	2219.96	2218	5	1.06E-02	****	1.38E+00	
0	1120.83	146	2590	1.73	2239.69	2237	7	2.03E-02	****	1.37E+00	
6	1325.96	1292	2409	3.60	2650.13	2639	39	1.79E-01	25.2	1.18E+00	
0	1526.89	66	565	1.79	3052.27	3050	7	9.22E-03	****	1.06E+00	
0	1552.16	46	587	0.71	3102.86	3099	7	6.34E-03	****	1.05E+00	
0	1687.25	94	368	2.62	3373.30	3370	8	1.30E-02	73.7	1.00E+00	
0	1706.74	93	576	3.57	3412.30	3406	14	1.29E-02	****	9.95E-01	
0	1765.06	28	136	0.98	3529.08	3527	5	3.95E-03	****	9.81E-01	
0	1771.14	59	283	2.41	3541.25	3536	10	8.24E-03	****	9.80E-01	
0	1792.79	20	196	1.32	3584.59	3581	7	2.72E-03	****	9.76E-01	
4	1992.72	46	117	1.91	3984.95	3981	15	6.37E-03	83.4	9.61E-01	
4	1996.33	54	122	2.28	3992.16	3981	15	7.55E-03	76.3	9.61E-01	

Flags: "T" = Tentatively associated

```

*****
*                                     GENERAL ENG. LABS, LLC.                               *
*                                     2040 Savage Road                                   *
*                                     Charleston, SC 29414                             *
*****
*                                     DETECTOR DATA                                   *
*
* Configuration      : DKA300:[CANBERRA.GAMMA.ARCHIVE.GAMMA]VER_GAMMA16_CAN.CNF;1*
* Acquisition date   : 22-MAR-2006 08:28:37  Detector SN#      : 1922864          *
* Detector ID        : GAMMA16                Sensitivity       : 3.00000          *
* Geometry           : CAN                    Energy tolerance: 2.00000          *
* Elapsed live time  : 0 02:00:00.00         Abundance limit  : 75.00000          *
* Elapsed real time  : 0 02:01:11.69         Half life ratio  : 8.00000          *
*****
*                                     SAMPLE DATA                                   *
*
* Sample date        : 1-APR-2005 12:00:00.  Nuclide Library  : CAL             *
* Sample ID          : VER_GAMMA16_CAN        Analyst initials: MJH1             *
* Batch Number       :                       Sample Quantity : 1.00000E+00 LITER *
*****
*                                     QC DATA                                   *
*
* CALIB. DATE/TIME  : 5-APR-2006 19:34:04.74MS Isotope       :
* MSD DPM            :                       MSD Isotope       :
* LCS DPM            :                       LCS Isotope       :
*****

```

Combined Activity-MDA Report

---- Identified Nuclides ----

Nuclide	Activity (pCi/LITER)	Act error	MDA (pCi/LITER)	MDA error	Act/MDA
CO-57	1.852E+04	1.448E+03	9.493E+01	7.365E+00	195.142
CO-60	3.965E+04	2.480E+03	5.609E+01	3.491E+00	706.876
Y-88	8.368E+04	4.934E+03	3.796E+02	2.161E+01	220.425
CD-109	7.820E+05	9.456E+04	2.400E+03	2.899E+02	325.827
SN-113	4.927E+04	3.209E+03	5.930E+02	3.696E+01	83.094
CS-137	2.444E+04	1.517E+03	6.997E+01	4.313E+00	349.331
CE-139	2.941E+04	2.472E+03	2.269E+02	1.884E+01	129.598
HG-203	5.395E+04	1.002E+04	9.723E+03	8.132E+02	5.549
PB-210	8.052E+05	8.949E+04	2.365E+04	2.456E+03	34.049
AM-241	6.584E+04	8.964E+03	4.690E+02	6.351E+01	140.401

QA filename : DKA300:[CANBERRA.GAMMA]QC_BKG_GAMMA16.QAF;1

Sample ID : BKG_GAMMA16 Sample quantity : 1.80 LITER
Sample date : 20-MAR-2006 00:00:00 Acquisition date : 20-MAR-2006 14:59:24
Elapsed live time: 0 16:40:00.00 Elapsed real time: 0 16:40:04.08

Out-of-range Test: BOUNDARY

Parameter Description	Lower	Upper	Value	Flag
BACKGROUND (GROSS COUNTS)	7.54E+04	9.49E+04	8.50E+04	
BACKGROUND (CPS)	1.26	1.58	1.42	

Flags: "*" means the out-of-range test is parameter-dependent

Approved by: *jml* Approval Date: 3 / 21 / 06

Gamma Spectroscopy Calibration VerificationInstrument: Gamma 12Calibration Date: 3/22/2006Geometry: CANStandard Id: 70530-278

Isotope		CALIBRATED ACTIVITY (PCI)	MEASURED ACTIVITY (PCI)	DIFFERENCE %
Pb-210		8.1682E+05	8.052E+05	-1.42
Am-241		6.2283E+04	6.584E+04	5.71
Cd-109		8.2222E+05	7.820E+05	-4.89
Co-57		1.8996E+04	1.852E+04	-2.51
Ce-139		2.8853E+04	2.941E+04	1.93
Sn-113		4.8141E+04	4.927E+04	2.35
Cs-137		2.4217E+04	2.444E+04	0.92
Co-60	1332.5	3.8655E+04	3.965E+04	2.57
Y-88	1836.06	8.5829E+04	8.368E+04	-2.50

Prepared By: *Michael P. Fenton*Date: 4/6/06Reviewed By: *J. L. Austin*Date: 4/6/2006

General Engineering Laboratories, LLC

2040 Savage Road, Charleston, SC 29414
(843)556-8171

Gamma Spectrometer Front End Electronics Setup

Detector: GAMMA 16

Date Performed: 3/16/06

Performed By: Muhaffez

<p>High Voltage Power Supply</p> <p>Model No. <u>3106D</u> High Voltage <u>4.0 kV</u></p>	<p>Spectroscopy Amplifier</p> <p>Model No. <u>2020</u> Course Gain <u>10</u> Fine Gain <u>1.238</u> Time Constant <u>4 μsec</u> Input polarity <u>+</u> BSLR rate <u>AUTO</u> BSLR mode <u>ASYM</u> Threshold <u>AUTO</u></p>
<p>ADC</p> <p>Model No. <u>8701</u> Gain <u>4k</u></p>	
<p>AIM Module</p> <p>Model No. <u>ND556</u> Address <u>NISA3:1</u></p>	

General Engineering Laboratories, LLC

2040 Savage Road, Charleston, SC 29414
(803)556-8171

Gamma Spectrometer Geometry Calibration Package

Detector: WELL

Geometry: CAN

	YES	NO	Comments
1) Is all calibration standard information enclosed for: the primary standard certificate? the secondard standard(s) documentation? the nuclide library used? the VMS certificate file?	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
	<input type="checkbox"/>	<input type="checkbox"/>	NA
	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
2) Is the detector efficiency curve printout included?	<input type="checkbox"/>	<input checked="" type="checkbox"/>	
3) Is the efficiency calibration report included and reviewed?	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
4) Is the raw count data included for: the calibration peak report? the calibration verification PEAK report? the calibration verification NID report? the last instrument background?	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
5) Are the calibration verification calculations included?	<input checked="" type="checkbox"/>	<input type="checkbox"/>	
6) Are the instrument settings included: amp, HVPS, ADC settings?	<input checked="" type="checkbox"/>	<input type="checkbox"/>	

Prepared By: Michael [Signature]

Date: 12/15/05

Reviewed By: [Signature]

Date: 12/15/05

Effective Date: 12/14/05

General Engineering Laboratories, LLC

2040 Savage Road, Charleston, SC 29414
(803)556-8171

Gamma Spectrometer Front End Electronics Setup

Detector: Well

Date Performed: 12/12/05

Performed By: Muhafitton

<p>High Voltage Power Supply</p> <p>Model No. <u>3106D</u> High Voltage <u>2.5KV</u></p>	<p>Spectroscopy Amplifier</p> <p>Model No. <u>2026</u> Course Gain <u>20</u> Fine Gain <u>0.542</u> Time Constant <u>4 μ sec.</u> Input polarity <u>POSITIVE</u> BSLR rate <u>N/A</u> BSLR mode <u>N/A</u> Threshold <u>N/A</u></p>
<p>ADC</p> <p>Model No. <u>8701</u> Gain <u>4000</u></p>	
<p>AIM Module</p> <p>Model No. <u>556A</u> Address <u>NIE04.2</u></p>	

Gamma Spectroscopy Calibration VerificationInstrument: WellCalibration Date: 12/14/2005Geometry: CANStandard Id: 70530-278

Isotope		CALIBRATED ACTIVITY (PCI)	MEASURED ACTIVITY (PCI)	DIFFERENCE %
Pb-210		8.1682E+05	7.865E+05	-3.71
Am-241		6.2283E+04	6.213E+04	-0.25
Cd-109		8.2222E+05	8.102E+05	-1.46
Co-57		1.8996E+04	1.950E+04	2.65
Ce-139		2.8853E+04	2.851E+04	-1.19
Sn-113		4.8141E+04	4.723E+04	-1.89
Cs-137		2.4217E+04	2.487E+04	2.70
Co-60	1332.5	3.8655E+04	3.810E+04	-1.44
Y-88	1836.06	8.5829E+04	8.701E+04	1.38

Prepared By: *Muhamed H. H. H.*Date: 12/15/05Reviewed By: *J. H. C. and J. H. C.*Date: 12/15/05

Verified:

VMS Quality Assurance Report V1.3 Generated 11-DEC-2005 12:16:35


QA filename : DKA300:[CANBERRA.GAMMA]QC_BKG_WELL.QAF;2

Sample ID : BKG_WELL Sample quantity : 1.80 LITER
Sample date : 10-DEC-2005 00:00:00 Acquisition date : 10-DEC-2005 19:27:01
Elapsed live time: 0 16:40:00.00 Elapsed real time: 0 16:40:12.72

Out-of-range Test: BOUNDARY

Parameter Description	Lower	Upper	Value	Flag
BACKGROUND (GROSS COUNTS)	8.07E+04	1.24E+05	1.01E+05	
BACKGROUND (CPS)	1.34	2.06	1.68	

Flags: "*" means the out-of-range test is parameter-dependent

Approved by: 

Approval Date: 12 / 11 / 05

```

*****
*                                     GENERAL ENG. LABS, LLC.                               *
*                                     2040 Savage Road                                   *
*                                     Charleston, SC 29414                             *
*****
Configuration      : DKA300:[CANBERRA.GAMMA.ARCHIVE.GAMMA]VER_WELL_CAN.CNF;1
Sample date        : 1-APR-2005 12:00:00. Acquisition date : 14-DEC-2005 17:17:48
Sample ID          : VER_WELL_CAN              Sample quantity : 1.00000E+00 LITER
Detector name     : WELL                      Detector geometry: CAN
Elapsed live time : 0 01:00:00.00            Elapsed real time: 0 01:01:15.52  2.1%
Energy tolerance  : 2.00000 KEV              Analyst Initials  : MJH1
Abundance limit   : 75.00000                Sensitivity       : 3.00000
Batch ID          :                          Detector SN#      : 3941466
Matrix Spike DPM  :                          LCS DPM       :
*****

```

Pk	It	Energy	Area	Bkgnd	FWHM	Channel	Left	Pw	Cts/Sec	%Err	Fit
1	0	32.94	8090	42222	1.45	64.85	62	8	2.25E+00	4.5	
2	1	36.16	2099	10359	1.36	71.25	70	27	5.83E-01	6.1	3.83E+02
3	1	40.19*	6404	41044	1.37	79.25	70	27	1.78E+00	5.7	
4	1	42.20	7325	40817	1.38	83.25	70	27	2.03E+00	5.1	
5	1	46.51*	126212	39800	1.39	91.80	70	27	3.51E+01	0.4	
6	0	59.47	120117	56340	1.32	117.56	110	15	3.34E+01	0.5	
7	10	66.54	2603	25638	2.05	131.60	126	25	7.23E-01	12.0	3.80E+00
8	10	69.04	3337	46040	2.81	136.56	126	25	9.27E-01	15.1	
9	10	72.96*	1748	35224	2.27	144.35	126	25	4.86E-01	21.2	
10	0	88.07*	140788	36704	1.32	174.36	168	14	3.91E+01	0.4	
11	0	122.09	58293	20487	1.34	241.96	234	15	1.62E+01	0.7	
12	0	136.50	7151	11280	1.33	270.59	266	11	1.99E+00	3.1	
13	0	156.62	194	6859	1.39	310.56	308	7	5.40E-02	71.0	
14	0	165.92*	37327	11395	1.39	329.05	323	13	1.04E+01	0.8	
15	0	199.37*	534	6782	1.82	395.51	391	9	1.48E-01	28.2	
16	0	255.10	777	6322	1.42	506.25	502	10	2.16E-01	19.5	
17	0	279.27*	3871	5995	1.53	554.28	549	11	1.08E+00	4.2	
18	0	309.70	233	4389	1.90	614.75	612	9	6.48E-02	51.6	
19	0	391.71*	19069	7046	1.52	777.72	769	16	5.30E+00	1.2	
20	0	511.27*	337	3672	1.31	1015.34	1011	11	9.37E-02	35.4	
21	0	530.86*	155	1686	1.02	1054.28	1052	6	4.31E-02	42.7	
22	0	573.83	91	1923	1.59	1139.69	1137	7	2.54E-02	80.4	
23	0	610.33*	24	1687	0.73	1212.23	1211	6	6.56E-03	276.8	
24	0	625.88	102	2504	1.45	1243.14	1239	9	2.84E-02	88.7	
25	0	629.80*	139	1633	1.14	1250.94	1248	6	3.87E-02	46.7	
26	0	661.67*	36964	5440	1.70	1314.29	1305	18	1.03E+01	0.7	
27	0	690.27	124	2402	2.16	1371.14	1367	9	3.45E-02	71.8	
28	0	744.04	100	1822	1.25	1478.03	1476	8	2.78E-02	74.3	
29	0	777.53*	126	1713	1.47	1544.61	1541	8	3.50E-02	57.5	
30	0	803.35*	96	1015	0.93	1595.95	1594	5	2.67E-02	50.7	
31	0	814.14*	429	2506	1.60	1617.41	1612	11	1.19E-01	23.1	
32	0	849.87	77	1407	1.21	1688.44	1685	6	2.15E-02	77.4	
33	0	875.35	98	1489	1.21	1739.10	1736	6	2.71E-02	63.3	
34	0	898.03*	20561	4400	1.83	1784.19	1775	17	5.71E+00	1.0	
35	0	1069.73	33	2166	3.43	2125.61	2118	11	9.17E-03	273.0	
36	0	1114.84*	100	1453	1.00	2215.34	2214	8	2.77E-02	66.8	
37	0	1159.38	83	853	1.86	2303.92	2300	7	2.31E-02	59.2	
38	0	1173.21*	37348	2431	2.05	2331.42	2322	19	1.04E+01	0.6	

Pk	It	Energy	Area	Bkgnd	FWHM	Channel	Left	Pw	Cts/Sec	%Err	Fit
39	0	1211.27*	62	505	1.68	2407.11	2404	8	1.71E-02	64.8	
40	0	1231.58	56	379	1.70	2447.51	2443	8	1.55E-02	61.9	
41	0	1270.20*	58	314	1.44	2524.31	2521	7	1.61E-02	52.5	
42	0	1318.08	74	341	1.18	2619.56	2616	7	2.05E-02	43.2	
43	5	1325.67	553	983	3.54	2634.67	2623	39	1.53E-01	15.9	1.07E+01
44	5	1332.50*	33504	562	2.23	2648.24	2623	39	9.31E+00	0.6	
45	0	1404.12	36	236	0.59	2790.71	2786	7	9.97E-03	72.9	
46	0	1459.28*	57	523	4.35	2900.44	2894	13	1.59E-02	83.7	
47	0	1551.48*	99	367	2.36	3083.88	3080	8	2.74E-02	35.2	
48	0	1587.75	69	293	0.88	3156.03	3154	6	1.92E-02	40.9	
49	0	1596.97	25	299	0.56	3174.38	3171	6	6.88E-03	112.0	
50	0	1623.14	97	727	7.89	3226.45	3219	21	2.70E-02	70.1	
51	0	1674.93	69	343	5.02	3329.51	3323	14	1.91E-02	59.0	
52	0	1782.30	70	91	4.84	3543.16	3538	12	1.94E-02	29.7	
53	0	1797.31*	29	67	1.63	3573.03	3570	7	8.06E-03	50.3	
54	0	1836.11*	11797	362	2.41	3650.25	3638	24	3.28E+00	1.0	
55	0	1952.53	23	75	4.63	3881.96	3877	15	6.39E-03	84.7	
56	0	2013.87	20	16	1.46	4004.04	4002	5	5.47E-03	39.2	

Flag: "*" = Peak area was modified by background subtraction

VAX/VMS Nuclide Identification Report Generated

```
*****
*                               General Eng. Labs, LLC.                               *
*                               2040 Savage Road                                       *
*                               Charleston, SC 29414                                   *
*****
```

DETECTOR DATA

```
* Configuration      : DKA300:[CANBERRA.GAMMA.ARCHIVE.GAMMA]VER_WELL_CAN          *
* Acquisition date   : 14-DEC-2005 17:17:48 Detector SN#      : 3941466          *
* Detector ID        : WELL                               Sensitivity      : 3.000          *
* Geometry           : CAN                               Energy tolerance: 2.000          *
* Elapsed live time  : 0 01:00:00.00                   Abundance limit : 75.000          *
* Elapsed real time  : 0 01:01:15.52                   Half life ratio  : 8.000          *
*****
```

SAMPLE DATA

```
* Sample date       : 1-APR-2005 12:00:00 Nuclide Library  : FERMC          *
* Sample ID         : VER_WELL_CAN                     Analyst initials: MJH1          *
* Batch Number      :                               Sample Quantity : 1.0000E+00 LITER          *
* Recovery          : 1.00000                         Carrier Weight   : 0.00000          *
*****
```

QC DATA

```
* Standard Weight   : 0.00000                               *
* CALIB. DATE/TIME : 14-DEC-2005 17:16:53 MS Isotope      :                               *
* MSD DPM           : *****                               MSD Isotope       :                               *
* LCS DPM           : 0.000                                LCS Isotope       :                               *
* LCSD DPM          : 0.000                                LCSD Isotope      :                               *
*****
```

Combined Activity-MDA Report

---- Identified Nuclides ----

Nuclide	Activity (pCi/LITER)	Act error	MDA (pCi/LITER)	
CO-57	1.950E+04	2.638E+02	1.533E+02	0.000E+00
CO-60	3.810E+04	4.318E+02	1.279E+02	0.000E+00
Y-88	8.701E+04	1.765E+03	4.402E+02	0.000E+00
CD-109	8.102E+05	6.444E+03	3.601E+03	0.000E+00
SN-113	4.723E+04	1.154E+03	7.098E+02	0.000E+00
CS-137	2.487E+04	3.480E+02	1.676E+02	0.000E+00
CE-139	2.851E+04	4.485E+02	2.896E+02	0.000E+00
HG-203	5.713E+04	4.795E+03	4.579E+03	0.000E+00
PB-210	7.865E+05	6.259E+03	5.155E+03	0.000E+00
AM-241	6.213E+04	6.487E+02	3.775E+02	0.000E+00

---- Non-Identified Nuclides ----

Nuclide	Key-Line Activity (pCi/LITER)	K.L. Act error) Ided	MDA (pCi/LITER)
---------	--------------------------------------	--------------------------	---------------------


```

*****
*                               GENERAL ENG. LABS, LLC.                               *
*                               2040 Savage Road                                       *
*                               Charleston, SC 29414                                 *
*****
Configuration      : DKA300:[CANBERRA.GAMMA.ARCHIVE.GAMMA]VER_WELL_CAN.CNF;1
Sample date        : 1-APR-2005 12:00:00. Acquisition date : 14-DEC-2005 17:17:48
Sample ID          : VER_WELL_CAN           Sample quantity  : 1.00000E+00 LITER
Detector name      : WELL                  Detector geometry: CAN
Elapsed live time  : 0 01:00:00.00         Elapsed real time  : 0 01:01:15.52  2.1%
Energy tolerance   : 2.00000 KEV           Analyst Initials   : MJH1
Abundance limit    : 75.00000              Sensitivity        : 3.00000
Batch ID           :                       Detector SN#       : 3941466
Matrix Spike DPM   :                       LCS DPM         :
*****

```

Nuclide Line Activity Report

Nuclide Type:

Nuclide	Energy	Area	%Abn	%Eff	Uncorrected pCi/LITER	Decay Corr pCi/LITER	2-Sigma %Error
CO-57	122.06	58293	85.51*	5.059E+00	1.012E+04	1.950E+04	1.35
	136.47	7151	10.47	4.895E+00	1.048E+04	2.019E+04	6.22
CO-60	1173.24	37348	99.90	8.068E-01	3.479E+04	3.817E+04	1.21
	1332.50	33504	99.98*	7.245E-01	3.473E+04	3.810E+04	1.13
Y-88	898.04	20561	93.40	1.013E+00	1.631E+04	8.683E+04	2.03
	1836.06	11797	99.38*	5.453E-01	1.634E+04	8.701E+04	2.03
CD-109	88.03	140788	3.79*	5.066E+00	5.505E+05	8.102E+05	0.80
SN-113	391.70	19069	64.90*	2.199E+00	1.003E+04	4.723E+04	2.44
CS-137	661.66	36964	85.12*	1.332E+00	2.447E+04	2.487E+04	1.40
CE-139	165.85	37327	80.35*	4.469E+00	7.804E+03	2.851E+04	1.57
HG-203	70.83	3337	4.75	4.551E+00	1.159E+04	5.318E+05	30.16
	72.87	1748	8.00	4.705E+00	3.486E+03	1.600E+05	42.47
	82.60	-----	3.55	4.973E+00	-----	Line Not Found	-----
	279.20	3871	77.30*	3.020E+00	1.245E+03	5.713E+04	8.39
PB-210	46.50	126212	4.05*	3.041E+00	7.695E+05	7.865E+05	0.80
AM-241	59.54	120117	35.90*	4.048E+00	6.206E+04	6.213E+04	1.04

Flag: "*" = Keyline

Summary of Nuclide Activity

Sample ID : VER_WELL_CAN

Acquisition date : 14-DEC-2005 17:17:48

Total number of lines in spectrum 56
 Number of unidentified lines 41
 Number of lines tentatively identified by NID 15 26.79%

Nuclide Type :

Nuclide	Hlife	Decay	Uncorrected pCi/LITER	Decay Corr pCi/LITER	Decay Corr 2-Sigma Error	2-Sigma %Error	Flags
CO-57	271.74D	1.93	1.012E+04	1.950E+04	0.026E+04	1.35	
CO-60	5.27Y	1.10	3.473E+04	3.810E+04	0.043E+04	1.13	
Y-88	106.63D	5.32	1.634E+04	8.701E+04	0.177E+04	2.03	
CD-109	461.40D	1.47	5.505E+05	8.102E+05	0.064E+05	0.80	
SN-113	115.09D	4.71	1.003E+04	4.723E+04	0.115E+04	2.44	
CS-137	30.00Y	1.02	2.447E+04	2.487E+04	0.035E+04	1.40	
CE-139	137.64D	3.65	7.804E+03	2.851E+04	0.045E+04	1.57	
HG-203	46.60D	45.9	1.245E+03	5.713E+04	0.480E+04	8.39	
PB-210	22.26Y	1.02	7.695E+05	7.865E+05	0.063E+05	0.80	
AM-241	432.20Y	1.00	6.206E+04	6.213E+04	0.065E+04	1.04	
Total Activity :			1.487E+06	1.961E+06			

Grand Total Activity : 1.487E+06 1.961E+06

Flags: "K" = Keyline not found
 "E" = Manually edited

"M" = Manually accepted
 "A" = Nuclide specific abn. limit

It	Energy	Area	Bkgnd	FWHM	Channel	Left	Pw	Cts/Sec	%Err	%Eff	Flags
0	32.94	8090	42222	1.45	64.85	62	8	2.25E+00	9.1	1.66E+00	
1	36.16	2099	10359	1.36	71.25	70	27	5.83E-01	12.2	2.00E+00	
1	40.19	6404	41044	1.37	79.25	70	27	1.78E+00	11.5	2.42E+00	
1	42.20	7325	40817	1.38	83.25	70	27	2.03E+00	10.2	2.63E+00	
10	66.54	2603	25638	2.05	131.60	126	25	7.23E-01	24.1	4.44E+00	
0	156.62	194	6859	1.39	310.56	308	7	5.40E-02	****	4.61E+00	
0	199.37	534	6782	1.82	395.51	391	9	1.48E-01	56.4	3.97E+00	
0	255.10	777	6322	1.42	506.25	502	10	2.16E-01	39.0	3.27E+00	
0	309.70	233	4389	1.90	614.75	612	9	6.48E-02	****	2.75E+00	
0	511.27	337	3672	1.31	1015.34	1011	11	9.37E-02	70.9	1.70E+00	
0	530.86	155	1686	1.02	1054.28	1052	6	4.31E-02	85.3	1.64E+00	
0	573.83	91	1923	1.59	1139.69	1137	7	2.54E-02	****	1.52E+00	
0	610.33	24	1687	0.73	1212.23	1211	6	6.56E-03	****	1.44E+00	
0	625.88	102	2504	1.45	1243.14	1239	9	2.84E-02	****	1.40E+00	
0	629.80	139	1633	1.14	1250.94	1248	6	3.87E-02	93.4	1.39E+00	
0	690.27	124	2402	2.16	1371.14	1367	9	3.45E-02	****	1.28E+00	
0	744.04	100	1822	1.25	1478.03	1476	8	2.78E-02	****	1.20E+00	
0	777.53	126	1713	1.47	1544.61	1541	8	3.50E-02	****	1.15E+00	
0	803.35	96	1015	0.93	1595.95	1594	5	2.67E-02	****	1.12E+00	
0	814.14	429	2506	1.60	1617.41	1612	11	1.19E-01	46.3	1.10E+00	
0	849.87	77	1407	1.21	1688.44	1685	6	2.15E-02	****	1.06E+00	
0	875.35	98	1489	1.21	1739.10	1736	6	2.71E-02	****	1.04E+00	
0	1069.73	33	2166	3.43	2125.61	2118	11	9.17E-03	****	8.72E-01	
0	1114.84	100	1453	1.00	2215.34	2214	8	2.77E-02	****	8.42E-01	
0	1159.38	83	853	1.86	2303.92	2300	7	2.31E-02	****	8.15E-01	
0	1211.27	62	505	1.68	2407.11	2404	8	1.71E-02	****	7.85E-01	
0	1231.58	56	379	1.70	2447.51	2443	8	1.55E-02	****	7.74E-01	
0	1270.20	58	314	1.44	2524.31	2521	7	1.61E-02	****	7.54E-01	
0	1318.08	74	341	1.18	2619.56	2616	7	2.05E-02	86.4	7.31E-01	
5	1325.67	553	983	3.54	2634.67	2623	39	1.53E-01	31.7	7.28E-01	
0	1404.12	36	236	0.59	2790.71	2786	7	9.97E-03	****	6.93E-01	
0	1459.28	57	523	4.35	2900.44	2894	13	1.59E-02	****	6.70E-01	
0	1551.48	99	367	2.36	3083.88	3080	8	2.74E-02	70.5	6.36E-01	
0	1587.75	69	293	0.88	3156.03	3154	6	1.92E-02	81.8	6.23E-01	
0	1596.97	25	299	0.56	3174.38	3171	6	6.88E-03	****	6.20E-01	
0	1623.14	97	727	7.89	3226.45	3219	21	2.70E-02	****	6.11E-01	
0	1674.93	69	343	5.02	3329.51	3323	14	1.91E-02	****	5.94E-01	
0	1782.30	70	91	4.84	3543.16	3538	12	1.94E-02	59.3	5.61E-01	
0	1797.31	29	67	1.63	3573.03	3570	7	8.06E-03	****	5.56E-01	
0	1952.53	23	75	4.63	3881.96	3877	15	6.39E-03	****	5.14E-01	
0	2013.87	20	16	1.46	4004.04	4002	5	5.47E-03	78.3	4.98E-01	

Flags: "T" = Tentatively associated

 * GENERAL ENG. LABS, LLC. *
 * 2040 Savage Road *
 * Charleston, SC 29414 *

 * DETECTOR DATA *
 * *
 * Configuration : DKA300:[CANBERRA.GAMMA.ARCHIVE.GAMMA]VER_WELL_CAN.CNF;1 *
 * Acquisition date : 14-DEC-2005 17:17:48 Detector SN# : 3941466 *
 * Detector ID : WELL Sensitivity : 3.00000 *
 * Geometry : CAN Energy tolerance: 2.00000 *
 * Elapsed live time: 0 01:00:00.00 Abundance limit : 75.00000 *
 * Elapsed real time: 0 01:01:15.52 Half life ratio : 8.00000 *

 * SAMPLE DATA *
 * *
 * Sample date : 1-APR-2005 12:00:00. Nuclide Library : CAL *
 * Sample ID : VER_WELL_CAN Analyst initials: MJH1 *
 * Batch Number : Sample Quantity : 1.00000E+00 LITER *

 * QC DATA *
 * *
 * CALIB. DATE/TIME : 14-DEC-2005 17:16:53.5MS Isotope : *
 * MSD DPM : MSD Isotope : *
 * LCS DPM : LCS Isotope : *

Combined Activity-MDA Report

---- Identified Nuclides ----

Nuclide	Activity (pCi/LITER)	Act error	MDA (pCi/LITER)	MDA error	Act/MDA
CO-57	1.950E+04	2.638E+02	1.533E+02	0.000E+00	127.159
CO-60	3.810E+04	4.318E+02	1.279E+02	0.000E+00	297.796
Y-88	8.701E+04	1.765E+03	4.402E+02	0.000E+00	197.670
CD-109	8.102E+05	6.444E+03	3.601E+03	0.000E+00	225.016
SN-113	4.723E+04	1.154E+03	7.098E+02	0.000E+00	66.545
CS-137	2.487E+04	3.480E+02	1.676E+02	0.000E+00	148.422
CE-139	2.851E+04	4.485E+02	2.896E+02	0.000E+00	98.418
HG-203	5.713E+04	4.795E+03	4.579E+03	0.000E+00	12.478
PB-210	7.865E+05	6.259E+03	5.155E+03	0.000E+00	152.566
AM-241	6.213E+04	6.487E+02	3.775E+02	0.000E+00	164.571

```

*****
*                               GENERAL ENG. LABS, LLC.                               *
*                               2040 Savage Road                                       *
*                               Charleston, SC 29414                                   *
*****
Configuration      : DKA300:[CANBERRA.GAMMA.ARCHIVE.GAMMA]CAL_WELL_CAN.CNF;1
Sample date        : 1-APR-2005 12:00:00. Acquisition date : 14-DEC-2005 15:09:59
Sample ID          : CAL_WELL_CAN           Sample quantity  : 1.00000E+00 LITER
Detector name      : WELL                  Detector geometry: CAN
Elapsed live time  : 0 01:00:00.00         Elapsed real time: 0 01:01:15.78  2.1%
Energy tolerance   : 2.00000 KEV          Analyst Initials  : MJH1
Abundance limit    : 75.00000             Sensitivity       : 3.00000
Batch ID           :                      Detector SN#      : 3941466
Matrix Spike DPM   :                      LCS DPM         :
*****

```

Pk	It	Energy	Area	Bkgnd	FWHM	Channel	Left	Pw	Cts/Sec	%Err	Fit
1	0	33.01	8246	41954	1.55	64.99	62	8	2.29E+00	4.4	
2	9	37.37*	5883	36050	2.91	73.65	70	27	1.63E+00	5.5	1.30E+02
3	9	41.25	15566	86773	2.94	81.36	70	27	4.32E+00	4.5	
4	9	44.00	10962	50654	1.67	86.83	70	27	3.05E+00	4.5	
5	9	46.52*	132120	44971	1.47	91.82	70	27	3.67E+01	0.4	
6	0	59.51	118513	53096	1.29	117.63	111	14	3.29E+01	0.5	
7	7	67.04	4333	33444	2.54	132.59	126	24	1.20E+00	9.1	4.66E+00
8	7	69.77	2487	29794	1.88	138.02	126	24	6.91E-01	13.9	
9	7	72.94*	2226	31922	2.19	144.32	126	24	6.18E-01	15.4	
10	0	88.06*	142647	39189	1.32	174.36	167	15	3.96E+01	0.4	
11	0	103.33	253	10867	1.47	204.69	202	7	7.02E-02	68.7	
12	0	122.12	58815	21574	1.37	242.03	234	16	1.63E+01	0.7	
13	0	136.54	7058	11508	1.38	270.68	266	11	1.96E+00	3.2	
14	0	165.94*	36981	11897	1.38	329.08	323	13	1.03E+01	0.8	
15	0	199.10*	273	5487	1.45	394.97	391	7	7.57E-02	45.5	
16	0	203.75	121	3853	0.74	404.22	402	5	3.37E-02	77.2	
17	0	255.24	878	5574	1.13	506.53	503	9	2.44E-01	15.7	
18	0	279.32*	3554	6174	1.41	554.37	550	11	9.87E-01	4.6	
19	0	391.76*	19250	6457	1.54	777.83	770	15	5.35E+00	1.2	
20	0	469.11	39	3000	0.75	931.54	931	7	1.09E-02	231.8	
21	0	661.69*	37044	5332	1.73	1314.32	1306	17	1.03E+01	0.7	
22	0	697.49	92	1645	1.36	1385.50	1382	6	2.55E-02	70.7	
23	0	793.28	125	1522	1.53	1575.92	1573	7	3.48E-02	52.5	
24	0	814.01*	391	2512	1.47	1617.14	1612	11	1.09E-01	25.3	
25	0	898.05*	20363	4638	1.87	1784.24	1776	17	5.66E+00	1.0	
26	0	1012.14	108	1801	1.97	2011.10	2007	9	3.00E-02	71.7	
27	0	1046.13	88	1097	1.49	2078.69	2077	6	2.43E-02	60.9	
28	0	1173.25*	37789	2386	2.03	2331.50	2321	20	1.05E+01	0.6	
29	0	1238.14	35	440	1.28	2460.56	2457	8	9.59E-03	106.6	
30	5	1325.67	516	1196	3.54	2634.67	2621	42	1.43E-01	17.6	6.82E+00
31	5	1332.53*	33702	632	2.21	2648.30	2621	42	9.36E+00	0.6	
32	0	1430.30	32	536	4.84	2842.79	2836	13	8.76E-03	152.5	
33	0	1485.64*	66	309	1.43	2952.89	2949	8	1.84E-02	47.8	
34	0	1753.86	21	208	5.28	3486.57	3479	16	5.83E-03	155.1	
35	0	1836.17*	11671	397	2.41	3650.38	3639	24	3.24E+00	1.0	
36	0	1886.85	12	29	1.42	3751.23	3748	6	3.31E-03	77.8	

Flag: "*" = Peak area was modified by background subtraction

Configuration : MCA0:[GAMMA]WELL\$1
 Analyses by : CALIBRATE V1.7, PEAK V16.4
 Detector Name : WELL Energy Calib Time: 13-DEC-2005 09:34:01
 Efficiency type : Empirical Effncy Calib Time: 14-DEC-2005 17:16:53
 Detector Geometry: WELL Shelf : 0

Energy Calibration Report

$$\text{Energy} = 0.2987 + 0.5034 * \text{Channel} + -1.2315E-07 * (\text{Channel} ** 2)$$

Nbr	Centroid Channel	True Energy	Computed Energy	Difference
1	91.73	46.50	46.47	0.026
2	117.44	59.54	59.42	0.121
3	174.31	88.03	88.04	-0.006
4	242.00	122.06	122.11	-0.050
5	329.06	165.85	165.93	-0.073
6	777.81	391.70	391.76	-0.055
7	1314.30	661.66	661.67	-0.014
8	1784.19	898.04	898.03	0.016
9	2331.37	1173.24	1173.19	0.051
10	2648.23	1332.50	1332.49	0.008
11	3650.20	1836.06	1836.09	-0.024

FWHM Calibration Report

$$\text{FWHM} = 1.046 + 3.1639E-02 * (\text{Energy} ** 1/2)$$

Nbr	Energy	True FWHM	Computed FWHM	Difference
1	46.50	1.48	1.26	0.215
2	59.54	1.33	1.29	0.036
3	88.03	1.33	1.34	-0.010
4	122.06	1.37	1.40	-0.028
5	165.85	1.39	1.45	-0.064
6	391.70	1.52	1.67	-0.148
7	661.66	1.76	1.86	-0.102
8	898.04	1.92	1.99	-0.075
9	1173.24	2.09	2.13	-0.043
10	1332.50	2.30	2.20	0.094
11	1836.06	2.53	2.40	0.124

Efficiency Calibration Report

$$\text{Eff} = \exp(a2 + a3 * x + a4 * x ** 2 + a5 * x ** 3 + a6 * x ** 4 + a7 * x ** 5), \quad x = \ln(a1 / \text{energy})$$

a1 a2 a3 a4 a5 a6 a7
 941.3 -4.633 0.8619 7.0681E-02 6.4484E-02 -7.1717E-02 8.2159E-03

Average Deviation = 1.46 % Reduced Chi-Square = 0.771

Nbr	Energy (KEV)	Measured Efficiency	Efficiency Error	Computed Efficiency	Diff/ Error	% Diff
-----	--------------	---------------------	------------------	---------------------	-------------	--------

1	46.50	3.06E-02	9.28E-04	3.04E-02	0.27	0.82
---	-------	----------	----------	----------	------	------

Nbr	Energy (KEV)	Measured Efficiency	Efficiency Error	Computed Efficiency	Diff/ /Error	% Diff
2	59.54	3.98E-02	1.21E-03	4.05E-02	-0.56	-1.71
3	88.03	5.05E-02	1.68E-03	5.07E-02	-0.08	-0.25
4	122.06	5.24E-02	1.61E-03	5.06E-02	1.11	3.41
5	165.85	4.37E-02	1.27E-03	4.47E-02	-0.75	-2.18
6	391.70	2.18E-02	6.20E-04	2.20E-02	-0.36	-1.01
7	661.66	1.37E-02	4.22E-04	1.33E-02	0.95	2.93
8	898.04	9.96E-03	2.79E-04	1.01E-02	-0.61	-1.70
9	1173.24	8.14E-03	2.25E-04	8.07E-03	0.32	0.88
10	1332.50	7.18E-03	1.91E-04	7.24E-03	-0.33	-0.87
11	1836.06	5.47E-03	1.53E-04	5.45E-03	0.11	0.30

Approved by: Muhafiz Khan
ftc well 12/15/05

Approval Date: 12 / 15 / 05

Print Time : 14-JUN-2005 17:43:24.41
 Certificate file name : DKA300:[CANBERRA.GAMMA]70530-278.CER;1
 Certificate title : CAN
 Certificate date : 1-APR-2005 12:00:00.00
 Certificate quantity : 1.00000E+00

Rcd	Nuclide	Halflife	CAL/ INIT	Energy	Rate	%Abun	Activity (uCi)
1	AM-241	432.20Y	Yes	59.54	8.2730E+02	35.90	6.2283E-02
2	CD-109	462.60D	No	88.03	1.1530E+03	3.79	8.2222E-01
3	Co-57	271.79D	No	122.06	6.0100E+02	85.51	1.8996E-02
4	CE-139	137.60D	No	165.85	8.5780E+02	80.35	2.8853E-02
5	SN-113	115.10D	No	391.70	1.1560E+03	64.90	4.8141E-02
6	CS-137	30.07Y	Yes	661.66	7.6270E+02	85.12	2.4217E-02
7	Y-88	106.60D	No	898.04	3.0220E+03	93.40	8.7447E-02
8	Y-88	106.60D	Yes	1836.06	3.1560E+03	99.38	8.5829E-02
9	Co-60	5.27Y	Yes	1173.24	1.4150E+03	99.90	3.8282E-02
10	CO-60	5.27Y	No	1332.50	1.4300E+03	99.98	3.8655E-02
11	PB-210	22.30Y	No	46.50	1.2240E+03	4.05	8.1682E-01

```

Library Title      :
Library file name  : DKA300:[CANBERRA.GAMMA]CAL.NLB;1
Date printed      : 6-DEC-2004 10:31:17.67
Number of nuclides : 10
Number of lines   : 17

```

Nuclide Name	Half-Life	Nuclide Type	Key Line	Energy	Abundance
CO-57	271.74D		*	122.06 keV	85.51 %
				136.47 keV	10.47 %
CO-60	5.27Y		*	1173.24 keV	99.90 %
				1332.50 keV	99.98 %
Y-88	106.63D		*	898.04 keV	93.40 %
				1836.06 keV	99.38 %
CD-109	461.40D		*	88.03 keV	3.79 %
SN-113	115.09D		*	391.70 keV	64.90 %
CS-137	30.00Y		*	661.66 keV	85.12 %
CE-139	137.64D		*	165.85 keV	80.35 %
HG-203	46.60D			70.83 keV	4.75 %
				72.87 keV	8.00 %
				82.60 keV	3.55 %
				279.20 keV	77.30 %
PB-210	22.26Y		*	46.50 keV	4.05 %
AM-241	432.20Y		*	59.54 keV	35.90 %

CERTIFICATE OF CALIBRATION

Standard Radionuclide Source

70530-278

100 mL Solid in 100 mL Aluminum Can

This standard radionuclide source was prepared using aliquots measured gravimetrically from master radionuclide solution sources. The Am-241 and Pb-210 were calibrated by 4 pi alpha liquid scintillation counting. All other radionuclides were calibrated using a germanium gamma spectrometer system. Calibration and purity were checked using a germanium gamma spectrometer system. At the time of calibration no interfering gamma-ray emitting impurities were detected. The gamma ray emission rates for the most intense gamma-ray lines are given. Analytix maintains traceability to the National Institute of Standards and Technology through a Measurements Assurance Program as described in US NRC Regulatory Guide 4.15, Revision 1, February 1979.

US Patent 4,430,258; UK Patent GB2,149,194B; CA Patent 1,196,776.
Density of solid matrix 1.15 g/cc.

Calibration Date: April 1, 2005 12:00 EST

ISOTOPE	GAMMA ENERGY	HALF-LIFE		GAMMA-RAYS PER SECOND	TOTAL UNCERTAINTY %
Pb-210	46.5	22.3	Y	1224	3.0
Am-241	59.5	432.2	Y	827.3	3.0
Cd-109	88	462.6	d	1153	3.3
Co-57	122	271.79	d	601.0	3.0
Ce-139	166	137.6	d	857.8	2.8
Hg-203	279	46.61	d	1856	2.7
Sn-113	392	115.1	d	1156	2.6
Cs-137	662	30.07	Y	762.7	3.0
Y-88	898	106.6	d	3022	2.6
Co-60	1173	5.271	Y	1415	2.7
Co-60	1332	5.271	Y	1430	2.6
Y-88	1836	106.6	d	3156	2.6

P O NUMBER 2832RD, Item 3

SOURCE PREPARED BY:

M. Dimitrova
M. Dimitrova, Radiochemist

Q A APPROVED:

SM. mfg 5-12-05

This standard will expire one year after the calibration date.

CONTINUING CALIBRATION DATA



Gas Flow Proportional Counter Checks for 09-APR-2006

Short Name	Parmname	Run Time	Count Time	Counts	CPM	Stdev	Status	Comments
LB4100A1	ALPHA BKG	07:24	500	15.0	0.03	-0.8	GOOD	
	BETA BKG	07:24	500	459	0.92	-0.15	GOOD	
	ALPHA EFF	08:40	30	23597	787	-0.1	GOOD	
	BETA EFF	08:40	30	1.79E+05	5950	0.75	GOOD	
LB4100A2	ALPHA BKG	07:24	500	27.0	0.05	-0.4	GOOD	
	BETA BKG	07:24	500	393	0.79	-0.45	GOOD	
	ALPHA EFF	08:40	30	15992	533	-0.29	GOOD	
	BETA EFF	08:40	30	1.31E+05	4370	0.97	GOOD	
LB4100A3	ALPHA BKG	07:24	500	23.0	0.05	-0.48	GOOD	
	BETA BKG	07:24	500	436	0.87	-0.4	GOOD	
	ALPHA EFF	08:40	30	22229	741	-0.35	GOOD	
	BETA EFF	08:40	30	1.59E+05	5310	0.78	GOOD	
<u>LB4100A4</u>	ALPHA BKG	07:24	500	15.0	0.03	-0.48	GOOD	
	BETA BKG	07:24	500	1254	2.51	4.53	DETL	Outside 2 sigma for >= 2 days
	ALPHA EFF	08:40	30	18809	627	-2.8	GOOD	
	BETA EFF	08:40	30	1.72E+05	5740	1.6	GOOD	
LB4100B1	ALPHA BKG	07:24	500	7.00	0.01	-0.68	GOOD	
	BETA BKG	07:24	500	427	0.85	-0.25	GOOD	
	ALPHA EFF	08:40	30	20720	691	-1.2	GOOD	
	BETA EFF	08:40	30	1.89E+05	6280	0.51	GOOD	
LB4100B2	ALPHA BKG	07:24	500	13.0	0.03	-0.46	GOOD	
	BETA BKG	07:24	500	388	0.78	-0.28	GOOD	
	ALPHA EFF	08:40	30	20672	689	-0.47	GOOD	
	BETA EFF	08:40	30	1.64E+05	5460	0.13	GOOD	
LB4100B3	ALPHA BKG	07:24	500	16.0	0.03	-0.45	GOOD	
	BETA BKG	07:24	500	580	1.16	-0.33	GOOD	
	ALPHA EFF	08:40	30	15885	530	0.08	GOOD	
	BETA EFF	08:40	30	1.23E+05	4100	0.78	GOOD	
<u>LB4100B4</u>	ALPHA BKG	07:24	500	13.0	0.03	-0.44	GOOD	
	BETA BKG	07:24	500	2073	4.15	30.7	DETL	Outside 2 sigma for >= 2 days
	ALPHA EFF	08:40	30	18490	616	-0.58	GOOD	
	BETA EFF	08:40	30	1.56E+05	5190	1.07	GOOD	
LB4100C1	ALPHA BKG	07:24	500	121	0.24	-0.01	GOOD	
	BETA BKG	07:24	500	594	1.19	-0.3	GOOD	
	ALPHA EFF	08:40	30	21999	733	0.88	GOOD	
	BETA EFF	08:40	30	1.35E+05	4501	0.22	GOOD	
LB4100C2	ALPHA BKG	07:24	500	43.0	0.09	0.26	GOOD	
	BETA BKG	07:24	500	414	0.83	-0.58	GOOD	
	ALPHA EFF	08:40	30	22230	741	1	GOOD	

○ = Alpha Lockout
≡ = Alpha/Beta Lockout

	BETA EFF	08:40	30	1.95E+05	6510	1.32	GOOD	
LB4100C3	ALPHA BKG	07:24	500	19.0	0.04	-0.55	GOOD	
	BETA BKG	07:24	500	431	0.86	-0.14	GOOD	
	ALPHA EFF	08:40	30	16654	555	0.13	GOOD	
	BETA EFF	08:40	30	1.35E+05	4500	0.12	GOOD	
LB4100C4	ALPHA BKG	07:24	500	29.0	0.06	0.14	GOOD	
	BETA BKG	07:24	500	405	0.81	-0.07	GOOD	
	ALPHA EFF	08:40	30	25462	849	1.07	GOOD	
	BETA EFF	08:40	30	2.20E+05	7320	0.71	GOOD	
LB4100D1	ALPHA BKG	07:24	500	153	0.31	4.87	DETL	Outside 2 sigma for >= 2 days
	BETA BKG	07:24	500	468	0.94	0.79	GOOD	
	ALPHA EFF	08:40	30	26400	880	-0.58	GOOD	
	BETA EFF	08:40	30	2.39E+05	7970	0.36	GOOD	
LB4100D2	ALPHA BKG	07:24	500	70.0	0.14	-0.13	GOOD	
	BETA BKG	07:24	500	472	0.94	-0.35	GOOD	
	ALPHA EFF	08:40	30	19133	638	-0.6	GOOD	
	BETA EFF	08:40	30	1.49E+05	4980	-0.13	GOOD	
LB4100D3	ALPHA BKG	07:24	500	17.0	0.03	-0.39	GOOD	
	BETA BKG	07:24	500	380	0.76	-0.07	GOOD	
	ALPHA EFF	08:40	30	17942	598	-1.3	GOOD	
	BETA EFF	08:40	30	1.50E+05	5010	1.12	GOOD	
LB4100D4	ALPHA BKG	07:24	500	20.0	0.04	-0.79	GOOD	
	BETA BKG	07:24	500	441	0.88	-0.19	GOOD	
	ALPHA EFF	08:40	30	20675	689	-1.1	GOOD	
	BETA EFF	08:40	30	1.84E+05	6130	1.09	GOOD	
LB4100E1	ALPHA BKG	07:29	500	94.0	0.19	0.08	GOOD	
	BETA BKG	07:29	500	698	1.4	0.83	GOOD	
	ALPHA EFF	08:45	30	33059	1100	-0.81	GOOD	
	BETA EFF	08:45	30	2.15E+05	7153	0.95	GOOD	
LB4100E2	ALPHA BKG	07:29	500	68.0	0.14	0.19	GOOD	
	BETA BKG	07:29	500	748	1.5	-0.46	GOOD	
	ALPHA EFF	08:45	30	34280	1140	-0.76	GOOD	
	BETA EFF	08:45	30	2.93E+05	9764	1.06	GOOD	
LB4100E3	ALPHA BKG	07:29	500	29.0	0.06	-0.4	GOOD	
	BETA BKG	07:29	500	527	1.05	-0.1	GOOD	
	ALPHA EFF	08:45	30	35223	1170	-0.55	GOOD	
	BETA EFF	08:45	30	2.27E+05	7570	-0.83	GOOD	
LB4100E4	ALPHA BKG	07:29	500	54.0	0.11	-0.37	GOOD	
	BETA BKG	07:29	500	909	1.82	-0.21	GOOD	
	ALPHA EFF	08:45	30	30173	1010	-0.48	GOOD	
	BETA EFF	08:45	30	2.26E+05	7540	0.18	GOOD	
LB4100F1	ALPHA BKG	07:29	500	35.0	0.07	-0.14	GOOD	
	BETA BKG	07:29	500	586	1.17	1.93	GOOD	
	ALPHA EFF	08:45	30	28746	958	0.25	GOOD	

	BETA EFF	08:45	30	2.04E+05	6810	0.63	GOOD	
<u>LB4100F2</u>	ALPHA BKG	07:29	500	33.0	0.07	-0.99	GOOD	
	BETA BKG	07:29	500	651	1.3	1.59	GOOD	
	ALPHA EFF	08:45	30	27663	922	2.05	DETL	Outside 2 sigma for >= 2 days
	BETA EFF	08:45	30	2.18E+05	7270	-0.43	GOOD	
LB4100F3	ALPHA BKG	07:29	500	51.0	0.1	-1.1	GOOD	
	BETA BKG	07:29	500	668	1.34	-0.18	PEND	Good. Not a lockout condition. -526 4.9.06
	ALPHA EFF	08:45	30	28120	937	1.17	GOOD	
	BETA EFF	08:45	30	2.59E+05	8620	0.96	GOOD	
LB4100F4	ALPHA BKG	07:29	500	15.0	0.03	-0.34	GOOD	
	BETA BKG	07:29	500	353	0.71	-0.6	GOOD	
	ALPHA EFF	08:45	30	24315	811	-2.2	GOOD	
	BETA EFF	08:45	30	2.00E+05	6680	1.07	GOOD	
<u>LB4100G1</u>	ALPHA BKG	07:29	500	35.0	0.07	-1.6	GOOD	
	BETA BKG	07:29	500	1087	2.17	3.56	DETL	Outside 2 sigma for >= 2 days
	ALPHA EFF	08:45	30	31962	1070	0.69	GOOD	
	BETA EFF	08:45	30	2.22E+05	7410	0.13	GOOD	
<u>LB4100G2</u>	ALPHA BKG	07:29	500	33.0	0.07	0.14	GOOD	
	BETA BKG	07:29	500	695	1.39	5.45	DETL	Outside 2 sigma for >= 2 days
	ALPHA EFF	08:45	30	31128	1040	-0.71	GOOD	
	BETA EFF	08:45	30	2.87E+05	9550	0.51	GOOD	
LB4100G3	ALPHA BKG	07:29	500	103	0.21	0	GOOD	
	BETA BKG	07:29	500	546	1.09	0.7	GOOD	
	ALPHA EFF	08:45	30	22567	752	0.49	GOOD	
	BETA EFF	08:45	30	2.46E+05	8190	-0.17	GOOD	
LB4100G4	ALPHA BKG	07:29	500	14.0	0.03	-0.59	GOOD	
	BETA BKG	07:29	500	457	0.91	-0.21	GOOD	
	ALPHA EFF	08:45	30	15327	511	0.86	GOOD	
	BETA EFF	08:45	30	1.53E+05	5110	2.07	GOOD	
LB4100H1	ALPHA BKG	07:29	500	52.0	0.1	0.31	GOOD	
	BETA BKG	07:29	500	351	0.7	-0.12	GOOD	
	ALPHA EFF	08:45	30	29574	986	-0.62	GOOD	
	BETA EFF	08:45	30	1.42E+05	4730	-0.22	GOOD	
LB4100H2	ALPHA BKG	07:29	500	32.0	0.06	-0.21	GOOD	
	BETA BKG	07:29	500	401	0.8	-0.7	GOOD	
	ALPHA EFF	08:45	30	18426	614	-0.26	GOOD	
	BETA EFF	08:45	30	1.53E+05	5090	1.47	GOOD	
LB4100H3	ALPHA BKG	07:29	500	37.0	0.07	-0.84	GOOD	
	BETA BKG	07:29	500	400	0.8	-0.1	GOOD	
	ALPHA EFF	08:45	30	18611	620	-0.74	GOOD	
	BETA EFF	08:45	30	1.52E+05	5050	-0.32	GOOD	
LB4100H4	ALPHA BKG	07:29	500	35.0	0.07	-0.11	GOOD	
	BETA BKG	07:29	500	426	0.85	0.86	GOOD	
	ALPHA EFF	08:45	30	18047	602	-0.77	GOOD	

	BETA EFF	08:45	30	1.21E+05	4030	-0.81	GOOD
PIC1A	ALPHA BKG	07:15	500	47.0	0.09	-0.89	GOOD
	BETA BKG	07:15	500	211	0.42	-0.7	GOOD
	ALPHA EFF	08:01	30	9502	317	-1.8	GOOD
	BETA EFF	08:01	30	1.96E+05	6530	-0.05	GOOD
PIC1B	ALPHA BKG	07:15	500	30.0	0.06	-0.86	GOOD
	BETA BKG	07:15	500	181	0.36	-0.08	GOOD
	ALPHA EFF	08:02	30	10863	362	-2	GOOD
	BETA EFF	08:02	30	2.14E+05	7130	-0.3	GOOD
PIC1C	ALPHA BKG	07:16	500	35.0	0.07	-0.54	GOOD
	BETA BKG	07:16	500	217	0.43	0.28	GOOD
	ALPHA EFF	08:02	30	15512	517	-0.87	GOOD
	BETA EFF	08:02	30	2.46E+05	8190	0.69	GOOD
PIC1D	ALPHA BKG	07:16	500	20.0	0.04	-1.5	GOOD
	BETA BKG	07:16	500	177	0.35	-0.64	GOOD
	ALPHA EFF	08:02	30	16778	559	-0.21	GOOD
	BETA EFF	08:02	30	1.89E+05	6310	0.65	GOOD
PIC2A	ALPHA BKG	07:16	500	38.0	0.08	-0.45	GOOD
	BETA BKG	07:16	500	203	0.41	-0.37	GOOD
	ALPHA EFF	08:02	30	15509	517	-1.5	GOOD
	BETA EFF	08:02	30	2.32E+05	7740	0.65	GOOD
PIC2B	ALPHA BKG	07:16	500	21.0	0.04	-0.87	GOOD
	BETA BKG	07:16	500	121	0.24	-0.72	GOOD
	ALPHA EFF	08:02	30	13511	450	-2.1	GOOD
	BETA EFF	08:02	30	2.30E+05	7660	0.89	GOOD
PIC2C	ALPHA BKG	07:16	500	36.0	0.07	-0.89	GOOD
	BETA BKG	07:16	500	175	0.35	-0.18	GOOD
	ALPHA EFF	08:03	30	19055	635	-0.59	GOOD
	BETA EFF	08:03	30	1.93E+05	6450	0.34	GOOD
PIC2D	ALPHA BKG	07:16	500	31.0	0.06	-1	GOOD
	BETA BKG	07:16	500	229	0.46	0.33	GOOD
	ALPHA EFF	08:03	30	16962	565	-1.3	GOOD
	BETA EFF	08:03	30	2.24E+05	7480	1.02	GOOD
PIC3A	ALPHA BKG	07:17	500	23.0	0.05	-1.7	GOOD
	BETA BKG	07:17	500	181	0.36	-0.58	GOOD
	ALPHA EFF	08:03	30	21859	729	-1.7	GOOD
	BETA EFF	08:03	30	1.79E+05	5970	1.64	GOOD
PIC3B	ALPHA BKG	07:17	500	35.0	0.07	-1.1	GOOD
	BETA BKG	07:17	500	191	0.38	-0.42	GOOD
	ALPHA EFF	08:03	30	21118	704	-0.54	GOOD
	BETA EFF	08:03	30	1.96E+05	6530	0.16	GOOD
PIC3C	ALPHA BKG	07:17	500	28.0	0.06	-1.1	GOOD
	BETA BKG	07:17	500	217	0.43	0.19	GOOD
	ALPHA EFF	08:03	30	17257	575	-1.3	GOOD

	BETA EFF	08:03	30	2.12E+05	7070	0.55	GOOD
PIC3D	ALPHA BKG	07:17	500	27.0	0.05	-1.4	GOOD
	BETA BKG	07:17	500	208	0.42	-0.14	GOOD
	ALPHA EFF	08:03	30	24798	827	-1.4	GOOD
	BETA EFF	08:03	30	2.14E+05	7130	-0.71	GOOD
PIC4A	ALPHA BKG	07:18	500	28.0	0.06	-1	GOOD
	BETA BKG	07:18	500	196	0.39	-0.64	GOOD
	ALPHA EFF	08:03	30	12529	418	-1.7	GOOD
	BETA EFF	08:03	30	1.76E+05	5860	0.98	GOOD
PIC4B	ALPHA BKG	07:18	500	84.0	0.17	1.33	GOOD
	BETA BKG	07:18	500	227	0.45	0.03	GOOD
	ALPHA EFF	08:04	30	17575	586	-2.8	GOOD
	BETA EFF	08:04	30	2.23E+05	7450	0.43	GOOD
PIC4C	ALPHA BKG	07:18	500	31.0	0.06	-1.2	GOOD
	BETA BKG	07:18	500	198	0.4	-0.34	GOOD
	ALPHA EFF	08:04	30	20082	669	-1.7	GOOD
	BETA EFF	08:04	30	2.02E+05	6740	1.04	GOOD
PIC4D	ALPHA BKG	07:18	500	66.0	0.13	0.03	GOOD
	BETA BKG	07:18	500	222	0.44	0.01	GOOD
	ALPHA EFF	08:04	30	20463	682	-1.3	GOOD
	BETA EFF	08:04	30	2.13E+05	7090	1.55	GOOD
PIC5A	ALPHA BKG	07:19	500	26.0	0.05	-0.51	GOOD
	BETA BKG	07:19	500	183	0.37	-0.44	GOOD
	ALPHA EFF	08:04	30	11612	387	-0.21	GOOD
	BETA EFF	08:04	30	3.98E+05	13300	-1.5	GOOD
PIC5B	ALPHA BKG	07:19	500	38.0	0.08	-0.11	GOOD
	BETA BKG	07:19	500	1105	2.21	0.62	RE RUN GOOD. Not a lockout condition. -SRB 4.9.06
	ALPHA EFF	08:04	30	10410	347	-0.01	GOOD
	BETA EFF	08:04	30	3.50E+05	11700	0.1	GOOD
PIC5C	ALPHA BKG	07:19	500	29.0	0.06	0.69	GOOD
	BETA BKG	07:19	500	140	0.28	-1	GOOD
	ALPHA EFF	08:05	30	10569	352	-0.18	GOOD
	BETA EFF	08:05	30	3.88E+05	12900	-1.1	GOOD
PIC5D	ALPHA BKG	07:19	500	19.0	0.04	-0.21	GOOD
	BETA BKG	07:19	500	178	0.36	0.3	GOOD
	ALPHA EFF	08:05	30	9088	303	-0.3	GOOD
	BETA EFF	08:05	30	3.09E+05	10300	-1.6	GOOD
PIC6A	ALPHA BKG	07:20	500	21.0	0.04	-0.32	GOOD
	BETA BKG	07:20	500	127	0.25	-1	GOOD
	ALPHA EFF	08:05	30	8130	271	-0.24	GOOD
	BETA EFF	08:05	30	2.80E+05	9350	-1.2	GOOD
PIC6B	ALPHA BKG	07:20	500	15.0	0.03	-0.52	GOOD
	BETA BKG	07:20	500	141	0.28	0.13	GOOD
	ALPHA EFF	08:05	30	10342	345	-0.49	GOOD

	BETA EFF	08:05	30	2.89E+05	9630	-1.7	GOOD	
PIC6C	ALPHA BKG	07:20	500	26.0	0.05	0.14	GOOD	
	BETA BKG	07:20	500	120	0.24	-0.56	GOOD	
	ALPHA EFF	08:05	30	14858	495	-0.14	GOOD	
	BETA EFF	08:05	30	3.50E+05	11700	-1.9	PEND Good. Not a lockout condition. -SRB 4.9.06	
PIC6D	ALPHA BKG	07:20	500	18.0	0.04	-0.24	GOOD	
	BETA BKG	07:20	500	186	0.37	0.07	GOOD	
	ALPHA EFF	08:06	30	11491	383	-0.19	GOOD	
	BETA EFF	08:06	30	3.59E+05	12000	-0.98	GOOD	
PIC7A	ALPHA BKG	07:20	500	33.0	0.07	-0.58	GOOD	
	BETA BKG	07:20	500	187	0.37	-0.64	GOOD	
	ALPHA EFF	08:06	30	9836	328	-0.5	GOOD	
	BETA EFF	08:06	30	3.77E+05	12600	-1.5	GOOD	
PIC7B	ALPHA BKG	07:20	500	133	0.27	-0.5	GOOD	
	BETA BKG	07:20	500	295	0.59	-0.43	GOOD	
	ALPHA EFF	08:06	30	10336	345	-0.43	GOOD	
	BETA EFF	08:06	30	3.18E+05	10600	-0.5	GOOD	
PIC7C	ALPHA BKG	07:21	500	48.0	0.1	-0.59	GOOD	
	BETA BKG	07:21	500	182	0.36	-0.82	GOOD	
	ALPHA EFF	08:06	30	11813	394	-0.15	GOOD	
	BETA EFF	08:06	30	3.82E+05	12700	-0.32	GOOD	
PIC7D	ALPHA BKG	07:21	500	62.0	0.12	-0.65	GOOD	
	BETA BKG	07:21	500	172	0.34	-0.62	GOOD	
	ALPHA EFF	08:06	30	8403	280	-0.29	GOOD	
	BETA EFF	08:06	30	2.81E+05	9370	-0.44	GOOD	
PIC8A	ALPHA BKG	07:21	500	52.0	0.1	-0.5	GOOD	
	BETA BKG	07:21	500	236	0.47	-0.74	GOOD	
	ALPHA EFF	08:06	30	12930	431	-0.09	GOOD	
	BETA EFF	08:06	30	3.73E+05	12400	-1.3	GOOD	
PIC8B	ALPHA BKG	07:21	500	26.0	0.05	-0.53	GOOD	
	BETA BKG	07:21	500	443	0.89	-0.36	GOOD	
	ALPHA EFF	08:06	30	9633	321	-0.56	GOOD	
	BETA EFF	08:06	30	3.70E+05	12300	-0.4	GOOD	
PIC8C	ALPHA BKG	07:21	500	101	0.2	-0.73	GOOD	
	BETA BKG	07:21	500	224	0.45	-0.46	GOOD	
	ALPHA EFF	08:07	30	14869	496	-0.03	GOOD	
	BETA EFF	08:07	30	4.27E+05	14200	-0.52	GOOD	
PIC8D	ALPHA BKG	07:22	500	94.0	0.19	-0.52	GOOD	
	BETA BKG	07:22	500	591	1.18	-0.43	GOOD	
	ALPHA EFF	08:07	30	11449	382	2.12	DETL	Outside 2 sigma for >= 2 days
	BETA EFF	08:07	30	3.72E+05	12400	0.16	GOOD	

Reviewed by SRB

Date 4.9.06

General Engineering Laboratories, LLC

Starting with bank 1
Ending with bank 19

	Detector	Parameter	Flag
7-APR-2006	2	PSFWHM-5000	Above
7-APR-2006	6	PSFWHM-5000	Below
7-APR-2006	6	PSENERGY-5000	Above
7-APR-2006	6	PSCENTRD-5000	Above
7-APR-2006	14	PSFWHM-5000	Below
7-APR-2006	14	PSENERGY-5000	Above
7-APR-2006	22	PSENERGY-5000	Above
7-APR-2006	24	PSFWHM-5000	Below
7-APR-2006	25	PSFWHM-5000	Below
7-APR-2006	25	PSCENTRD-5000	Below
7-APR-2006	39	PSENERGY-5000	Above
7-APR-2006	67	PSFWHM-5000	Above
7-APR-2006	68	PSFWHM-5000	Above
7-APR-2006	71	PSENERGY-5000	Above
7-APR-2006	74	PSENERGY-5000	Above
7-APR-2006	84	PSENERGY-5000	Above
7-APR-2006	97	PSENERGY-5000	Above
7-APR-2006	105	PSENERGY-5000	Above
7-APR-2006	106	PSFWHM-5000	Above
7-APR-2006	115	PSFWHM-5000	Above
7-APR-2006	131	PSFWHM-5000	Above

DETECTORS NOT LISTED HAVE PASSED ALL QUALITY ASSURANCE PARAMETERS

APPROVAL DATE: 4/7/06

APPROVAL TIME: 730

APPROVED BY: *CD*

PROCEDURE # GL-RAD-I-009

Report completed at 7-APR-2006 01:09:37.42

Review of QA results (Daily checks) 7-APR-2006 01:09:40.11

Starting with bank 1

Ending with bank 19

This is a list of Detectors that may not have properly transferred to the QA file

APPROVAL DATE: 4/7/06 APPROVAL TIME: 730

APPROVED BY:  PROCEDURE # GL-RAD-I-009

Report completed at 7-APR-2006 01:12:21.24

Starting with bank 1

Ending with bank 19

	Detector	Parameter	Flag
8-APR-2006	4	PSFWHM-5000	Above
8-APR-2006	6	PSFWHM-5000	Below
8-APR-2006	6	PSENERGY-5000	Above
8-APR-2006	6	PSCENTRD-5000	Above
8-APR-2006	12	PSFWHM-5000	Above
8-APR-2006	14	PSFWHM-5000	Below
8-APR-2006	14	PSENERGY-5000	Above
8-APR-2006	22	PSENERGY-5000	Above
8-APR-2006	24	PSFWHM-5000	Below
8-APR-2006	25	PSFWHM-5000	Below
8-APR-2006	25	PSCENTRD-5000	Below
8-APR-2006	39	PSENERGY-5000	Above
8-APR-2006	67	PSFWHM-5000	Above
8-APR-2006	68	PSFWHM-5000	Above
8-APR-2006	71	PSFWHM-5000	Below
8-APR-2006	71	PSENERGY-5000	Above
8-APR-2006	74	PSENERGY-5000	Above
8-APR-2006	84	PSENERGY-5000	Above
8-APR-2006	88	PSFWHM-5000	Above
8-APR-2006	97	PSENERGY-5000	Above
8-APR-2006	105	PSENERGY-5000	Above
8-APR-2006	108	PSFWHM-5000	Above

8-APR-2006	109	PSFWHM-5000	Above
8-APR-2006	115	PSFWHM-5000	Above
8-APR-2006	131	PSFWHM-5000	Above

DETECTORS NOT LISTED HAVE PASSED ALL QUALITY ASSURANCE PARAMETERS

APPROVAL DATE: 4.8.06 APPROVAL TIME: 8:35

APPROVED BY: SRB PROCEDURE # GL-RAD-I-009

Report completed at 8-APR-2006 08:31:20.96

Review of QA results (Daily checks) 8-APR-2006 08:31:22.10

Starting with bank 1
Ending with bank 19

This is a list of Detectors that may not have properly transferred to the QA file

APPROVAL DATE: 4.8.06 APPROVAL TIME: 8:35

APPROVED BY: SLB PROCEDURE # GL-RAD-I-009

Report completed at 8-APR-2006 08:32:07.39

QA filename : DKA300:[CANBERRA.GAMMA]QC_GAMMA16.QAF;2
 Sample ID : QC_GAMMA16 Sample quantity : 1.00 LITER
 Sample date : 1-APR-2004 12:00:00 Acquisition date : 10-APR-2006 05:34:07
 Elapsed live time: 0 00:05:00.00 Elapsed real time: 0 00:05:02.14

Out-of-range Test: BOUNDARY

Parameter Description	Lower	Upper	Value	Flag
PEAK CENTROID (CHANS) CD-109	172	180	174	
PEAK CENTROID (CHANS) CS-137	1319	1327	1320	
PEAK CENTROID (CHANS) CO-60	2661	2669	2660	Below*
*PEAK ENERGY (keV) CD-109	86	90	88	
*PEAK ENERGY (keV) CS-137	660	664	661	
*PEAK ENERGY (keV) CO-60	1330	1334	1331	
*PEAK FWHM (keV) CD-109	0.1	2.0	1.1	
*PEAK FWHM (keV) CS-137	0.1	3.0	1.5	
*PEAK FWHM (keV) CO-60	0.1	3.0	2.0	
DECAY CORR ACTIVITY (pCi) CD-109	7.41E+05	9.05E+05	7.59E+05	
DECAY CORR ACTIVITY (pCi) CS-137	2.24E+04	2.74E+04	2.52E+04	
DECAY CORR. ACTIVITY (pCi) CO-60	3.55E+04	4.34E+04	4.11E+04	

Flags: "*" means the out-of-range test is parameter-dependent

Approved by: *mm* Approval Date: 4 / 10 / 06

** PEAK ENERGY WITHIN LIMITS.*

QA filename : DKA300:[CANBERRA.GAMMA]QC_GAMMA13.QAF;3

Sample ID : QC_GAMMA13 Sample quantity : 1.00 LITER
 Sample date : 1-APR-2002 12:00:00 Acquisition date : 11-APR-2006 08:40:21
 Elapsed live time: 0 00:05:00.00 Elapsed real time: 0 00:05:03.01

Out-of-range Test: BOUNDARY

Parameter Description	Lower	Upper	Value	Flag
PEAK CENTROID (CHANS) CD-109	174	182	178	
PEAK CENTROID (CHANS) CS-137	1320	1328	1324	
PEAK CENTROID (CHANS) CO-60	2660	2668	2663	
*PEAK ENERGY (keV) CD-109	86	90	88	
*PEAK ENERGY (keV) CS-137	660	664	661	
*PEAK ENERGY (keV) CO-60	1330	1334	1331	
*PEAK FWHM (keV) CD-109	0.1	2.0	1.0	
*PEAK FWHM (keV) CS-137	0.1	3.0	1.5	
*PEAK FWHM (keV) CO-60	0.1	3.0	2.1	
DECAY CORR ACTIVITY (pCi) CD-109	7.61E+05	9.30E+05	9.04E+05	
DECAY CORR ACTIVITY (pCi) CS-137	2.92E+04	3.24E+04	3.10E+04	
DECAY CORR. ACTIVITY (pCi) CO-60	3.68E+04	4.50E+04	4.34E+04	

Flags: "*" means the out-of-range test is parameter-dependent

Approved by: my Approval Date: 4 / 11 / 06

QA filename : DKA300:[CANBERRA.GAMMA]QC_GAMMA16.QAF;2

Sample ID : QC_GAMMA16 Sample quantity : 1.00 LITER
 Sample date : 1-APR-2004 12:00:00 Acquisition date : 11-APR-2006 06:03:19
 Elapsed live time: 0 00:05:00.00 Elapsed real time: 0 00:05:02.14

Out-of-range Test: BOUNDARY

Parameter Description	Lower	Upper	Value	Flag
PEAK CENTROID (CHANS) CD-109	172	180	174	
PEAK CENTROID (CHANS) CS-137	1319	1327	1320	
PEAK CENTROID (CHANS) CO-60	2661	2669	2660	Below*
*PEAK ENERGY (keV) CD-109	86	90	88	
*PEAK ENERGY (keV) CS-137	660	664	661	
*PEAK ENERGY (keV) CO-60	1330	1334	1331	
*PEAK FWHM (keV) CD-109	0.1	2.0	1.1	
*PEAK FWHM (keV) CS-137	0.1	3.0	1.5	
*PEAK FWHM (keV) CO-60	0.1	3.0	1.8	
DECAY CORR ACTIVITY (pCi) CD-109	7.41E+05	9.05E+05	7.69E+05	
DECAY CORR ACTIVITY (pCi) CS-137	2.24E+04	2.74E+04	2.46E+04	
DECAY CORR. ACTIVITY (pCi) CO-60	3.55E+04	4.34E+04	4.14E+04	

Flags: "*" means the out-of-range test is parameter-dependent


Approved by: Approval Date: 4 / 11 / 06

** Peak Energy within bounds.*


BACKGROUND AND EFFICIENCY DATA

PIC2A 04/13/2006


Alpha BKG

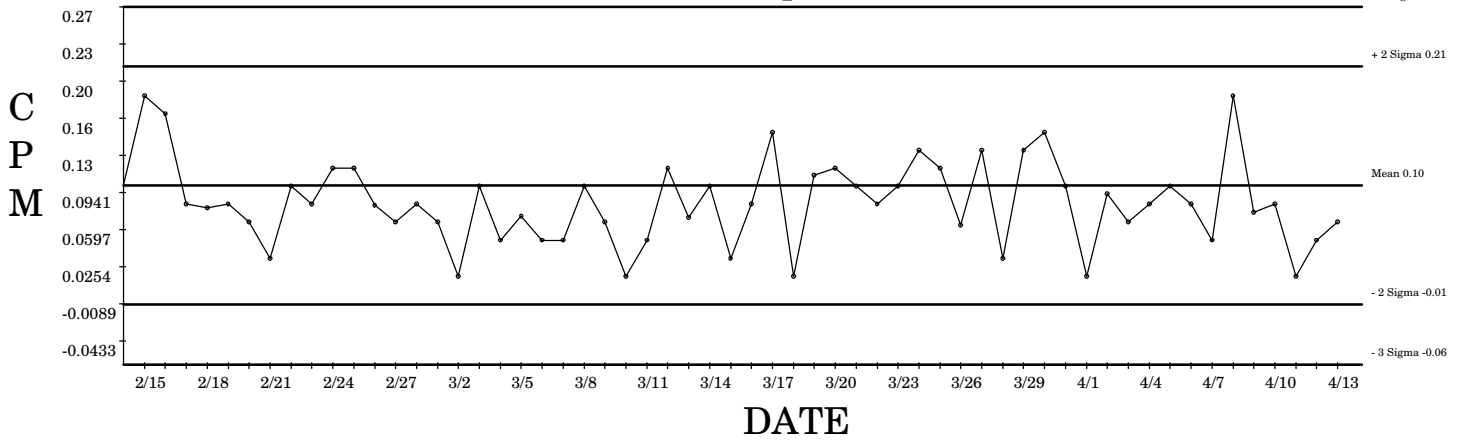


Beta BKG

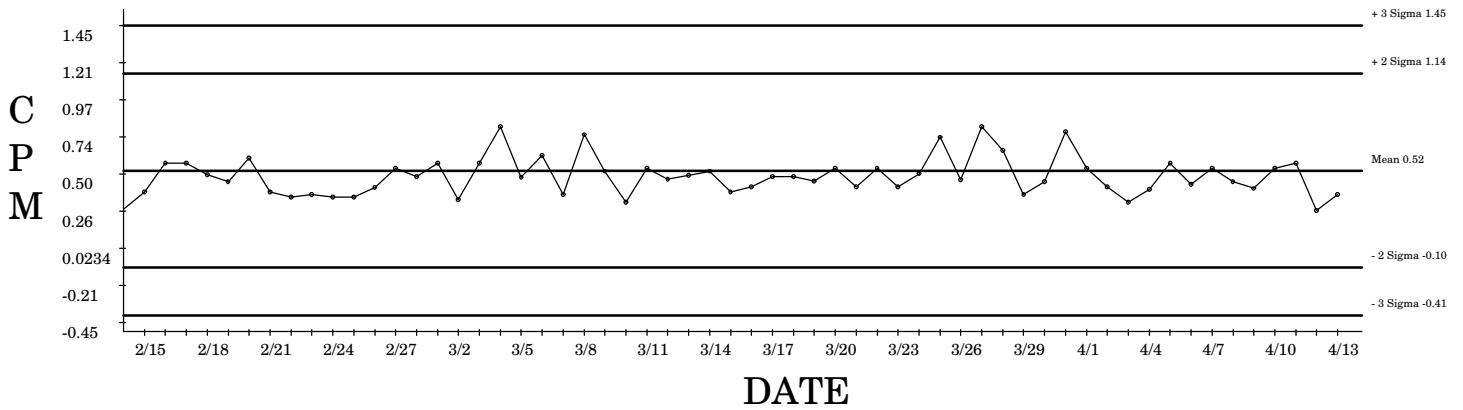

Alpha EFF

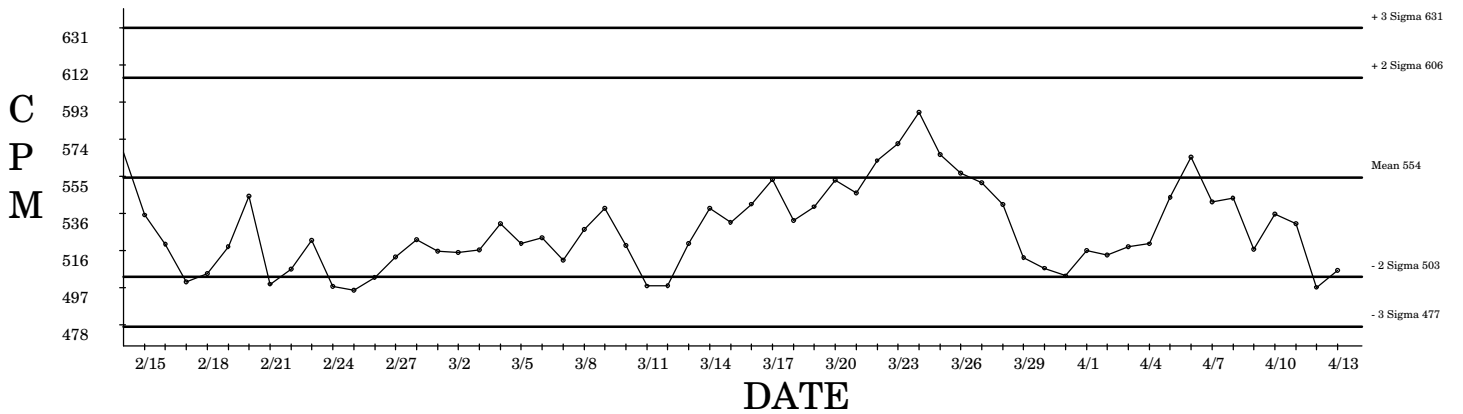


Beta EFF

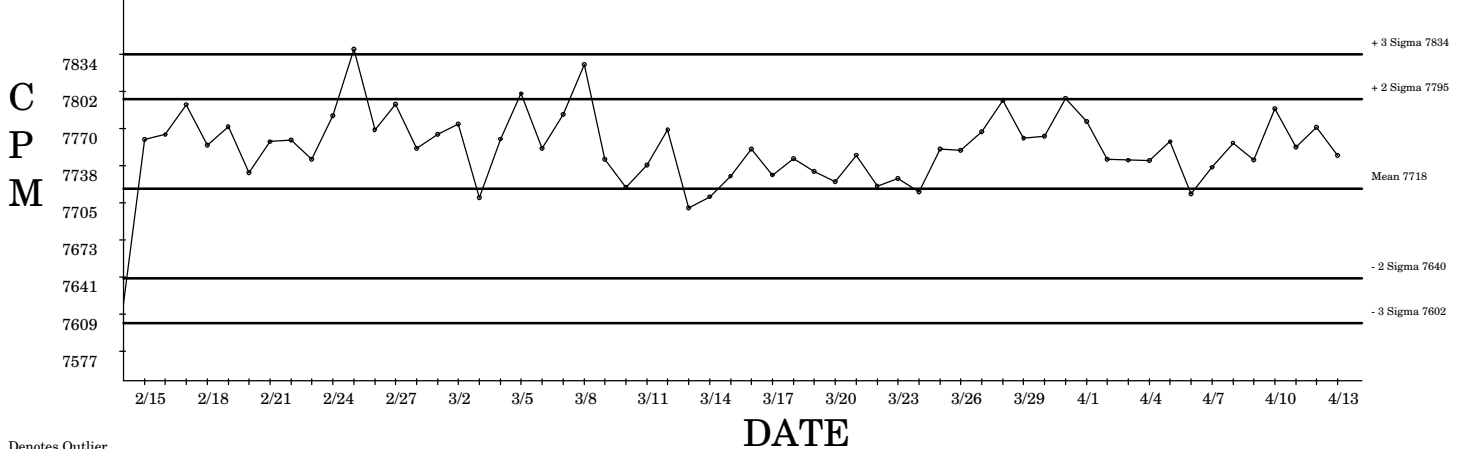


○ Denotes Outlier

PIC2B 04/09/2006


Alpha BKG

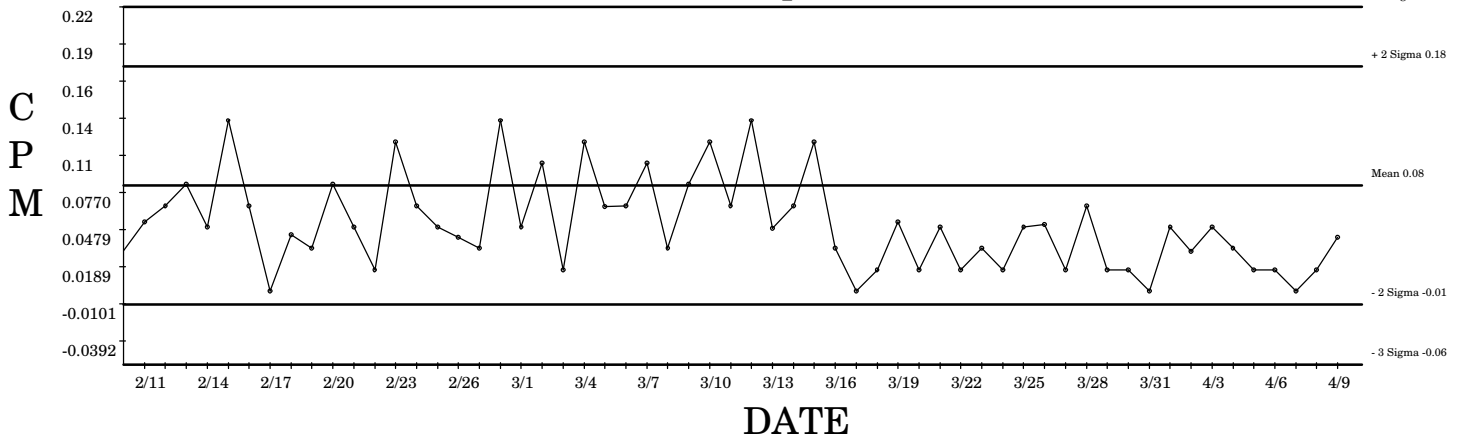


Beta BKG

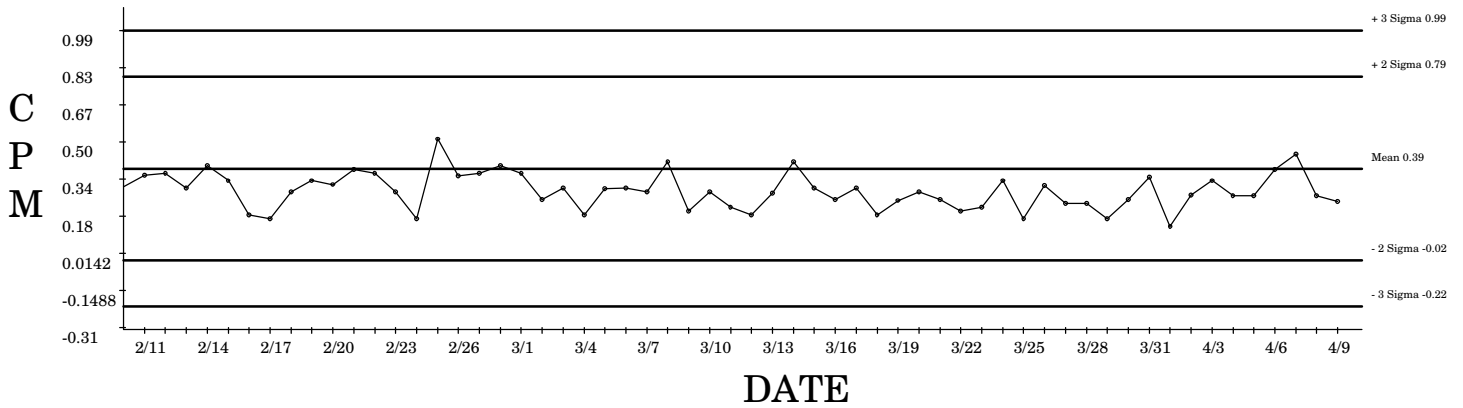

Alpha EFF

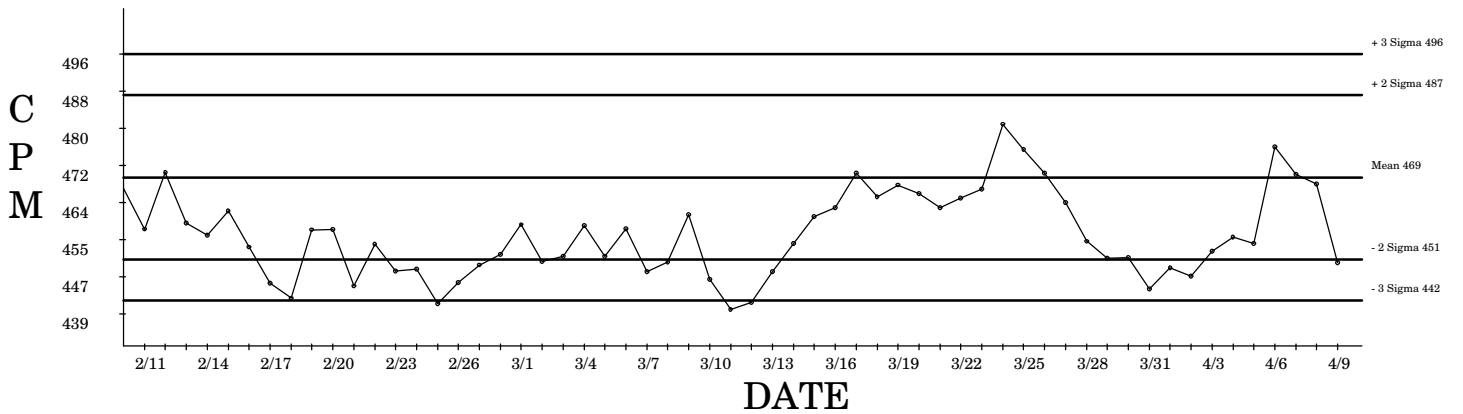


Beta EFF

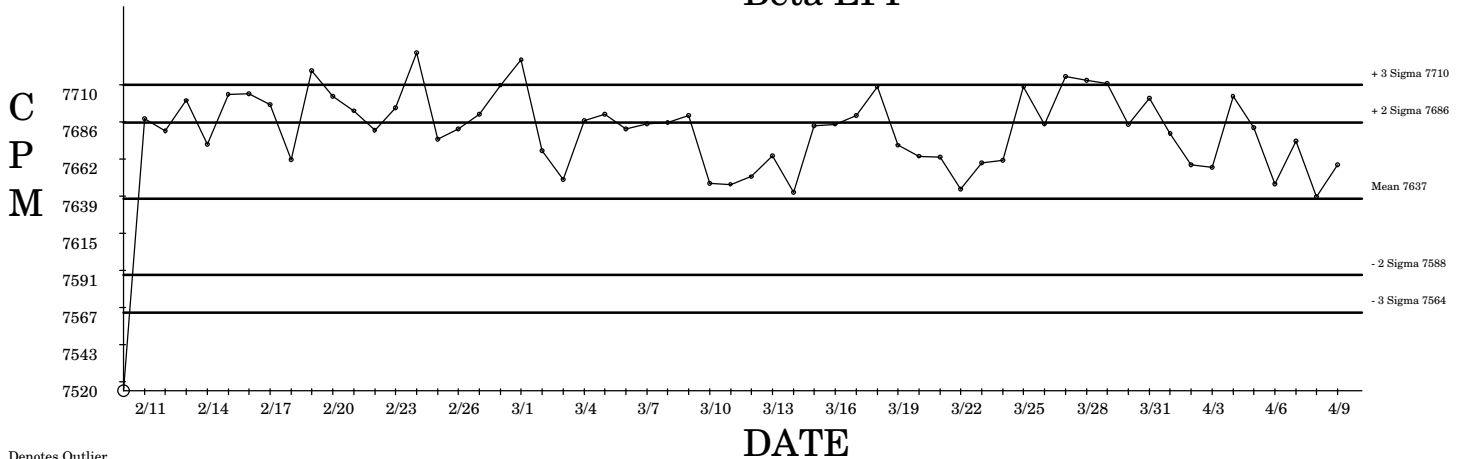


○ Denotes Outlier

PIC2C 04/09/2006


Alpha BKG

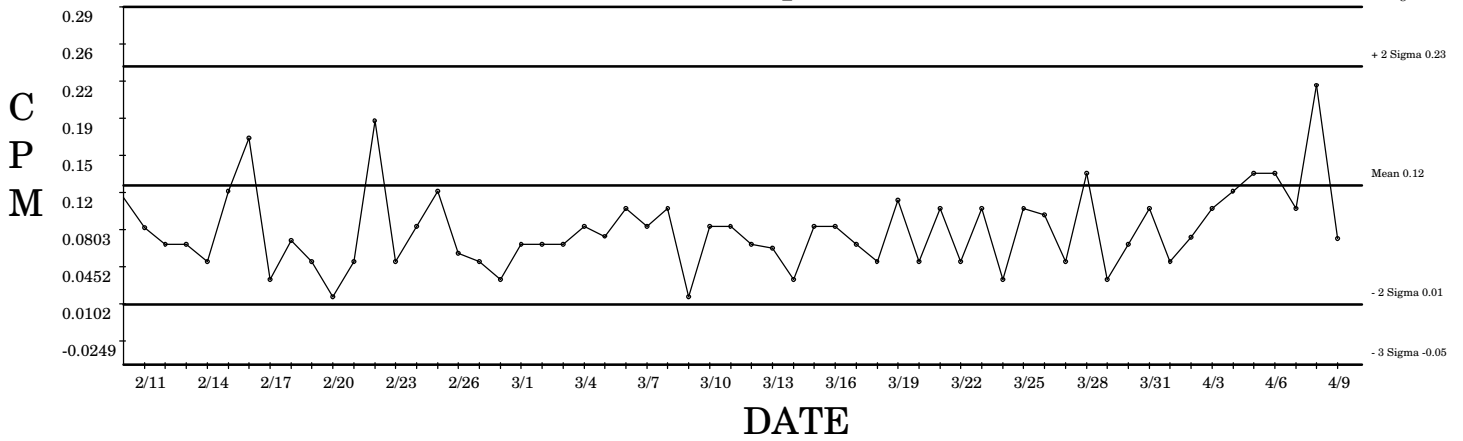


Beta BKG

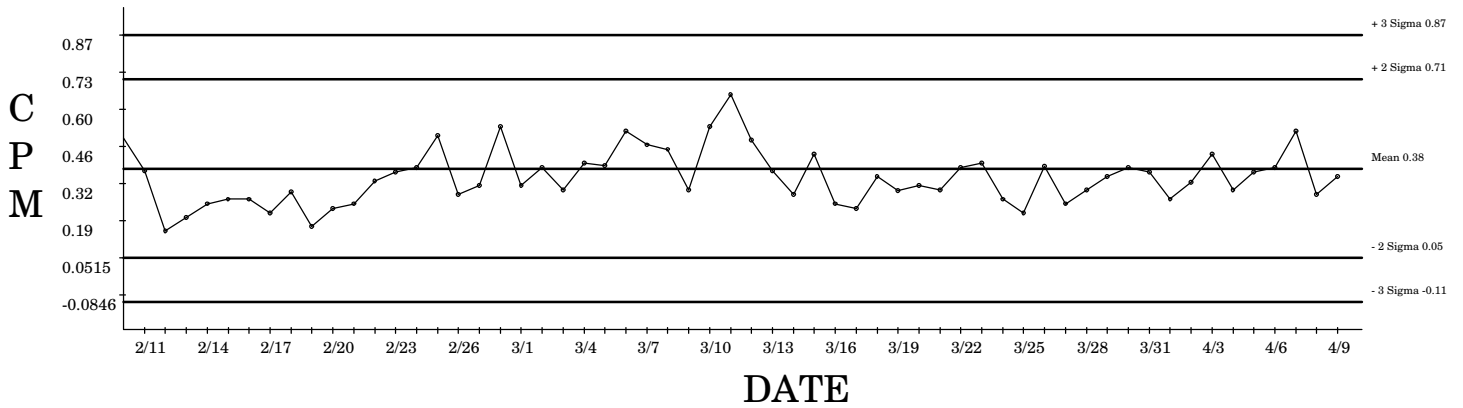

Alpha EFF

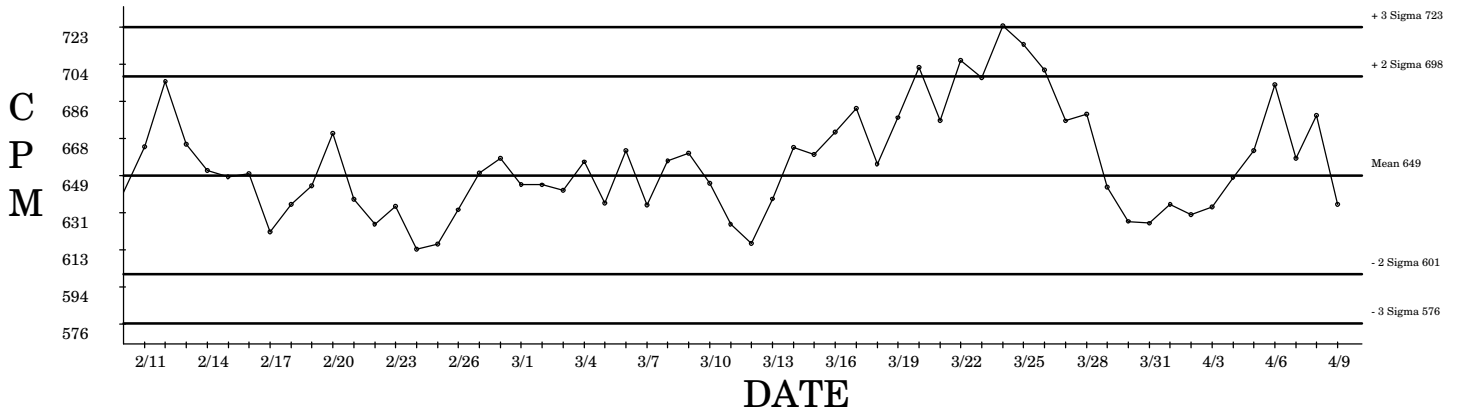


Beta EFF

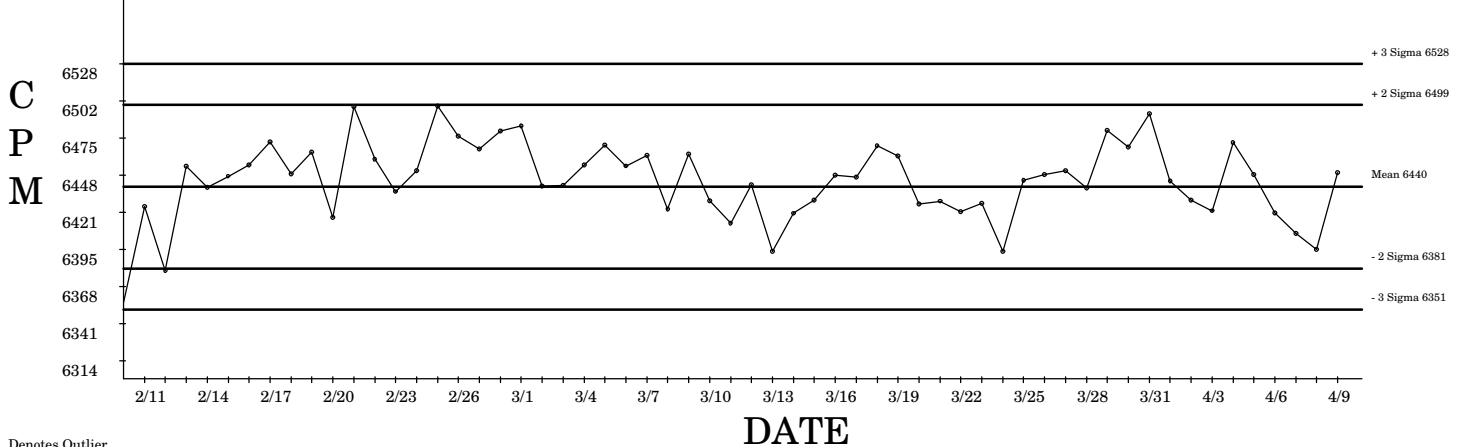


○ Denotes Outlier

PIC2D 04/09/2006


Alpha BKG

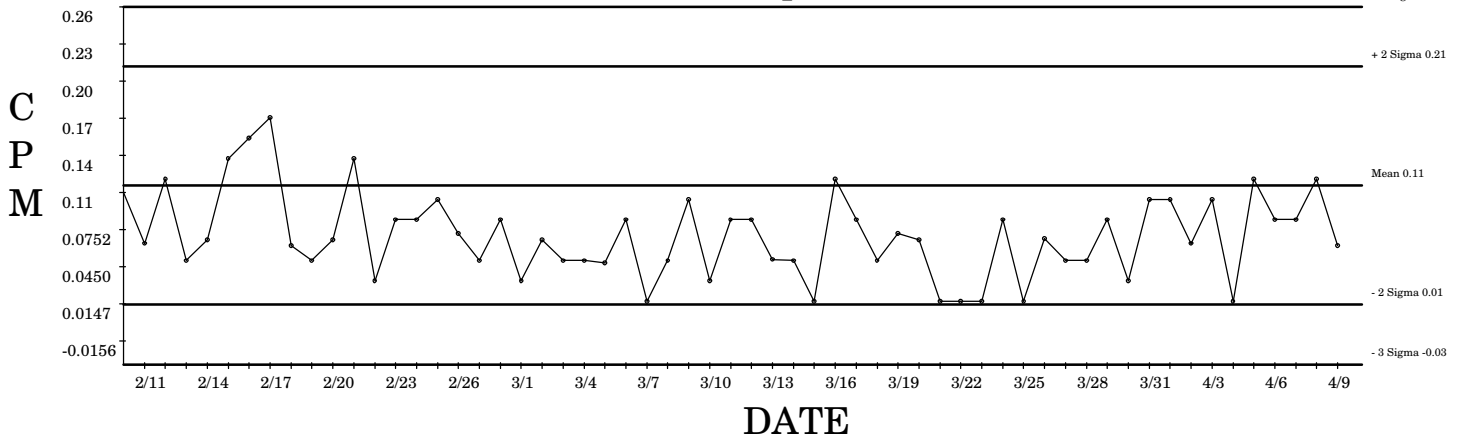


Beta BKG

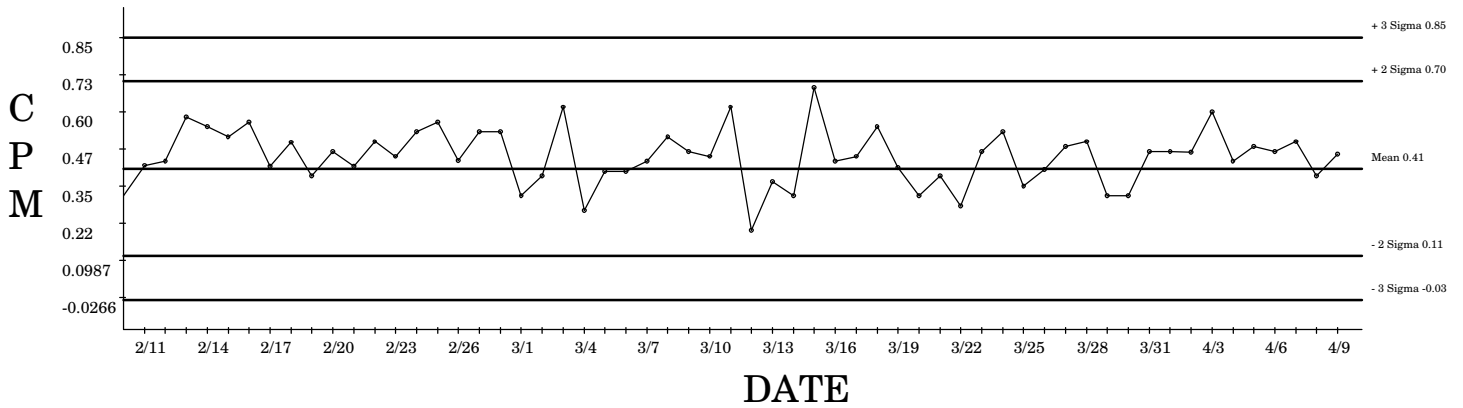

Alpha EFF

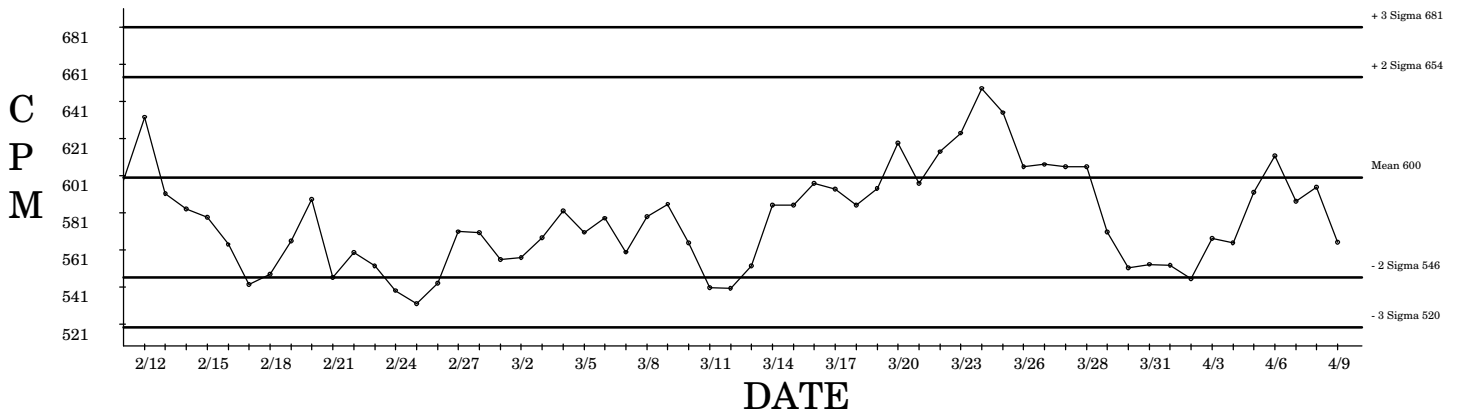


Beta EFF

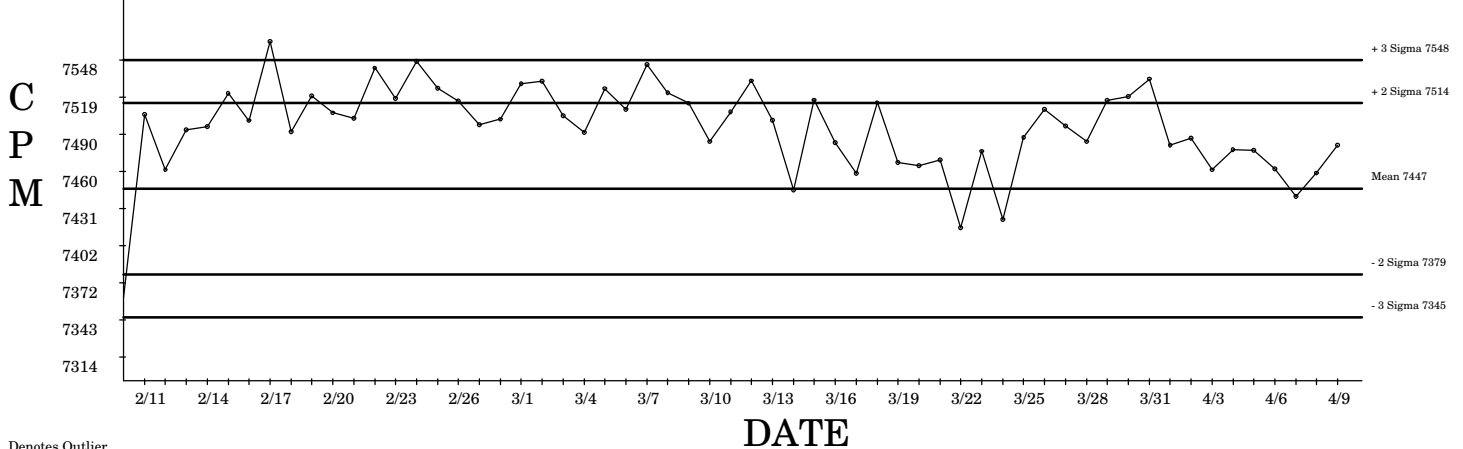


○ Denotes Outlier

PIC3B 04/09/2006


Alpha BKG

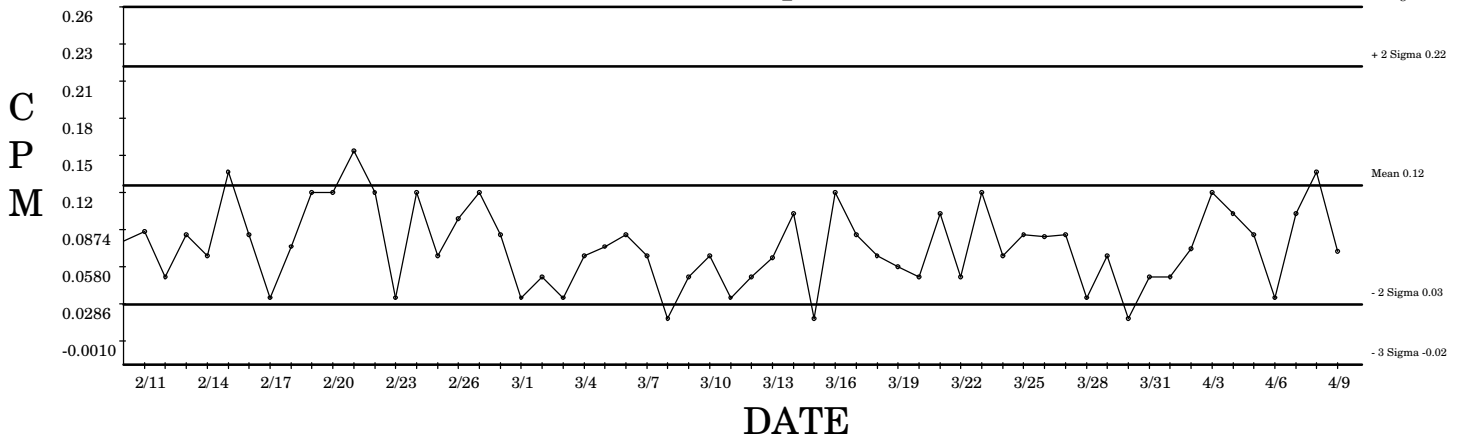


Beta BKG

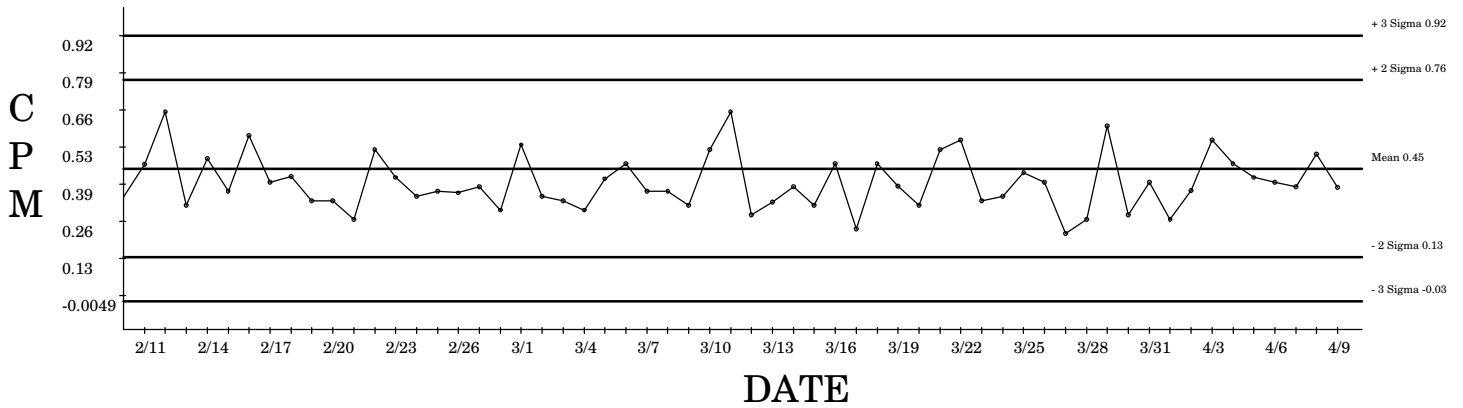

Alpha EFF

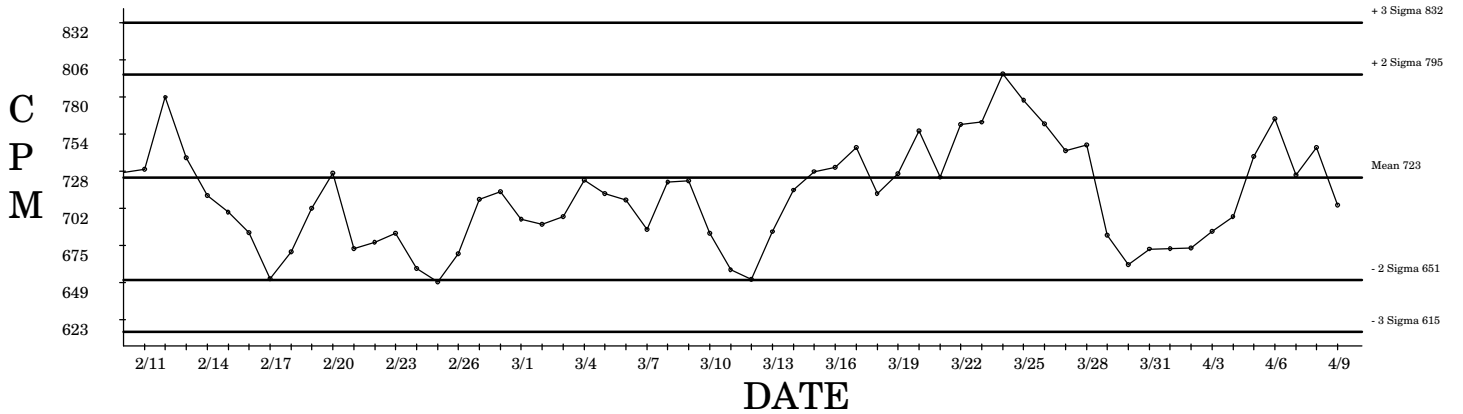


Beta EFF

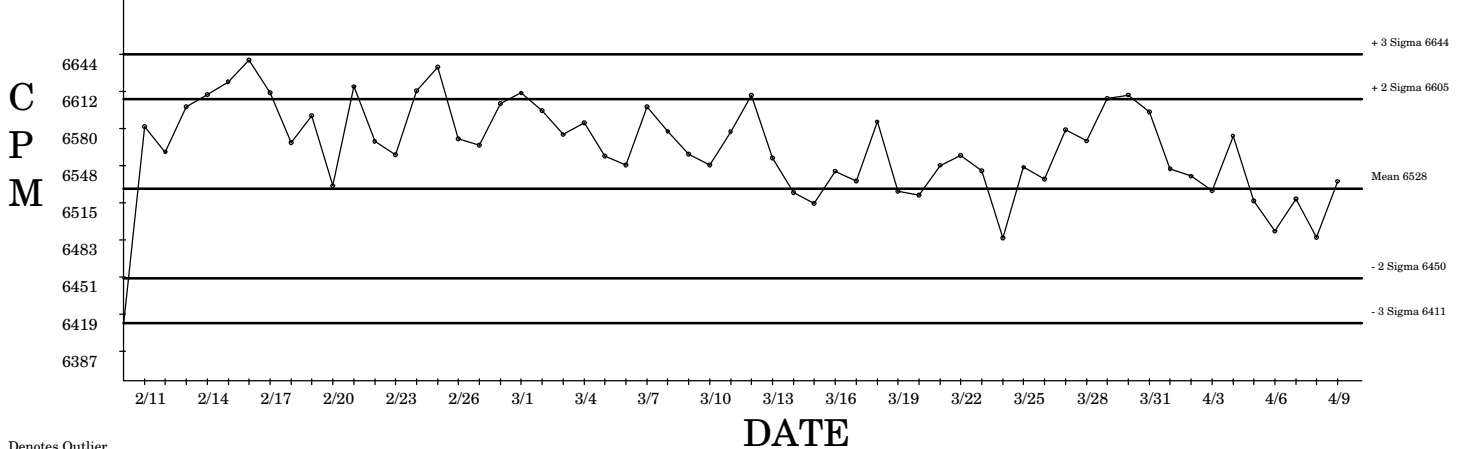


○ Denotes Outlier


PIC3C 04/09/2006
Alpha BKG

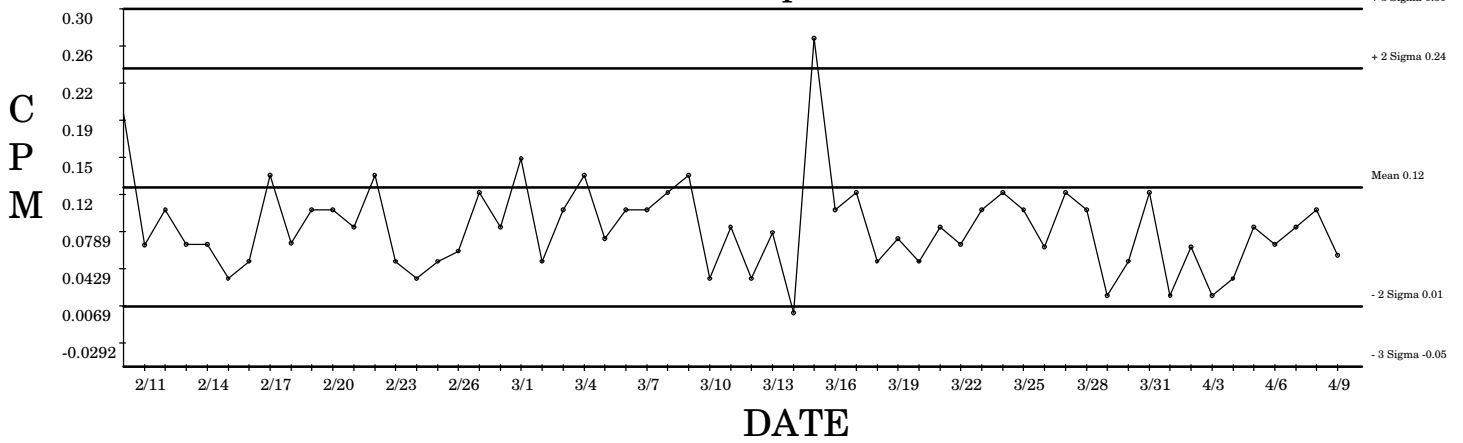


Beta BKG

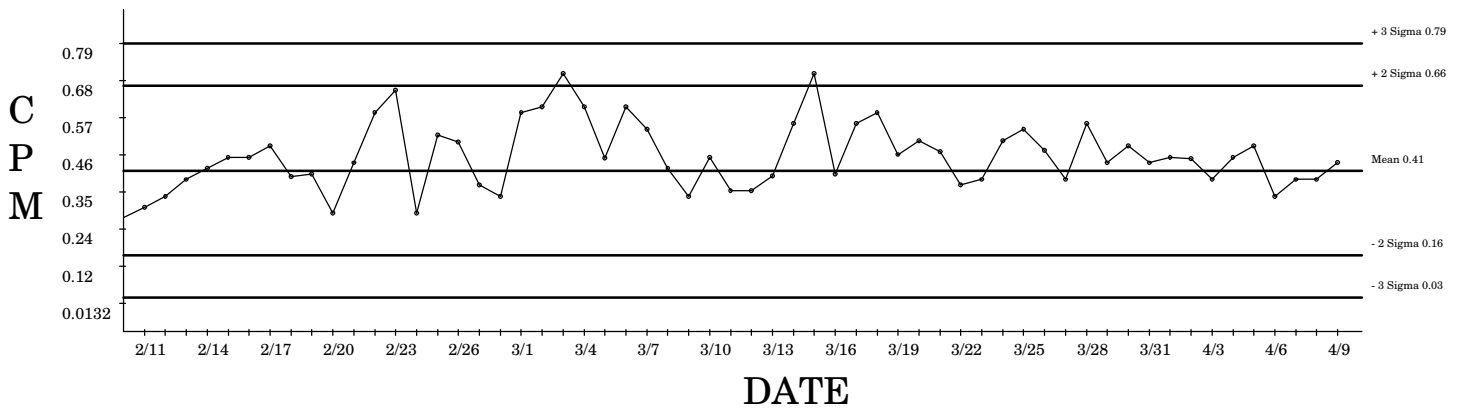

Alpha EFF

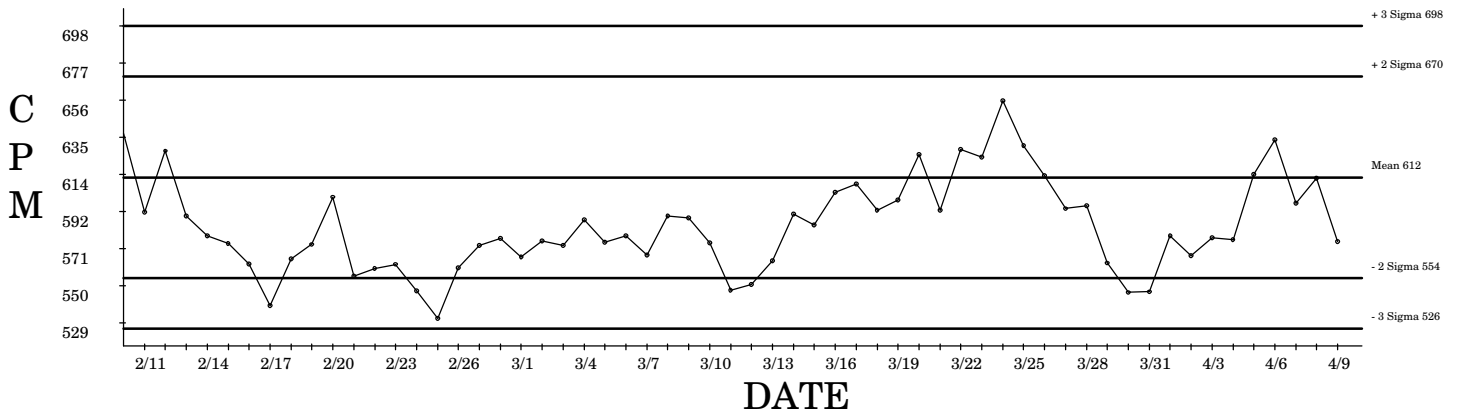


Beta EFF

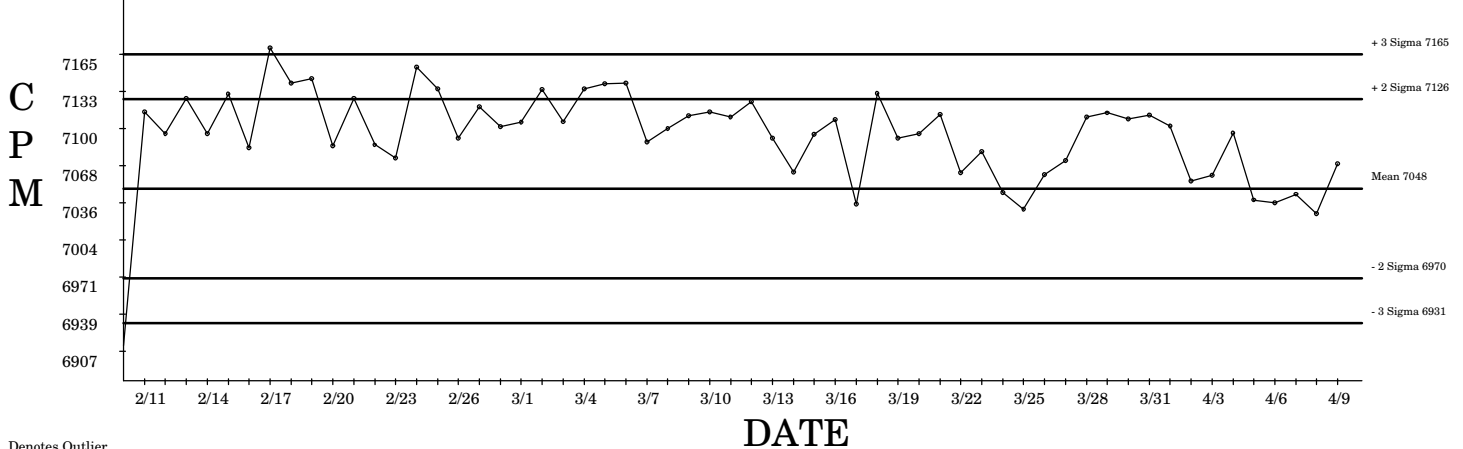


○ Denotes Outlier

PIC3D 04/09/2006


Alpha BKG

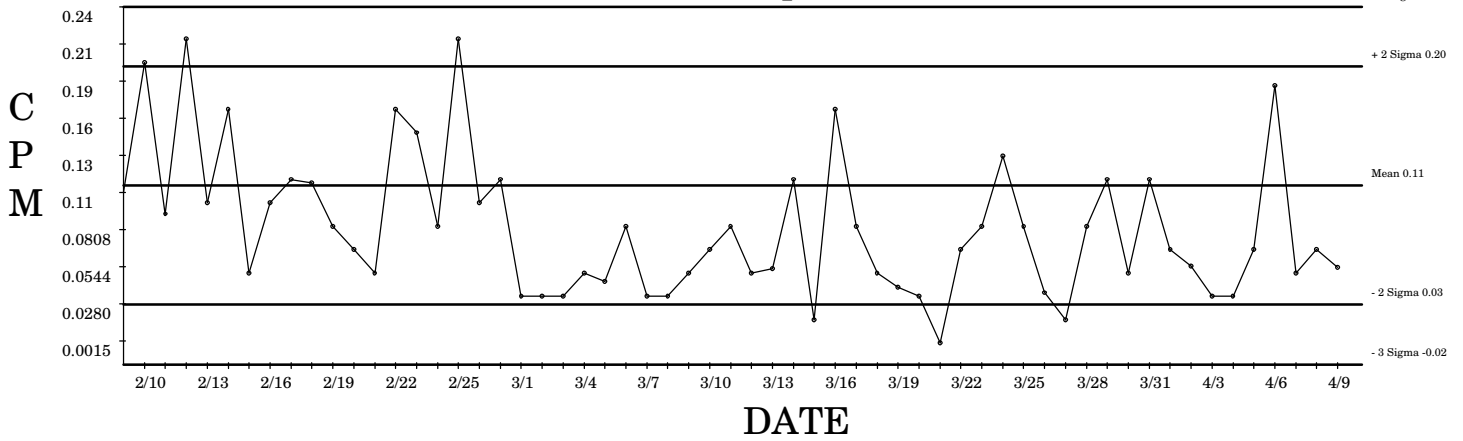


Beta BKG

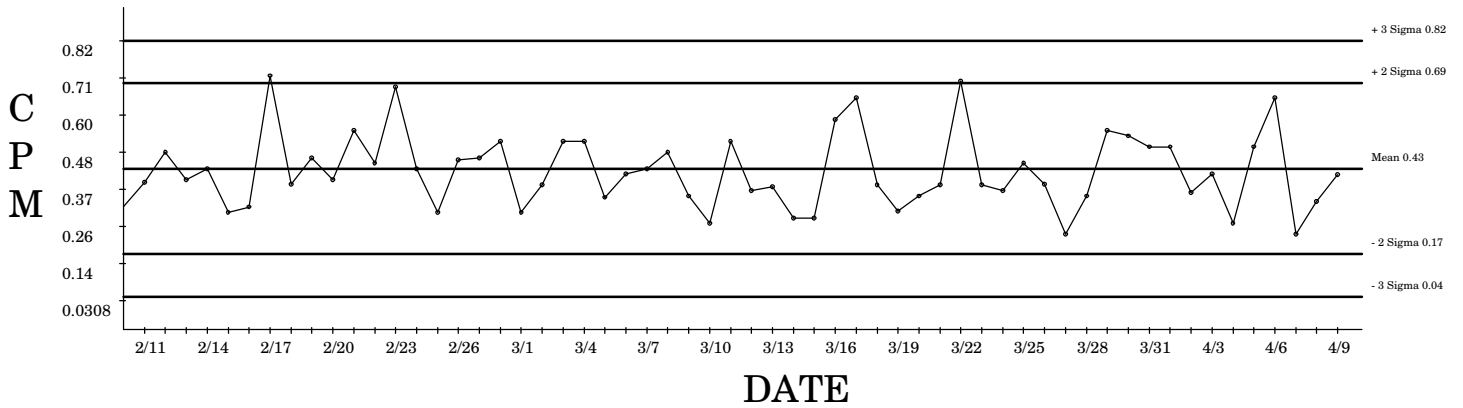

Alpha EFF

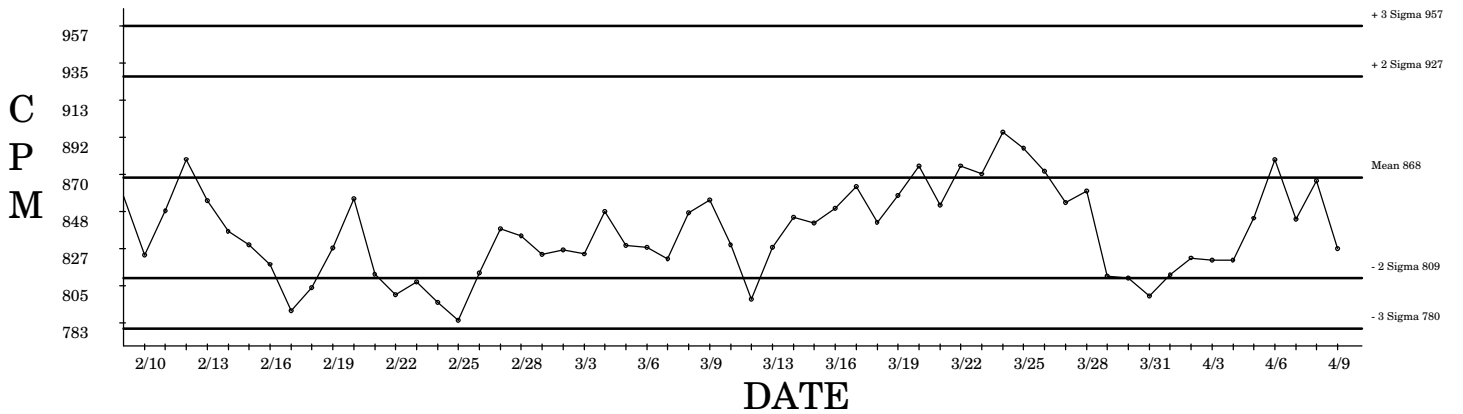


Beta EFF

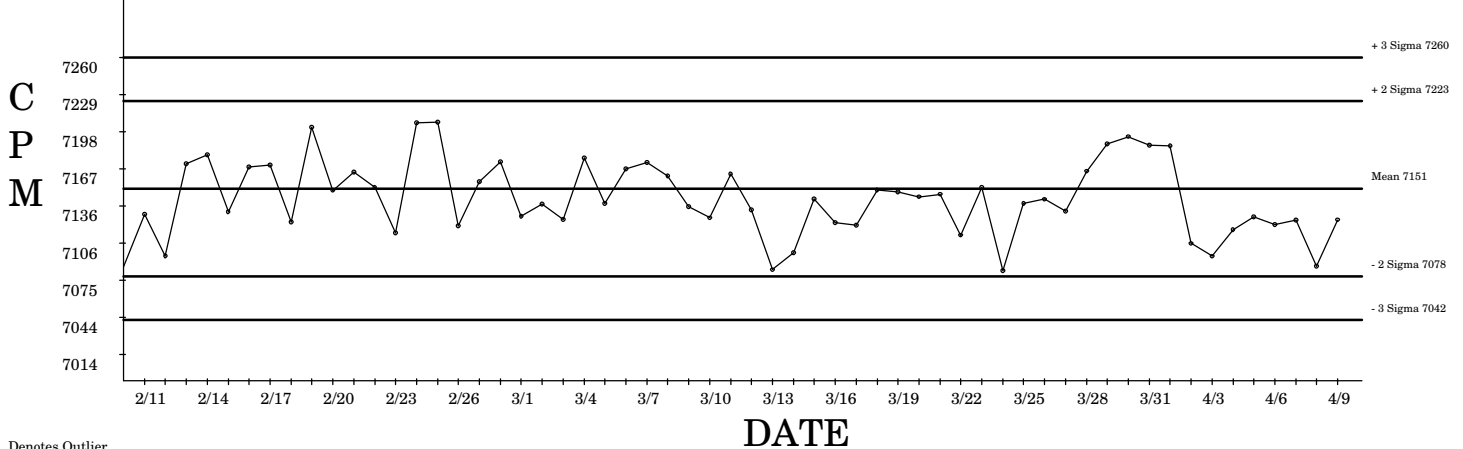


○ Denotes Outlier


PIC4A 04/09/2006
Alpha BKG

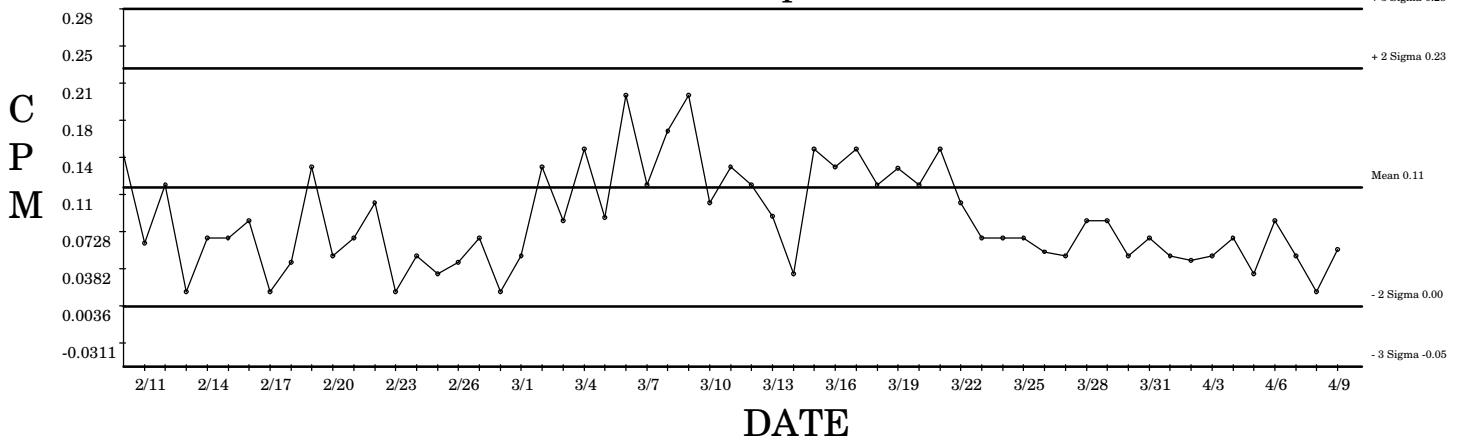


Beta BKG

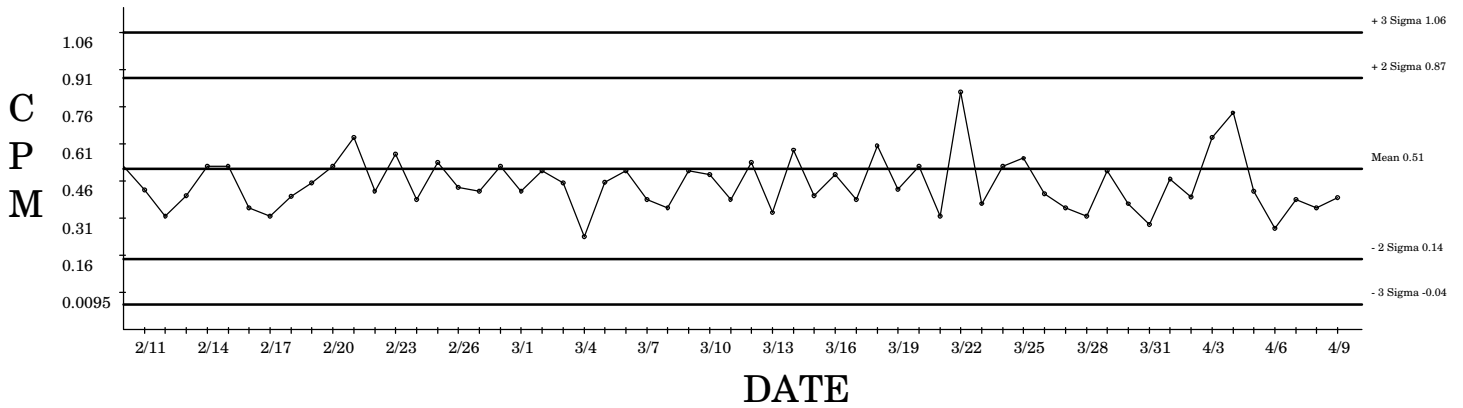

Alpha EFF

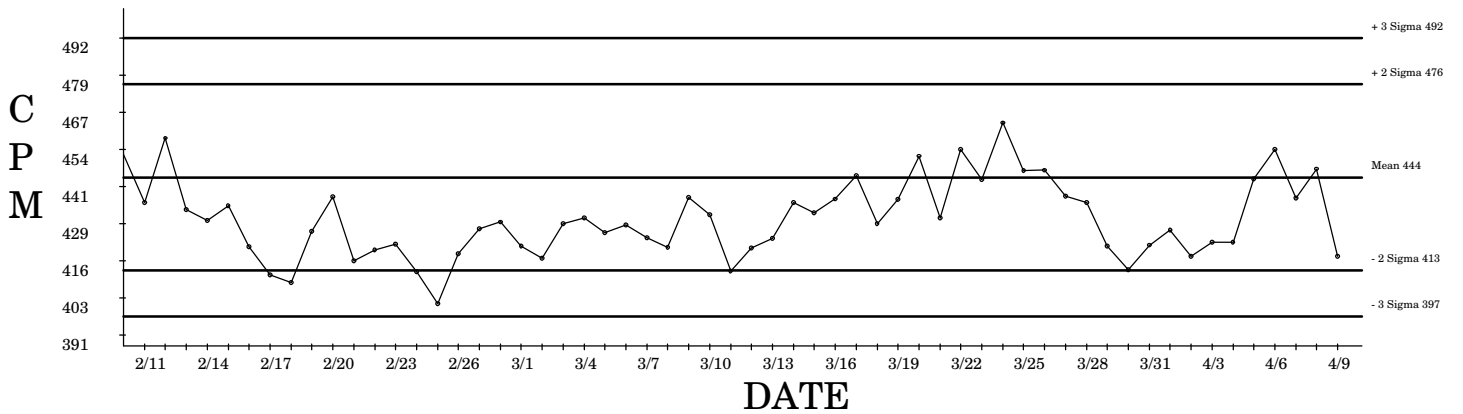


Beta EFF

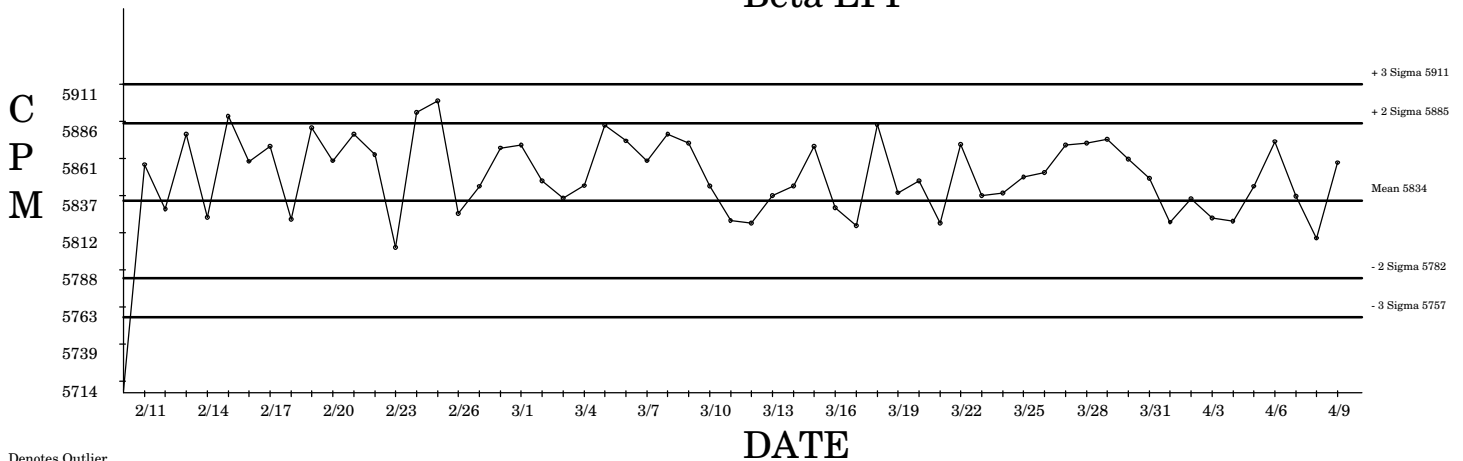


○ Denotes Outlier


PIC4B 04/09/2006
Alpha BKG

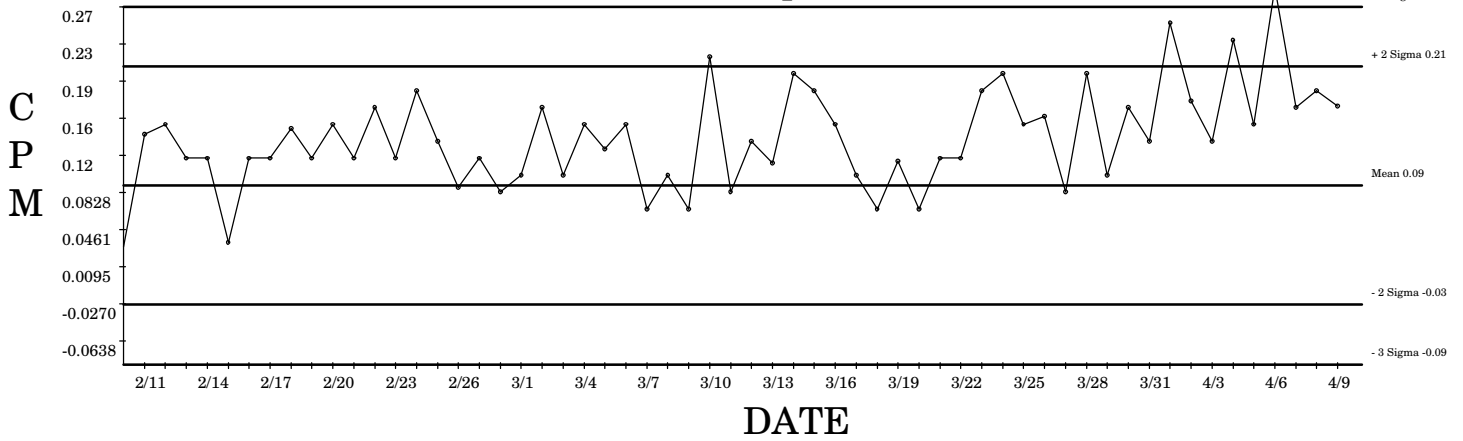


Beta BKG

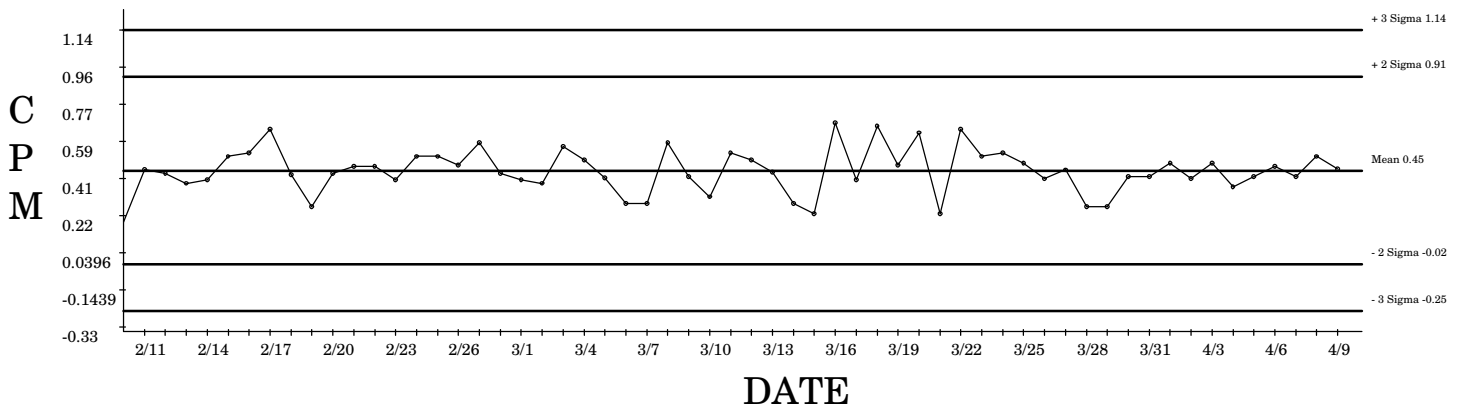

Alpha EFF

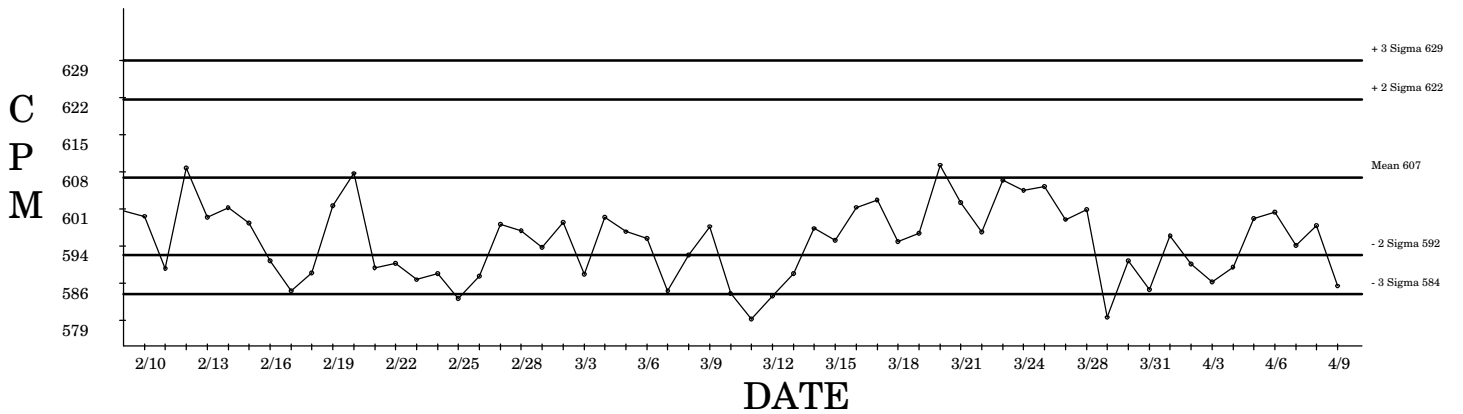


Beta EFF

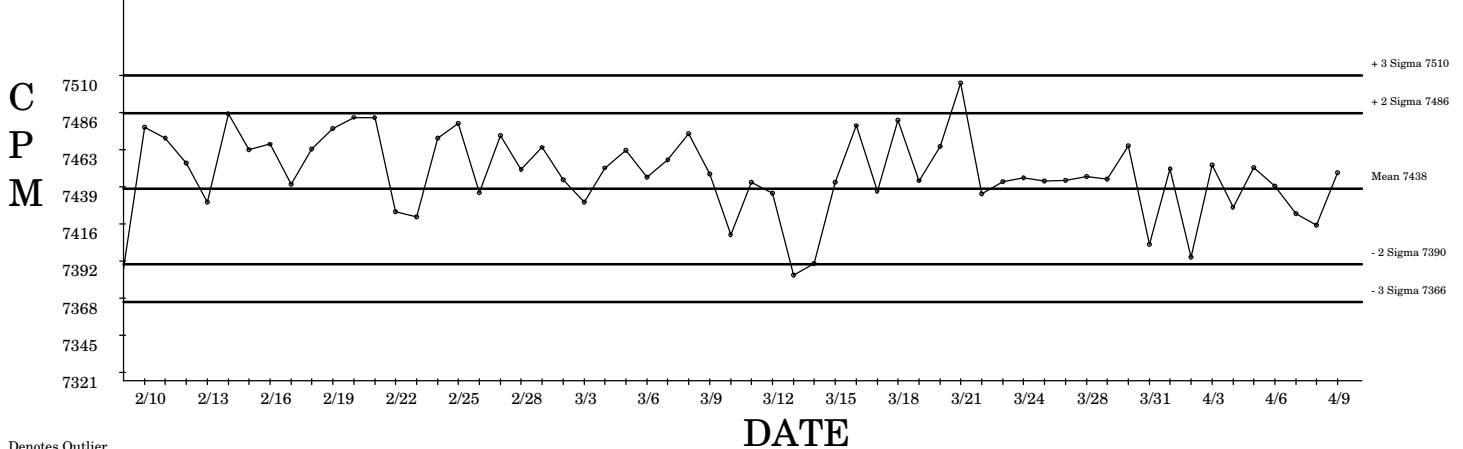


○ Denotes Outlier

QA filename : DKA100:[ENV_ALPHA.QA.W]w001.QAF;5
 Parameter Name : AVRGEFF (Average Efficiency)
 Start/End Dates : 3-OCT-2005 07:10:37 through 6-APR-2006 12:00:00
 Lower/Upper Lmts: 0.260000 through 0.290000

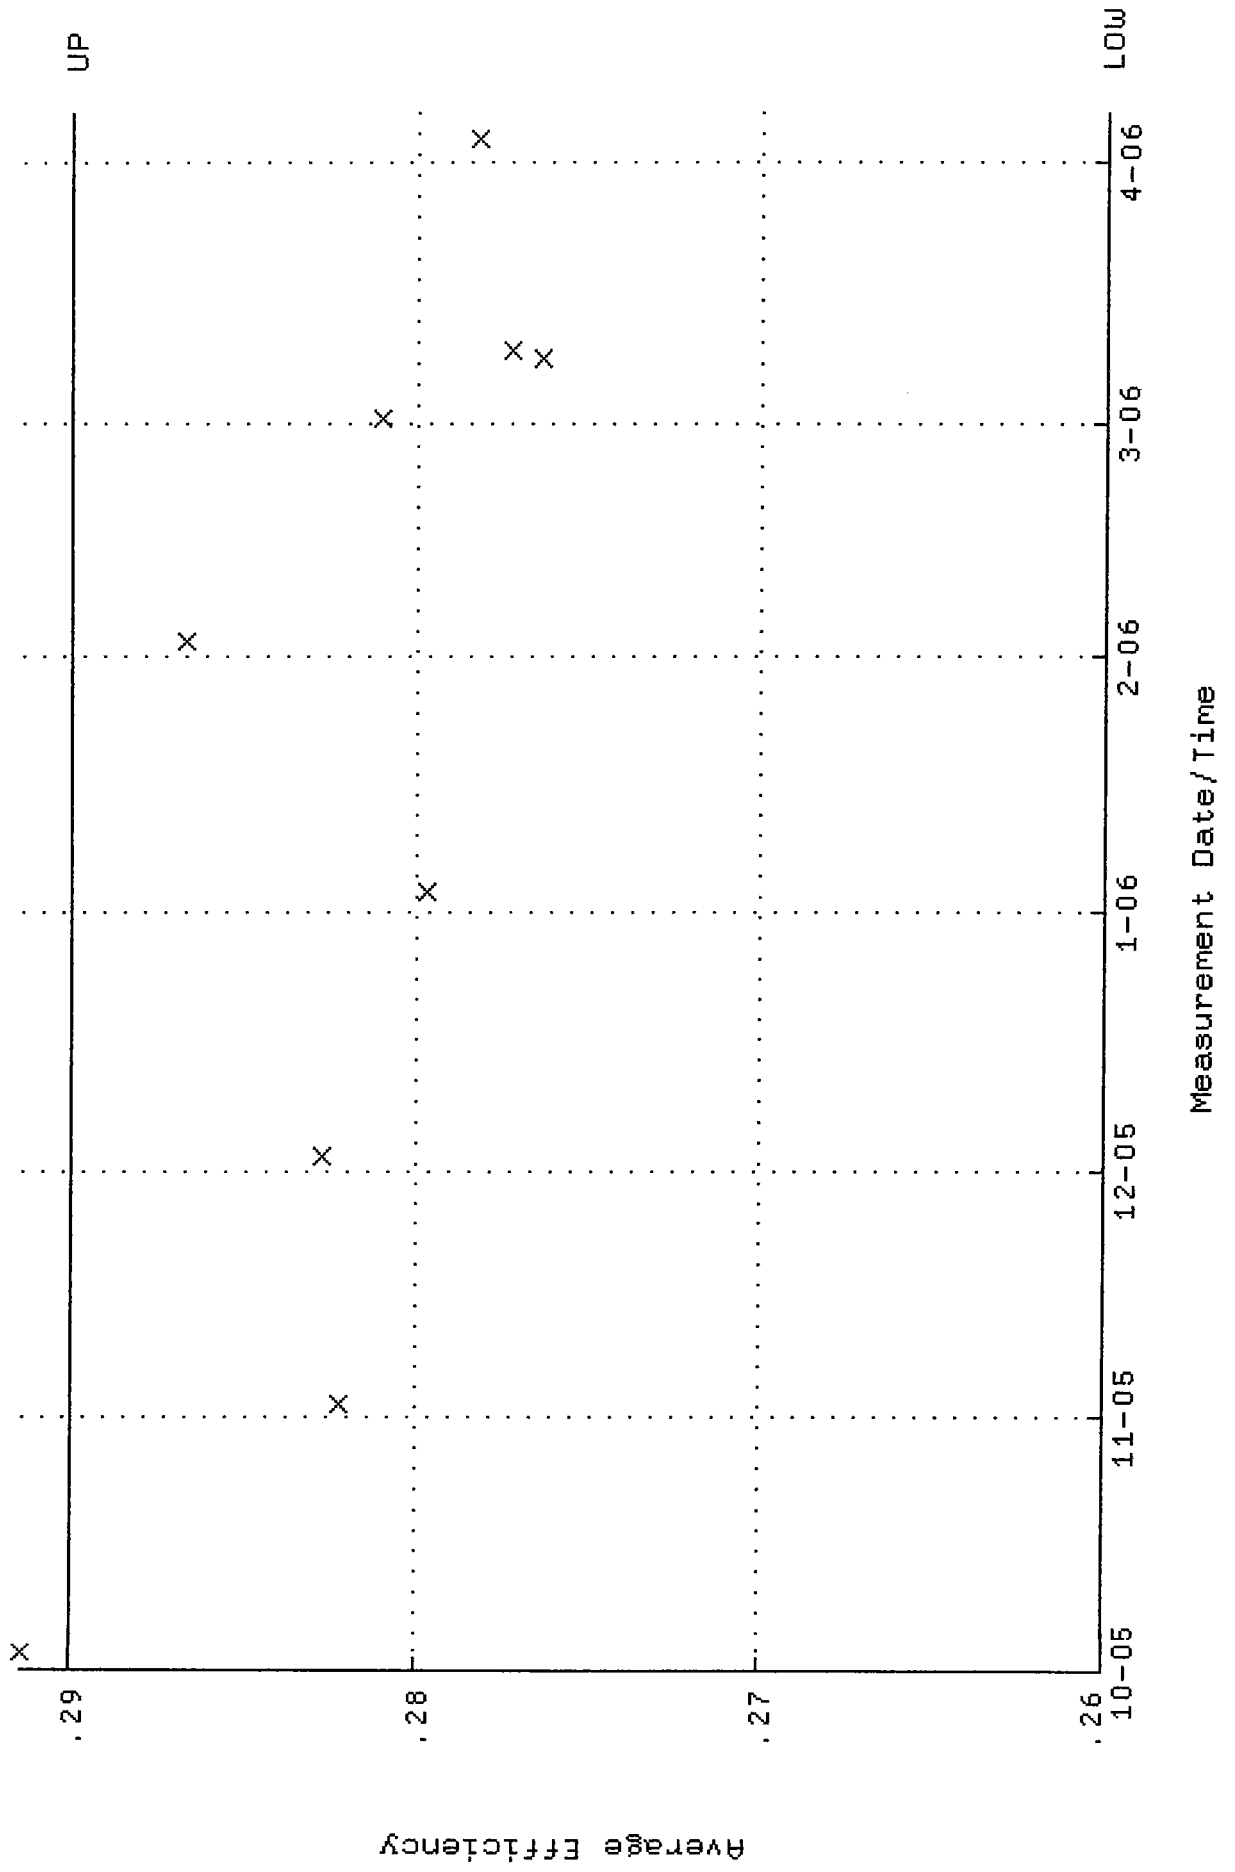


QA filename : DKA100:[ENV_ALPHA,QA,W]W001.QAF;5
 Parameter Name : NLAIVITY-GD148 (NUCLIDE ACTIVITY GD-148)
 Start/End Dates : 3-OCT-2005 07:10:37 through 6-APR-2006 12:00:00
 Lower/Upper Lmts: 60.0000 through 150.0000

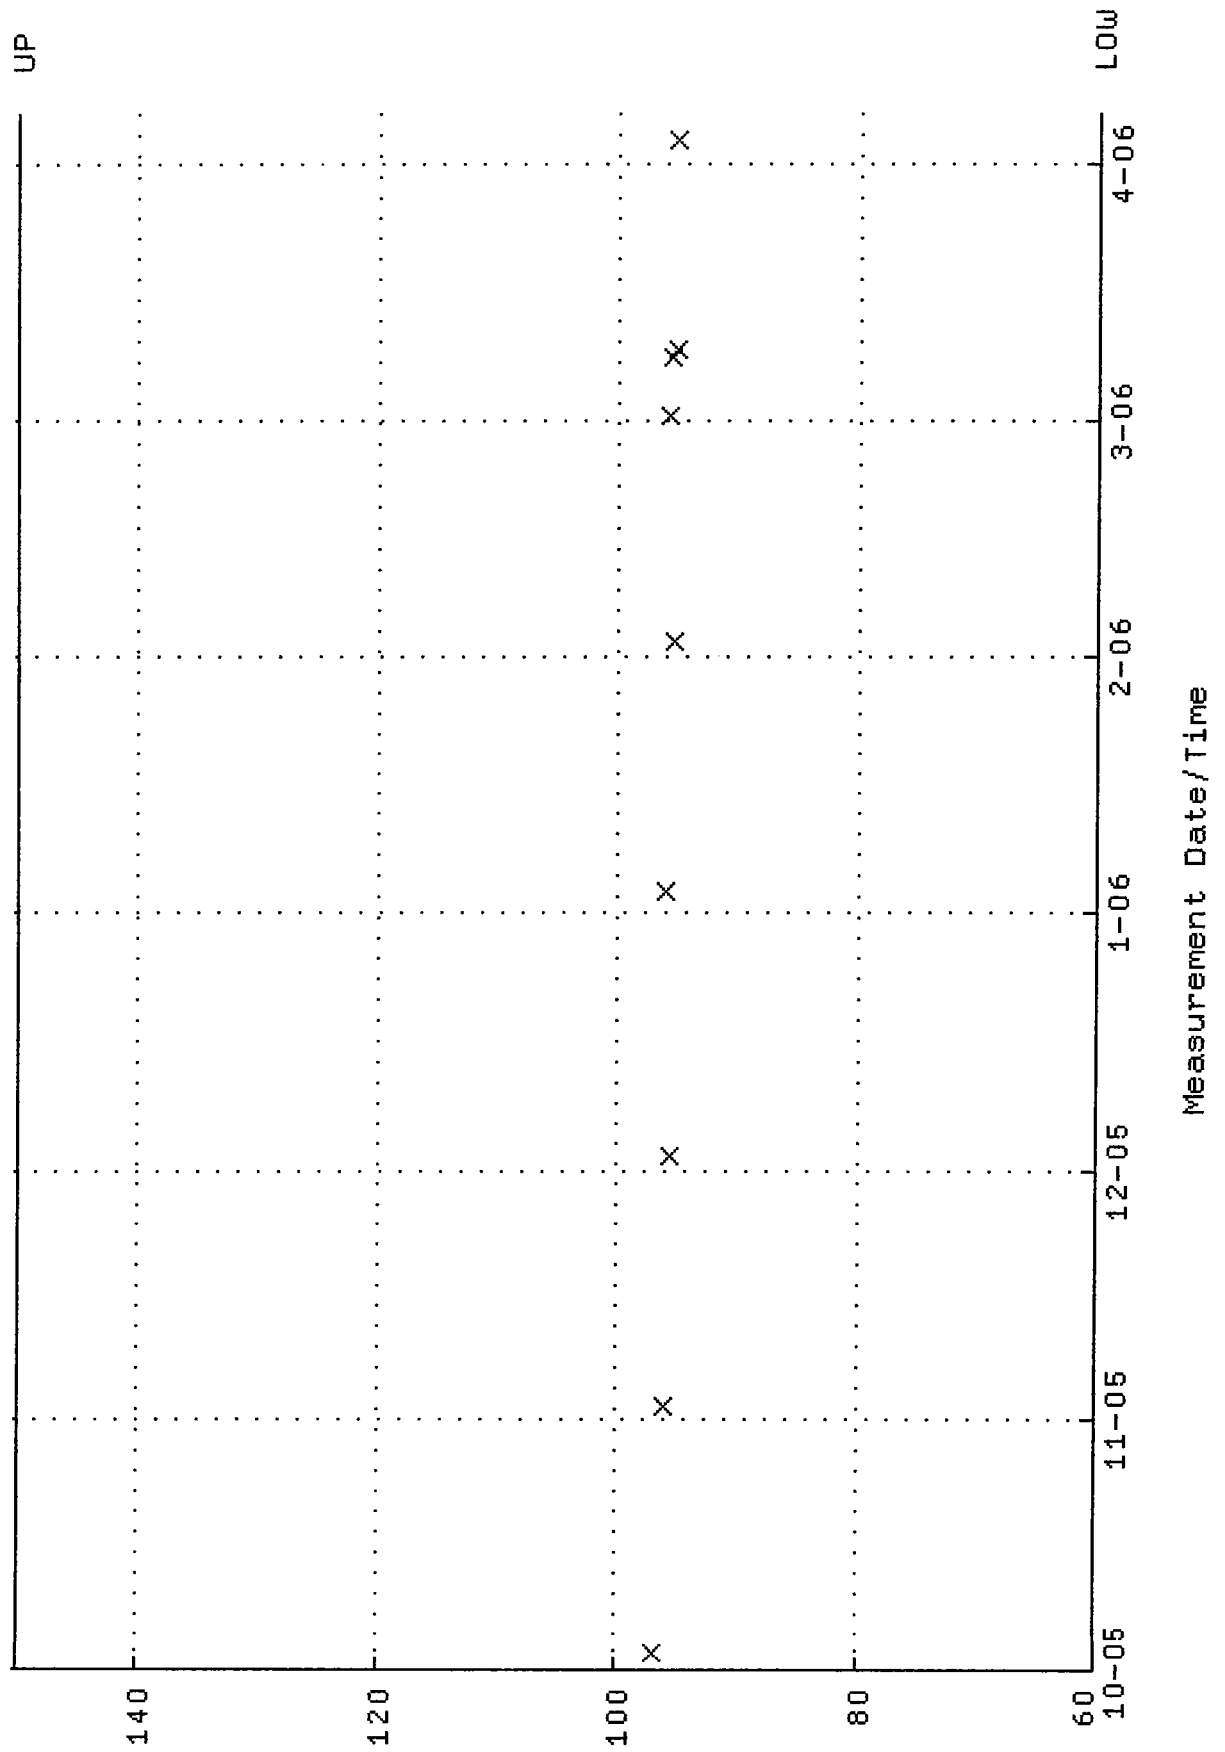


NUCLIDE ACTIVITY GD-

QA filename : DKA100:[ENV_ALPHA.QA.B]B001.QAF;1
 Parameter Name : BACKGROUND (Background Rate)
 Start/End Dates : 2-OCT-2005 13:25:38 through 6-APR-2006 12:00:00
 Lower/Upper Lmts: 0.000000E+00 through 2.000000E-02

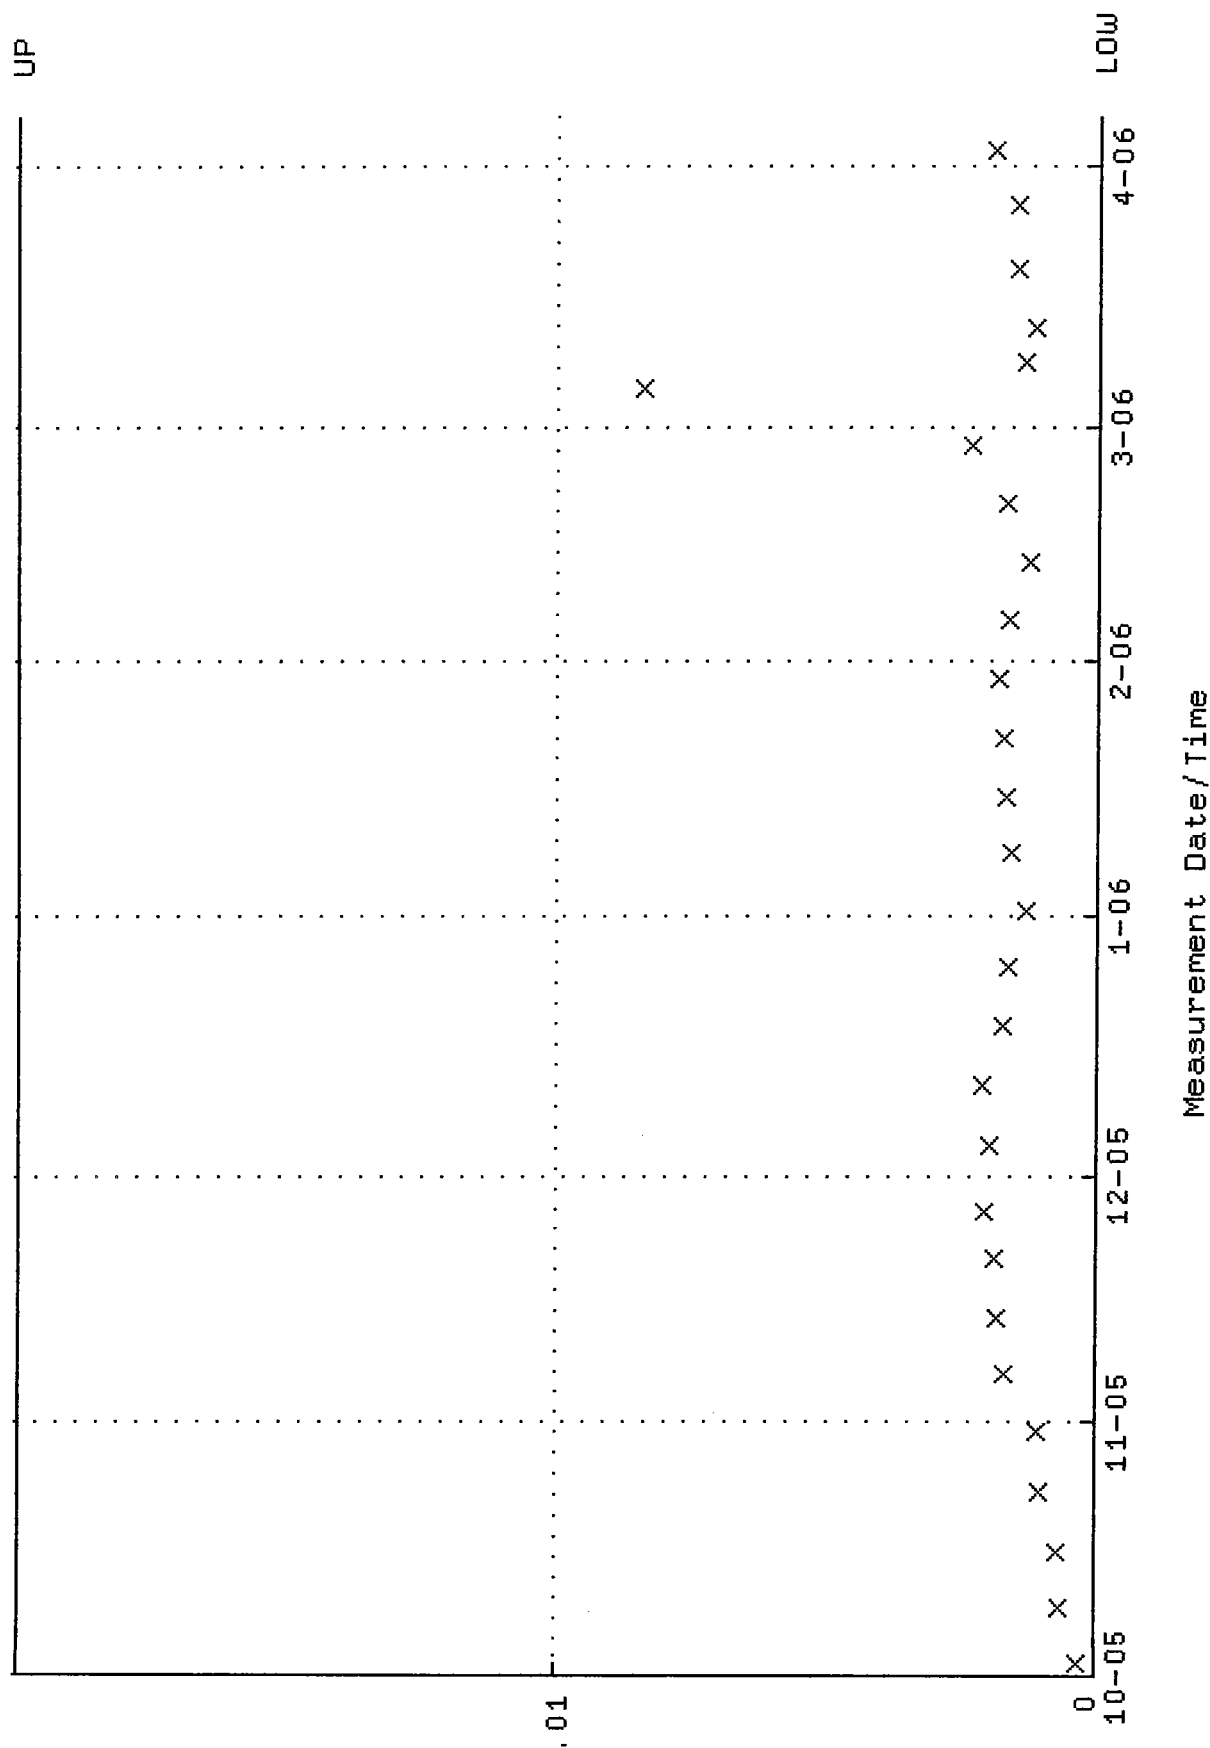


Background Rate

QA filename : DKA100:[ENV_ALPHA.QA.W]W003.QAF;3
 Parameter Name : AVREFF (Average Efficiency)
 Start/End Dates : 3-OCT-2005 07:10:37 through 6-APR-2006 12:00:00
 Lower/Upper Lmts: 0.280000 through 0.320000

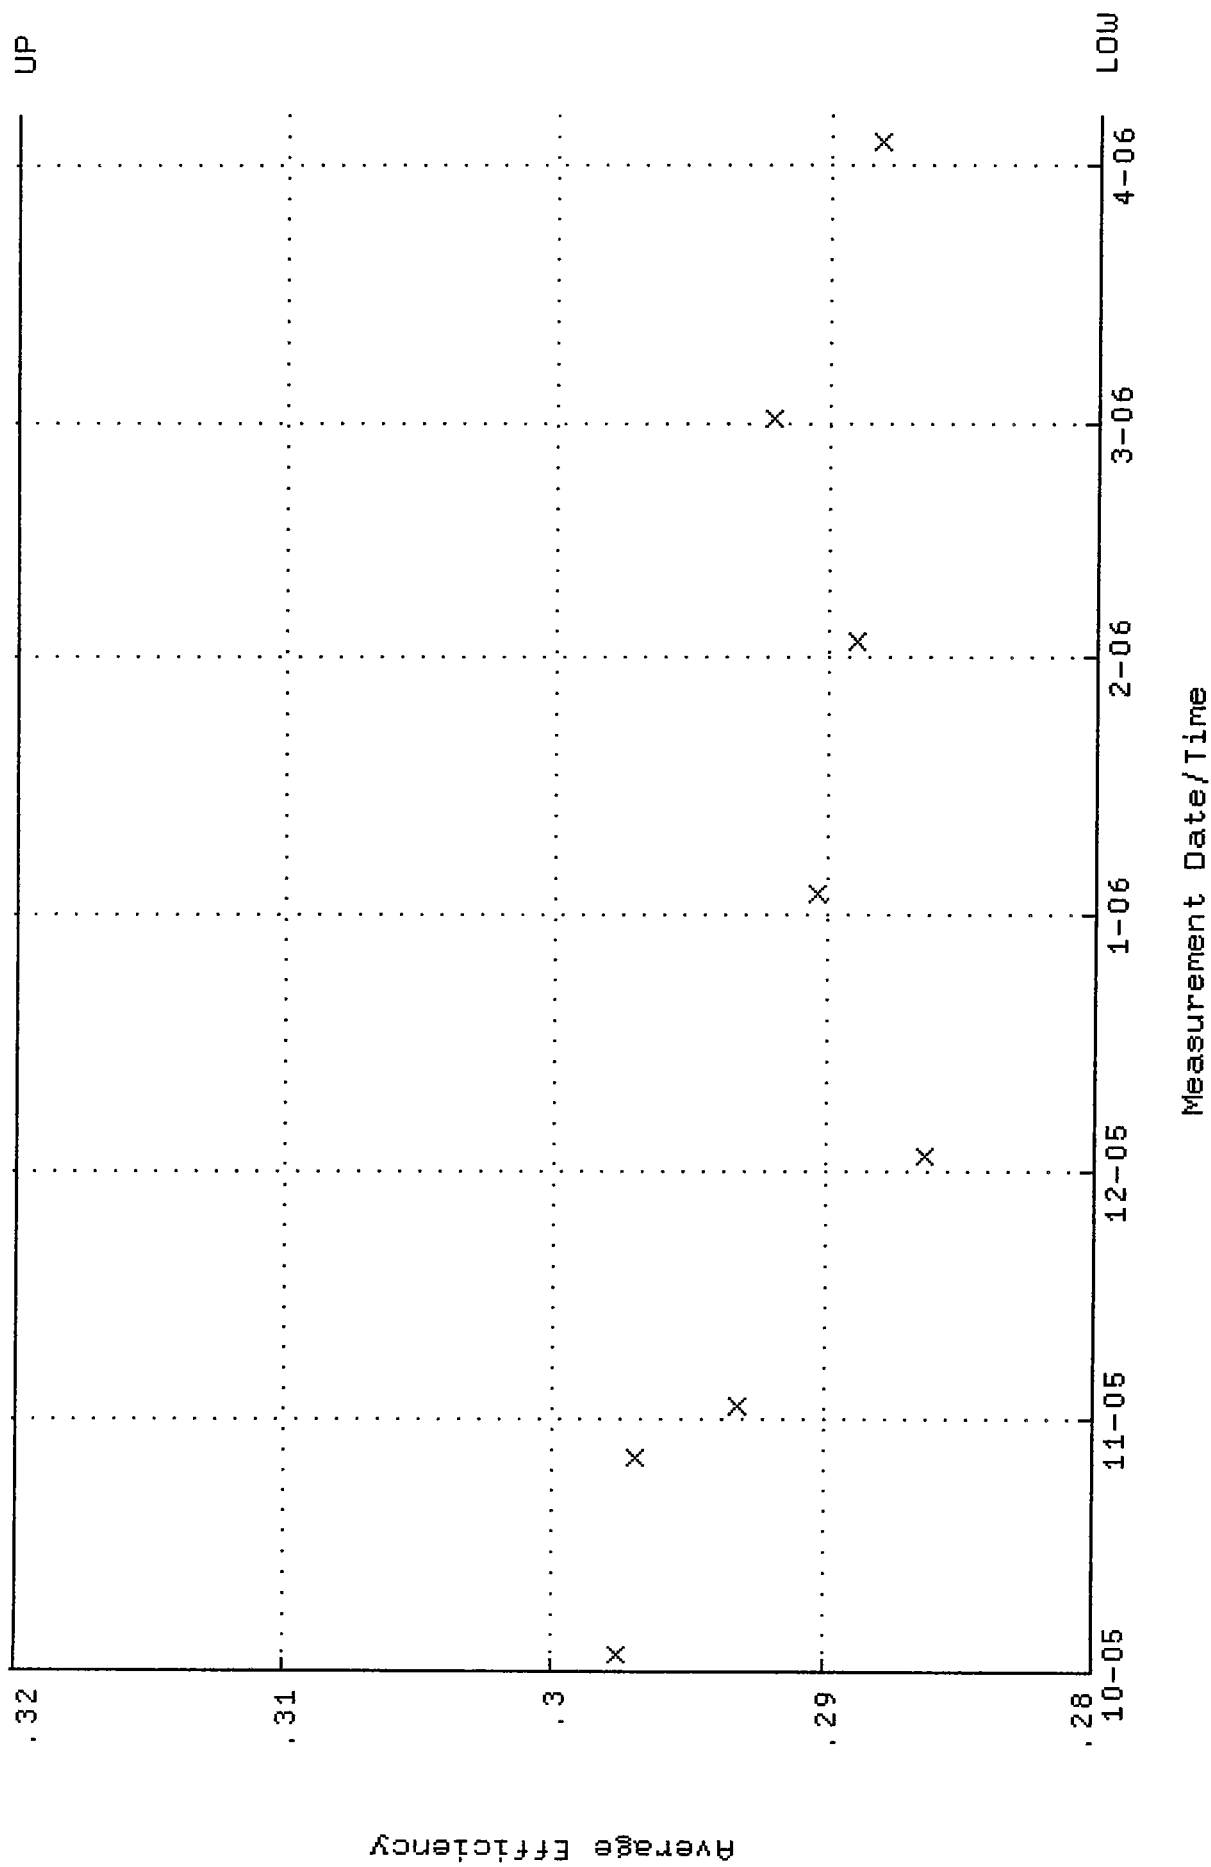


QA filename : DKA100:[ENV_ALPHA.QA.w]w003.QAF;3
 Parameter Name : NLAIVITY-GD148 (NUCLIDE ACTIVITY GD-148)
 Start/End Dates : 3-OCT-2005 07:10:37 through 6-APR-2006 12:00:00
 Lower/Upper Lmts: 60.0000 through 150.0000

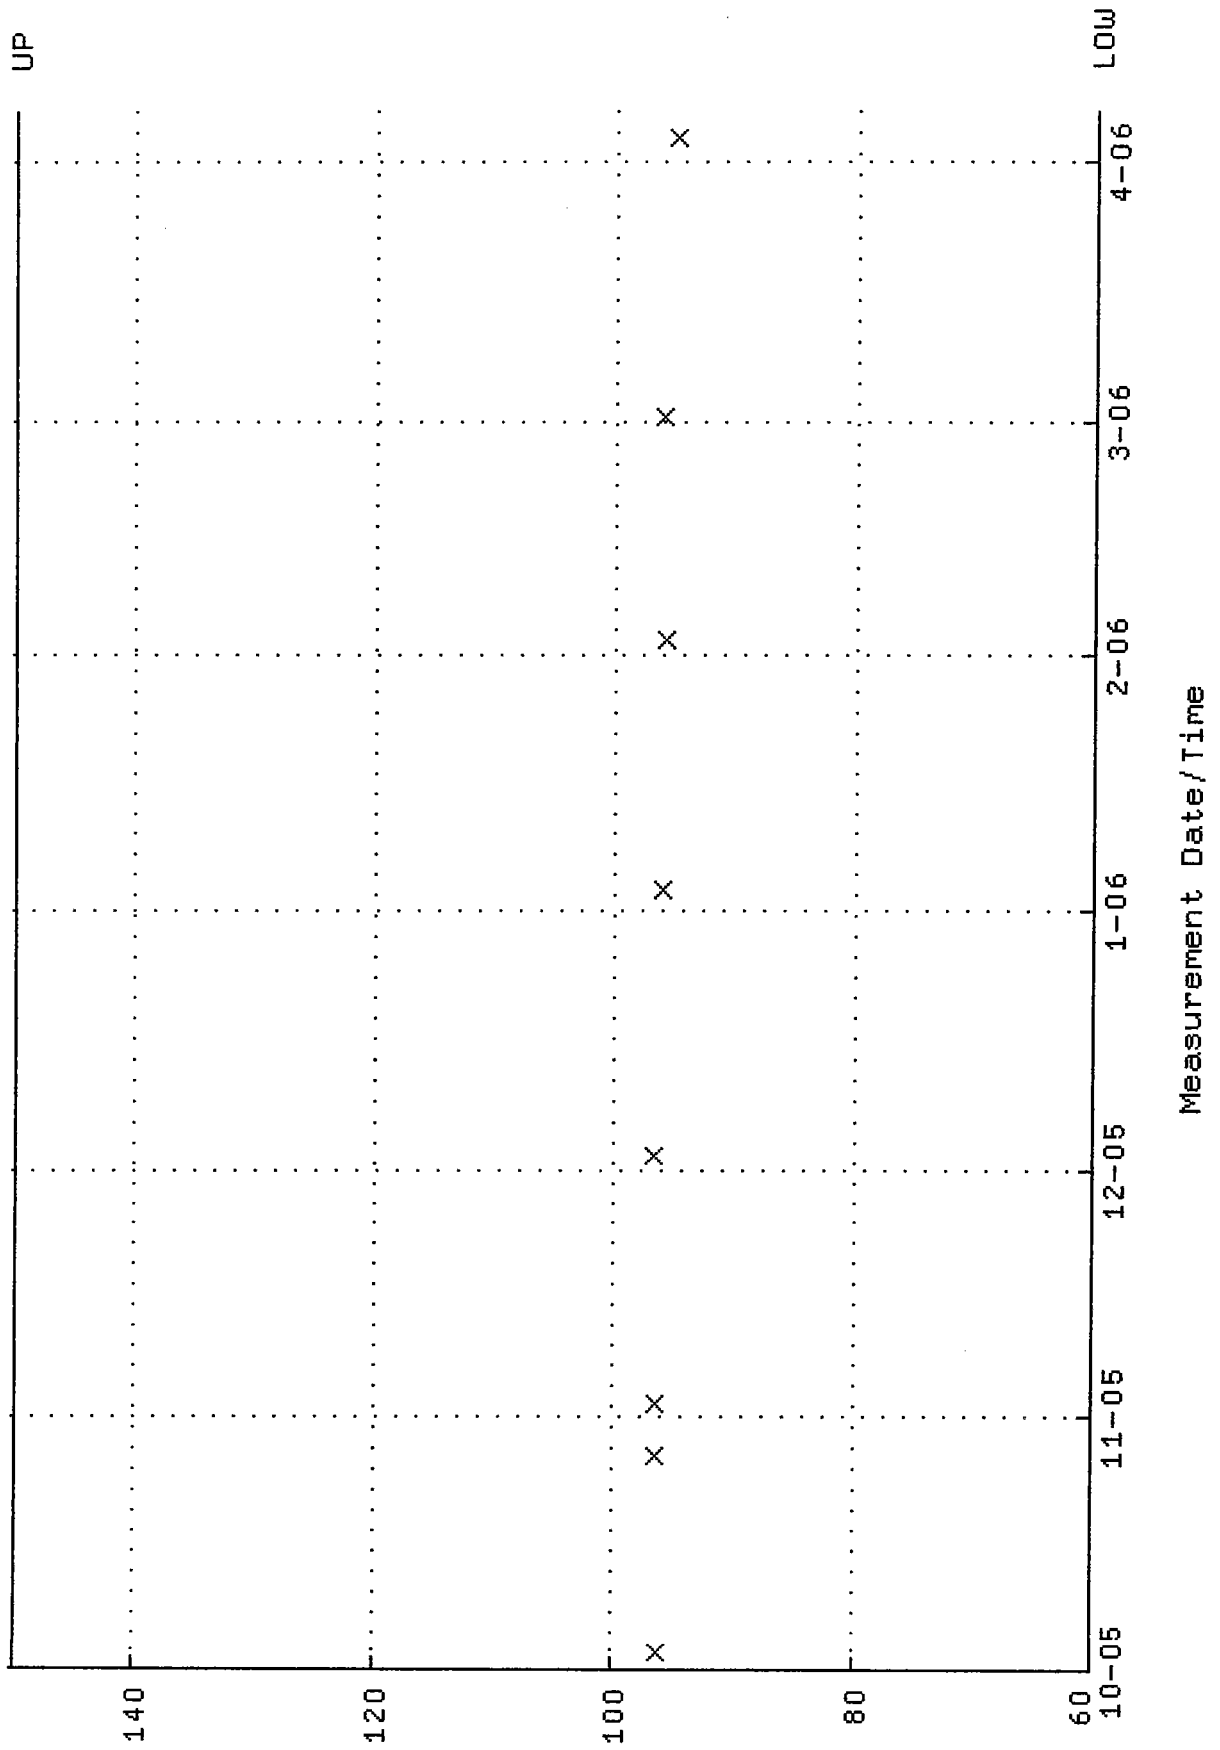


NUCLIDE ACTIVITY GD-


QA filename : DKA100:[ENV_ALPHA.QA.B]B003.QAF;1
Parameter Name : BACKRATE (Background Rate)
Start/End Dates : 2-OCT-2005 13:25:38 through 6-APR-2006 12:00:00
Lower/Upper Lmts: 0.000000E+00 through 2.000000E-02

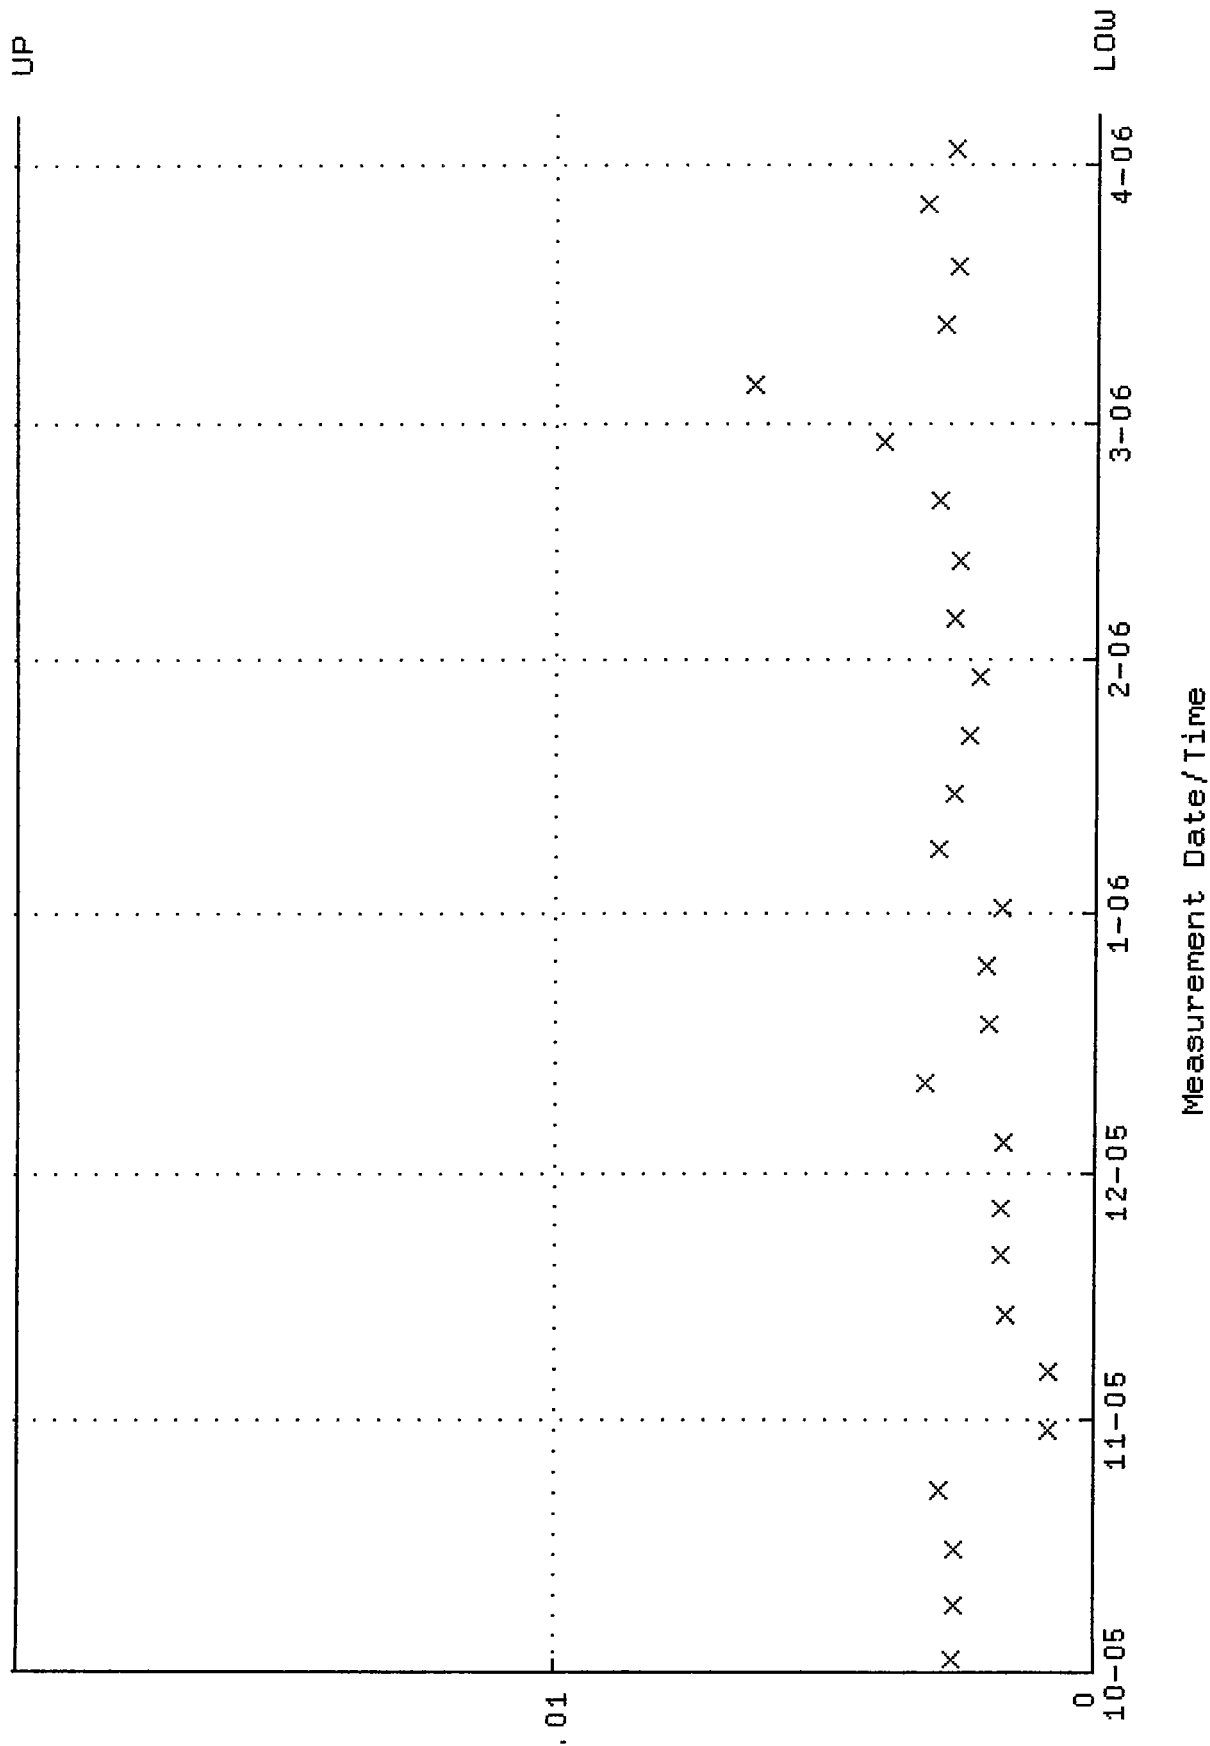


QA filename : DKA100:[ENV_ALPHA.QA.W]W004.QAF;3
 Parameter Name : AVRGEFF (Average Efficiency)
 Start/End Dates : 3-OCT-2005 07:10:37 through 6-APR-2006 12:00:00
 Lower/Upper Lmts: 0.300000 through 0.330000

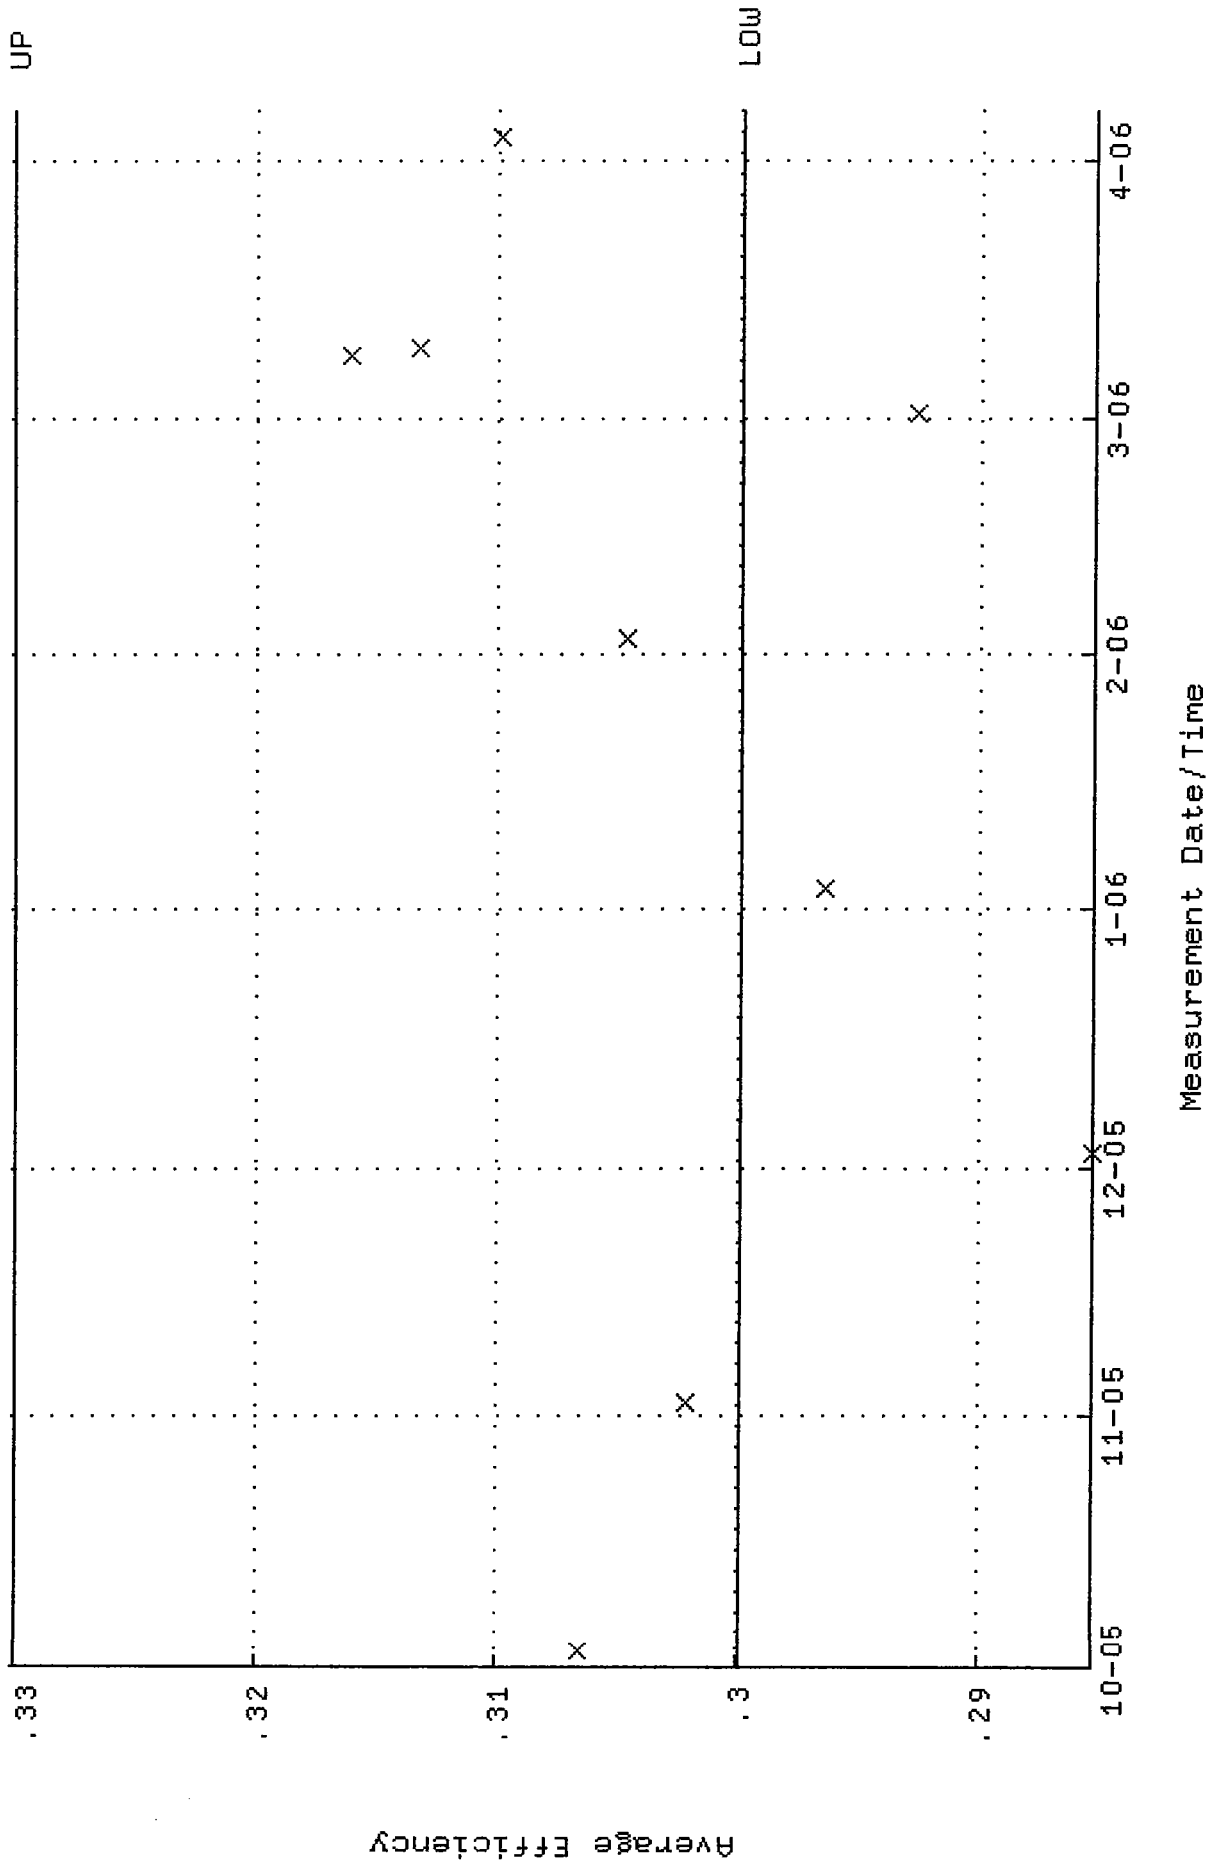


QA filename : DKA100:[ENV_ALPHA.QA.W]W004.QAF;3
 Parameter Name : NLAIVITY-GD148 (NUCLIDE ACTIVITY GD-148)
 Start/End Dates : 3-OCT-2005 07:10:37 through 6-APR-2006 12:00:00
 Lower/Upper Lmts: 60.0000 through 150.0000

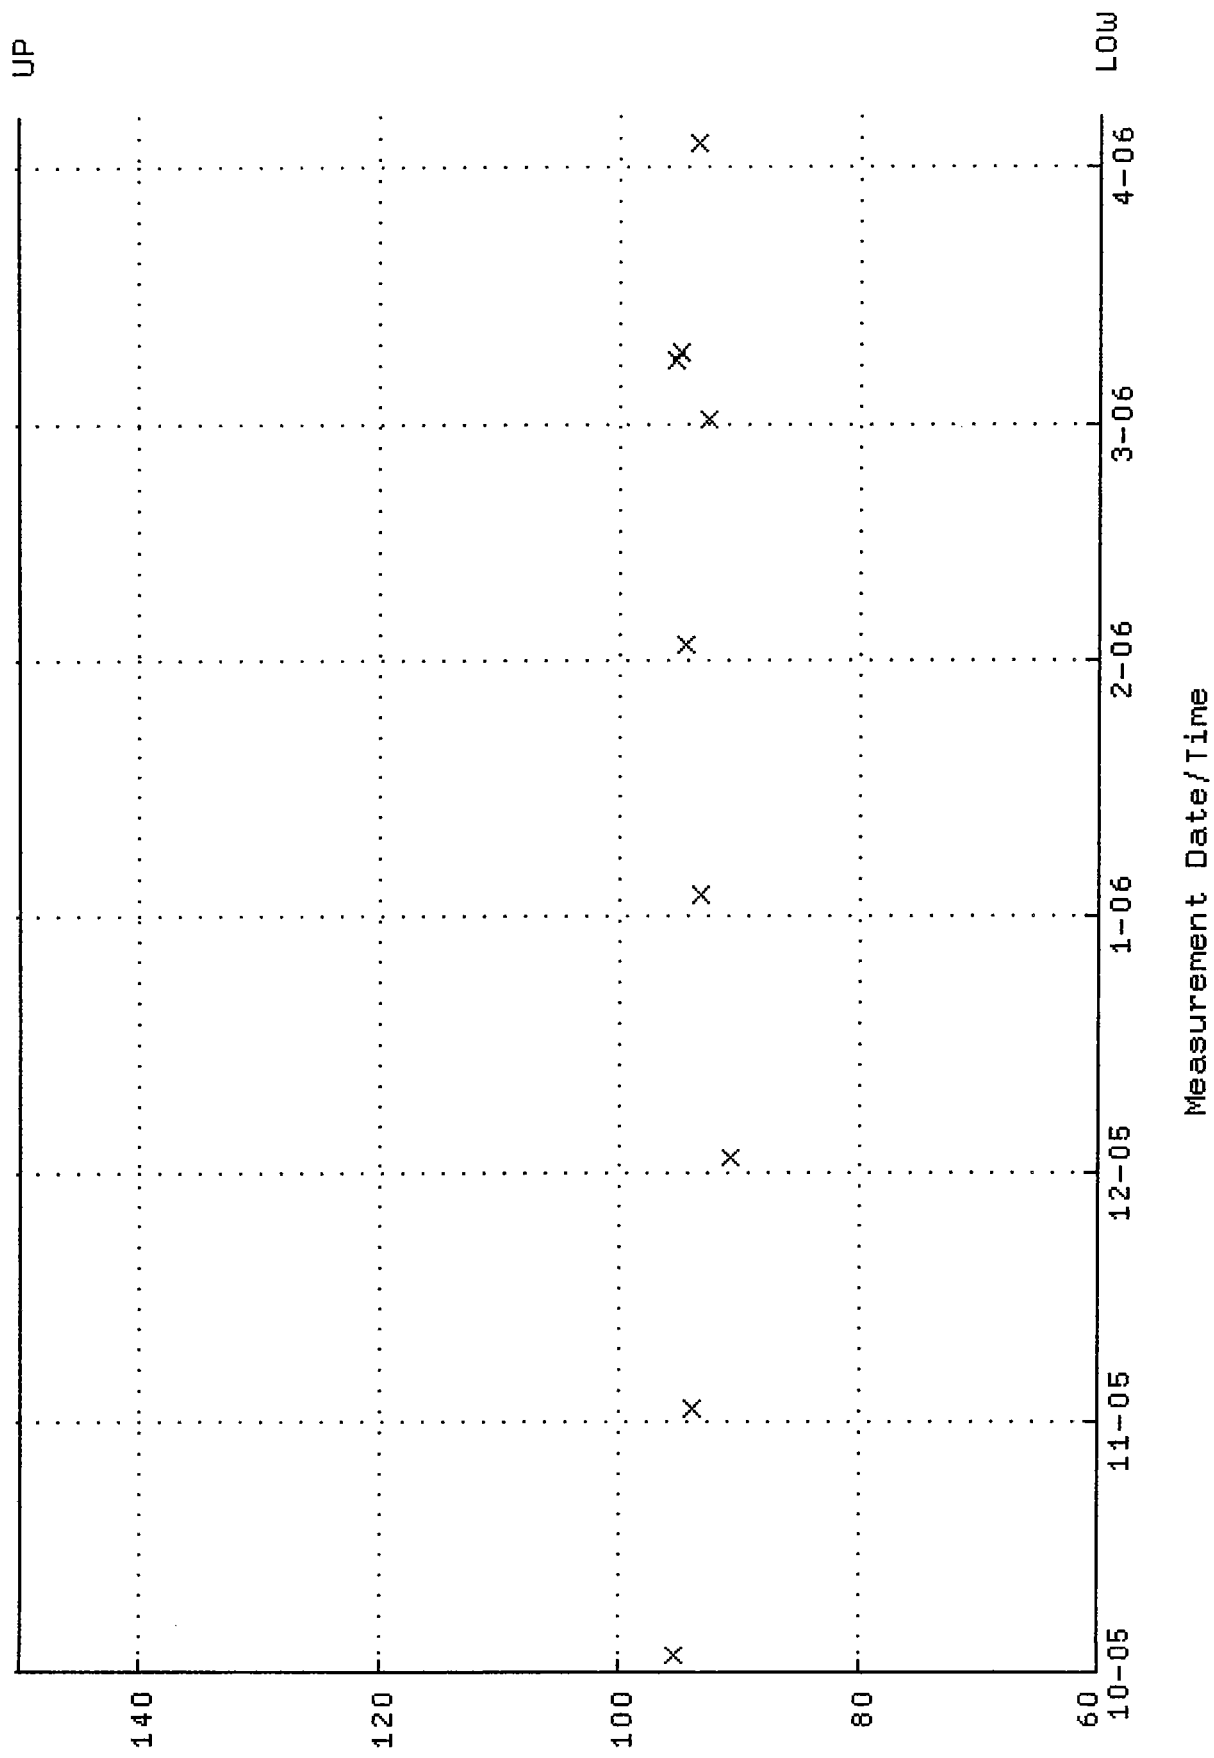

QA filename : DKA100:[ENV_ALPHA.QA.B]B004.QAF;1
 Parameter Name : BACKRATE (Background Rate)
 Start/End Dates : 2-OCT-2005 13:25:38 through 6-APR-2006 12:00:00
 Lower/Upper Lmts: 0.000000E+00 through 2.000000E-02

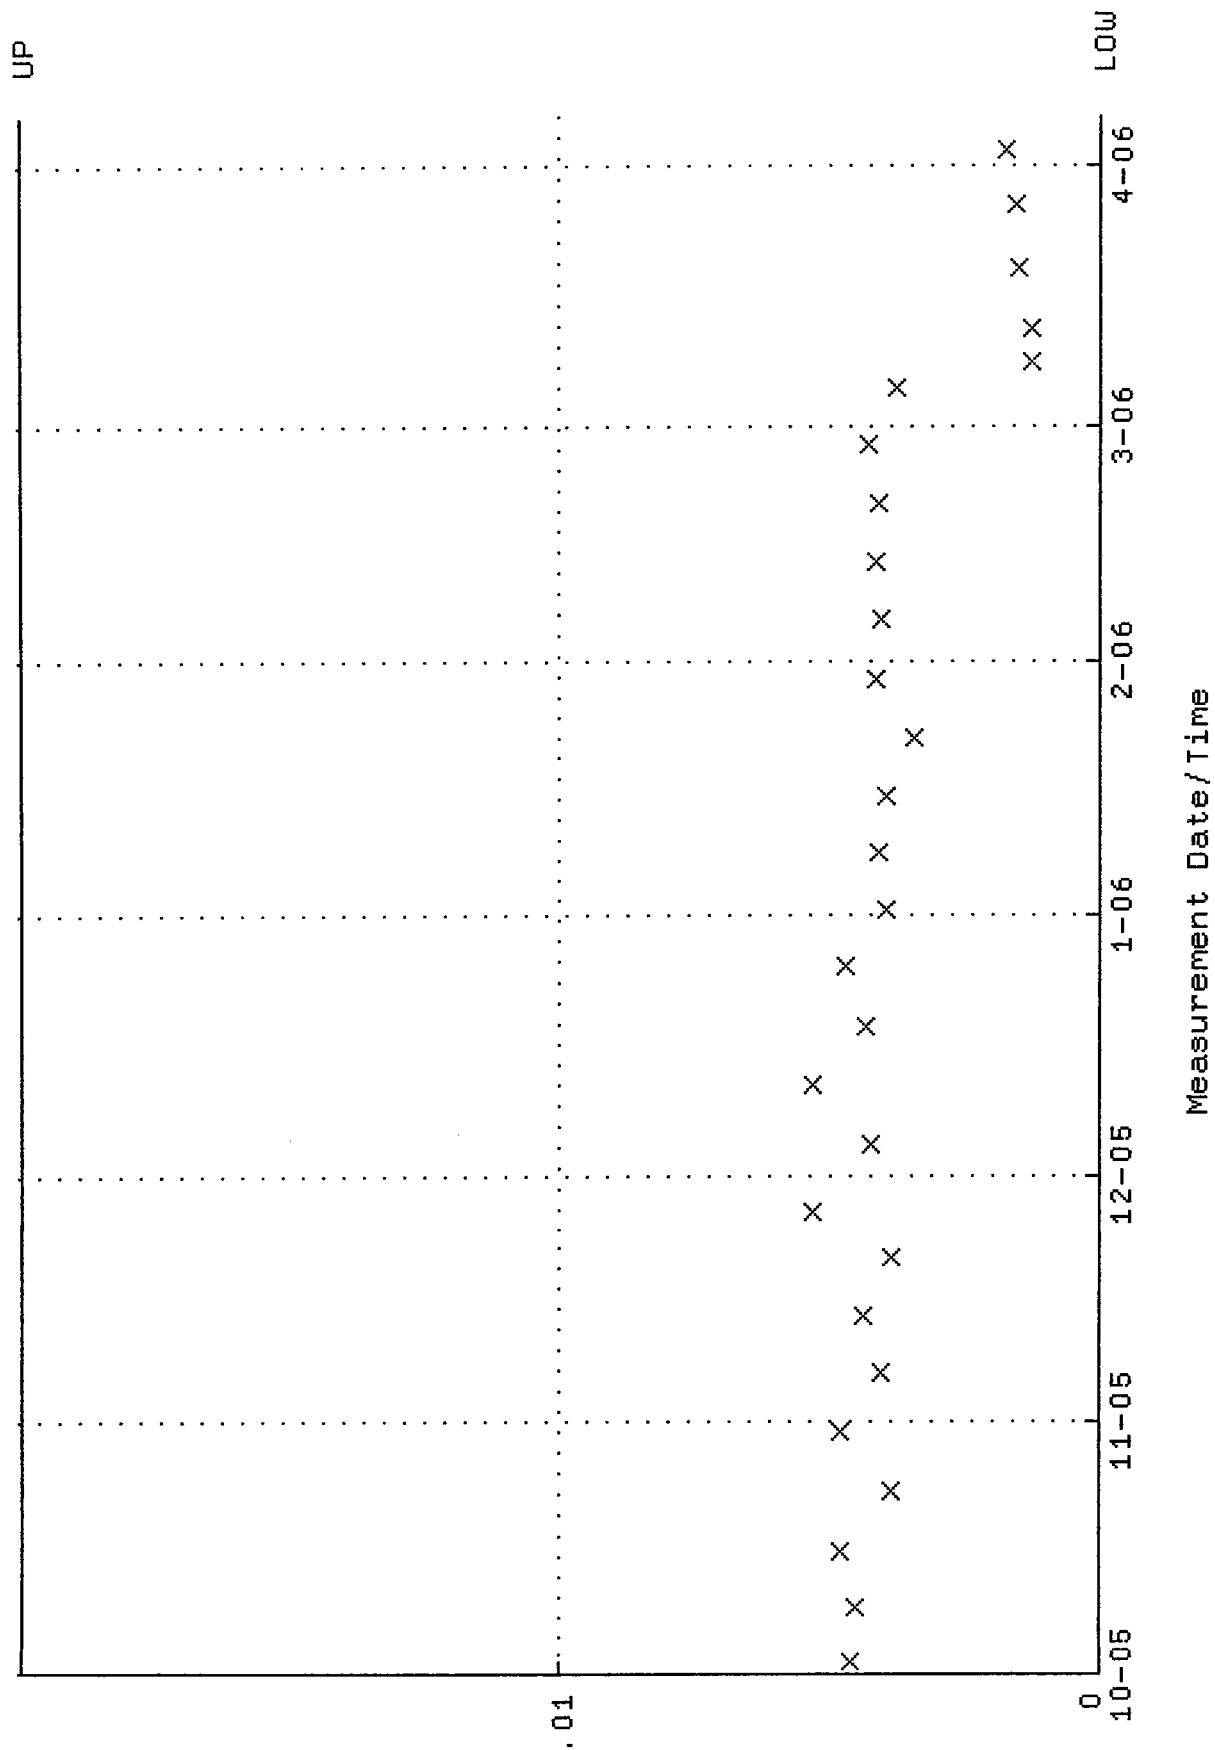


QA filename : DKA100:[ENV_ALPHA.QA.W]W005.QAF;4
 Parameter Name : AVRGEFF (Average Efficiency)
 Start/End Dates : 3-OCT-2005 07:10:37 through 6-APR-2006 12:00:00
 Lower/Upper Lmts: 0.280000 through 0.370000

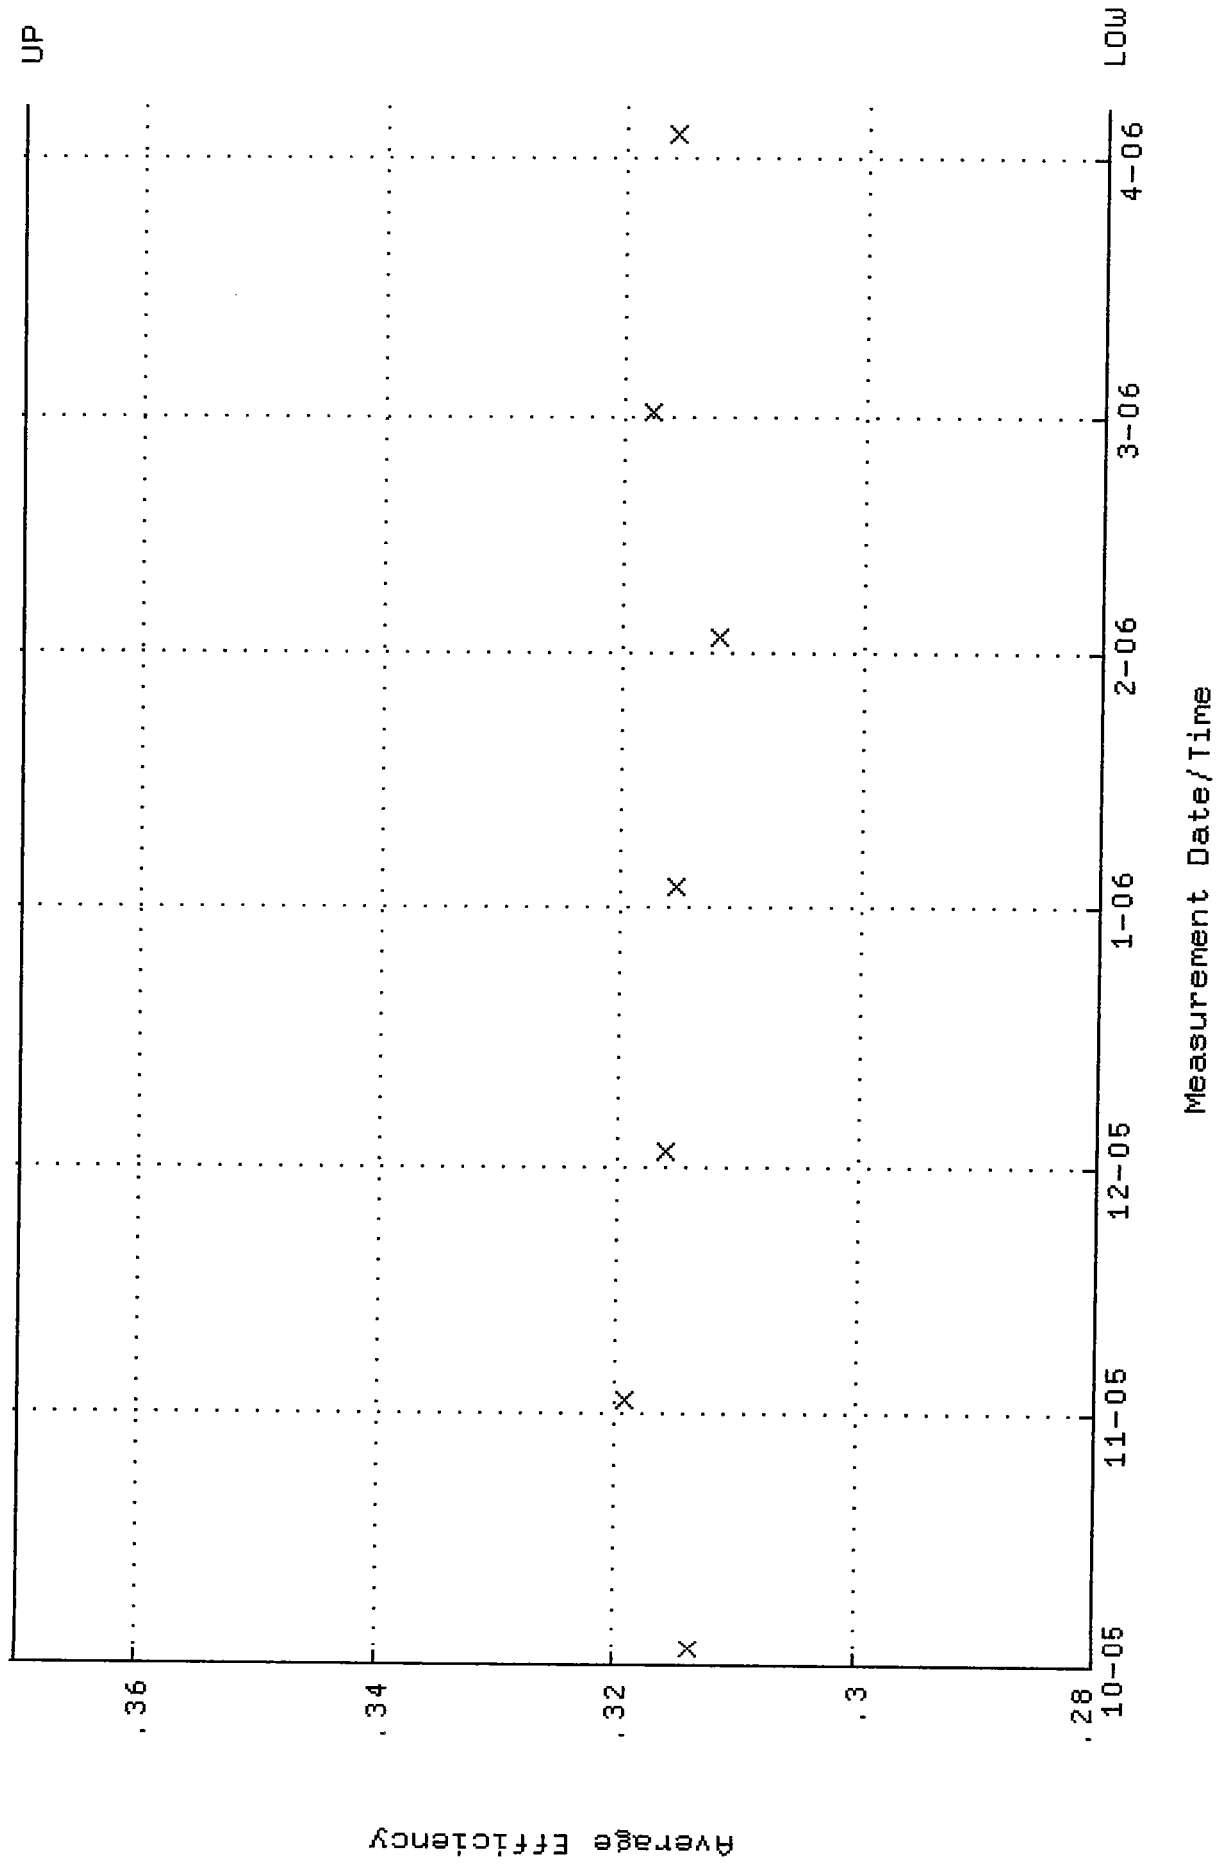


Average Efficiency

QA filename : DKA100:[ENV_ALPHA.QA.W]W005.QAF;4
Parameter Name : NLAIVITY-GD148 (NUCLIDE ACTIVITY GD-148)
Start/End Dates : 3-OCT-2005 07:10:37 through 6-APR-2006 12:00:00
Lower/Upper Lmts: 60.0000 through 150.0000

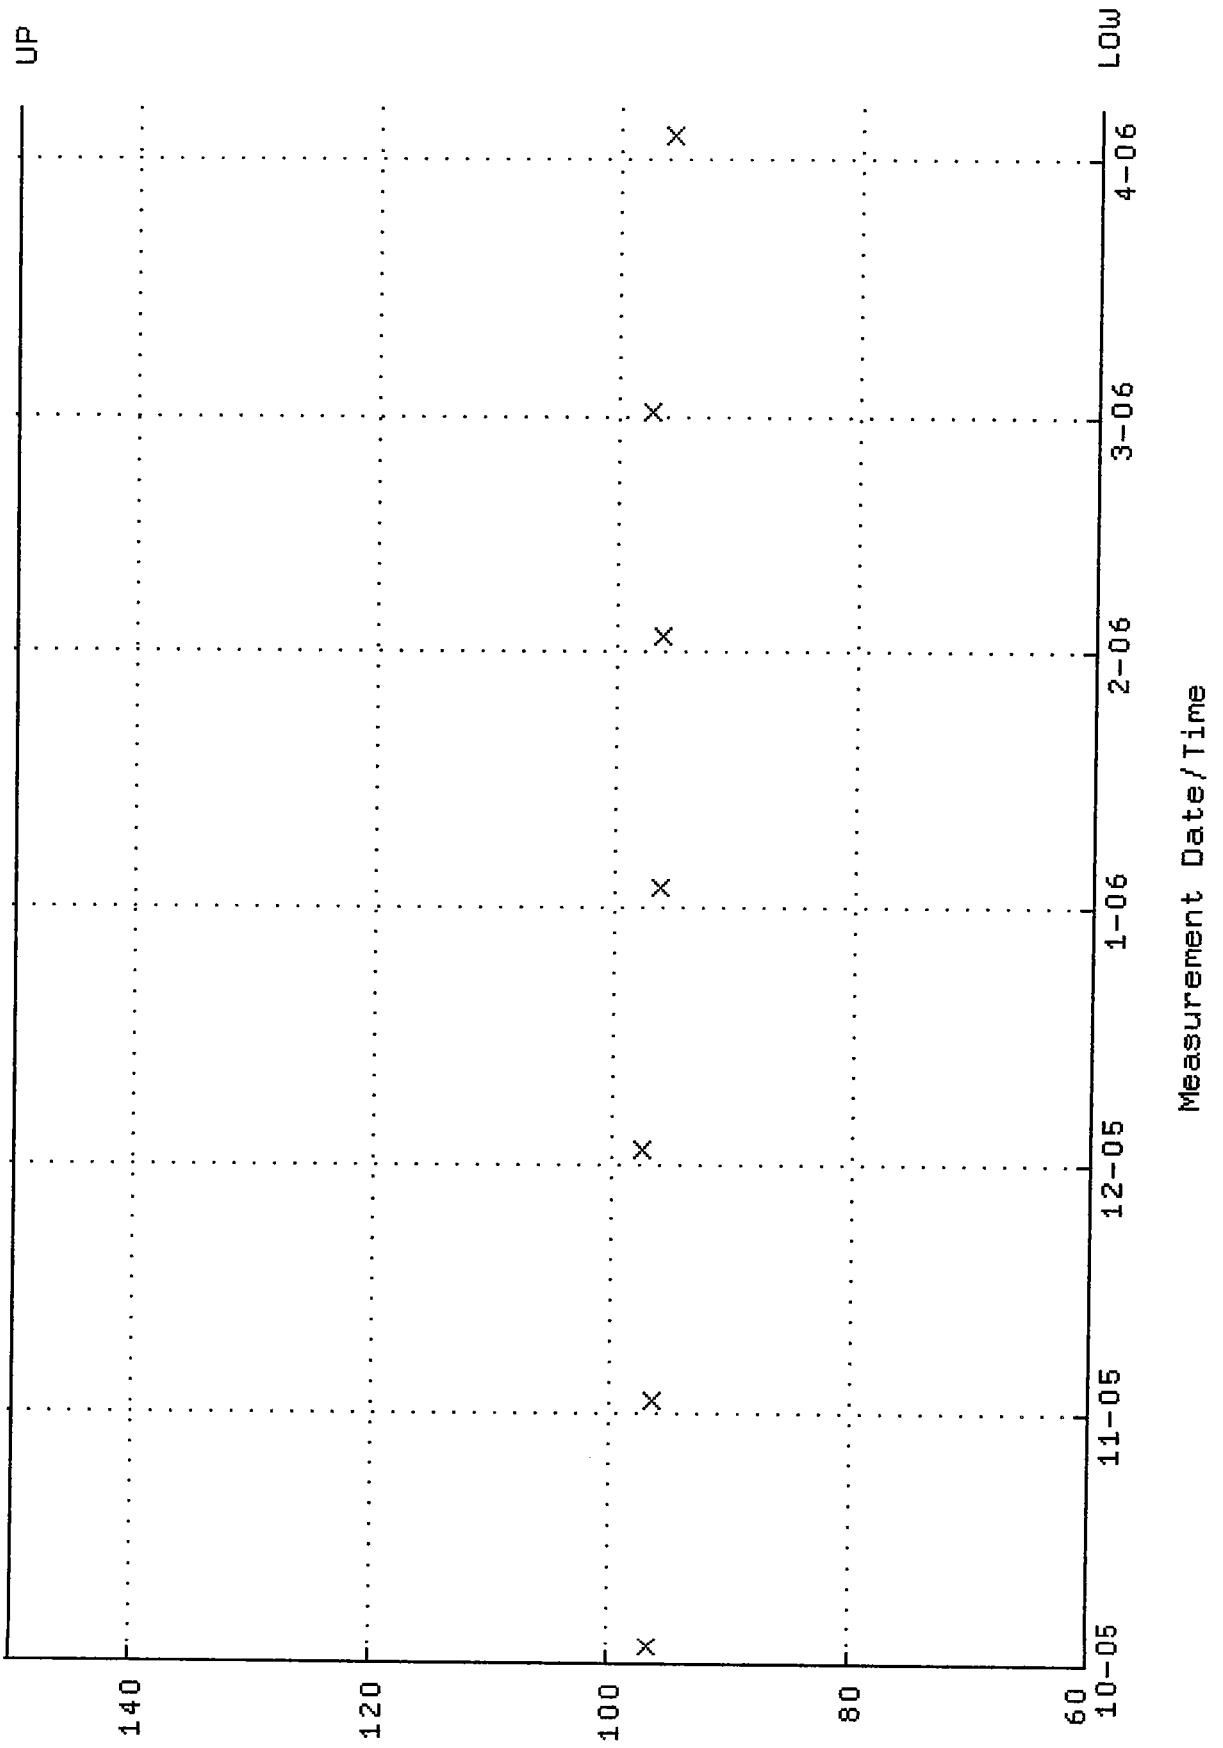


NUCLIDE ACTIVITY GD-

QA filename : DKA100:[ENV_ALPHA.QA.B]B005.QAF;2
 Parameter Name : BACKRATE (Background Rate)
 Start/End Dates : 2-OCT-2005 13:25:38 through 6-APR-2006 12:00:00
 Lower/Upper Lmts: 0.000000E+00 through 2.000000E-02

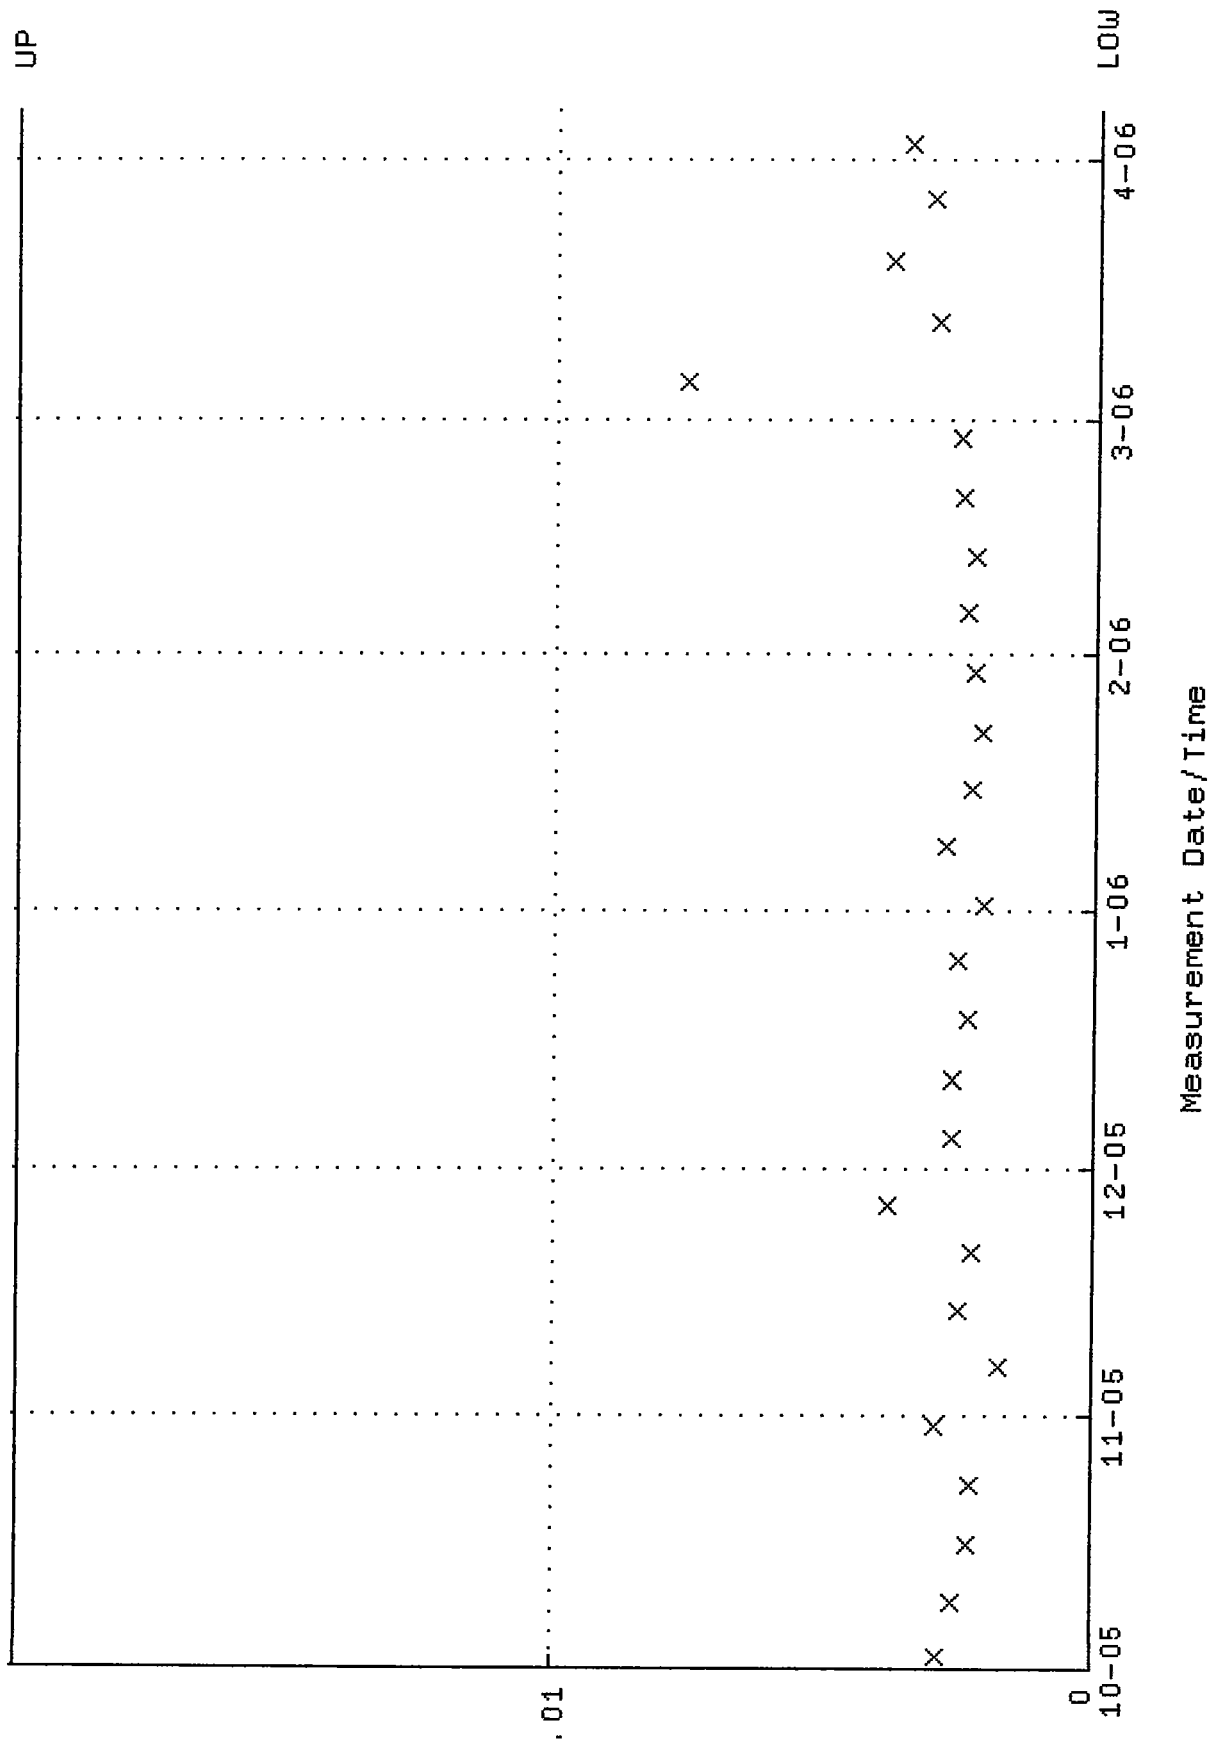


Background Rate


QA filename : DKA100:[ENV_ALPHA.QA.W]W018.QAF;3
 Parameter Name : AVRGEFF (Average Efficiency)
 Start/End Dates : 3-OCT-2005 07:10:41 through 6-APR-2006 12:00:00
 Lower/Upper Lmts: 0.250000 through 0.270000

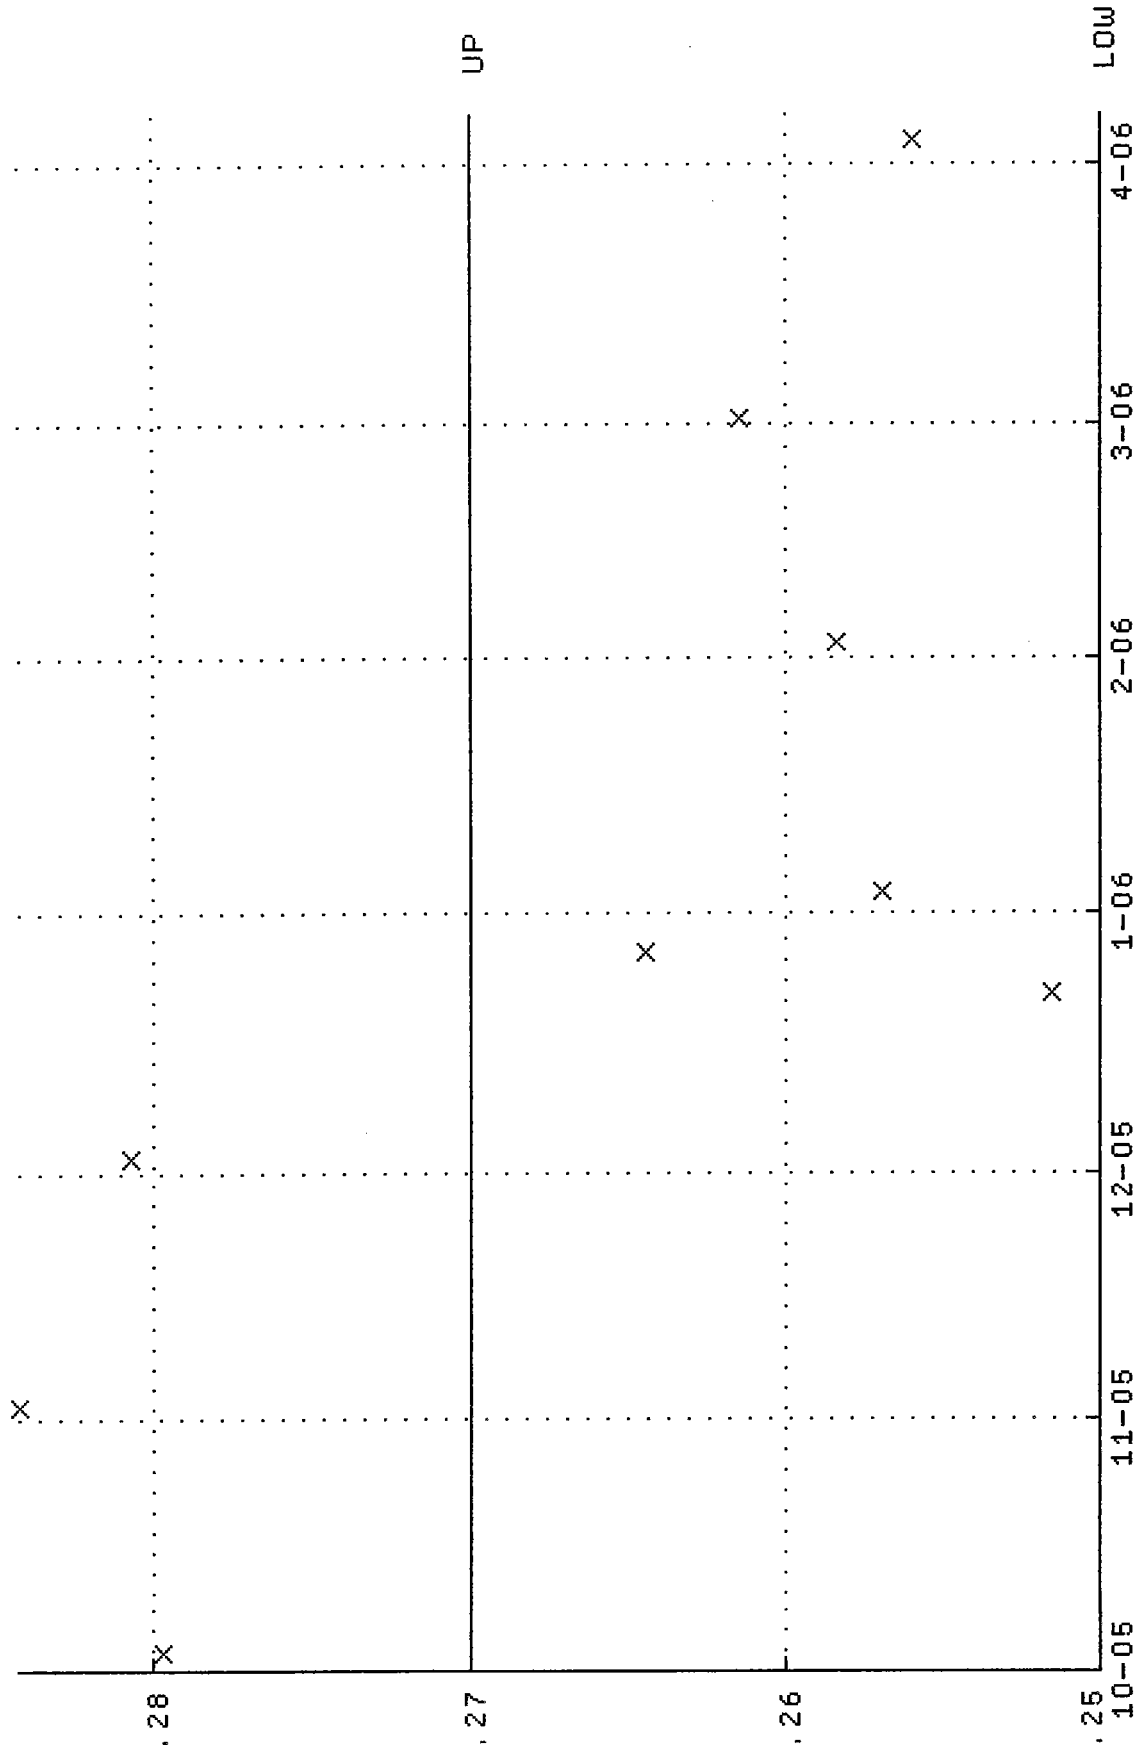


QA filename : DKA100:[ENV_ALPHA,QA,W]W018.QAF;3
 Parameter Name : NLAIVITY-GD148 (NUCLIDE ACTIVITY GD-148)
 Start/End Dates : 3-OCT-2005 07:10:41 through 6-APR-2006 12:00:00
 Lower/Upper Lmts: 60.0000 through 150.0000

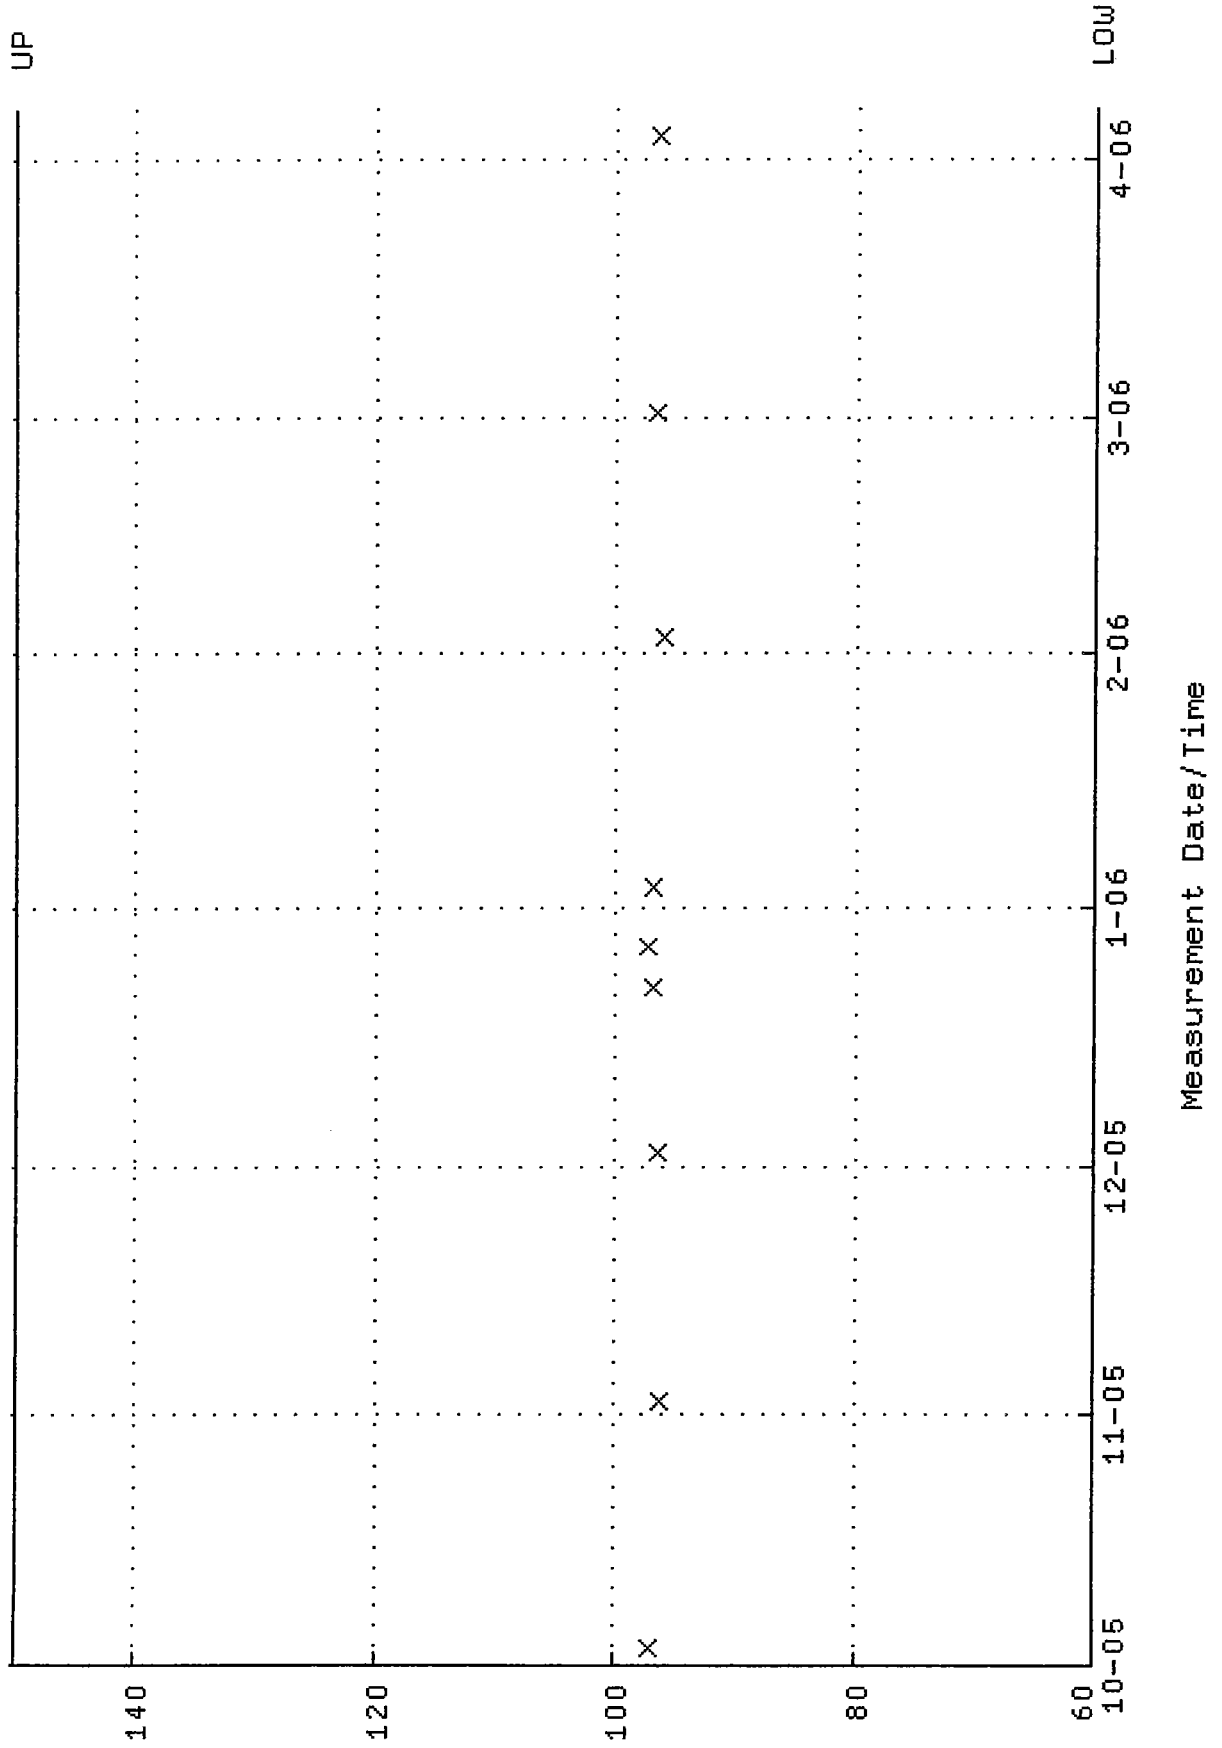


QA filename : DKA100:[ENV_ALPHA.QA.B]B018.QAF;1
 Parameter Name : BACKRATE (Background Rate)
 Start/End Dates : 2-OCT-2005 13:25:40 through 6-APR-2006 12:00:00
 Lower/Upper Lmts: 0.000000E+00 through 2.000000E-02

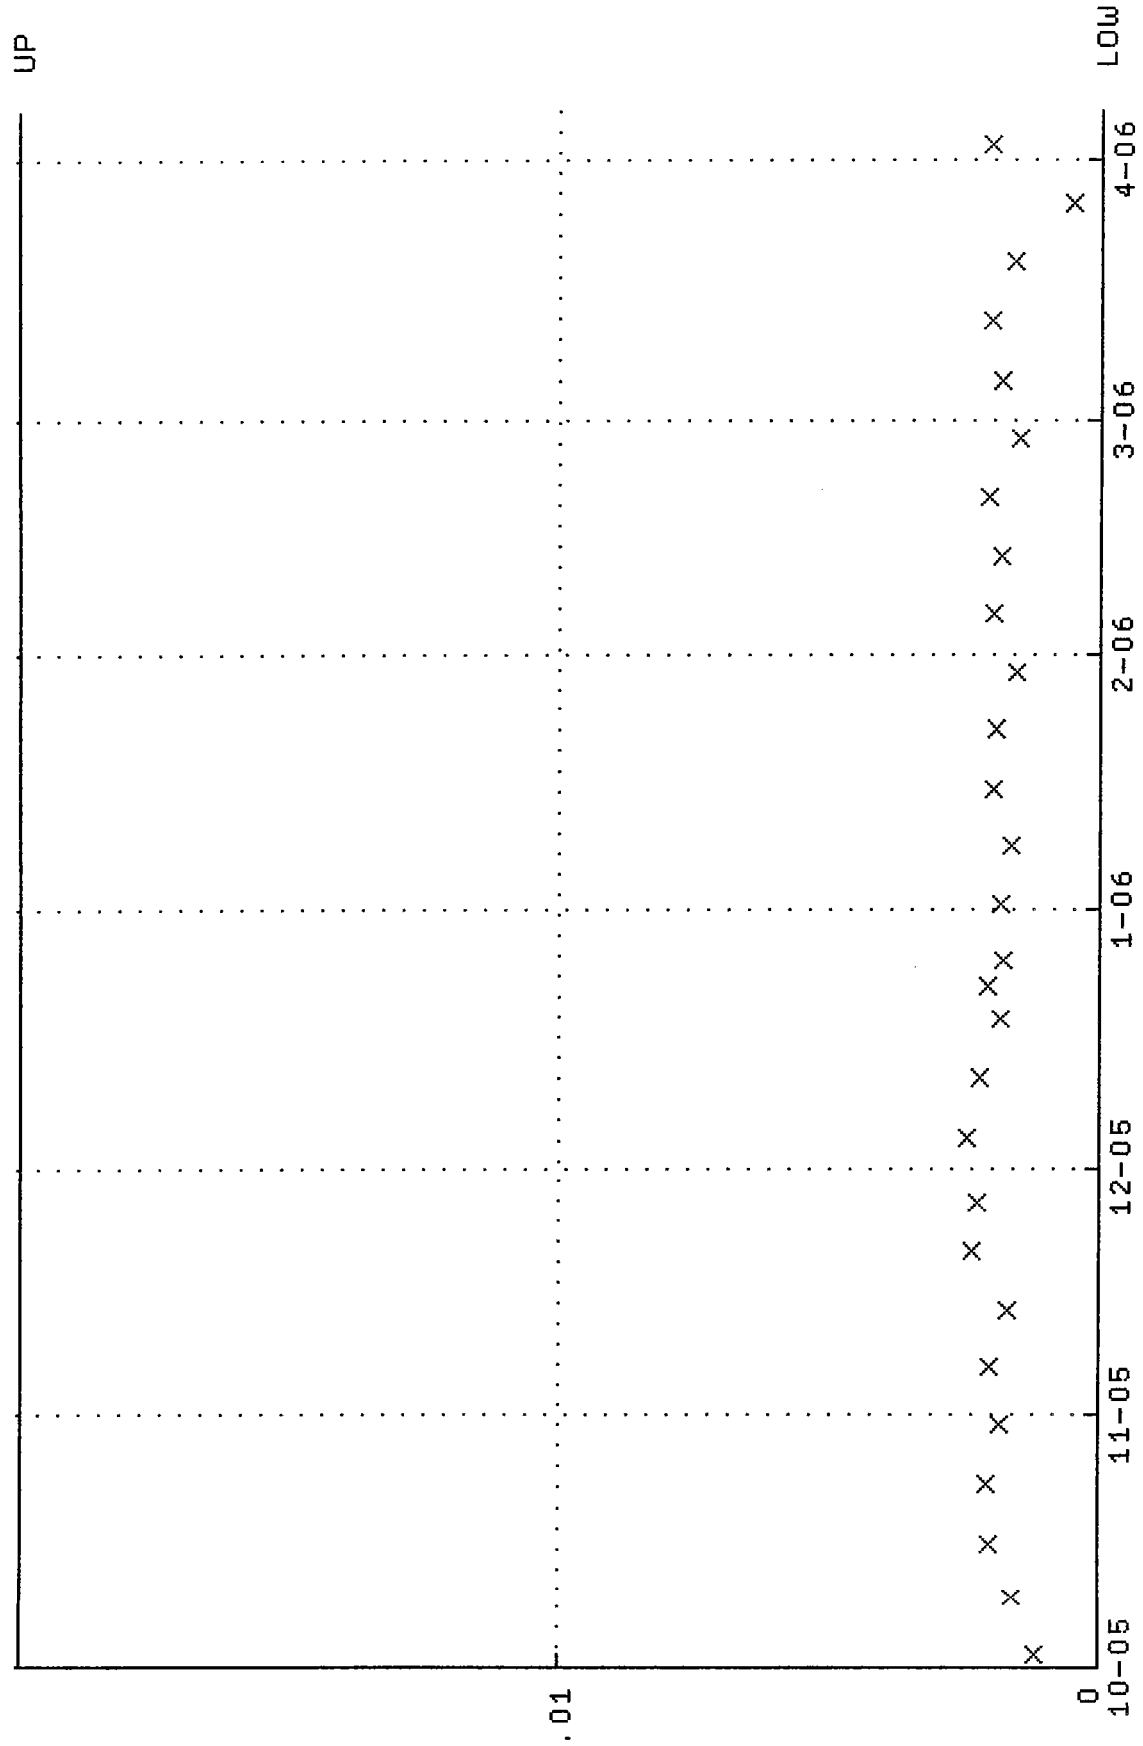


QA filename : DKA100:[ENV_ALPHA.QA.W]W030.QAF;3
 Parameter Name : AVRGEFF (Average Efficiency)
 Start/End Dates : 3-OCT-2005 12:02:07 through 6-APR-2006 12:00:00
 Lower/Upper Lmts: 0.240000 through 0.330000

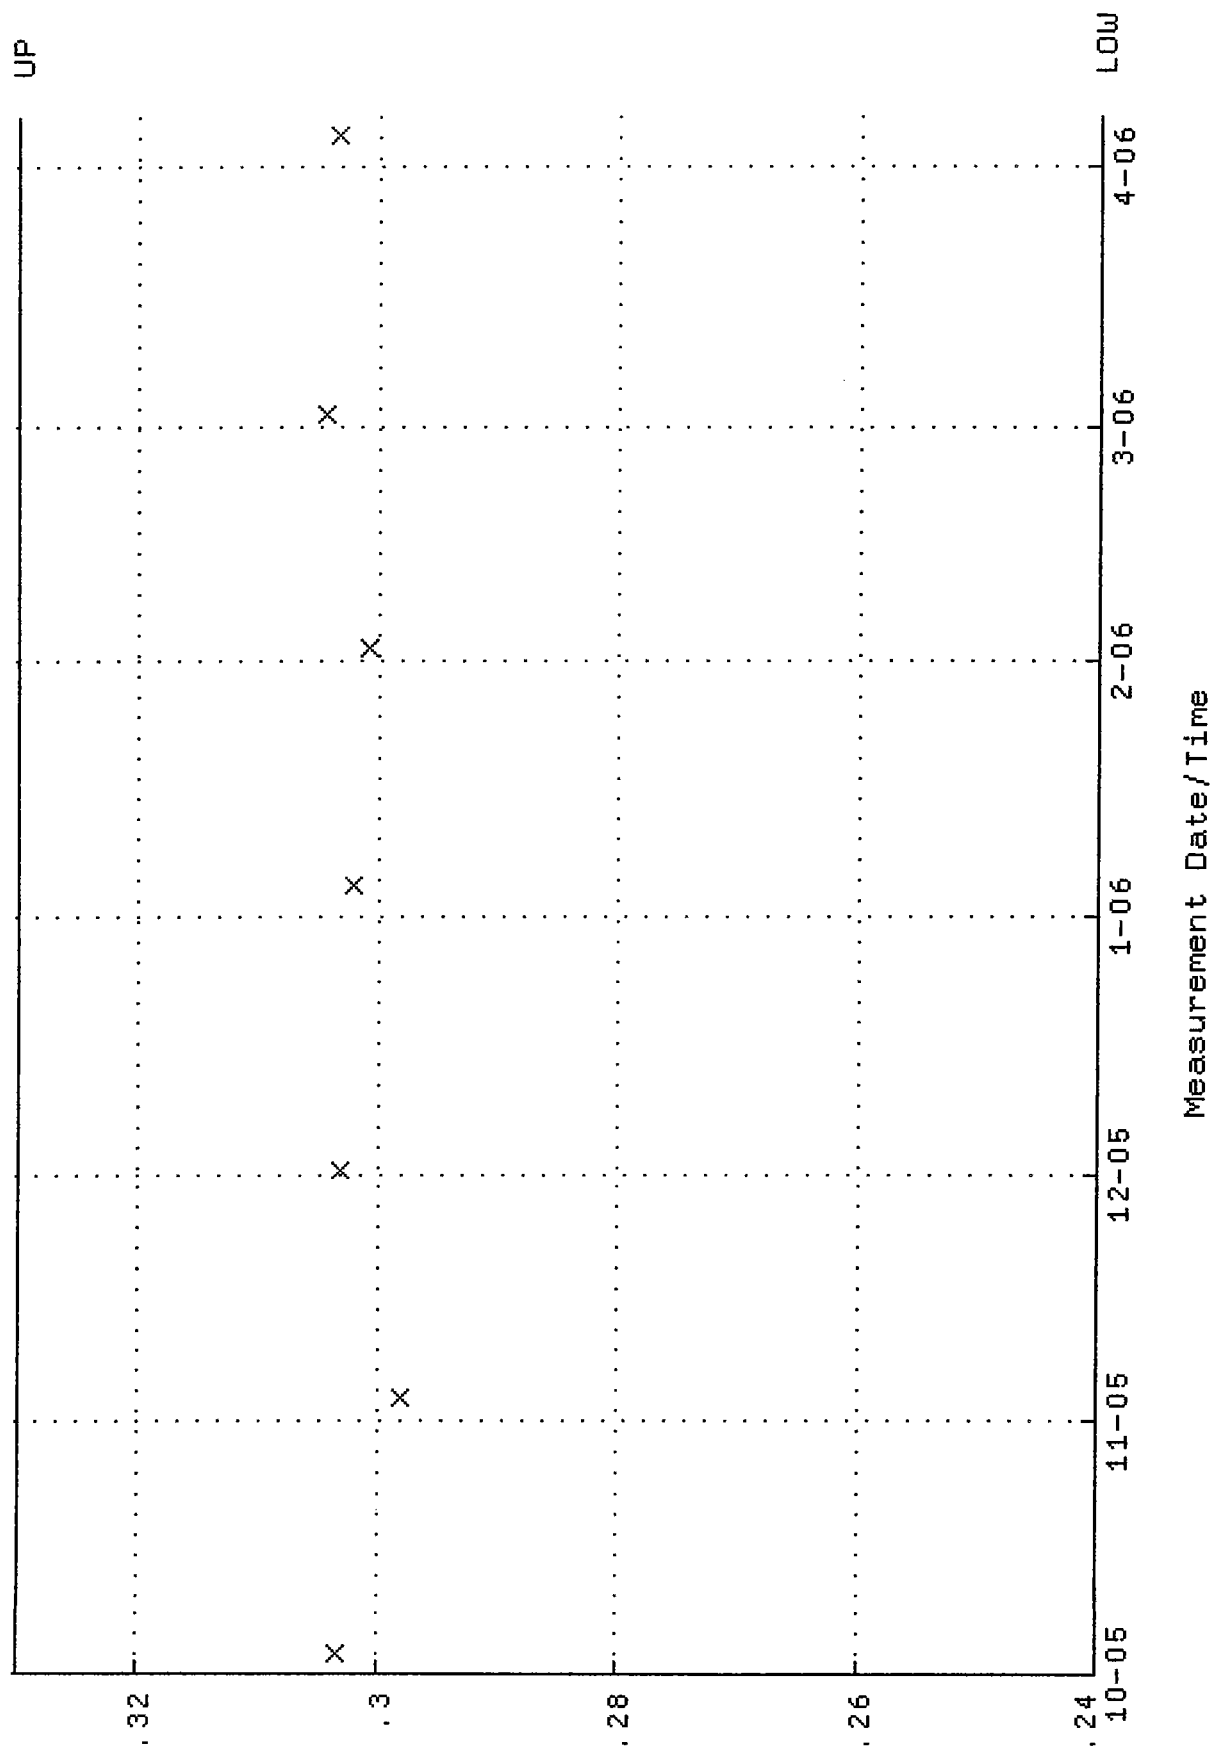


QA filename : DKA100:[ENV_ALPHA.QA.W]W030.QAF;3
 Parameter Name : NLAIVITY-GD148 (NUCLIDE ACTIVITY GD-148)
 Start/End Dates : 3-OCT-2005 12:02:07 through 6-APR-2006 12:00:00
 Lower/Upper Lmts: 60.0000 through 150.000

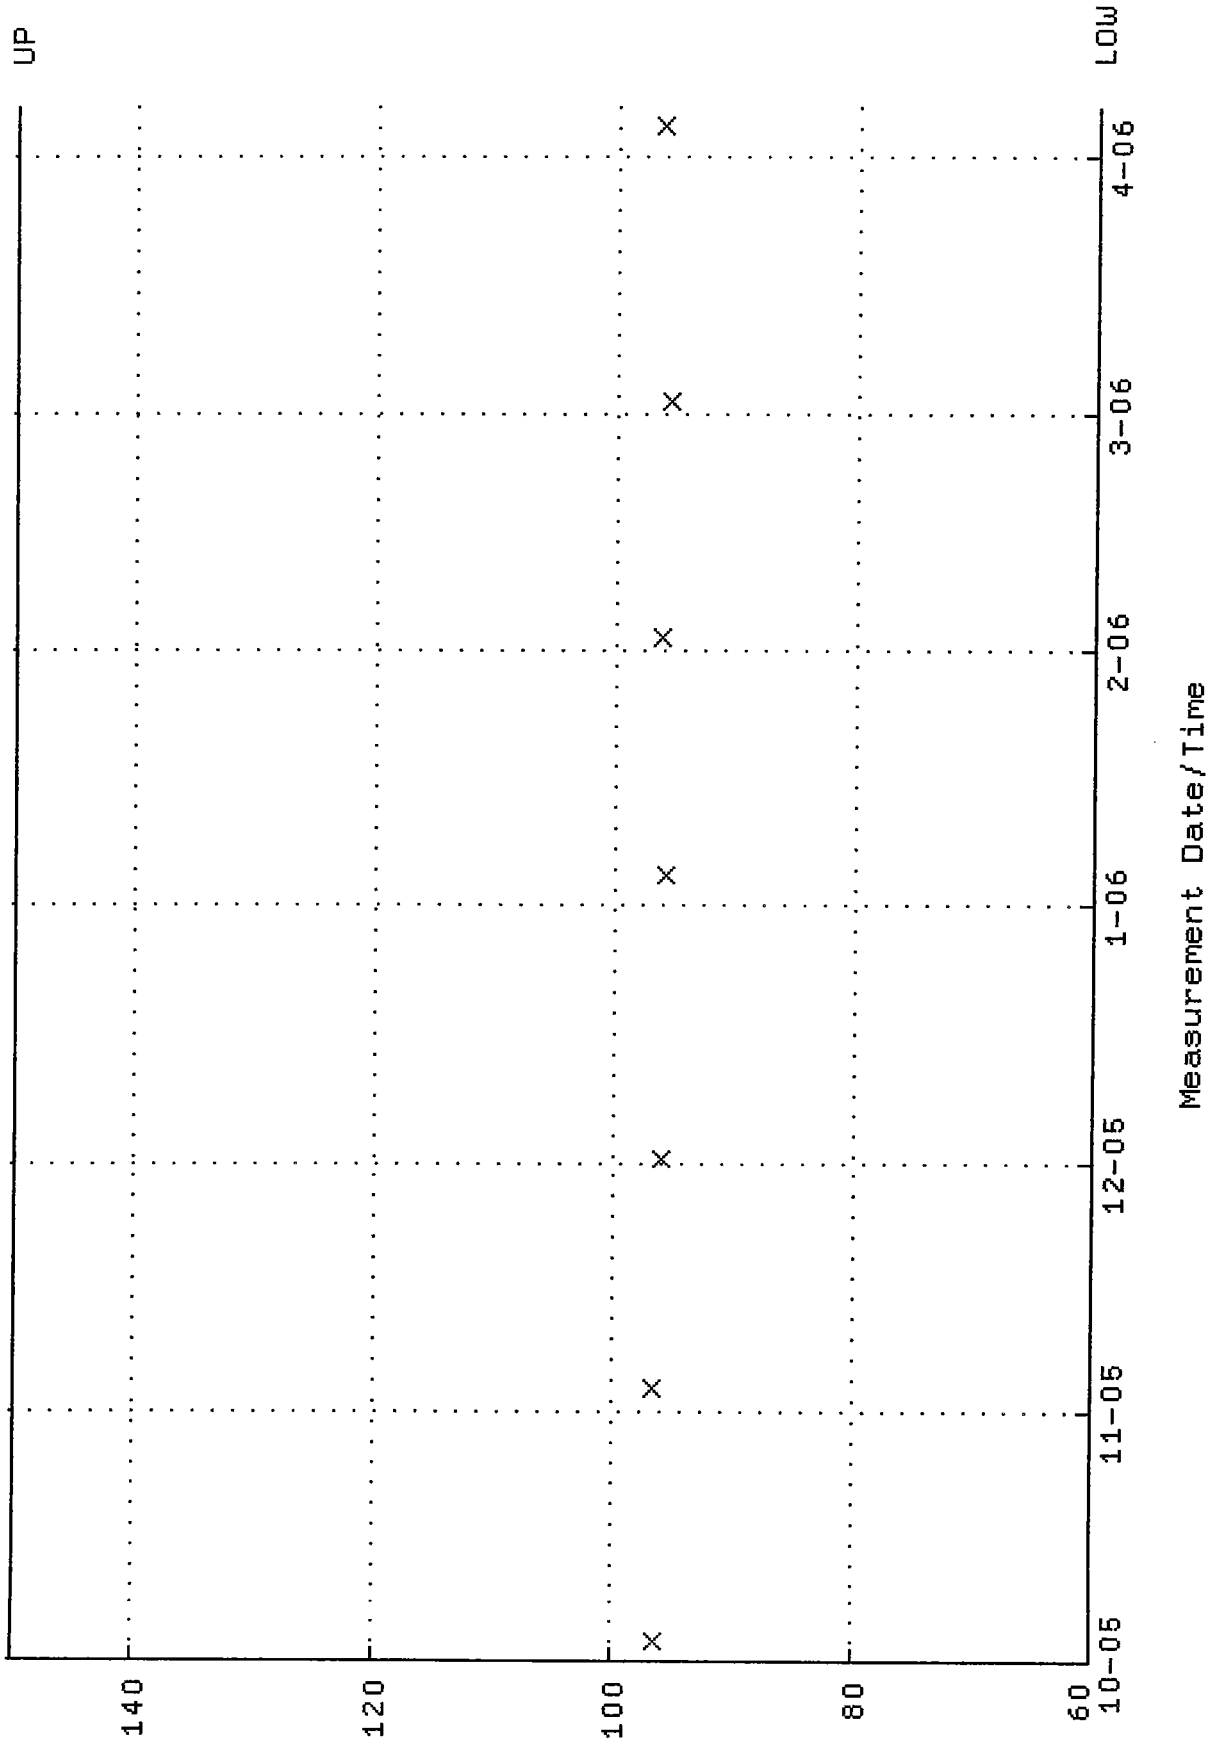


QA filename : DKA100:[ENV_ALPHA.QA.B]B030.QAF;1
 Parameter Name : BACKRATE (Background Rate)
 Start/End Dates : 2-OCT-2005 13:25:42 through 6-APR-2006 12:00:00
 Lower/Upper Lmts: 0.000000E+00 through 2.000000E-02

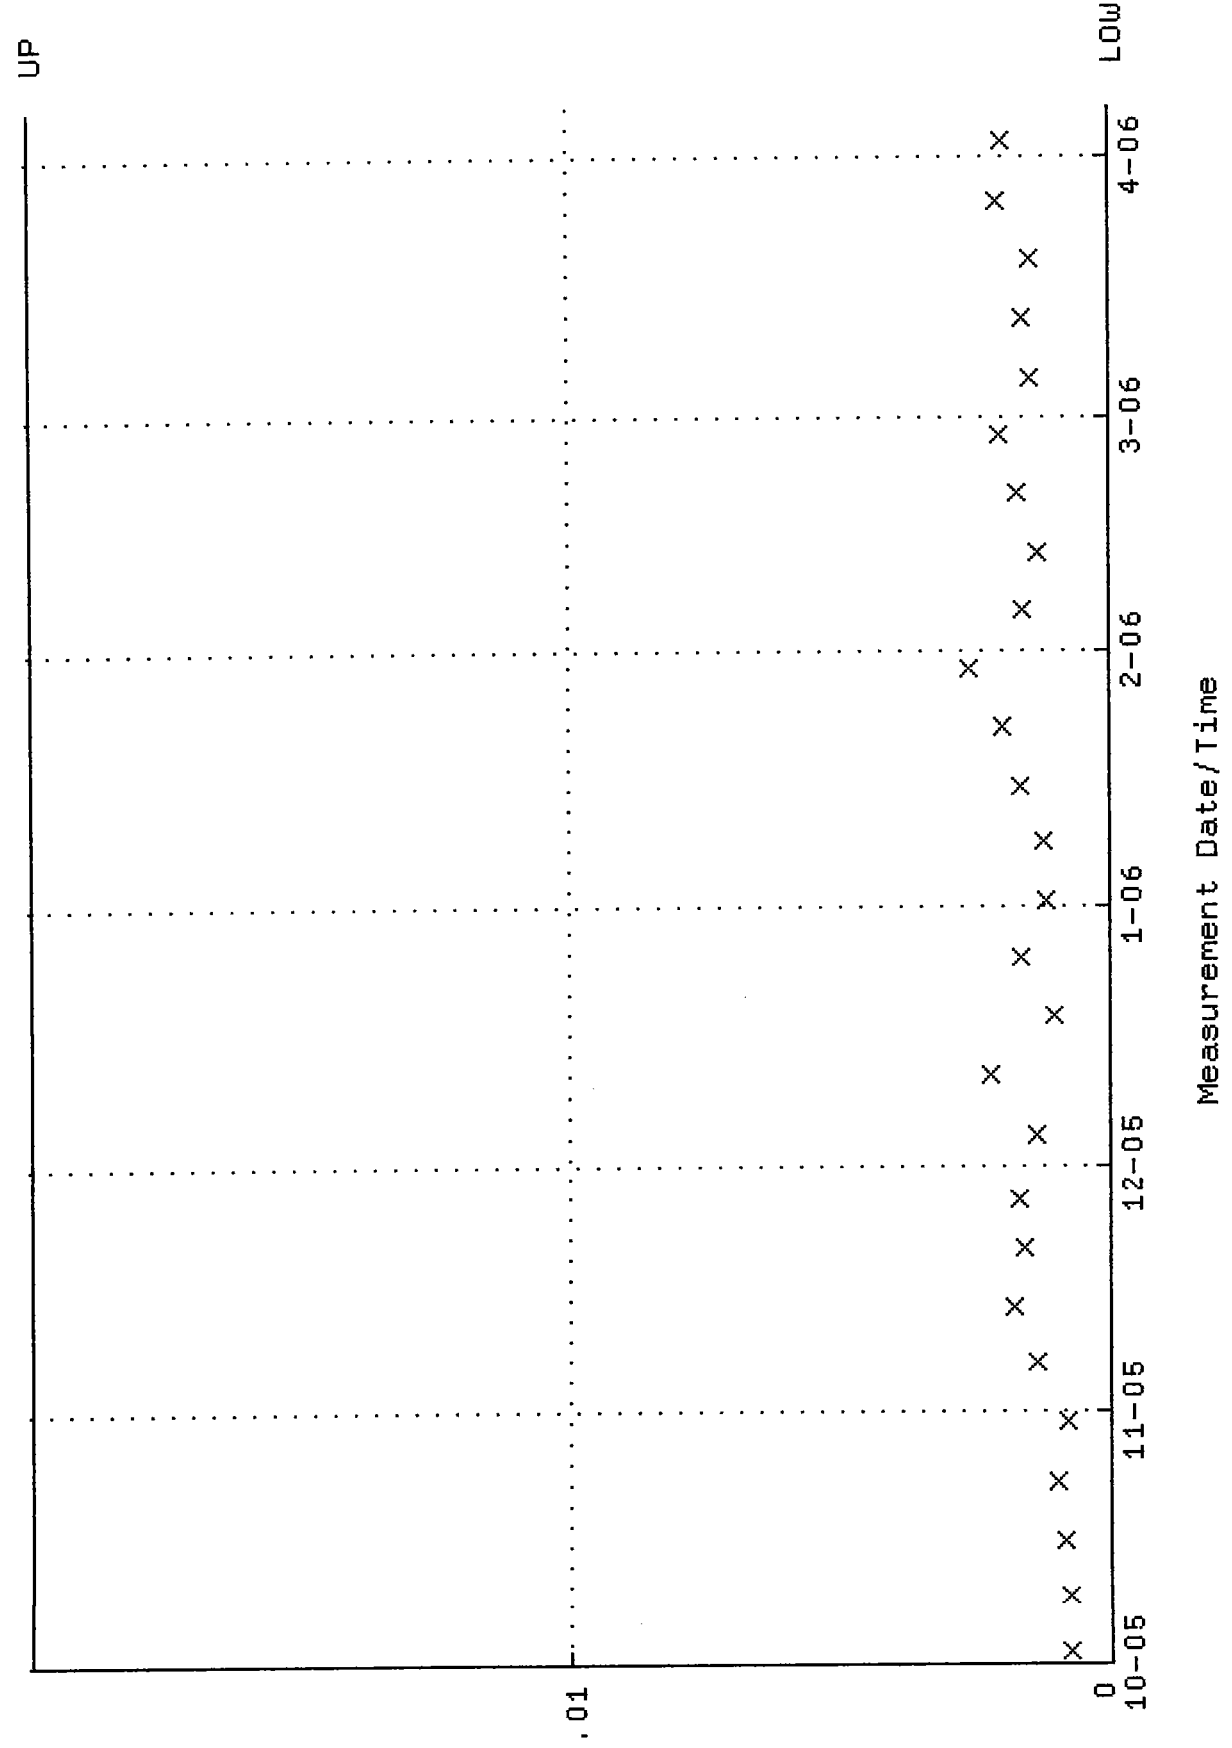


QA filename : DKA100:[ENV_ALPHA.QA.W]W032.QAF;4
 Parameter Name : AVRGEFF (Average Efficiency)
 Start/End Dates : 3-OCT-2005 12:02:09 through 6-APR-2006 12:00:00
 Lower/Upper Lmts: 0.280000 through 0.370000

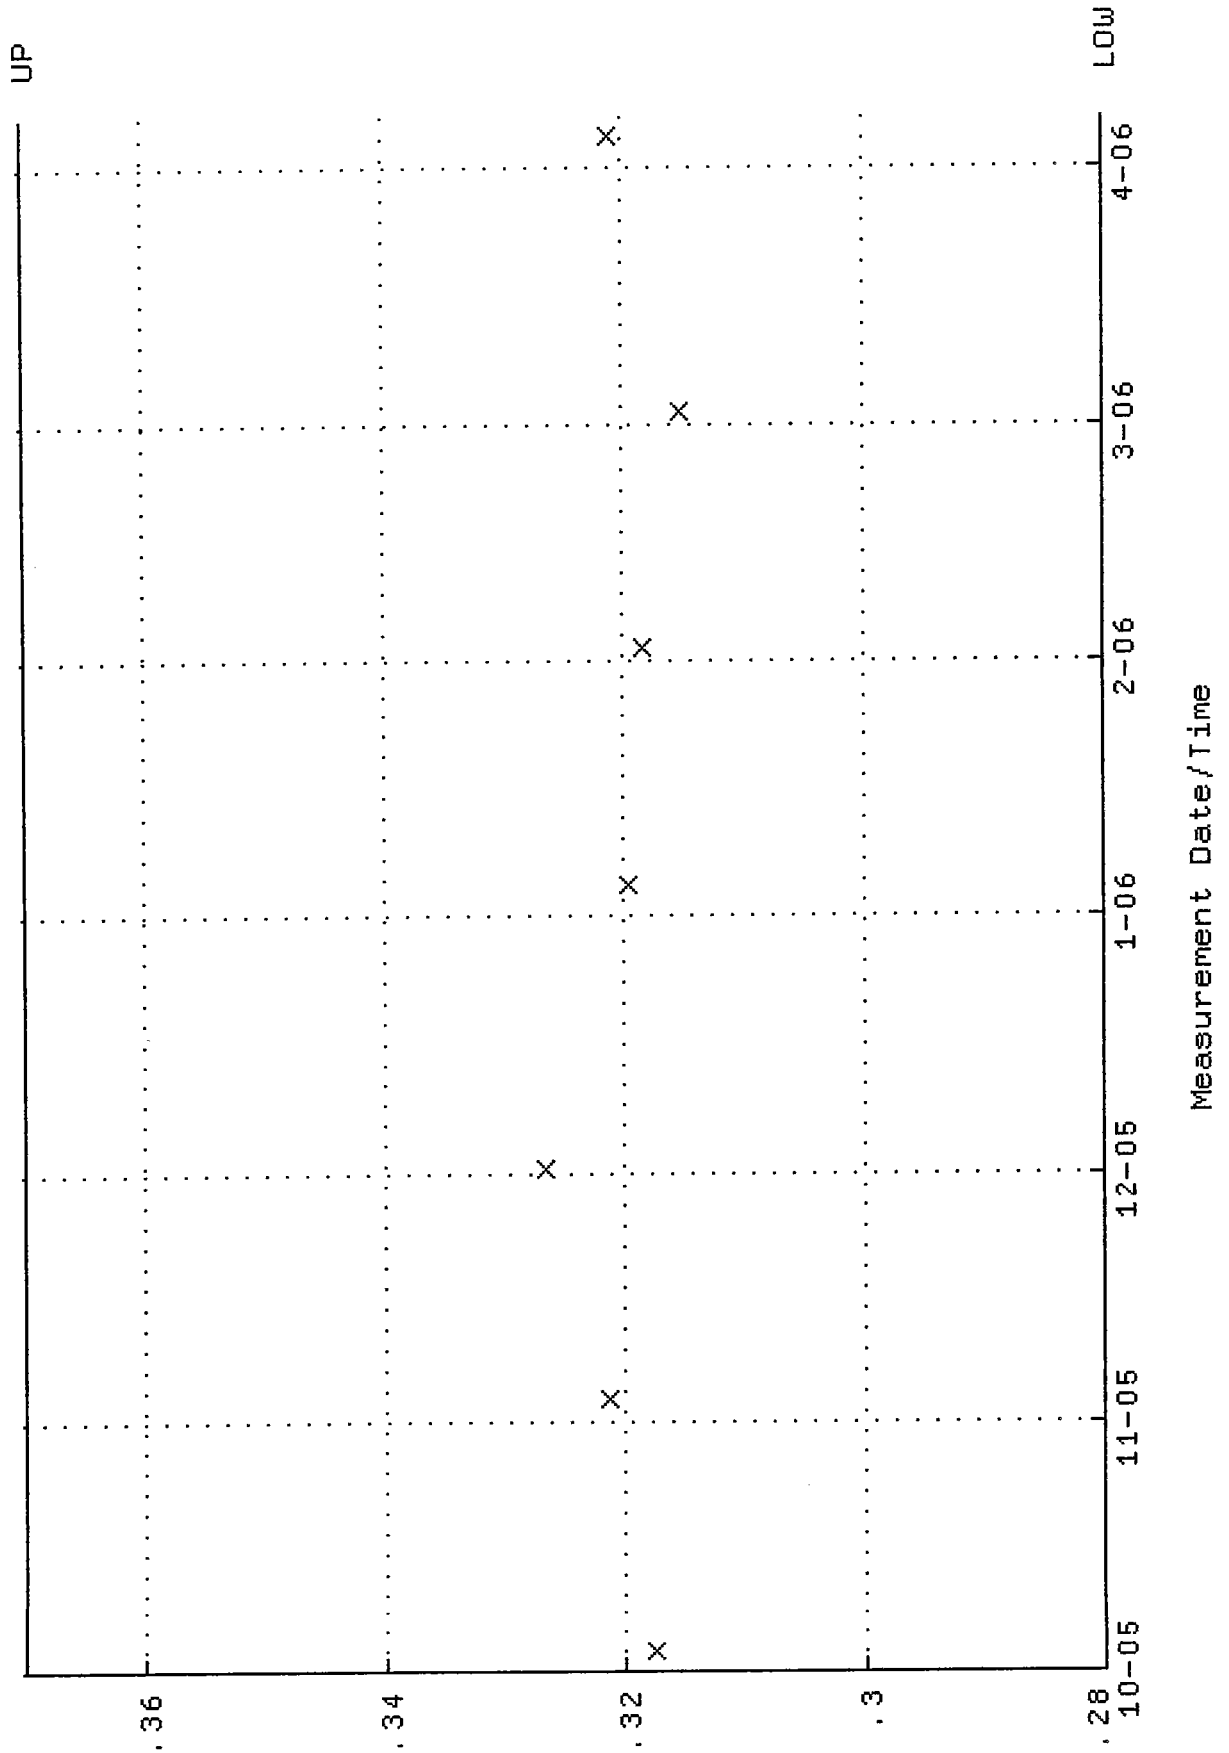


QA filename : DKA100:[ENVY_ALPHA.QA.W]W032.QAF; 4
 Parameter Name : NLAIVITY-GD148 (NUCLIDE ACTIVITY GD-148)
 Start/End Dates : 3-OCT-2005 12:02:09 through 6-APR-2006 12:00:00
 Lower/Upper Lmts: 60.0000 through 150.0000

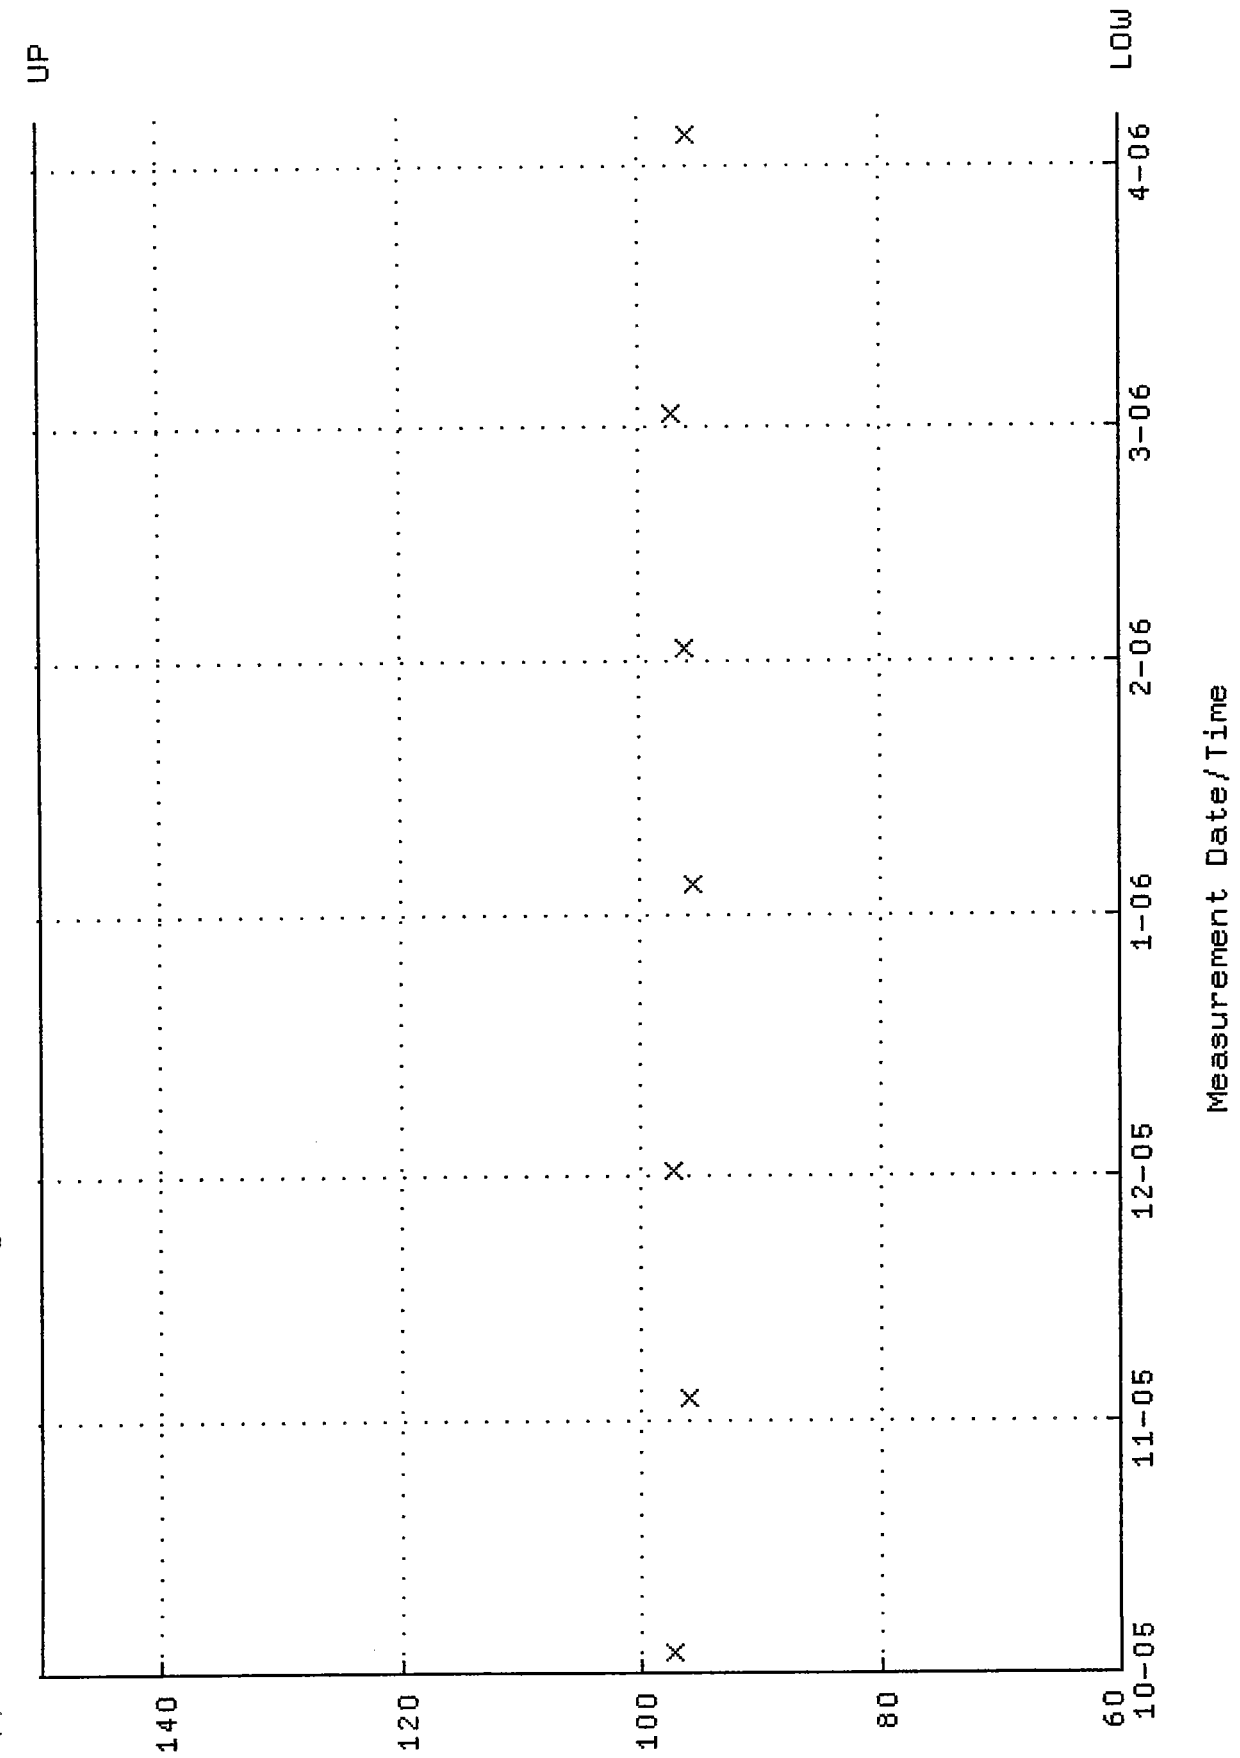


QA filename : DKA100:[ENV_ALPHA.QA.B]B032.QAF;2
 Parameter Name : BACKRATE (Background Rate)
 Start/End Dates : 2-OCT-2005 13:25:42 through 6-APR-2006 12:00:00
 Lower/Upper Lmts: 0.000000E+00 through 2.000000E-02

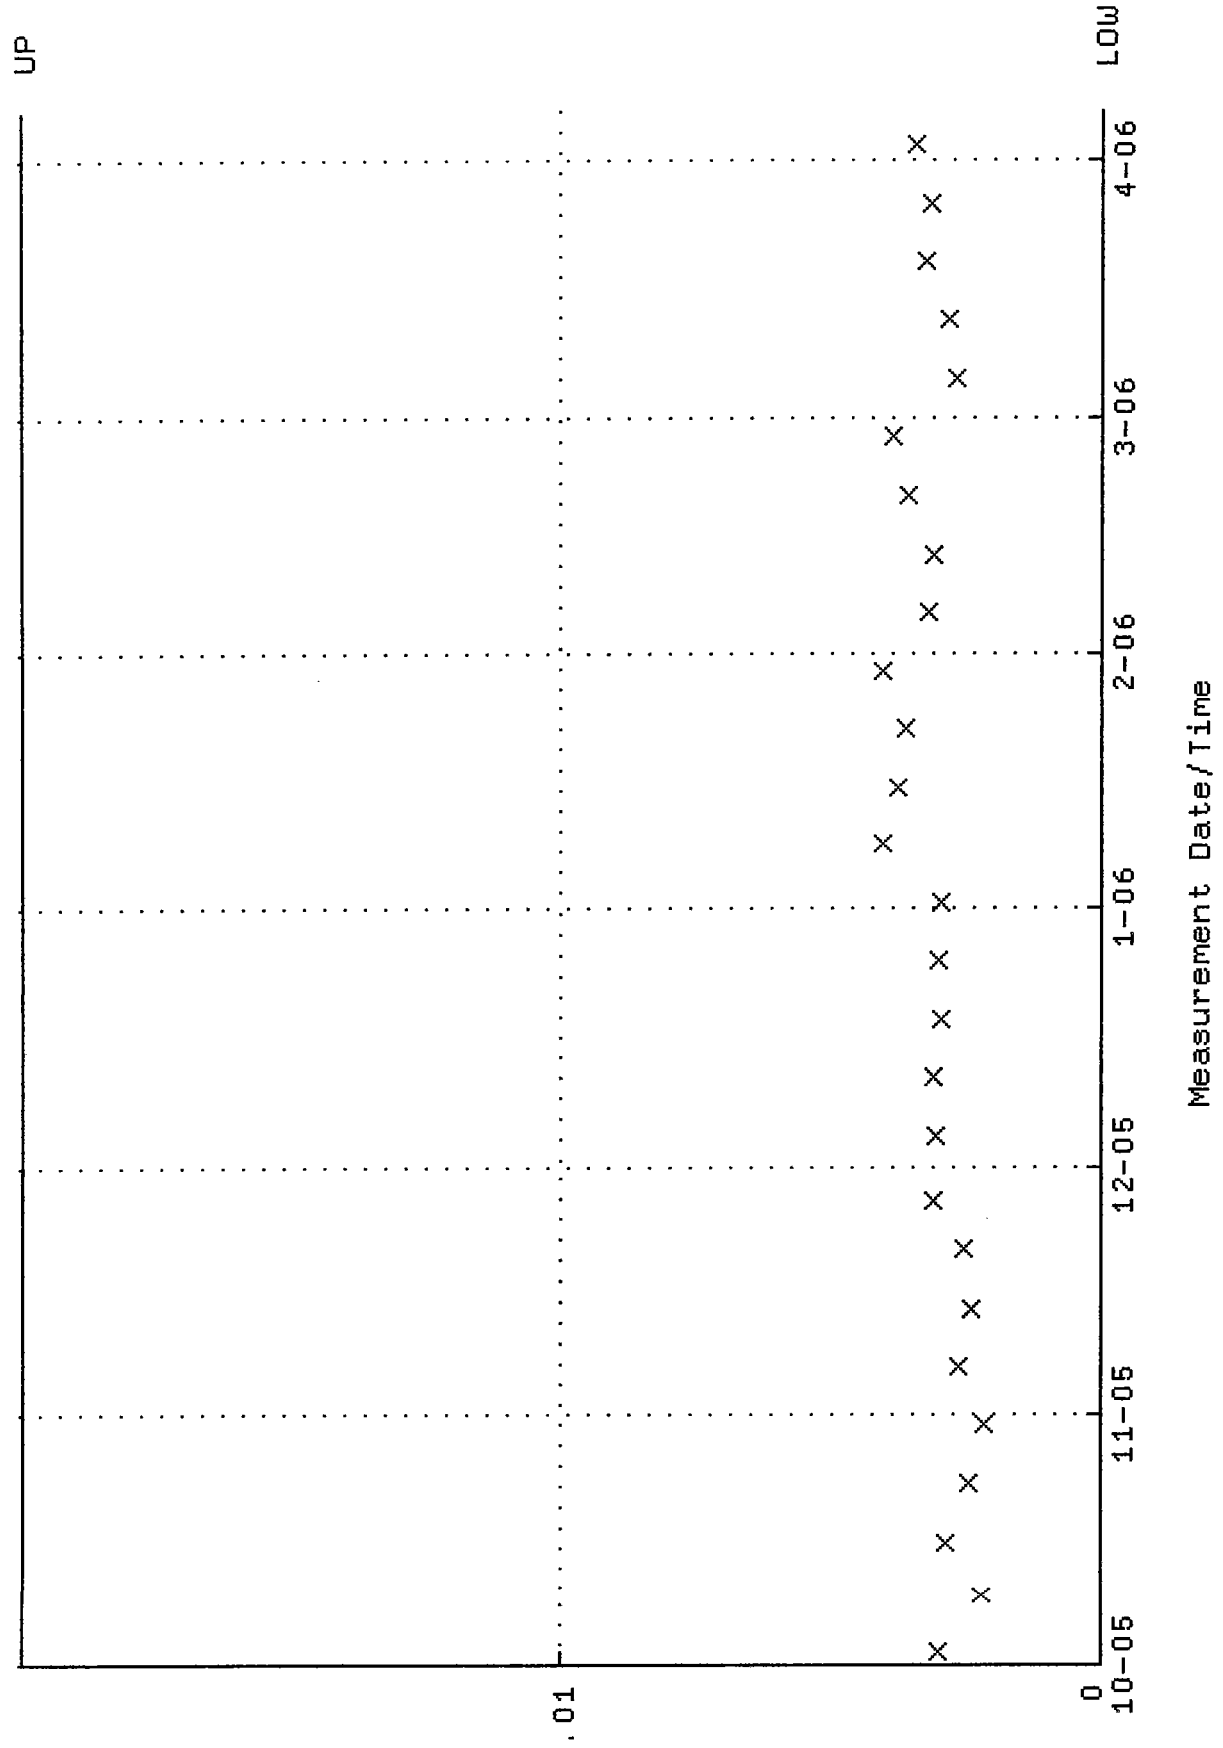


QA filename : DKA100:[ENV_ALPHA.QA.w]w033.QAF;3
 Parameter Name : AVRGEFF (Average Efficiency)
 Start/End Dates : 3-OCT-2005 12:02:09 through 6-APR-2006 12:00:00
 Lower/Upper Lmts: 0.280000 through 0.370000

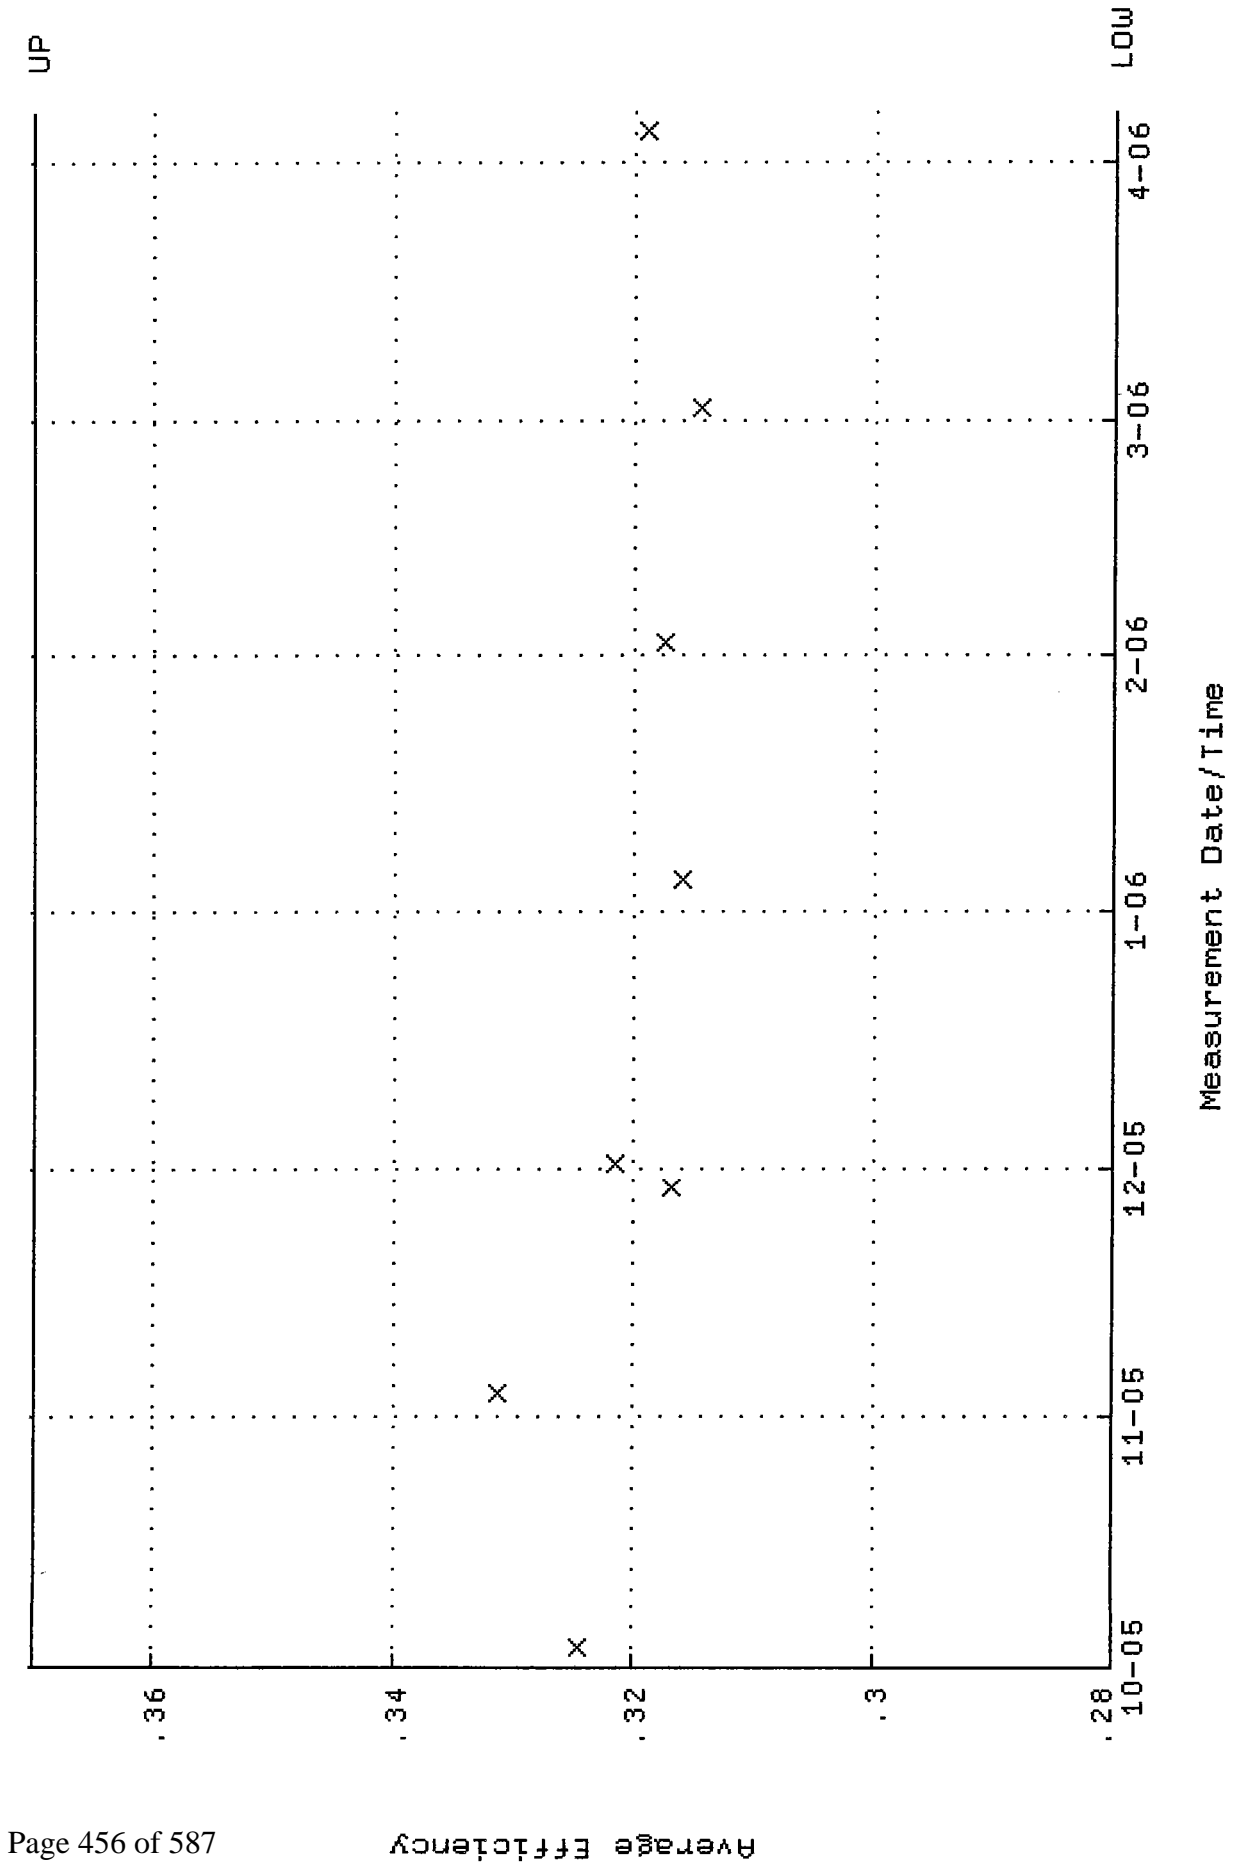


QA filename : DKA100:[ENV_ALPHA.QA.W]W033.QAF;3
 Parameter Name : NLAIVITY-GD148 (NUCLIDE ACTIVITY GD-148)
 Start/End Dates : 3-OCT-2005 12:02:09 through 6-APR-2006 12:00:00
 Lower/Upper Lmts: 60.0000 through 150.0000

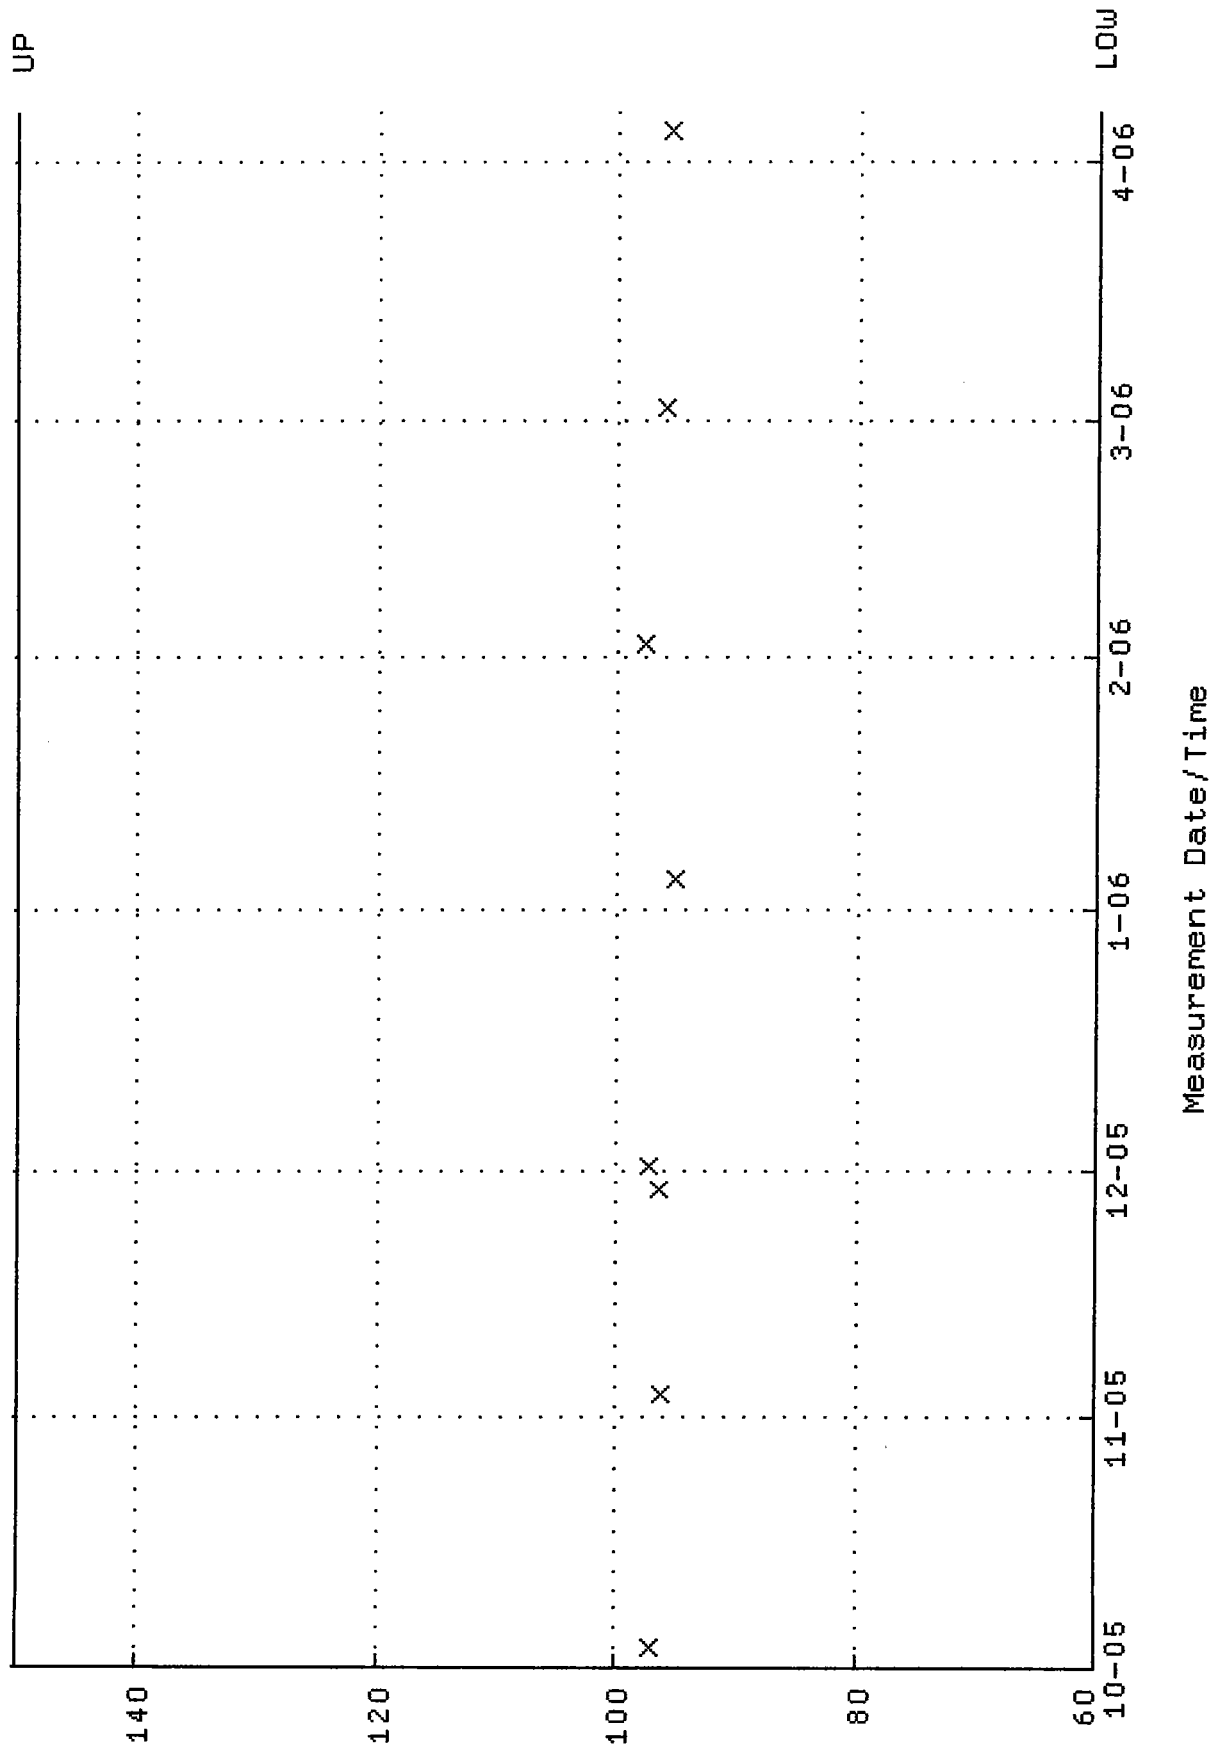


QA filename : DKA100:[ENV_ALPHA.QA.B]B033.QAF;1
 Parameter Name : BACKRATE (Background Rate)
 Start/End Dates : 2-OCT-2005 13:25:42 through 6-APR-2006 12:00:00
 Lower/Upper Lmts: 0.000000E+00 through 2.000000E-02

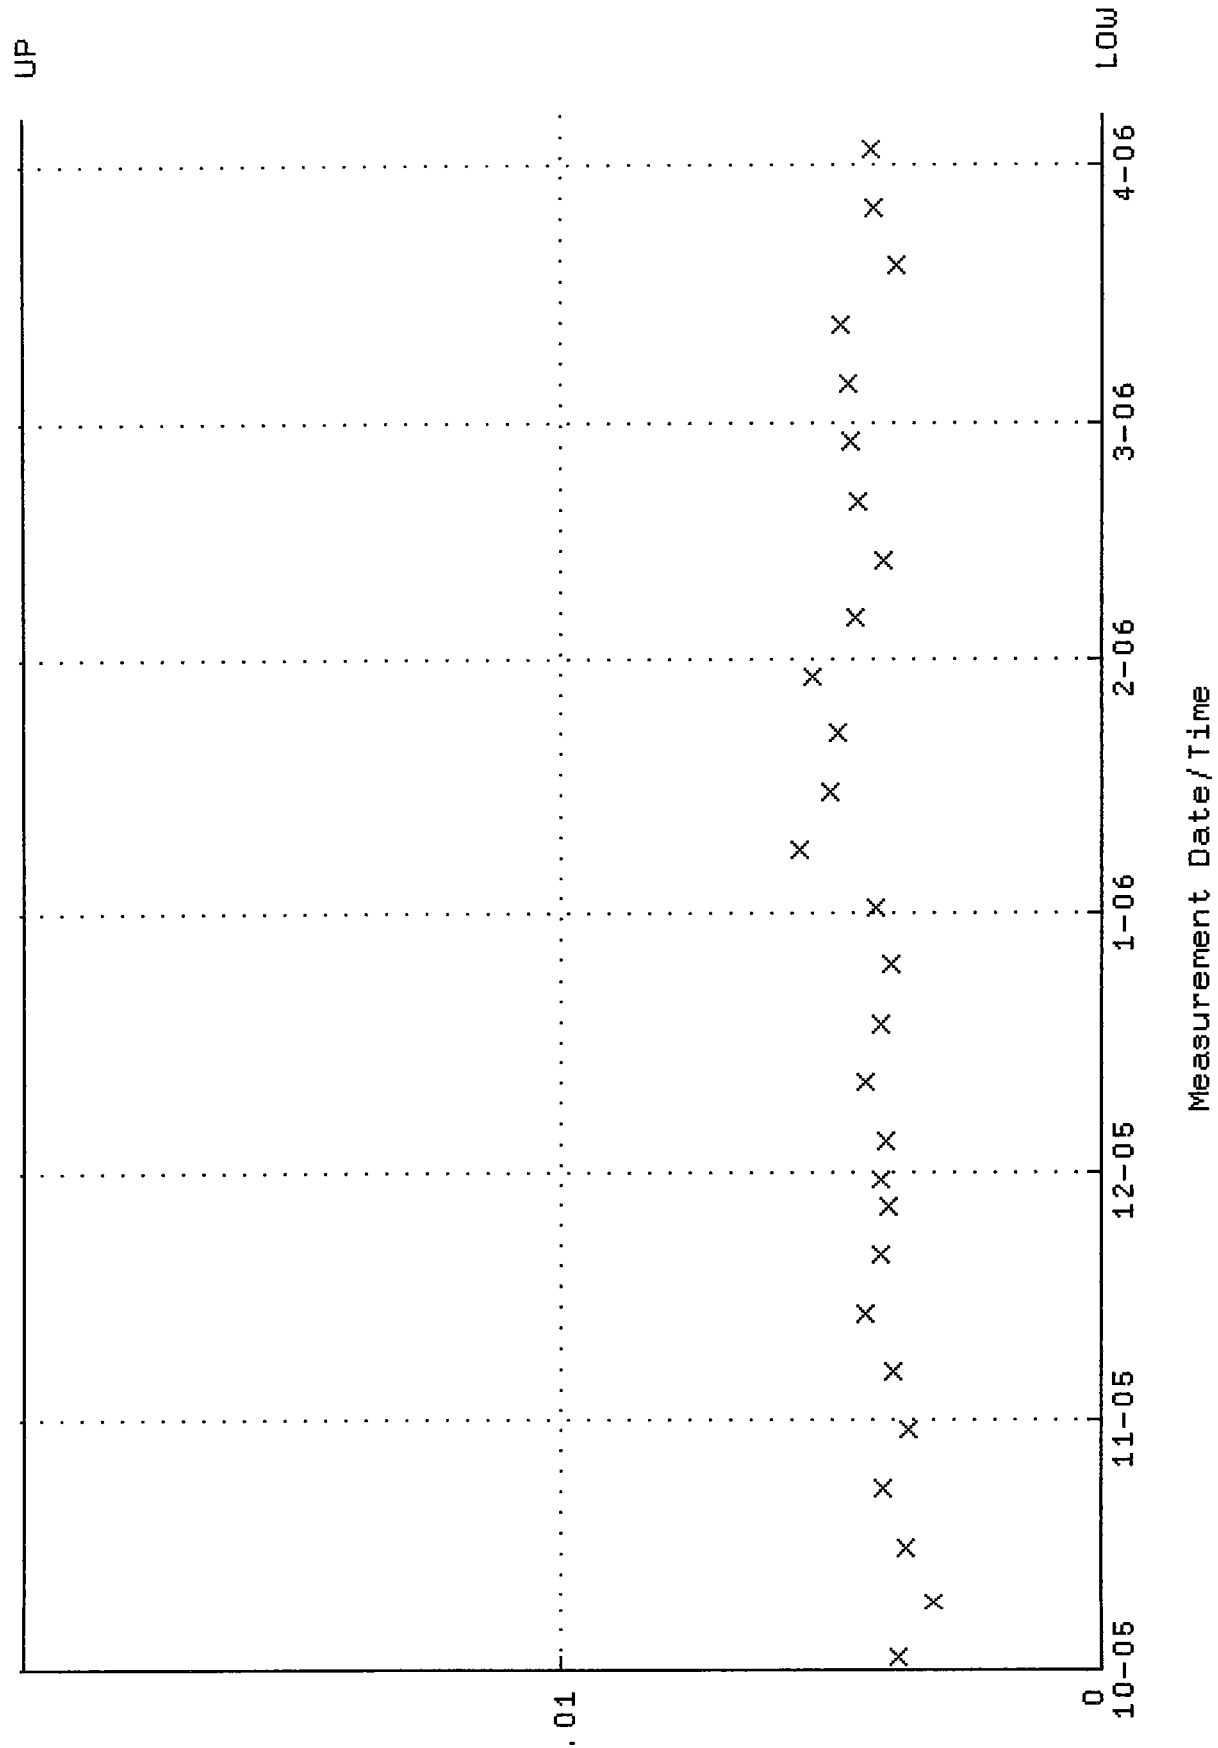


QA filename : DKA100:[ENV_ALPHA.QA.W]W034.QAF;3
 Parameter Name : AVRGEFF (Average Efficiency)
 Start/End Dates : 3-OCT-2005 12:02:09 through 6-APR-2006 12:00:00
 Lower/Upper Lmts: 0.280000 through 0.370000

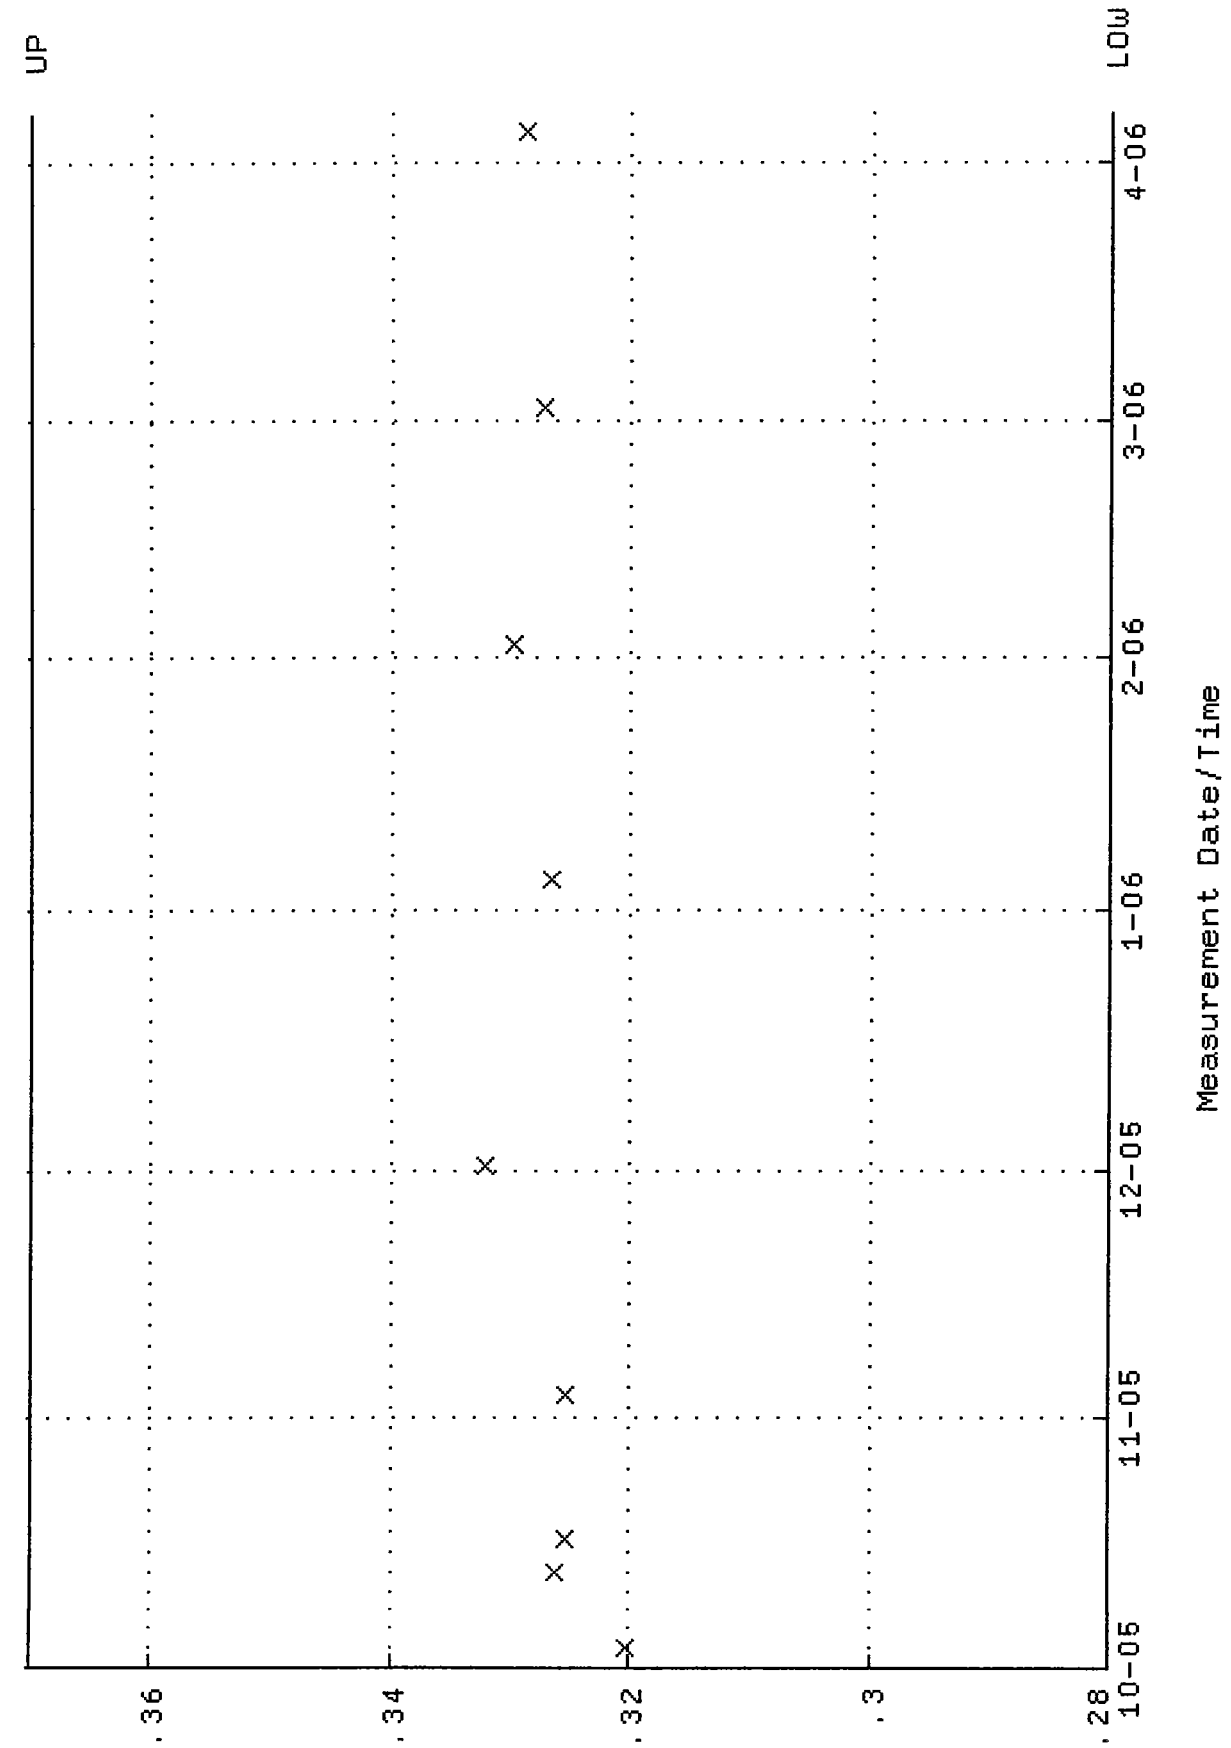


QA filename : DKA100:[ENV_ALPHA.QA.W]W034.QAF;3
 Parameter Name : NLAIVITY-GD148 (NUCLIDE ACTIVITY GD-148)
 Start/End Dates : 3-OCT-2005 12:02:09 through 6-APR-2006 12:00:00
 Lower/Upper Lmts: 60.0000 through 150.0000

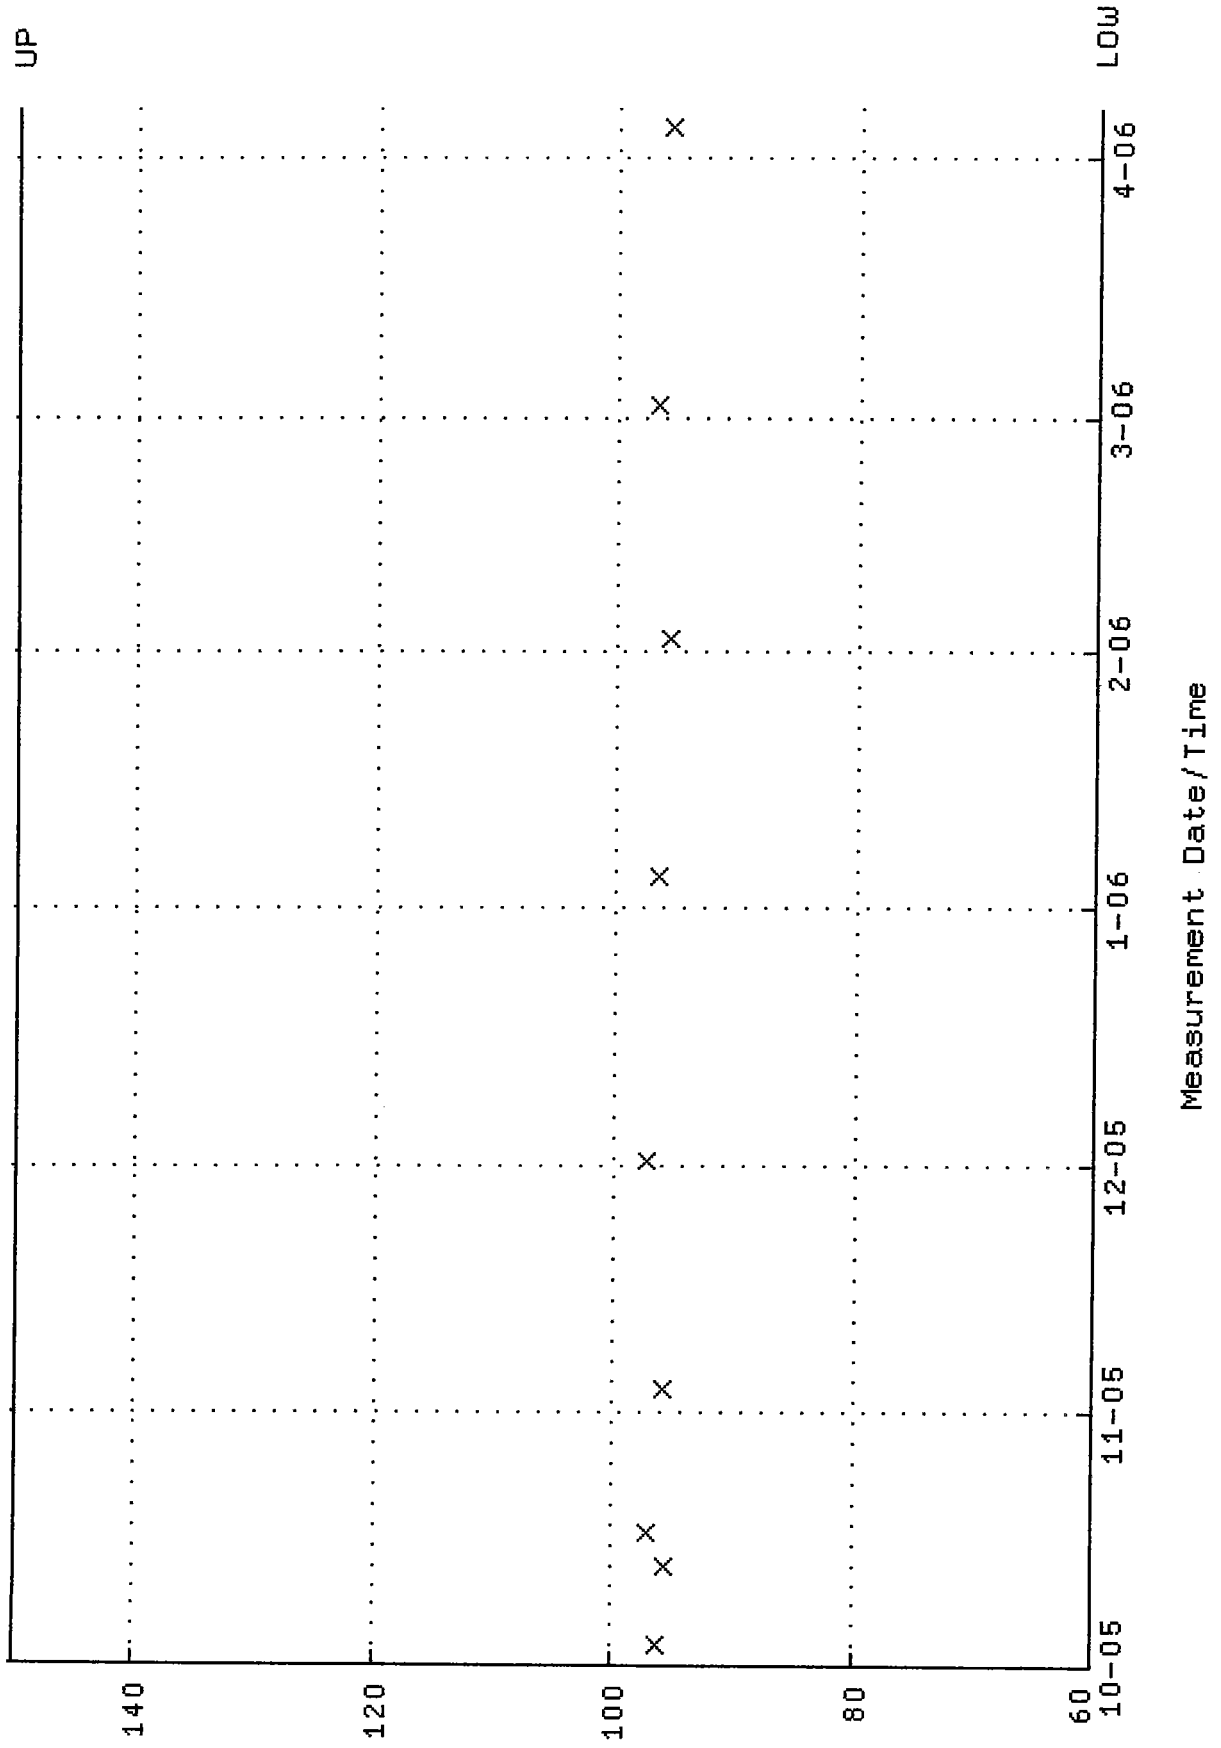


QA filename : DKA100:[ENV_ALPHA.QA.B]B034.QAF;1
 Parameter Name : BACKRATE (Background Rate)
 Start/End Dates : 2-OCT-2005 13:25:42 through 6-APR-2006 12:00:00
 Lower/Upper Lmts: 0.000000E+00 through 2.000000E-02

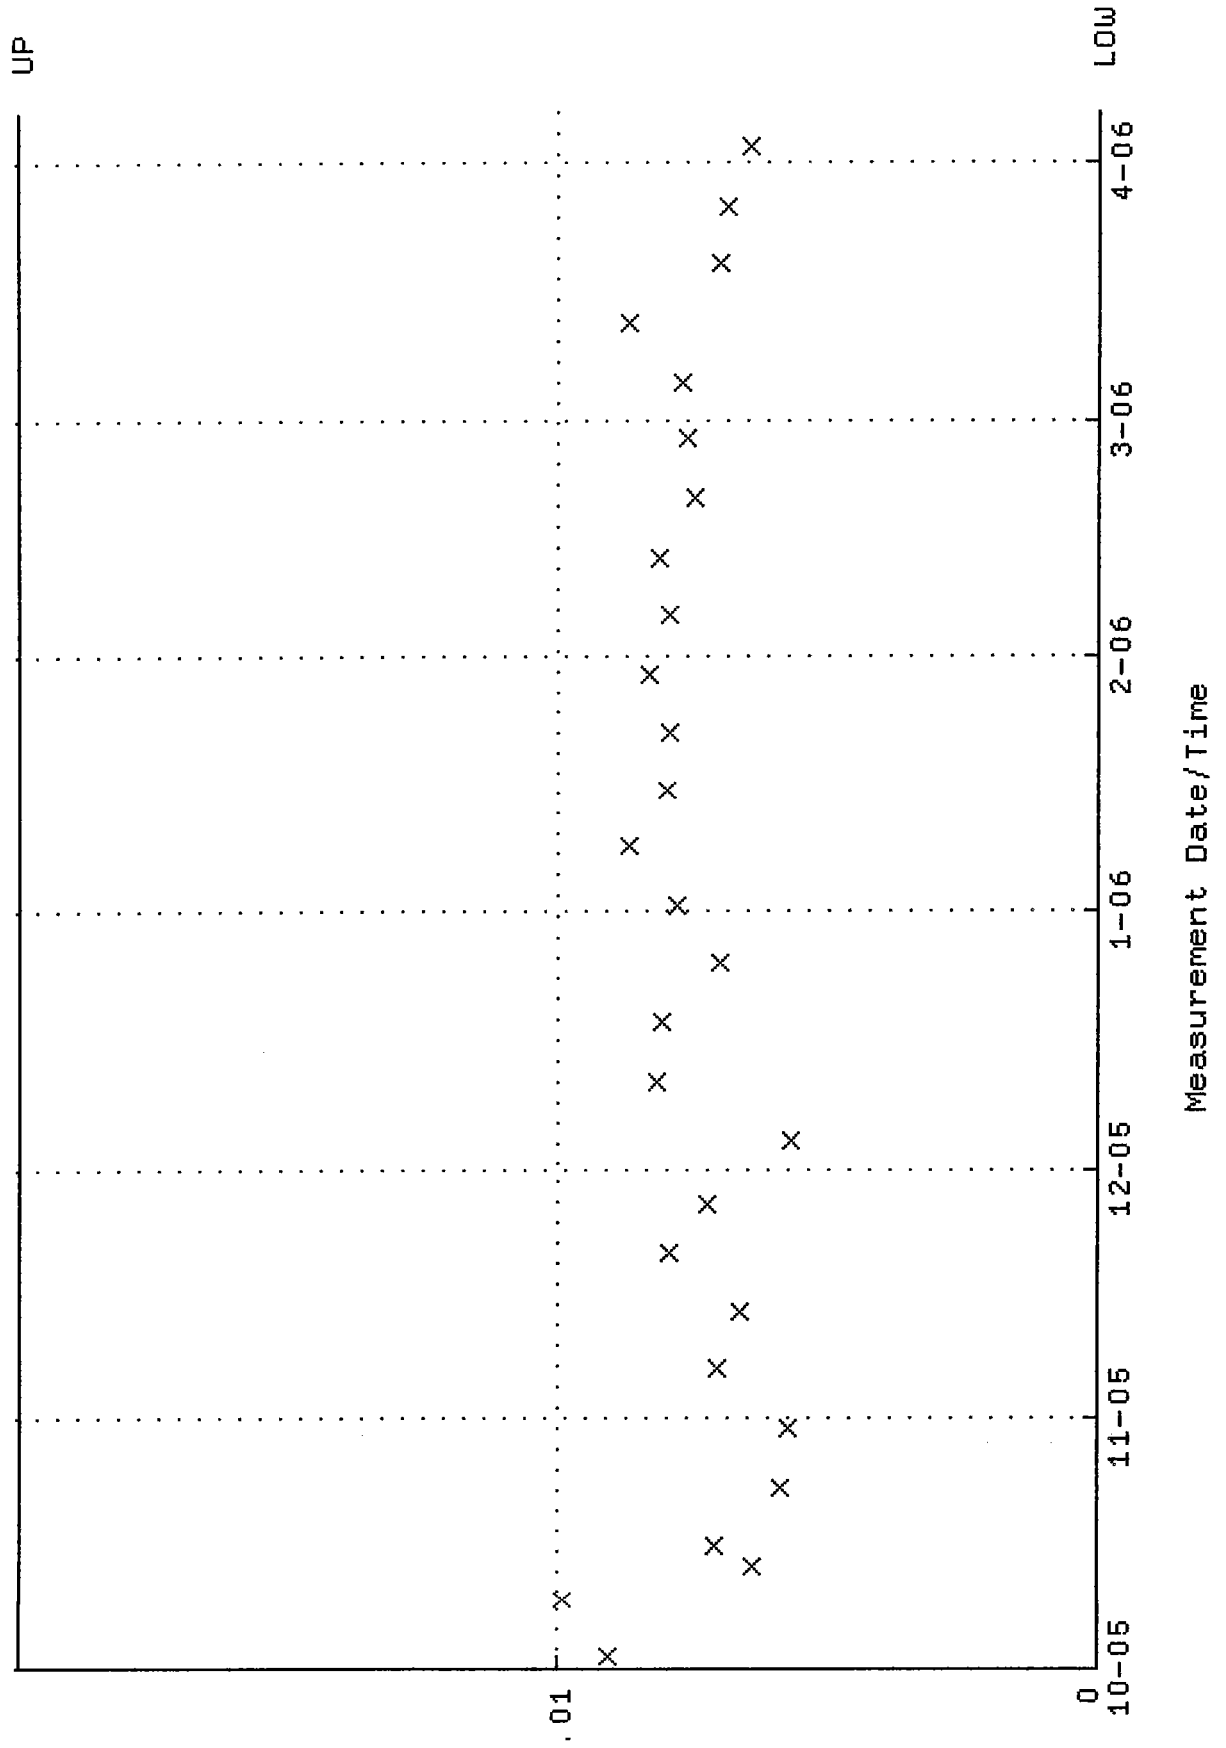


QA filename : DKA100:[ENV_ALPHA.QA.w]w037.QAF;4
 Parameter Name : AVRGEFF (Average Efficiency)
 Start/End Dates : 3-OCT-2005 12:02:11 through 6-APR-2006 12:00:00
 Lower/Upper Lmts: 0.320000 through 0.360000

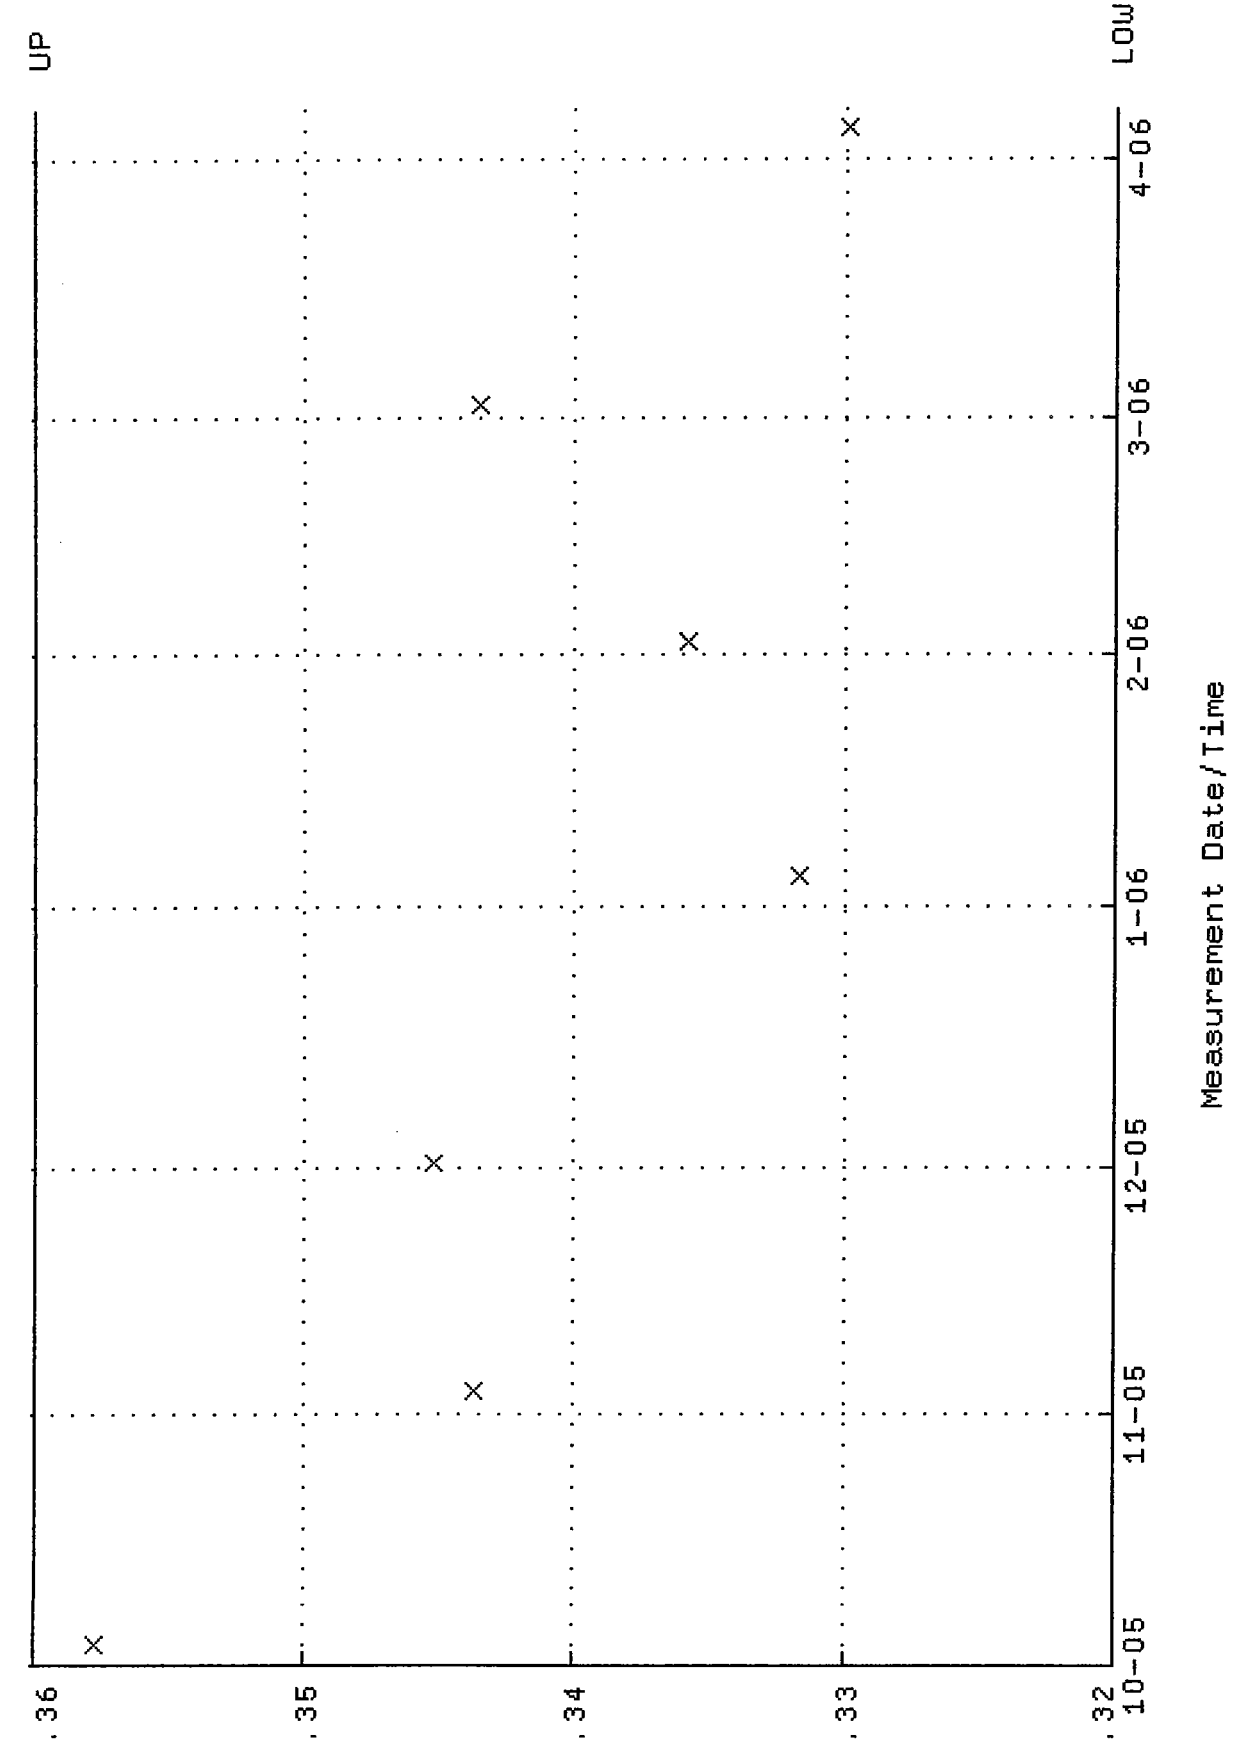


QA filename : DKA100:[ENV_ALPHA.QA.w]w037.QAF; 4
 Parameter Name : NLAIVITY-GD148 (NUCLIDE ACTIVITY GD-148)
 Start/End Dates : 3-OCT-2005 12:02:11 through 6-APR-2006 12:00:00
 Lower/Upper Lmts: 60.0000 through 150.0000

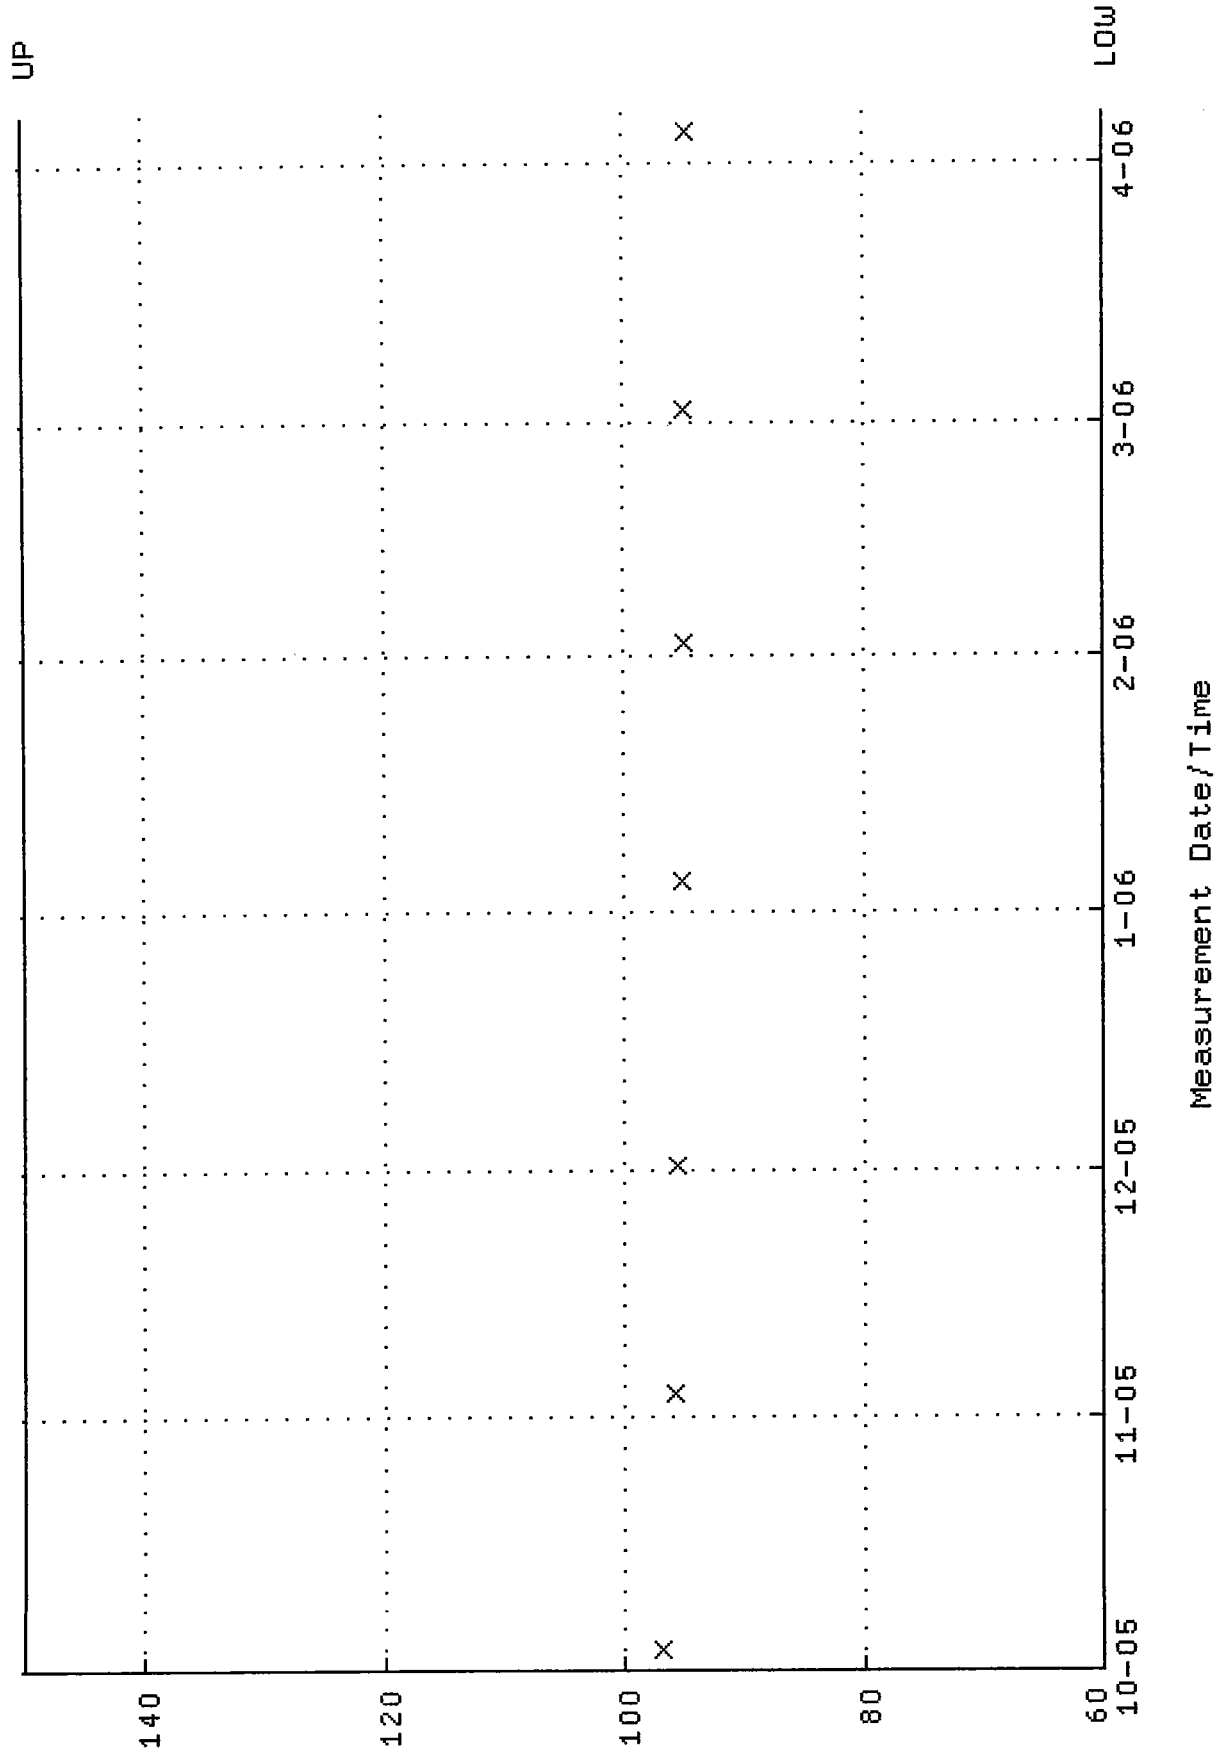


QA filename : DKA100:[ENV_ALPHA.QA.B]B037.QAF;1
 Parameter Name : BACKRATE (Background Rate)
 Start/End Dates : 2-OCT-2005 13:25:43 through 6-APR-2006 12:00:00
 Lower/Upper Lmts: 0.000000E+00 through 2.000000E-02

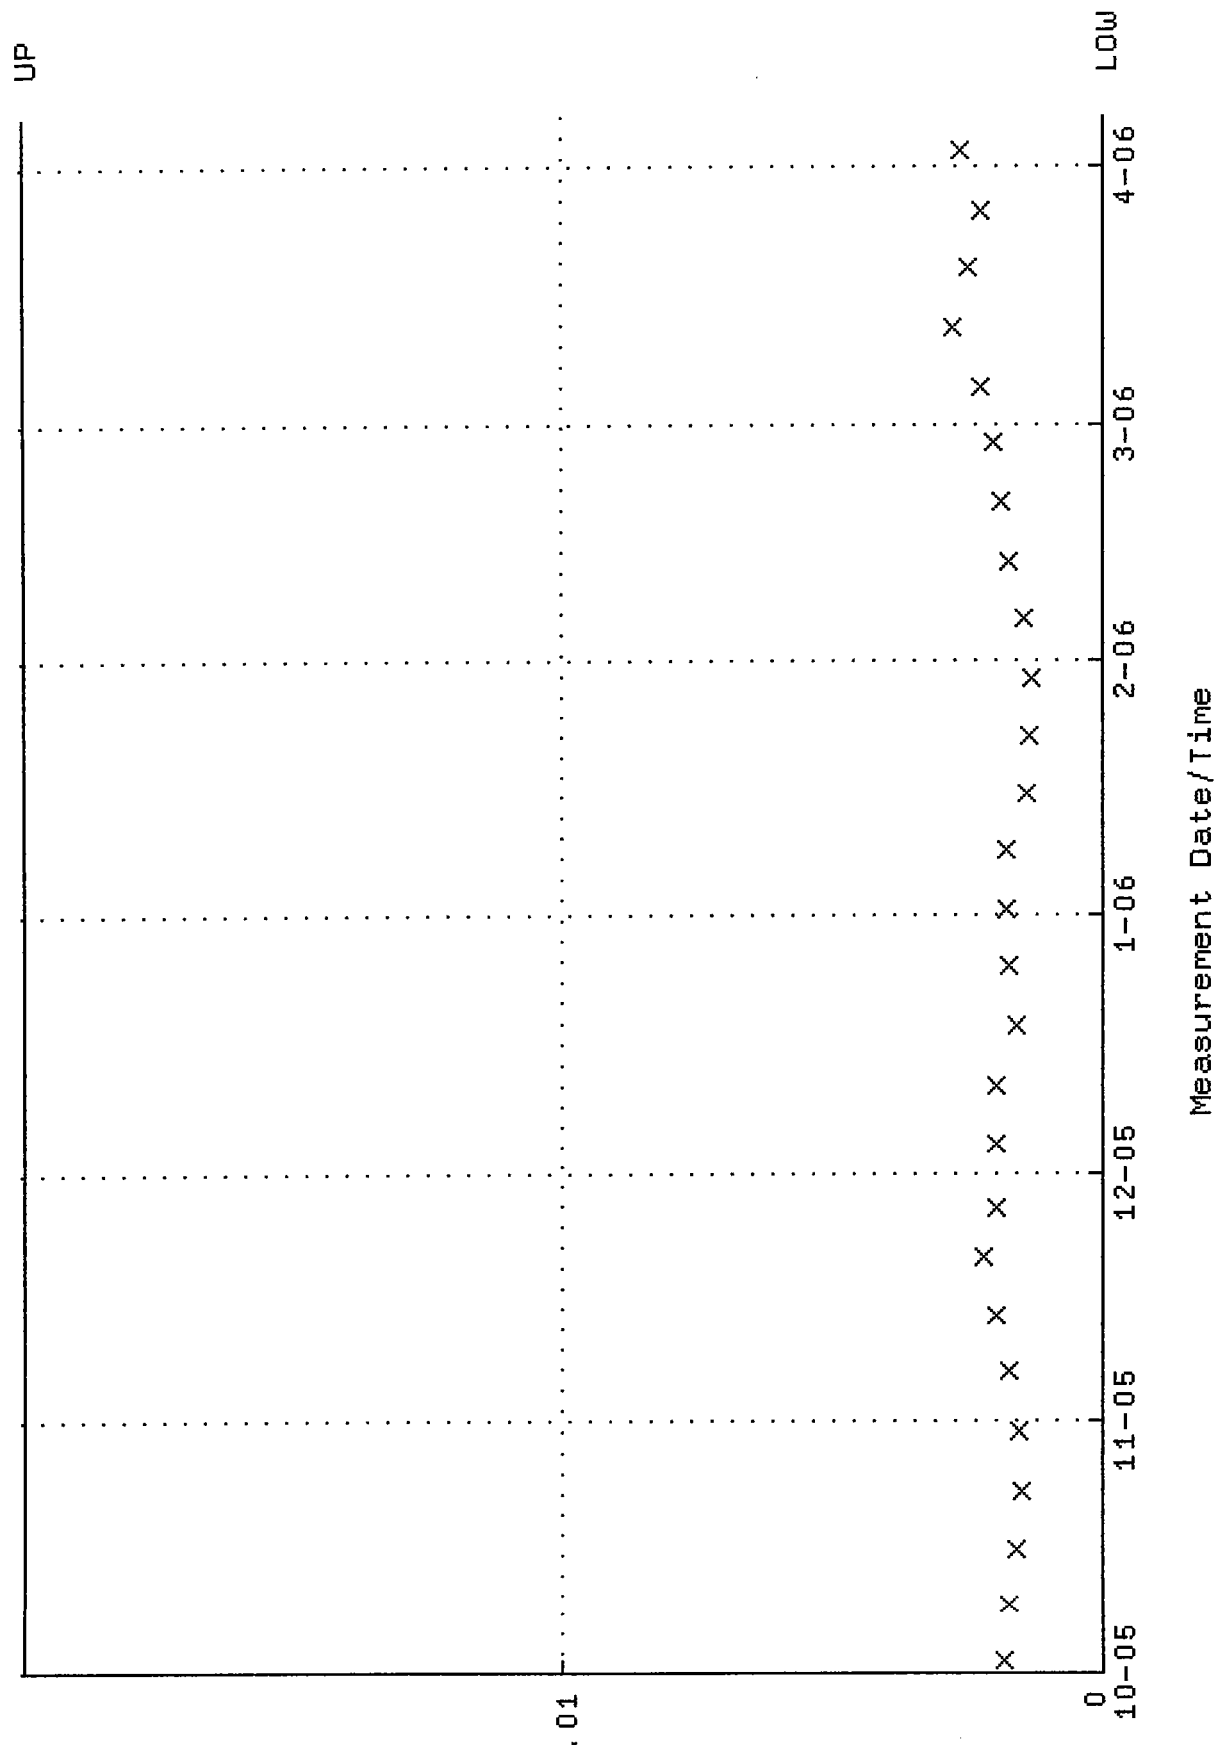


QA filename : DKA100:[ENV_ALPHA.QA.W]W078.QAF;6
 Parameter Name : AVRGEFF (Average Efficiency)
 Start/End Dates : 5-OCT-2005 12:08:53 through 6-APR-2006 12:00:00
 Lower/Upper Lmts: 0.280000 through 0.370000

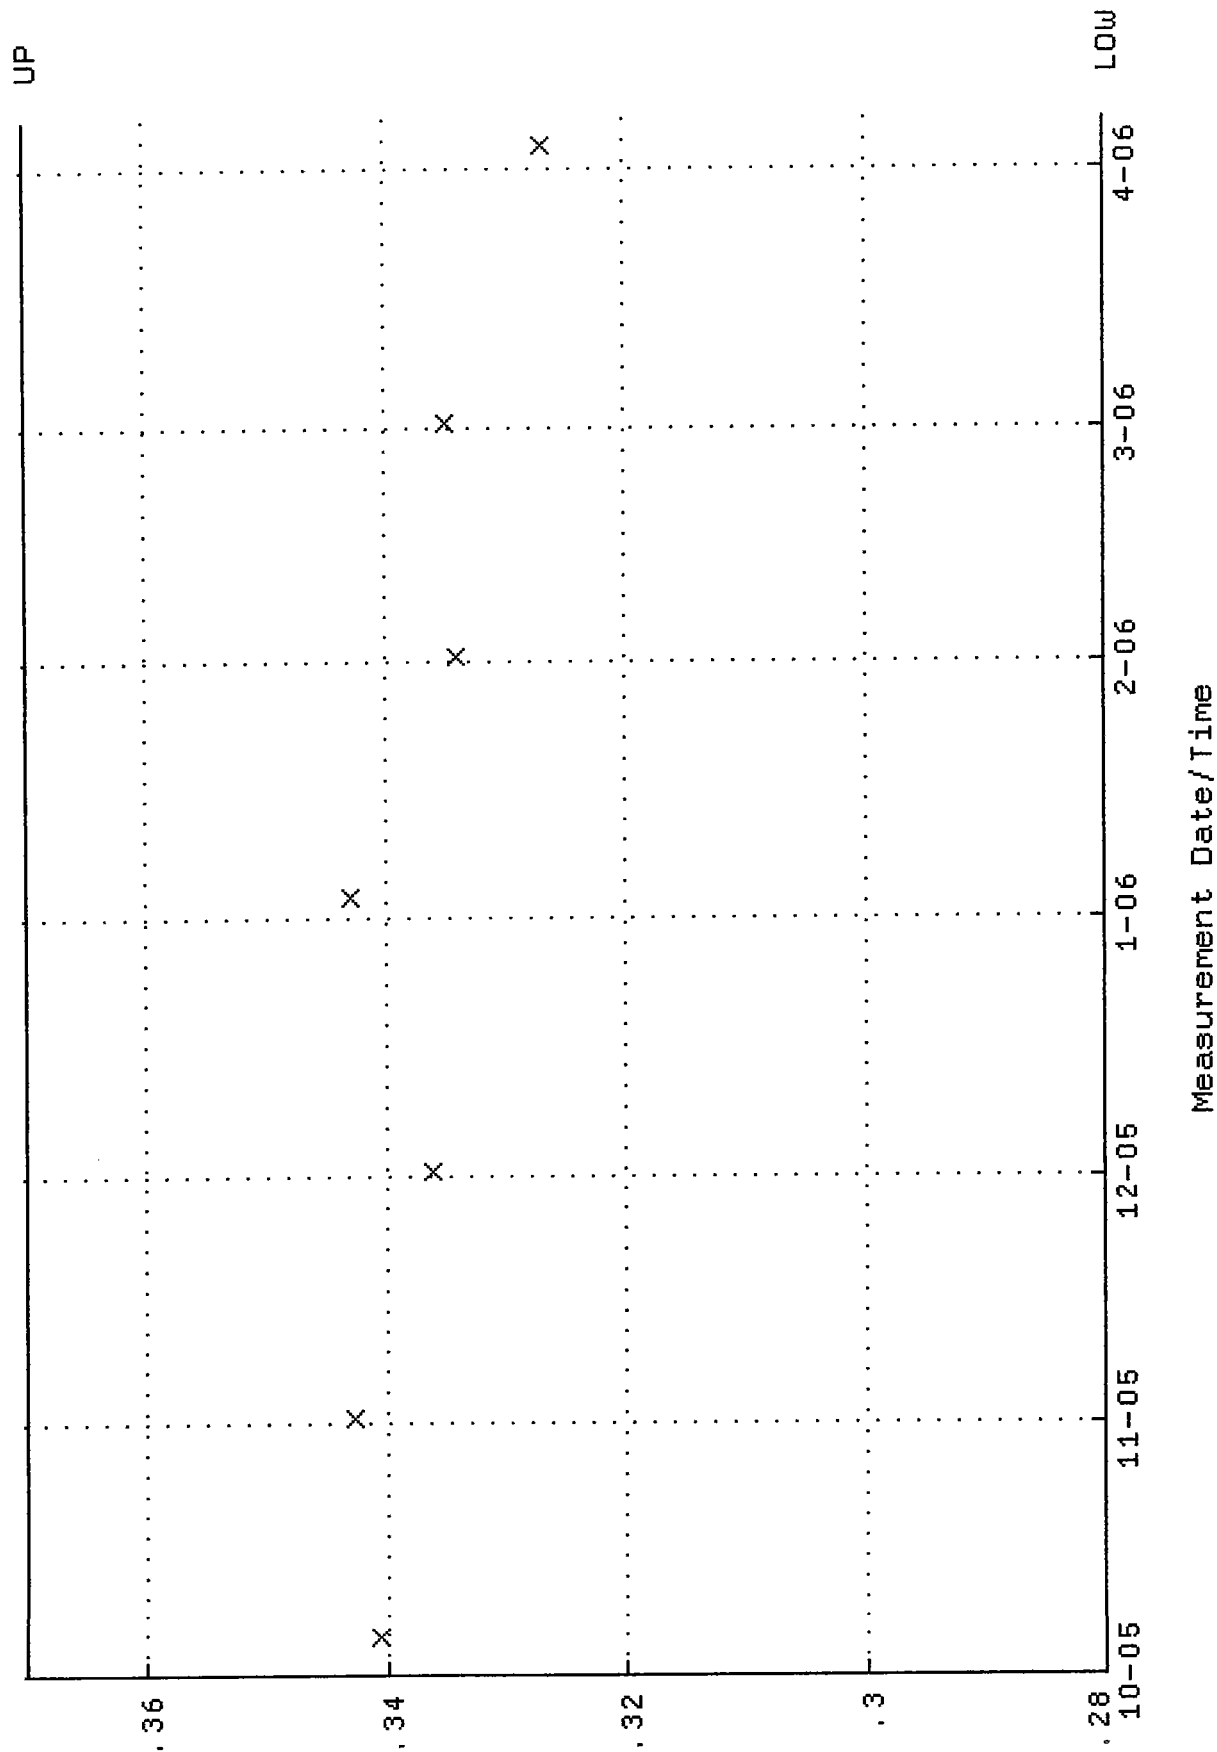


QA filename : DKA100:[ENV_ALPHA.QA.W]W078.QAF;6
 Parameter Name : NLAIVITY-GD148 (NUCLIDE ACTIVITY GD-148)
 Start/End Dates : 5-OCT-2005 12:08:53 through 6-APR-2006 12:00:00
 Lower/Upper Lmts: 60.0000 through 150.0000

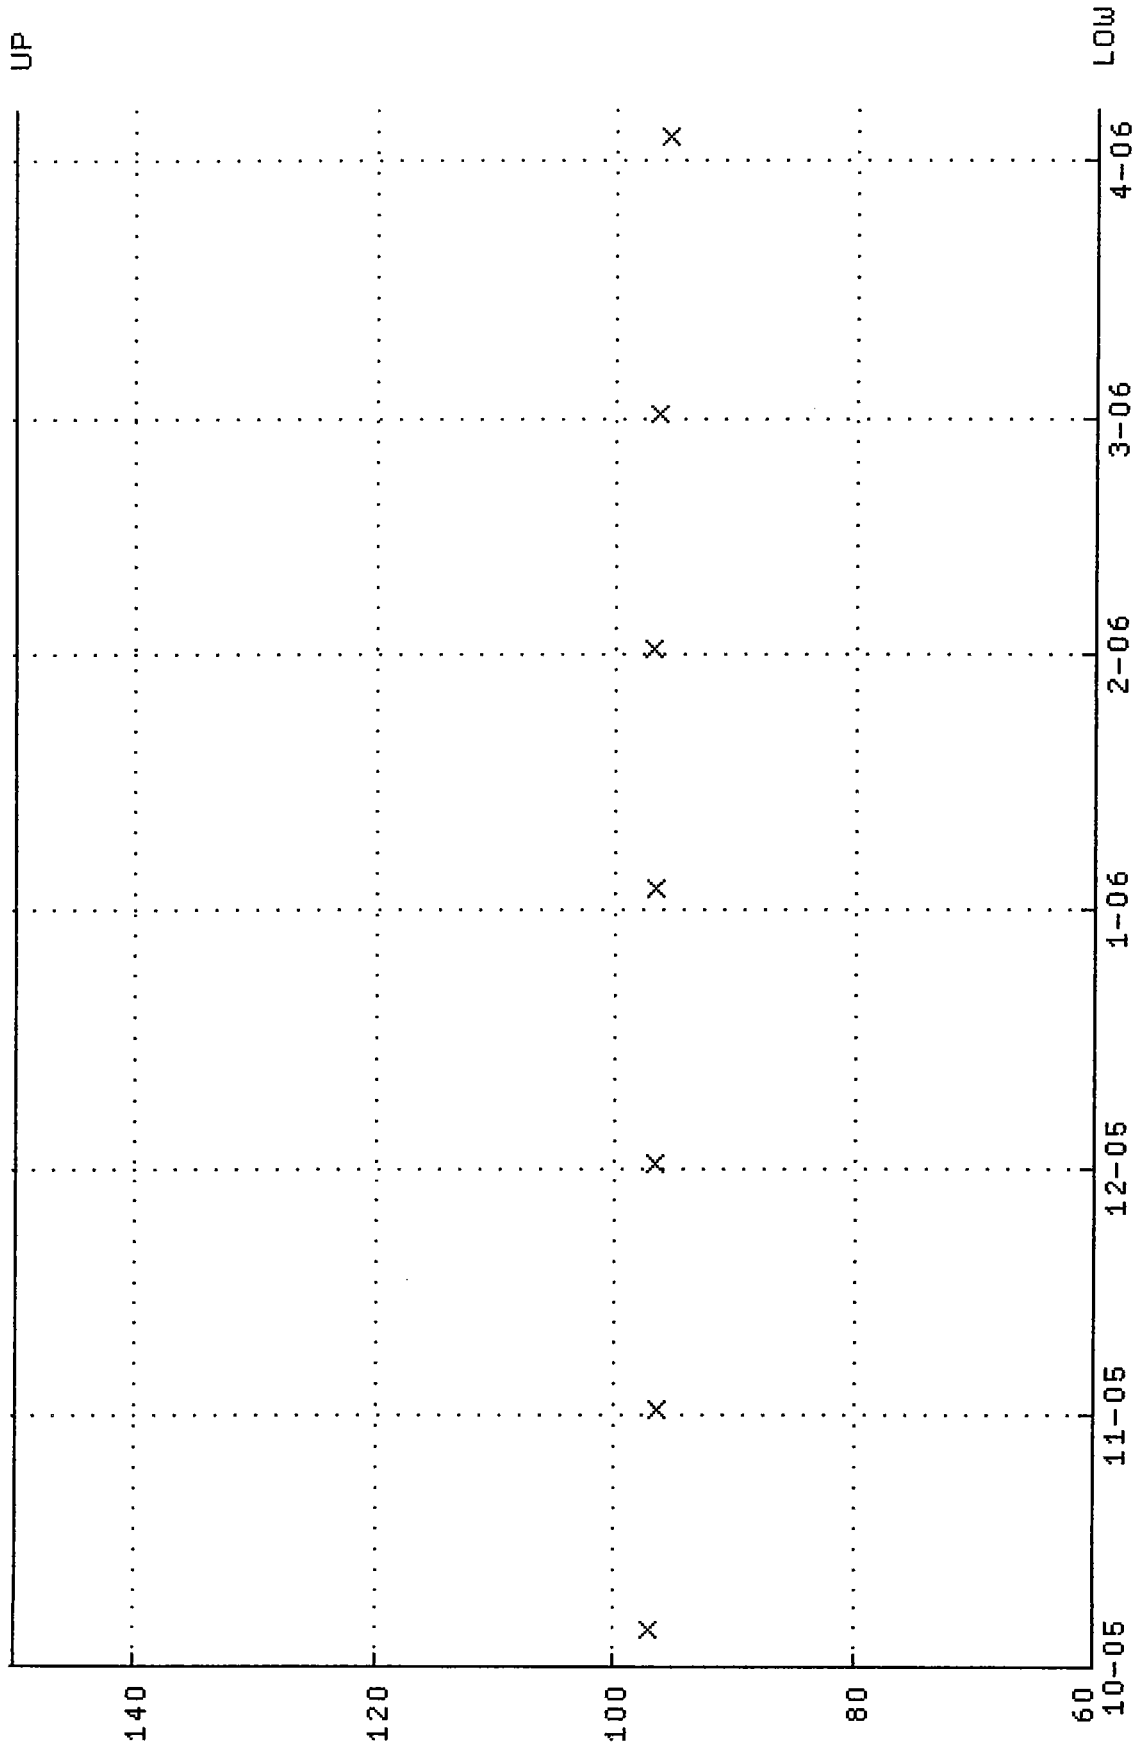


QA filename : DKA100:[ENV_ALPHA.QA.W]W079.QAF;4
 Parameter Name : AVRGEFF (Average Efficiency)
 Start/End Dates : 5-OCT-2005 12:08:53 through 6-APR-2006 12:00:00
 Lower/Upper Lmts: 0.280000 through 0.370000

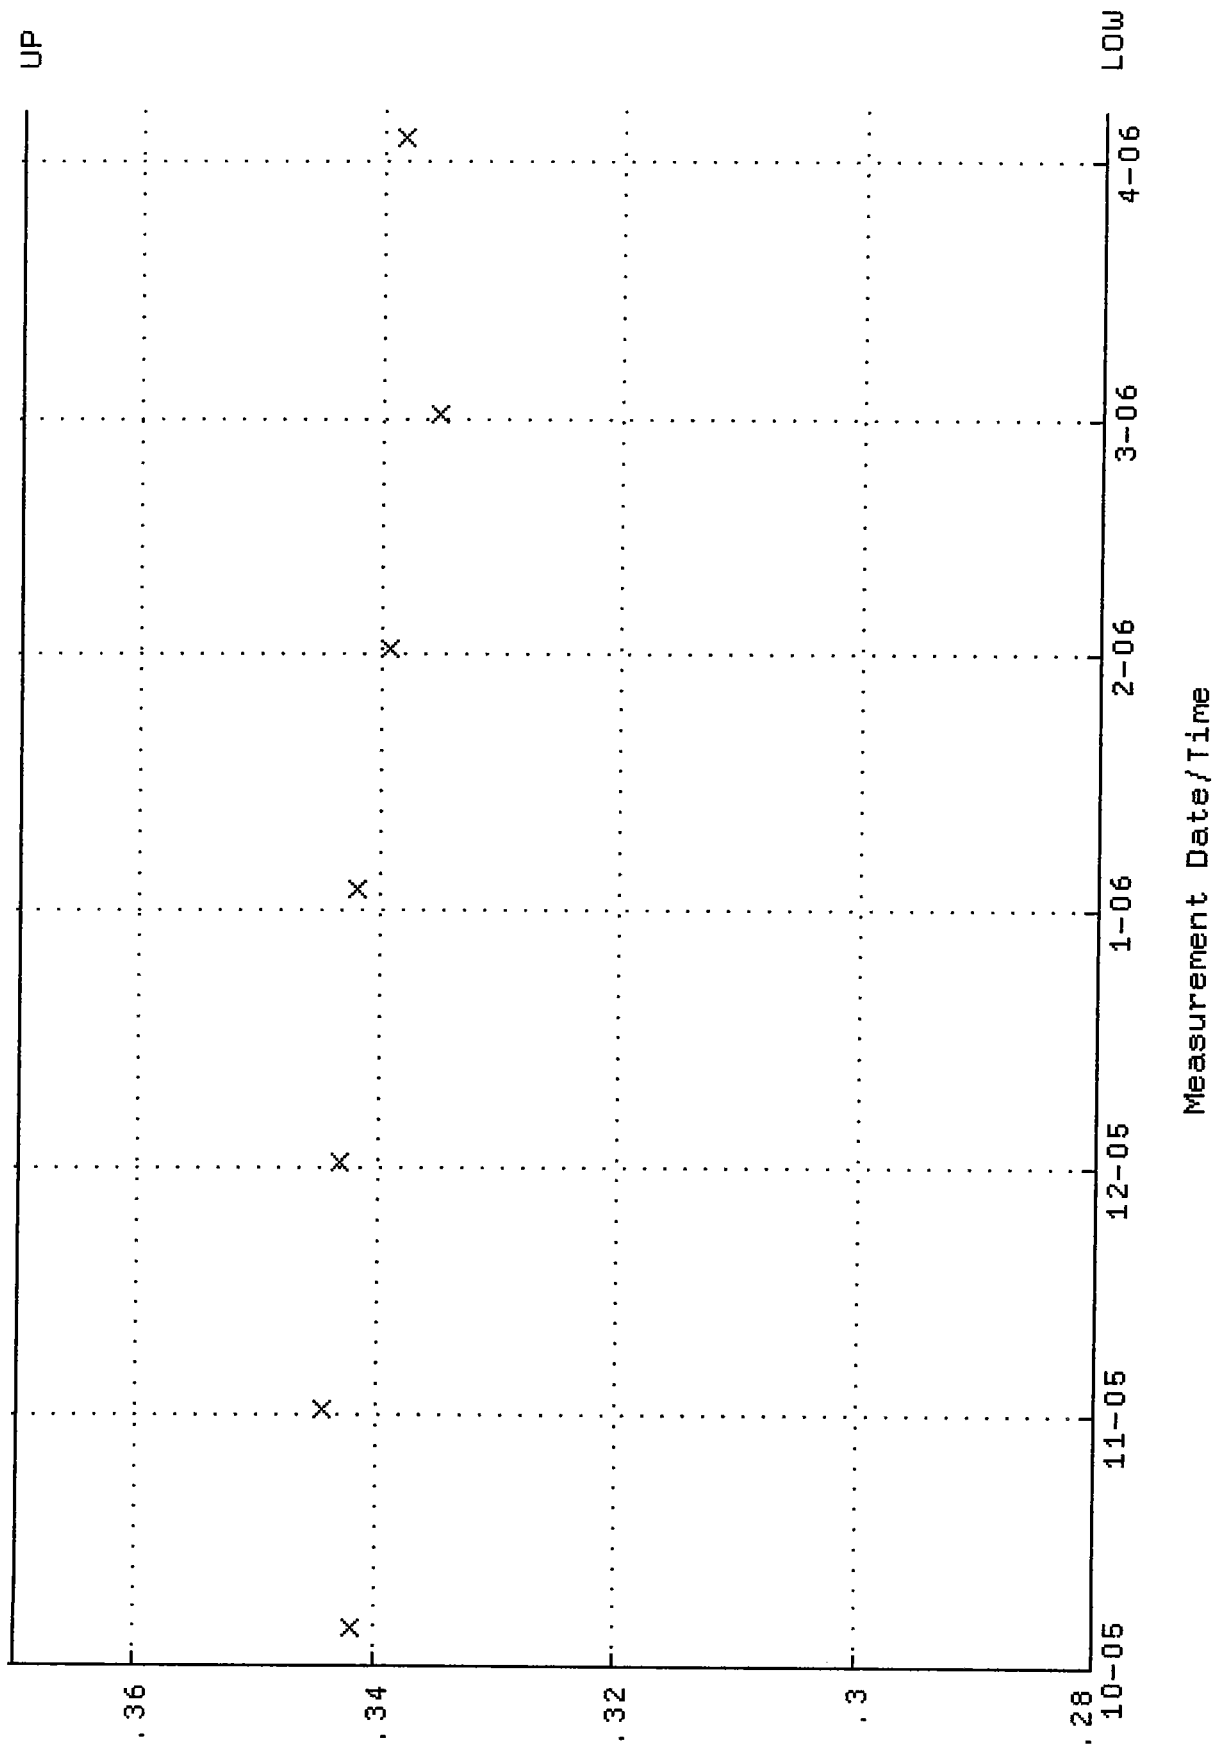


QA filename : DKA100:[ENV_ALPHA.QA.W]W079.QAF;4
 Parameter Name : NACTIVITY-GD148 (NUCLIDE ACTIVITY GD-148)
 Start/End Dates : 5-OCT-2005 12:08:53 through 6-APR-2006 12:00:00
 Lower/Upper Lmts: 60.0000 through 150.0000

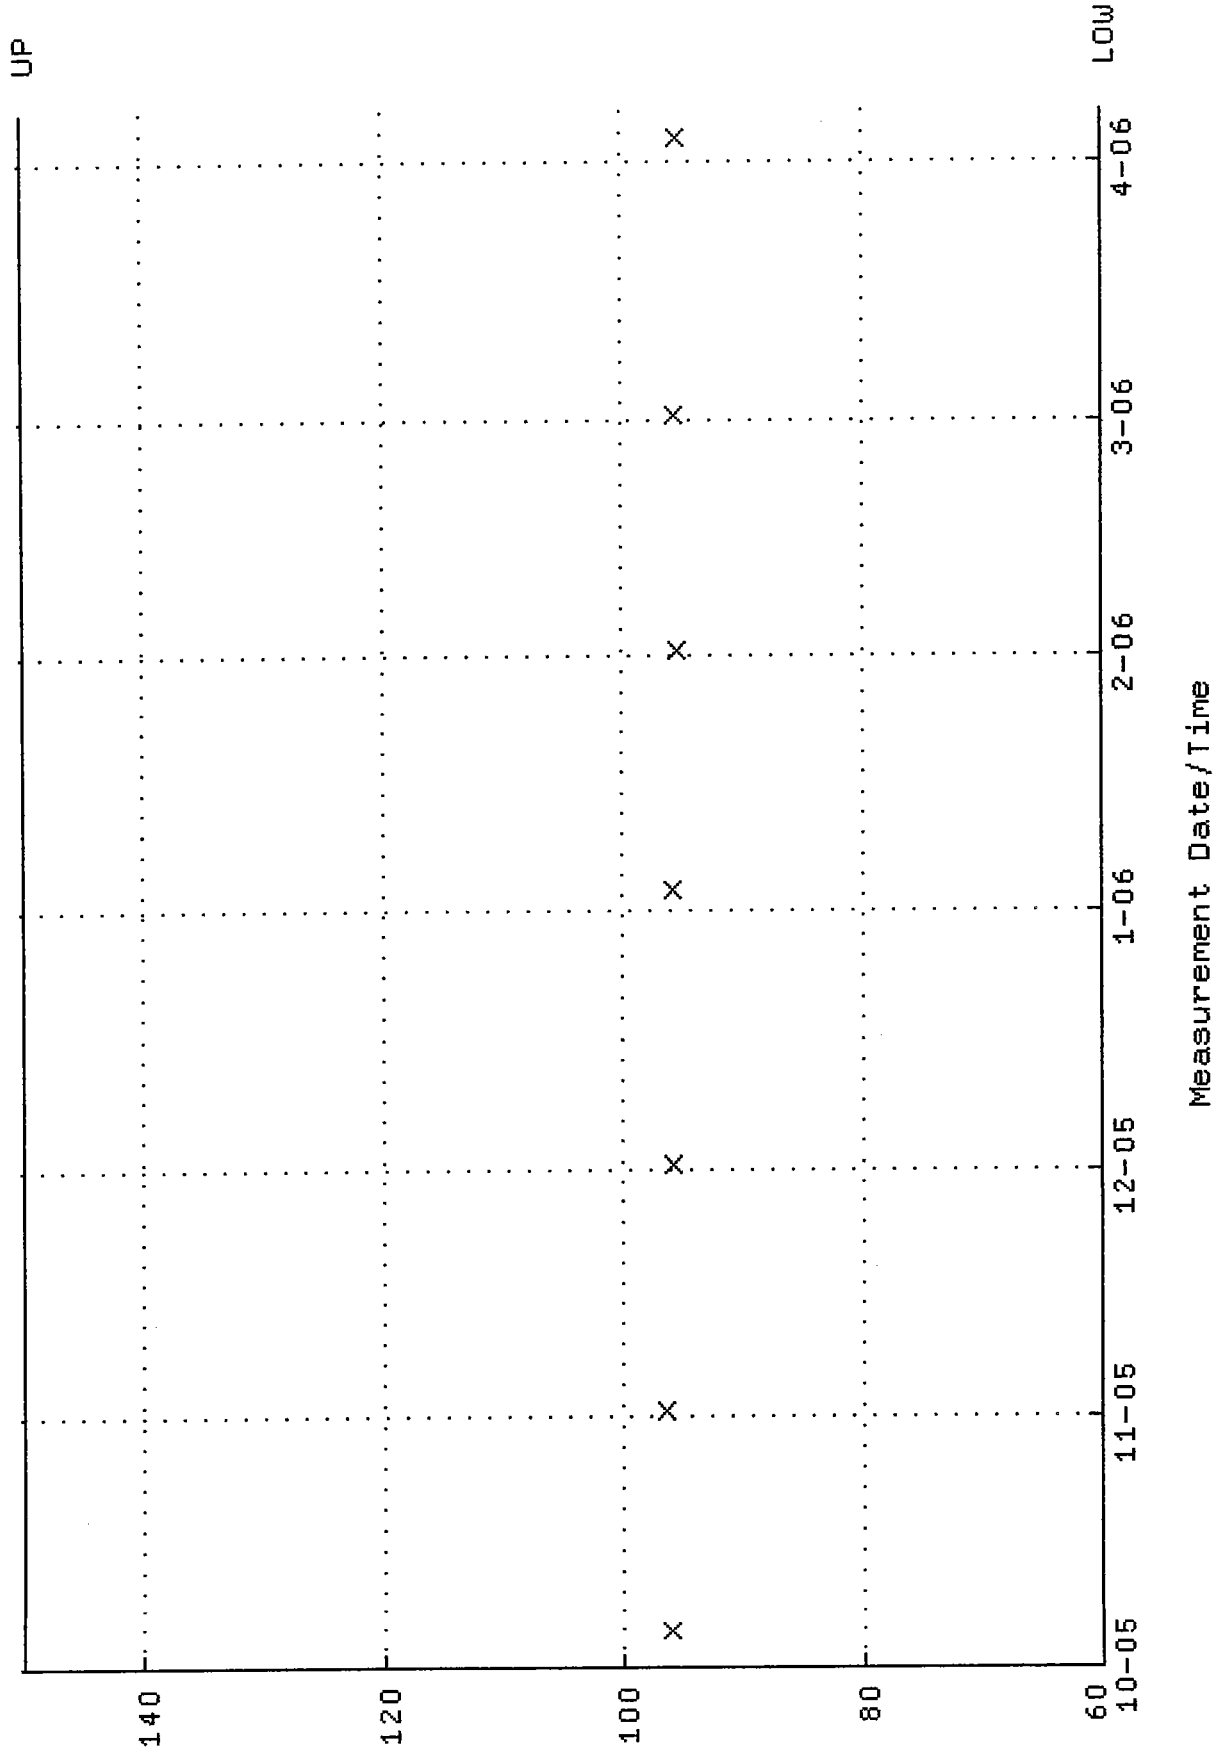


QA filename : DKA100: [ENV_ALPHA.QA.B]B079.QAF; 2
 Parameter Name : BACKRATE (Background Rate)
 Start/End Dates : 2-OCT-2005 13:57:18 through 6-APR-2006 12:00:00
 Lower/Upper Lmts: 0.000000E+00 through 2.000000E-02

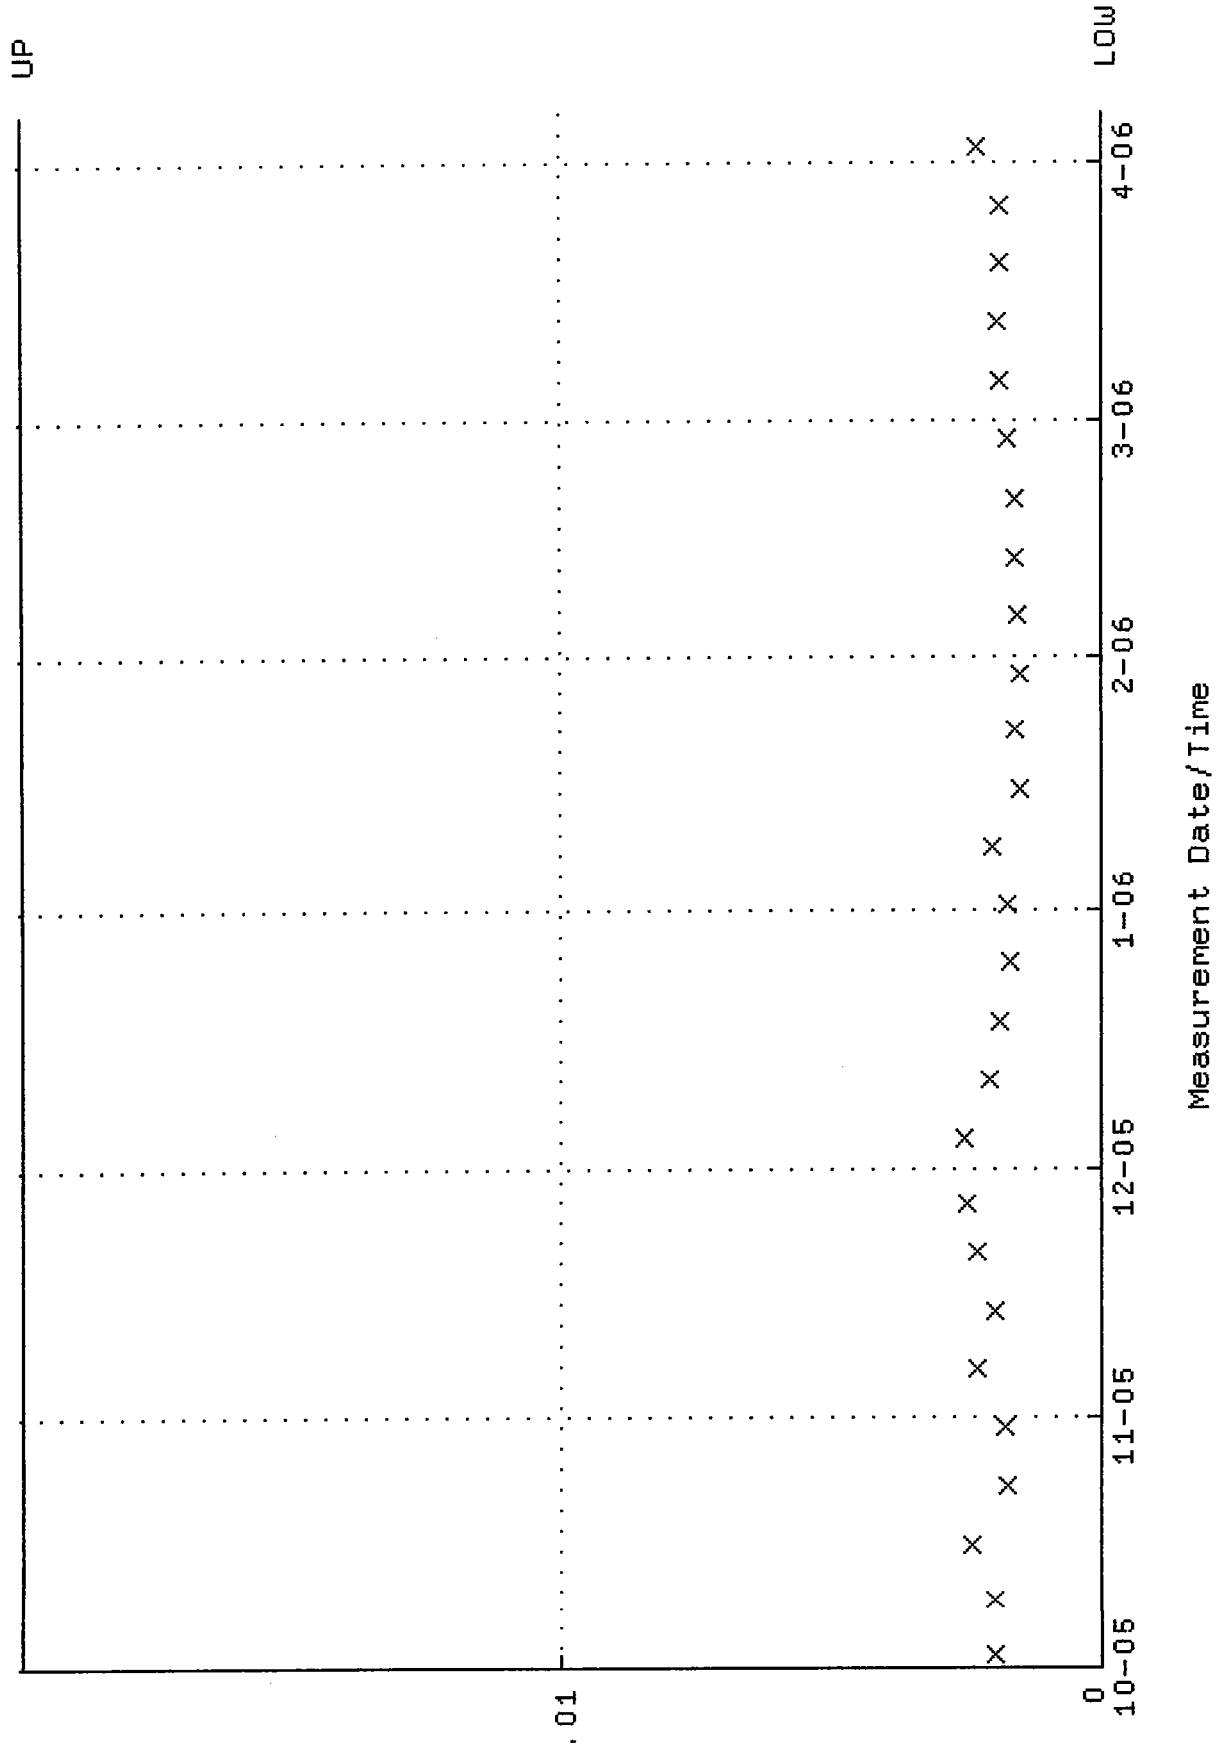


QA filename : DKA100:[ENV_ALPHA.QA.W]W080.QAF;4
 Parameter Name : AVRGEFF (Average Efficiency)
 Start/End Dates : 5-OCT-2005 12:08:53 through 6-APR-2006 12:00:00
 Lower/Upper Lmts: 0.280000 through 0.370000

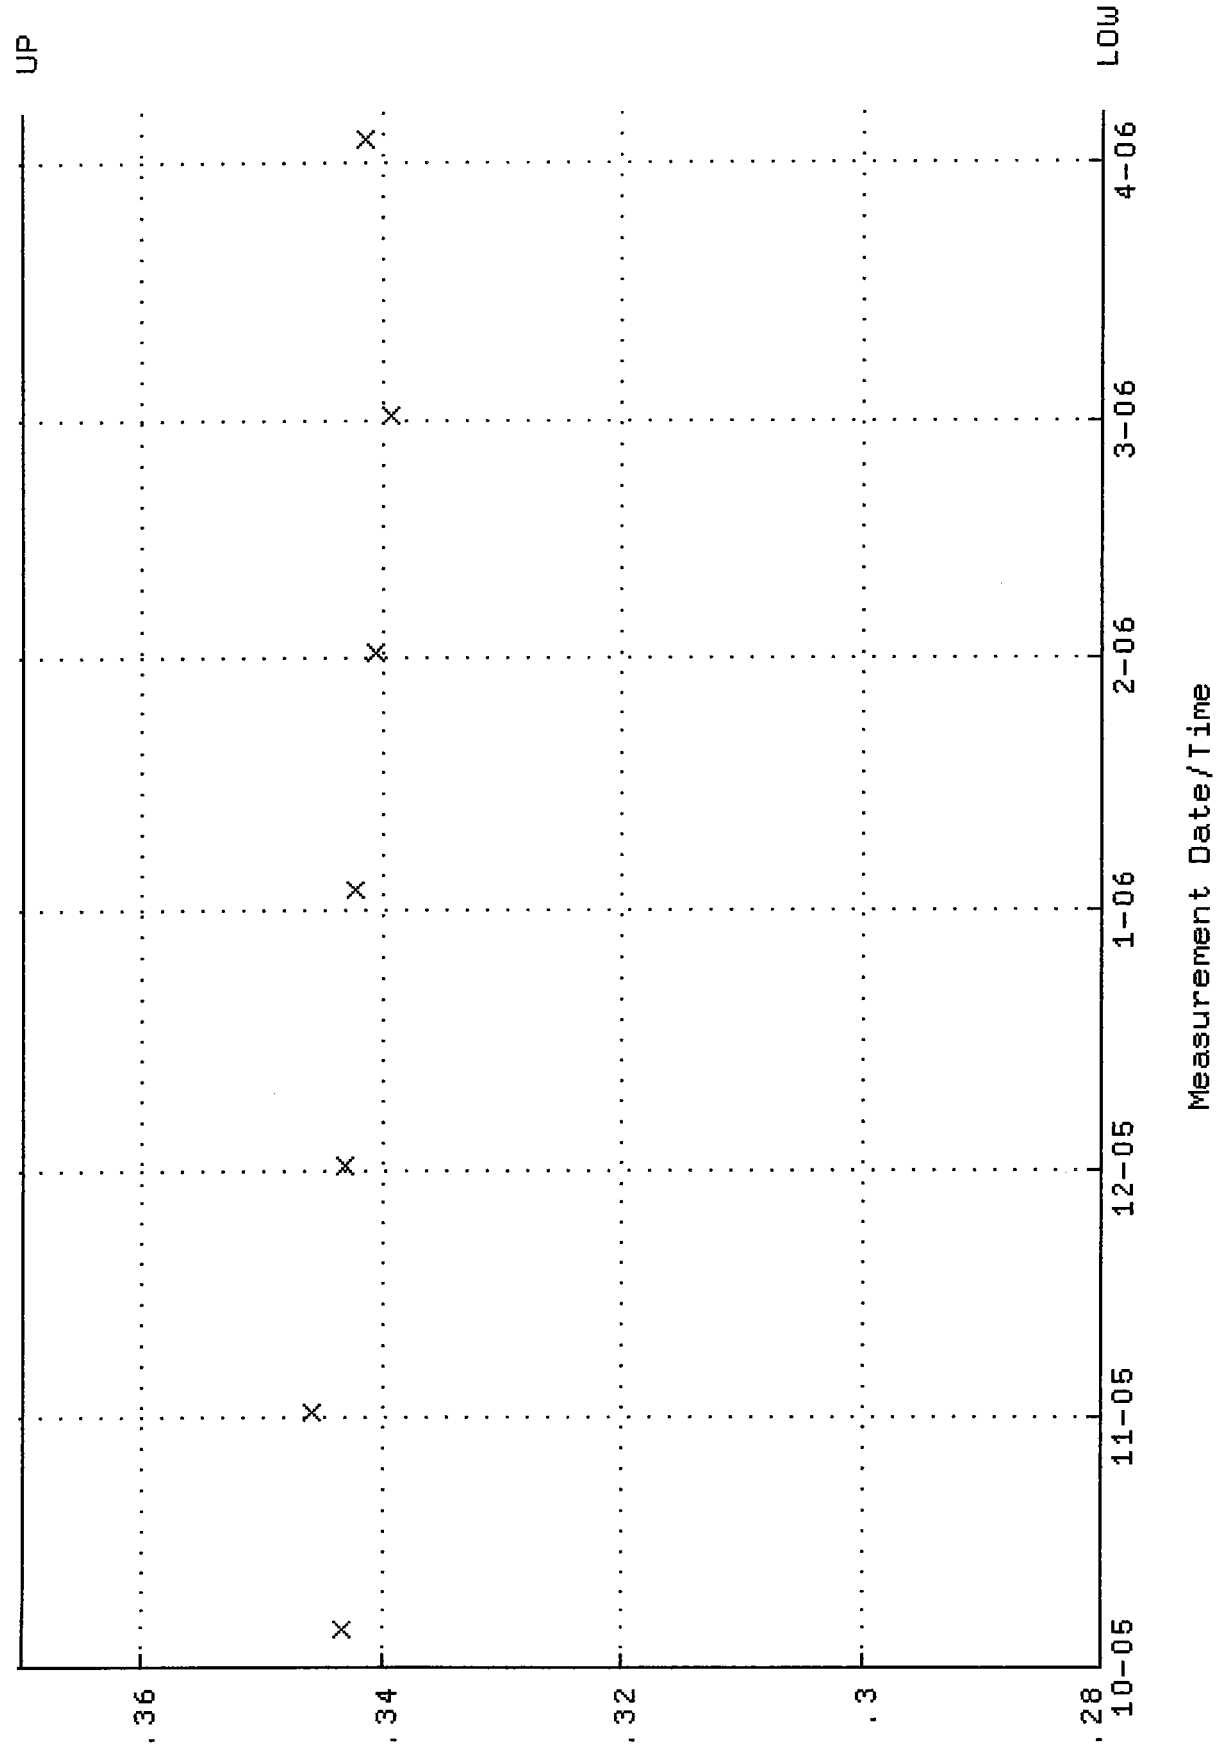


QA filename : DKA100:[ENV_ALPHA.QA.W]W080.QAF;4
 Parameter Name : NLAIVITY-GD148 (NUCLIDE ACTIVITY GD-148)
 Start/End Dates : 5-OCT-2005 12:08:53 through 6-APR-2006 12:00:00
 Lower/Upper Lmts: 60.0000 through 150.0000

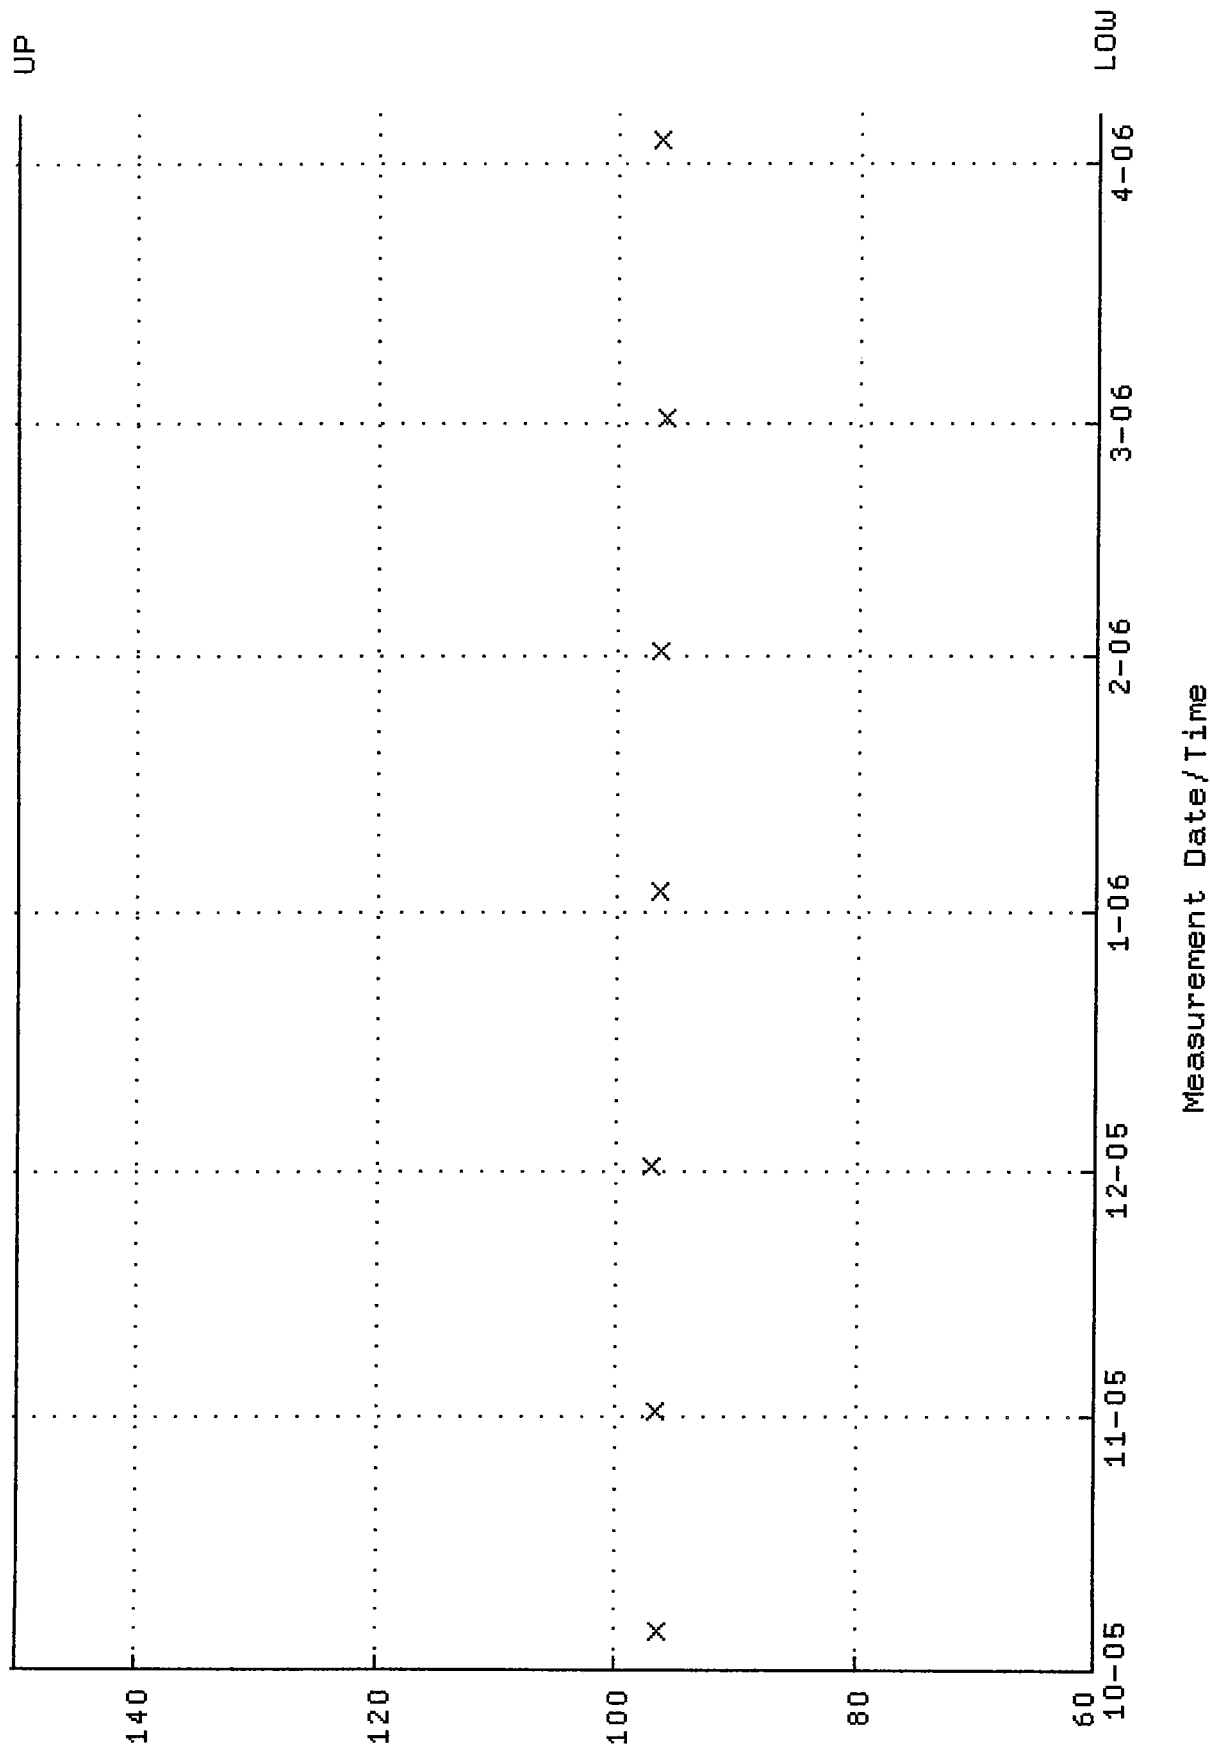


QA filename : DKA100:[ENV_ALPHA.QA.B]B080.QAF;2
Parameter Name : BACKRATE (Background Rate)
Start/End Dates : 2-OCT-2005 13:57:18 through 6-APR-2006 12:00:00
Lower/Upper Lmts: 0.000000E+00 through 2.000000E-02

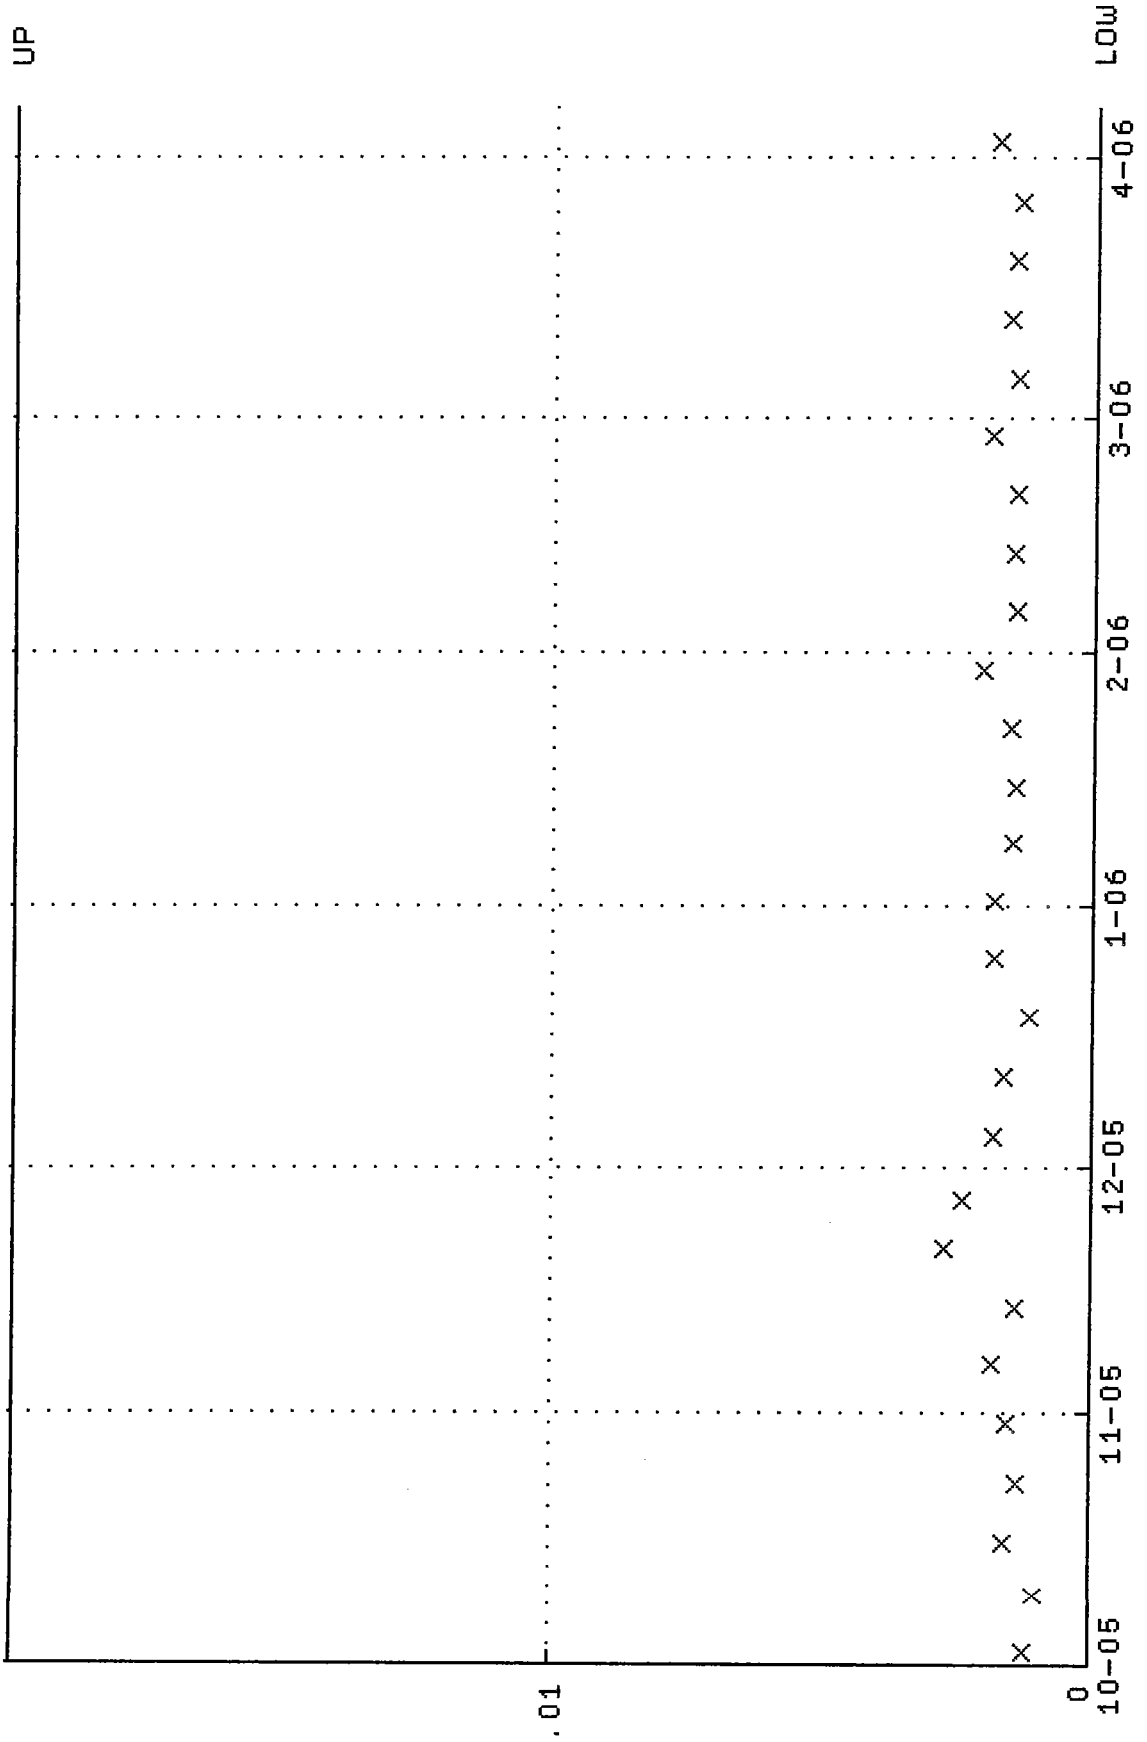


QA filename : DKA100:[ENV_ALPHA.QA.W]W081.QAF;5
 Parameter Name : AVRGEFF (Average Efficiency)
 Start/End Dates : 5-OCT-2005 12:08:53 through 6-APR-2006 12:00:00
 Lower/Upper Lmts: 0.257434 through 0.316366

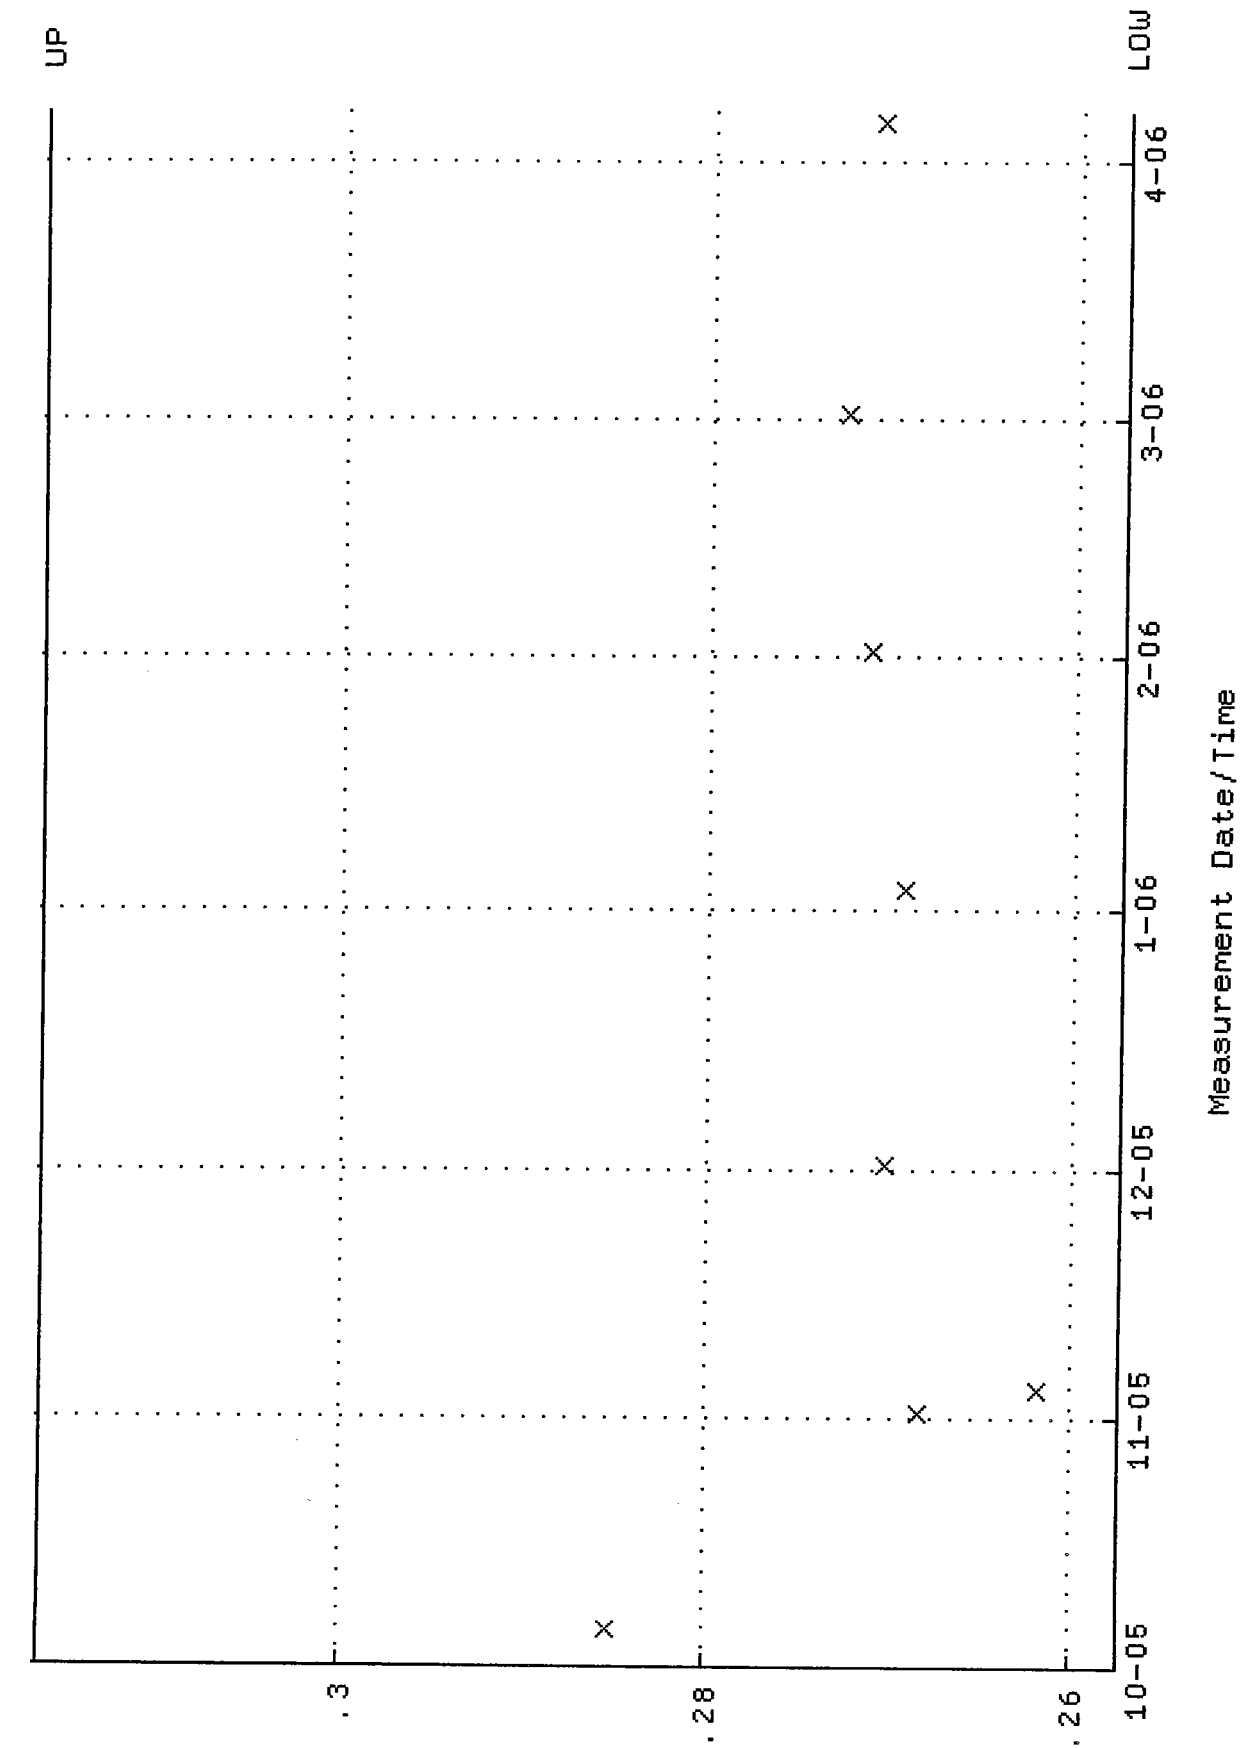


QA filename : DKA100:[ENV-ALPHA.QA.W]W081.QAF; 5
 Parameter Name : NLAIVITY-GD148 (NUCLIDE ACTIVITY GD-148)
 Start/End Dates : 5-OCT-2005 12:08:53 through 6-APR-2006 12:00:00
 Lower/Upper Lmts: 60.0000 through 150.000

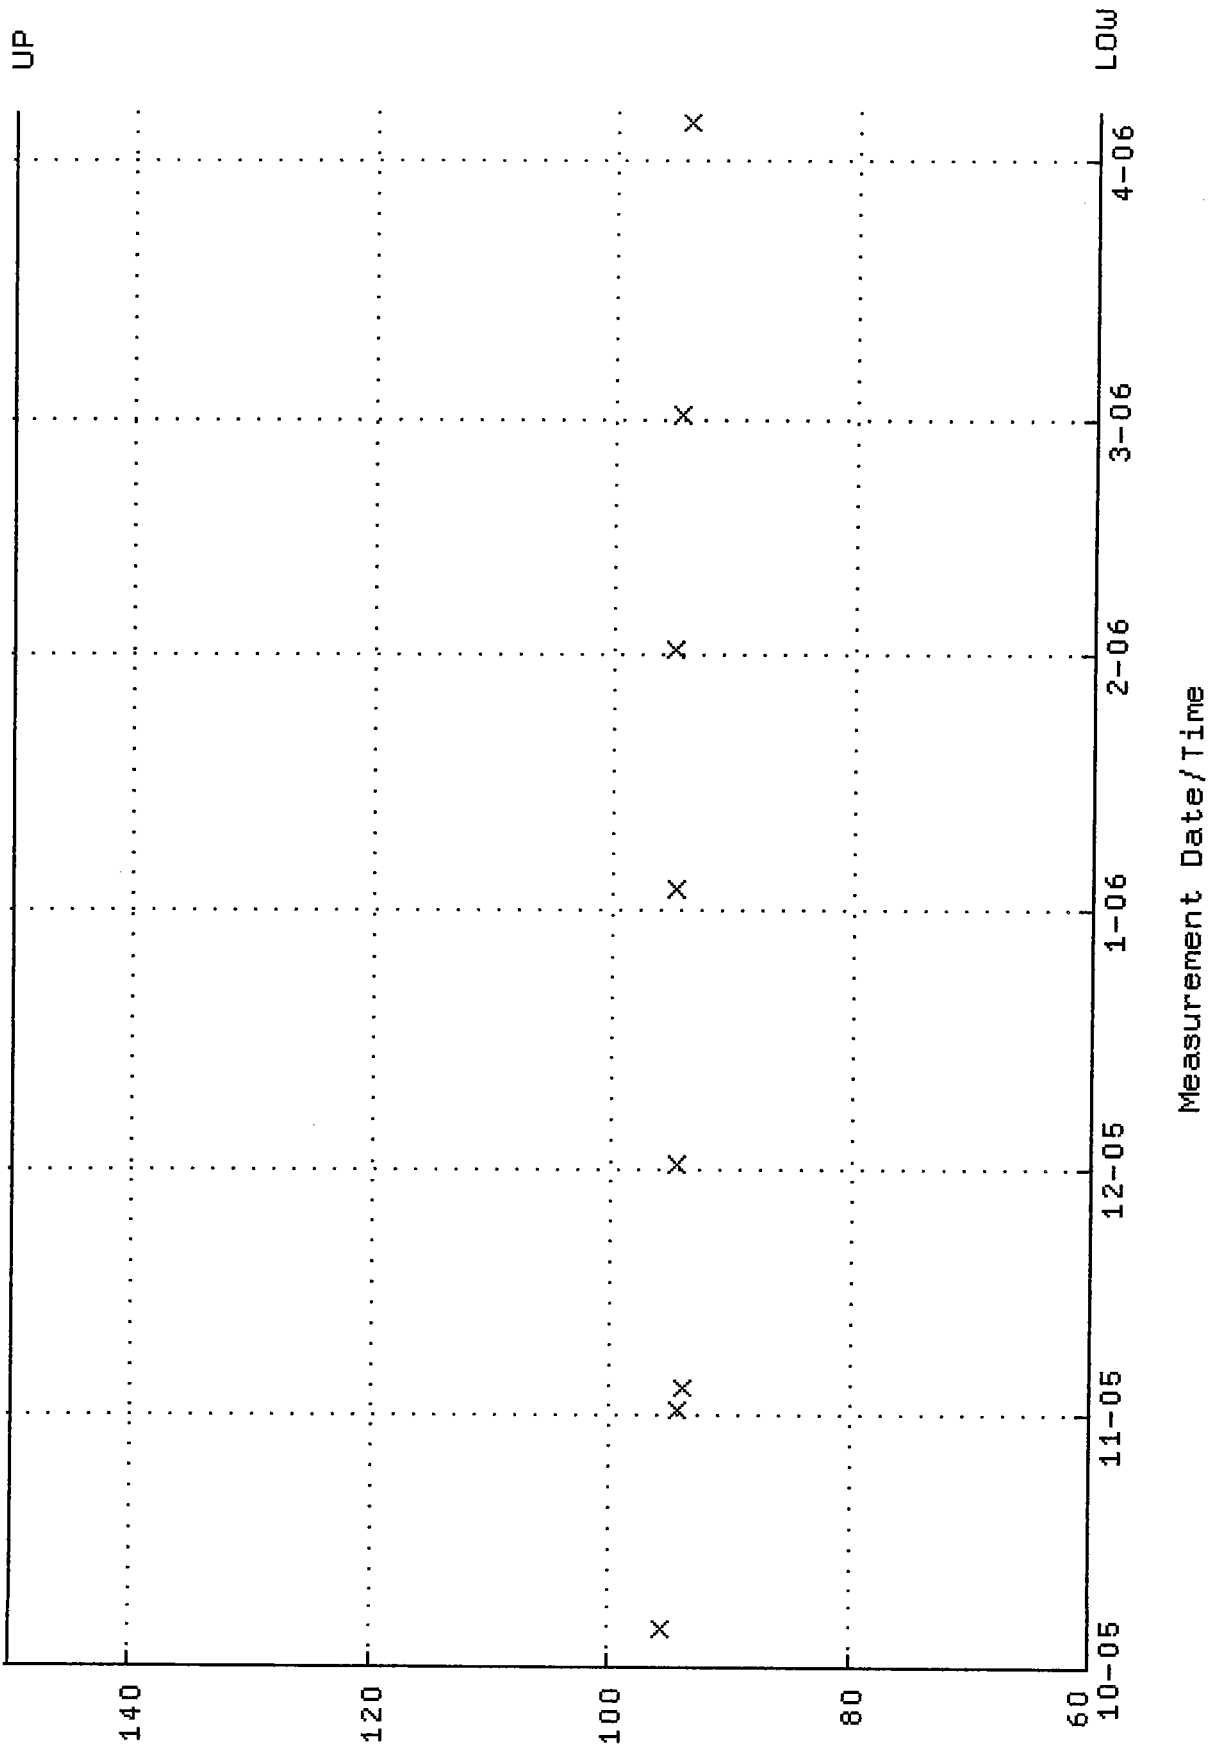


QA filename : DKA100:[ENV_ALPHA.QA.B]B081.QAF;2
 Parameter Name : BACKRATE (Background Rate)
 Start/End Dates : 2-OCT-2005 13:57:18 through 6-APR-2006 12:00:00
 Lower/Upper Lmts: 0.000000E+00 through 2.000000E-02

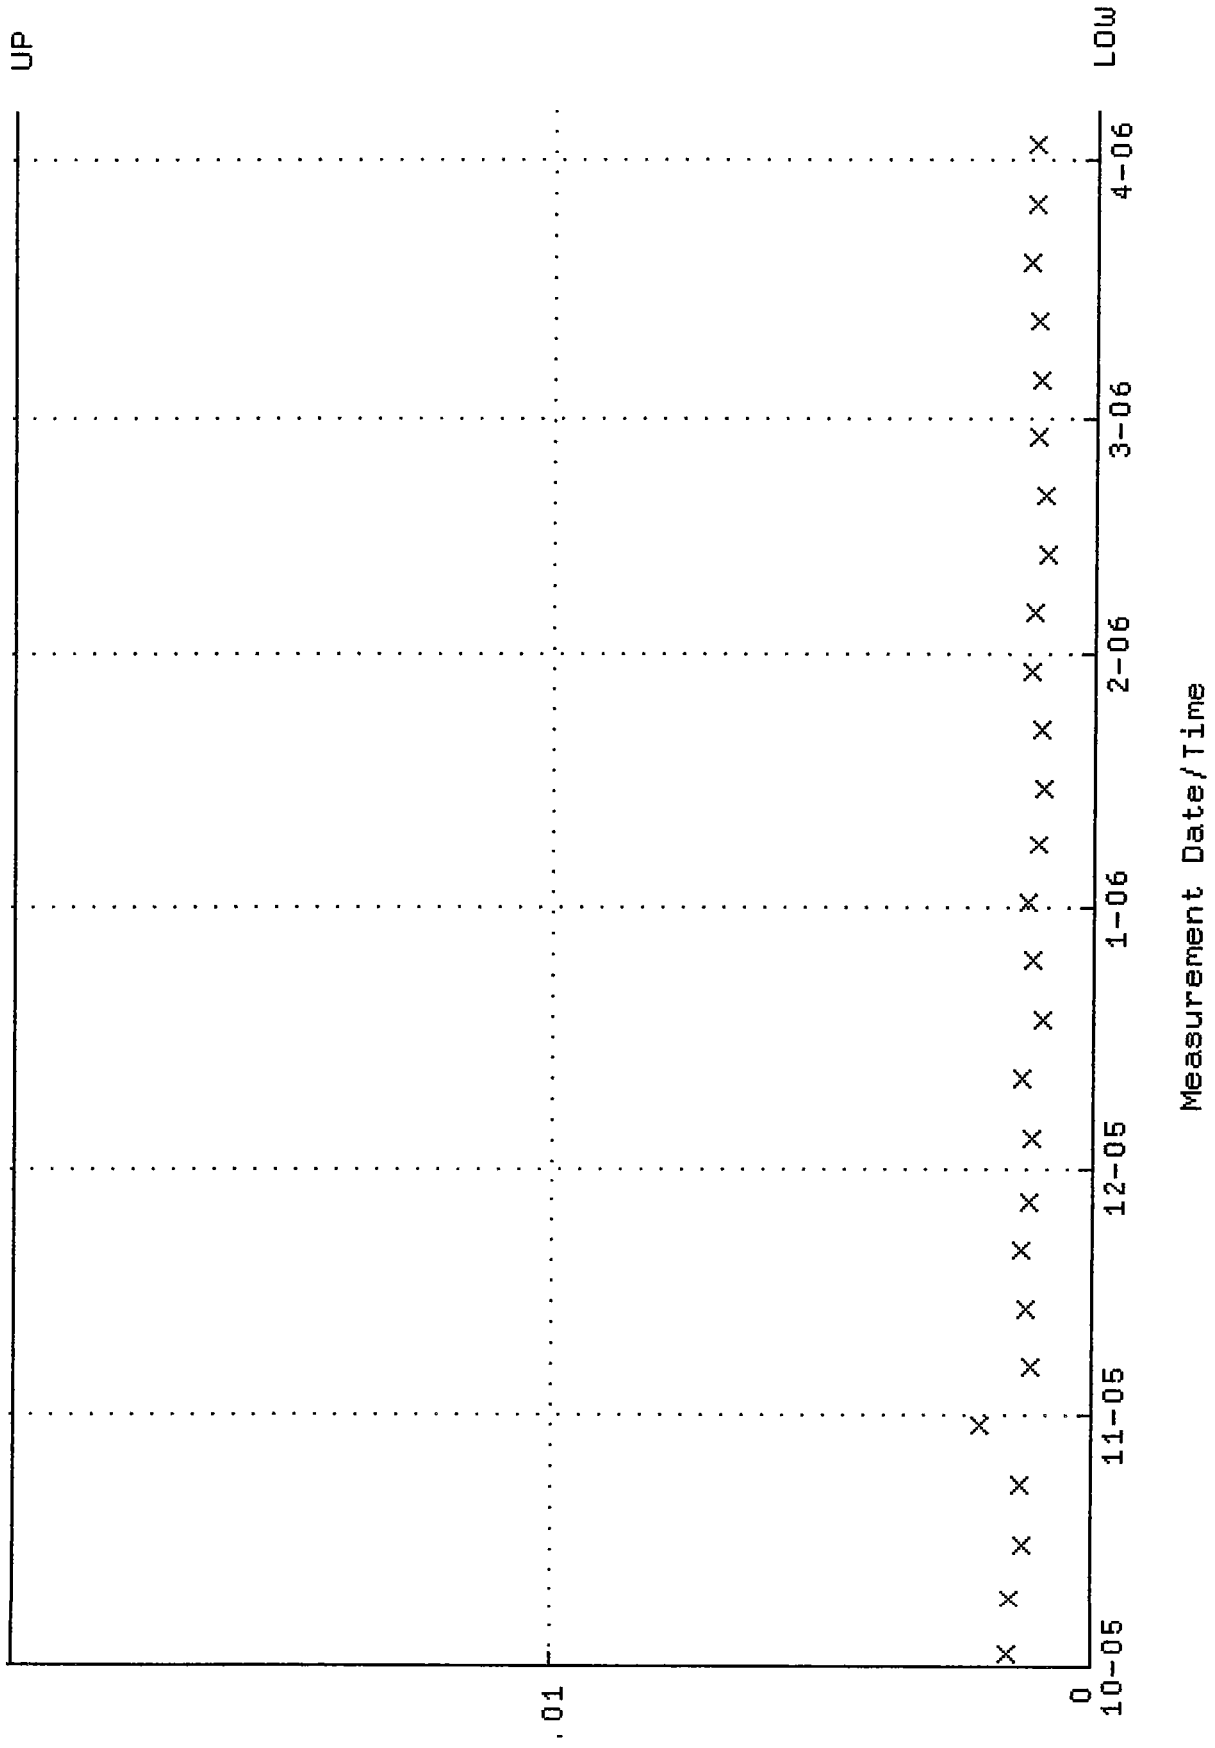


QA filename : DKA100:[ENV_ALPHA]QC_GAMMA13.QAF;3
Parameter Name : PSFWHM-661 (PEAK FWHM (keV) CS-137)
Start/End Dates : 2-OCT-2005 14:56:36 through 31-MAR-2006 12:00:00
Lower/Upper Lmts: 0.100000 through 3.000000

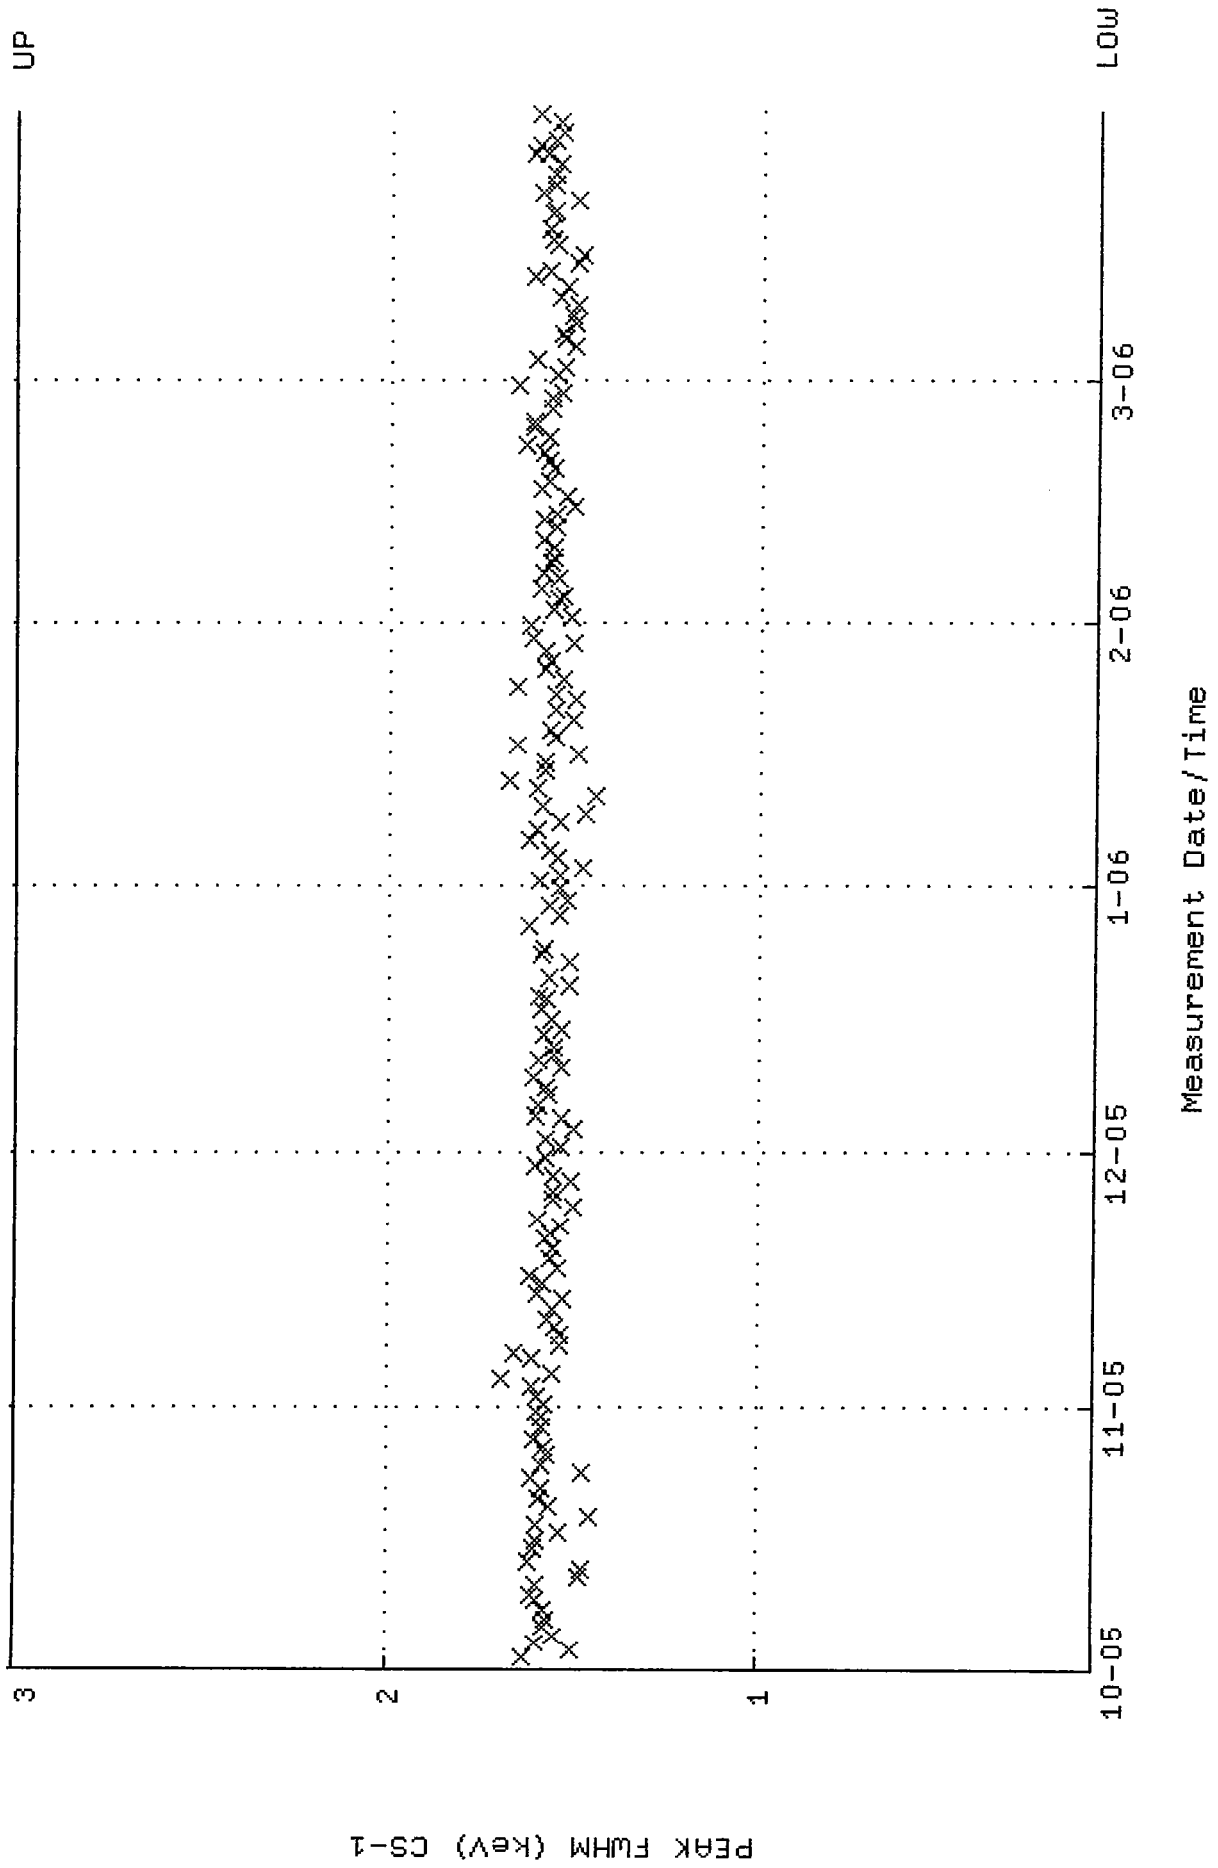

QA filename : DKA100:[ENV_ALPHA]QC_BKG_GAMMA13.QAF;2
Parameter Name : BACKRATE (BACKGROUND (CPS))
Start/End Dates : 1-OCT-2005 21:09:20 through 31-MAR-2006 12:00:00
Lower/Upper Lmts: 3.08008 through 3.53992

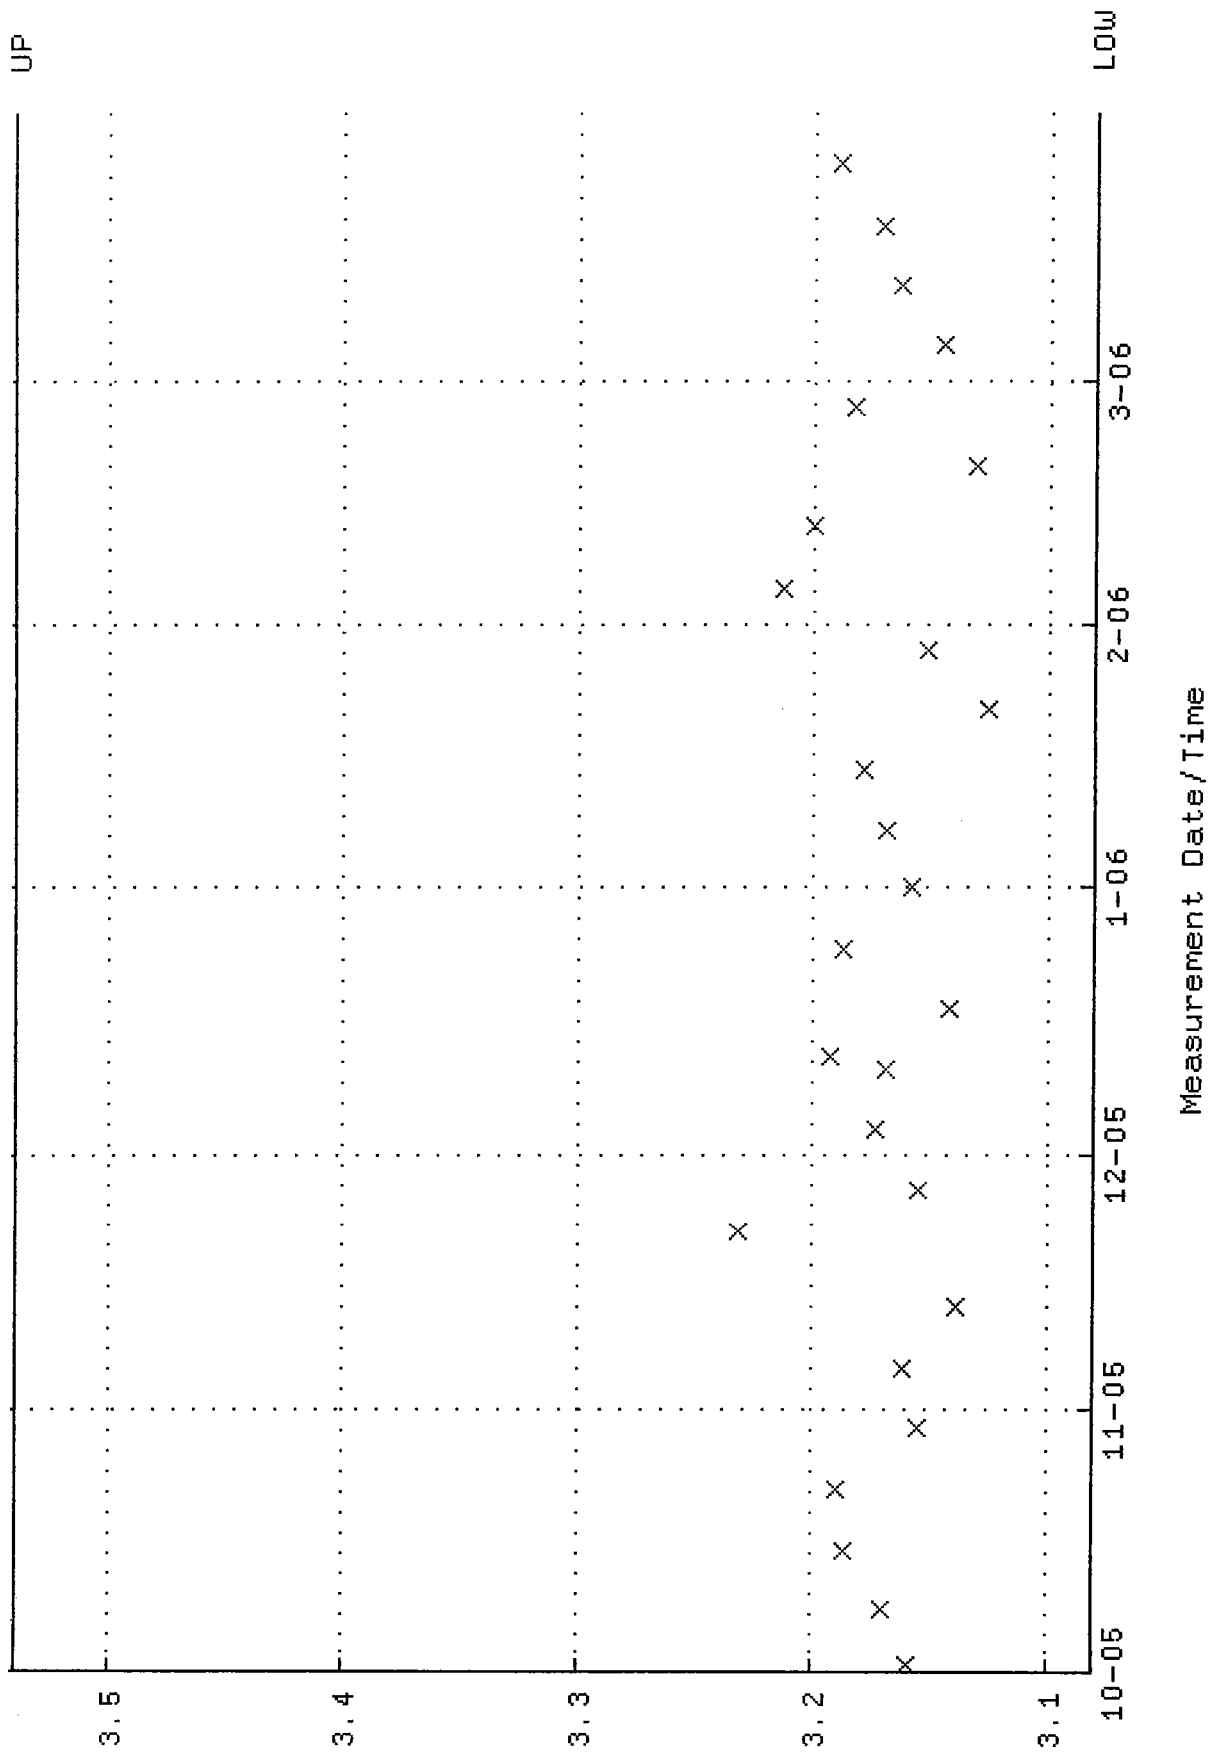


QA filename : DKA100:[ENV_ALPHA]QC_GAMMA16.QAF;2
 Parameter Name : PSFWHM-661 (PEAK FWHM (keV) CS-137)
 Start/End Dates : 1-OCT-2005 12:08:06 through 31-MAR-2006 12:00:00
 Lower/Upper Lmts: 0.100000 through 3.000000

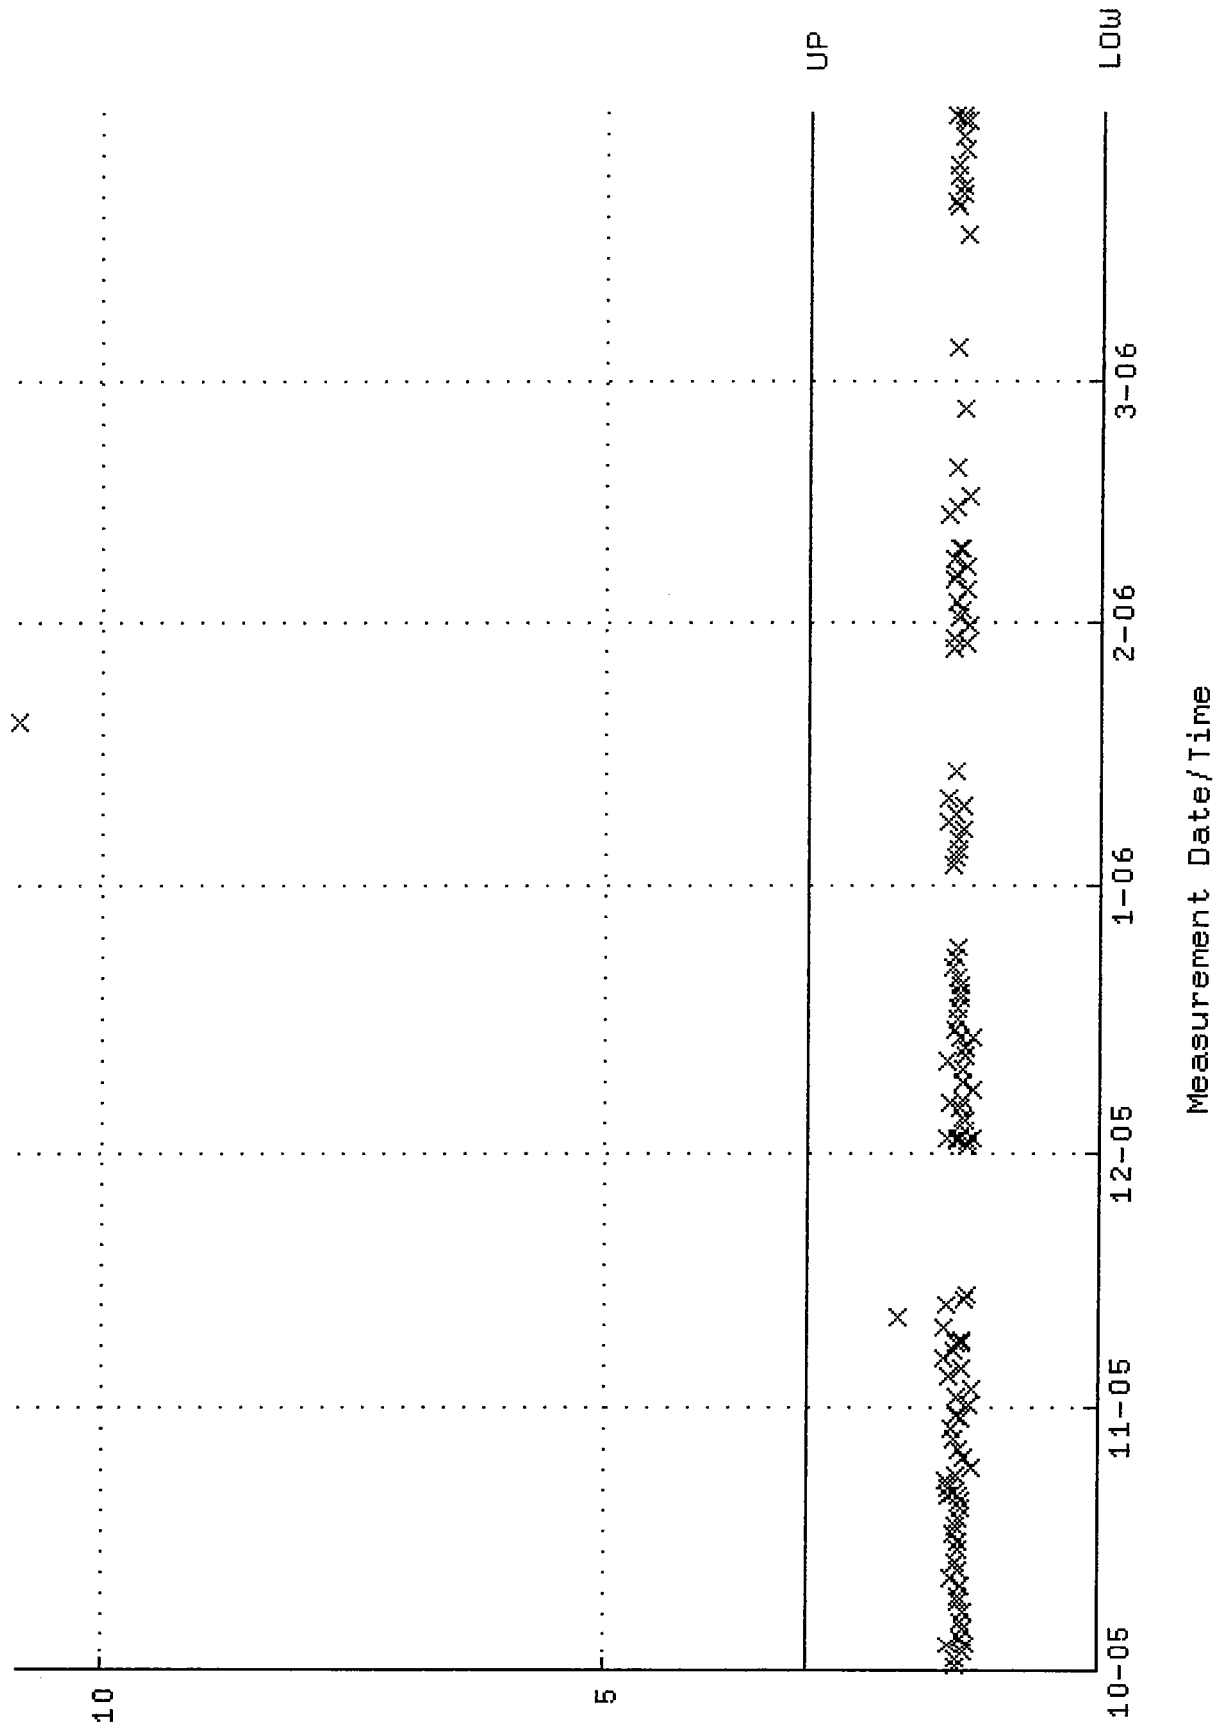


PEAK FWHM (keV) CS-1


QA filename : DKA100:[ENV_ALPHA]QC-BKG-GAMMA16.QAF;1
 Parameter Name : BACKRATE (BACKGROUND (CPS))
 Start/End Dates : 1-OCT-2005 21:09:34 through 31-MAR-2006 12:00:00
 Lower/Upper Lmts: 1.25600 through 1.58211

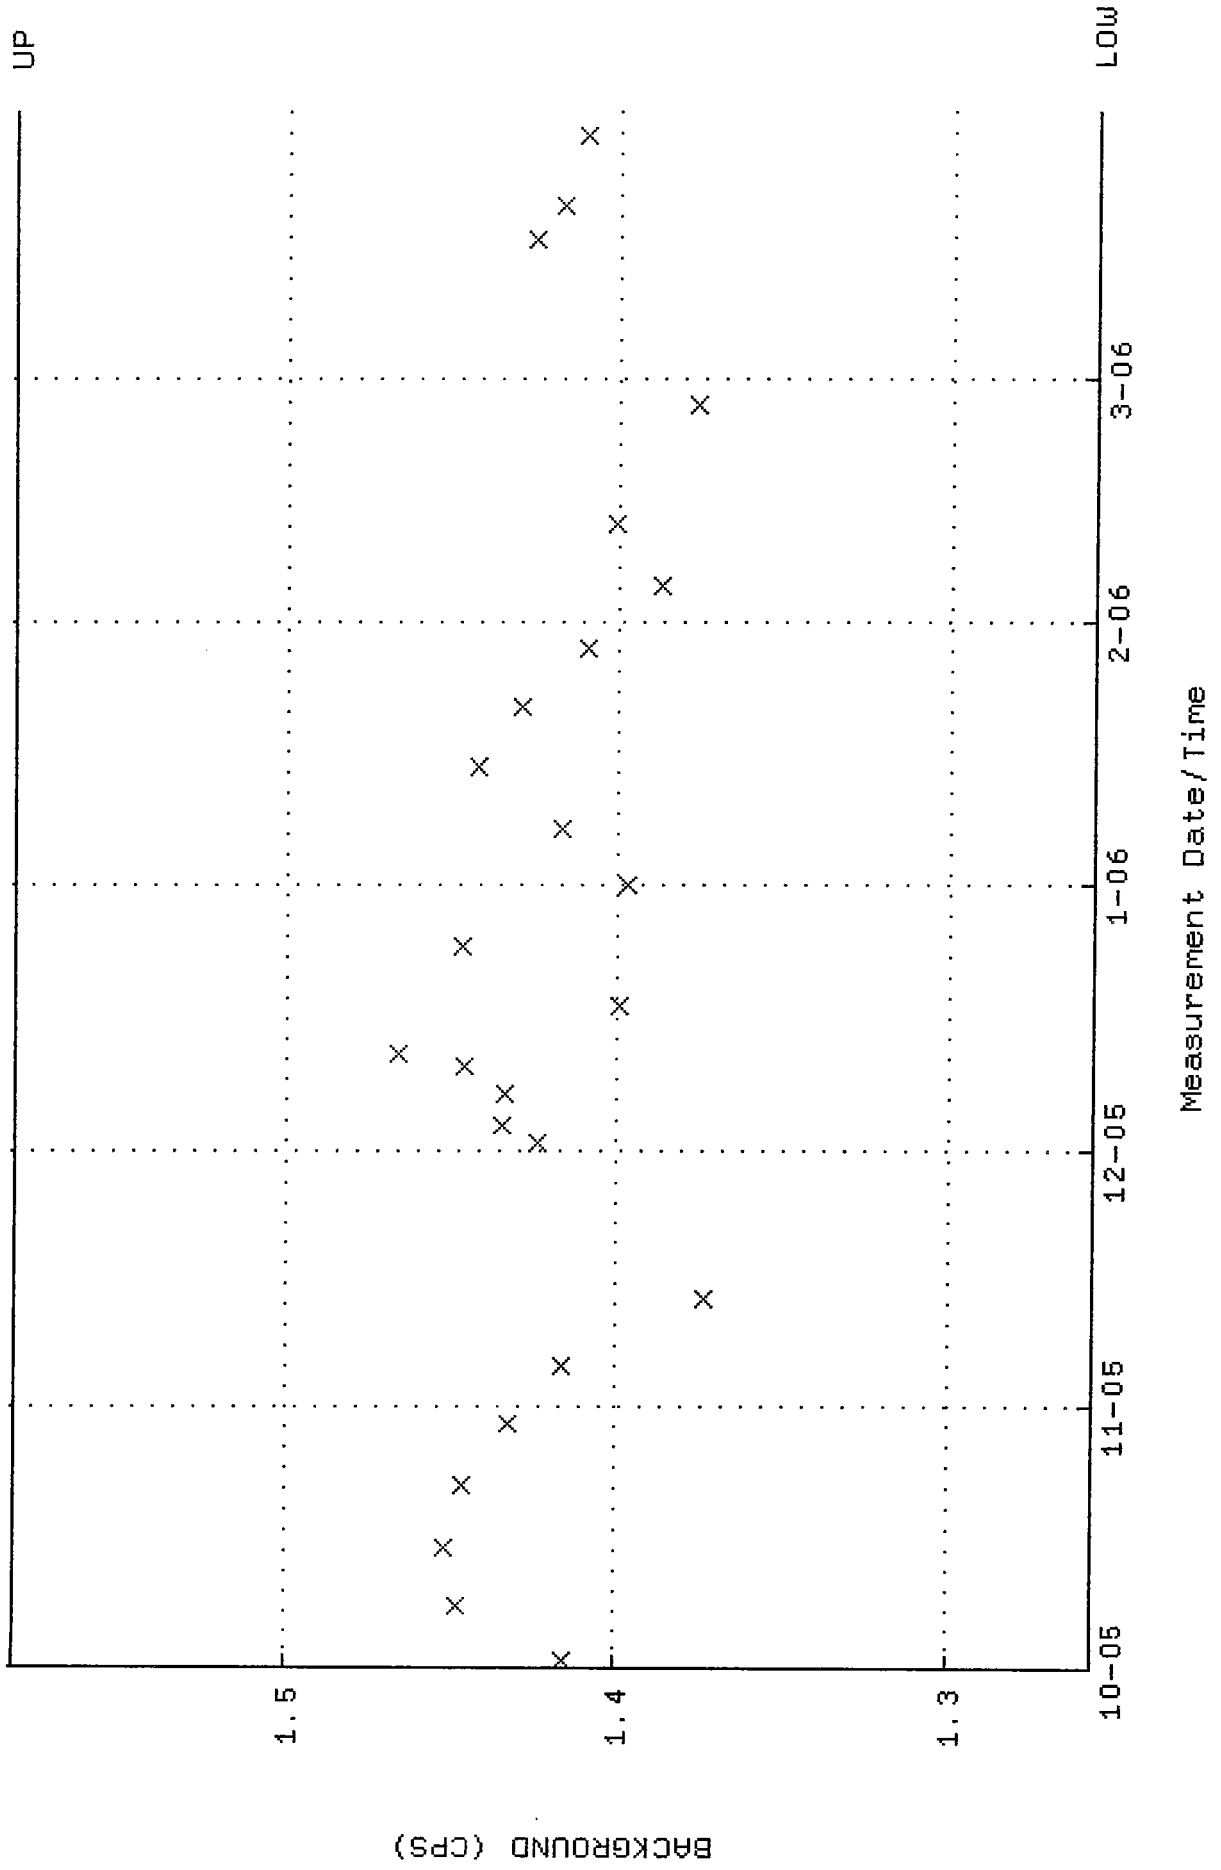

QA filename : DKA100:[ENV_ALPHA]QC_WELL.QAF;4
Parameter Name : PSFWHM-661 (PEAK FWHM (keV) CS-137)
Start/End Dates : 2-OCT-2005 11:34:54 through 31-MAR-2006 12:00:00
Lower/Upper Lmts: 0.100000 through 3.000000

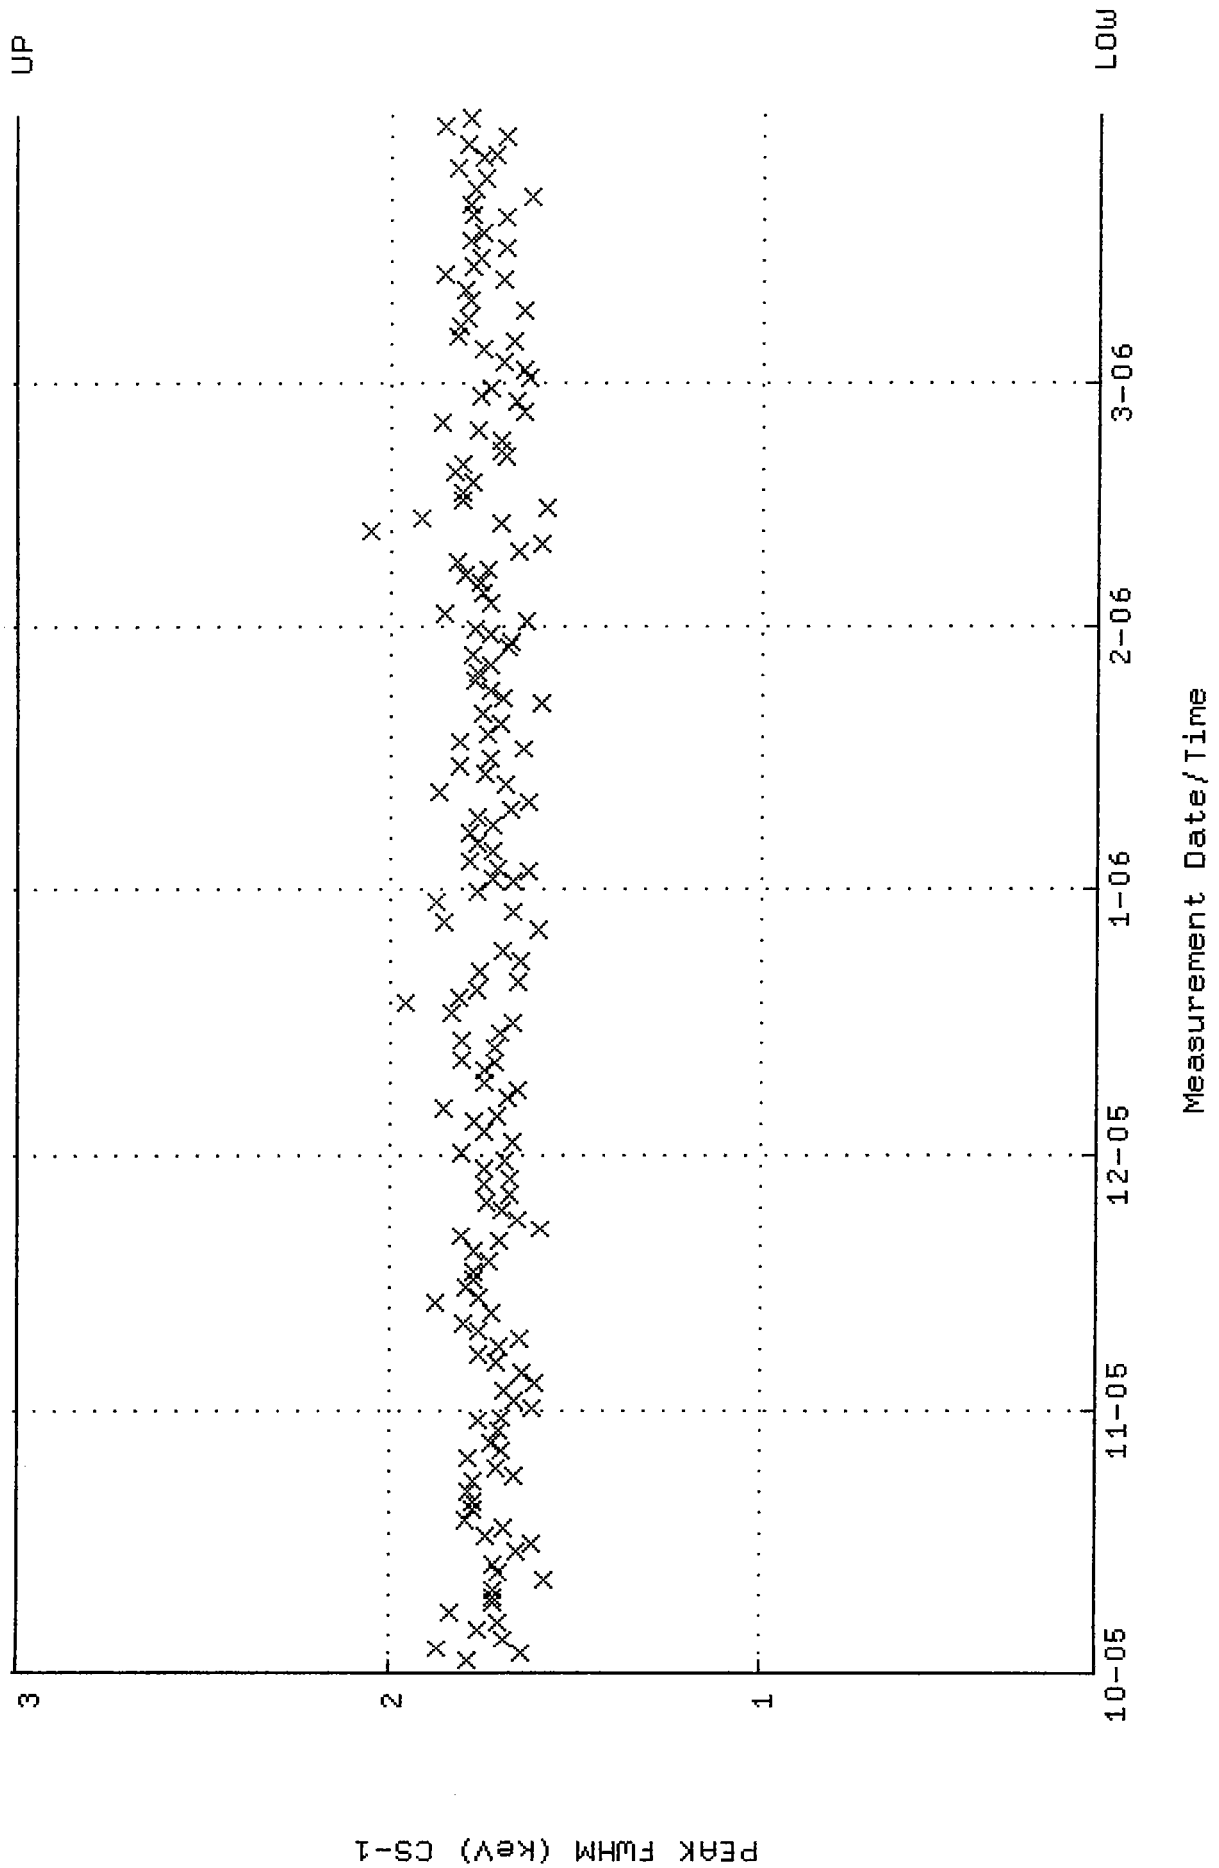





QA filename : DKA100:[ENV_ALPHA]QC_BKG_WELL.QAF;2
 Parameter Name : BACKRATE (BACKGROUND (CPS))
 Start/End Dates : 2-OCT-2005 11:46:24 through 31-MAR-2006 12:00:00
 Lower/Upper Lmts: 1.34470 through 2.05930

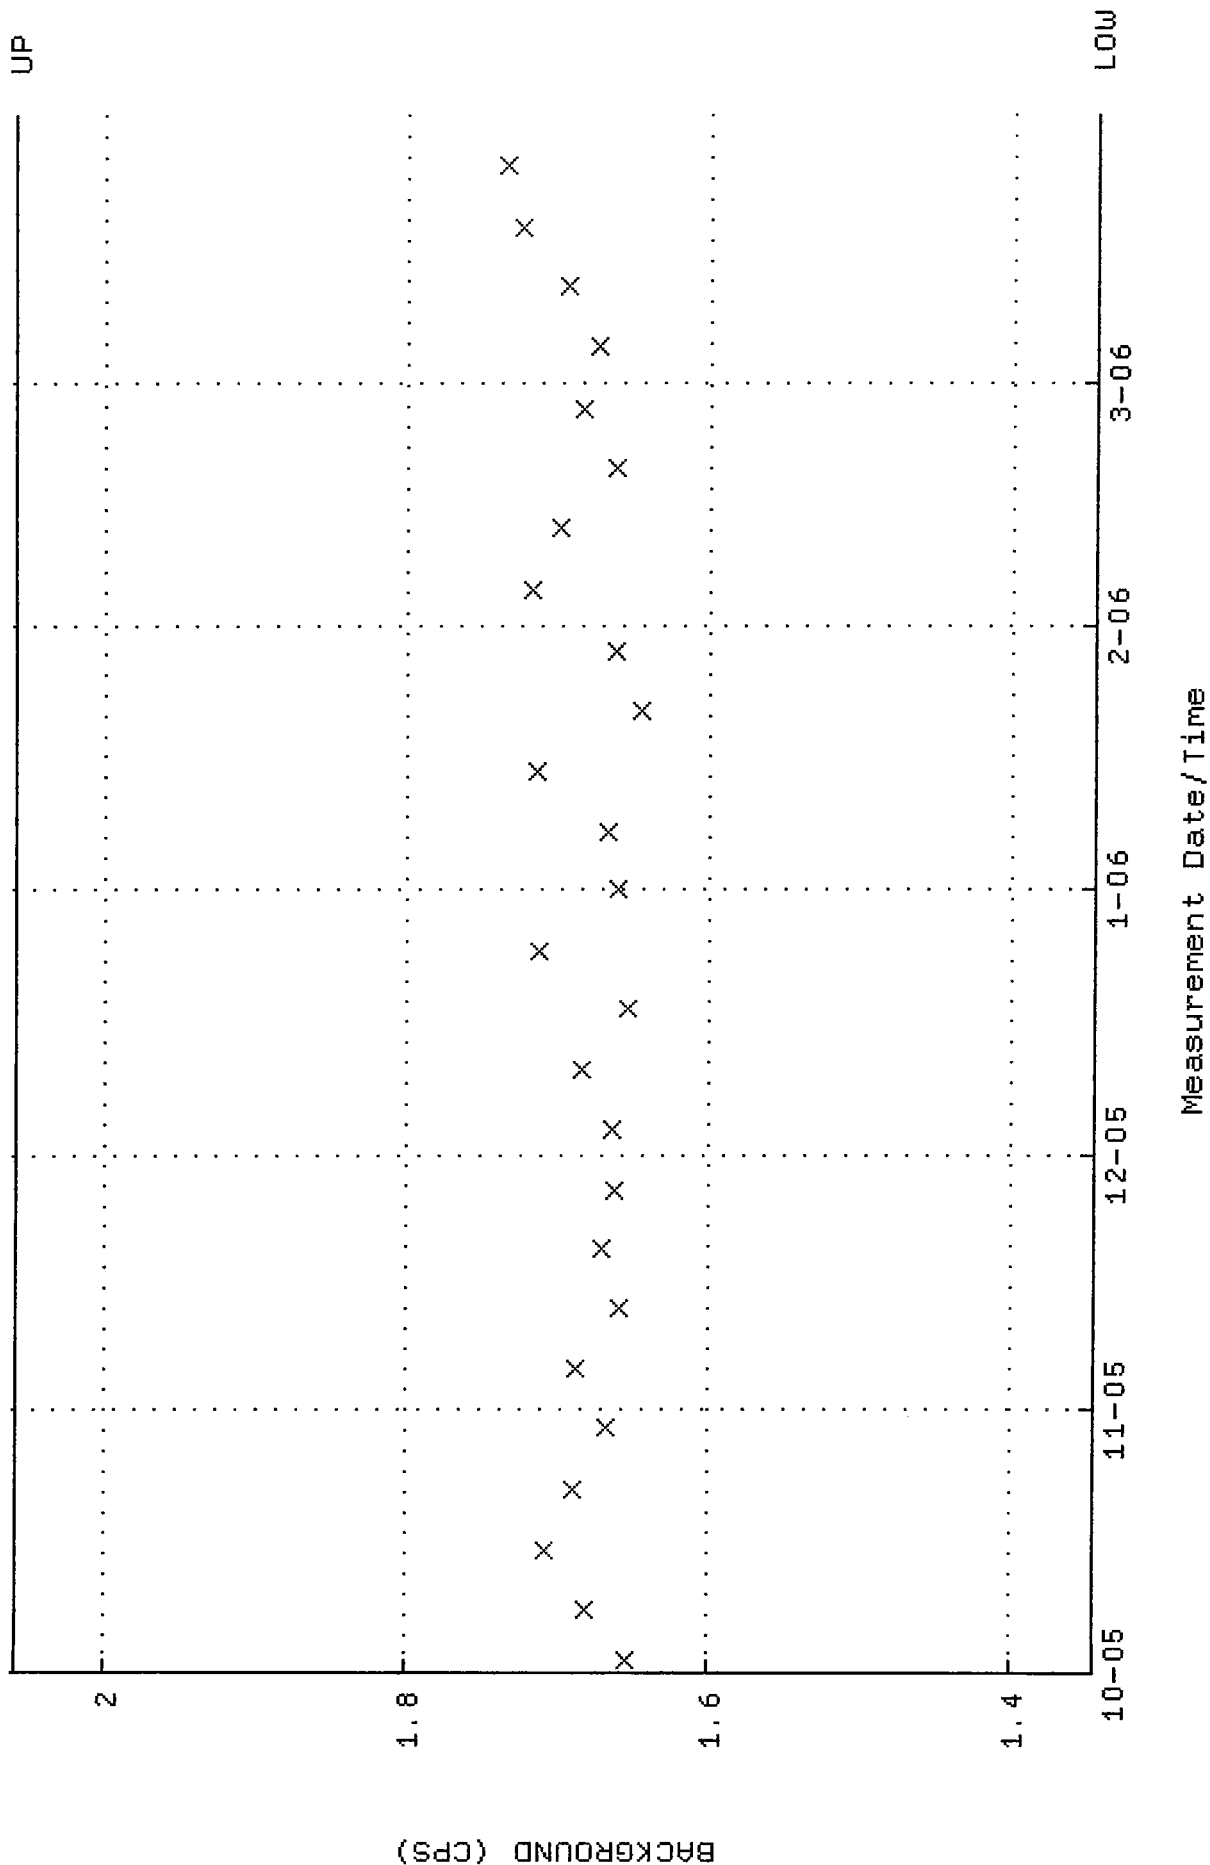

QUALITY CONTROL CHARTS


SPC Graph for Gas Flow Lead-210 in Solids 4/9/2006

Lead-210 BLANK

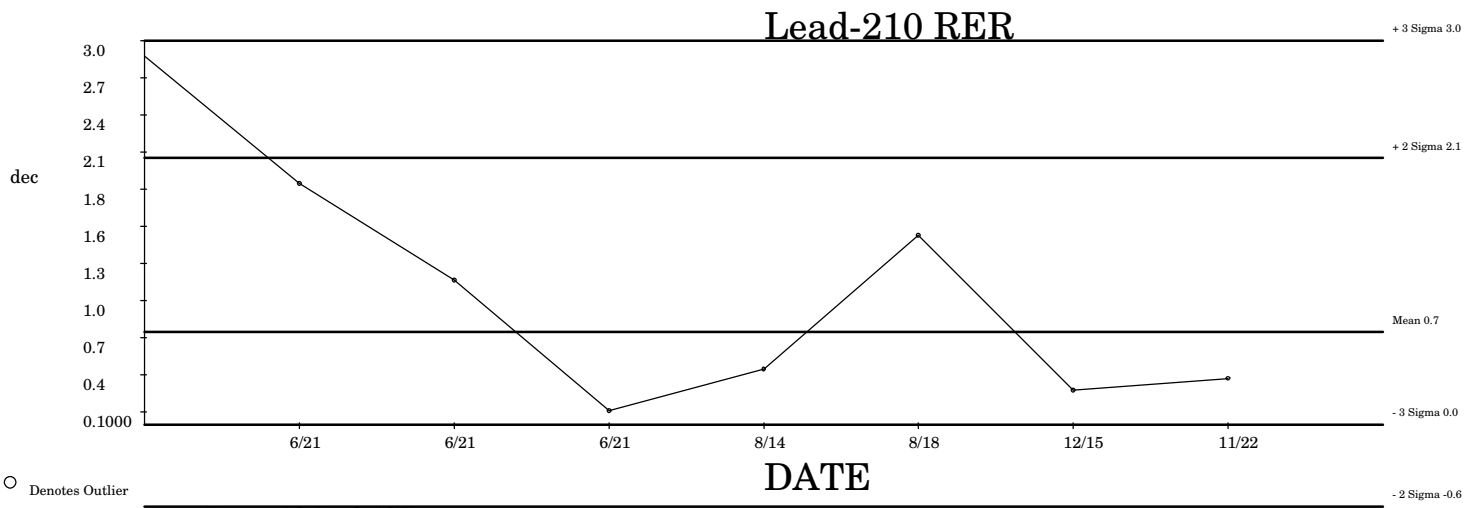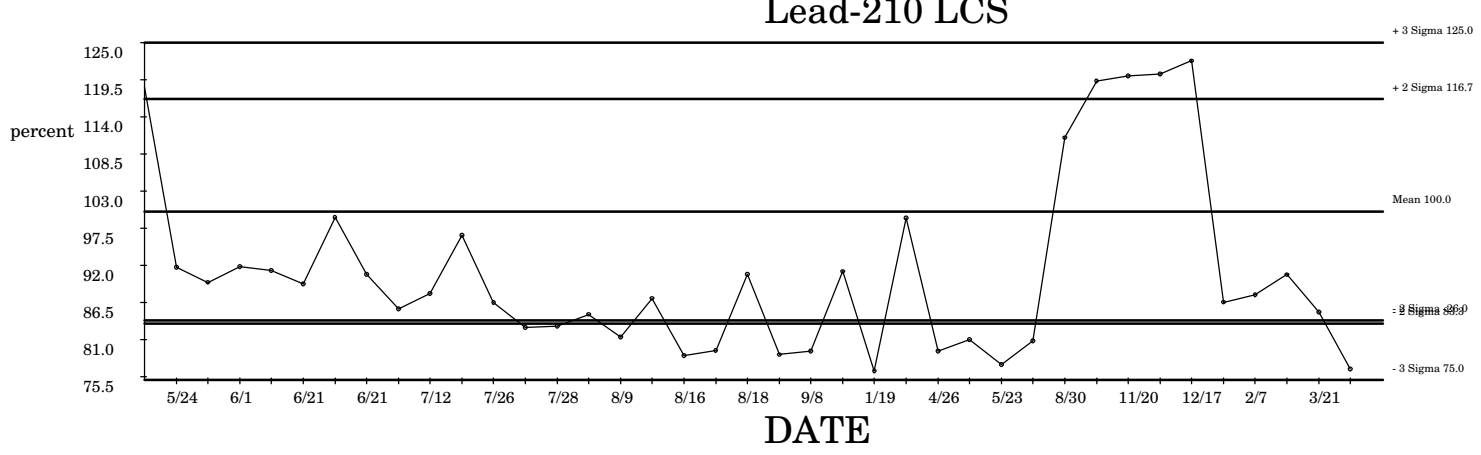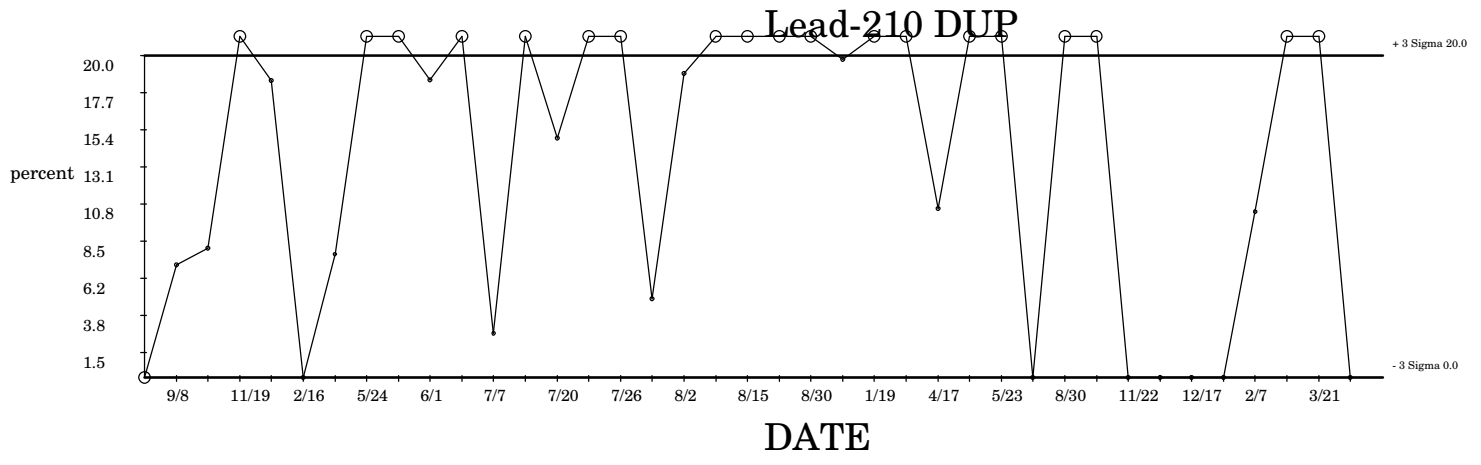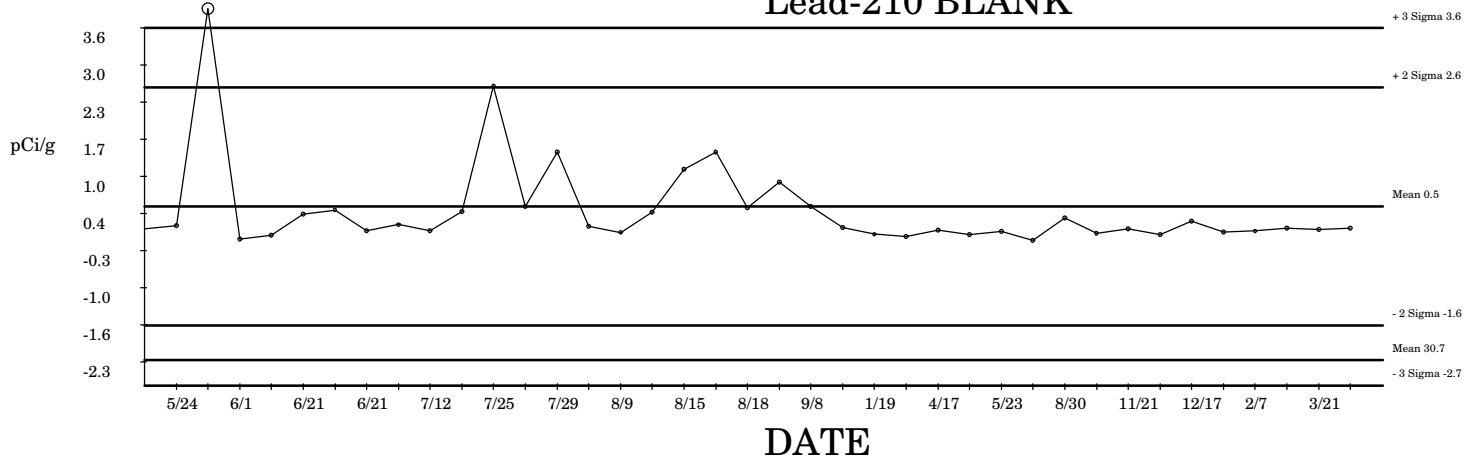

○ Denotes Outlier

SPC Graph for Gas Flow Lead-210 in Solids 4/9/2006 Lead-210 SPIKE

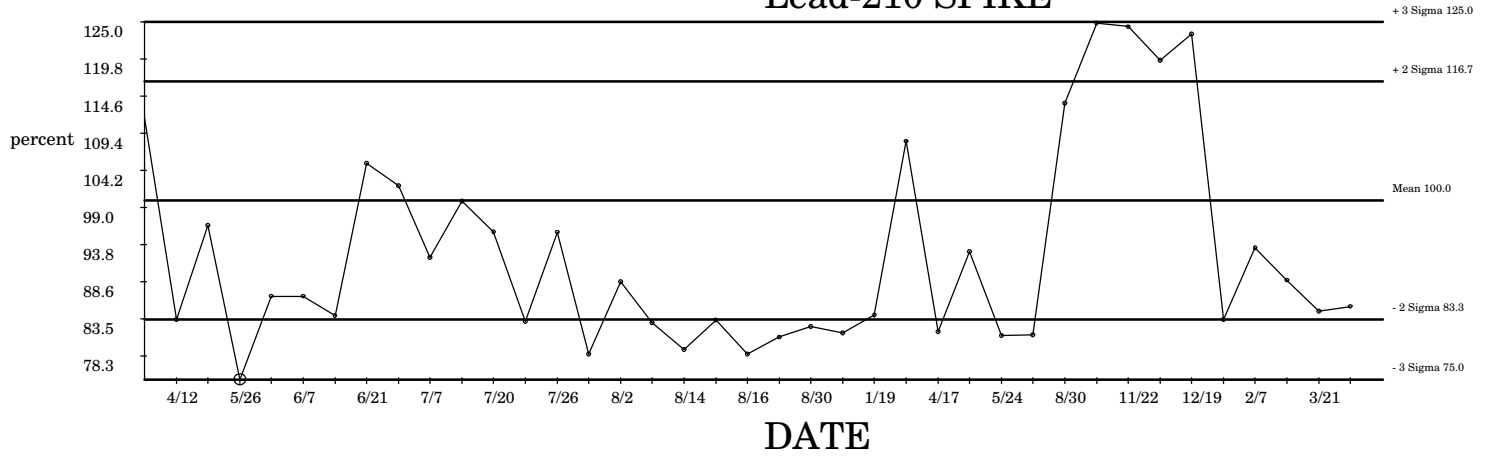

○ Denotes Outlier

Data used for Gas Flow Lead-210 in Solids 10-APR-2006

Lead-210 BLANK: Limits LCL = -2.7 UCL = 3.6

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
322628	1200600727	13-APR-2004 16:03	DONE	1	0.37	pCi/g	0.47	-2.7	-1.6	2.58	3.63	1.05
330965	1200620138	24-MAY-2004 10:37	DONE	0	-0.32	pCi/g	0.47	-2.7	-1.6	2.58	3.63	1.05
333934	1200626932	26-MAY-2004 12:22	DUSE	6	5.2	pCi/g	0.47	-2.7	-1.6	2.58	3.63	1.05
336451	1200632647	01-JUN-2004 17:50	DONE	0	-0.55	pCi/g	0.47	-2.7	-1.6	2.58	3.63	1.05
337155	1200634385	07-JUN-2004 08:16	DONE	0	-0.49	pCi/g	0.47	-2.7	-1.6	2.58	3.63	1.05
340853	1200643312	21-JUN-2004 09:04	DONE	0	-0.12	pCi/g	0.47	-2.7	-1.6	2.58	3.63	1.05
340852	1200643308	21-JUN-2004 10:24	DONE	0	-0.06	pCi/g	0.47	-2.7	-1.6	2.58	3.63	1.05
340854	1200643316	21-JUN-2004 12:48	DONE	0	-0.41	pCi/g	0.47	-2.7	-1.6	2.58	3.63	1.05
344683	1200652605	07-JUL-2004 11:05	DONE	0	-0.3	pCi/g	0.47	-2.7	-1.6	2.58	3.63	1.05
345863	1200655310	12-JUL-2004 12:24	DONE	0	-0.4	pCi/g	0.47	-2.7	-1.6	2.58	3.63	1.05
346907	1200657807	20-JUL-2004 06:31	DONE	0	-0.09	pCi/g	0.47	-2.7	-1.6	2.58	3.63	1.05
349408	1200663951	25-JUL-2004 20:10	DONE	3	2	pCi/g	0.47	-2.7	-1.6	2.58	3.63	1.05
348807	1200662463	26-JUL-2004 04:52	DONE	0	-0	pCi/g	0.47	-2.7	-1.6	2.58	3.63	1.05
350666	1200666973	29-JUL-2004 05:47	DONE	1	0.91	pCi/g	0.47	-2.7	-1.6	2.58	3.63	1.05
350579	1200666738	02-AUG-2004 12:51	DONE	0	-0.33	pCi/g	0.47	-2.7	-1.6	2.58	3.63	1.05
352502	1200671517	09-AUG-2004 09:06	DONE	0	-0.43	pCi/g	0.47	-2.7	-1.6	2.58	3.63	1.05
352503	1200671521	14-AUG-2004 03:38	DONE	0	-0.09	pCi/g	0.47	-2.7	-1.6	2.58	3.63	1.05
355295	1200678069	15-AUG-2004 22:03	DONE	1	0.62	pCi/g	0.47	-2.7	-1.6	2.58	3.63	1.05
355768	1200679185	17-AUG-2004 02:18	DONE	1	0.91	pCi/g	0.47	-2.7	-1.6	2.58	3.63	1.05
353310	1200673377	18-AUG-2004 10:42	DONE	0	-0.02	pCi/g	0.47	-2.7	-1.6	2.58	3.63	1.05
359688	1200688226	30-AUG-2004 04:45	DONE	1	0.41	pCi/g	0.47	-2.7	-1.6	2.58	3.63	1.05
361952	1200693376	08-SEP-2004 16:10	DONE	0	-0	pCi/g	0.47	-2.7	-1.6	2.58	3.63	1.05
385979	1200751688	15-DEC-2004 09:29	DONE	0	-0.35	pCi/g	0.47	-2.7	-1.6	2.58	3.63	1.05
392820	1200768316	19-JAN-2005 09:26	DONE	0	-0.47	pCi/g	0.47	-2.7	-1.6	2.58	3.63	1.05
405418	1200798077	10-MAR-2005 18:58	DONE	0	-0.5	pCi/g	0.47	-2.7	-1.6	2.58	3.63	1.05
415574	1200822203	17-APR-2005 22:49	DONE	0	-0.4	pCi/g	0.47	-2.7	-1.6	2.58	3.63	1.05
418355	1200829064	01-MAY-2005 22:50	DONE	0	-0.47	pCi/g	0.47	-2.7	-1.6	2.58	3.63	1.05
424026	1200842937	23-MAY-2005 06:55	DONE	0	-0.42	pCi/g	0.47	-2.7	-1.6	2.58	3.63	1.05
429603	1200856585	20-JUN-2005 20:32	DONE	0	-0.56	pCi/g	0.47	-2.7	-1.6	2.58	3.63	1.05
455860	1200919487	30-AUG-2005 07:26	DONE	0	-0.19	pCi/g	0.47	-2.7	-1.6	2.58	3.63	1.05
470738	1200955079	19-OCT-2005 10:43	DONE	0	-0.45	pCi/g	0.47	-2.7	-1.6	2.58	3.63	1.05
479184	1200975538	21-NOV-2005 12:52	DONE	0	-0.38	pCi/g	0.47	-2.7	-1.6	2.58	3.63	1.05
482517	1200983367	06-DEC-2005 10:33	DONE	0	-0.47	pCi/g	0.47	-2.7	-1.6	2.58	3.63	1.05
485401	1200990518	17-DEC-2005 20:40	DONE	0	-0.24	pCi/g	0.47	-2.7	-1.6	2.58	3.63	1.05
491487	1201004535	17-JAN-2006 10:22	DONE	0	-0.43	pCi/g	0.47	-2.7	-1.6	2.58	3.63	1.05
498367	1201020049	07-FEB-2006 10:38	DONE	0	-0.41	pCi/g	0.47	-2.7	-1.6	2.58	3.63	1.05
511471	1201050513	15-MAR-2006 23:30	DONE	0	-0.36	pCi/g	0.47	-2.7	-1.6	2.58	3.63	1.05
511473	1201050521	21-MAR-2006 11:51	DONE	0	-0.39	pCi/g	0.47	-2.7	-1.6	2.58	3.63	1.05
517517	1201063764	09-APR-2006 09:57	DONE	0	-0.36	pCi/g	0.47	-2.7	-1.6	2.58	3.63	1.05

Lead-210 DUP: Limits LCL = 0 UCL = 20

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
264844	1200459098	04-AUG-2003 12:24	DONE	33	0.08	percent	30.7	0	-26	87.3	20.0	28.3
273724	1200481614	08-SEP-2003 13:12	DONE	7	-0.84	percent	30.7	0	-26	87.3	20.0	28.3
288690	1200518946	10-NOV-2003 14:40	DONE	8	-0.8	percent	30.7	0	-26	87.3	20.0	28.3
288976	1200519739	19-NOV-2003 14:31	DONE	62	1.1	percent	30.7	0	-26	87.3	20.0	28.3

305923	1200560409	01-FEB-2004 15:46	DONE	18	-0.43	percent	30.7	0	-26	87.3	20.0	28.3
307587	1200564193	16-FEB-2004 12:32	DONE	0	-1	percent	30.7	0	-26	87.3	20.0	28.3
322629	1200600730	12-APR-2004 11:07	DONE	8	-0.81	percent	30.7	0	-26	87.3	20.0	28.3
330965	1200620139	24-MAY-2004 10:37	DONE	39	0.3	percent	30.7	0	-26	87.3	20.0	28.3
333934	1200626933	26-MAY-2004 12:22	DUSE	92	2.2	percent	30.7	0	-26	87.3	20.0	28.3
336451	1200632648	01-JUN-2004 17:50	DONE	19	-0.43	percent	30.7	0	-26	87.3	20.0	28.3
337155	1200634386	07-JUN-2004 08:16	DONE	42	0.41	percent	30.7	0	-26	87.3	20.0	28.3
344683	1200652606	07-JUL-2004 11:05	DONE	3	-0.99	percent	30.7	0	-26	87.3	20.0	28.3
345863	1200655311	12-JUL-2004 12:24	DONE	27	-0.15	percent	30.7	0	-26	87.3	20.0	28.3
346907	1200657808	20-JUL-2004 06:31	DONE	15	-0.56	percent	30.7	0	-26	87.3	20.0	28.3
349408	1200663952	25-JUL-2004 20:10	DONE	28	-0.1	percent	30.7	0	-26	87.3	20.0	28.3
348807	1200662464	26-JUL-2004 04:52	DONE	52	0.74	percent	30.7	0	-26	87.3	20.0	28.3
350666	1200666974	29-JUL-2004 05:47	DONE	5	-0.91	percent	30.7	0	-26	87.3	20.0	28.3
350579	1200666739	02-AUG-2004 12:51	DONE	19	-0.42	percent	30.7	0	-26	87.3	20.0	28.3
352502	1200671518	09-AUG-2004 09:06	DONE	80	1.7	percent	30.7	0	-26	87.3	20.0	28.3
355295	1200678070	15-AUG-2004 22:03	DONE	63	1.1	percent	30.7	0	-26	87.3	20.0	28.3
355768	1200679186	15-AUG-2004 22:03	DONE	62	1.1	percent	30.7	0	-26	87.3	20.0	28.3
359688	1200688227	30-AUG-2004 04:45	DONE	95	2.3	percent	30.7	0	-26	87.3	20.0	28.3
361952	1200693377	08-SEP-2004 16:10	DONE	20	-0.38	percent	30.7	0	-26	87.3	20.0	28.3
392820	1200768317	19-JAN-2005 09:26	DONE	39	0.29	percent	30.7	0	-26	87.3	20.0	28.3
405418	1200798078	10-MAR-2005 18:58	DONE	54	0.84	percent	30.7	0	-26	87.3	20.0	28.3
415574	1200822204	17-APR-2005 22:49	DONE	11	-0.71	percent	30.7	0	-26	87.3	20.0	28.3
418355	1200829065	01-MAY-2005 22:50	DONE	30	-0.03	percent	30.7	0	-26	87.3	20.0	28.3
424026	1200842938	23-MAY-2005 06:55	DONE	26	-0.18	percent	30.7	0	-26	87.3	20.0	28.3
429603	1200856586	20-JUN-2005 20:32	DONE	0	-1	percent	30.7	0	-26	87.3	20.0	28.3
455860	1200919488	30-AUG-2005 07:26	DONE	28	-0.1	percent	30.7	0	-26	87.3	20.0	28.3
470738	1200955080	19-OCT-2005 10:43	DONE	57	0.93	percent	30.7	0	-26	87.3	20.0	28.3
479184	1200975539	22-NOV-2005 09:38	DONE	0	-1	percent	30.7	0	-26	87.3	20.0	28.3
482517	1200983368	06-DEC-2005 10:34	DONE	0	-1	percent	30.7	0	-26	87.3	20.0	28.3
485401	1200990519	17-DEC-2005 20:40	DONE	0	-1	percent	30.7	0	-26	87.3	20.0	28.3
491487	1201004536	17-JAN-2006 10:22	DONE	0	-1	percent	30.7	0	-26	87.3	20.0	28.3
498367	1201020050	07-FEB-2006 10:38	DONE	10	-0.72	percent	30.7	0	-26	87.3	20.0	28.3
511471	1201050514	15-MAR-2006 23:34	DONE	63	1.1	percent	30.7	0	-26	87.3	20.0	28.3
511473	1201050522	21-MAR-2006 11:52	DONE	84	1.9	percent	30.7	0	-26	87.3	20.0	28.3
517517	1201063765	09-APR-2006 09:57	DONE	0	-1	percent	30.7	0	-26	87.3	20.0	28.3

Lead-210 LCS: Limits LCL = 75 UCL = 125

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
322628	1200600728	13-APR-2004 16:03	DONE	82	-2	percent	100	75.0	83.3	117	125	8.33
330965	1200620141	24-MAY-2004 10:37	DONE	92	-01	percent	100	75.0	83.3	117	125	8.33
333934	1200626935	26-MAY-2004 12:22	DUSE	89	-1	percent	100	75.0	83.3	117	125	8.33
336451	1200632650	01-JUN-2004 10:35	DONE	92	-0.98	percent	100	75.0	83.3	117	125	8.33
337155	1200634388	07-JUN-2004 08:16	DONE	91	-1	percent	100	75.0	83.3	117	125	8.33
340853	1200643315	21-JUN-2004 09:04	DONE	89	-1	percent	100	75.0	83.3	117	125	8.33
340852	1200643311	21-JUN-2004 10:24	DONE	99	-0.11	percent	100	75.0	83.3	117	125	8.33
340854	1200643319	21-JUN-2004 14:14	DONE	91	-1	percent	100	75.0	83.3	117	125	8.33
344683	1200652608	07-JUL-2004 11:05	DONE	86	-2	percent	100	75.0	83.3	117	125	8.33
345863	1200655313	12-JUL-2004 15:05	DONE	88	-1	percent	100	75.0	83.3	117	125	8.33
346907	1200657810	20-JUL-2004 12:08	DONE	96	-0.43	percent	100	75.0	83.3	117	125	8.33
348807	1200662466	26-JUL-2004 09:43	DONE	86	-2	percent	100	75.0	83.3	117	125	8.33

349408	1200663954	26-JUL-2004 09:43	DONE	83	-2	percent	100	75.0	83.3	117	125	8.33
350666	1200666976	28-JUL-2004 18:25	DONE	83	-2	percent	100	75.0	83.3	117	125	8.33
350579	1200666741	02-AUG-2004 12:51	DONE	85	-2	percent	100	75.0	83.3	117	125	8.33
352502	1200671520	09-AUG-2004 09:06	DONE	81	-2	percent	100	75.0	83.3	117	125	8.33
352503	1200671524	14-AUG-2004 03:39	DONE	87	-2	percent	100	75.0	83.3	117	125	8.33
355295	1200678072	16-AUG-2004 08:54	DONE	79	-3	percent	100	75.0	83.3	117	125	8.33
355768	1200679188	16-AUG-2004 08:57	DONE	79	-2	percent	100	75.0	83.3	117	125	8.33
353310	1200673380	18-AUG-2004 10:42	DONE	91	-1	percent	100	75.0	83.3	117	125	8.33
359688	1200688229	30-AUG-2004 11:32	DONE	79	-3	percent	100	75.0	83.3	117	125	8.33
361952	1200693379	08-SEP-2004 08:49	DONE	79	-2	percent	100	75.0	83.3	117	125	8.33
385979	1200751690	15-DEC-2004 09:29	DONE	91	-1	percent	100	75.0	83.3	117	125	8.33
392820	1200768319	19-JAN-2005 07:26	DONE	76	-3	percent	100	75.0	83.3	117	125	8.33
405418	1200798080	10-MAR-2005 18:58	DONE	99	-0.12	percent	100	75.0	83.3	117	125	8.33
415574	1200822206	26-APR-2005 08:20	DONE	79	-2	percent	100	75.0	83.3	117	125	8.33
418355	1200829067	01-MAY-2005 22:49	DONE	81	-2	percent	100	75.0	83.3	117	125	8.33
424026	1200842940	23-MAY-2005 06:55	DONE	77	-3	percent	100	75.0	83.3	117	125	8.33
429603	1200856588	20-JUN-2005 21:37	DONE	81	-2	percent	100	75.0	83.3	117	125	8.33
455860	1200919490	30-AUG-2005 07:26	DONE	111	1.3	percent	100	75.0	83.3	117	125	8.33
470738	1200955082	19-OCT-2005 10:43	DONE	119	2.3	percent	100	75.0	83.3	117	125	8.33
479184	1200975541	20-NOV-2005 23:00	DONE	120	2.4	percent	100	75.0	83.3	117	125	8.33
482517	1200983370	06-DEC-2005 10:34	DONE	120	2.4	percent	100	75.0	83.3	117	125	8.33
485401	1200990521	17-DEC-2005 21:33	DONE	122	2.7	percent	100	75.0	83.3	117	125	8.33
491487	1201004538	17-JAN-2006 10:23	DONE	87	-2	percent	100	75.0	83.3	117	125	8.33
498367	1201020052	07-FEB-2006 12:13	DONE	88	-1	percent	100	75.0	83.3	117	125	8.33
511471	1201050516	15-MAR-2006 23:30	DONE	91	-1	percent	100	75.0	83.3	117	125	8.33
511473	1201050524	21-MAR-2006 11:52	DONE	85	-2	percent	100	75.0	83.3	117	125	8.33
517517	1201063767	09-APR-2006 09:57	DONE	77	-3	percent	100	75.0	83.3	117	125	8.33

Lead-210 RER: Limits LCL = 0 UCL = 3


Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
273724	1200481614	08-SEP-2003 13:12	DONE	0.12	-0.89	dec	0.72	0	-0.638	2.09	3.00	0.68
340853	1200643313	21-JUN-2004 09:04	DONE	1.89	1.7	dec	0.72	0	-0.638	2.09	3.00	0.68
340852	1200643309	21-JUN-2004 10:24	DONE	1.13	0.6	dec	0.72	0	-0.638	2.09	3.00	0.68
340854	1200643317	21-JUN-2004 12:48	DONE	0.11	-0.9	dec	0.72	0	-0.638	2.09	3.00	0.68
352503	1200671522	14-AUG-2004 03:39	DONE	0.44	-0.42	dec	0.72	0	-0.638	2.09	3.00	0.68
353310	1200673378	18-AUG-2004 10:42	DONE	1.48	1.1	dec	0.72	0	-0.638	2.09	3.00	0.68
385979	1200751689	15-DEC-2004 09:29	DONE	0.27	-0.67	dec	0.72	0	-0.638	2.09	3.00	0.68
479184	1200975539	22-NOV-2005 09:38	DONE	0.36	-0.53	dec	0.72	0	-0.638	2.09	3.00	0.68

Lead-210 SPIKE: Limits LCL = 75 UCL = 125


Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
322629	1200600731	12-APR-2004 11:07	DONE	88	-1	percent	100	75.0	83.3	117	125	8.33
322629	1200600732	12-APR-2004 11:07	DONE	83	-2	percent	100	75.0	83.3	117	125	8.33
330965	1200620140	24-MAY-2004 10:37	DONE	97	-0.42	percent	100	75.0	83.3	117	125	8.33
333934	1200626934	26-MAY-2004 12:22	DUSE	-5	-10	percent	100	75.0	83.3	117	125	8.33
336451	1200632649	01-JUN-2004 10:30	DONE	87	-2	percent	100	75.0	83.3	117	125	8.33
337155	1200634387	07-JUN-2004 08:16	DONE	87	-2	percent	100	75.0	83.3	117	125	8.33
340853	1200643314	21-JUN-2004 09:04	DONE	84	-2	percent	100	75.0	83.3	117	125	8.33
340852	1200643310	21-JUN-2004 10:24	DONE	105	0.62	percent	100	75.0	83.3	117	125	8.33
340854	1200643318	21-JUN-2004 14:14	DONE	102	0.25	percent	100	75.0	83.3	117	125	8.33

344683	1200652607	07-JUL-2004 11:05	DONE	92	-0.95	percent	100	75.0	83.3	117	125	8.33
345863	1200655312	12-JUL-2004 15:05	DONE	100	-0.01	percent	100	75.0	83.3	117	125	8.33
346907	1200657809	20-JUL-2004 12:08	DONE	96	-0.52	percent	100	75.0	83.3	117	125	8.33
348807	1200662465	26-JUL-2004 09:43	DONE	83	-2	percent	100	75.0	83.3	117	125	8.33
349408	1200663953	26-JUL-2004 09:43	DONE	96	-0.53	percent	100	75.0	83.3	117	125	8.33
350666	1200666975	28-JUL-2004 18:25	DONE	79	-3	percent	100	75.0	83.3	117	125	8.33
350579	1200666740	02-AUG-2004 12:51	DONE	89	-1	percent	100	75.0	83.3	117	125	8.33
352502	1200671519	09-AUG-2004 09:06	DONE	83	-2	percent	100	75.0	83.3	117	125	8.33
352503	1200671523	14-AUG-2004 03:39	DONE	79	-2	percent	100	75.0	83.3	117	125	8.33
355295	1200678071	16-AUG-2004 08:53	DONE	83	-2	percent	100	75.0	83.3	117	125	8.33
355768	1200679187	16-AUG-2004 08:57	DONE	79	-3	percent	100	75.0	83.3	117	125	8.33
353310	1200673379	18-AUG-2004 10:42	DONE	81	-2	percent	100	75.0	83.3	117	125	8.33
359688	1200688228	30-AUG-2004 10:23	DONE	82	-2	percent	100	75.0	83.3	117	125	8.33
361952	1200693378	08-SEP-2004 08:49	DONE	82	-2	percent	100	75.0	83.3	117	125	8.33
392820	1200768318	19-JAN-2005 07:26	DONE	84	-2	percent	100	75.0	83.3	117	125	8.33
405418	1200798079	10-MAR-2005 18:58	DONE	108	01	percent	100	75.0	83.3	117	125	8.33
415574	1200822205	17-APR-2005 22:35	DONE	82	-2	percent	100	75.0	83.3	117	125	8.33
418355	1200829066	01-MAY-2005 22:49	DONE	93	-0.86	percent	100	75.0	83.3	117	125	8.33
424026	1200842939	24-MAY-2005 18:27	DONE	81	-2	percent	100	75.0	83.3	117	125	8.33
429603	1200856587	20-JUN-2005 20:32	DONE	81	-2	percent	100	75.0	83.3	117	125	8.33
455860	1200919489	30-AUG-2005 07:26	DONE	114	1.6	percent	100	75.0	83.3	117	125	8.33
470738	1200955081	19-OCT-2005 10:43	DONE	125	3	percent	100	75.0	83.3	117	125	8.33
479184	1200975540	22-NOV-2005 21:58	DONE	124	2.9	percent	100	75.0	83.3	117	125	8.33
482517	1200983369	06-DEC-2005 10:34	DONE	120	2.4	percent	100	75.0	83.3	117	125	8.33
485401	1200990520	19-DEC-2005 10:52	DONE	123	2.8	percent	100	75.0	83.3	117	125	8.33
491487	1201004537	17-JAN-2006 10:22	DONE	83	-2	percent	100	75.0	83.3	117	125	8.33
498367	1201020051	07-FEB-2006 10:38	DONE	93	-0.79	percent	100	75.0	83.3	117	125	8.33
511471	1201050515	15-MAR-2006 23:30	DONE	89	-1	percent	100	75.0	83.3	117	125	8.33
511473	1201050523	21-MAR-2006 11:52	DONE	85	-2	percent	100	75.0	83.3	117	125	8.33
517517	1201063766	09-APR-2006 09:57	DONE	85	-2	percent	100	75.0	83.3	117	125	8.33





SPC Graph for Gamma Spec in Solids 4/12/2006 Americium-241 LCS

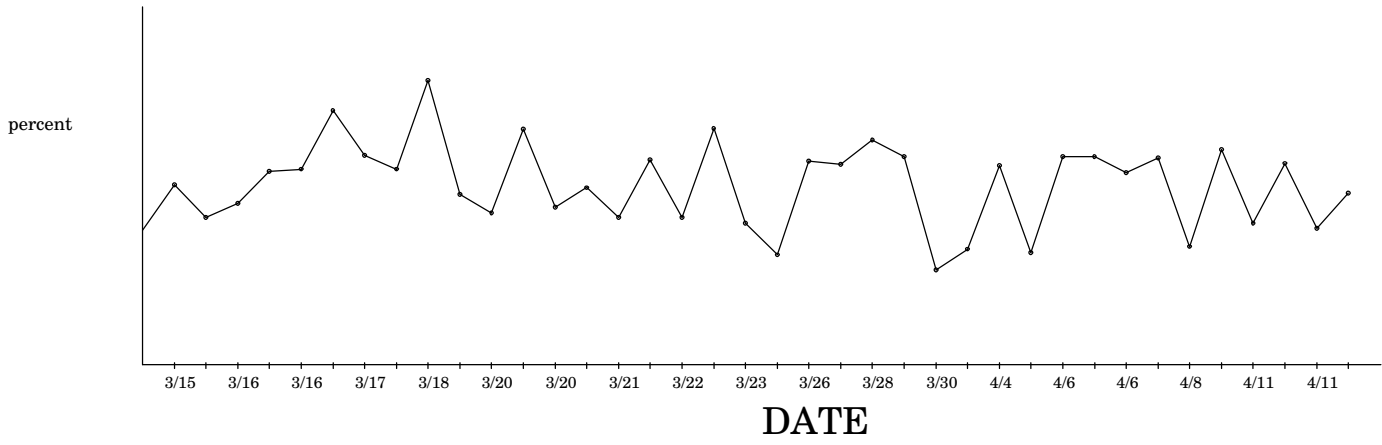

Americium-241 RER




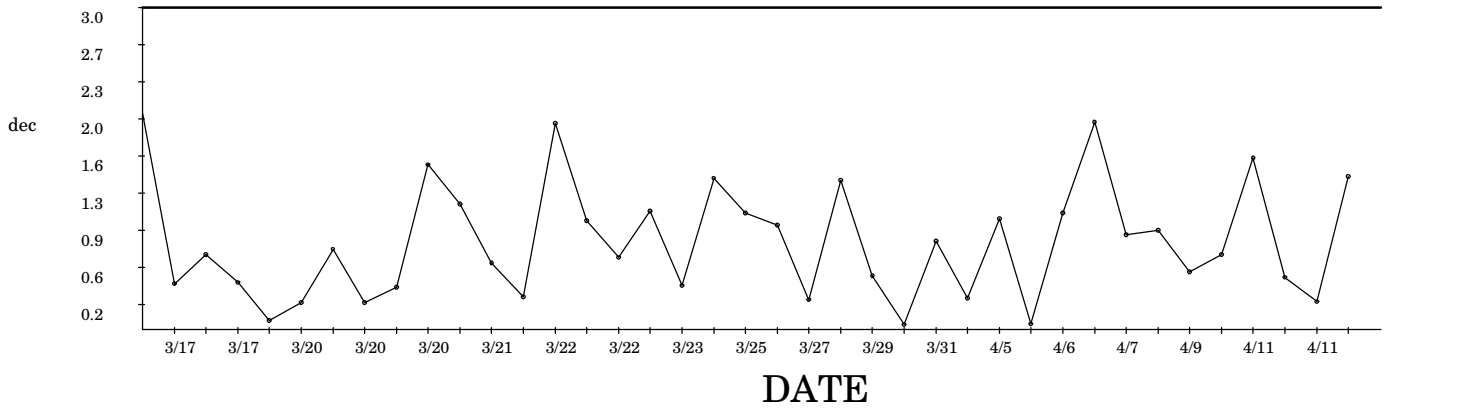


SPC Graph for Gamma Spec in Solids 4/12/2006 Cesium-137 BLANK

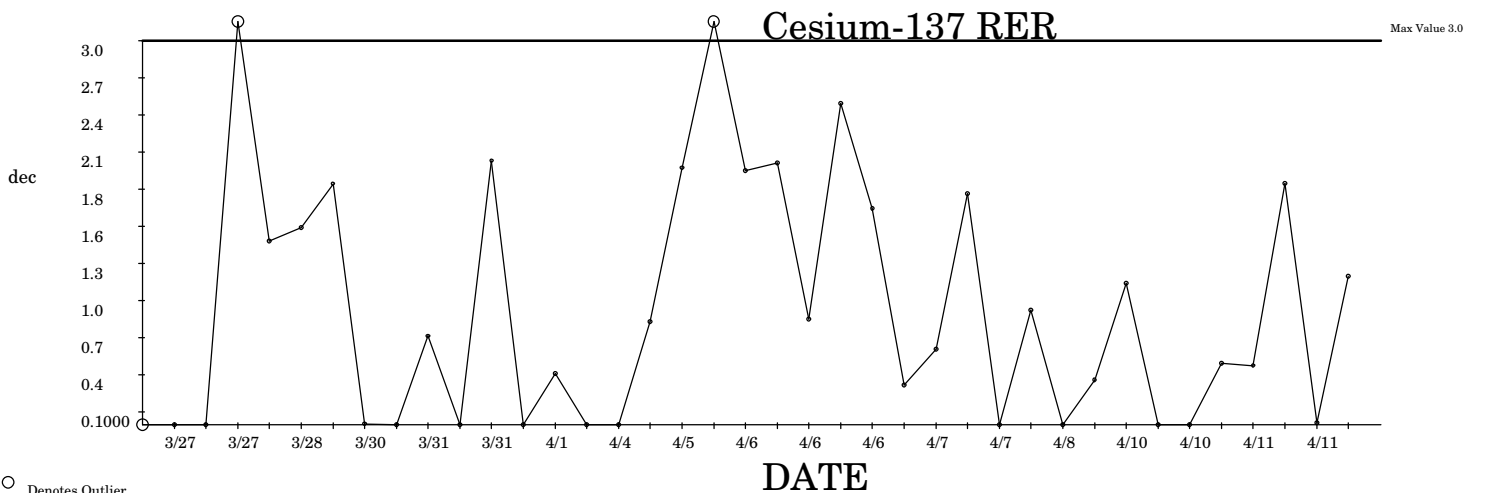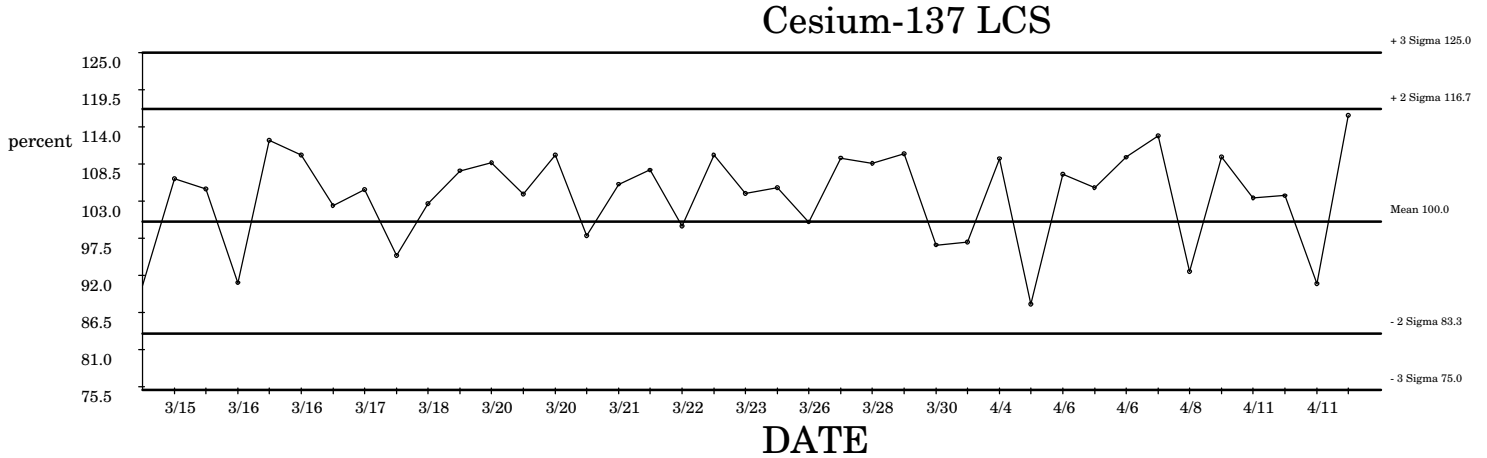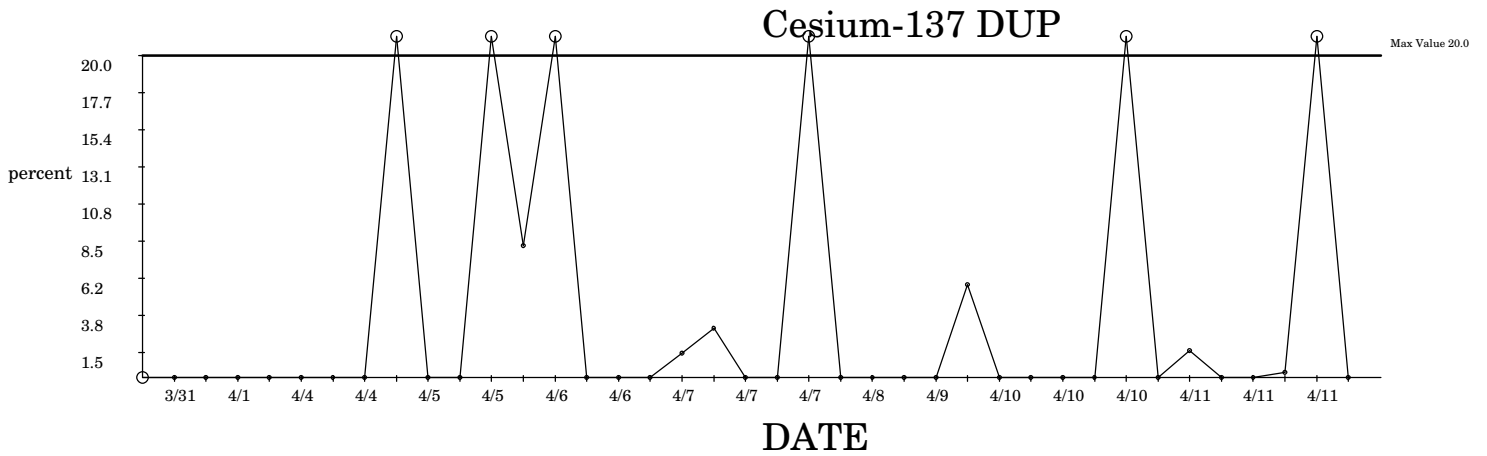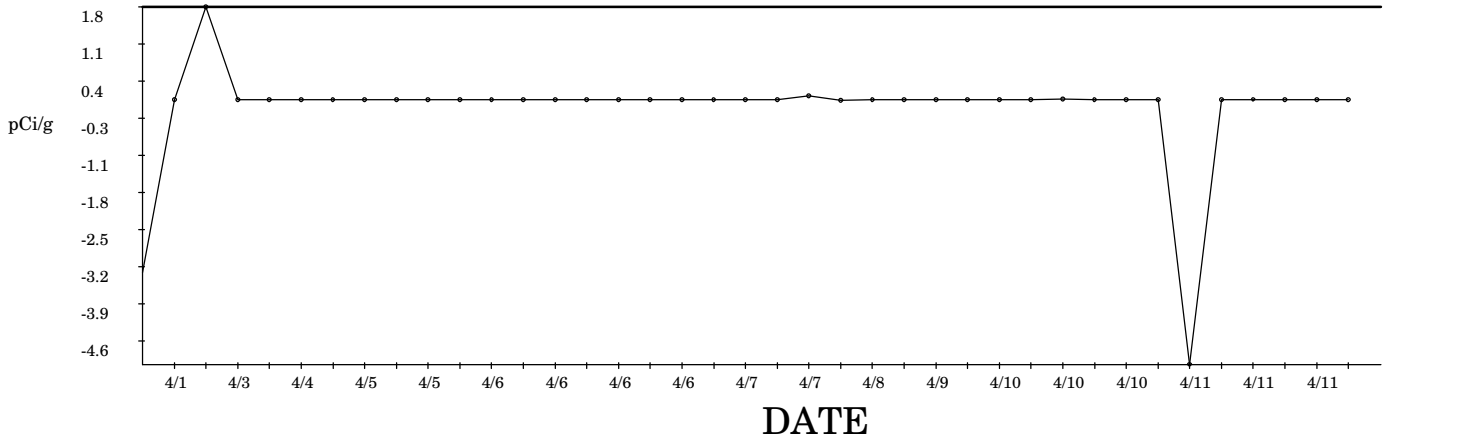


○ Denotes Outlier

SPC Graph for Gamma Spec in Solids 4/12/2006 Cobalt-60 BLANK

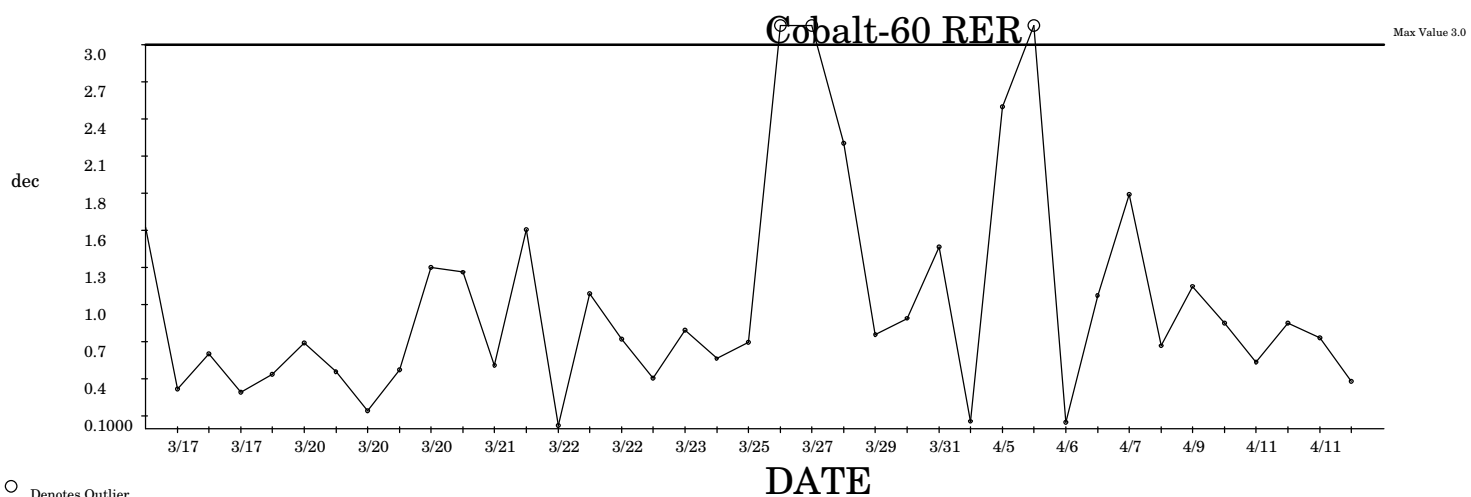
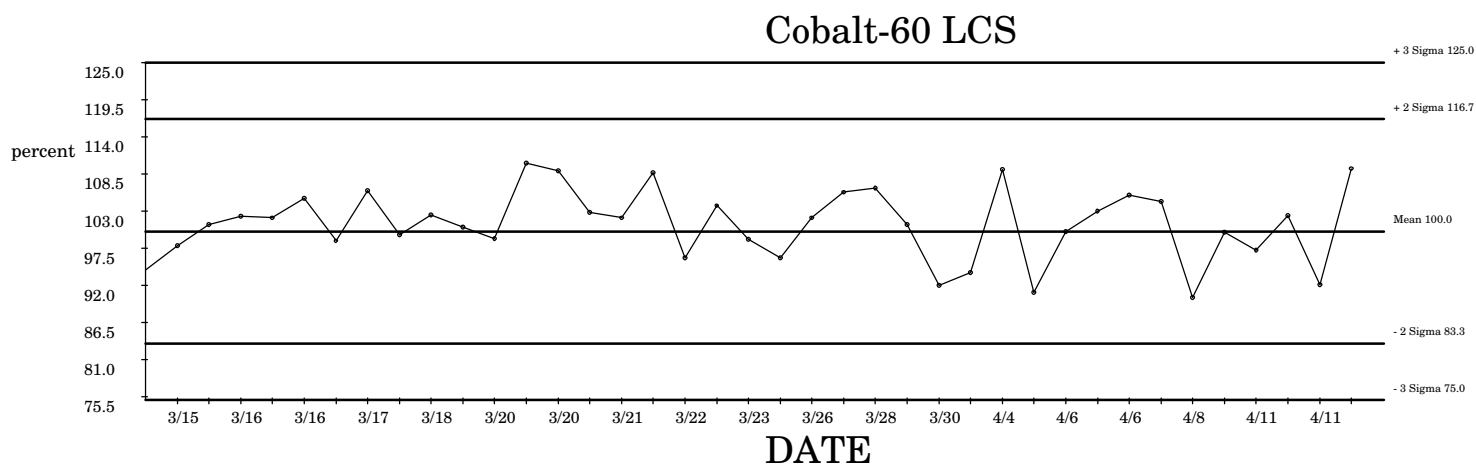
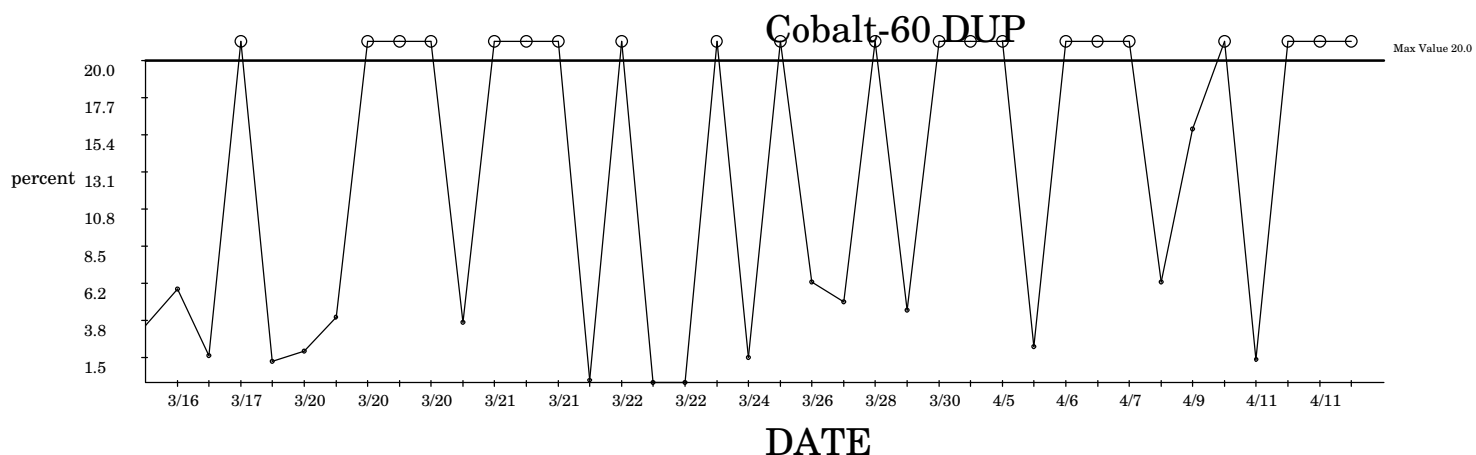
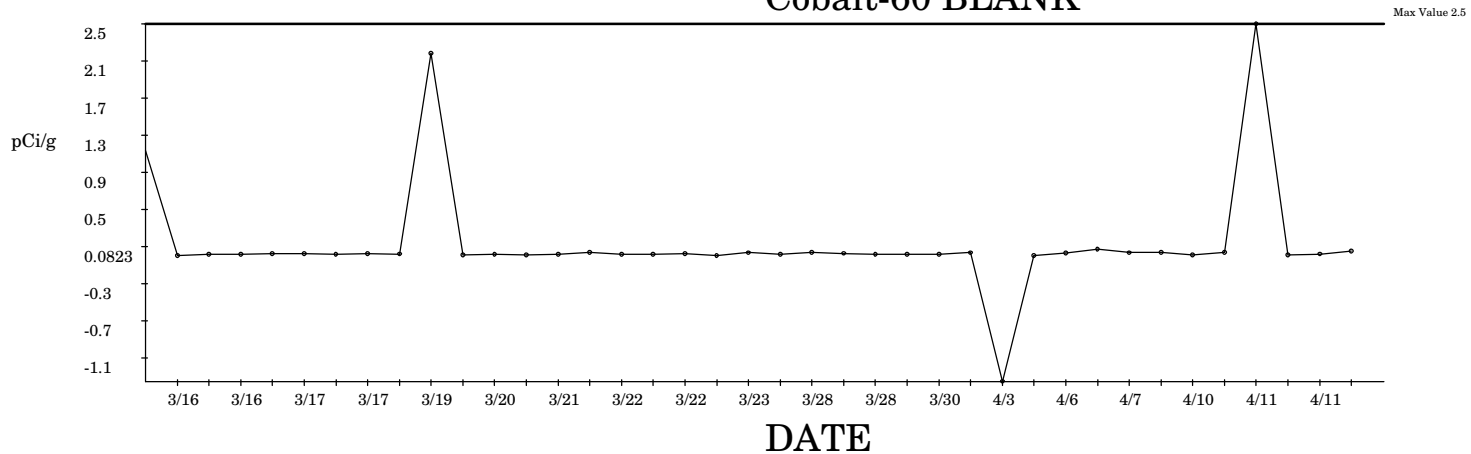


○ Denotes Outlier

SPC Graph for Gamma Spec in Solids 4/12/2006 Lead-212 RER




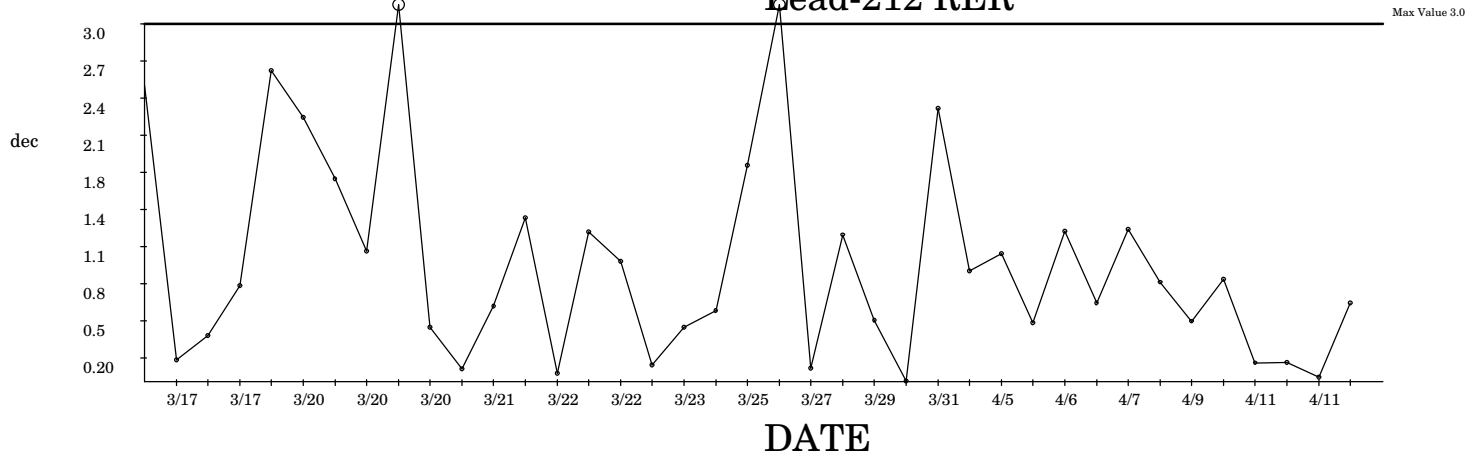


SPC Graph for Gamma Spec in Solids 4/12/2006 Radium-226 BLANK

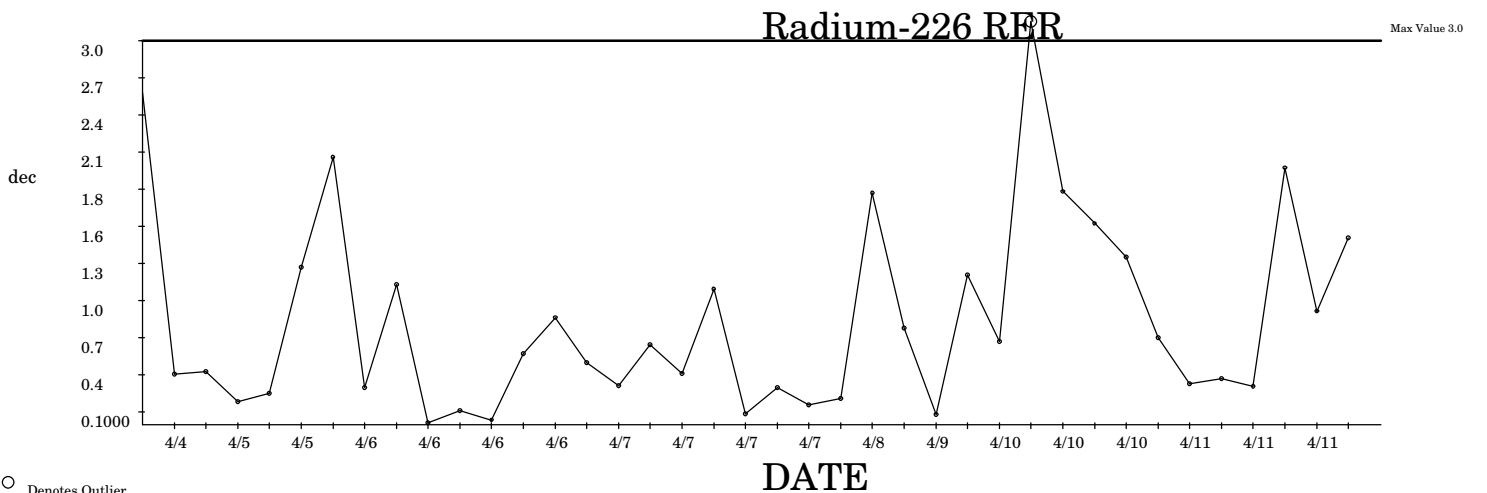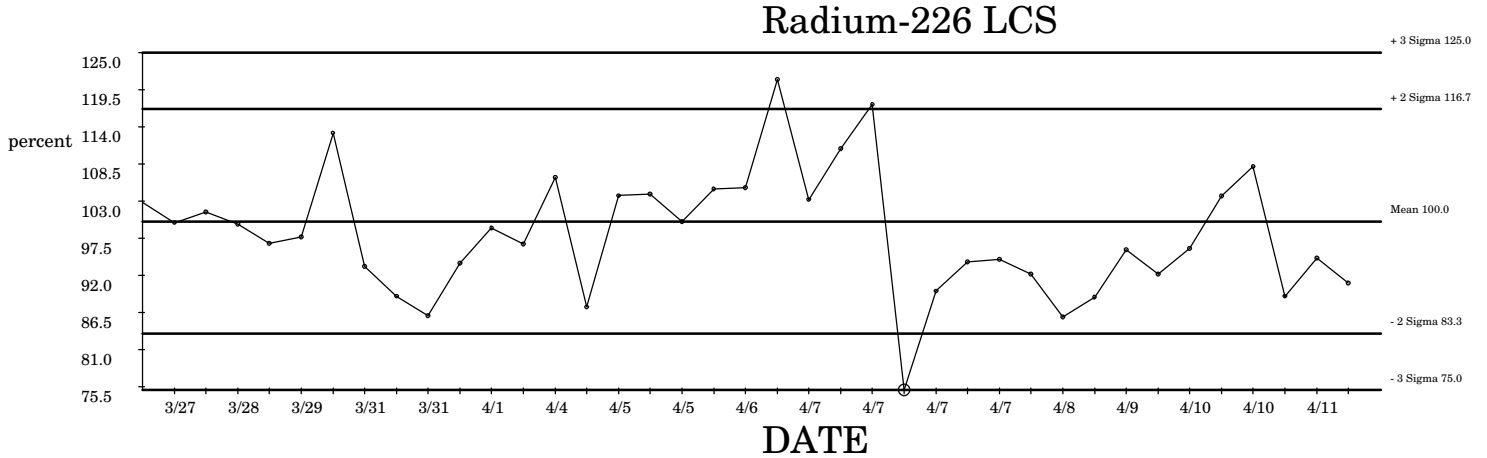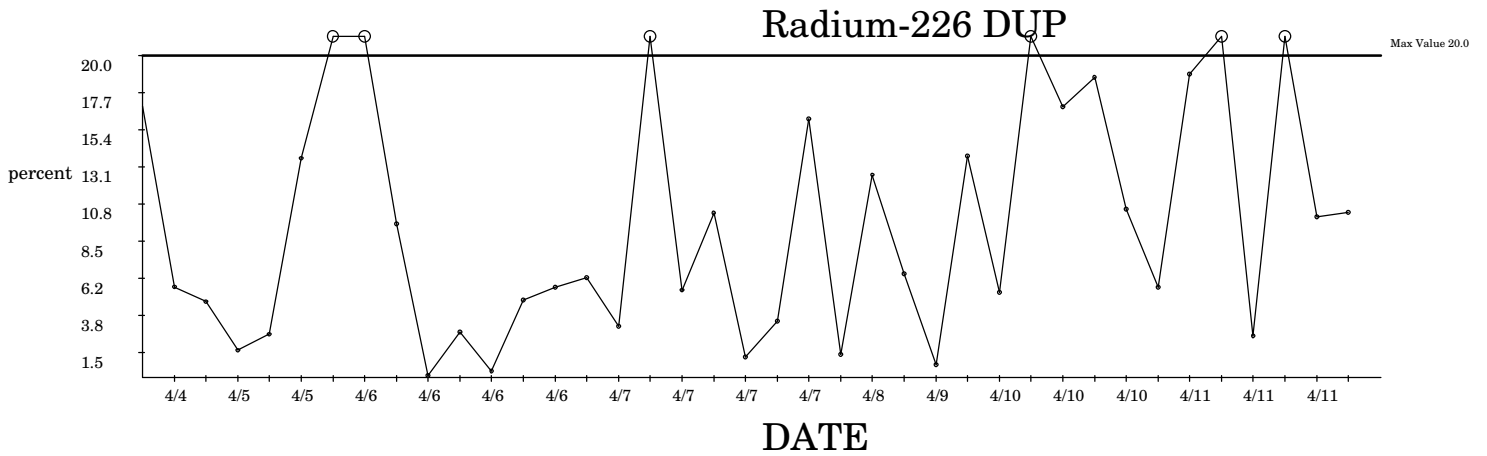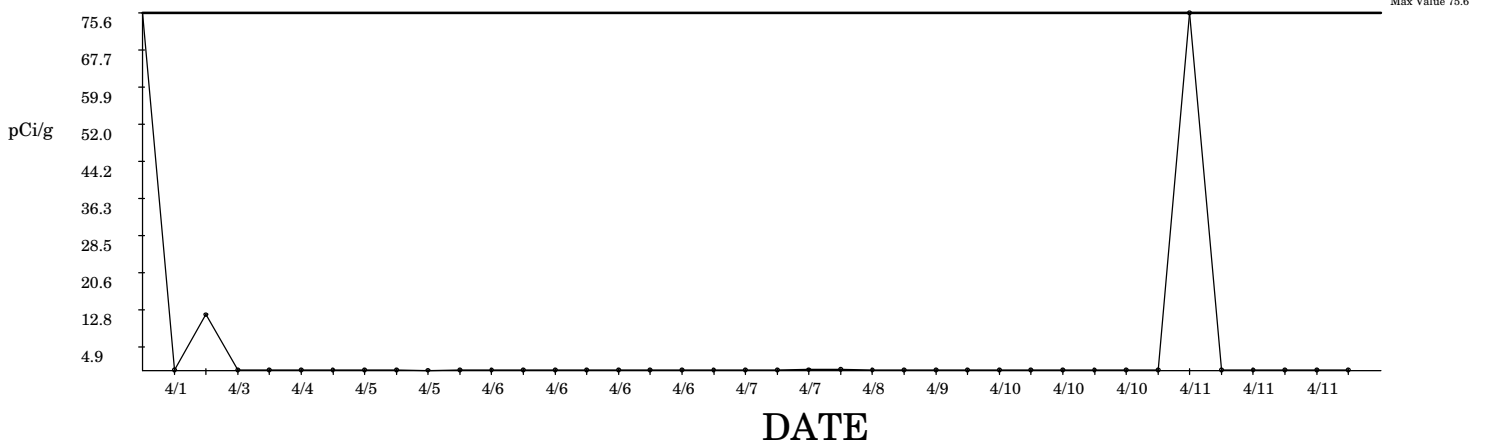

○ Denotes Outlier

SPC Graph for Gamma Spec in Solids 4/12/2006 Radium-228 BLANK

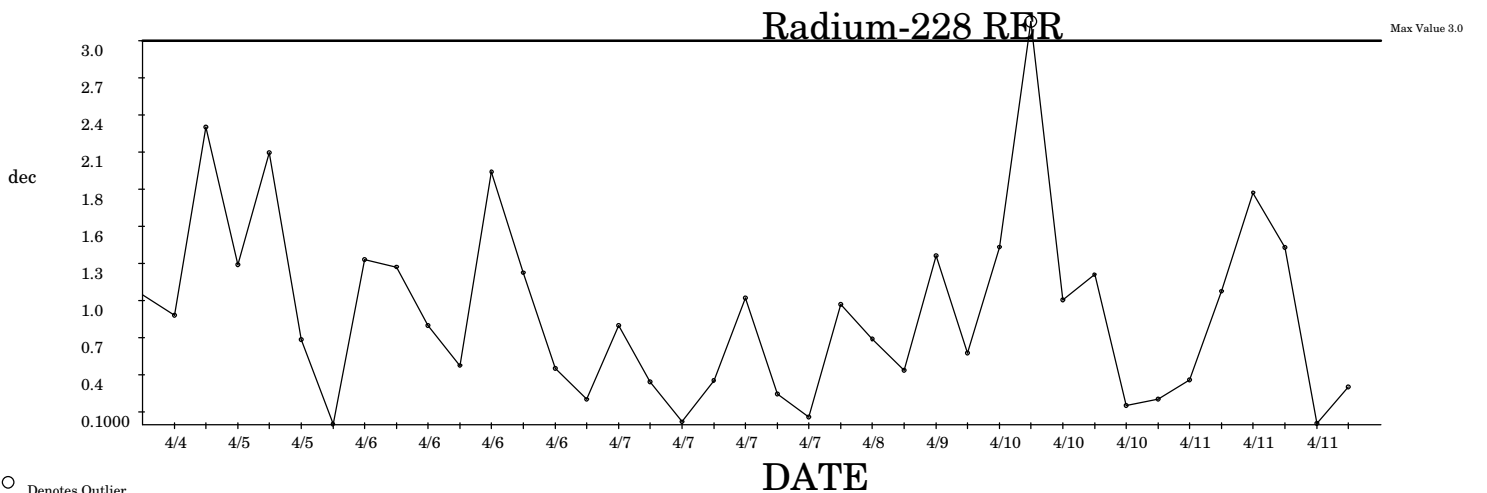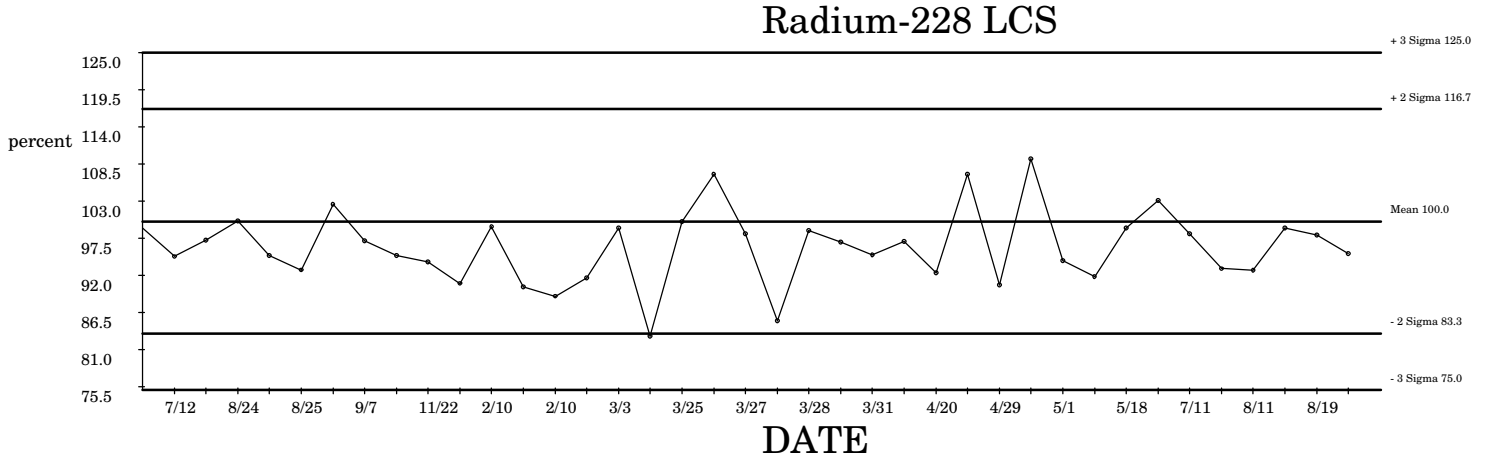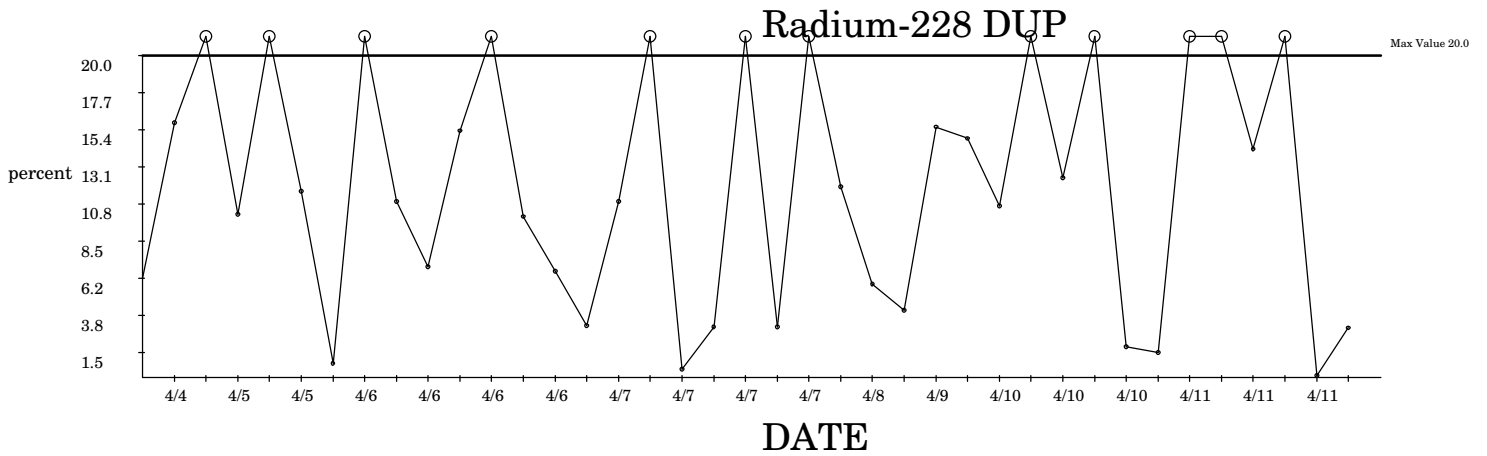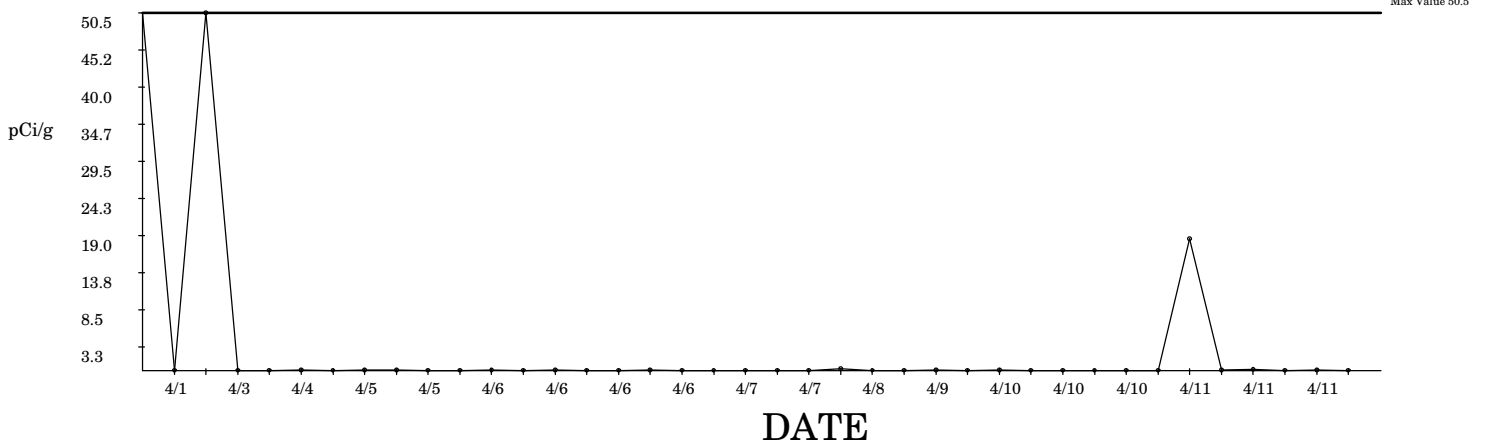

○ Denotes Outlier

Data used for Gamma Spec in Solids 13-APR-2006

Americium-241 LCS: Limits LCL = 75 UCL = 125

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
509664	1201046396	15-MAR-2006 07:07	DONE	106	0.74	percent	100	75.0	83.3	117	125	8.33
509666	1201046400	15-MAR-2006 08:15	DONE	100	0.01	percent	100	75.0	83.3	117	125	8.33
498916	1201021254	15-MAR-2006 10:52	DUSE	96	-0.53	percent	100	75.0	83.3	117	125	8.33
511947	1201051584	16-MAR-2006 03:52	DONE	98	-0.3	percent	100	75.0	83.3	117	125	8.33
507629	1201041705	16-MAR-2006 13:15	DONE	102	0.24	percent	100	75.0	83.3	117	125	8.33
507626	1201041699	16-MAR-2006 15:21	DONE	102	0.28	percent	100	75.0	83.3	117	125	8.33
507622	1201041689	17-MAR-2006 06:12	DUSE	111	1.3	percent	100	75.0	83.3	117	125	8.33
508637	1201044145	17-MAR-2006 07:42	DONE	104	0.5	percent	100	75.0	83.3	117	125	8.33
508605	1201044043	17-MAR-2006 09:19	DONE	102	0.28	percent	100	75.0	83.3	117	125	8.33
505207	1201035926	18-MAR-2006 13:44	DONE	115	1.8	percent	100	75.0	83.3	117	125	8.33
512599	1201053131	20-MAR-2006 06:21	DONE	99	-0.15	percent	100	75.0	83.3	117	125	8.33
512597	1201053125	20-MAR-2006 07:29	DONE	96	-0.46	percent	100	75.0	83.3	117	125	8.33
508903	1201044758	20-MAR-2006 14:37	DONE	108	0.95	percent	100	75.0	83.3	117	125	8.33
499544	1201022693	20-MAR-2006 19:52	DONE	97	-0.36	percent	100	75.0	83.3	117	125	8.33
512598	1201053128	20-MAR-2006 20:59	DONE	100	-0.04	percent	100	75.0	83.3	117	125	8.33
506206	1201055202	21-MAR-2006 17:35	DONE	96	-0.53	percent	100	75.0	83.3	117	125	8.33
509439	1201046013	22-MAR-2006 17:38	DUSE	104	0.43	percent	100	75.0	83.3	117	125	8.33
509445	1201046017	22-MAR-2006 17:56	DUSE	96	-0.54	percent	100	75.0	83.3	117	125	8.33
509577	1201046236	22-MAR-2006 22:50	DUSE	108	0.96	percent	100	75.0	83.3	117	125	8.33
509449	1201046024	23-MAR-2006 12:45	DUSE	95	-0.64	percent	100	75.0	83.3	117	125	8.33
509579	1201046243	25-MAR-2006 14:21	DUSE	90	-1	percent	100	75.0	83.3	117	125	8.33
498915	1201021245	26-MAR-2006 20:50	DUSE	103	0.41	percent	100	75.0	83.3	117	125	8.33
513814	1201055632	28-MAR-2006 04:36	DONE	103	0.36	percent	100	75.0	83.3	117	125	8.33
513815	1201055635	28-MAR-2006 20:48	DONE	106	0.77	percent	100	75.0	83.3	117	125	8.33
512778	1201053531	30-MAR-2006 09:25	DONE	104	0.48	percent	100	75.0	83.3	117	125	8.33
514959	1201058063	30-MAR-2006 14:51	DUSE	88	-1	percent	100	75.0	83.3	117	125	8.33
513797	1201055598	31-MAR-2006 06:06	DONE	91	-1	percent	100	75.0	83.3	117	125	8.33
512787	1201053543	04-APR-2006 09:03	DONE	103	0.34	percent	100	75.0	83.3	117	125	8.33
516236	1201060950	05-APR-2006 06:02	DUSE	91	-1	percent	100	75.0	83.3	117	125	8.33
513810	1201055629	06-APR-2006 08:46	DONE	104	0.48	percent	100	75.0	83.3	117	125	8.33
517045	1201062678	06-APR-2006 11:31	DONE	104	0.48	percent	100	75.0	83.3	117	125	8.33
517980	1201064811	06-APR-2006 12:37	DONE	102	0.22	percent	100	75.0	83.3	117	125	8.33
517983	1201064814	07-APR-2006 06:28	DONE	104	0.47	percent	100	75.0	83.3	117	125	8.33
513432	1201054907	08-APR-2006 20:51	DONE	91	-1	percent	100	75.0	83.3	117	125	8.33
513162	1201054361	09-APR-2006 21:18	DONE	105	0.61	percent	100	75.0	83.3	117	125	8.33
519008	1201067118	11-APR-2006 13:11	DUSE	95	-0.63	percent	100	75.0	83.3	117	125	8.33
513802	1201055609	11-APR-2006 14:31	DONE	103	0.37	percent	100	75.0	83.3	117	125	8.33
519499	1201068200	11-APR-2006 17:47	DUSE	94	-0.72	percent	100	75.0	83.3	117	125	8.33
518359	1201065661	11-APR-2006 20:04	DONE	99	-0.13	percent	100	75.0	83.3	117	125	8.33

Americium-241 RER: Limits LCL = 0 UCL = 3

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
509666	1201046399	16-MAR-2006 21:46	DONE	0.98	0.39	dec	0.79	0	-0.221	1.8	3.00	0.5
508605	1201044042	17-MAR-2006 00:39	DONE	0.43	-0.72	dec	0.79	0	-0.221	1.8	3.00	0.5
507622	1201041687	17-MAR-2006 00:40	DUSE	0.7	-0.18	dec	0.79	0	-0.221	1.8	3.00	0.5
508637	1201044144	17-MAR-2006 10:33	DONE	0.44	-0.69	dec	0.79	0	-0.221	1.8	3.00	0.5

498916	1201021255	20-MAR-2006 01:43	DUSE	0.08	-1	dec	0.79	0	-0.221	1.8	3.00	0.5
498916	1201021256	20-MAR-2006 01:43	DUSE	0.25	-1	dec	0.79	0	-0.221	1.8	3.00	0.5
512599	1201053130	20-MAR-2006 10:07	DONE	0.75	-0.08	dec	0.79	0	-0.221	1.8	3.00	0.5
508903	1201044757	20-MAR-2006 14:36	DONE	0.25	-1	dec	0.79	0	-0.221	1.8	3.00	0.5
505207	1201035925	20-MAR-2006 20:56	DONE	0.39	-0.79	dec	0.79	0	-0.221	1.8	3.00	0.5
512597	1201053124	20-MAR-2006 22:02	DONE	1.54	1.5	dec	0.79	0	-0.221	1.8	3.00	0.5
499544	1201022691	21-MAR-2006 05:31	DONE	1.17	0.76	dec	0.79	0	-0.221	1.8	3.00	0.5
512598	1201053127	21-MAR-2006 10:48	DONE	0.62	-0.33	dec	0.79	0	-0.221	1.8	3.00	0.5
506206	1201055201	21-MAR-2006 19:40	DONE	0.3	-0.96	dec	0.79	0	-0.221	1.8	3.00	0.5
498916	1201021257	22-MAR-2006 05:44	DUSE	1.92	2.3	dec	0.79	0	-0.221	1.8	3.00	0.5
509445	1201046016	22-MAR-2006 18:51	DUSE	1.01	0.44	dec	0.79	0	-0.221	1.8	3.00	0.5
509439	1201046012	22-MAR-2006 20:39	DUSE	0.67	-0.23	dec	0.79	0	-0.221	1.8	3.00	0.5
509577	1201046235	22-MAR-2006 22:31	DUSE	1.1	0.63	dec	0.79	0	-0.221	1.8	3.00	0.5
509449	1201046023	23-MAR-2006 05:27	DUSE	0.41	-0.75	dec	0.79	0	-0.221	1.8	3.00	0.5
498915	1201021243	24-MAR-2006 16:26	DUSE	1.41	1.2	dec	0.79	0	-0.221	1.8	3.00	0.5
509579	1201046242	25-MAR-2006 12:07	DUSE	1.08	0.59	dec	0.79	0	-0.221	1.8	3.00	0.5
498915	1201021246	26-MAR-2006 23:53	DUSE	0.97	0.36	dec	0.79	0	-0.221	1.8	3.00	0.5
513814	1201055631	27-MAR-2006 23:07	DONE	0.28	-1	dec	0.79	0	-0.221	1.8	3.00	0.5
513815	1201055634	28-MAR-2006 20:48	DONE	1.39	1.2	dec	0.79	0	-0.221	1.8	3.00	0.5
514959	1201058061	29-MAR-2006 12:17	DUSE	0.5	-0.57	dec	0.79	0	-0.221	1.8	3.00	0.5
512778	1201053530	30-MAR-2006 14:52	DONE	0.04	-1	dec	0.79	0	-0.221	1.8	3.00	0.5
513797	1201055597	31-MAR-2006 06:04	DONE	0.82	0.07	dec	0.79	0	-0.221	1.8	3.00	0.5
512787	1201053542	01-APR-2006 20:06	DONE	0.29	-0.98	dec	0.79	0	-0.221	1.8	3.00	0.5
517045	1201062677	05-APR-2006 22:28	DONE	1.03	0.48	dec	0.79	0	-0.221	1.8	3.00	0.5
516236	1201060949	06-APR-2006 06:01	DUSE	0.05	-1	dec	0.79	0	-0.221	1.8	3.00	0.5
513810	1201055628	06-APR-2006 10:52	DONE	1.09	0.59	dec	0.79	0	-0.221	1.8	3.00	0.5
517980	1201064809	07-APR-2006 06:16	DONE	1.93	2.3	dec	0.79	0	-0.221	1.8	3.00	0.5
517983	1201064813	07-APR-2006 06:28	DONE	0.88	0.19	dec	0.79	0	-0.221	1.8	3.00	0.5
513432	1201054906	07-APR-2006 21:54	DONE	0.92	0.27	dec	0.79	0	-0.221	1.8	3.00	0.5
513162	1201054360	09-APR-2006 21:34	DONE	0.53	-0.5	dec	0.79	0	-0.221	1.8	3.00	0.5
513799	1201055604	10-APR-2006 15:42	DUSE	0.7	-0.18	dec	0.79	0	-0.221	1.8	3.00	0.5
519499	1201068199	11-APR-2006 16:44	DUSE	1.6	1.6	dec	0.79	0	-0.221	1.8	3.00	0.5
519008	1201067117	11-APR-2006 19:22	DUSE	0.49	-0.6	dec	0.79	0	-0.221	1.8	3.00	0.5
518359	1201065660	11-APR-2006 21:47	DUSE	0.26	-1	dec	0.79	0	-0.221	1.8	3.00	0.5
513802	1201055608	11-APR-2006 23:19	DUSE	1.42	1.3	dec	0.79	0	-0.221	1.8	3.00	0.5

Cesium-137 BLANK: Limits LCL = -2.7 UCL = 2.5

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
512787	1201053541	01-APR-2006 20:05	DONE	0	0.12	pCi/g	-0.08	-2.7	-1.8	1.65	2.51	0.86
510153	1201047482	01-APR-2006 20:23	DUSE	0	0.09	pCi/g	-0.08	-2.7	-1.8	1.65	2.51	0.86
516236	1201060948	03-APR-2006 22:12	DONE	2	2.2	pCi/g	-0.08	-2.7	-1.8	1.65	2.51	0.86
510153	1201047482	03-APR-2006 23:22	DUSE	0	0.09	pCi/g	-0.08	-2.7	-1.8	1.65	2.51	0.86
510952	1201049298	04-APR-2006 01:43	DONE	0	0.09	pCi/g	-0.08	-2.7	-1.8	1.65	2.51	0.86
510881	1201049180	04-APR-2006 05:48	DONE	0	0.09	pCi/g	-0.08	-2.7	-1.8	1.65	2.51	0.86
516989	1201062554	05-APR-2006 08:18	DUSE	0	0.09	pCi/g	-0.08	-2.7	-1.8	1.65	2.51	0.86
508902	1201044753	05-APR-2006 09:43	DUSE	0	0.09	pCi/g	-0.08	-2.7	-1.8	1.65	2.51	0.86
508900	1201044747	05-APR-2006 17:35	DUSE	0	0.09	pCi/g	-0.08	-2.7	-1.8	1.65	2.51	0.86
517983	1201064812	05-APR-2006 18:28	DONE	0	0.1	pCi/g	-0.08	-2.7	-1.8	1.65	2.51	0.86
516986	1201062545	06-APR-2006 08:33	DUSE	0	0.09	pCi/g	-0.08	-2.7	-1.8	1.65	2.51	0.86
513810	1201055627	06-APR-2006 09:43	DONE	0	0.09	pCi/g	-0.08	-2.7	-1.8	1.65	2.51	0.86

516987	1201062548	06-APR-2006 10:43	DUSE	0	0.09	pCi/g	-0.08	-2.7	-1.8	1.65	2.51	0.86
517045	1201062676	06-APR-2006 10:56	DONE	0	0.1	pCi/g	-0.08	-2.7	-1.8	1.65	2.51	0.86
516991	1201062560	06-APR-2006 11:51	DUSE	0	0.09	pCi/g	-0.08	-2.7	-1.8	1.65	2.51	0.86
516993	1201062566	06-APR-2006 16:35	DUSE	0	0.09	pCi/g	-0.08	-2.7	-1.8	1.65	2.51	0.86
510982	1201049354	06-APR-2006 16:39	DONE	0	0.09	pCi/g	-0.08	-2.7	-1.8	1.65	2.51	0.86
510976	1201049346	06-APR-2006 18:46	DUSE	0	0.09	pCi/g	-0.08	-2.7	-1.8	1.65	2.51	0.86
516996	1201062572	07-APR-2006 06:08	DUSE	0	0.09	pCi/g	-0.08	-2.7	-1.8	1.65	2.51	0.86
516999	1201062578	07-APR-2006 08:19	DUSE	0	0.09	pCi/g	-0.08	-2.7	-1.8	1.65	2.51	0.86
511760	1201051194	07-APR-2006 10:19	DONE	0	0.09	pCi/g	-0.08	-2.7	-1.8	1.65	2.51	0.86
517980	1201064808	07-APR-2006 14:52	DONE	0	0.19	pCi/g	-0.08	-2.7	-1.8	1.65	2.51	0.86
513432	1201054905	07-APR-2006 17:03	DONE	0	0.08	pCi/g	-0.08	-2.7	-1.8	1.65	2.51	0.86
517004	1201062584	08-APR-2006 16:03	DUSE	0	0.09	pCi/g	-0.08	-2.7	-1.8	1.65	2.51	0.86
517006	1201062590	08-APR-2006 21:37	DONE	0	0.09	pCi/g	-0.08	-2.7	-1.8	1.65	2.51	0.86
517018	1201062614	09-APR-2006 21:09	DUSE	0	0.09	pCi/g	-0.08	-2.7	-1.8	1.65	2.51	0.86
517011	1201062602	10-APR-2006 06:23	DONE	0	0.09	pCi/g	-0.08	-2.7	-1.8	1.65	2.51	0.86
513162	1201054359	10-APR-2006 06:36	DONE	0	0.09	pCi/g	-0.08	-2.7	-1.8	1.65	2.51	0.86
517009	1201062596	10-APR-2006 10:47	DONE	0	0.09	pCi/g	-0.08	-2.7	-1.8	1.65	2.51	0.86
513799	1201055603	10-APR-2006 11:17	DUSE	0	0.12	pCi/g	-0.08	-2.7	-1.8	1.65	2.51	0.86
517015	1201062608	10-APR-2006 13:00	DUSE	0	0.09	pCi/g	-0.08	-2.7	-1.8	1.65	2.51	0.86
512595	1201053117	10-APR-2006 13:17	DONE	0	0.09	pCi/g	-0.08	-2.7	-1.8	1.65	2.51	0.86
513054	1201054080	11-APR-2006 11:51	DUSE	0	0.09	pCi/g	-0.08	-2.7	-1.8	1.65	2.51	0.86
519499	1201068198	11-APR-2006 14:26	DONE	-5	-6	pCi/g	-0.08	-2.7	-1.8	1.65	2.51	0.86
519008	1201067116	11-APR-2006 18:52	DONE	0	0.09	pCi/g	-0.08	-2.7	-1.8	1.65	2.51	0.86
518359	1201065659	11-APR-2006 18:53	DONE	0	0.11	pCi/g	-0.08	-2.7	-1.8	1.65	2.51	0.86
513058	1201054086	11-APR-2006 21:43	DUSE	0	0.09	pCi/g	-0.08	-2.7	-1.8	1.65	2.51	0.86
513802	1201055607	11-APR-2006 23:19	DUSE	0	0.1	pCi/g	-0.08	-2.7	-1.8	1.65	2.51	0.86
513780	1201055549	11-APR-2006 23:45	DUSE	0	0.09	pCi/g	-0.08	-2.7	-1.8	1.65	2.51	0.86

Cesium-137 DUP: Limits LCL = 0 UCL = 20

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
513797	1201055597	31-MAR-2006 06:04	DONE	369	3.3	percent	38.2	0	-160	238	20.0	99.9
510133	1201047438	31-MAR-2006 09:54	DONE	0	-0.38	percent	38.2	0	-160	238	20.0	99.9
510151	1201047469	01-APR-2006 17:56	DONE	0	-0.38	percent	38.2	0	-160	238	20.0	99.9
510153	1201047483	01-APR-2006 20:23	DUSE	0	-0.38	percent	38.2	0	-160	238	20.0	99.9
510153	1201047483	03-APR-2006 23:01	DUSE	0	-0.38	percent	38.2	0	-160	238	20.0	99.9
510952	1201049299	04-APR-2006 01:41	DONE	0	-0.38	percent	38.2	0	-160	238	20.0	99.9
510881	1201049181	04-APR-2006 06:40	DONE	0	-0.38	percent	38.2	0	-160	238	20.0	99.9
510153	1201047483	04-APR-2006 07:57	DUSE	0	-0.38	percent	38.2	0	-160	238	20.0	99.9
516989	1201062555	05-APR-2006 08:18	DUSE	26	-0.12	percent	38.2	0	-160	238	20.0	99.9
508902	1201044754	05-APR-2006 09:43	DUSE	0	-0.38	percent	38.2	0	-160	238	20.0	99.9
508900	1201044748	05-APR-2006 17:36	DUSE	0	-0.38	percent	38.2	0	-160	238	20.0	99.9
517045	1201062677	05-APR-2006 22:28	DONE	31	-0.07	percent	38.2	0	-160	238	20.0	99.9
516236	1201060949	06-APR-2006 06:01	DONE	8	-0.3	percent	38.2	0	-160	238	20.0	99.9
513810	1201055628	06-APR-2006 10:52	DONE	248	2.1	percent	38.2	0	-160	238	20.0	99.9
516991	1201062561	06-APR-2006 12:45	DUSE	0	-0.38	percent	38.2	0	-160	238	20.0	99.9
516993	1201062567	06-APR-2006 16:35	DUSE	0	-0.38	percent	38.2	0	-160	238	20.0	99.9
516996	1201062573	07-APR-2006 06:09	DUSE	0	-0.38	percent	38.2	0	-160	238	20.0	99.9
517980	1201064809	07-APR-2006 06:16	DONE	2	-0.37	percent	38.2	0	-160	238	20.0	99.9
517983	1201064813	07-APR-2006 06:28	DONE	3	-0.35	percent	38.2	0	-160	238	20.0	99.9
511760	1201051195	07-APR-2006 10:20	DONE	0	-0.38	percent	38.2	0	-160	238	20.0	99.9

516996	1201062573	07-APR-2006 10:31	DUSE	0	-0.38	percent	38.2	0	-160	238	20.0	99.9
513432	1201054906	07-APR-2006 21:54	DONE	359	3.2	percent	38.2	0	-160	238	20.0	99.9
510976	1201049347	07-APR-2006 22:28	DUSE	0	-0.38	percent	38.2	0	-160	238	20.0	99.9
517004	1201062585	08-APR-2006 16:02	DUSE	0	-0.38	percent	38.2	0	-160	238	20.0	99.9
517006	1201062591	08-APR-2006 21:38	DONE	0	-0.38	percent	38.2	0	-160	238	20.0	99.9
517018	1201062615	09-APR-2006 21:10	DUSE	0	-0.38	percent	38.2	0	-160	238	20.0	99.9
513162	1201054360	09-APR-2006 21:34	DONE	6	-0.32	percent	38.2	0	-160	238	20.0	99.9
517011	1201062603	10-APR-2006 06:23	DONE	0	-0.38	percent	38.2	0	-160	238	20.0	99.9
517009	1201062597	10-APR-2006 10:48	DONE	0	-0.38	percent	38.2	0	-160	238	20.0	99.9
517015	1201062609	10-APR-2006 10:51	DUSE	0	-0.38	percent	38.2	0	-160	238	20.0	99.9
512595	1201053118	10-APR-2006 13:18	DONE	0	-0.38	percent	38.2	0	-160	238	20.0	99.9
513799	1201055604	10-APR-2006 15:42	DUSE	137	0.99	percent	38.2	0	-160	238	20.0	99.9
513054	1201054081	11-APR-2006 10:21	DUSE	0	-0.38	percent	38.2	0	-160	238	20.0	99.9
519499	1201068199	11-APR-2006 16:44	DONE	2	-0.37	percent	38.2	0	-160	238	20.0	99.9
519008	1201067117	11-APR-2006 19:22	DONE	0	-0.38	percent	38.2	0	-160	238	20.0	99.9
513058	1201054087	11-APR-2006 21:43	DUSE	0	-0.38	percent	38.2	0	-160	238	20.0	99.9
518359	1201065660	11-APR-2006 21:47	DONE	0	-0.38	percent	38.2	0	-160	238	20.0	99.9
513802	1201055608	11-APR-2006 23:19	DUSE	298	2.6	percent	38.2	0	-160	238	20.0	99.9
513780	1201055550	11-APR-2006 23:45	DUSE	0	-0.38	percent	38.2	0	-160	238	20.0	99.9

Cesium-137 LCS: Limits LCL = 75 UCL = 125

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
509664	1201046396	15-MAR-2006 07:07	DONE	110	1.1	percent	100	75.0	83.3	117	125	8.33
509666	1201046400	15-MAR-2006 08:15	DONE	106	0.76	percent	100	75.0	83.3	117	125	8.33
498916	1201021254	15-MAR-2006 10:52	DONE	105	0.58	percent	100	75.0	83.3	117	125	8.33
511947	1201051584	16-MAR-2006 03:52	DONE	91	-1	percent	100	75.0	83.3	117	125	8.33
507629	1201041705	16-MAR-2006 13:15	DONE	112	1.4	percent	100	75.0	83.3	117	125	8.33
507626	1201041699	16-MAR-2006 15:21	DONE	110	1.2	percent	100	75.0	83.3	117	125	8.33
507622	1201041689	17-MAR-2006 06:12	DONE	102	0.28	percent	100	75.0	83.3	117	125	8.33
508637	1201044145	17-MAR-2006 07:42	DONE	105	0.56	percent	100	75.0	83.3	117	125	8.33
508605	1201044043	17-MAR-2006 09:19	DONE	95	-0.61	percent	100	75.0	83.3	117	125	8.33
505207	1201035926	18-MAR-2006 13:44	DONE	103	0.31	percent	100	75.0	83.3	117	125	8.33
512599	1201053131	20-MAR-2006 06:21	DONE	108	0.9	percent	100	75.0	83.3	117	125	8.33
512597	1201053125	20-MAR-2006 07:29	DONE	109	1	percent	100	75.0	83.3	117	125	8.33
508903	1201044758	20-MAR-2006 14:37	DONE	104	0.48	percent	100	75.0	83.3	117	125	8.33
499544	1201022693	20-MAR-2006 19:52	DONE	110	1.2	percent	100	75.0	83.3	117	125	8.33
512598	1201053128	20-MAR-2006 20:59	DONE	98	-0.25	percent	100	75.0	83.3	117	125	8.33
506206	1201055202	21-MAR-2006 17:35	DONE	106	0.66	percent	100	75.0	83.3	117	125	8.33
509439	1201046013	22-MAR-2006 17:38	DONE	108	0.91	percent	100	75.0	83.3	117	125	8.33
509445	1201046017	22-MAR-2006 17:56	DONE	99	-0.08	percent	100	75.0	83.3	117	125	8.33
509577	1201046236	22-MAR-2006 22:50	DONE	110	1.2	percent	100	75.0	83.3	117	125	8.33
509449	1201046024	23-MAR-2006 12:45	DONE	104	0.49	percent	100	75.0	83.3	117	125	8.33
509579	1201046243	25-MAR-2006 14:21	DONE	105	0.6	percent	100	75.0	83.3	117	125	8.33
498915	1201021245	26-MAR-2006 20:50	DONE	100	-0.01	percent	100	75.0	83.3	117	125	8.33
513814	1201055632	28-MAR-2006 04:36	DONE	109	1.1	percent	100	75.0	83.3	117	125	8.33
513815	1201055635	28-MAR-2006 20:48	DONE	109	1	percent	100	75.0	83.3	117	125	8.33
512778	1201053531	30-MAR-2006 09:25	DONE	110	1.2	percent	100	75.0	83.3	117	125	8.33
514959	1201058063	30-MAR-2006 14:51	DONE	97	-0.42	percent	100	75.0	83.3	117	125	8.33
513797	1201055598	31-MAR-2006 06:06	DONE	97	-0.37	percent	100	75.0	83.3	117	125	8.33
512787	1201053543	04-APR-2006 09:03	DONE	109	1.1	percent	100	75.0	83.3	117	125	8.33

516236	1201060950	05-APR-2006 06:02	DONE	88	-1	percent	100	75.0	83.3	117	125	8.33
513810	1201055629	06-APR-2006 08:46	DONE	107	0.84	percent	100	75.0	83.3	117	125	8.33
517045	1201062678	06-APR-2006 11:31	DONE	105	0.6	percent	100	75.0	83.3	117	125	8.33
517980	1201064811	06-APR-2006 12:37	DONE	110	1.1	percent	100	75.0	83.3	117	125	8.33
517983	1201064814	07-APR-2006 06:28	DONE	113	1.5	percent	100	75.0	83.3	117	125	8.33
513432	1201054907	08-APR-2006 20:51	DONE	93	-0.89	percent	100	75.0	83.3	117	125	8.33
513162	1201054361	09-APR-2006 21:18	DONE	110	1.1	percent	100	75.0	83.3	117	125	8.33
519008	1201067118	11-APR-2006 13:11	DONE	103	0.41	percent	100	75.0	83.3	117	125	8.33
513802	1201055609	11-APR-2006 14:31	DONE	104	0.46	percent	100	75.0	83.3	117	125	8.33
519499	1201068200	11-APR-2006 17:47	DONE	91	-1	percent	100	75.0	83.3	117	125	8.33
518359	1201065661	11-APR-2006 20:04	DONE	116	1.9	percent	100	75.0	83.3	117	125	8.33

Cesium-137 RER: Limits LCL = 0 UCL = 3

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
498915	1201021246	26-MAR-2006 23:53	DONE	5.16	1.9	dec	1.32	0	-2.7	5.37	3.00	2.02
508865	1201044688	27-MAR-2006 20:50	DONE	0	-0.65	dec	1.32	0	-2.7	5.37	3.00	2.02
513785	1201055565	27-MAR-2006 21:18	DONE	0	-0.65	dec	1.32	0	-2.7	5.37	3.00	2.02
513814	1201055631	27-MAR-2006 23:07	DONE	8.84	3.7	dec	1.32	0	-2.7	5.37	3.00	2.02
515289	1201058837	28-MAR-2006 10:16	DUSE	1.43	0.06	dec	1.32	0	-2.7	5.37	3.00	2.02
513815	1201055634	28-MAR-2006 20:48	DONE	1.54	0.11	dec	1.32	0	-2.7	5.37	3.00	2.02
514959	1201058061	29-MAR-2006 12:17	DONE	1.88	0.28	dec	1.32	0	-2.7	5.37	3.00	2.02
512778	1201053530	30-MAR-2006 14:52	DONE	0.01	-0.65	dec	1.32	0	-2.7	5.37	3.00	2.02
510114	1201047413	30-MAR-2006 21:20	DONE	0	-0.65	dec	1.32	0	-2.7	5.37	3.00	2.02
513797	1201055597	31-MAR-2006 06:04	DONE	0.69	-0.31	dec	1.32	0	-2.7	5.37	3.00	2.02
510133	1201047438	31-MAR-2006 09:54	DONE	0	-0.65	dec	1.32	0	-2.7	5.37	3.00	2.02
510144	1201047451	31-MAR-2006 18:41	DONE	2.06	0.37	dec	1.32	0	-2.7	5.37	3.00	2.02
510151	1201047469	01-APR-2006 17:56	DONE	0	-0.65	dec	1.32	0	-2.7	5.37	3.00	2.02
512787	1201053542	01-APR-2006 20:06	DONE	0.4	-0.45	dec	1.32	0	-2.7	5.37	3.00	2.02
510952	1201049299	04-APR-2006 01:41	DONE	0	-0.65	dec	1.32	0	-2.7	5.37	3.00	2.02
510881	1201049181	04-APR-2006 06:40	DONE	0	-0.65	dec	1.32	0	-2.7	5.37	3.00	2.02
516989	1201062555	05-APR-2006 08:18	DUSE	0.81	-0.25	dec	1.32	0	-2.7	5.37	3.00	2.02
517045	1201062677	05-APR-2006 22:28	DONE	2.01	0.34	dec	1.32	0	-2.7	5.37	3.00	2.02
516236	1201060949	06-APR-2006 06:01	DONE	8.48	3.5	dec	1.32	0	-2.7	5.37	3.00	2.02
516986	1201062546	06-APR-2006 08:33	DUSE	1.98	0.33	dec	1.32	0	-2.7	5.37	3.00	2.02
516987	1201062549	06-APR-2006 10:43	DUSE	2.05	0.36	dec	1.32	0	-2.7	5.37	3.00	2.02
513810	1201055628	06-APR-2006 10:52	DONE	0.82	-0.24	dec	1.32	0	-2.7	5.37	3.00	2.02
510976	1201049347	06-APR-2006 18:47	DUSE	2.51	0.59	dec	1.32	0	-2.7	5.37	3.00	2.02
510982	1201049355	06-APR-2006 18:47	DONE	1.69	0.18	dec	1.32	0	-2.7	5.37	3.00	2.02
517980	1201064809	07-APR-2006 06:16	DONE	0.31	-0.5	dec	1.32	0	-2.7	5.37	3.00	2.02
517983	1201064813	07-APR-2006 06:28	DONE	0.59	-0.36	dec	1.32	0	-2.7	5.37	3.00	2.02
516999	1201062579	07-APR-2006 08:20	DUSE	1.81	0.24	dec	1.32	0	-2.7	5.37	3.00	2.02
511760	1201051195	07-APR-2006 10:20	DONE	0	-0.65	dec	1.32	0	-2.7	5.37	3.00	2.02
513432	1201054906	07-APR-2006 21:54	DONE	0.89	-0.21	dec	1.32	0	-2.7	5.37	3.00	2.02
517006	1201062591	08-APR-2006 21:38	DONE	0	-0.65	dec	1.32	0	-2.7	5.37	3.00	2.02
513162	1201054360	09-APR-2006 21:34	DONE	0.35	-0.48	dec	1.32	0	-2.7	5.37	3.00	2.02
517011	1201062603	10-APR-2006 06:23	DONE	1.11	-0.11	dec	1.32	0	-2.7	5.37	3.00	2.02
517009	1201062597	10-APR-2006 10:48	DONE	0	-0.65	dec	1.32	0	-2.7	5.37	3.00	2.02
512595	1201053118	10-APR-2006 13:18	DONE	0	-0.65	dec	1.32	0	-2.7	5.37	3.00	2.02
513799	1201055604	10-APR-2006 15:42	DUSE	0.48	-0.41	dec	1.32	0	-2.7	5.37	3.00	2.02
519499	1201068199	11-APR-2006 16:44	DONE	0.46	-0.42	dec	1.32	0	-2.7	5.37	3.00	2.02

519008	1201067117	11-APR-2006 19:22	DONE	1.88	0.28	dec	1.32	0	-2.7	5.37	3.00	2.02
518359	1201065660	11-APR-2006 21:47	DONE	0.01	-0.65	dec	1.32	0	-2.7	5.37	3.00	2.02
513802	1201055608	11-APR-2006 23:19	DUSE	1.16	-0.08	dec	1.32	0	-2.7	5.37	3.00	2.02

Cobalt-60 BLANK: Limits LCL = -1.6 UCL = 1.8

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
509664	1201046394	15-MAR-2006 22:41	DONE	0	-0.16	pCi/g	0.09	-1.6	-1	1.22	1.79	0.57
507629	1201041703	16-MAR-2006 13:14	DONE	0	-0.18	pCi/g	0.09	-1.6	-1	1.22	1.79	0.57
507626	1201041697	16-MAR-2006 15:21	DONE	0	-0.15	pCi/g	0.09	-1.6	-1	1.22	1.79	0.57
509666	1201046398	16-MAR-2006 21:46	DONE	0	-0.16	pCi/g	0.09	-1.6	-1	1.22	1.79	0.57
508605	1201044041	17-MAR-2006 00:38	DONE	0	-0.15	pCi/g	0.09	-1.6	-1	1.22	1.79	0.57
507622	1201041686	17-MAR-2006 00:40	DONE	0	-0.14	pCi/g	0.09	-1.6	-1	1.22	1.79	0.57
508637	1201044143	17-MAR-2006 08:21	DONE	0	-0.16	pCi/g	0.09	-1.6	-1	1.22	1.79	0.57
508903	1201044756	17-MAR-2006 22:59	DONE	0	-0.14	pCi/g	0.09	-1.6	-1	1.22	1.79	0.57
505207	1201035924	18-MAR-2006 00:57	DONE	0	-0.15	pCi/g	0.09	-1.6	-1	1.22	1.79	0.57
498916	1201021252	19-MAR-2006 18:01	DONE	2	3.6	pCi/g	0.09	-1.6	-1	1.22	1.79	0.57
512599	1201053129	20-MAR-2006 10:06	DONE	0	-0.17	pCi/g	0.09	-1.6	-1	1.22	1.79	0.57
512597	1201053123	20-MAR-2006 19:22	DONE	0	-0.16	pCi/g	0.09	-1.6	-1	1.22	1.79	0.57
499544	1201022690	20-MAR-2006 21:27	DONE	0	-0.16	pCi/g	0.09	-1.6	-1	1.22	1.79	0.57
512598	1201053126	21-MAR-2006 12:16	DONE	0	-0.16	pCi/g	0.09	-1.6	-1	1.22	1.79	0.57
506206	1201055200	21-MAR-2006 15:02	DONE	0	-0.12	pCi/g	0.09	-1.6	-1	1.22	1.79	0.57
509445	1201046015	22-MAR-2006 16:50	DUSE	0	-0.16	pCi/g	0.09	-1.6	-1	1.22	1.79	0.57
509439	1201046011	22-MAR-2006 17:38	DONE	0	-0.16	pCi/g	0.09	-1.6	-1	1.22	1.79	0.57
509449	1201046022	22-MAR-2006 20:37	DUSE	0	-0.14	pCi/g	0.09	-1.6	-1	1.22	1.79	0.57
509577	1201046234	22-MAR-2006 22:47	DONE	0	-0.18	pCi/g	0.09	-1.6	-1	1.22	1.79	0.57
498915	1201021242	23-MAR-2006 10:30	DONE	0	-0.13	pCi/g	0.09	-1.6	-1	1.22	1.79	0.57
509579	1201046241	25-MAR-2006 12:07	DUSE	0	-0.16	pCi/g	0.09	-1.6	-1	1.22	1.79	0.57
513814	1201055630	28-MAR-2006 06:09	DONE	0	-0.12	pCi/g	0.09	-1.6	-1	1.22	1.79	0.57
513815	1201055633	28-MAR-2006 20:47	DONE	0	-0.14	pCi/g	0.09	-1.6	-1	1.22	1.79	0.57
514959	1201058060	28-MAR-2006 22:16	DONE	0	-0.15	pCi/g	0.09	-1.6	-1	1.22	1.79	0.57
512778	1201053529	30-MAR-2006 14:51	DONE	0	-0.15	pCi/g	0.09	-1.6	-1	1.22	1.79	0.57
513797	1201055596	30-MAR-2006 23:40	DONE	0	-0.16	pCi/g	0.09	-1.6	-1	1.22	1.79	0.57
512787	1201053541	01-APR-2006 20:05	DONE	0	-0.13	pCi/g	0.09	-1.6	-1	1.22	1.79	0.57
516236	1201060948	03-APR-2006 22:12	DONE	-1	-3	pCi/g	0.09	-1.6	-1	1.22	1.79	0.57
517983	1201064812	05-APR-2006 18:28	DONE	0	-0.18	pCi/g	0.09	-1.6	-1	1.22	1.79	0.57
513810	1201055627	06-APR-2006 09:43	DONE	0	-0.13	pCi/g	0.09	-1.6	-1	1.22	1.79	0.57
517045	1201062676	06-APR-2006 10:56	DONE	0	-0.06	pCi/g	0.09	-1.6	-1	1.22	1.79	0.57
517980	1201064808	07-APR-2006 14:52	DONE	0	-0.13	pCi/g	0.09	-1.6	-1	1.22	1.79	0.57
513432	1201054905	07-APR-2006 17:03	DONE	0	-0.12	pCi/g	0.09	-1.6	-1	1.22	1.79	0.57
513162	1201054359	10-APR-2006 06:36	DONE	0	-0.17	pCi/g	0.09	-1.6	-1	1.22	1.79	0.57
513799	1201055603	10-APR-2006 11:17	DUSE	0	-0.12	pCi/g	0.09	-1.6	-1	1.22	1.79	0.57
519499	1201068198	11-APR-2006 14:26	DONE	2	4.2	pCi/g	0.09	-1.6	-1	1.22	1.79	0.57
519008	1201067116	11-APR-2006 18:52	DUSE	0	-0.16	pCi/g	0.09	-1.6	-1	1.22	1.79	0.57
518359	1201065659	11-APR-2006 18:53	DUSE	0	-0.15	pCi/g	0.09	-1.6	-1	1.22	1.79	0.57
513802	1201055607	11-APR-2006 23:19	DUSE	0	-0.1	pCi/g	0.09	-1.6	-1	1.22	1.79	0.57

Cobalt-60 DUP: Limits LCL = 0 UCL = 20

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
507626	1201041698	16-MAR-2006 15:21	DONE	16	-0.38	percent	297	0	-1200	1790	20.0	745
509666	1201046399	16-MAR-2006 21:46	DONE	6	-0.39	percent	297	0	-1200	1790	20.0	745

508605	1201044042	17-MAR-2006 00:39	DONE	2	-0.4	percent	297	0	-1200	1790	20.0	745
507622	1201041687	17-MAR-2006 00:40	DONE	599	0.4	percent	297	0	-1200	1790	20.0	745
508637	1201044144	17-MAR-2006 10:33	DONE	1	-0.4	percent	297	0	-1200	1790	20.0	745
498916	1201021255	20-MAR-2006 01:43	DONE	2	-0.4	percent	297	0	-1200	1790	20.0	745
498916	1201021256	20-MAR-2006 01:43	DONE	4	-0.39	percent	297	0	-1200	1790	20.0	745
512599	1201053130	20-MAR-2006 10:07	DONE	175	-0.16	percent	297	0	-1200	1790	20.0	745
508903	1201044757	20-MAR-2006 14:36	DONE	4264	5.3	percent	297	0	-1200	1790	20.0	745
505207	1201035925	20-MAR-2006 20:56	DONE	60	-0.32	percent	297	0	-1200	1790	20.0	745
512597	1201053124	20-MAR-2006 22:02	DONE	4	-0.39	percent	297	0	-1200	1790	20.0	745
499544	1201022691	21-MAR-2006 05:31	DONE	1088	1.1	percent	297	0	-1200	1790	20.0	745
512598	1201053127	21-MAR-2006 10:48	DONE	23	-0.37	percent	297	0	-1200	1790	20.0	745
506206	1201055201	21-MAR-2006 19:40	DONE	470	0.23	percent	297	0	-1200	1790	20.0	745
498916	1201021257	22-MAR-2006 05:44	DONE	0	-0.4	percent	297	0	-1200	1790	20.0	745
509445	1201046016	22-MAR-2006 18:51	DUSE	1773	2	percent	297	0	-1200	1790	20.0	745
509439	1201046012	22-MAR-2006 20:39	DONE	0	-0.4	percent	297	0	-1200	1790	20.0	745
509577	1201046235	22-MAR-2006 22:31	DONE	0	-0.4	percent	297	0	-1200	1790	20.0	745
509449	1201046023	23-MAR-2006 05:27	DUSE	390	0.12	percent	297	0	-1200	1790	20.0	745
498915	1201021243	24-MAR-2006 16:26	DONE	2	-0.4	percent	297	0	-1200	1790	20.0	745
509579	1201046242	25-MAR-2006 12:07	DUSE	56	-0.32	percent	297	0	-1200	1790	20.0	745
498915	1201021246	26-MAR-2006 23:53	DONE	6	-0.39	percent	297	0	-1200	1790	20.0	745
513814	1201055631	27-MAR-2006 23:07	DONE	5	-0.39	percent	297	0	-1200	1790	20.0	745
513815	1201055634	28-MAR-2006 20:48	DONE	25	-0.36	percent	297	0	-1200	1790	20.0	745
514959	1201058061	29-MAR-2006 12:17	DONE	5	-0.39	percent	297	0	-1200	1790	20.0	745
512778	1201053530	30-MAR-2006 14:52	DONE	202	-0.13	percent	297	0	-1200	1790	20.0	745
513797	1201055597	31-MAR-2006 06:04	DONE	319	0.03	percent	297	0	-1200	1790	20.0	745
517045	1201062677	05-APR-2006 22:28	DONE	153	-0.19	percent	297	0	-1200	1790	20.0	745
516236	1201060949	06-APR-2006 06:01	DONE	2	-0.4	percent	297	0	-1200	1790	20.0	745
513810	1201055628	06-APR-2006 10:52	DONE	27	-0.36	percent	297	0	-1200	1790	20.0	745
517980	1201064809	07-APR-2006 06:16	DONE	103	-0.26	percent	297	0	-1200	1790	20.0	745
517983	1201064813	07-APR-2006 06:28	DONE	625	0.44	percent	297	0	-1200	1790	20.0	745
513432	1201054906	07-APR-2006 21:54	DONE	6	-0.39	percent	297	0	-1200	1790	20.0	745
513162	1201054360	09-APR-2006 21:34	DONE	16	-0.38	percent	297	0	-1200	1790	20.0	745
513799	1201055604	10-APR-2006 15:42	DUSE	221	-0.1	percent	297	0	-1200	1790	20.0	745
519499	1201068199	11-APR-2006 16:44	DONE	1	-0.4	percent	297	0	-1200	1790	20.0	745
519008	1201067117	11-APR-2006 19:22	DUSE	106	-0.26	percent	297	0	-1200	1790	20.0	745
518359	1201065660	11-APR-2006 21:47	DUSE	49	-0.33	percent	297	0	-1200	1790	20.0	745
513802	1201055608	11-APR-2006 23:19	DUSE	779	0.65	percent	297	0	-1200	1790	20.0	745

Cobalt-60 LCS: Limits LCL = 75 UCL = 125

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
509664	1201046396	15-MAR-2006 07:07	DONE	106	0.68	percent	100	75.0	83.3	117	125	8.33
509666	1201046400	15-MAR-2006 08:15	DONE	98	-0.25	percent	100	75.0	83.3	117	125	8.33
498916	1201021254	15-MAR-2006 10:52	DONE	101	0.12	percent	100	75.0	83.3	117	125	8.33
511947	1201051584	16-MAR-2006 03:52	DONE	102	0.26	percent	100	75.0	83.3	117	125	8.33
507629	1201041705	16-MAR-2006 13:15	DONE	102	0.24	percent	100	75.0	83.3	117	125	8.33
507626	1201041699	16-MAR-2006 15:21	DONE	105	0.59	percent	100	75.0	83.3	117	125	8.33
507622	1201041689	17-MAR-2006 06:12	DONE	99	-0.17	percent	100	75.0	83.3	117	125	8.33
508637	1201044145	17-MAR-2006 07:42	DONE	106	0.72	percent	100	75.0	83.3	117	125	8.33
508605	1201044043	17-MAR-2006 09:19	DONE	100	-0.06	percent	100	75.0	83.3	117	125	8.33
505207	1201035926	18-MAR-2006 13:44	DONE	102	0.29	percent	100	75.0	83.3	117	125	8.33

512599	1201053131	20-MAR-2006 06:21	DONE	101	0.07	percent	100	75.0	83.3	117	125	8.33
512597	1201053125	20-MAR-2006 07:29	DONE	99	-0.13	percent	100	75.0	83.3	117	125	8.33
508903	1201044758	20-MAR-2006 14:37	DONE	110	1.2	percent	100	75.0	83.3	117	125	8.33
499544	1201022693	20-MAR-2006 19:52	DONE	109	1.1	percent	100	75.0	83.3	117	125	8.33
512598	1201053128	20-MAR-2006 20:59	DONE	103	0.34	percent	100	75.0	83.3	117	125	8.33
506206	1201055202	21-MAR-2006 17:35	DONE	102	0.24	percent	100	75.0	83.3	117	125	8.33
509439	1201046013	22-MAR-2006 17:38	DONE	109	1	percent	100	75.0	83.3	117	125	8.33
509445	1201046017	22-MAR-2006 17:56	DUSE	96	-0.47	percent	100	75.0	83.3	117	125	8.33
509577	1201046236	22-MAR-2006 22:50	DONE	104	0.46	percent	100	75.0	83.3	117	125	8.33
509449	1201046024	23-MAR-2006 12:45	DUSE	99	-0.14	percent	100	75.0	83.3	117	125	8.33
509579	1201046243	25-MAR-2006 14:21	DUSE	96	-0.47	percent	100	75.0	83.3	117	125	8.33
498915	1201021245	26-MAR-2006 20:50	DONE	102	0.24	percent	100	75.0	83.3	117	125	8.33
513814	1201055632	28-MAR-2006 04:36	DONE	106	0.7	percent	100	75.0	83.3	117	125	8.33
513815	1201055635	28-MAR-2006 20:48	DONE	106	0.77	percent	100	75.0	83.3	117	125	8.33
512778	1201053531	30-MAR-2006 09:25	DONE	101	0.12	percent	100	75.0	83.3	117	125	8.33
514959	1201058063	30-MAR-2006 14:51	DONE	92	-0.96	percent	100	75.0	83.3	117	125	8.33
513797	1201055598	31-MAR-2006 06:06	DONE	94	-0.73	percent	100	75.0	83.3	117	125	8.33
512787	1201053543	04-APR-2006 09:03	DONE	109	1.1	percent	100	75.0	83.3	117	125	8.33
516236	1201060950	05-APR-2006 06:02	DONE	91	-1	percent	100	75.0	83.3	117	125	8.33
513810	1201055629	06-APR-2006 08:46	DONE	100	0	percent	100	75.0	83.3	117	125	8.33
517045	1201062678	06-APR-2006 11:31	DONE	103	0.36	percent	100	75.0	83.3	117	125	8.33
517980	1201064811	06-APR-2006 12:37	DONE	105	0.65	percent	100	75.0	83.3	117	125	8.33
517983	1201064814	07-APR-2006 06:28	DONE	104	0.53	percent	100	75.0	83.3	117	125	8.33
513432	1201054907	08-APR-2006 20:51	DONE	90	-1	percent	100	75.0	83.3	117	125	8.33
513162	1201054361	09-APR-2006 21:18	DONE	100	-0.02	percent	100	75.0	83.3	117	125	8.33
519008	1201067118	11-APR-2006 13:11	DUSE	97	-0.33	percent	100	75.0	83.3	117	125	8.33
513802	1201055609	11-APR-2006 14:31	DONE	102	0.28	percent	100	75.0	83.3	117	125	8.33
519499	1201068200	11-APR-2006 17:47	DONE	92	-0.95	percent	100	75.0	83.3	117	125	8.33
518359	1201065661	11-APR-2006 20:04	DONE	109	1.1	percent	100	75.0	83.3	117	125	8.33

Cobalt-60 RER: Limits LCL = 0 UCL = 3

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
509666	1201046399	16-MAR-2006 21:46	DONE	1.43	-0.06	dec	1.62	0	-5.1	8.37	3.00	3.37
508605	1201044042	17-MAR-2006 00:39	DONE	0.31	-0.39	dec	1.62	0	-5.1	8.37	3.00	3.37
507622	1201041687	17-MAR-2006 00:40	DONE	0.58	-0.31	dec	1.62	0	-5.1	8.37	3.00	3.37
508637	1201044144	17-MAR-2006 10:33	DONE	0.28	-0.4	dec	1.62	0	-5.1	8.37	3.00	3.37
498916	1201021255	20-MAR-2006 01:43	DONE	0.43	-0.35	dec	1.62	0	-5.1	8.37	3.00	3.37
498916	1201021256	20-MAR-2006 01:43	DONE	0.67	-0.28	dec	1.62	0	-5.1	8.37	3.00	3.37
512599	1201053130	20-MAR-2006 10:07	DONE	0.44	-0.35	dec	1.62	0	-5.1	8.37	3.00	3.37
508903	1201044757	20-MAR-2006 14:36	DONE	0.14	-0.44	dec	1.62	0	-5.1	8.37	3.00	3.37
505207	1201035925	20-MAR-2006 20:56	DONE	0.46	-0.34	dec	1.62	0	-5.1	8.37	3.00	3.37
512597	1201053124	20-MAR-2006 22:02	DONE	1.26	-0.11	dec	1.62	0	-5.1	8.37	3.00	3.37
499544	1201022691	21-MAR-2006 05:31	DONE	1.22	-0.12	dec	1.62	0	-5.1	8.37	3.00	3.37
512598	1201053127	21-MAR-2006 10:48	DONE	0.49	-0.33	dec	1.62	0	-5.1	8.37	3.00	3.37
506206	1201055201	21-MAR-2006 19:40	DONE	1.56	-0.02	dec	1.62	0	-5.1	8.37	3.00	3.37
498916	1201021257	22-MAR-2006 05:44	DONE	0.02	-0.47	dec	1.62	0	-5.1	8.37	3.00	3.37
509445	1201046016	22-MAR-2006 18:51	DUSE	1.05	-0.17	dec	1.62	0	-5.1	8.37	3.00	3.37
509439	1201046012	22-MAR-2006 20:39	DONE	0.7	-0.27	dec	1.62	0	-5.1	8.37	3.00	3.37
509577	1201046235	22-MAR-2006 22:31	DONE	0.39	-0.36	dec	1.62	0	-5.1	8.37	3.00	3.37
509449	1201046023	23-MAR-2006 05:27	DUSE	0.77	-0.25	dec	1.62	0	-5.1	8.37	3.00	3.37

498915	1201021243	24-MAR-2006 16:26	DONE	0.55	-0.32	dec	1.62	0	-5.1	8.37	3.00	3.37
509579	1201046242	25-MAR-2006 12:07	DUSE	0.68	-0.28	dec	1.62	0	-5.1	8.37	3.00	3.37
498915	1201021246	26-MAR-2006 23:53	DONE	9.5	2.3	dec	1.62	0	-5.1	8.37	3.00	3.37
513814	1201055631	27-MAR-2006 23:07	DONE	4.81	0.94	dec	1.62	0	-5.1	8.37	3.00	3.37
513815	1201055634	28-MAR-2006 20:48	DONE	2.23	0.18	dec	1.62	0	-5.1	8.37	3.00	3.37
514959	1201058061	29-MAR-2006 12:17	DONE	0.73	-0.26	dec	1.62	0	-5.1	8.37	3.00	3.37
512778	1201053530	30-MAR-2006 14:52	DONE	0.86	-0.22	dec	1.62	0	-5.1	8.37	3.00	3.37
513797	1201055597	31-MAR-2006 06:04	DONE	1.42	-0.06	dec	1.62	0	-5.1	8.37	3.00	3.37
512787	1201053542	01-APR-2006 20:06	DONE	0.06	-0.46	dec	1.62	0	-5.1	8.37	3.00	3.37
517045	1201062677	05-APR-2006 22:28	DONE	2.52	0.27	dec	1.62	0	-5.1	8.37	3.00	3.37
516236	1201060949	06-APR-2006 06:01	DONE	19.7	5.3	dec	1.62	0	-5.1	8.37	3.00	3.37
513810	1201055628	06-APR-2006 10:52	DONE	0.05	-0.47	dec	1.62	0	-5.1	8.37	3.00	3.37
517980	1201064809	07-APR-2006 06:16	DONE	1.04	-0.17	dec	1.62	0	-5.1	8.37	3.00	3.37
517983	1201064813	07-APR-2006 06:28	DONE	1.83	0.06	dec	1.62	0	-5.1	8.37	3.00	3.37
513432	1201054906	07-APR-2006 21:54	DONE	0.65	-0.29	dec	1.62	0	-5.1	8.37	3.00	3.37
513162	1201054360	09-APR-2006 21:34	DONE	1.11	-0.15	dec	1.62	0	-5.1	8.37	3.00	3.37
513799	1201055604	10-APR-2006 15:42	DUSE	0.83	-0.23	dec	1.62	0	-5.1	8.37	3.00	3.37
519499	1201068199	11-APR-2006 16:44	DONE	0.52	-0.33	dec	1.62	0	-5.1	8.37	3.00	3.37
519008	1201067117	11-APR-2006 19:22	DUSE	0.83	-0.24	dec	1.62	0	-5.1	8.37	3.00	3.37
518359	1201065660	11-APR-2006 21:47	DUSE	0.71	-0.27	dec	1.62	0	-5.1	8.37	3.00	3.37
513802	1201055608	11-APR-2006 23:19	DUSE	0.37	-0.37	dec	1.62	0	-5.1	8.37	3.00	3.37

Lead-212 RER: Limits LCL = 0 UCL = 3

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
509666	1201046399	16-MAR-2006 21:46	DONE	0.52	-0.45	dec	1.05	0	-1.3	3.41	3.00	1.18
508605	1201044042	17-MAR-2006 00:39	DONE	0.18	-0.74	dec	1.05	0	-1.3	3.41	3.00	1.18
507622	1201041687	17-MAR-2006 00:40	DONE	0.38	-0.56	dec	1.05	0	-1.3	3.41	3.00	1.18
508637	1201044144	17-MAR-2006 10:33	DONE	0.8	-0.21	dec	1.05	0	-1.3	3.41	3.00	1.18
498916	1201021255	20-MAR-2006 01:43	DUSE	2.61	1.3	dec	1.05	0	-1.3	3.41	3.00	1.18
498916	1201021256	20-MAR-2006 01:43	DUSE	2.22	0.99	dec	1.05	0	-1.3	3.41	3.00	1.18
512599	1201053130	20-MAR-2006 10:07	DONE	1.7	0.55	dec	1.05	0	-1.3	3.41	3.00	1.18
508903	1201044757	20-MAR-2006 14:36	DONE	1.09	0.04	dec	1.05	0	-1.3	3.41	3.00	1.18
505207	1201035925	20-MAR-2006 20:56	DONE	5.43	3.7	dec	1.05	0	-1.3	3.41	3.00	1.18
512597	1201053124	20-MAR-2006 22:02	DONE	0.45	-0.5	dec	1.05	0	-1.3	3.41	3.00	1.18
499544	1201022691	21-MAR-2006 05:31	DONE	0.11	-0.8	dec	1.05	0	-1.3	3.41	3.00	1.18
512598	1201053127	21-MAR-2006 10:48	DONE	0.63	-0.35	dec	1.05	0	-1.3	3.41	3.00	1.18
506206	1201055201	21-MAR-2006 19:40	DONE	1.37	0.27	dec	1.05	0	-1.3	3.41	3.00	1.18
498916	1201021257	22-MAR-2006 05:44	DUSE	0.07	-0.83	dec	1.05	0	-1.3	3.41	3.00	1.18
509445	1201046016	22-MAR-2006 18:51	DUSE	1.25	0.17	dec	1.05	0	-1.3	3.41	3.00	1.18
509439	1201046012	22-MAR-2006 20:39	DUSE	1.01	-0.03	dec	1.05	0	-1.3	3.41	3.00	1.18
509577	1201046235	22-MAR-2006 22:31	DUSE	0.14	-0.77	dec	1.05	0	-1.3	3.41	3.00	1.18
509449	1201046023	23-MAR-2006 05:27	DUSE	0.45	-0.5	dec	1.05	0	-1.3	3.41	3.00	1.18
498915	1201021243	24-MAR-2006 16:26	DUSE	0.59	-0.39	dec	1.05	0	-1.3	3.41	3.00	1.18
509579	1201046242	25-MAR-2006 12:07	DONE	1.81	0.65	dec	1.05	0	-1.3	3.41	3.00	1.18
498915	1201021246	26-MAR-2006 23:53	DUSE	5.06	3.4	dec	1.05	0	-1.3	3.41	3.00	1.18
513814	1201055631	27-MAR-2006 23:07	DONE	0.11	-0.79	dec	1.05	0	-1.3	3.41	3.00	1.18
513815	1201055634	28-MAR-2006 20:48	DONE	1.23	0.15	dec	1.05	0	-1.3	3.41	3.00	1.18
514959	1201058061	29-MAR-2006 12:17	DUSE	0.51	-0.45	dec	1.05	0	-1.3	3.41	3.00	1.18
512778	1201053530	30-MAR-2006 14:52	DONE	00	-0.89	dec	1.05	0	-1.3	3.41	3.00	1.18
513797	1201055597	31-MAR-2006 06:04	DONE	2.29	1.1	dec	1.05	0	-1.3	3.41	3.00	1.18

512787	1201053542	01-APR-2006 20:06	DONE	0.93	-0.1	dec	1.05	0	-1.3	3.41	3.00	1.18
517045	1201062677	05-APR-2006 22:28	DONE	1.07	0.02	dec	1.05	0	-1.3	3.41	3.00	1.18
516236	1201060949	06-APR-2006 06:01	DONE	0.49	-0.47	dec	1.05	0	-1.3	3.41	3.00	1.18
513810	1201055628	06-APR-2006 10:52	DONE	1.26	0.18	dec	1.05	0	-1.3	3.41	3.00	1.18
517980	1201064809	07-APR-2006 06:16	DONE	0.66	-0.33	dec	1.05	0	-1.3	3.41	3.00	1.18
517983	1201064813	07-APR-2006 06:28	DONE	1.27	0.19	dec	1.05	0	-1.3	3.41	3.00	1.18
513432	1201054906	07-APR-2006 21:54	DONE	0.83	-0.18	dec	1.05	0	-1.3	3.41	3.00	1.18
513162	1201054360	09-APR-2006 21:34	DONE	0.5	-0.46	dec	1.05	0	-1.3	3.41	3.00	1.18
513799	1201055604	10-APR-2006 15:42	DONE	0.86	-0.16	dec	1.05	0	-1.3	3.41	3.00	1.18
519499	1201068199	11-APR-2006 16:44	DONE	0.16	-0.76	dec	1.05	0	-1.3	3.41	3.00	1.18
519008	1201067117	11-APR-2006 19:22	DUSE	0.16	-0.75	dec	1.05	0	-1.3	3.41	3.00	1.18
518359	1201065660	11-APR-2006 21:47	DUSE	0.04	-0.86	dec	1.05	0	-1.3	3.41	3.00	1.18
513802	1201055608	11-APR-2006 23:19	DONE	0.66	-0.33	dec	1.05	0	-1.3	3.41	3.00	1.18

Radium-226 BLANK: Limits LCL = -34.4 UCL = 38.9

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
512787	1201053541	01-APR-2006 20:05	DONE	0	-0.18	pCi/g	2.25	-34	-22	26.7	38.9	12.2
510153	1201047482	01-APR-2006 20:23	DUSE	0	-0.18	pCi/g	2.25	-34	-22	26.7	38.9	12.2
516236	1201060948	03-APR-2006 22:12	DUSE	12	0.78	pCi/g	2.25	-34	-22	26.7	38.9	12.2
510153	1201047482	03-APR-2006 23:22	DONE	0	-0.18	pCi/g	2.25	-34	-22	26.7	38.9	12.2
510952	1201049298	04-APR-2006 01:43	DONE	0	-0.18	pCi/g	2.25	-34	-22	26.7	38.9	12.2
510881	1201049180	04-APR-2006 05:48	DONE	0	-0.18	pCi/g	2.25	-34	-22	26.7	38.9	12.2
516989	1201062554	05-APR-2006 08:18	DONE	0	-0.18	pCi/g	2.25	-34	-22	26.7	38.9	12.2
508902	1201044753	05-APR-2006 09:43	DONE	0	-0.18	pCi/g	2.25	-34	-22	26.7	38.9	12.2
508900	1201044747	05-APR-2006 17:35	DONE	0	-0.18	pCi/g	2.25	-34	-22	26.7	38.9	12.2
517983	1201064812	05-APR-2006 18:28	DUSE	0	-0.19	pCi/g	2.25	-34	-22	26.7	38.9	12.2
516986	1201062545	06-APR-2006 08:33	DONE	0	-0.18	pCi/g	2.25	-34	-22	26.7	38.9	12.2
513810	1201055627	06-APR-2006 09:43	DONE	0	-0.18	pCi/g	2.25	-34	-22	26.7	38.9	12.2
516987	1201062548	06-APR-2006 10:43	DONE	0	-0.18	pCi/g	2.25	-34	-22	26.7	38.9	12.2
517045	1201062676	06-APR-2006 10:56	DUSE	0	-0.18	pCi/g	2.25	-34	-22	26.7	38.9	12.2
516991	1201062560	06-APR-2006 11:51	DONE	0	-0.18	pCi/g	2.25	-34	-22	26.7	38.9	12.2
516993	1201062566	06-APR-2006 16:35	DONE	0	-0.18	pCi/g	2.25	-34	-22	26.7	38.9	12.2
510982	1201049354	06-APR-2006 16:39	DONE	0	-0.18	pCi/g	2.25	-34	-22	26.7	38.9	12.2
510976	1201049346	06-APR-2006 18:46	DONE	0	-0.18	pCi/g	2.25	-34	-22	26.7	38.9	12.2
516996	1201062572	07-APR-2006 06:08	DONE	0	-0.18	pCi/g	2.25	-34	-22	26.7	38.9	12.2
516999	1201062578	07-APR-2006 08:19	DONE	0	-0.18	pCi/g	2.25	-34	-22	26.7	38.9	12.2
511760	1201051194	07-APR-2006 10:19	DONE	0	-0.18	pCi/g	2.25	-34	-22	26.7	38.9	12.2
517980	1201064808	07-APR-2006 14:52	DUSE	0	-0.18	pCi/g	2.25	-34	-22	26.7	38.9	12.2
513432	1201054905	07-APR-2006 17:03	DUSE	0	-0.17	pCi/g	2.25	-34	-22	26.7	38.9	12.2
517004	1201062584	08-APR-2006 16:03	DONE	0	-0.18	pCi/g	2.25	-34	-22	26.7	38.9	12.2
517006	1201062590	08-APR-2006 21:37	DONE	0	-0.18	pCi/g	2.25	-34	-22	26.7	38.9	12.2
517018	1201062614	09-APR-2006 21:09	DONE	0	-0.18	pCi/g	2.25	-34	-22	26.7	38.9	12.2
517011	1201062602	10-APR-2006 06:23	DONE	0	-0.18	pCi/g	2.25	-34	-22	26.7	38.9	12.2
513162	1201054359	10-APR-2006 06:36	DUSE	0	-0.18	pCi/g	2.25	-34	-22	26.7	38.9	12.2
517009	1201062596	10-APR-2006 10:47	DONE	0	-0.18	pCi/g	2.25	-34	-22	26.7	38.9	12.2
513799	1201055603	10-APR-2006 11:17	DONE	0	-0.18	pCi/g	2.25	-34	-22	26.7	38.9	12.2
517015	1201062608	10-APR-2006 13:00	DONE	0	-0.18	pCi/g	2.25	-34	-22	26.7	38.9	12.2
512595	1201053117	10-APR-2006 13:17	DONE	0	-0.18	pCi/g	2.25	-34	-22	26.7	38.9	12.2
513054	1201054080	11-APR-2006 11:51	DONE	0	-0.18	pCi/g	2.25	-34	-22	26.7	38.9	12.2
519499	1201068198	11-APR-2006 14:26	DUSE	76	6	pCi/g	2.25	-34	-22	26.7	38.9	12.2

519008	1201067116	11-APR-2006 18:52	DUSE	0	-0.18	pCi/g	2.25	-34	-22	26.7	38.9	12.2
518359	1201065659	11-APR-2006 18:53	DUSE	0	-0.18	pCi/g	2.25	-34	-22	26.7	38.9	12.2
513058	1201054086	11-APR-2006 21:43	DONE	0	-0.18	pCi/g	2.25	-34	-22	26.7	38.9	12.2
513802	1201055607	11-APR-2006 23:19	DONE	0	-0.18	pCi/g	2.25	-34	-22	26.7	38.9	12.2
513780	1201055549	11-APR-2006 23:45	DONE	0	-0.18	pCi/g	2.25	-34	-22	26.7	38.9	12.2

Radium-226 DUP: Limits LCL = 0 UCL = 20

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
510952	1201049299	04-APR-2006 01:41	DONE	3	-0.45	percent	21.9	0	-62	106	20.0	41.9
510881	1201049181	04-APR-2006 06:40	DONE	6	-0.39	percent	21.9	0	-62	106	20.0	41.9
510153	1201047483	04-APR-2006 07:57	DONE	5	-0.41	percent	21.9	0	-62	106	20.0	41.9
516989	1201062555	05-APR-2006 08:18	DONE	2	-0.48	percent	21.9	0	-62	106	20.0	41.9
508902	1201044754	05-APR-2006 09:43	DONE	3	-0.46	percent	21.9	0	-62	106	20.0	41.9
508900	1201044748	05-APR-2006 17:36	DONE	14	-0.2	percent	21.9	0	-62	106	20.0	41.9
517045	1201062677	05-APR-2006 22:28	DUSE	171	3.6	percent	21.9	0	-62	106	20.0	41.9
516236	1201060949	06-APR-2006 06:01	DUSE	105	2	percent	21.9	0	-62	106	20.0	41.9
516986	1201062546	06-APR-2006 08:33	DONE	10	-0.3	percent	21.9	0	-62	106	20.0	41.9
516987	1201062549	06-APR-2006 10:43	DONE	0	-0.52	percent	21.9	0	-62	106	20.0	41.9
513810	1201055628	06-APR-2006 10:52	DONE	3	-0.46	percent	21.9	0	-62	106	20.0	41.9
516991	1201062561	06-APR-2006 12:45	DONE	0	-0.51	percent	21.9	0	-62	106	20.0	41.9
516993	1201062567	06-APR-2006 16:35	DONE	5	-0.41	percent	21.9	0	-62	106	20.0	41.9
510976	1201049347	06-APR-2006 18:47	DUSE	6	-0.39	percent	21.9	0	-62	106	20.0	41.9
510982	1201049355	06-APR-2006 18:47	DONE	6	-0.38	percent	21.9	0	-62	106	20.0	41.9
516996	1201062573	07-APR-2006 06:09	DUSE	3	-0.45	percent	21.9	0	-62	106	20.0	41.9
517980	1201064809	07-APR-2006 06:16	DUSE	78	1.3	percent	21.9	0	-62	106	20.0	41.9
517983	1201064813	07-APR-2006 06:28	DUSE	5	-0.39	percent	21.9	0	-62	106	20.0	41.9
516999	1201062579	07-APR-2006 08:20	DONE	10	-0.28	percent	21.9	0	-62	106	20.0	41.9
511760	1201051195	07-APR-2006 10:20	DONE	1	-0.49	percent	21.9	0	-62	106	20.0	41.9
516996	1201062573	07-APR-2006 10:31	DONE	3	-0.44	percent	21.9	0	-62	106	20.0	41.9
513432	1201054906	07-APR-2006 21:54	DUSE	16	-0.14	percent	21.9	0	-62	106	20.0	41.9
510976	1201049347	07-APR-2006 22:28	DONE	1	-0.49	percent	21.9	0	-62	106	20.0	41.9
517004	1201062585	08-APR-2006 16:02	DONE	13	-0.22	percent	21.9	0	-62	106	20.0	41.9
517006	1201062591	08-APR-2006 21:38	DONE	6	-0.37	percent	21.9	0	-62	106	20.0	41.9
517018	1201062615	09-APR-2006 21:10	DONE	1	-0.5	percent	21.9	0	-62	106	20.0	41.9
513162	1201054360	09-APR-2006 21:34	DUSE	14	-0.2	percent	21.9	0	-62	106	20.0	41.9
517011	1201062603	10-APR-2006 06:23	DONE	5	-0.4	percent	21.9	0	-62	106	20.0	41.9
517009	1201062597	10-APR-2006 10:48	DONE	51	0.7	percent	21.9	0	-62	106	20.0	41.9
517015	1201062609	10-APR-2006 10:51	DONE	17	-0.12	percent	21.9	0	-62	106	20.0	41.9
512595	1201053118	10-APR-2006 13:18	DONE	19	-0.08	percent	21.9	0	-62	106	20.0	41.9
513799	1201055604	10-APR-2006 15:42	DONE	10	-0.27	percent	21.9	0	-62	106	20.0	41.9
513054	1201054081	11-APR-2006 10:21	DONE	6	-0.39	percent	21.9	0	-62	106	20.0	41.9
519499	1201068199	11-APR-2006 16:44	DUSE	19	-0.07	percent	21.9	0	-62	106	20.0	41.9
519008	1201067117	11-APR-2006 19:22	DUSE	35	0.32	percent	21.9	0	-62	106	20.0	41.9
513058	1201054087	11-APR-2006 21:43	DONE	3	-0.46	percent	21.9	0	-62	106	20.0	41.9
518359	1201065660	11-APR-2006 21:47	DUSE	180	3.8	percent	21.9	0	-62	106	20.0	41.9
513802	1201055608	11-APR-2006 23:19	DONE	10	-0.29	percent	21.9	0	-62	106	20.0	41.9
513780	1201055550	11-APR-2006 23:45	DONE	10	-0.28	percent	21.9	0	-62	106	20.0	41.9

Radium-226 LCS: Limits LCL = 75 UCL = 125

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
----------	---------	----------	--------	-------	-----------	-------	------	-----	-----	-----	-----	-------

508864	1201044686	27-MAR-2006 17:32	DONE	97	-0.34	percent	100	75.0	83.3	117	125	8.33
513785	1201055566	27-MAR-2006 18:45	DONE	100	-0.02	percent	100	75.0	83.3	117	125	8.33
508865	1201044689	27-MAR-2006 21:56	DONE	101	0.17	percent	100	75.0	83.3	117	125	8.33
513779	1201055548	28-MAR-2006 08:25	DONE	100	-0.05	percent	100	75.0	83.3	117	125	8.33
515289	1201058838	28-MAR-2006 10:08	DONE	97	-0.4	percent	100	75.0	83.3	117	125	8.33
513783	1201055560	29-MAR-2006 07:56	DONE	98	-0.28	percent	100	75.0	83.3	117	125	8.33
515230	1201058656	30-MAR-2006 04:39	DONE	113	1.6	percent	100	75.0	83.3	117	125	8.33
510133	1201047439	31-MAR-2006 10:31	DONE	93	-0.8	percent	100	75.0	83.3	117	125	8.33
510114	1201047414	31-MAR-2006 13:58	DONE	89	-1	percent	100	75.0	83.3	117	125	8.33
510144	1201047452	31-MAR-2006 17:31	DONE	86	-2	percent	100	75.0	83.3	117	125	8.33
510151	1201047470	31-MAR-2006 21:07	DONE	94	-0.74	percent	100	75.0	83.3	117	125	8.33
516059	1201060578	01-APR-2006 11:49	DONE	99	-0.12	percent	100	75.0	83.3	117	125	8.33
510153	1201047484	03-APR-2006 05:22	DONE	97	-0.4	percent	100	75.0	83.3	117	125	8.33
510952	1201049300	04-APR-2006 00:35	DONE	107	0.78	percent	100	75.0	83.3	117	125	8.33
510881	1201049182	04-APR-2006 06:47	DONE	87	-2	percent	100	75.0	83.3	117	125	8.33
516989	1201062556	05-APR-2006 08:19	DONE	104	0.46	percent	100	75.0	83.3	117	125	8.33
508902	1201044755	05-APR-2006 09:44	DONE	104	0.48	percent	100	75.0	83.3	117	125	8.33
508900	1201044749	05-APR-2006 17:37	DONE	100	0	percent	100	75.0	83.3	117	125	8.33
516986	1201062547	06-APR-2006 08:34	DONE	105	0.58	percent	100	75.0	83.3	117	125	8.33
516987	1201062550	06-APR-2006 09:41	DONE	105	0.6	percent	100	75.0	83.3	117	125	8.33
516993	1201062568	06-APR-2006 18:48	DUSE	121	2.5	percent	100	75.0	83.3	117	125	8.33
516996	1201062574	07-APR-2006 06:22	DONE	103	0.39	percent	100	75.0	83.3	117	125	8.33
516999	1201062580	07-APR-2006 08:20	DONE	111	1.3	percent	100	75.0	83.3	117	125	8.33
516993	1201062568	07-APR-2006 09:23	DONE	117	2.1	percent	100	75.0	83.3	117	125	8.33
510976	1201049348	07-APR-2006 13:56	DUSE	0	-12	percent	100	75.0	83.3	117	125	8.33
510982	1201049356	07-APR-2006 16:32	DONE	90	-1	percent	100	75.0	83.3	117	125	8.33
516991	1201062562	07-APR-2006 17:34	DONE	94	-0.72	percent	100	75.0	83.3	117	125	8.33
511760	1201051196	07-APR-2006 18:35	DONE	94	-0.67	percent	100	75.0	83.3	117	125	8.33
510976	1201049348	07-APR-2006 20:56	DONE	92	-0.94	percent	100	75.0	83.3	117	125	8.33
517006	1201062592	08-APR-2006 21:40	DONE	86	-2	percent	100	75.0	83.3	117	125	8.33
517004	1201062586	08-APR-2006 22:57	DONE	89	-1	percent	100	75.0	83.3	117	125	8.33
517018	1201062616	09-APR-2006 21:08	DONE	96	-0.51	percent	100	75.0	83.3	117	125	8.33
517011	1201062604	09-APR-2006 22:21	DONE	92	-0.94	percent	100	75.0	83.3	117	125	8.33
517009	1201062598	10-APR-2006 10:48	DONE	96	-0.48	percent	100	75.0	83.3	117	125	8.33
517015	1201062610	10-APR-2006 12:03	DONE	104	0.45	percent	100	75.0	83.3	117	125	8.33
512595	1201053119	10-APR-2006 13:19	DONE	108	0.97	percent	100	75.0	83.3	117	125	8.33
513054	1201054082	11-APR-2006 11:51	DONE	89	-1	percent	100	75.0	83.3	117	125	8.33
513058	1201054088	11-APR-2006 13:59	DONE	95	-0.66	percent	100	75.0	83.3	117	125	8.33
513780	1201055551	11-APR-2006 23:46	DONE	91	-1	percent	100	75.0	83.3	117	125	8.33

Radium-226 RER: Limits LCL = 0 UCL = 3

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
510952	1201049299	04-APR-2006 01:41	DONE	0.41	-0.4	dec	0.85	0	-1.4	3.06	3.00	1.1
510881	1201049181	04-APR-2006 06:40	DONE	0.4	-0.41	dec	0.85	0	-1.4	3.06	3.00	1.1
510153	1201047483	04-APR-2006 07:57	DONE	0.41	-0.4	dec	0.85	0	-1.4	3.06	3.00	1.1
516989	1201062555	05-APR-2006 08:18	DONE	0.18	-0.61	dec	0.85	0	-1.4	3.06	3.00	1.1
508902	1201044754	05-APR-2006 09:43	DONE	0.24	-0.55	dec	0.85	0	-1.4	3.06	3.00	1.1
508900	1201044748	05-APR-2006 17:36	DONE	1.23	0.34	dec	0.85	0	-1.4	3.06	3.00	1.1
517045	1201062677	05-APR-2006 22:28	DUSE	2.09	1.1	dec	0.85	0	-1.4	3.06	3.00	1.1
516236	1201060949	06-APR-2006 06:01	DUSE	0.29	-0.51	dec	0.85	0	-1.4	3.06	3.00	1.1

516986	1201062546	06-APR-2006 08:33	DONE	1.09	0.22	dec	0.85	0	-1.4	3.06	3.00	1.1
516987	1201062549	06-APR-2006 10:43	DONE	0.01	-0.76	dec	0.85	0	-1.4	3.06	3.00	1.1
513810	1201055628	06-APR-2006 10:52	DONE	0.11	-0.67	dec	0.85	0	-1.4	3.06	3.00	1.1
516991	1201062561	06-APR-2006 12:45	DONE	0.04	-0.74	dec	0.85	0	-1.4	3.06	3.00	1.1
516993	1201062567	06-APR-2006 16:35	DONE	0.55	-0.27	dec	0.85	0	-1.4	3.06	3.00	1.1
510976	1201049347	06-APR-2006 18:47	DUSE	0.84	-0.01	dec	0.85	0	-1.4	3.06	3.00	1.1
510982	1201049355	06-APR-2006 18:47	DONE	0.49	-0.33	dec	0.85	0	-1.4	3.06	3.00	1.1
516996	1201062573	07-APR-2006 06:09	DUSE	0.3	-0.5	dec	0.85	0	-1.4	3.06	3.00	1.1
517980	1201064809	07-APR-2006 06:16	DUSE	0.63	-0.2	dec	0.85	0	-1.4	3.06	3.00	1.1
517983	1201064813	07-APR-2006 06:28	DUSE	0.4	-0.41	dec	0.85	0	-1.4	3.06	3.00	1.1
516999	1201062579	07-APR-2006 08:20	DONE	1.06	0.19	dec	0.85	0	-1.4	3.06	3.00	1.1
511760	1201051195	07-APR-2006 10:20	DONE	0.08	-0.7	dec	0.85	0	-1.4	3.06	3.00	1.1
516996	1201062573	07-APR-2006 10:31	DONE	0.29	-0.51	dec	0.85	0	-1.4	3.06	3.00	1.1
513432	1201054906	07-APR-2006 21:54	DUSE	0.15	-0.63	dec	0.85	0	-1.4	3.06	3.00	1.1
510976	1201049347	07-APR-2006 22:28	DONE	0.2	-0.59	dec	0.85	0	-1.4	3.06	3.00	1.1
517004	1201062585	08-APR-2006 16:02	DONE	1.81	0.87	dec	0.85	0	-1.4	3.06	3.00	1.1
517006	1201062591	08-APR-2006 21:38	DONE	0.75	-0.09	dec	0.85	0	-1.4	3.06	3.00	1.1
517018	1201062615	09-APR-2006 21:10	DONE	0.08	-0.7	dec	0.85	0	-1.4	3.06	3.00	1.1
513162	1201054360	09-APR-2006 21:34	DUSE	1.17	0.29	dec	0.85	0	-1.4	3.06	3.00	1.1
517011	1201062603	10-APR-2006 06:23	DONE	0.65	-0.18	dec	0.85	0	-1.4	3.06	3.00	1.1
517009	1201062597	10-APR-2006 10:48	DONE	6.54	5.2	dec	0.85	0	-1.4	3.06	3.00	1.1
517015	1201062609	10-APR-2006 10:51	DONE	1.82	0.88	dec	0.85	0	-1.4	3.06	3.00	1.1
512595	1201053118	10-APR-2006 13:18	DONE	1.57	0.65	dec	0.85	0	-1.4	3.06	3.00	1.1
513799	1201055604	10-APR-2006 15:42	DONE	1.31	0.42	dec	0.85	0	-1.4	3.06	3.00	1.1
513054	1201054081	11-APR-2006 10:21	DONE	0.68	-0.16	dec	0.85	0	-1.4	3.06	3.00	1.1
519499	1201068199	11-APR-2006 16:44	DUSE	0.32	-0.48	dec	0.85	0	-1.4	3.06	3.00	1.1
519008	1201067117	11-APR-2006 19:22	DUSE	0.36	-0.44	dec	0.85	0	-1.4	3.06	3.00	1.1
513058	1201054087	11-APR-2006 21:43	DONE	0.3	-0.5	dec	0.85	0	-1.4	3.06	3.00	1.1
518359	1201065660	11-APR-2006 21:47	DUSE	2.01	1	dec	0.85	0	-1.4	3.06	3.00	1.1
513802	1201055608	11-APR-2006 23:19	DONE	0.89	0.03	dec	0.85	0	-1.4	3.06	3.00	1.1
513780	1201055550	11-APR-2006 23:45	DONE	1.46	0.55	dec	0.85	0	-1.4	3.06	3.00	1.1

Radium-228 BLANK: Limits LCL = -23.8 UCL = 27.4

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
512787	1201053541	01-APR-2006 20:05	DONE	0	-0.21	pCi/g	1.79	-24	-15	18.9	27.4	8.54
510153	1201047482	01-APR-2006 20:23	DUSE	0	-0.21	pCi/g	1.79	-24	-15	18.9	27.4	8.54
516236	1201060948	03-APR-2006 22:12	DONE	50	5.7	pCi/g	1.79	-24	-15	18.9	27.4	8.54
510153	1201047482	03-APR-2006 23:22	DONE	0	-0.21	pCi/g	1.79	-24	-15	18.9	27.4	8.54
510952	1201049298	04-APR-2006 01:43	DONE	0	-0.21	pCi/g	1.79	-24	-15	18.9	27.4	8.54
510881	1201049180	04-APR-2006 05:48	DONE	0	-0.21	pCi/g	1.79	-24	-15	18.9	27.4	8.54
516989	1201062554	05-APR-2006 08:18	DONE	0	-0.21	pCi/g	1.79	-24	-15	18.9	27.4	8.54
508902	1201044753	05-APR-2006 09:43	DONE	0	-0.21	pCi/g	1.79	-24	-15	18.9	27.4	8.54
508900	1201044747	05-APR-2006 17:35	DONE	0	-0.2	pCi/g	1.79	-24	-15	18.9	27.4	8.54
517983	1201064812	05-APR-2006 18:28	DONE	0	-0.21	pCi/g	1.79	-24	-15	18.9	27.4	8.54
516986	1201062545	06-APR-2006 08:33	DONE	0	-0.21	pCi/g	1.79	-24	-15	18.9	27.4	8.54
513810	1201055627	06-APR-2006 09:43	DONE	0	-0.21	pCi/g	1.79	-24	-15	18.9	27.4	8.54
516987	1201062548	06-APR-2006 10:43	DONE	0	-0.21	pCi/g	1.79	-24	-15	18.9	27.4	8.54
517045	1201062676	06-APR-2006 10:56	DONE	0	-0.2	pCi/g	1.79	-24	-15	18.9	27.4	8.54
516991	1201062560	06-APR-2006 11:51	DONE	0	-0.21	pCi/g	1.79	-24	-15	18.9	27.4	8.54
516993	1201062566	06-APR-2006 16:35	DONE	0	-0.21	pCi/g	1.79	-24	-15	18.9	27.4	8.54

510982	1201049354	06-APR-2006 16:39	DONE	0	-0.21	pCi/g	1.79	-24	-15	18.9	27.4	8.54
510976	1201049346	06-APR-2006 18:46	DONE	0	-0.21	pCi/g	1.79	-24	-15	18.9	27.4	8.54
516996	1201062572	07-APR-2006 06:08	DONE	0	-0.21	pCi/g	1.79	-24	-15	18.9	27.4	8.54
516999	1201062578	07-APR-2006 08:19	DONE	0	-0.21	pCi/g	1.79	-24	-15	18.9	27.4	8.54
511760	1201051194	07-APR-2006 10:19	DONE	0	-0.21	pCi/g	1.79	-24	-15	18.9	27.4	8.54
517980	1201064808	07-APR-2006 14:52	DONE	0	-0.21	pCi/g	1.79	-24	-15	18.9	27.4	8.54
513432	1201054905	07-APR-2006 17:03	DONE	0	-0.18	pCi/g	1.79	-24	-15	18.9	27.4	8.54
517004	1201062584	08-APR-2006 16:03	DONE	0	-0.21	pCi/g	1.79	-24	-15	18.9	27.4	8.54
517006	1201062590	08-APR-2006 21:37	DONE	0	-0.21	pCi/g	1.79	-24	-15	18.9	27.4	8.54
517018	1201062614	09-APR-2006 21:09	DONE	0	-0.21	pCi/g	1.79	-24	-15	18.9	27.4	8.54
517011	1201062602	10-APR-2006 06:23	DONE	0	-0.21	pCi/g	1.79	-24	-15	18.9	27.4	8.54
513162	1201054359	10-APR-2006 06:36	DUSE	0	-0.2	pCi/g	1.79	-24	-15	18.9	27.4	8.54
517009	1201062596	10-APR-2006 10:47	DONE	0	-0.21	pCi/g	1.79	-24	-15	18.9	27.4	8.54
513799	1201055603	10-APR-2006 11:17	DONE	0	-0.21	pCi/g	1.79	-24	-15	18.9	27.4	8.54
517015	1201062608	10-APR-2006 13:00	DONE	0	-0.21	pCi/g	1.79	-24	-15	18.9	27.4	8.54
512595	1201053117	10-APR-2006 13:17	DONE	0	-0.21	pCi/g	1.79	-24	-15	18.9	27.4	8.54
513054	1201054080	11-APR-2006 11:51	DONE	0	-0.21	pCi/g	1.79	-24	-15	18.9	27.4	8.54
519499	1201068198	11-APR-2006 14:26	DONE	19	2	pCi/g	1.79	-24	-15	18.9	27.4	8.54
519008	1201067116	11-APR-2006 18:52	DUSE	0	-0.21	pCi/g	1.79	-24	-15	18.9	27.4	8.54
518359	1201065659	11-APR-2006 18:53	DUSE	0	-0.19	pCi/g	1.79	-24	-15	18.9	27.4	8.54
513058	1201054086	11-APR-2006 21:43	DONE	0	-0.21	pCi/g	1.79	-24	-15	18.9	27.4	8.54
513802	1201055607	11-APR-2006 23:19	DONE	0	-0.21	pCi/g	1.79	-24	-15	18.9	27.4	8.54
513780	1201055549	11-APR-2006 23:45	DONE	0	-0.21	pCi/g	1.79	-24	-15	18.9	27.4	8.54

Radium-228 DUP: Limits LCL = 0 UCL = 20

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
510952	1201049299	04-APR-2006 01:41	DONE	14	-0.24	percent	20.7	0	-36	77.8	20.0	28.5
510881	1201049181	04-APR-2006 06:40	DONE	16	-0.17	percent	20.7	0	-36	77.8	20.0	28.5
510153	1201047483	04-APR-2006 07:57	DONE	27	0.24	percent	20.7	0	-36	77.8	20.0	28.5
516989	1201062555	05-APR-2006 08:18	DONE	10	-0.37	percent	20.7	0	-36	77.8	20.0	28.5
508902	1201044754	05-APR-2006 09:43	DONE	36	0.54	percent	20.7	0	-36	77.8	20.0	28.5
508900	1201044748	05-APR-2006 17:36	DONE	12	-0.32	percent	20.7	0	-36	77.8	20.0	28.5
517045	1201062677	05-APR-2006 22:28	DONE	1	-0.7	percent	20.7	0	-36	77.8	20.0	28.5
516236	1201060949	06-APR-2006 06:01	DONE	70	1.7	percent	20.7	0	-36	77.8	20.0	28.5
516986	1201062546	06-APR-2006 08:33	DONE	11	-0.34	percent	20.7	0	-36	77.8	20.0	28.5
516987	1201062549	06-APR-2006 10:43	DONE	7	-0.48	percent	20.7	0	-36	77.8	20.0	28.5
513810	1201055628	06-APR-2006 10:52	DONE	15	-0.19	percent	20.7	0	-36	77.8	20.0	28.5
516991	1201062561	06-APR-2006 12:45	DONE	28	0.26	percent	20.7	0	-36	77.8	20.0	28.5
516993	1201062567	06-APR-2006 16:35	DONE	10	-0.38	percent	20.7	0	-36	77.8	20.0	28.5
510976	1201049347	06-APR-2006 18:47	DUSE	7	-0.49	percent	20.7	0	-36	77.8	20.0	28.5
510982	1201049355	06-APR-2006 18:47	DONE	3	-0.61	percent	20.7	0	-36	77.8	20.0	28.5
516996	1201062573	07-APR-2006 06:09	DUSE	11	-0.34	percent	20.7	0	-36	77.8	20.0	28.5
517980	1201064809	07-APR-2006 06:16	DONE	38	0.61	percent	20.7	0	-36	77.8	20.0	28.5
517983	1201064813	07-APR-2006 06:28	DONE	1	-0.71	percent	20.7	0	-36	77.8	20.0	28.5
516999	1201062579	07-APR-2006 08:20	DONE	3	-0.62	percent	20.7	0	-36	77.8	20.0	28.5
511760	1201051195	07-APR-2006 10:20	DONE	26	0.2	percent	20.7	0	-36	77.8	20.0	28.5
516996	1201062573	07-APR-2006 10:31	DONE	3	-0.62	percent	20.7	0	-36	77.8	20.0	28.5
513432	1201054906	07-APR-2006 21:54	DONE	26	0.18	percent	20.7	0	-36	77.8	20.0	28.5
510976	1201049347	07-APR-2006 22:28	DONE	12	-0.31	percent	20.7	0	-36	77.8	20.0	28.5
517004	1201062585	08-APR-2006 16:02	DONE	6	-0.52	percent	20.7	0	-36	77.8	20.0	28.5

517006	1201062591	08-APR-2006 21:38	DONE	4	-0.58	percent	20.7	0	-36	77.8	20.0	28.5
517018	1201062615	09-APR-2006 21:10	DONE	16	-0.18	percent	20.7	0	-36	77.8	20.0	28.5
513162	1201054360	09-APR-2006 21:34	DUSE	15	-0.21	percent	20.7	0	-36	77.8	20.0	28.5
517011	1201062603	10-APR-2006 06:23	DONE	11	-0.35	percent	20.7	0	-36	77.8	20.0	28.5
517009	1201062597	10-APR-2006 10:48	DONE	38	0.61	percent	20.7	0	-36	77.8	20.0	28.5
517015	1201062609	10-APR-2006 10:51	DONE	12	-0.29	percent	20.7	0	-36	77.8	20.0	28.5
512595	1201053118	10-APR-2006 13:18	DONE	23	0.07	percent	20.7	0	-36	77.8	20.0	28.5
513799	1201055604	10-APR-2006 15:42	DONE	2	-0.66	percent	20.7	0	-36	77.8	20.0	28.5
513054	1201054081	11-APR-2006 10:21	DONE	2	-0.67	percent	20.7	0	-36	77.8	20.0	28.5
519499	1201068199	11-APR-2006 16:44	DONE	27	0.22	percent	20.7	0	-36	77.8	20.0	28.5
519008	1201067117	11-APR-2006 19:22	DUSE	146	4.4	percent	20.7	0	-36	77.8	20.0	28.5
513058	1201054087	11-APR-2006 21:43	DONE	14	-0.23	percent	20.7	0	-36	77.8	20.0	28.5
518359	1201065660	11-APR-2006 21:47	DUSE	103	2.9	percent	20.7	0	-36	77.8	20.0	28.5
513802	1201055608	11-APR-2006 23:19	DONE	0	-0.72	percent	20.7	0	-36	77.8	20.0	28.5
513780	1201055550	11-APR-2006 23:45	DONE	3	-0.62	percent	20.7	0	-36	77.8	20.0	28.5

Radium-228 LCS: Limits LCL = 75 UCL = 125




Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
345003	1200653378	01-JUL-2004 19:26	DONE	101	0.12	percent	100	75.0	83.3	117	125	8.33
347180	1200658503	12-JUL-2004 13:36	DONE	95	-0.62	percent	100	75.0	83.3	117	125	8.33
343603	1200650208	16-JUL-2004 11:52	DONE	97	-0.34	percent	100	75.0	83.3	117	125	8.33
359453	1200687782	24-AUG-2004 23:18	DONE	100	0.01	percent	100	75.0	83.3	117	125	8.33
359457	1200687791	25-AUG-2004 12:11	DONE	95	-0.61	percent	100	75.0	83.3	117	125	8.33
359710	1200688274	25-AUG-2004 17:01	DONE	93	-0.86	percent	100	75.0	83.3	117	125	8.33
359720	1200688312	01-SEP-2004 14:23	DONE	103	0.3	percent	100	75.0	83.3	117	125	8.33
358061	1200684548	07-SEP-2004 14:48	DONE	97	-0.35	percent	100	75.0	83.3	117	125	8.33
364331	1200699256	09-SEP-2004 12:09	DONE	95	-0.61	percent	100	75.0	83.3	117	125	8.33
382774	1200743863	22-NOV-2004 07:06	DONE	94	-0.72	percent	100	75.0	83.3	117	125	8.33
382466	1200743128	09-DEC-2004 16:58	DONE	91	-1	percent	100	75.0	83.3	117	125	8.33
399581	1200784220	10-FEB-2005 10:29	DONE	99	-0.09	percent	100	75.0	83.3	117	125	8.33
399617	1200784322	10-FEB-2005 14:55	DONE	90	-1	percent	100	75.0	83.3	117	125	8.33
399589	1200784243	10-FEB-2005 17:20	DONE	89	-1	percent	100	75.0	83.3	117	125	8.33
399828	1200784836	11-FEB-2005 09:15	DONE	92	-1	percent	100	75.0	83.3	117	125	8.33
406056	1200799617	03-MAR-2005 19:09	DONE	99	-0.12	percent	100	75.0	83.3	117	125	8.33
407061	1200801919	09-MAR-2005 06:55	DONE	83	-2	percent	100	75.0	83.3	117	125	8.33
411084	1200811555	25-MAR-2005 15:34	DONE	100	-0.01	percent	100	75.0	83.3	117	125	8.33
411079	1200811539	27-MAR-2005 10:22	DONE	107	0.84	percent	100	75.0	83.3	117	125	8.33
411095	1200811624	27-MAR-2005 12:17	DONE	98	-0.22	percent	100	75.0	83.3	117	125	8.33
411096	1200811596	27-MAR-2005 13:59	DONE	85	-2	percent	100	75.0	83.3	117	125	8.33
411082	1200811549	28-MAR-2005 08:30	DONE	99	-0.17	percent	100	75.0	83.3	117	125	8.33
411081	1200811544	28-MAR-2005 12:15	DONE	97	-0.37	percent	100	75.0	83.3	117	125	8.33
412955	1200816027	31-MAR-2005 11:08	DONE	95	-0.6	percent	100	75.0	83.3	117	125	8.33
416592	1200824751	14-APR-2005 10:02	DONE	97	-0.36	percent	100	75.0	83.3	117	125	8.33
418044	1200828270	20-APR-2005 07:19	DONE	92	-0.91	percent	100	75.0	83.3	117	125	8.33
418049	1200828282	20-APR-2005 18:10	DONE	107	0.84	percent	100	75.0	83.3	117	125	8.33
420732	1200834636	29-APR-2005 15:09	DONE	91	-1	percent	100	75.0	83.3	117	125	8.33
420479	1200834014	30-APR-2005 13:54	DONE	109	1.1	percent	100	75.0	83.3	117	125	8.33
420733	1200834642	01-MAY-2005 20:43	DONE	94	-0.7	percent	100	75.0	83.3	117	125	8.33
420727	1200834633	01-MAY-2005 21:49	DONE	92	-0.99	percent	100	75.0	83.3	117	125	8.33
425591	1200846646	18-MAY-2005 07:36	DUSE	99	-0.12	percent	100	75.0	83.3	117	125	8.33

439055	1200879082	05-JUL-2005 15:03	DONE	103	0.37	percent	100	75.0	83.3	117	125	8.33
439482	1200880146	11-JUL-2005 11:42	DONE	98	-0.22	percent	100	75.0	83.3	117	125	8.33
446335	1200896857	28-JUL-2005 21:31	DONE	93	-0.84	percent	100	75.0	83.3	117	125	8.33
450952	1200907783	11-AUG-2005 19:15	DONE	93	-0.87	percent	100	75.0	83.3	117	125	8.33
454223	1200915333	19-AUG-2005 09:34	DONE	99	-0.12	percent	100	75.0	83.3	117	125	8.33
454227	1200915343	19-AUG-2005 21:57	DONE	98	-0.24	percent	100	75.0	83.3	117	125	8.33
458471	1200925741	02-SEP-2005 12:34	DONE	95	-0.57	percent	100	75.0	83.3	117	125	8.33

Radium-228 RER: Limits LCL = 0 UCL = 3



Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
510952	1201049299	04-APR-2006 01:41	DONE	1.98	1.1	dec	0.95	0	-0.856	2.76	3.00	0.9
510881	1201049181	04-APR-2006 06:40	DONE	0.85	-0.11	dec	0.95	0	-0.856	2.76	3.00	0.9
510153	1201047483	04-APR-2006 07:57	DONE	2.32	1.5	dec	0.95	0	-0.856	2.76	3.00	0.9
516989	1201062555	05-APR-2006 08:18	DONE	1.25	0.33	dec	0.95	0	-0.856	2.76	3.00	0.9
508902	1201044754	05-APR-2006 09:43	DONE	2.12	1.3	dec	0.95	0	-0.856	2.76	3.00	0.9
508900	1201044748	05-APR-2006 17:36	DONE	0.66	-0.32	dec	0.95	0	-0.856	2.76	3.00	0.9
517045	1201062677	05-APR-2006 22:28	DONE	00	-1	dec	0.95	0	-0.856	2.76	3.00	0.9
516236	1201060949	06-APR-2006 06:01	DONE	1.29	0.37	dec	0.95	0	-0.856	2.76	3.00	0.9
516986	1201062546	06-APR-2006 08:33	DONE	1.23	0.31	dec	0.95	0	-0.856	2.76	3.00	0.9
516987	1201062549	06-APR-2006 10:43	DONE	0.78	-0.19	dec	0.95	0	-0.856	2.76	3.00	0.9
513810	1201055628	06-APR-2006 10:52	DONE	0.46	-0.54	dec	0.95	0	-0.856	2.76	3.00	0.9
516991	1201062561	06-APR-2006 12:45	DONE	1.98	1.1	dec	0.95	0	-0.856	2.76	3.00	0.9
516993	1201062567	06-APR-2006 16:35	DONE	1.19	0.26	dec	0.95	0	-0.856	2.76	3.00	0.9
510976	1201049347	06-APR-2006 18:47	DUSE	0.44	-0.56	dec	0.95	0	-0.856	2.76	3.00	0.9
510982	1201049355	06-APR-2006 18:47	DONE	0.2	-0.83	dec	0.95	0	-0.856	2.76	3.00	0.9
516996	1201062573	07-APR-2006 06:09	DUSE	0.78	-0.19	dec	0.95	0	-0.856	2.76	3.00	0.9
517980	1201064809	07-APR-2006 06:16	DONE	0.33	-0.68	dec	0.95	0	-0.856	2.76	3.00	0.9
517983	1201064813	07-APR-2006 06:28	DONE	0.02	-1	dec	0.95	0	-0.856	2.76	3.00	0.9
516999	1201062579	07-APR-2006 08:20	DONE	0.34	-0.67	dec	0.95	0	-0.856	2.76	3.00	0.9
511760	1201051195	07-APR-2006 10:20	DONE	0.99	0.04	dec	0.95	0	-0.856	2.76	3.00	0.9
516996	1201062573	07-APR-2006 10:31	DONE	0.24	-0.79	dec	0.95	0	-0.856	2.76	3.00	0.9
513432	1201054906	07-APR-2006 21:54	DONE	0.06	-0.99	dec	0.95	0	-0.856	2.76	3.00	0.9
510976	1201049347	07-APR-2006 22:28	DONE	0.94	-0.02	dec	0.95	0	-0.856	2.76	3.00	0.9
517004	1201062585	08-APR-2006 16:02	DONE	0.67	-0.31	dec	0.95	0	-0.856	2.76	3.00	0.9
517006	1201062591	08-APR-2006 21:38	DONE	0.43	-0.58	dec	0.95	0	-0.856	2.76	3.00	0.9
517018	1201062615	09-APR-2006 21:10	DONE	1.32	0.41	dec	0.95	0	-0.856	2.76	3.00	0.9
513162	1201054360	09-APR-2006 21:34	DUSE	0.56	-0.43	dec	0.95	0	-0.856	2.76	3.00	0.9
517011	1201062603	10-APR-2006 06:23	DONE	1.39	0.48	dec	0.95	0	-0.856	2.76	3.00	0.9
517009	1201062597	10-APR-2006 10:48	DONE	4.9	4.4	dec	0.95	0	-0.856	2.76	3.00	0.9
517015	1201062609	10-APR-2006 10:51	DONE	0.98	0.03	dec	0.95	0	-0.856	2.76	3.00	0.9
512595	1201053118	10-APR-2006 13:18	DONE	1.17	0.24	dec	0.95	0	-0.856	2.76	3.00	0.9
513799	1201055604	10-APR-2006 15:42	DONE	0.15	-0.89	dec	0.95	0	-0.856	2.76	3.00	0.9
513054	1201054081	11-APR-2006 10:21	DONE	0.2	-0.83	dec	0.95	0	-0.856	2.76	3.00	0.9
519499	1201068199	11-APR-2006 16:44	DONE	0.35	-0.67	dec	0.95	0	-0.856	2.76	3.00	0.9
519008	1201067117	11-APR-2006 19:22	DUSE	1.04	0.1	dec	0.95	0	-0.856	2.76	3.00	0.9
513058	1201054087	11-APR-2006 21:43	DONE	1.81	0.95	dec	0.95	0	-0.856	2.76	3.00	0.9
518359	1201065660	11-APR-2006 21:47	DUSE	1.39	0.48	dec	0.95	0	-0.856	2.76	3.00	0.9
513802	1201055608	11-APR-2006 23:19	DONE	0.01	-1	dec	0.95	0	-0.856	2.76	3.00	0.9
513780	1201055550	11-APR-2006 23:45	DONE	0.3	-0.72	dec	0.95	0	-0.856	2.76	3.00	0.9

SPC Graph for Alpha SpecUranium in Solids 4/10/2006 Uranium-233/234 BLANK

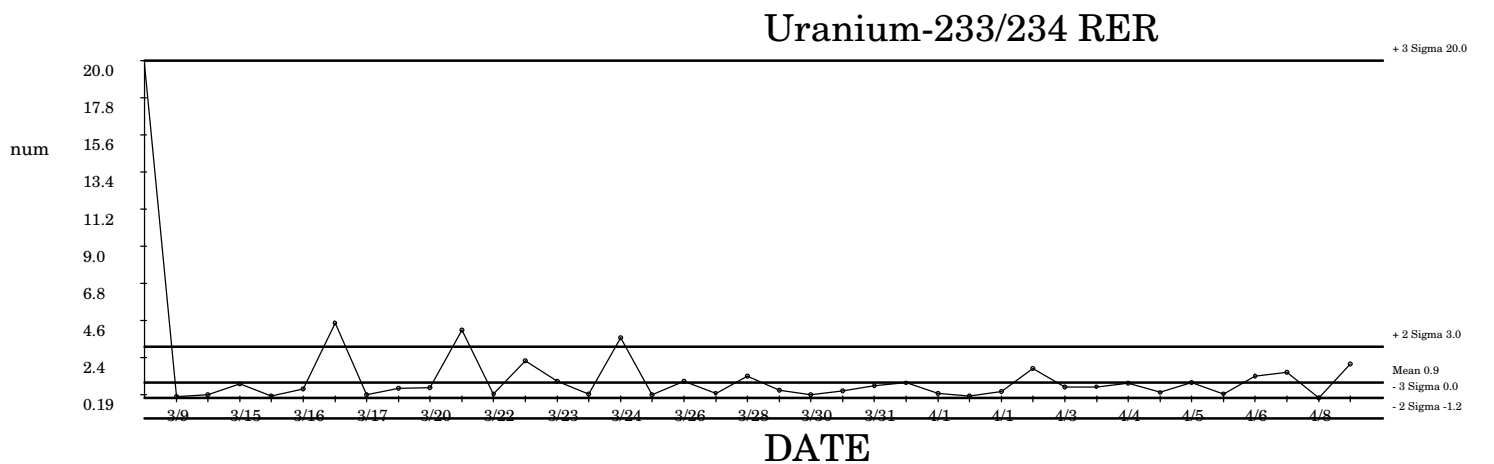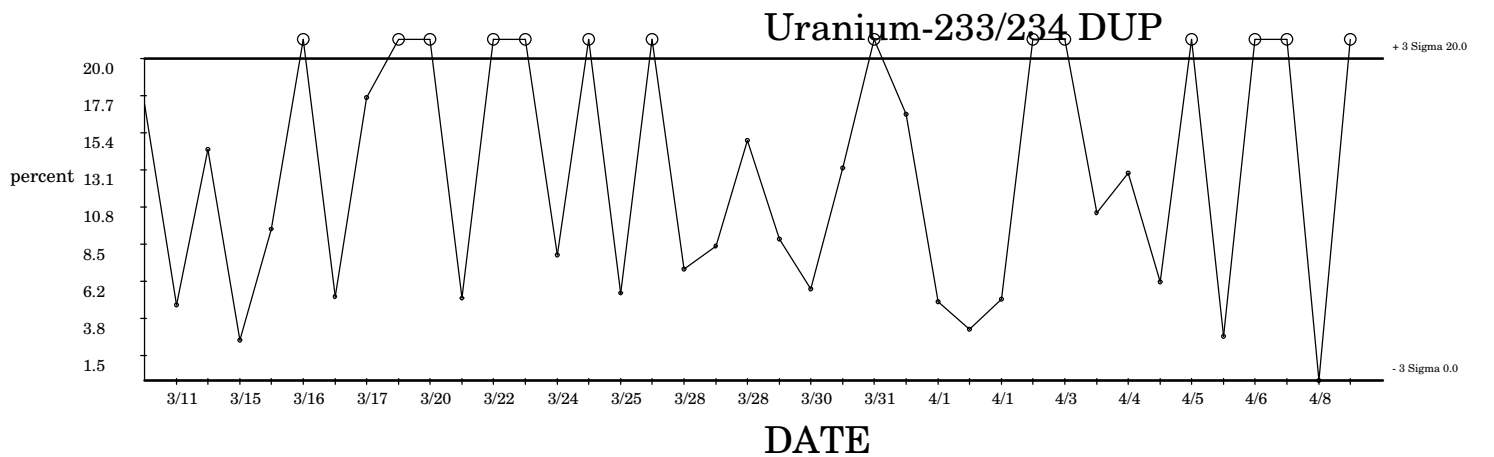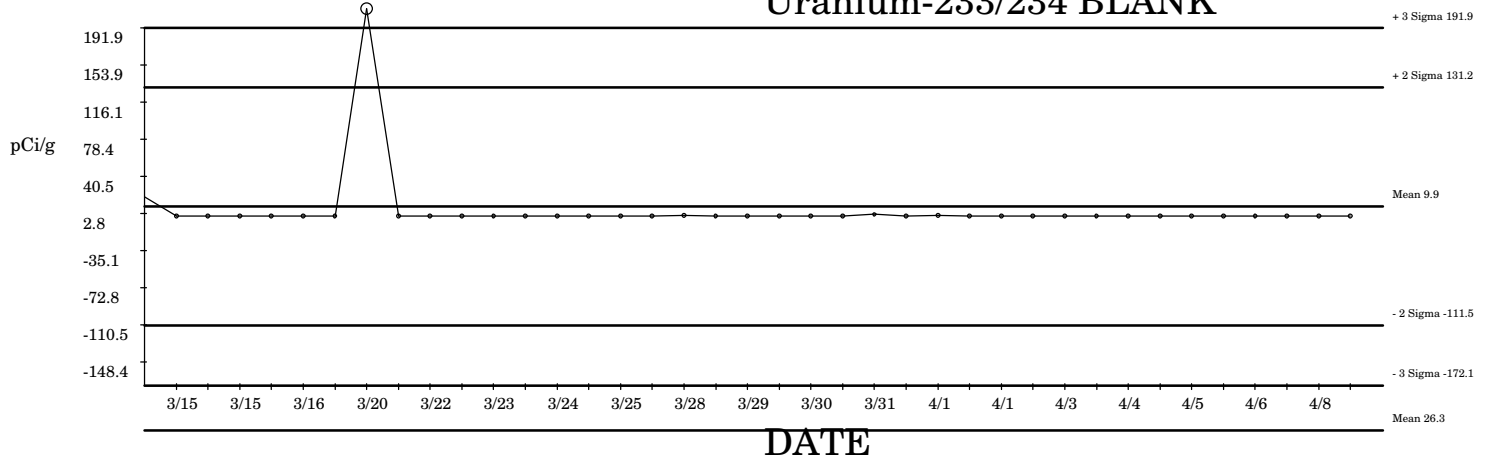

○ Denotes Outlier


SPC Graph for Alpha SpecUranium in Solids 4/10/2006 Uranium-235/236 BLANK

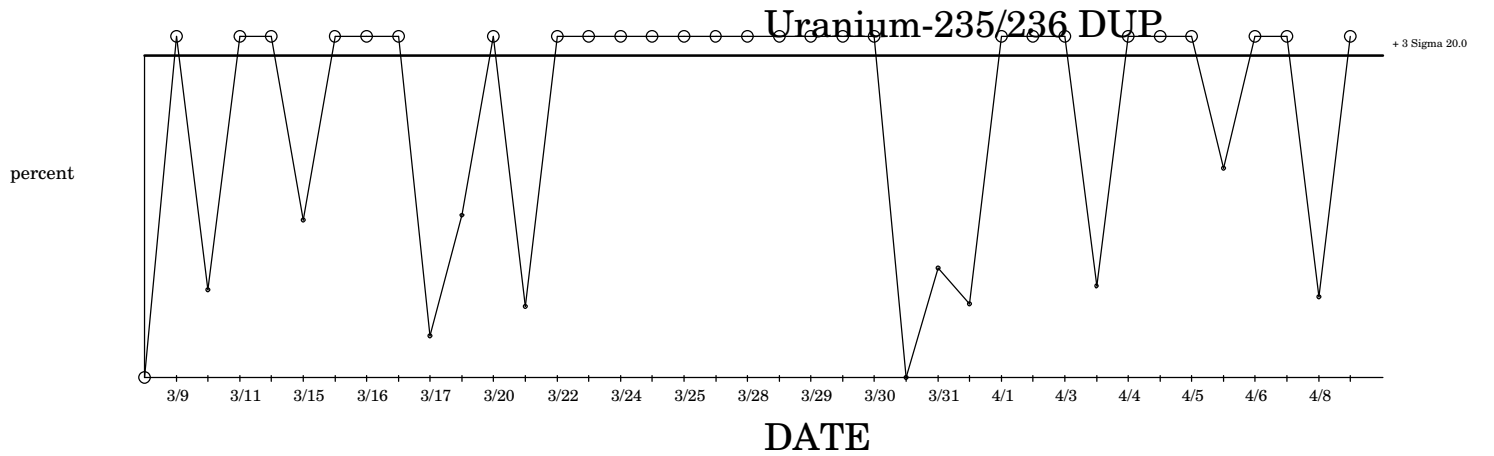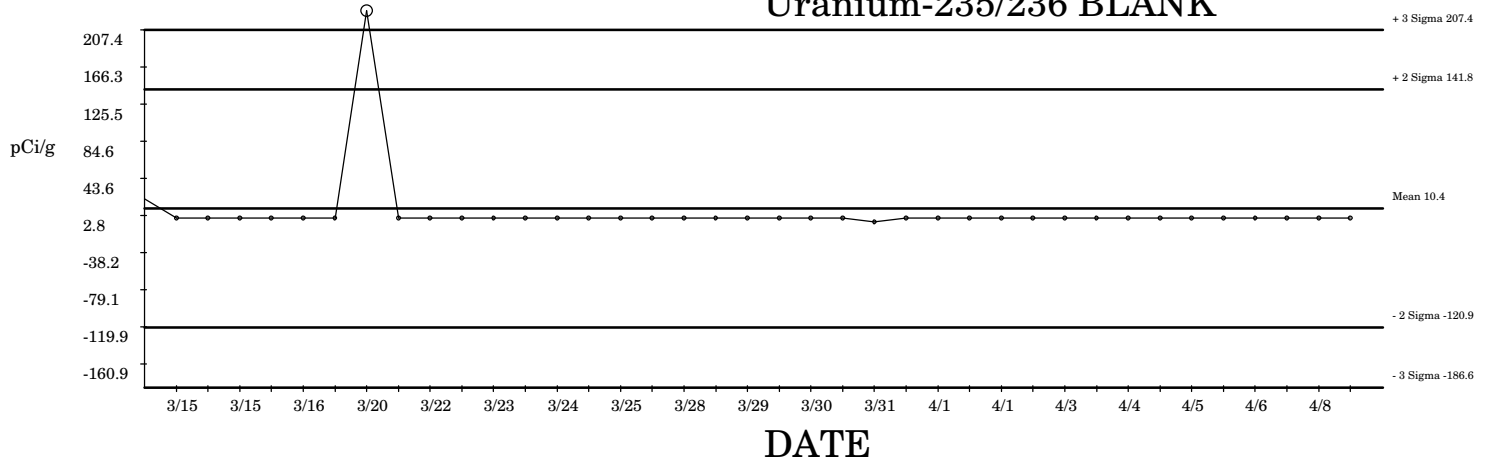

○ Denotes Outlier




Uranium-235/236 RER

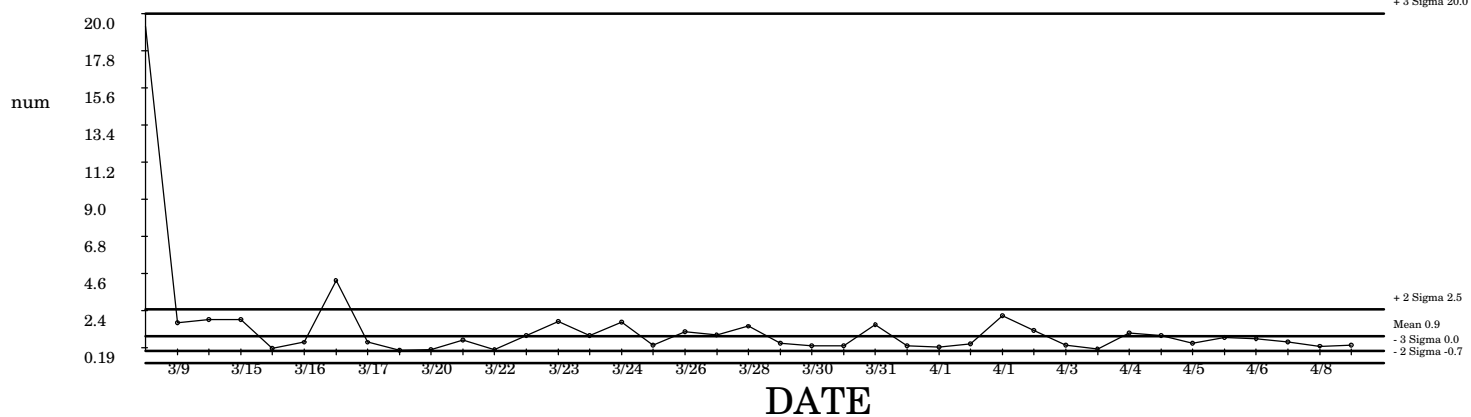





Uranium-238 LCS

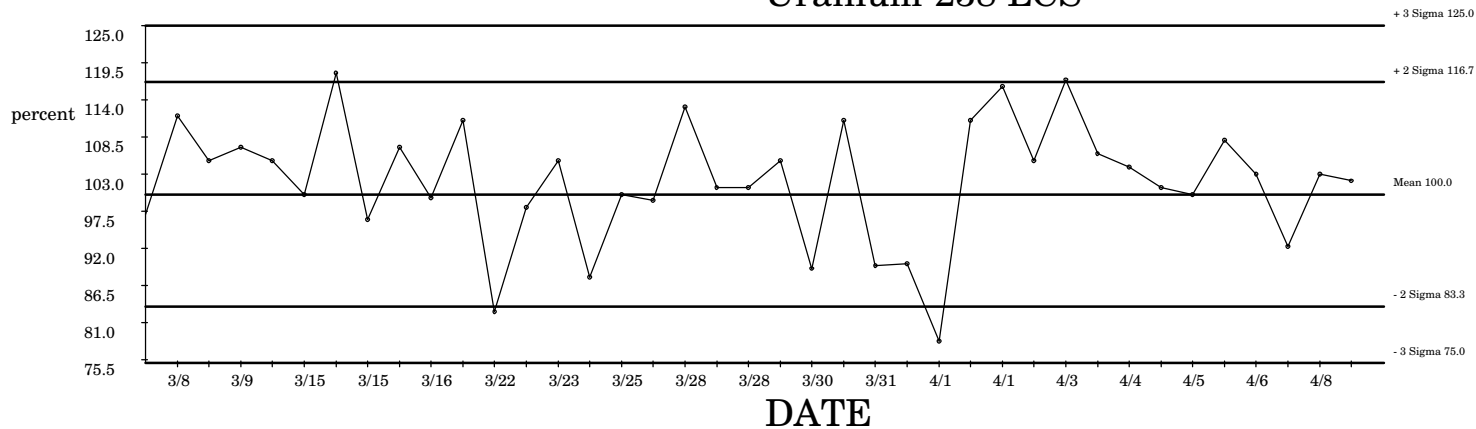

Uranium-238 RER

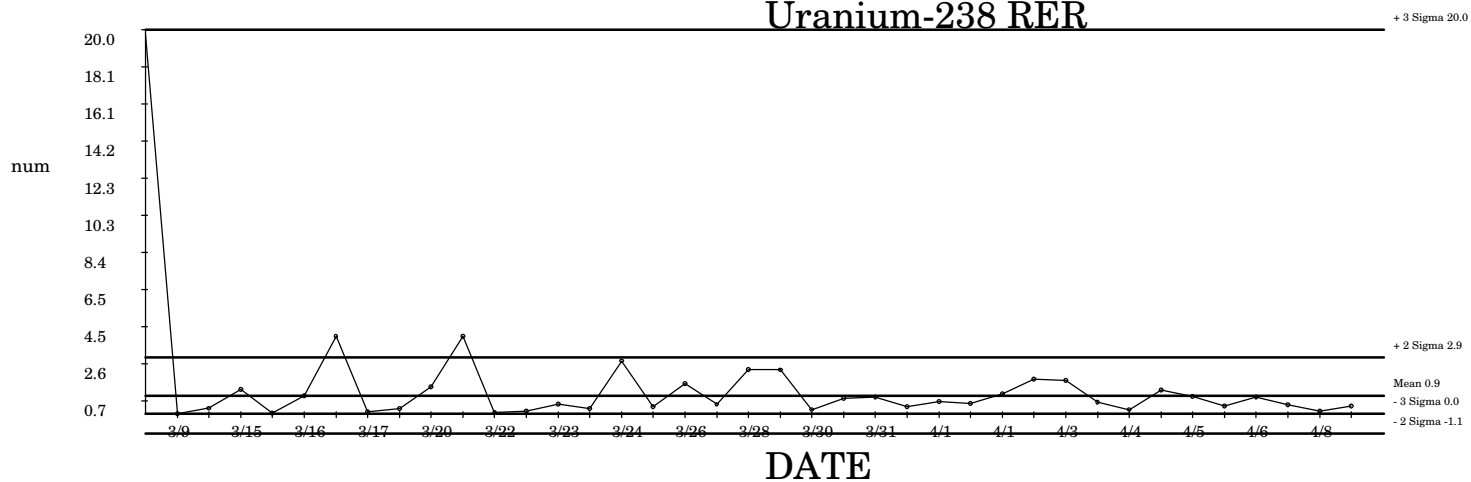

SPC Graph for Alpha SpecUranium in Solids 4/10/2006 Uranium-238 SPIKE

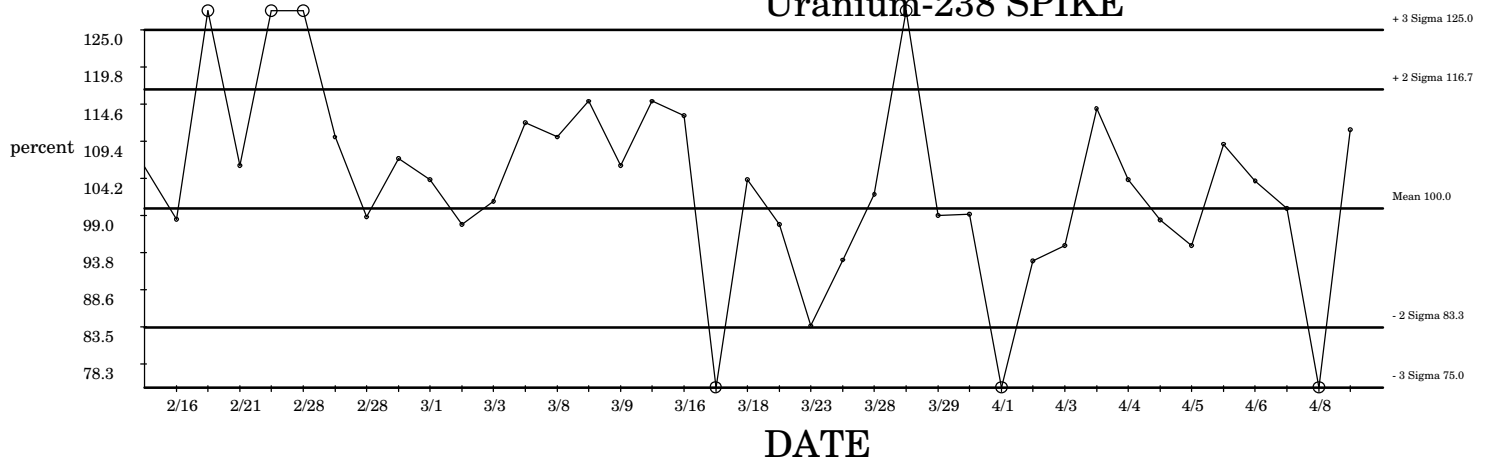

○ Denotes Outlier

Data used for Alpha Spec Uranium in Solids 11-APR-2006

Uranium-233/234 BLANK: Limits LCL = -172.1 UCL = 191.9

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
510234	1201047741	11-MAR-2006 14:29	DUSE	0	-0.16	pCi/g	9.86	-170	-110	131	192	60.7
509833	1201046785	15-MAR-2006 09:16	DONE	0	-0.16	pCi/g	9.86	-170	-110	131	192	60.7
511711	1201051087	15-MAR-2006 09:16	DONE	0	-0.16	pCi/g	9.86	-170	-110	131	192	60.7
510648	1201048635	15-MAR-2006 12:44	DONE	0	-0.16	pCi/g	9.86	-170	-110	131	192	60.7
511205	1201049867	15-MAR-2006 16:54	DONE	0	-0.16	pCi/g	9.86	-170	-110	131	192	60.7
510653	1201048649	16-MAR-2006 14:20	DONE	0	-0.16	pCi/g	9.86	-170	-110	131	192	60.7
511197	1201049839	17-MAR-2006 13:41	DUSE	0	-0.16	pCi/g	9.86	-170	-110	131	192	60.7
512186	1201052164	20-MAR-2006 16:57	DONE	379	6.1	pCi/g	9.86	-170	-110	131	192	60.7
511556	1201050731	20-MAR-2006 20:55	DUSE	0	-0.16	pCi/g	9.86	-170	-110	131	192	60.7
513065	1201054107	22-MAR-2006 14:23	DONE	0	-0.16	pCi/g	9.86	-170	-110	131	192	60.7
512000	1201051707	22-MAR-2006 19:22	DONE	0	-0.16	pCi/g	9.86	-170	-110	131	192	60.7
513417	1201054860	23-MAR-2006 23:50	DONE	0	-0.16	pCi/g	9.86	-170	-110	131	192	60.7
513967	1201055907	24-MAR-2006 17:20	DONE	0	-0.16	pCi/g	9.86	-170	-110	131	192	60.7
511995	1201051696	24-MAR-2006 17:20	DUSE	0	-0.16	pCi/g	9.86	-170	-110	131	192	60.7
511573	1201050778	24-MAR-2006 19:41	DUSE	0	-0.16	pCi/g	9.86	-170	-110	131	192	60.7
511656	1201050971	25-MAR-2006 10:35	DONE	0	-0.16	pCi/g	9.86	-170	-110	131	192	60.7
513419	1201054868	26-MAR-2006 07:39	DONE	0	-0.16	pCi/g	9.86	-170	-110	131	192	60.7
513434	1201054911	28-MAR-2006 11:41	DONE	1	-0.15	pCi/g	9.86	-170	-110	131	192	60.7
506038	1201037885	28-MAR-2006 16:43	DONE	0	-0.16	pCi/g	9.86	-170	-110	131	192	60.7
515154	1201058499	29-MAR-2006 08:48	DONE	0	-0.16	pCi/g	9.86	-170	-110	131	192	60.7
514145	1201056277	29-MAR-2006 22:27	DONE	0	-0.16	pCi/g	9.86	-170	-110	131	192	60.7
515145	1201058488	30-MAR-2006 14:53	DONE	0	-0.16	pCi/g	9.86	-170	-110	131	192	60.7
515262	1201058713	31-MAR-2006 00:27	DONE	0	-0.16	pCi/g	9.86	-170	-110	131	192	60.7
512056	1201051825	31-MAR-2006 13:48	DONE	2	-0.13	pCi/g	9.86	-170	-110	131	192	60.7
512024	1201051755	31-MAR-2006 15:55	DONE	0	-0.16	pCi/g	9.86	-170	-110	131	192	60.7
514172	1201056341	01-APR-2006 09:22	DONE	1	-0.15	pCi/g	9.86	-170	-110	131	192	60.7
512045	1201051809	01-APR-2006 13:50	DONE	0	-0.16	pCi/g	9.86	-170	-110	131	192	60.7
515259	1201058705	01-APR-2006 14:24	DONE	0	-0.16	pCi/g	9.86	-170	-110	131	192	60.7
515558	1201059454	03-APR-2006 06:56	DONE	0	-0.16	pCi/g	9.86	-170	-110	131	192	60.7
515551	1201059426	03-APR-2006 06:56	DONE	0	-0.16	pCi/g	9.86	-170	-110	131	192	60.7
516219	1201060904	04-APR-2006 07:47	DONE	0	-0.16	pCi/g	9.86	-170	-110	131	192	60.7
512063	1201051849	04-APR-2006 10:18	DONE	0	-0.16	pCi/g	9.86	-170	-110	131	192	60.7
515564	1201059470	04-APR-2006 16:37	DONE	0	-0.16	pCi/g	9.86	-170	-110	131	192	60.7
512069	1201051877	05-APR-2006 09:52	DONE	0	-0.16	pCi/g	9.86	-170	-110	131	192	60.7
517591	1201063933	05-APR-2006 21:53	DONE	0	-0.16	pCi/g	9.86	-170	-110	131	192	60.7
517143	1201062895	06-APR-2006 08:11	DONE	0	-0.16	pCi/g	9.86	-170	-110	131	192	60.7
516346	1201061153	06-APR-2006 13:23	DONE	0	-0.16	pCi/g	9.86	-170	-110	131	192	60.7
518034	1201064928	08-APR-2006 15:43	DONE	0	-0.16	pCi/g	9.86	-170	-110	131	192	60.7
517155	1201062931	08-APR-2006 15:43	DONE	0	-0.16	pCi/g	9.86	-170	-110	131	192	60.7

Uranium-233/234 DUP: Limits LCL = 0 UCL = 20

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
508590	1201044014	09-MAR-2006 18:21	DONE	3	-0.69	percent	26.3	0	-42	94.1	20.0	33.9
510234	1201047742	11-MAR-2006 14:29	DUSE	5	-0.64	percent	26.3	0	-42	94.1	20.0	33.9
511711	1201051088	15-MAR-2006 09:16	DONE	14	-0.35	percent	26.3	0	-42	94.1	20.0	33.9
511205	1201049868	15-MAR-2006 16:54	DONE	3	-0.7	percent	26.3	0	-42	94.1	20.0	33.9

510648	1201048636	16-MAR-2006 09:25	DONE	9	-0.5	percent	26.3	0	-42	94.1	20.0	33.9
509833	1201046786	16-MAR-2006 10:10	DONE	55	0.84	percent	26.3	0	-42	94.1	20.0	33.9
510653	1201048650	17-MAR-2006 13:41	DONE	5	-0.62	percent	26.3	0	-42	94.1	20.0	33.9
511197	1201049840	17-MAR-2006 15:33	DUSE	18	-0.26	percent	26.3	0	-42	94.1	20.0	33.9
512186	1201052165	20-MAR-2006 16:57	DONE	34	0.22	percent	26.3	0	-42	94.1	20.0	33.9
511556	1201050732	20-MAR-2006 20:55	DUSE	121	2.8	percent	26.3	0	-42	94.1	20.0	33.9
513065	1201054108	22-MAR-2006 14:23	DONE	5	-0.63	percent	26.3	0	-42	94.1	20.0	33.9
512000	1201051708	22-MAR-2006 19:22	DONE	40	0.42	percent	26.3	0	-42	94.1	20.0	33.9
513417	1201054861	23-MAR-2006 23:50	DONE	41	0.43	percent	26.3	0	-42	94.1	20.0	33.9
513967	1201055908	24-MAR-2006 17:20	DONE	8	-0.55	percent	26.3	0	-42	94.1	20.0	33.9
511995	1201051697	24-MAR-2006 17:20	DUSE	26	-0.01	percent	26.3	0	-42	94.1	20.0	33.9
511656	1201050972	25-MAR-2006 10:35	DONE	5	-0.62	percent	26.3	0	-42	94.1	20.0	33.9
513419	1201054869	26-MAR-2006 07:39	DONE	44	0.53	percent	26.3	0	-42	94.1	20.0	33.9
513434	1201054912	28-MAR-2006 11:41	DONE	7	-0.57	percent	26.3	0	-42	94.1	20.0	33.9
506038	1201037886	28-MAR-2006 16:43	DONE	8	-0.53	percent	26.3	0	-42	94.1	20.0	33.9
515154	1201058500	28-MAR-2006 22:08	DONE	15	-0.34	percent	26.3	0	-42	94.1	20.0	33.9
514145	1201056278	29-MAR-2006 22:27	DONE	9	-0.52	percent	26.3	0	-42	94.1	20.0	33.9
512024	1201051756	30-MAR-2006 14:07	DONE	6	-0.61	percent	26.3	0	-42	94.1	20.0	33.9
515145	1201058489	30-MAR-2006 14:53	DONE	13	-0.39	percent	26.3	0	-42	94.1	20.0	33.9
515262	1201058714	31-MAR-2006 00:27	DONE	30	0.1	percent	26.3	0	-42	94.1	20.0	33.9
512056	1201051826	31-MAR-2006 13:48	DONE	17	-0.29	percent	26.3	0	-42	94.1	20.0	33.9
514172	1201056342	01-APR-2006 09:22	DONE	5	-0.63	percent	26.3	0	-42	94.1	20.0	33.9
512045	1201051810	01-APR-2006 13:50	DONE	3	-0.68	percent	26.3	0	-42	94.1	20.0	33.9
515259	1201058706	01-APR-2006 14:24	DONE	5	-0.63	percent	26.3	0	-42	94.1	20.0	33.9
515558	1201059455	03-APR-2006 06:56	DONE	78	1.5	percent	26.3	0	-42	94.1	20.0	33.9
515551	1201059427	03-APR-2006 06:56	DONE	131	3.1	percent	26.3	0	-42	94.1	20.0	33.9
516219	1201060905	04-APR-2006 07:47	DONE	10	-0.47	percent	26.3	0	-42	94.1	20.0	33.9
512063	1201051850	04-APR-2006 10:18	DONE	13	-0.4	percent	26.3	0	-42	94.1	20.0	33.9
512069	1201051878	05-APR-2006 09:52	DONE	6	-0.6	percent	26.3	0	-42	94.1	20.0	33.9
515564	1201059471	05-APR-2006 15:35	DONE	27	0.01	percent	26.3	0	-42	94.1	20.0	33.9
517591	1201063934	05-APR-2006 21:53	DONE	3	-0.7	percent	26.3	0	-42	94.1	20.0	33.9
517143	1201062896	06-APR-2006 08:11	DONE	123	2.9	percent	26.3	0	-42	94.1	20.0	33.9
516346	1201061154	06-APR-2006 13:23	DONE	25	-0.04	percent	26.3	0	-42	94.1	20.0	33.9
518034	1201064929	08-APR-2006 15:43	DONE	0	-0.78	percent	26.3	0	-42	94.1	20.0	33.9
517155	1201062932	08-APR-2006 15:43	DONE	57	0.91	percent	26.3	0	-42	94.1	20.0	33.9

Uranium-233/234 RER: Limits LCL = 0 UCL = 20

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
508588	1201044006	09-MAR-2006 15:47	DONE	0.22	-0.65	num	0.91	0	-1.2	3.03	20.0	1.06
508590	1201044014	09-MAR-2006 18:21	DONE	0.09	-0.77	num	0.91	0	-1.2	3.03	20.0	1.06
510234	1201047742	11-MAR-2006 14:29	DUSE	0.19	-0.68	num	0.91	0	-1.2	3.03	20.0	1.06
511711	1201051088	15-MAR-2006 09:16	DONE	0.84	-0.07	num	0.91	0	-1.2	3.03	20.0	1.06
511205	1201049868	15-MAR-2006 16:54	DONE	0.1	-0.76	num	0.91	0	-1.2	3.03	20.0	1.06
510648	1201048636	16-MAR-2006 09:25	DONE	0.52	-0.36	num	0.91	0	-1.2	3.03	20.0	1.06
509833	1201046786	16-MAR-2006 10:10	DONE	4.43	3.3	num	0.91	0	-1.2	3.03	20.0	1.06
510653	1201048650	17-MAR-2006 13:41	DONE	0.19	-0.68	num	0.91	0	-1.2	3.03	20.0	1.06
511197	1201049840	17-MAR-2006 15:33	DUSE	0.57	-0.32	num	0.91	0	-1.2	3.03	20.0	1.06
512186	1201052165	20-MAR-2006 16:57	DONE	0.6	-0.29	num	0.91	0	-1.2	3.03	20.0	1.06
511556	1201050732	20-MAR-2006 20:55	DUSE	4.02	2.9	num	0.91	0	-1.2	3.03	20.0	1.06
513065	1201054108	22-MAR-2006 14:23	DONE	0.22	-0.65	num	0.91	0	-1.2	3.03	20.0	1.06

512000	1201051708	22-MAR-2006 19:22	DONE	2.2	1.2	num	0.91	0	-1.2	3.03	20.0	1.06
513417	1201054861	23-MAR-2006 23:50	DONE	0.99	0.08	num	0.91	0	-1.2	3.03	20.0	1.06
513967	1201055908	24-MAR-2006 17:20	DONE	0.22	-0.65	num	0.91	0	-1.2	3.03	20.0	1.06
511995	1201051697	24-MAR-2006 17:20	DUSE	3.58	2.5	num	0.91	0	-1.2	3.03	20.0	1.06
511656	1201050972	25-MAR-2006 10:35	DONE	0.18	-0.69	num	0.91	0	-1.2	3.03	20.0	1.06
513419	1201054869	26-MAR-2006 07:39	DONE	0.99	0.08	num	0.91	0	-1.2	3.03	20.0	1.06
513434	1201054912	28-MAR-2006 11:41	DONE	0.28	-0.59	num	0.91	0	-1.2	3.03	20.0	1.06
515154	1201058500	28-MAR-2006 22:08	DONE	1.3	0.37	num	0.91	0	-1.2	3.03	20.0	1.06
514145	1201056278	29-MAR-2006 22:27	DONE	0.46	-0.43	num	0.91	0	-1.2	3.03	20.0	1.06
512024	1201051756	30-MAR-2006 14:07	DONE	0.19	-0.68	num	0.91	0	-1.2	3.03	20.0	1.06
515145	1201058489	30-MAR-2006 14:53	DONE	0.42	-0.47	num	0.91	0	-1.2	3.03	20.0	1.06
515262	1201058714	31-MAR-2006 00:27	DONE	0.73	-0.17	num	0.91	0	-1.2	3.03	20.0	1.06
512056	1201051826	31-MAR-2006 13:48	DONE	0.89	-0.02	num	0.91	0	-1.2	3.03	20.0	1.06
514172	1201056342	01-APR-2006 09:22	DONE	0.26	-0.61	num	0.91	0	-1.2	3.03	20.0	1.06
512045	1201051810	01-APR-2006 13:50	DONE	0.12	-0.75	num	0.91	0	-1.2	3.03	20.0	1.06
515259	1201058706	01-APR-2006 14:24	DONE	0.39	-0.49	num	0.91	0	-1.2	3.03	20.0	1.06
515558	1201059455	03-APR-2006 06:56	DONE	1.76	0.8	num	0.91	0	-1.2	3.03	20.0	1.06
515551	1201059427	03-APR-2006 06:56	DONE	0.65	-0.25	num	0.91	0	-1.2	3.03	20.0	1.06
516219	1201060905	04-APR-2006 07:47	DONE	0.66	-0.23	num	0.91	0	-1.2	3.03	20.0	1.06
512063	1201051850	04-APR-2006 10:18	DONE	0.86	-0.04	num	0.91	0	-1.2	3.03	20.0	1.06
512069	1201051878	05-APR-2006 09:52	DONE	0.32	-0.55	num	0.91	0	-1.2	3.03	20.0	1.06
515564	1201059471	05-APR-2006 15:35	DONE	0.91	00	num	0.91	0	-1.2	3.03	20.0	1.06
517591	1201063934	05-APR-2006 21:53	DONE	0.25	-0.62	num	0.91	0	-1.2	3.03	20.0	1.06
517143	1201062896	06-APR-2006 08:11	DONE	1.31	0.38	num	0.91	0	-1.2	3.03	20.0	1.06
516346	1201061154	06-APR-2006 13:23	DONE	1.51	0.57	num	0.91	0	-1.2	3.03	20.0	1.06
518034	1201064929	08-APR-2006 15:43	DONE	0	-0.86	num	0.91	0	-1.2	3.03	20.0	1.06
517155	1201062932	08-APR-2006 15:43	DONE	2.02	1	num	0.91	0	-1.2	3.03	20.0	1.06

Uranium-235/236 BLANK: Limits LCL = -186.6 UCL = 207.4

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
510234	1201047741	11-MAR-2006 14:29	DUSE	0	-0.16	pCi/g	10.4	-190	-120	142	207	65.7
509833	1201046785	15-MAR-2006 09:16	DONE	0	-0.16	pCi/g	10.4	-190	-120	142	207	65.7
511711	1201051087	15-MAR-2006 09:16	DONE	0	-0.16	pCi/g	10.4	-190	-120	142	207	65.7
510648	1201048635	15-MAR-2006 12:44	DONE	0	-0.16	pCi/g	10.4	-190	-120	142	207	65.7
511205	1201049867	15-MAR-2006 16:54	DONE	0	-0.16	pCi/g	10.4	-190	-120	142	207	65.7
510653	1201048649	16-MAR-2006 14:20	DONE	0	-0.16	pCi/g	10.4	-190	-120	142	207	65.7
511197	1201049839	17-MAR-2006 13:41	DUSE	0	-0.16	pCi/g	10.4	-190	-120	142	207	65.7
512186	1201052164	20-MAR-2006 16:57	DONE	410	6.1	pCi/g	10.4	-190	-120	142	207	65.7
511556	1201050731	20-MAR-2006 20:55	DUSE	0	-0.16	pCi/g	10.4	-190	-120	142	207	65.7
513065	1201054107	22-MAR-2006 14:23	DONE	0	-0.16	pCi/g	10.4	-190	-120	142	207	65.7
512000	1201051707	22-MAR-2006 19:22	DONE	0	-0.16	pCi/g	10.4	-190	-120	142	207	65.7
513417	1201054860	23-MAR-2006 23:50	DONE	0	-0.16	pCi/g	10.4	-190	-120	142	207	65.7
513967	1201055907	24-MAR-2006 17:20	DONE	0	-0.16	pCi/g	10.4	-190	-120	142	207	65.7
511995	1201051696	24-MAR-2006 17:20	DUSE	0	-0.16	pCi/g	10.4	-190	-120	142	207	65.7
511573	1201050778	24-MAR-2006 19:41	DUSE	0	-0.16	pCi/g	10.4	-190	-120	142	207	65.7
511656	1201050971	25-MAR-2006 10:35	DONE	0	-0.16	pCi/g	10.4	-190	-120	142	207	65.7
513419	1201054868	26-MAR-2006 07:39	DONE	0	-0.16	pCi/g	10.4	-190	-120	142	207	65.7
513434	1201054911	28-MAR-2006 11:41	DONE	0	-0.16	pCi/g	10.4	-190	-120	142	207	65.7
506038	1201037885	28-MAR-2006 16:43	DUSE	0	-0.16	pCi/g	10.4	-190	-120	142	207	65.7
515154	1201058499	29-MAR-2006 08:48	DONE	0	-0.16	pCi/g	10.4	-190	-120	142	207	65.7

514145	1201056277	29-MAR-2006 22:27	DONE	0	-0.16	pCi/g	10.4	-190	-120	142	207	65.7
515145	1201058488	30-MAR-2006 14:53	DONE	0	-0.16	pCi/g	10.4	-190	-120	142	207	65.7
515262	1201058713	31-MAR-2006 00:27	DONE	0	-0.16	pCi/g	10.4	-190	-120	142	207	65.7
512056	1201051825	31-MAR-2006 13:48	DONE	-4	-0.22	pCi/g	10.4	-190	-120	142	207	65.7
512024	1201051755	31-MAR-2006 15:55	DUSE	0	-0.16	pCi/g	10.4	-190	-120	142	207	65.7
514172	1201056341	01-APR-2006 09:22	DONE	0	-0.16	pCi/g	10.4	-190	-120	142	207	65.7
512045	1201051809	01-APR-2006 13:50	DUSE	0	-0.16	pCi/g	10.4	-190	-120	142	207	65.7
515259	1201058705	01-APR-2006 14:24	DONE	0	-0.16	pCi/g	10.4	-190	-120	142	207	65.7
515558	1201059454	03-APR-2006 06:56	DONE	0	-0.16	pCi/g	10.4	-190	-120	142	207	65.7
515551	1201059426	03-APR-2006 06:56	DONE	0	-0.16	pCi/g	10.4	-190	-120	142	207	65.7
516219	1201060904	04-APR-2006 07:47	DONE	0	-0.16	pCi/g	10.4	-190	-120	142	207	65.7
512063	1201051849	04-APR-2006 10:18	DONE	0	-0.16	pCi/g	10.4	-190	-120	142	207	65.7
515564	1201059470	04-APR-2006 16:37	DONE	0	-0.16	pCi/g	10.4	-190	-120	142	207	65.7
512069	1201051877	05-APR-2006 09:52	DONE	0	-0.16	pCi/g	10.4	-190	-120	142	207	65.7
517591	1201063933	05-APR-2006 21:53	DONE	0	-0.16	pCi/g	10.4	-190	-120	142	207	65.7
517143	1201062895	06-APR-2006 08:11	DONE	0	-0.16	pCi/g	10.4	-190	-120	142	207	65.7
516346	1201061153	06-APR-2006 13:23	DONE	0	-0.16	pCi/g	10.4	-190	-120	142	207	65.7
518034	1201064928	08-APR-2006 15:43	DONE	0	-0.16	pCi/g	10.4	-190	-120	142	207	65.7
517155	1201062931	08-APR-2006 15:43	DONE	0	-0.16	pCi/g	10.4	-190	-120	142	207	65.7

Uranium-235/236 DUP: Limits LCL = 0 UCL = 20

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
509121	1201045269	09-MAR-2006 15:47	DONE	63	-0.04	percent	67.2	0	-100	239	20.0	86
508588	1201044006	09-MAR-2006 15:47	DONE	94	0.31	percent	67.2	0	-100	239	20.0	86
508590	1201044014	09-MAR-2006 18:21	DONE	5	-0.72	percent	67.2	0	-100	239	20.0	86
510234	1201047742	11-MAR-2006 14:29	DUSE	94	0.31	percent	67.2	0	-100	239	20.0	86
511711	1201051088	15-MAR-2006 09:16	DONE	201	1.6	percent	67.2	0	-100	239	20.0	86
511205	1201049868	15-MAR-2006 16:54	DONE	10	-0.67	percent	67.2	0	-100	239	20.0	86
510648	1201048636	16-MAR-2006 09:25	DONE	33	-0.4	percent	67.2	0	-100	239	20.0	86
509833	1201046786	16-MAR-2006 10:10	DONE	96	0.33	percent	67.2	0	-100	239	20.0	86
510653	1201048650	17-MAR-2006 13:41	DONE	38	-0.34	percent	67.2	0	-100	239	20.0	86
511197	1201049840	17-MAR-2006 15:33	DUSE	3	-0.75	percent	67.2	0	-100	239	20.0	86
512186	1201052165	20-MAR-2006 16:57	DONE	10	-0.66	percent	67.2	0	-100	239	20.0	86
511556	1201050732	20-MAR-2006 20:55	DUSE	60	-0.08	percent	67.2	0	-100	239	20.0	86
513065	1201054108	22-MAR-2006 14:23	DONE	4	-0.73	percent	67.2	0	-100	239	20.0	86
512000	1201051708	22-MAR-2006 19:22	DONE	74	0.08	percent	67.2	0	-100	239	20.0	86
513417	1201054861	23-MAR-2006 23:50	DONE	228	1.9	percent	67.2	0	-100	239	20.0	86
513967	1201055908	24-MAR-2006 17:20	DONE	104	0.43	percent	67.2	0	-100	239	20.0	86
511995	1201051697	24-MAR-2006 17:20	DUSE	28	-0.46	percent	67.2	0	-100	239	20.0	86
511656	1201050972	25-MAR-2006 10:35	DONE	38	-0.33	percent	67.2	0	-100	239	20.0	86
513419	1201054869	26-MAR-2006 07:39	DONE	167	1.2	percent	67.2	0	-100	239	20.0	86
513434	1201054912	28-MAR-2006 11:41	DONE	25	-0.49	percent	67.2	0	-100	239	20.0	86
515154	1201058500	28-MAR-2006 22:08	DONE	54	-0.15	percent	67.2	0	-100	239	20.0	86
514145	1201056278	29-MAR-2006 22:27	DONE	70	0.03	percent	67.2	0	-100	239	20.0	86
512024	1201051756	30-MAR-2006 14:07	DUSE	25	-0.49	percent	67.2	0	-100	239	20.0	86
515145	1201058489	30-MAR-2006 14:53	DONE	30	-0.43	percent	67.2	0	-100	239	20.0	86
515262	1201058714	31-MAR-2006 00:27	DONE	0	-0.78	percent	67.2	0	-100	239	20.0	86
512056	1201051826	31-MAR-2006 13:48	DONE	7	-0.7	percent	67.2	0	-100	239	20.0	86
514172	1201056342	01-APR-2006 09:22	DONE	5	-0.73	percent	67.2	0	-100	239	20.0	86
512045	1201051810	01-APR-2006 13:50	DUSE	43	-0.28	percent	67.2	0	-100	239	20.0	86

515259	1201058706	01-APR-2006 14:24	DONE	70	0.03	percent	67.2	0	-100	239	20.0	86
515558	1201059455	03-APR-2006 06:56	DONE	324	3	percent	67.2	0	-100	239	20.0	86
516219	1201060905	04-APR-2006 07:47	DONE	6	-0.71	percent	67.2	0	-100	239	20.0	86
512063	1201051850	04-APR-2006 10:18	DONE	40	-0.31	percent	67.2	0	-100	239	20.0	86
512069	1201051878	05-APR-2006 09:52	DONE	75	0.09	percent	67.2	0	-100	239	20.0	86
515564	1201059471	05-APR-2006 15:35	DONE	37	-0.35	percent	67.2	0	-100	239	20.0	86
517591	1201063934	05-APR-2006 21:53	DONE	13	-0.63	percent	67.2	0	-100	239	20.0	86
517143	1201062896	06-APR-2006 08:11	DONE	386	3.7	percent	67.2	0	-100	239	20.0	86
516346	1201061154	06-APR-2006 13:23	DONE	25	-0.49	percent	67.2	0	-100	239	20.0	86
518034	1201064929	08-APR-2006 15:43	DONE	5	-0.72	percent	67.2	0	-100	239	20.0	86
517155	1201062932	08-APR-2006 15:43	DONE	28	-0.45	percent	67.2	0	-100	239	20.0	86

Uranium-235/236 RER: Limits LCL = 0 UCL = 20

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stddev
508588	1201044006	09-MAR-2006 15:47	DONE	0.74	-0.16	num	0.87	0	-0.721	2.47	20.0	0.8
508590	1201044014	09-MAR-2006 18:21	DONE	1.67	1	num	0.87	0	-0.721	2.47	20.0	0.8
510234	1201047742	11-MAR-2006 14:29	DUSE	1.86	1.2	num	0.87	0	-0.721	2.47	20.0	0.8
511711	1201051088	15-MAR-2006 09:16	DONE	1.87	1.2	num	0.87	0	-0.721	2.47	20.0	0.8
511205	1201049868	15-MAR-2006 16:54	DONE	0.17	-0.89	num	0.87	0	-0.721	2.47	20.0	0.8
510648	1201048636	16-MAR-2006 09:25	DONE	0.51	-0.45	num	0.87	0	-0.721	2.47	20.0	0.8
509833	1201046786	16-MAR-2006 10:10	DONE	4.18	4.1	num	0.87	0	-0.721	2.47	20.0	0.8
510653	1201048650	17-MAR-2006 13:41	DONE	0.52	-0.45	num	0.87	0	-0.721	2.47	20.0	0.8
511197	1201049840	17-MAR-2006 15:33	DUSE	0.03	-1	num	0.87	0	-0.721	2.47	20.0	0.8
512186	1201052165	20-MAR-2006 16:57	DONE	0.06	-1	num	0.87	0	-0.721	2.47	20.0	0.8
511556	1201050732	20-MAR-2006 20:55	DUSE	0.65	-0.28	num	0.87	0	-0.721	2.47	20.0	0.8
513065	1201054108	22-MAR-2006 14:23	DONE	0.08	-01	num	0.87	0	-0.721	2.47	20.0	0.8
512000	1201051708	22-MAR-2006 19:22	DONE	0.92	0.06	num	0.87	0	-0.721	2.47	20.0	0.8
513417	1201054861	23-MAR-2006 23:50	DONE	1.75	1.1	num	0.87	0	-0.721	2.47	20.0	0.8
513967	1201055908	24-MAR-2006 17:20	DONE	0.92	0.06	num	0.87	0	-0.721	2.47	20.0	0.8
511995	1201051697	24-MAR-2006 17:20	DUSE	1.72	1.1	num	0.87	0	-0.721	2.47	20.0	0.8
511656	1201050972	25-MAR-2006 10:35	DONE	0.36	-0.65	num	0.87	0	-0.721	2.47	20.0	0.8
513419	1201054869	26-MAR-2006 07:39	DONE	1.16	0.36	num	0.87	0	-0.721	2.47	20.0	0.8
513434	1201054912	28-MAR-2006 11:41	DONE	0.96	0.11	num	0.87	0	-0.721	2.47	20.0	0.8
515154	1201058500	28-MAR-2006 22:08	DONE	1.47	0.74	num	0.87	0	-0.721	2.47	20.0	0.8
514145	1201056278	29-MAR-2006 22:27	DONE	0.45	-0.53	num	0.87	0	-0.721	2.47	20.0	0.8
512024	1201051756	30-MAR-2006 14:07	DUSE	0.32	-0.7	num	0.87	0	-0.721	2.47	20.0	0.8
515145	1201058489	30-MAR-2006 14:53	DONE	0.3	-0.71	num	0.87	0	-0.721	2.47	20.0	0.8
515262	1201058714	31-MAR-2006 00:27	DONE	1.55	0.84	num	0.87	0	-0.721	2.47	20.0	0.8
512056	1201051826	31-MAR-2006 13:48	DONE	0.31	-0.71	num	0.87	0	-0.721	2.47	20.0	0.8
514172	1201056342	01-APR-2006 09:22	DONE	0.22	-0.82	num	0.87	0	-0.721	2.47	20.0	0.8
512045	1201051810	01-APR-2006 13:50	DUSE	0.43	-0.56	num	0.87	0	-0.721	2.47	20.0	0.8
515259	1201058706	01-APR-2006 14:24	DONE	2.08	1.5	num	0.87	0	-0.721	2.47	20.0	0.8
515558	1201059455	03-APR-2006 06:56	DONE	1.21	0.43	num	0.87	0	-0.721	2.47	20.0	0.8
515551	1201059427	03-APR-2006 06:56	DONE	0.35	-0.65	num	0.87	0	-0.721	2.47	20.0	0.8
516219	1201060905	04-APR-2006 07:47	DONE	0.12	-0.94	num	0.87	0	-0.721	2.47	20.0	0.8
512063	1201051850	04-APR-2006 10:18	DONE	1.06	0.23	num	0.87	0	-0.721	2.47	20.0	0.8
512069	1201051878	05-APR-2006 09:52	DONE	0.92	0.06	num	0.87	0	-0.721	2.47	20.0	0.8
515564	1201059471	05-APR-2006 15:35	DONE	0.46	-0.52	num	0.87	0	-0.721	2.47	20.0	0.8
517591	1201063934	05-APR-2006 21:53	DONE	0.79	-0.1	num	0.87	0	-0.721	2.47	20.0	0.8
517143	1201062896	06-APR-2006 08:11	DONE	0.74	-0.17	num	0.87	0	-0.721	2.47	20.0	0.8

516346	1201061154	06-APR-2006 13:23	DONE	0.52	-0.44	num	0.87	0	-0.721	2.47	20.0	0.8
518034	1201064929	08-APR-2006 15:43	DONE	0.28	-0.74	num	0.87	0	-0.721	2.47	20.0	0.8
517155	1201062932	08-APR-2006 15:43	DONE	0.34	-0.67	num	0.87	0	-0.721	2.47	20.0	0.8

Uranium-238 BLANK: Limits LCL = -85.7 UCL = 95.9

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
510234	1201047741	11-MAR-2006 14:29	DUSE	0	-0.17	pCi/g	5.13	-86	-55	65.7	95.9	30.3
509833	1201046785	15-MAR-2006 09:16	DONE	0	-0.17	pCi/g	5.13	-86	-55	65.7	95.9	30.3
511711	1201051087	15-MAR-2006 09:16	DONE	0	-0.17	pCi/g	5.13	-86	-55	65.7	95.9	30.3
510648	1201048635	15-MAR-2006 12:44	DONE	0	-0.17	pCi/g	5.13	-86	-55	65.7	95.9	30.3
511205	1201049867	15-MAR-2006 16:54	DONE	0	-0.17	pCi/g	5.13	-86	-55	65.7	95.9	30.3
510653	1201048649	16-MAR-2006 14:20	DONE	0	-0.17	pCi/g	5.13	-86	-55	65.7	95.9	30.3
511197	1201049839	17-MAR-2006 13:41	DUSE	0	-0.17	pCi/g	5.13	-86	-55	65.7	95.9	30.3
512186	1201052164	20-MAR-2006 16:57	DONE	189	6.1	pCi/g	5.13	-86	-55	65.7	95.9	30.3
511556	1201050731	20-MAR-2006 20:55	DUSE	0	-0.17	pCi/g	5.13	-86	-55	65.7	95.9	30.3
513065	1201054107	22-MAR-2006 14:23	DONE	0	-0.17	pCi/g	5.13	-86	-55	65.7	95.9	30.3
512000	1201051707	22-MAR-2006 19:22	DONE	0	-0.17	pCi/g	5.13	-86	-55	65.7	95.9	30.3
513417	1201054860	23-MAR-2006 23:50	DONE	0	-0.17	pCi/g	5.13	-86	-55	65.7	95.9	30.3
513967	1201055907	24-MAR-2006 17:20	DONE	0	-0.17	pCi/g	5.13	-86	-55	65.7	95.9	30.3
511995	1201051696	24-MAR-2006 17:20	DUSE	0	-0.17	pCi/g	5.13	-86	-55	65.7	95.9	30.3
511573	1201050778	24-MAR-2006 19:41	DUSE	0	-0.17	pCi/g	5.13	-86	-55	65.7	95.9	30.3
511656	1201050971	25-MAR-2006 10:35	DONE	0	-0.17	pCi/g	5.13	-86	-55	65.7	95.9	30.3
513419	1201054868	26-MAR-2006 07:39	DONE	0	-0.17	pCi/g	5.13	-86	-55	65.7	95.9	30.3
513434	1201054911	28-MAR-2006 11:41	DONE	0	-0.16	pCi/g	5.13	-86	-55	65.7	95.9	30.3
506038	1201037885	28-MAR-2006 16:43	DONE	0	-0.17	pCi/g	5.13	-86	-55	65.7	95.9	30.3
515154	1201058499	29-MAR-2006 08:48	DONE	0	-0.17	pCi/g	5.13	-86	-55	65.7	95.9	30.3
514145	1201056277	29-MAR-2006 22:27	DONE	0	-0.17	pCi/g	5.13	-86	-55	65.7	95.9	30.3
515145	1201058488	30-MAR-2006 14:53	DONE	0	-0.17	pCi/g	5.13	-86	-55	65.7	95.9	30.3
515262	1201058713	31-MAR-2006 00:27	DONE	0	-0.17	pCi/g	5.13	-86	-55	65.7	95.9	30.3
512056	1201051825	31-MAR-2006 13:48	DONE	11	0.18	pCi/g	5.13	-86	-55	65.7	95.9	30.3
512024	1201051755	31-MAR-2006 15:55	DONE	0	-0.17	pCi/g	5.13	-86	-55	65.7	95.9	30.3
514172	1201056341	01-APR-2006 09:22	DONE	0	-0.17	pCi/g	5.13	-86	-55	65.7	95.9	30.3
512045	1201051809	01-APR-2006 13:50	DONE	0	-0.17	pCi/g	5.13	-86	-55	65.7	95.9	30.3
515259	1201058705	01-APR-2006 14:24	DONE	0	-0.17	pCi/g	5.13	-86	-55	65.7	95.9	30.3
515558	1201059454	03-APR-2006 06:56	DONE	0	-0.17	pCi/g	5.13	-86	-55	65.7	95.9	30.3
515551	1201059426	03-APR-2006 06:56	DONE	0	-0.17	pCi/g	5.13	-86	-55	65.7	95.9	30.3
516219	1201060904	04-APR-2006 07:47	DONE	0	-0.17	pCi/g	5.13	-86	-55	65.7	95.9	30.3
512063	1201051849	04-APR-2006 10:18	DONE	0	-0.17	pCi/g	5.13	-86	-55	65.7	95.9	30.3
515564	1201059470	04-APR-2006 16:37	DONE	0	-0.17	pCi/g	5.13	-86	-55	65.7	95.9	30.3
512069	1201051877	05-APR-2006 09:52	DONE	0	-0.17	pCi/g	5.13	-86	-55	65.7	95.9	30.3
517591	1201063933	05-APR-2006 21:53	DONE	0	-0.17	pCi/g	5.13	-86	-55	65.7	95.9	30.3
517143	1201062895	06-APR-2006 08:11	DONE	0	-0.17	pCi/g	5.13	-86	-55	65.7	95.9	30.3
516346	1201061153	06-APR-2006 13:23	DONE	0	-0.17	pCi/g	5.13	-86	-55	65.7	95.9	30.3
518034	1201064928	08-APR-2006 15:43	DONE	0	-0.17	pCi/g	5.13	-86	-55	65.7	95.9	30.3
517155	1201062931	08-APR-2006 15:43	DONE	0	-0.17	pCi/g	5.13	-86	-55	65.7	95.9	30.3

Uranium-238 DUP: Limits LCL = 0 UCL = 20

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
508590	1201044014	09-MAR-2006 18:21	DONE	1	-0.5	percent	36	0	-100	176	20.0	70.2
510234	1201047742	11-MAR-2006 14:29	DUSE	7	-0.41	percent	36	0	-100	176	20.0	70.2

511711	1201051088	15-MAR-2006 09:16	DONE	21	-0.21	percent	36	0	-100	176	20.0	70.2
511205	1201049868	15-MAR-2006 16:54	DONE	1	-0.5	percent	36	0	-100	176	20.0	70.2
510648	1201048636	16-MAR-2006 09:25	DONE	18	-0.26	percent	36	0	-100	176	20.0	70.2
509833	1201046786	16-MAR-2006 10:10	DONE	54	0.26	percent	36	0	-100	176	20.0	70.2
510653	1201048650	17-MAR-2006 13:41	DONE	3	-0.47	percent	36	0	-100	176	20.0	70.2
511197	1201049840	17-MAR-2006 15:33	DUSE	9	-0.39	percent	36	0	-100	176	20.0	70.2
512186	1201052165	20-MAR-2006 16:57	DONE	200	2.3	percent	36	0	-100	176	20.0	70.2
511556	1201050732	20-MAR-2006 20:55	DUSE	119	1.2	percent	36	0	-100	176	20.0	70.2
513065	1201054108	22-MAR-2006 14:23	DONE	2	-0.49	percent	36	0	-100	176	20.0	70.2
512000	1201051708	22-MAR-2006 19:22	DONE	3	-0.47	percent	36	0	-100	176	20.0	70.2
513417	1201054861	23-MAR-2006 23:50	DONE	20	-0.23	percent	36	0	-100	176	20.0	70.2
513967	1201055908	24-MAR-2006 17:20	DONE	9	-0.39	percent	36	0	-100	176	20.0	70.2
511995	1201051697	24-MAR-2006 17:20	DUSE	21	-0.22	percent	36	0	-100	176	20.0	70.2
511656	1201050972	25-MAR-2006 10:35	DONE	11	-0.35	percent	36	0	-100	176	20.0	70.2
513419	1201054869	26-MAR-2006 07:39	DONE	61	0.36	percent	36	0	-100	176	20.0	70.2
513434	1201054912	28-MAR-2006 11:41	DONE	12	-0.34	percent	36	0	-100	176	20.0	70.2
506038	1201037886	28-MAR-2006 16:43	DONE	3	-0.47	percent	36	0	-100	176	20.0	70.2
515154	1201058500	28-MAR-2006 22:08	DONE	29	-0.09	percent	36	0	-100	176	20.0	70.2
514145	1201056278	29-MAR-2006 22:27	DONE	47	0.15	percent	36	0	-100	176	20.0	70.2
512024	1201051756	30-MAR-2006 14:07	DONE	6	-0.43	percent	36	0	-100	176	20.0	70.2
515145	1201058489	30-MAR-2006 14:53	DONE	25	-0.16	percent	36	0	-100	176	20.0	70.2
515262	1201058714	31-MAR-2006 00:27	DONE	38	0.03	percent	36	0	-100	176	20.0	70.2
512056	1201051826	31-MAR-2006 13:48	DONE	7	-0.42	percent	36	0	-100	176	20.0	70.2
514172	1201056342	01-APR-2006 09:22	DONE	13	-0.33	percent	36	0	-100	176	20.0	70.2
512045	1201051810	01-APR-2006 13:50	DONE	15	-0.3	percent	36	0	-100	176	20.0	70.2
515259	1201058706	01-APR-2006 14:24	DONE	13	-0.33	percent	36	0	-100	176	20.0	70.2
515558	1201059455	03-APR-2006 06:56	DONE	72	0.52	percent	36	0	-100	176	20.0	70.2
515551	1201059427	03-APR-2006 06:56	DONE	395	5.1	percent	36	0	-100	176	20.0	70.2
516219	1201060905	04-APR-2006 07:47	DONE	10	-0.38	percent	36	0	-100	176	20.0	70.2
512063	1201051850	04-APR-2006 10:18	DONE	5	-0.44	percent	36	0	-100	176	20.0	70.2
512069	1201051878	05-APR-2006 09:52	DONE	26	-0.15	percent	36	0	-100	176	20.0	70.2
515564	1201059471	05-APR-2006 15:35	DONE	26	-0.15	percent	36	0	-100	176	20.0	70.2
517591	1201063934	05-APR-2006 21:53	DONE	4	-0.45	percent	36	0	-100	176	20.0	70.2
517143	1201062896	06-APR-2006 08:11	DONE	79	0.61	percent	36	0	-100	176	20.0	70.2
516346	1201061154	06-APR-2006 13:23	DONE	8	-0.39	percent	36	0	-100	176	20.0	70.2
518034	1201064929	08-APR-2006 15:43	DONE	2	-0.49	percent	36	0	-100	176	20.0	70.2
517155	1201062932	08-APR-2006 15:43	DONE	11	-0.36	percent	36	0	-100	176	20.0	70.2

Uranium-238 LCS: Limits LCL = 75 UCL = 125

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
509084	1201045148	08-MAR-2006 13:55	DONE	103	0.36	percent	100	75.0	83.3	117	125	8.33
508638	1201044148	08-MAR-2006 17:42	DONE	112	1.4	percent	100	75.0	83.3	117	125	8.33
509121	1201045270	09-MAR-2006 15:47	DONE	105	0.6	percent	100	75.0	83.3	117	125	8.33
508588	1201044008	09-MAR-2006 15:47	DONE	107	0.84	percent	100	75.0	83.3	117	125	8.33
508590	1201044016	09-MAR-2006 18:21	DONE	105	0.6	percent	100	75.0	83.3	117	125	8.33
509833	1201046788	15-MAR-2006 09:16	DONE	100	0	percent	100	75.0	83.3	117	125	8.33
511711	1201051090	15-MAR-2006 09:16	DONE	118	2.2	percent	100	75.0	83.3	117	125	8.33
511205	1201049869	15-MAR-2006 16:54	DONE	96	-0.44	percent	100	75.0	83.3	117	125	8.33
510648	1201048638	16-MAR-2006 09:25	DONE	107	0.84	percent	100	75.0	83.3	117	125	8.33
510653	1201048651	16-MAR-2006 15:06	DONE	100	-0.06	percent	100	75.0	83.3	117	125	8.33

512186	1201052167	18-MAR-2006 09:47	DONE	111	1.3	percent	100	75.0	83.3	117	125	8.33
513065	1201054109	22-MAR-2006 14:23	DONE	83	-2	percent	100	75.0	83.3	117	125	8.33
512000	1201051710	22-MAR-2006 19:22	DONE	98	-0.23	percent	100	75.0	83.3	117	125	8.33
513417	1201054863	23-MAR-2006 23:50	DONE	105	0.6	percent	100	75.0	83.3	117	125	8.33
513967	1201055909	24-MAR-2006 17:20	DONE	88	-1	percent	100	75.0	83.3	117	125	8.33
511656	1201050973	25-MAR-2006 10:35	DONE	100	0	percent	100	75.0	83.3	117	125	8.33
513419	1201054871	26-MAR-2006 07:39	DONE	99	-0.11	percent	100	75.0	83.3	117	125	8.33
513434	1201054913	28-MAR-2006 11:41	DONE	113	1.6	percent	100	75.0	83.3	117	125	8.33
506038	1201037888	28-MAR-2006 16:43	DONE	101	0.12	percent	100	75.0	83.3	117	125	8.33
515154	1201058502	28-MAR-2006 22:08	DONE	101	0.12	percent	100	75.0	83.3	117	125	8.33
514145	1201056280	29-MAR-2006 22:27	DONE	105	0.6	percent	100	75.0	83.3	117	125	8.33
512024	1201051757	30-MAR-2006 14:07	DONE	89	-1	percent	100	75.0	83.3	117	125	8.33
515145	1201058490	30-MAR-2006 18:03	DONE	111	1.3	percent	100	75.0	83.3	117	125	8.33
515262	1201058716	31-MAR-2006 07:47	DONE	89	-1	percent	100	75.0	83.3	117	125	8.33
512056	1201051827	31-MAR-2006 13:48	DONE	90	-1	percent	100	75.0	83.3	117	125	8.33
514172	1201056344	01-APR-2006 09:22	DONE	78	-3	percent	100	75.0	83.3	117	125	8.33
515259	1201058708	01-APR-2006 09:22	DONE	111	1.3	percent	100	75.0	83.3	117	125	8.33
512045	1201051811	01-APR-2006 13:50	DONE	116	1.9	percent	100	75.0	83.3	117	125	8.33
515558	1201059457	03-APR-2006 06:56	DONE	105	0.6	percent	100	75.0	83.3	117	125	8.33
515551	1201059429	03-APR-2006 06:56	DONE	117	2	percent	100	75.0	83.3	117	125	8.33
516219	1201060907	04-APR-2006 07:47	DONE	106	0.72	percent	100	75.0	83.3	117	125	8.33
512063	1201051852	04-APR-2006 10:18	DONE	104	0.48	percent	100	75.0	83.3	117	125	8.33
515564	1201059472	04-APR-2006 16:37	DONE	101	0.12	percent	100	75.0	83.3	117	125	8.33
512069	1201051880	05-APR-2006 09:52	DONE	100	0	percent	100	75.0	83.3	117	125	8.33
517143	1201062898	06-APR-2006 08:11	DONE	108	0.96	percent	100	75.0	83.3	117	125	8.33
517591	1201063936	06-APR-2006 08:11	DONE	103	0.36	percent	100	75.0	83.3	117	125	8.33
516346	1201061156	06-APR-2006 13:23	DONE	92	-0.92	percent	100	75.0	83.3	117	125	8.33
518034	1201064931	08-APR-2006 15:43	DONE	103	0.36	percent	100	75.0	83.3	117	125	8.33
517155	1201062934	08-APR-2006 15:43	DONE	102	0.24	percent	100	75.0	83.3	117	125	8.33

Uranium-238 RER: Limits LCL = 0 UCL = 20

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
508588	1201044006	09-MAR-2006 15:47	DONE	0.27	-0.67	num	0.94	0	-1.1	2.93	20.0	0.99
508590	1201044014	09-MAR-2006 18:21	DONE	0.02	-0.93	num	0.94	0	-1.1	2.93	20.0	0.99
510234	1201047742	11-MAR-2006 14:29	DUSE	0.29	-0.65	num	0.94	0	-1.1	2.93	20.0	0.99
511711	1201051088	15-MAR-2006 09:16	DONE	1.25	0.32	num	0.94	0	-1.1	2.93	20.0	0.99
511205	1201049868	15-MAR-2006 16:54	DONE	0.02	-0.92	num	0.94	0	-1.1	2.93	20.0	0.99
510648	1201048636	16-MAR-2006 09:25	DONE	0.94	0.01	num	0.94	0	-1.1	2.93	20.0	0.99
509833	1201046786	16-MAR-2006 10:10	DONE	4.02	3.1	num	0.94	0	-1.1	2.93	20.0	0.99
510653	1201048650	17-MAR-2006 13:41	DONE	0.11	-0.84	num	0.94	0	-1.1	2.93	20.0	0.99
511197	1201049840	17-MAR-2006 15:33	DUSE	0.28	-0.66	num	0.94	0	-1.1	2.93	20.0	0.99
512186	1201052165	20-MAR-2006 16:57	DONE	1.39	0.45	num	0.94	0	-1.1	2.93	20.0	0.99
511556	1201050732	20-MAR-2006 20:55	DUSE	4.03	3.1	num	0.94	0	-1.1	2.93	20.0	0.99
513065	1201054108	22-MAR-2006 14:23	DONE	0.08	-0.86	num	0.94	0	-1.1	2.93	20.0	0.99
512000	1201051708	22-MAR-2006 19:22	DONE	0.13	-0.81	num	0.94	0	-1.1	2.93	20.0	0.99
513417	1201054861	23-MAR-2006 23:50	DONE	0.52	-0.42	num	0.94	0	-1.1	2.93	20.0	0.99
513967	1201055908	24-MAR-2006 17:20	DONE	0.27	-0.68	num	0.94	0	-1.1	2.93	20.0	0.99
511995	1201051697	24-MAR-2006 17:20	DUSE	2.75	1.8	num	0.94	0	-1.1	2.93	20.0	0.99
511656	1201050972	25-MAR-2006 10:35	DONE	0.37	-0.57	num	0.94	0	-1.1	2.93	20.0	0.99
513419	1201054869	26-MAR-2006 07:39	DONE	1.56	0.63	num	0.94	0	-1.1	2.93	20.0	0.99




513434	1201054912	28-MAR-2006 11:41	DONE	0.49	-0.45	num	0.94	0	-1.1	2.93	20.0	0.99
515154	1201058500	28-MAR-2006 22:08	DONE	2.3	1.4	num	0.94	0	-1.1	2.93	20.0	0.99
514145	1201056278	29-MAR-2006 22:27	DONE	2.29	1.4	num	0.94	0	-1.1	2.93	20.0	0.99
512024	1201051756	30-MAR-2006 14:07	DONE	0.21	-0.73	num	0.94	0	-1.1	2.93	20.0	0.99
515145	1201058489	30-MAR-2006 14:53	DONE	0.81	-0.13	num	0.94	0	-1.1	2.93	20.0	0.99
515262	1201058714	31-MAR-2006 00:27	DONE	0.85	-0.09	num	0.94	0	-1.1	2.93	20.0	0.99
512056	1201051826	31-MAR-2006 13:48	DONE	0.37	-0.57	num	0.94	0	-1.1	2.93	20.0	0.99
514172	1201056342	01-APR-2006 09:22	DONE	0.65	-0.29	num	0.94	0	-1.1	2.93	20.0	0.99
512045	1201051810	01-APR-2006 13:50	DONE	0.54	-0.4	num	0.94	0	-1.1	2.93	20.0	0.99
515259	1201058706	01-APR-2006 14:24	DONE	1.02	0.09	num	0.94	0	-1.1	2.93	20.0	0.99
515558	1201059455	03-APR-2006 06:56	DONE	1.8	0.87	num	0.94	0	-1.1	2.93	20.0	0.99
515551	1201059427	03-APR-2006 06:56	DONE	1.73	0.8	num	0.94	0	-1.1	2.93	20.0	0.99
516219	1201060905	04-APR-2006 07:47	DONE	0.61	-0.33	num	0.94	0	-1.1	2.93	20.0	0.99
512063	1201051850	04-APR-2006 10:18	DONE	0.22	-0.72	num	0.94	0	-1.1	2.93	20.0	0.99
512069	1201051878	05-APR-2006 09:52	DONE	1.24	0.3	num	0.94	0	-1.1	2.93	20.0	0.99
515564	1201059471	05-APR-2006 15:35	DONE	0.89	-0.05	num	0.94	0	-1.1	2.93	20.0	0.99
517591	1201063934	05-APR-2006 21:53	DONE	0.41	-0.53	num	0.94	0	-1.1	2.93	20.0	0.99
517143	1201062896	06-APR-2006 08:11	DONE	0.86	-0.08	num	0.94	0	-1.1	2.93	20.0	0.99
516346	1201061154	06-APR-2006 13:23	DONE	0.46	-0.48	num	0.94	0	-1.1	2.93	20.0	0.99
518034	1201064929	08-APR-2006 15:43	DONE	0.13	-0.81	num	0.94	0	-1.1	2.93	20.0	0.99
517155	1201062932	08-APR-2006 15:43	DONE	0.41	-0.53	num	0.94	0	-1.1	2.93	20.0	0.99

Uranium-238 SPIKE: Limits LCL = 75 UCL = 125

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
503672	1201032614	16-FEB-2006 21:40	DONE	94	-0.7	percent	100	75.0	83.3	117	125	8.33
503668	1201032259	16-FEB-2006 21:41	DONE	99	-0.18	percent	100	75.0	83.3	117	125	8.33
503154	1201031112	17-FEB-2006 11:01	DUSE	1350	150	percent	100	75.0	83.3	117	125	8.33
505620	1201036924	21-FEB-2006 23:51	DONE	106	0.72	percent	100	75.0	83.3	117	125	8.33
505875	1201037477	23-FEB-2006 10:53	DONE	2102	240	percent	100	75.0	83.3	117	125	8.33
507246	1201040730	28-FEB-2006 15:46	DONE	203	12	percent	100	75.0	83.3	117	125	8.33
507176	1201040560	28-FEB-2006 20:08	DONE	110	1.2	percent	100	75.0	83.3	117	125	8.33
504464	1201034139	28-FEB-2006 20:08	DONE	99	-0.14	percent	100	75.0	83.3	117	125	8.33
504465	1201034143	01-MAR-2006 16:22	DONE	107	0.84	percent	100	75.0	83.3	117	125	8.33
504468	1201034155	01-MAR-2006 16:22	DONE	104	0.48	percent	100	75.0	83.3	117	125	8.33
508045	1201042751	02-MAR-2006 22:23	DONE	98	-0.26	percent	100	75.0	83.3	117	125	8.33
506034	1201037875	03-MAR-2006 15:56	DONE	101	0.12	percent	100	75.0	83.3	117	125	8.33
504175	1201033489	08-MAR-2006 08:59	DONE	112	1.4	percent	100	75.0	83.3	117	125	8.33
509084	1201045147	08-MAR-2006 13:55	DONE	110	1.2	percent	100	75.0	83.3	117	125	8.33
508588	1201044007	09-MAR-2006 15:47	DONE	115	1.8	percent	100	75.0	83.3	117	125	8.33
508590	1201044015	09-MAR-2006 18:21	DONE	106	0.72	percent	100	75.0	83.3	117	125	8.33
511711	1201051089	15-MAR-2006 09:16	DONE	115	1.8	percent	100	75.0	83.3	117	125	8.33
510648	1201048637	16-MAR-2006 09:25	DONE	113	1.6	percent	100	75.0	83.3	117	125	8.33
509833	1201046787	16-MAR-2006 10:10	DONE	49	-6	percent	100	75.0	83.3	117	125	8.33
512186	1201052166	18-MAR-2006 09:47	DONE	104	0.48	percent	100	75.0	83.3	117	125	8.33
512000	1201051709	22-MAR-2006 19:22	DONE	98	-0.26	percent	100	75.0	83.3	117	125	8.33
513417	1201054862	23-MAR-2006 23:50	DONE	84	-2	percent	100	75.0	83.3	117	125	8.33
513419	1201054870	26-MAR-2006 07:39	DONE	93	-0.86	percent	100	75.0	83.3	117	125	8.33
506038	1201037887	28-MAR-2006 16:43	DONE	102	0.24	percent	100	75.0	83.3	117	125	8.33
515154	1201058501	28-MAR-2006 22:08	DONE	138	4.6	percent	100	75.0	83.3	117	125	8.33
514145	1201056279	29-MAR-2006 22:27	DONE	99	-0.12	percent	100	75.0	83.3	117	125	8.33

515262	1201058715	31-MAR-2006 07:47	DONE	99	-0.1	percent	100	75.0	83.3	117	125	8.33
514172	1201056343	01-APR-2006 09:22	DONE	4	-10	percent	100	75.0	83.3	117	125	8.33
515259	1201058707	01-APR-2006 09:22	DONE	93	-0.88	percent	100	75.0	83.3	117	125	8.33
515558	1201059456	03-APR-2006 06:56	DONE	95	-0.62	percent	100	75.0	83.3	117	125	8.33
515551	1201059428	03-APR-2006 06:56	DONE	114	1.7	percent	100	75.0	83.3	117	125	8.33
516219	1201060906	04-APR-2006 07:47	DONE	104	0.48	percent	100	75.0	83.3	117	125	8.33
512063	1201051851	04-APR-2006 10:18	DONE	98	-0.19	percent	100	75.0	83.3	117	125	8.33
512069	1201051879	05-APR-2006 09:52	DONE	95	-0.62	percent	100	75.0	83.3	117	125	8.33
517143	1201062897	06-APR-2006 08:11	DONE	109	1.1	percent	100	75.0	83.3	117	125	8.33
517591	1201063935	06-APR-2006 08:11	DONE	104	0.47	percent	100	75.0	83.3	117	125	8.33
516346	1201061155	06-APR-2006 13:23	DONE	100	0	percent	100	75.0	83.3	117	125	8.33
518034	1201064930	08-APR-2006 15:43	DONE	-221	-40	percent	100	75.0	83.3	117	125	8.33
517155	1201062933	08-APR-2006 15:43	DONE	111	1.3	percent	100	75.0	83.3	117	125	8.33





SPC Graph for Alpha SpecThorium in Solids 4/10/2006 Thorium-228 BLANK

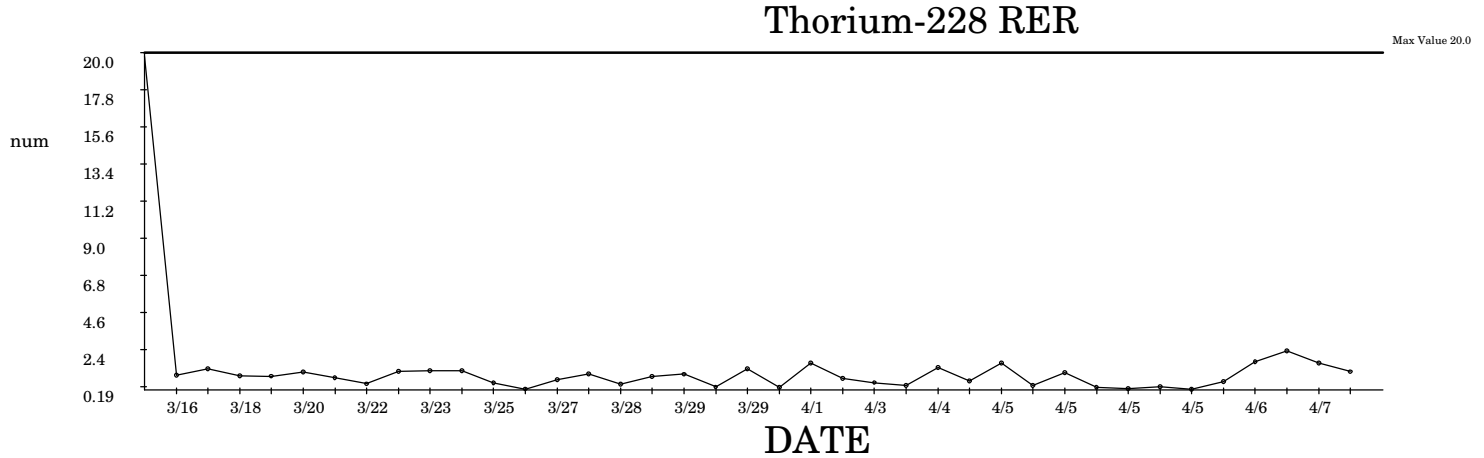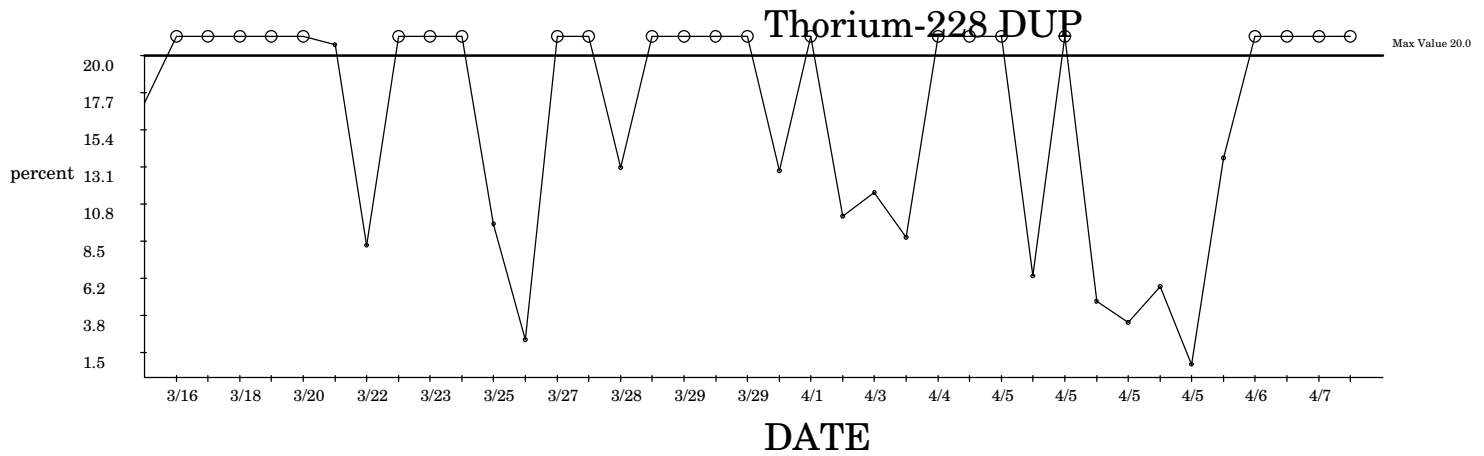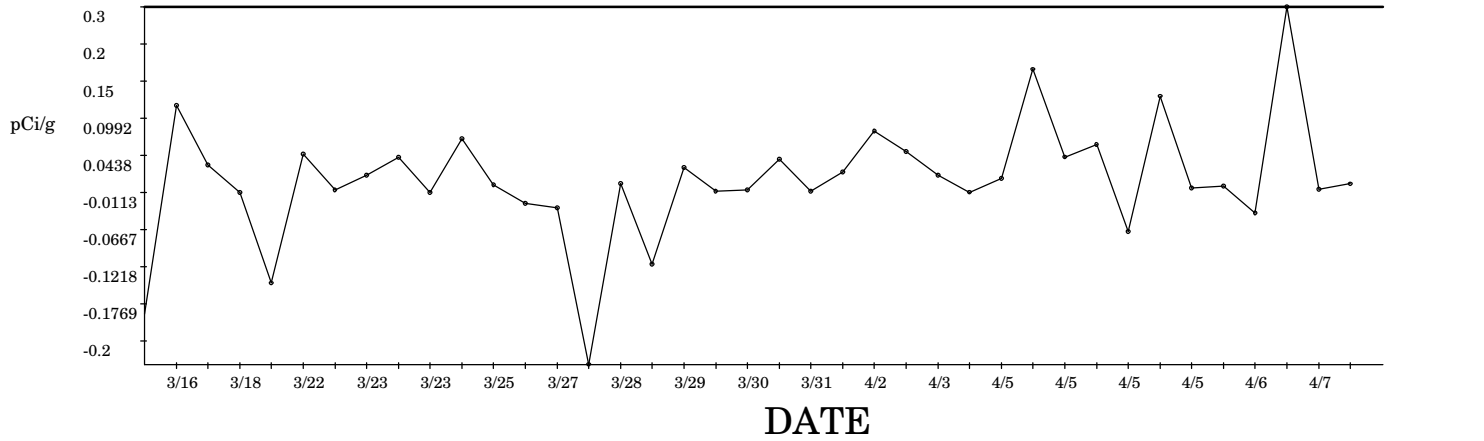

○ Denotes Outlier


SPC Graph for Alpha SpecThorium in Solids 4/10/2006

Thorium-230 BLANK

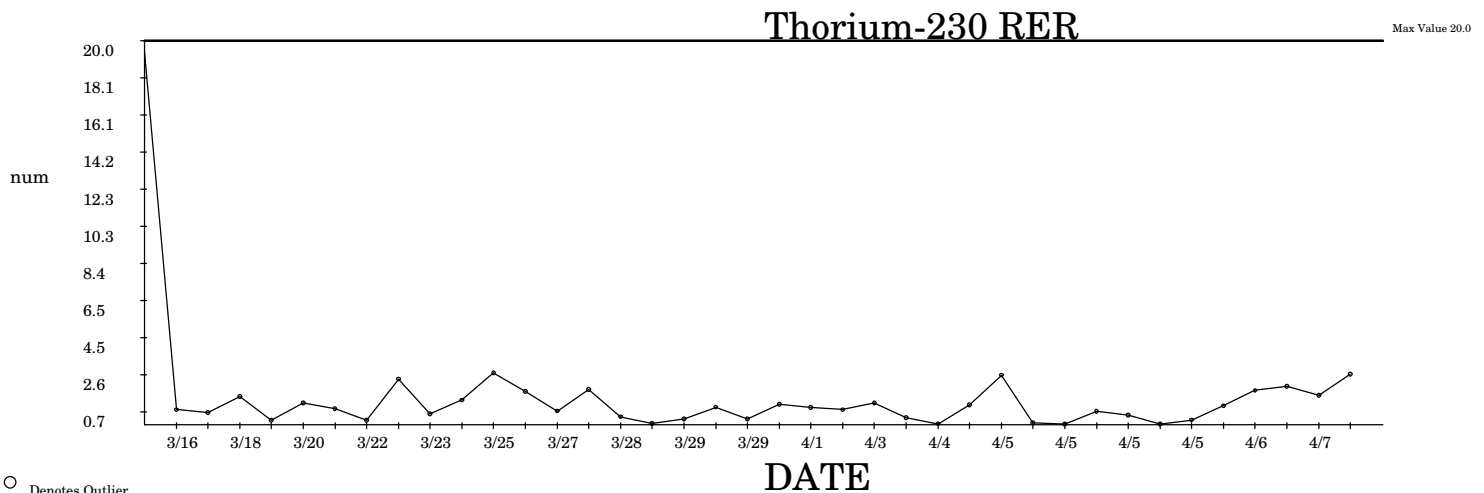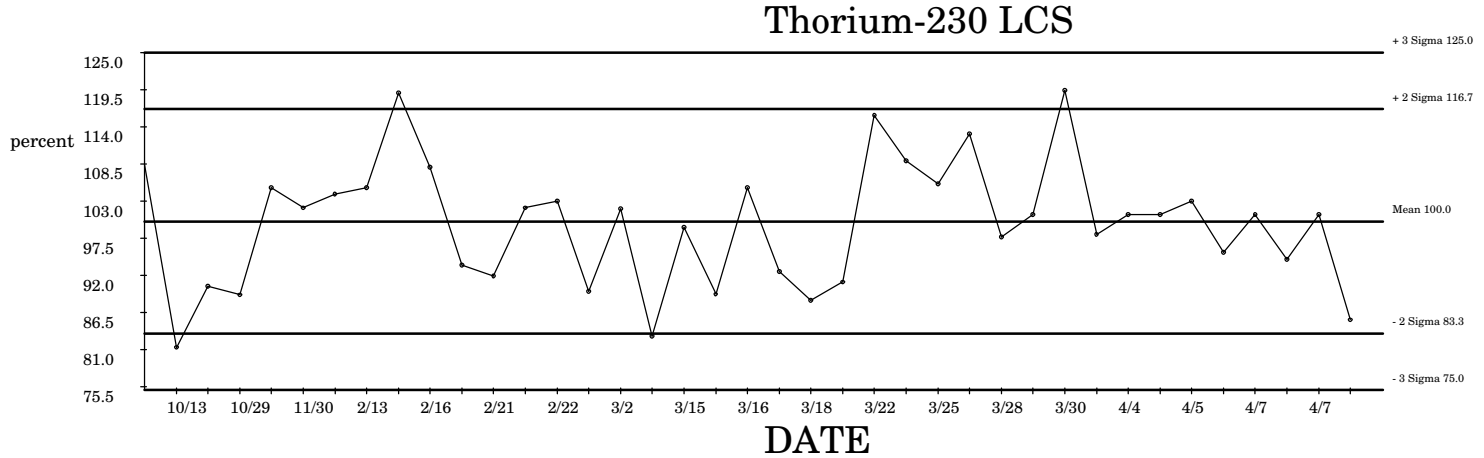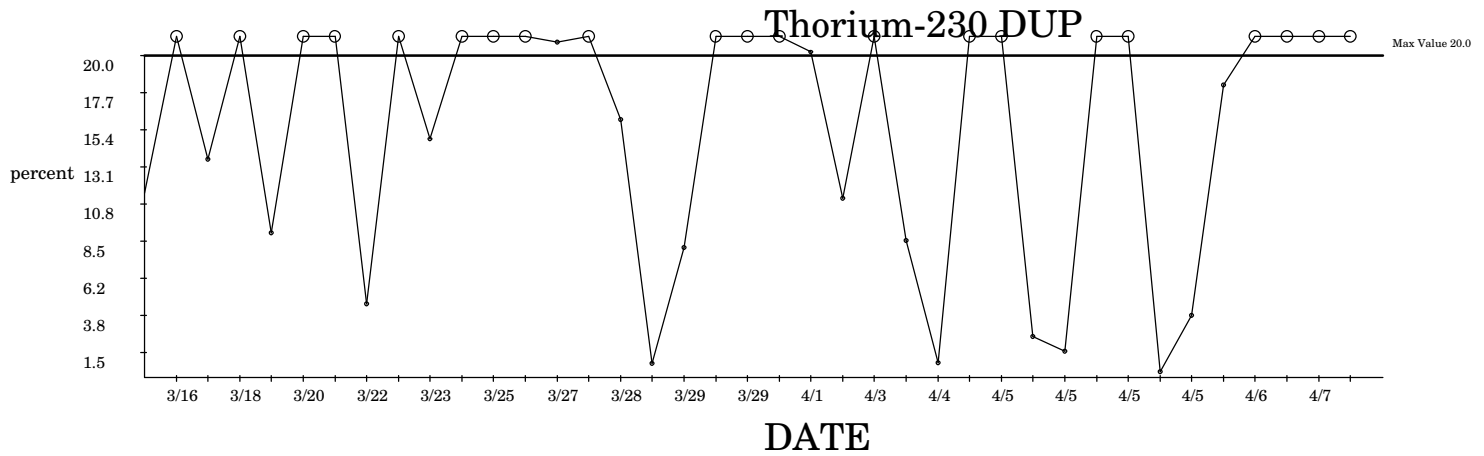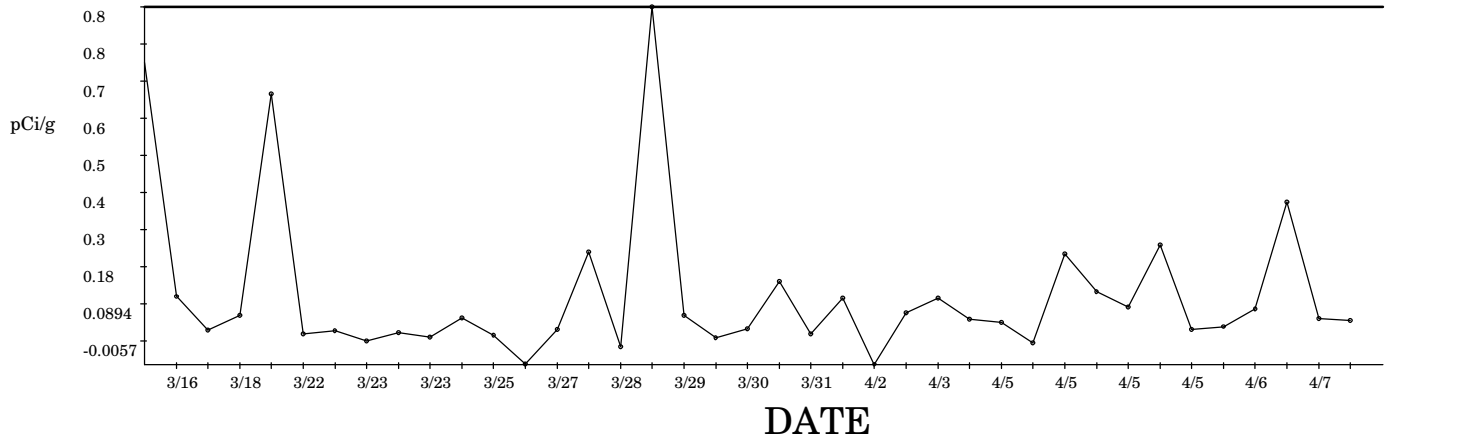

○ Denotes Outlier





SPC Graph for Alpha SpecThorium in Solids 4/10/2006 Thorium-230 SPIKE

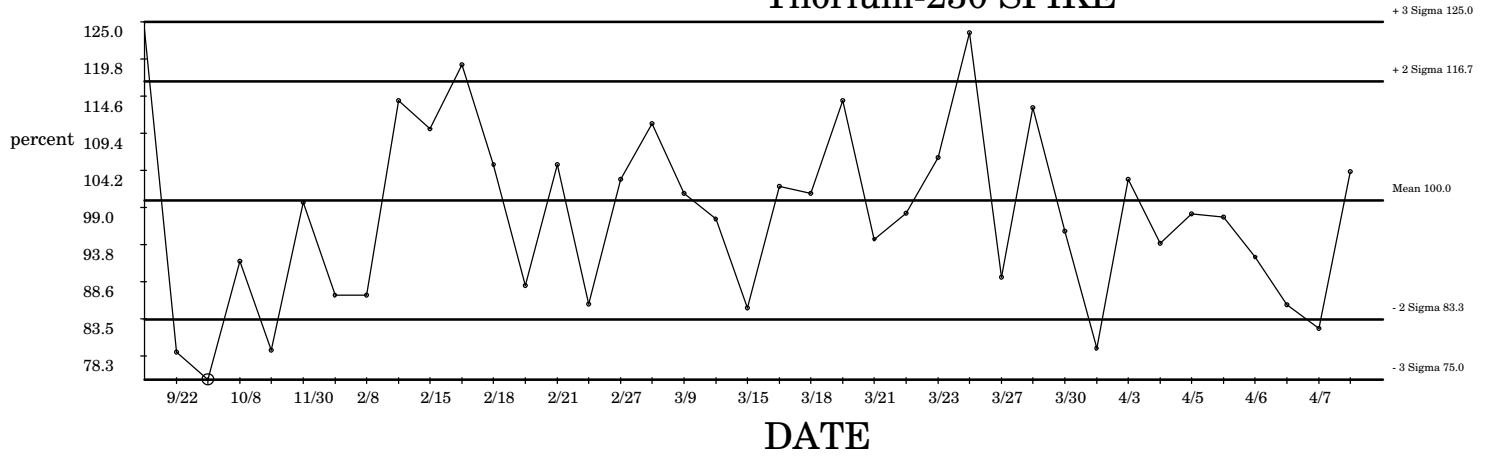

○ Denotes Outlier


SPC Graph for Alpha SpecThorium in Solids 4/10/2006

Thorium-232 BLANK

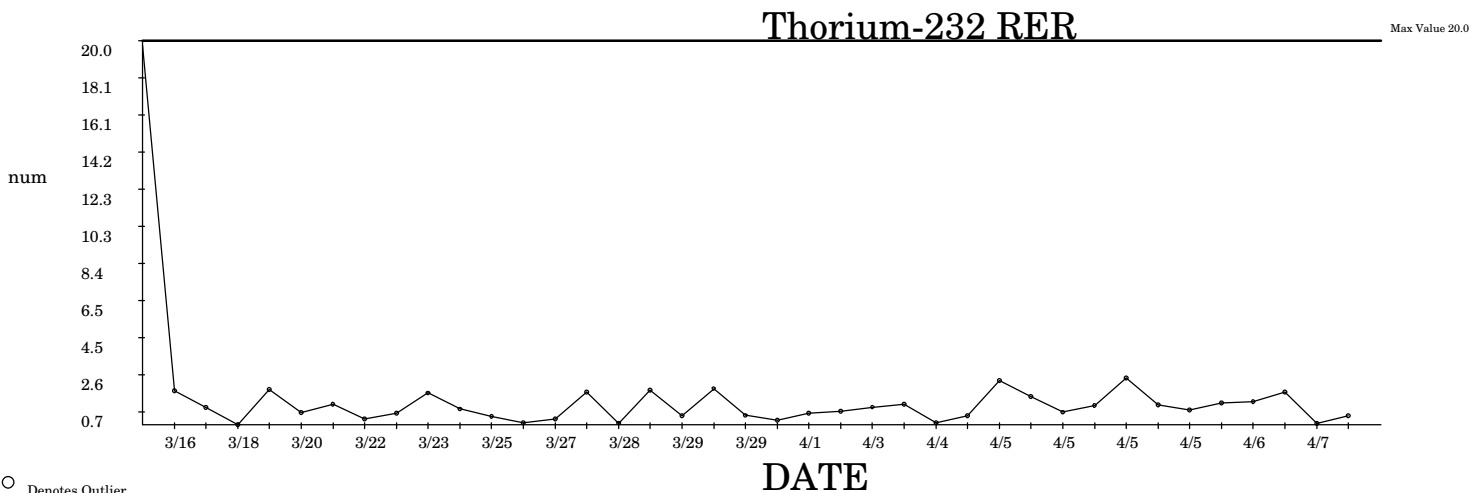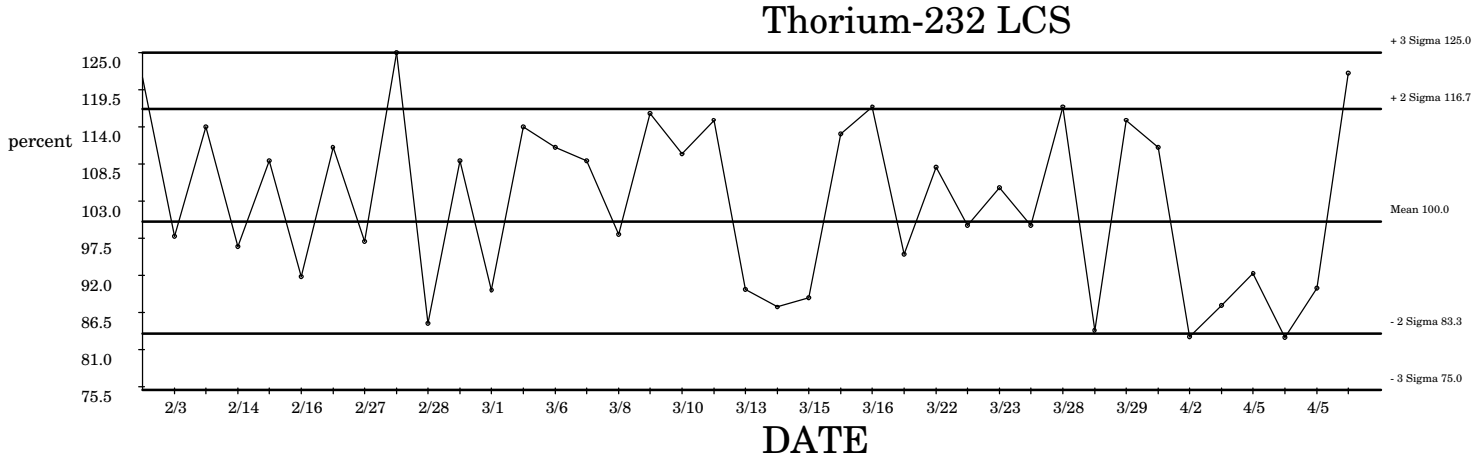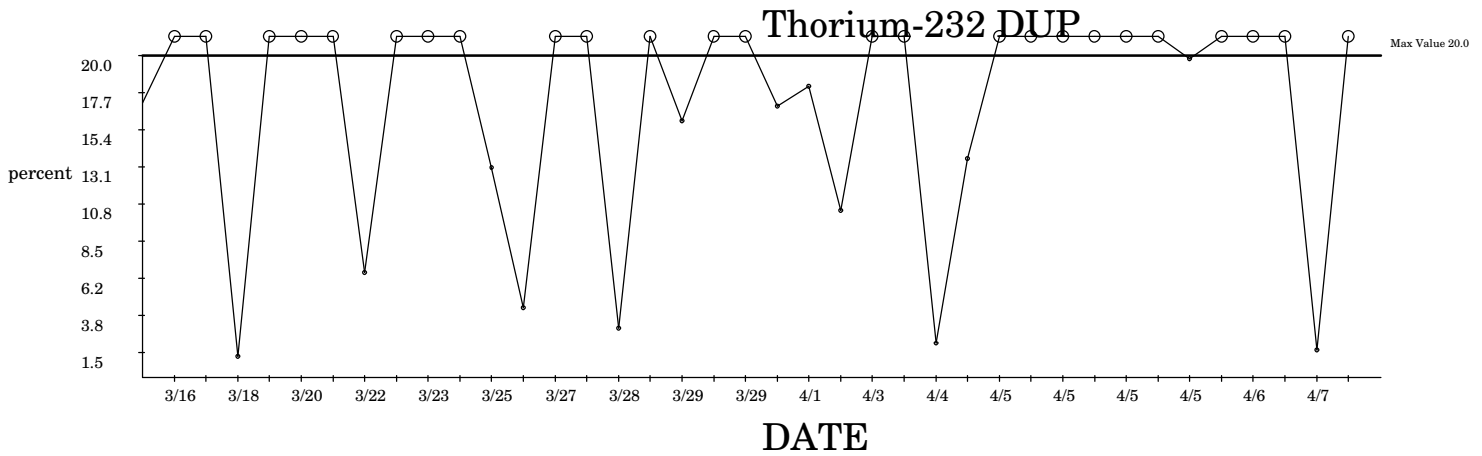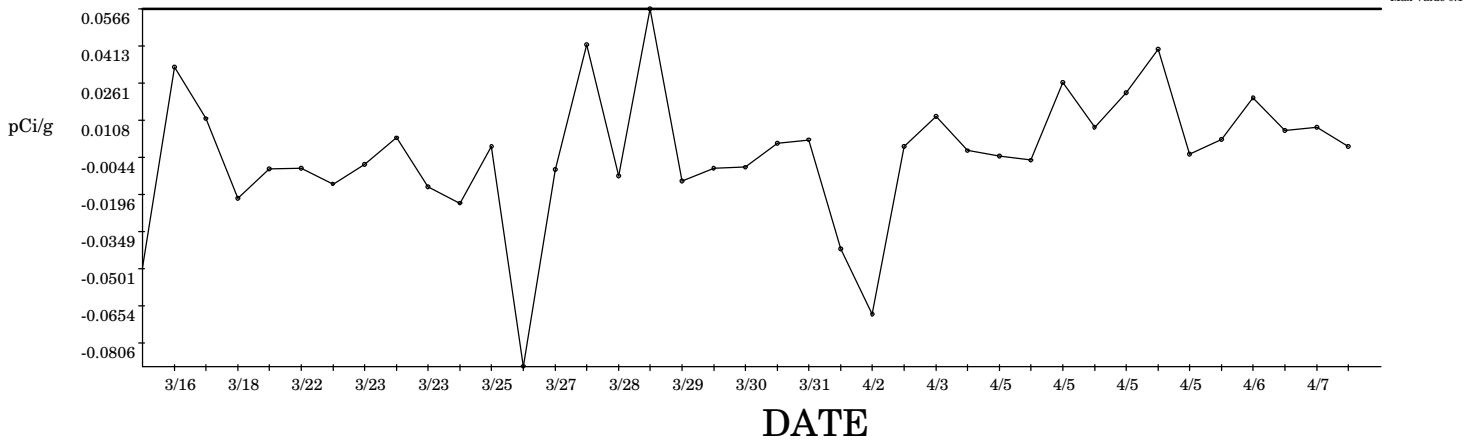

○ Denotes Outlier

SPC Graph for Alpha SpecThorium in Solids 4/10/2006 Thorium-232 SPIKE

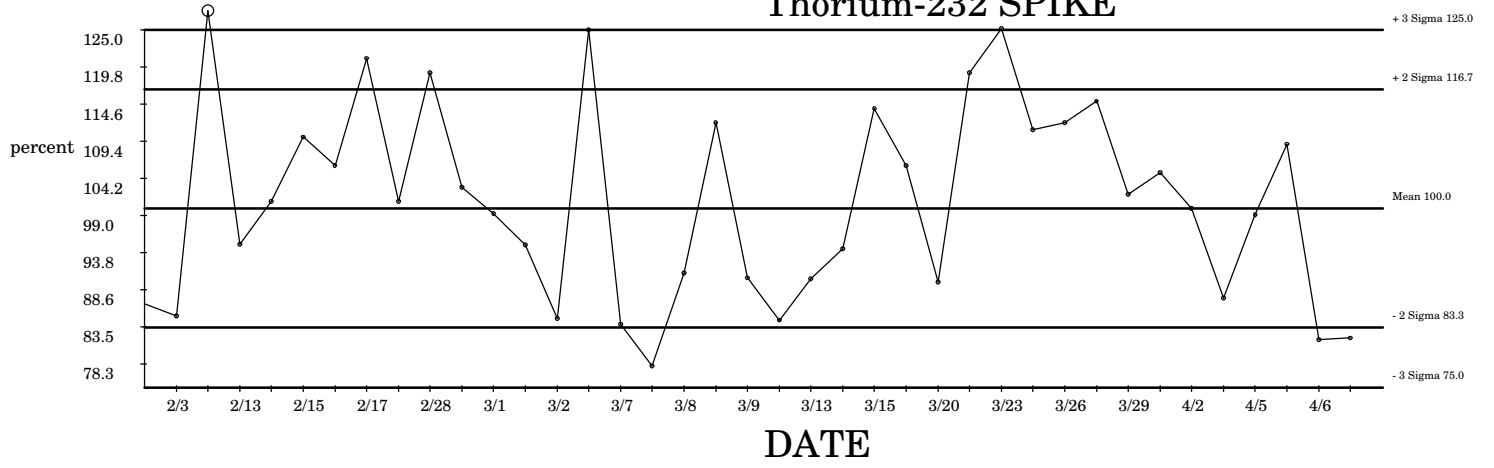

○ Denotes Outlier

Data used for Alpha SpecThorium in Solids 11-APR-2006

Thorium-228 BLANK: Limits LCL = -.3 UCL = .3

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stddev
509059	1201045077	16-MAR-2006 08:39	DONE	0	2	pCi/g	0.02	-0.25	-0.161	0.19	0.28	0.09
510647	1201048631	16-MAR-2006 10:55	DONE	0	1.1	pCi/g	0.02	-0.25	-0.161	0.19	0.28	0.09
511635	1201050914	18-MAR-2006 15:00	DUSE	0	0.15	pCi/g	0.02	-0.25	-0.161	0.19	0.28	0.09
511985	1201051674	18-MAR-2006 15:00	DUSE	0	-0.32	pCi/g	0.02	-0.25	-0.161	0.19	0.28	0.09
511630	1201050905	20-MAR-2006 07:42	DONE	0	-2	pCi/g	0.02	-0.25	-0.161	0.19	0.28	0.09
511996	1201051700	22-MAR-2006 14:23	DONE	0	0.34	pCi/g	0.02	-0.25	-0.161	0.19	0.28	0.09
513053	1201054070	22-MAR-2006 19:41	DUSE	0	-0.27	pCi/g	0.02	-0.25	-0.161	0.19	0.28	0.09
513051	1201054062	23-MAR-2006 08:31	DUSE	0	-0.03	pCi/g	0.02	-0.25	-0.161	0.19	0.28	0.09
511992	1201051686	23-MAR-2006 21:21	DONE	0	0.28	pCi/g	0.02	-0.25	-0.161	0.19	0.28	0.09
513052	1201054066	23-MAR-2006 23:50	DUSE	0	-0.31	pCi/g	0.02	-0.25	-0.161	0.19	0.28	0.09
513416	1201054856	24-MAR-2006 12:39	DONE	0	0.59	pCi/g	0.02	-0.25	-0.161	0.19	0.28	0.09
514672	1201057502	25-MAR-2006 19:34	DUSE	0	-0.18	pCi/g	0.02	-0.25	-0.161	0.19	0.28	0.09
513418	1201054864	26-MAR-2006 07:39	DONE	0	-0.49	pCi/g	0.02	-0.25	-0.161	0.19	0.28	0.09
513759	1201055494	27-MAR-2006 17:14	DUSE	0	-0.57	pCi/g	0.02	-0.25	-0.161	0.19	0.28	0.09
513435	1201054914	28-MAR-2006 11:41	DONE	0	-3	pCi/g	0.02	-0.25	-0.161	0.19	0.28	0.09
512017	1201051748	28-MAR-2006 16:43	DUSE	0	-0.16	pCi/g	0.02	-0.25	-0.161	0.19	0.28	0.09
514175	1201056354	29-MAR-2006 15:32	DUSE	0	-2	pCi/g	0.02	-0.25	-0.161	0.19	0.28	0.09
515260	1201058709	29-MAR-2006 16:59	DONE	0	0.11	pCi/g	0.02	-0.25	-0.161	0.19	0.28	0.09
515263	1201058717	29-MAR-2006 22:27	DUSE	0	-0.29	pCi/g	0.02	-0.25	-0.161	0.19	0.28	0.09
515264	1201058721	30-MAR-2006 09:13	DUSE	0	-0.26	pCi/g	0.02	-0.25	-0.161	0.19	0.28	0.09
514144	1201056273	30-MAR-2006 18:04	DONE	0	0.25	pCi/g	0.02	-0.25	-0.161	0.19	0.28	0.09
515871	1201060180	31-MAR-2006 23:48	DUSE	0	-0.28	pCi/g	0.02	-0.25	-0.161	0.19	0.28	0.09
515258	1201058701	01-APR-2006 09:23	DONE	0	0.03	pCi/g	0.02	-0.25	-0.161	0.19	0.28	0.09
515550	1201059422	02-APR-2006 07:36	DONE	0	0.72	pCi/g	0.02	-0.25	-0.161	0.19	0.28	0.09
515556	1201059443	03-APR-2006 06:56	DUSE	0	0.38	pCi/g	0.02	-0.25	-0.161	0.19	0.28	0.09
516132	1201060710	03-APR-2006 12:42	DUSE	0	-0.03	pCi/g	0.02	-0.25	-0.161	0.19	0.28	0.09
516806	1201062214	04-APR-2006 22:21	DUSE	0	-0.31	pCi/g	0.02	-0.25	-0.161	0.19	0.28	0.09
516800	1201062199	05-APR-2006 09:51	DUSE	0	-0.08	pCi/g	0.02	-0.25	-0.161	0.19	0.28	0.09
512068	1201051873	05-APR-2006 09:52	DONE	0	1.8	pCi/g	0.02	-0.25	-0.161	0.19	0.28	0.09
512060	1201051841	05-APR-2006 10:05	DONE	0	0.28	pCi/g	0.02	-0.25	-0.161	0.19	0.28	0.09
517558	1201063868	05-APR-2006 15:35	DONE	0	0.49	pCi/g	0.02	-0.25	-0.161	0.19	0.28	0.09
517144	1201062899	05-APR-2006 15:35	DONE	0	-0.96	pCi/g	0.02	-0.25	-0.161	0.19	0.28	0.09
515901	1201060261	05-APR-2006 19:49	DUSE	0	1.3	pCi/g	0.02	-0.25	-0.161	0.19	0.28	0.09
517138	1201062879	05-APR-2006 19:53	DUSE	0	-0.24	pCi/g	0.02	-0.25	-0.161	0.19	0.28	0.09
517139	1201062883	06-APR-2006 08:11	DUSE	0	-0.2	pCi/g	0.02	-0.25	-0.161	0.19	0.28	0.09
516344	1201061149	06-APR-2006 13:23	DONE	0	-0.66	pCi/g	0.02	-0.25	-0.161	0.19	0.28	0.09
517153	1201062927	07-APR-2006 18:07	DONE	0	2.8	pCi/g	0.02	-0.25	-0.161	0.19	0.28	0.09
518029	1201064909	07-APR-2006 23:26	DUSE	0	-0.26	pCi/g	0.02	-0.25	-0.161	0.19	0.28	0.09
518036	1201064937	07-APR-2006 23:26	DUSE	0	-0.17	pCi/g	0.02	-0.25	-0.161	0.19	0.28	0.09

Thorium-228 DUP: Limits LCL = 0 UCL = 20

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stddev
511710	1201051084	15-MAR-2006 13:59	DONE	3	-0.79	percent	39.2	0	-53	131	20.0	45.9
509059	1201045078	16-MAR-2006 08:39	DONE	36	-0.06	percent	39.2	0	-53	131	20.0	45.9
510647	1201048632	16-MAR-2006 23:45	DONE	42	0.05	percent	39.2	0	-53	131	20.0	45.9
511635	1201050915	18-MAR-2006 15:00	DUSE	85	0.99	percent	39.2	0	-53	131	20.0	45.9

511985	1201051675	18-MAR-2006 15:00	DUSE	90	1.1	percent	39.2	0	-53	131	20.0	45.9
511630	1201050906	20-MAR-2006 07:42	DONE	22	-0.38	percent	39.2	0	-53	131	20.0	45.9
513052	1201054067	22-MAR-2006 12:16	DUSE	21	-0.4	percent	39.2	0	-53	131	20.0	45.9
511996	1201051701	22-MAR-2006 14:23	DONE	8	-0.68	percent	39.2	0	-53	131	20.0	45.9
513053	1201054071	22-MAR-2006 19:41	DUSE	112	1.6	percent	39.2	0	-53	131	20.0	45.9
513051	1201054063	23-MAR-2006 08:31	DUSE	36	-0.07	percent	39.2	0	-53	131	20.0	45.9
513416	1201054857	23-MAR-2006 23:50	DONE	50	0.24	percent	39.2	0	-53	131	20.0	45.9
511992	1201051687	25-MAR-2006 19:34	DONE	10	-0.65	percent	39.2	0	-53	131	20.0	45.9
513418	1201054865	26-MAR-2006 07:39	DONE	2	-0.8	percent	39.2	0	-53	131	20.0	45.9
513759	1201055495	27-MAR-2006 17:14	DUSE	48	0.19	percent	39.2	0	-53	131	20.0	45.9
513435	1201054915	28-MAR-2006 11:41	DONE	36	-0.07	percent	39.2	0	-53	131	20.0	45.9
512017	1201051749	28-MAR-2006 16:43	DUSE	13	-0.57	percent	39.2	0	-53	131	20.0	45.9
514175	1201056355	29-MAR-2006 15:32	DUSE	26	-0.3	percent	39.2	0	-53	131	20.0	45.9
514144	1201056274	29-MAR-2006 19:54	DONE	39	-0	percent	39.2	0	-53	131	20.0	45.9
515263	1201058718	29-MAR-2006 22:27	DUSE	48	0.18	percent	39.2	0	-53	131	20.0	45.9
515260	1201058710	29-MAR-2006 22:27	DONE	87	1	percent	39.2	0	-53	131	20.0	45.9
515264	1201058722	30-MAR-2006 09:13	DUSE	13	-0.57	percent	39.2	0	-53	131	20.0	45.9
515258	1201058702	01-APR-2006 09:23	DONE	44	0.11	percent	39.2	0	-53	131	20.0	45.9
515550	1201059423	02-APR-2006 07:36	DONE	10	-0.64	percent	39.2	0	-53	131	20.0	45.9
515556	1201059444	03-APR-2006 06:56	DUSE	12	-0.6	percent	39.2	0	-53	131	20.0	45.9
516132	1201060711	03-APR-2006 12:42	DUSE	9	-0.66	percent	39.2	0	-53	131	20.0	45.9
515871	1201060181	04-APR-2006 07:44	DUSE	33	-0.13	percent	39.2	0	-53	131	20.0	45.9
516806	1201062215	05-APR-2006 08:19	DUSE	23	-0.34	percent	39.2	0	-53	131	20.0	45.9
516800	1201062200	05-APR-2006 09:51	DUSE	258	4.8	percent	39.2	0	-53	131	20.0	45.9
512068	1201051874	05-APR-2006 09:52	DONE	6	-0.72	percent	39.2	0	-53	131	20.0	45.9
512060	1201051842	05-APR-2006 10:05	DONE	29	-0.21	percent	39.2	0	-53	131	20.0	45.9
517558	1201063869	05-APR-2006 15:35	DONE	5	-0.75	percent	39.2	0	-53	131	20.0	45.9
517144	1201062900	05-APR-2006 15:35	DONE	3	-0.78	percent	39.2	0	-53	131	20.0	45.9
515901	1201060262	05-APR-2006 17:13	DUSE	6	-0.73	percent	39.2	0	-53	131	20.0	45.9
517138	1201062880	05-APR-2006 19:53	DUSE	1	-0.84	percent	39.2	0	-53	131	20.0	45.9
517139	1201062884	06-APR-2006 08:11	DUSE	14	-0.56	percent	39.2	0	-53	131	20.0	45.9
516344	1201061150	06-APR-2006 13:23	DONE	50	0.24	percent	39.2	0	-53	131	20.0	45.9
517153	1201062928	07-APR-2006 18:07	DONE	53	0.3	percent	39.2	0	-53	131	20.0	45.9
518029	1201064910	07-APR-2006 23:26	DUSE	57	0.39	percent	39.2	0	-53	131	20.0	45.9
518036	1201064938	07-APR-2006 23:26	DUSE	90	1.1	percent	39.2	0	-53	131	20.0	45.9

Thorium-228 RER: Limits LCL = 0 UCL = 20

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
511710	1201051084	15-MAR-2006 13:59	DONE	0.23	-1	num	0.78	0	-0.304	1.87	20.0	0.54
509059	1201045078	16-MAR-2006 08:39	DONE	0.89	0.19	num	0.78	0	-0.304	1.87	20.0	0.54
510647	1201048632	16-MAR-2006 23:45	DONE	1.27	0.89	num	0.78	0	-0.304	1.87	20.0	0.54
511635	1201050915	18-MAR-2006 15:00	DUSE	0.83	0.08	num	0.78	0	-0.304	1.87	20.0	0.54
511985	1201051675	18-MAR-2006 15:00	DUSE	0.81	0.05	num	0.78	0	-0.304	1.87	20.0	0.54
511630	1201050906	20-MAR-2006 07:42	DONE	1.06	0.5	num	0.78	0	-0.304	1.87	20.0	0.54
513052	1201054067	22-MAR-2006 12:16	DUSE	0.71	-0.13	num	0.78	0	-0.304	1.87	20.0	0.54
511996	1201051701	22-MAR-2006 14:23	DONE	0.37	-0.77	num	0.78	0	-0.304	1.87	20.0	0.54
513053	1201054071	22-MAR-2006 19:41	DUSE	1.11	0.6	num	0.78	0	-0.304	1.87	20.0	0.54
513051	1201054063	23-MAR-2006 08:31	DUSE	1.15	0.67	num	0.78	0	-0.304	1.87	20.0	0.54
513416	1201054857	23-MAR-2006 23:50	DONE	1.15	0.67	num	0.78	0	-0.304	1.87	20.0	0.54
511992	1201051687	25-MAR-2006 19:34	DONE	0.4	-0.7	num	0.78	0	-0.304	1.87	20.0	0.54

513418	1201054865	26-MAR-2006 07:39	DONE	0.06	-1	num	0.78	0	-0.304	1.87	20.0	0.54
513759	1201055495	27-MAR-2006 17:14	DUSE	0.59	-0.36	num	0.78	0	-0.304	1.87	20.0	0.54
513435	1201054915	28-MAR-2006 11:41	DONE	0.96	0.33	num	0.78	0	-0.304	1.87	20.0	0.54
512017	1201051749	28-MAR-2006 16:43	DUSE	0.36	-0.79	num	0.78	0	-0.304	1.87	20.0	0.54
514175	1201056355	29-MAR-2006 15:32	DUSE	0.78	-0	num	0.78	0	-0.304	1.87	20.0	0.54
514144	1201056274	29-MAR-2006 19:54	DONE	0.93	0.28	num	0.78	0	-0.304	1.87	20.0	0.54
515263	1201058718	29-MAR-2006 22:27	DUSE	0.18	-1	num	0.78	0	-0.304	1.87	20.0	0.54
515260	1201058710	29-MAR-2006 22:27	DONE	1.27	0.89	num	0.78	0	-0.304	1.87	20.0	0.54
515264	1201058722	30-MAR-2006 09:13	DUSE	0.17	-1	num	0.78	0	-0.304	1.87	20.0	0.54
515258	1201058702	01-APR-2006 09:23	DONE	1.58	1.5	num	0.78	0	-0.304	1.87	20.0	0.54
515550	1201059423	02-APR-2006 07:36	DONE	0.67	-0.2	num	0.78	0	-0.304	1.87	20.0	0.54
515556	1201059444	03-APR-2006 06:56	DUSE	0.43	-0.65	num	0.78	0	-0.304	1.87	20.0	0.54
516132	1201060711	03-APR-2006 12:42	DUSE	0.27	-0.94	num	0.78	0	-0.304	1.87	20.0	0.54
515871	1201060181	04-APR-2006 07:44	DUSE	1.33	1	num	0.78	0	-0.304	1.87	20.0	0.54
516806	1201062215	05-APR-2006 08:19	DUSE	0.53	-0.46	num	0.78	0	-0.304	1.87	20.0	0.54
516800	1201062200	05-APR-2006 09:51	DUSE	1.58	1.5	num	0.78	0	-0.304	1.87	20.0	0.54
512068	1201051874	05-APR-2006 09:52	DONE	0.27	-0.94	num	0.78	0	-0.304	1.87	20.0	0.54
512060	1201051842	05-APR-2006 10:05	DONE	1.02	0.43	num	0.78	0	-0.304	1.87	20.0	0.54
517558	1201063869	05-APR-2006 15:35	DONE	0.17	-1	num	0.78	0	-0.304	1.87	20.0	0.54
517144	1201062900	05-APR-2006 15:35	DONE	0.07	-1	num	0.78	0	-0.304	1.87	20.0	0.54
515901	1201060262	05-APR-2006 17:13	DUSE	0.18	-1	num	0.78	0	-0.304	1.87	20.0	0.54
517138	1201062880	05-APR-2006 19:53	DUSE	0.02	-1	num	0.78	0	-0.304	1.87	20.0	0.54
517139	1201062884	06-APR-2006 08:11	DUSE	0.5	-0.53	num	0.78	0	-0.304	1.87	20.0	0.54
516344	1201061150	06-APR-2006 13:23	DONE	1.67	1.6	num	0.78	0	-0.304	1.87	20.0	0.54
517153	1201062928	07-APR-2006 18:07	DONE	2.31	2.8	num	0.78	0	-0.304	1.87	20.0	0.54
518029	1201064910	07-APR-2006 23:26	DUSE	1.58	1.5	num	0.78	0	-0.304	1.87	20.0	0.54
518036	1201064938	07-APR-2006 23:26	DUSE	1.08	0.55	num	0.78	0	-0.304	1.87	20.0	0.54

Thorium-230 BLANK: Limits LCL = -.4 UCL = .6

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
509059	1201045077	16-MAR-2006 08:39	DONE	0	-0.11	pCi/g	0.1	-0.424	-0.25	0.44	0.62	0.17
510647	1201048631	16-MAR-2006 10:55	DONE	0	0.06	pCi/g	0.1	-0.424	-0.25	0.44	0.62	0.17
511635	1201050914	18-MAR-2006 15:00	DONE	0	-0.44	pCi/g	0.1	-0.424	-0.25	0.44	0.62	0.17
511985	1201051674	18-MAR-2006 15:00	DONE	0	-0.21	pCi/g	0.1	-0.424	-0.25	0.44	0.62	0.17
511630	1201050905	20-MAR-2006 07:42	DONE	1	3	pCi/g	0.1	-0.424	-0.25	0.44	0.62	0.17
511996	1201051700	22-MAR-2006 14:23	DONE	0	-0.49	pCi/g	0.1	-0.424	-0.25	0.44	0.62	0.17
513053	1201054070	22-MAR-2006 19:41	DONE	0	-0.44	pCi/g	0.1	-0.424	-0.25	0.44	0.62	0.17
513051	1201054062	23-MAR-2006 08:31	DONE	0	-0.59	pCi/g	0.1	-0.424	-0.25	0.44	0.62	0.17
511992	1201051686	23-MAR-2006 21:21	DONE	0	-0.47	pCi/g	0.1	-0.424	-0.25	0.44	0.62	0.17
513052	1201054066	23-MAR-2006 23:50	DONE	0	-0.53	pCi/g	0.1	-0.424	-0.25	0.44	0.62	0.17
513416	1201054856	24-MAR-2006 12:39	DONE	0	-0.25	pCi/g	0.1	-0.424	-0.25	0.44	0.62	0.17
514672	1201057502	25-MAR-2006 19:34	DONE	0	-0.5	pCi/g	0.1	-0.424	-0.25	0.44	0.62	0.17
513418	1201054864	26-MAR-2006 07:39	DONE	0	-0.93	pCi/g	0.1	-0.424	-0.25	0.44	0.62	0.17
513759	1201055494	27-MAR-2006 17:14	DONE	0	-0.42	pCi/g	0.1	-0.424	-0.25	0.44	0.62	0.17
513435	1201054914	28-MAR-2006 11:41	DONE	0	0.72	pCi/g	0.1	-0.424	-0.25	0.44	0.62	0.17
512017	1201051748	28-MAR-2006 16:43	DUSE	0	-0.68	pCi/g	0.1	-0.424	-0.25	0.44	0.62	0.17
514175	1201056354	29-MAR-2006 15:32	DUSE	1	4.3	pCi/g	0.1	-0.424	-0.25	0.44	0.62	0.17
515260	1201058709	29-MAR-2006 16:59	DONE	0	-0.22	pCi/g	0.1	-0.424	-0.25	0.44	0.62	0.17
515263	1201058717	29-MAR-2006 22:27	DONE	0	-0.55	pCi/g	0.1	-0.424	-0.25	0.44	0.62	0.17
515264	1201058721	30-MAR-2006 09:13	DONE	0	-0.41	pCi/g	0.1	-0.424	-0.25	0.44	0.62	0.17

514144	1201056273	30-MAR-2006 18:04	DONE	0	0.29	pCi/g	0.1	-0.424	-0.25	0.44	0.62	0.17
515871	1201060180	31-MAR-2006 23:48	DONE	0	-0.49	pCi/g	0.1	-0.424	-0.25	0.44	0.62	0.17
515258	1201058701	01-APR-2006 09:23	DONE	0	0.04	pCi/g	0.1	-0.424	-0.25	0.44	0.62	0.17
515550	1201059422	02-APR-2006 07:36	DONE	0	-0.94	pCi/g	0.1	-0.424	-0.25	0.44	0.62	0.17
515556	1201059443	03-APR-2006 06:56	DUSE	0	-0.18	pCi/g	0.1	-0.424	-0.25	0.44	0.62	0.17
516132	1201060710	03-APR-2006 12:42	DONE	0	0.04	pCi/g	0.1	-0.424	-0.25	0.44	0.62	0.17
516806	1201062214	04-APR-2006 22:21	DONE	0	-0.27	pCi/g	0.1	-0.424	-0.25	0.44	0.62	0.17
516800	1201062199	05-APR-2006 09:51	DONE	0	-0.32	pCi/g	0.1	-0.424	-0.25	0.44	0.62	0.17
512068	1201051873	05-APR-2006 09:52	DONE	0	-0.62	pCi/g	0.1	-0.424	-0.25	0.44	0.62	0.17
512060	1201051841	05-APR-2006 10:05	DONE	0	0.69	pCi/g	0.1	-0.424	-0.25	0.44	0.62	0.17
517558	1201063868	05-APR-2006 15:35	DONE	0	0.13	pCi/g	0.1	-0.424	-0.25	0.44	0.62	0.17
517144	1201062899	05-APR-2006 15:35	DONE	0	-0.09	pCi/g	0.1	-0.424	-0.25	0.44	0.62	0.17
515901	1201060261	05-APR-2006 19:49	DUSE	0	0.82	pCi/g	0.1	-0.424	-0.25	0.44	0.62	0.17
517138	1201062879	05-APR-2006 19:53	DONE	0	-0.42	pCi/g	0.1	-0.424	-0.25	0.44	0.62	0.17
517139	1201062883	06-APR-2006 08:11	DONE	0	-0.38	pCi/g	0.1	-0.424	-0.25	0.44	0.62	0.17
516344	1201061149	06-APR-2006 13:23	DONE	0	-0.12	pCi/g	0.1	-0.424	-0.25	0.44	0.62	0.17
517153	1201062927	07-APR-2006 18:07	DONE	0	1.5	pCi/g	0.1	-0.424	-0.25	0.44	0.62	0.17
518029	1201064909	07-APR-2006 23:26	DONE	0	-0.26	pCi/g	0.1	-0.424	-0.25	0.44	0.62	0.17
518036	1201064937	07-APR-2006 23:26	DONE	0	-0.29	pCi/g	0.1	-0.424	-0.25	0.44	0.62	0.17

Thorium-230 DUP: Limits LCL = 0 UCL = 20

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
511710	1201051084	15-MAR-2006 13:59	DONE	9	-0.78	percent	29.3	0	-24	82.2	20.0	26.4
509059	1201045078	16-MAR-2006 08:39	DONE	32	0.09	percent	29.3	0	-24	82.2	20.0	26.4
510647	1201048632	16-MAR-2006 23:45	DONE	14	-0.6	percent	29.3	0	-24	82.2	20.0	26.4
511635	1201050915	18-MAR-2006 15:00	DONE	57	1	percent	29.3	0	-24	82.2	20.0	26.4
511985	1201051675	18-MAR-2006 15:00	DONE	9	-0.77	percent	29.3	0	-24	82.2	20.0	26.4
511630	1201050906	20-MAR-2006 07:42	DONE	52	0.85	percent	29.3	0	-24	82.2	20.0	26.4
513052	1201054067	22-MAR-2006 12:16	DONE	23	-0.22	percent	29.3	0	-24	82.2	20.0	26.4
511996	1201051701	22-MAR-2006 14:23	DONE	5	-0.93	percent	29.3	0	-24	82.2	20.0	26.4
513053	1201054071	22-MAR-2006 19:41	DONE	80	1.9	percent	29.3	0	-24	82.2	20.0	26.4
513051	1201054063	23-MAR-2006 08:31	DONE	15	-0.55	percent	29.3	0	-24	82.2	20.0	26.4
513416	1201054857	23-MAR-2006 23:50	DONE	40	0.41	percent	29.3	0	-24	82.2	20.0	26.4
511992	1201051687	25-MAR-2006 19:34	DONE	34	0.17	percent	29.3	0	-24	82.2	20.0	26.4
513418	1201054865	26-MAR-2006 07:39	DONE	64	1.3	percent	29.3	0	-24	82.2	20.0	26.4
513759	1201055495	27-MAR-2006 17:14	DONE	21	-0.32	percent	29.3	0	-24	82.2	20.0	26.4
513435	1201054915	28-MAR-2006 11:41	DONE	122	3.5	percent	29.3	0	-24	82.2	20.0	26.4
512017	1201051749	28-MAR-2006 16:43	DUSE	16	-0.5	percent	29.3	0	-24	82.2	20.0	26.4
514175	1201056355	29-MAR-2006 15:32	DUSE	1	-1	percent	29.3	0	-24	82.2	20.0	26.4
514144	1201056274	29-MAR-2006 19:54	DONE	8	-0.8	percent	29.3	0	-24	82.2	20.0	26.4
515263	1201058718	29-MAR-2006 22:27	DONE	35	0.23	percent	29.3	0	-24	82.2	20.0	26.4
515260	1201058710	29-MAR-2006 22:27	DONE	23	-0.25	percent	29.3	0	-24	82.2	20.0	26.4
515264	1201058722	30-MAR-2006 09:13	DONE	32	0.1	percent	29.3	0	-24	82.2	20.0	26.4
515258	1201058702	01-APR-2006 09:23	DONE	20	-0.34	percent	29.3	0	-24	82.2	20.0	26.4
515550	1201059423	02-APR-2006 07:36	DONE	11	-0.69	percent	29.3	0	-24	82.2	20.0	26.4
515556	1201059444	03-APR-2006 06:56	DUSE	30	0.02	percent	29.3	0	-24	82.2	20.0	26.4
516132	1201060711	03-APR-2006 12:42	DONE	9	-0.79	percent	29.3	0	-24	82.2	20.0	26.4
515871	1201060181	04-APR-2006 07:44	DONE	1	-1	percent	29.3	0	-24	82.2	20.0	26.4
516806	1201062215	05-APR-2006 08:19	DONE	28	-0.07	percent	29.3	0	-24	82.2	20.0	26.4
516800	1201062200	05-APR-2006 09:51	DONE	70	1.6	percent	29.3	0	-24	82.2	20.0	26.4

512068	1201051874	05-APR-2006 09:52	DONE	3	-1	percent	29.3	0	-24	82.2	20.0	26.4
512060	1201051842	05-APR-2006 10:05	DONE	2	-1	percent	29.3	0	-24	82.2	20.0	26.4
517558	1201063869	05-APR-2006 15:35	DONE	21	-0.3	percent	29.3	0	-24	82.2	20.0	26.4
517144	1201062900	05-APR-2006 15:35	DONE	25	-0.14	percent	29.3	0	-24	82.2	20.0	26.4
515901	1201060262	05-APR-2006 17:13	DUSE	0	-1	percent	29.3	0	-24	82.2	20.0	26.4
517138	1201062880	05-APR-2006 19:53	DONE	4	-0.96	percent	29.3	0	-24	82.2	20.0	26.4
517139	1201062884	06-APR-2006 08:11	DONE	18	-0.42	percent	29.3	0	-24	82.2	20.0	26.4
516344	1201061150	06-APR-2006 13:23	DONE	55	0.96	percent	29.3	0	-24	82.2	20.0	26.4
517153	1201062928	07-APR-2006 18:07	DONE	56	01	percent	29.3	0	-24	82.2	20.0	26.4
518029	1201064910	07-APR-2006 23:26	DONE	34	0.18	percent	29.3	0	-24	82.2	20.0	26.4
518036	1201064938	07-APR-2006 23:26	DONE	66	1.4	percent	29.3	0	-24	82.2	20.0	26.4

Thorium-230 LCS: Limits LCL = 75 UCL = 125

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
468546	1200949878	08-OCT-2005 11:20	DONE	92	-1	percent	100	75.0	83.3	117	125	8.33
469909	1200953017	13-OCT-2005 14:33	DONE	81	-2	percent	100	75.0	83.3	117	125	8.33
474649	1200964500	26-OCT-2005 11:44	DONE	90	-1	percent	100	75.0	83.3	117	125	8.33
473628	1200962206	29-OCT-2005 17:54	DONE	89	-1	percent	100	75.0	83.3	117	125	8.33
477050	1200970382	12-NOV-2005 14:49	DONE	105	0.6	percent	100	75.0	83.3	117	125	8.33
484101	1200987270	30-NOV-2005 14:54	DONE	102	0.24	percent	100	75.0	83.3	117	125	8.33
501251	1201026784	08-FEB-2006 22:33	DONE	104	0.48	percent	100	75.0	83.3	117	125	8.33
502256	1201029224	13-FEB-2006 20:20	DONE	105	0.6	percent	100	75.0	83.3	117	125	8.33
503140	1201031089	15-FEB-2006 23:29	DONE	119	2.3	percent	100	75.0	83.3	117	125	8.33
503146	1201031097	16-FEB-2006 21:40	DONE	108	0.96	percent	100	75.0	83.3	117	125	8.33
504921	1201035218	18-FEB-2006 21:35	DONE	94	-0.78	percent	100	75.0	83.3	117	125	8.33
505231	1201036007	21-FEB-2006 23:52	DONE	92	-0.97	percent	100	75.0	83.3	117	125	8.33
505233	1201036015	21-FEB-2006 23:52	DONE	102	0.24	percent	100	75.0	83.3	117	125	8.33
505622	1201036907	22-FEB-2006 21:19	DONE	103	0.36	percent	100	75.0	83.3	117	125	8.33
505914	1201037581	28-FEB-2006 20:09	DONE	90	-1	percent	100	75.0	83.3	117	125	8.33
508120	1201042932	02-MAR-2006 22:23	DONE	102	0.22	percent	100	75.0	83.3	117	125	8.33
508286	1201043313	09-MAR-2006 22:56	DONE	83	-2	percent	100	75.0	83.3	117	125	8.33
511064	1201049593	15-MAR-2006 07:51	DONE	99	-0.11	percent	100	75.0	83.3	117	125	8.33
511066	1201049597	15-MAR-2006 09:16	DONE	89	-1	percent	100	75.0	83.3	117	125	8.33
509059	1201045080	16-MAR-2006 09:25	DONE	105	0.6	percent	100	75.0	83.3	117	125	8.33
511635	1201050917	18-MAR-2006 15:00	DONE	93	-0.89	percent	100	75.0	83.3	117	125	8.33
511985	1201051677	18-MAR-2006 15:00	DONE	88	-1	percent	100	75.0	83.3	117	125	8.33
513053	1201054073	21-MAR-2006 17:40	DONE	91	-1	percent	100	75.0	83.3	117	125	8.33
513052	1201054069	22-MAR-2006 12:16	DONE	116	1.9	percent	100	75.0	83.3	117	125	8.33
513051	1201054065	23-MAR-2006 08:31	DONE	109	1.1	percent	100	75.0	83.3	117	125	8.33
514672	1201057504	25-MAR-2006 19:34	DONE	106	0.67	percent	100	75.0	83.3	117	125	8.33
513759	1201055497	28-MAR-2006 14:57	DONE	113	1.6	percent	100	75.0	83.3	117	125	8.33
512017	1201051750	28-MAR-2006 16:43	DONE	98	-0.28	percent	100	75.0	83.3	117	125	8.33
515263	1201058720	29-MAR-2006 22:27	DONE	101	0.12	percent	100	75.0	83.3	117	125	8.33
515264	1201058724	30-MAR-2006 09:13	DONE	119	2.3	percent	100	75.0	83.3	117	125	8.33
516132	1201060713	03-APR-2006 12:42	DONE	98	-0.23	percent	100	75.0	83.3	117	125	8.33
515871	1201060183	04-APR-2006 07:44	DONE	101	0.12	percent	100	75.0	83.3	117	125	8.33
516806	1201062217	04-APR-2006 22:21	DONE	101	0.12	percent	100	75.0	83.3	117	125	8.33
517138	1201062882	05-APR-2006 19:53	DONE	103	0.36	percent	100	75.0	83.3	117	125	8.33
516800	1201062202	06-APR-2006 08:11	DONE	95	-0.55	percent	100	75.0	83.3	117	125	8.33
517139	1201062886	07-APR-2006 13:44	DONE	101	0.12	percent	100	75.0	83.3	117	125	8.33

518029	1201064912	07-APR-2006 23:26	DONE	94	-0.67	percent	100	75.0	83.3	117	125	8.33
518036	1201064940	07-APR-2006 23:26	DONE	101	0.12	percent	100	75.0	83.3	117	125	8.33
517153	1201062930	08-APR-2006 08:46	DONE	85	-2	percent	100	75.0	83.3	117	125	8.33

Thorium-230 RER: Limits LCL = 0 UCL = 20

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
511710	1201051084	15-MAR-2006 13:59	DONE	0.6	-0.47	num	0.97	0	-0.569	2.5	20.0	0.77
509059	1201045078	16-MAR-2006 08:39	DONE	0.78	-0.24	num	0.97	0	-0.569	2.5	20.0	0.77
510647	1201048632	16-MAR-2006 23:45	DONE	0.64	-0.43	num	0.97	0	-0.569	2.5	20.0	0.77
511635	1201050915	18-MAR-2006 15:00	DONE	1.47	0.66	num	0.97	0	-0.569	2.5	20.0	0.77
511985	1201051675	18-MAR-2006 15:00	DONE	0.22	-0.97	num	0.97	0	-0.569	2.5	20.0	0.77
511630	1201050906	20-MAR-2006 07:42	DONE	1.15	0.24	num	0.97	0	-0.569	2.5	20.0	0.77
513052	1201054067	22-MAR-2006 12:16	DONE	0.83	-0.18	num	0.97	0	-0.569	2.5	20.0	0.77
511996	1201051701	22-MAR-2006 14:23	DONE	0.24	-0.95	num	0.97	0	-0.569	2.5	20.0	0.77
513053	1201054071	22-MAR-2006 19:41	DONE	2.38	1.8	num	0.97	0	-0.569	2.5	20.0	0.77
513051	1201054063	23-MAR-2006 08:31	DONE	0.55	-0.54	num	0.97	0	-0.569	2.5	20.0	0.77
513416	1201054857	23-MAR-2006 23:50	DONE	1.28	0.41	num	0.97	0	-0.569	2.5	20.0	0.77
511992	1201051687	25-MAR-2006 19:34	DONE	2.7	2.3	num	0.97	0	-0.569	2.5	20.0	0.77
513418	1201054865	26-MAR-2006 07:39	DONE	1.74	1	num	0.97	0	-0.569	2.5	20.0	0.77
513759	1201055495	27-MAR-2006 17:14	DONE	0.71	-0.33	num	0.97	0	-0.569	2.5	20.0	0.77
513435	1201054915	28-MAR-2006 11:41	DONE	1.83	1.1	num	0.97	0	-0.569	2.5	20.0	0.77
512017	1201051749	28-MAR-2006 16:43	DUSE	0.41	-0.72	num	0.97	0	-0.569	2.5	20.0	0.77
514175	1201056355	29-MAR-2006 15:32	DUSE	0.06	-1	num	0.97	0	-0.569	2.5	20.0	0.77
514144	1201056274	29-MAR-2006 19:54	DONE	0.31	-0.86	num	0.97	0	-0.569	2.5	20.0	0.77
515263	1201058718	29-MAR-2006 22:27	DONE	0.92	-0.07	num	0.97	0	-0.569	2.5	20.0	0.77
515260	1201058710	29-MAR-2006 22:27	DONE	0.31	-0.85	num	0.97	0	-0.569	2.5	20.0	0.77
515264	1201058722	30-MAR-2006 09:13	DONE	1.08	0.15	num	0.97	0	-0.569	2.5	20.0	0.77
515258	1201058702	01-APR-2006 09:23	DONE	0.9	-0.09	num	0.97	0	-0.569	2.5	20.0	0.77
515550	1201059423	02-APR-2006 07:36	DONE	0.78	-0.24	num	0.97	0	-0.569	2.5	20.0	0.77
515556	1201059444	03-APR-2006 06:56	DUSE	1.14	0.23	num	0.97	0	-0.569	2.5	20.0	0.77
516132	1201060711	03-APR-2006 12:42	DONE	0.38	-0.77	num	0.97	0	-0.569	2.5	20.0	0.77
515871	1201060181	04-APR-2006 07:44	DONE	0.05	-1	num	0.97	0	-0.569	2.5	20.0	0.77
516806	1201062215	05-APR-2006 08:19	DONE	1.04	0.09	num	0.97	0	-0.569	2.5	20.0	0.77
516800	1201062200	05-APR-2006 09:51	DONE	2.58	2.1	num	0.97	0	-0.569	2.5	20.0	0.77
512068	1201051874	05-APR-2006 09:52	DONE	0.11	-1	num	0.97	0	-0.569	2.5	20.0	0.77
512060	1201051842	05-APR-2006 10:05	DONE	0.04	-1	num	0.97	0	-0.569	2.5	20.0	0.77
517558	1201063869	05-APR-2006 15:35	DONE	0.71	-0.33	num	0.97	0	-0.569	2.5	20.0	0.77
517144	1201062900	05-APR-2006 15:35	DONE	0.5	-0.6	num	0.97	0	-0.569	2.5	20.0	0.77
515901	1201060262	05-APR-2006 17:13	DUSE	0.02	-1	num	0.97	0	-0.569	2.5	20.0	0.77
517138	1201062880	05-APR-2006 19:53	DONE	0.25	-0.93	num	0.97	0	-0.569	2.5	20.0	0.77
517139	1201062884	06-APR-2006 08:11	DONE	0.98	0.02	num	0.97	0	-0.569	2.5	20.0	0.77
516344	1201061150	06-APR-2006 13:23	DONE	1.78	1.1	num	0.97	0	-0.569	2.5	20.0	0.77
517153	1201062928	07-APR-2006 18:07	DONE	2.01	1.4	num	0.97	0	-0.569	2.5	20.0	0.77
518029	1201064910	07-APR-2006 23:26	DONE	1.54	0.74	num	0.97	0	-0.569	2.5	20.0	0.77
518036	1201064938	07-APR-2006 23:26	DONE	2.64	2.2	num	0.97	0	-0.569	2.5	20.0	0.77

Thorium-230 SPIKE: Limits LCL = 75 UCL = 125

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
458331	1200925417	19-SEP-2005 17:20	DONE	76	-3	percent	100	75.0	83.3	117	125	8.33
458329	1200925413	22-SEP-2005 10:43	DONE	79	-3	percent	100	75.0	83.3	117	125	8.33

458322	1200925401	22-SEP-2005 10:43	DONE	67	-4	percent	100	75.0	83.3	117	125	8.33
468546	1200949877	08-OCT-2005 11:20	DONE	92	-1	percent	100	75.0	83.3	117	125	8.33
474649	1200964499	26-OCT-2005 11:44	DONE	79	-3	percent	100	75.0	83.3	117	125	8.33
484101	1200987269	30-NOV-2005 14:54	DONE	100	-0.04	percent	100	75.0	83.3	117	125	8.33
501251	1201026783	08-FEB-2006 22:33	DONE	87	-2	percent	100	75.0	83.3	117	125	8.33
501251	1201026786	08-FEB-2006 22:33	DONE	87	-2	percent	100	75.0	83.3	117	125	8.33
502256	1201029223	13-FEB-2006 20:20	DONE	114	1.7	percent	100	75.0	83.3	117	125	8.33
503140	1201031088	15-FEB-2006 23:29	DONE	110	1.2	percent	100	75.0	83.3	117	125	8.33
503146	1201031096	16-FEB-2006 21:40	DONE	119	2.3	percent	100	75.0	83.3	117	125	8.33
504921	1201035217	18-FEB-2006 21:35	DONE	105	0.6	percent	100	75.0	83.3	117	125	8.33
505231	1201036006	21-FEB-2006 23:52	DONE	88	-1	percent	100	75.0	83.3	117	125	8.33
505233	1201036014	21-FEB-2006 23:52	DONE	105	0.6	percent	100	75.0	83.3	117	125	8.33
505622	1201036906	22-FEB-2006 21:19	DONE	86	-2	percent	100	75.0	83.3	117	125	8.33
505914	1201037580	27-FEB-2006 22:01	DONE	103	0.36	percent	100	75.0	83.3	117	125	8.33
508120	1201042931	02-MAR-2006 22:23	DONE	111	1.3	percent	100	75.0	83.3	117	125	8.33
508286	1201043312	09-MAR-2006 22:56	DONE	101	0.12	percent	100	75.0	83.3	117	125	8.33
511064	1201049592	14-MAR-2006 21:50	DONE	97	-0.31	percent	100	75.0	83.3	117	125	8.33
511066	1201049596	15-MAR-2006 09:16	DONE	85	-2	percent	100	75.0	83.3	117	125	8.33
509059	1201045079	17-MAR-2006 09:53	DONE	102	0.24	percent	100	75.0	83.3	117	125	8.33
511985	1201051676	18-MAR-2006 15:00	DONE	101	0.12	percent	100	75.0	83.3	117	125	8.33
511635	1201050916	20-MAR-2006 16:57	DONE	114	1.7	percent	100	75.0	83.3	117	125	8.33
513053	1201054072	21-MAR-2006 17:40	DONE	95	-0.65	percent	100	75.0	83.3	117	125	8.33
513052	1201054068	22-MAR-2006 12:16	DONE	98	-0.22	percent	100	75.0	83.3	117	125	8.33
513051	1201054064	23-MAR-2006 08:31	DONE	106	0.72	percent	100	75.0	83.3	117	125	8.33
514672	1201057503	25-MAR-2006 19:34	DONE	123	2.8	percent	100	75.0	83.3	117	125	8.33
513759	1201055496	27-MAR-2006 17:14	DONE	89	-1	percent	100	75.0	83.3	117	125	8.33
515263	1201058719	29-MAR-2006 22:27	DONE	113	1.6	percent	100	75.0	83.3	117	125	8.33
515264	1201058723	30-MAR-2006 09:13	DONE	96	-0.51	percent	100	75.0	83.3	117	125	8.33
515871	1201060182	31-MAR-2006 23:48	DONE	79	-2	percent	100	75.0	83.3	117	125	8.33
516132	1201060712	03-APR-2006 12:42	DONE	103	0.36	percent	100	75.0	83.3	117	125	8.33
516806	1201062216	04-APR-2006 22:21	DONE	94	-0.72	percent	100	75.0	83.3	117	125	8.33
516800	1201062201	05-APR-2006 09:51	DONE	98	-0.23	percent	100	75.0	83.3	117	125	8.33
517138	1201062881	05-APR-2006 19:53	DONE	98	-0.28	percent	100	75.0	83.3	117	125	8.33
517139	1201062885	06-APR-2006 08:11	DONE	92	-0.95	percent	100	75.0	83.3	117	125	8.33
517153	1201062929	07-APR-2006 18:07	DONE	85	-2	percent	100	75.0	83.3	117	125	8.33
518029	1201064911	07-APR-2006 23:26	DONE	82	-2	percent	100	75.0	83.3	117	125	8.33
518036	1201064939	07-APR-2006 23:26	DONE	104	0.48	percent	100	75.0	83.3	117	125	8.33

Thorium-232 BLANK: Limits LCL = -.1 UCL = .1

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
509059	1201045077	16-MAR-2006 08:39	DONE	0	0.65	pCi/g	-0.001	-0.081	-0.055	0.05	0.08	0.03
510647	1201048631	16-MAR-2006 10:55	DONE	0	1.3	pCi/g	-0.001	-0.081	-0.055	0.05	0.08	0.03
511635	1201050914	18-MAR-2006 15:00	DUSE	0	0.49	pCi/g	-0.001	-0.081	-0.055	0.05	0.08	0.03
511985	1201051674	18-MAR-2006 15:00	DUSE	0	-0.74	pCi/g	-0.001	-0.081	-0.055	0.05	0.08	0.03
511630	1201050905	20-MAR-2006 07:42	DONE	0	-0.29	pCi/g	-0.001	-0.081	-0.055	0.05	0.08	0.03
511996	1201051700	22-MAR-2006 14:23	DONE	0	-0.28	pCi/g	-0.001	-0.081	-0.055	0.05	0.08	0.03
513053	1201054070	22-MAR-2006 19:41	DUSE	0	-0.52	pCi/g	-0.001	-0.081	-0.055	0.05	0.08	0.03
513051	1201054062	23-MAR-2006 08:31	DUSE	0	-0.22	pCi/g	-0.001	-0.081	-0.055	0.05	0.08	0.03
511992	1201051686	23-MAR-2006 21:21	DONE	0	0.19	pCi/g	-0.001	-0.081	-0.055	0.05	0.08	0.03
513052	1201054066	23-MAR-2006 23:50	DUSE	0	-0.57	pCi/g	-0.001	-0.081	-0.055	0.05	0.08	0.03

513416	1201054856	24-MAR-2006 12:39	DONE	0	-0.82	pCi/g	-0.001	-0.081	-0.055	0.05	0.08	0.03
514672	1201057502	25-MAR-2006 19:34	DUSE	0	0.05	pCi/g	-0.001	-0.081	-0.055	0.05	0.08	0.03
513418	1201054864	26-MAR-2006 07:39	DONE	0	-3	pCi/g	-0.001	-0.081	-0.055	0.05	0.08	0.03
513759	1201055494	27-MAR-2006 17:14	DUSE	0	-0.3	pCi/g	-0.001	-0.081	-0.055	0.05	0.08	0.03
513435	1201054914	28-MAR-2006 11:41	DONE	0	1.6	pCi/g	-0.001	-0.081	-0.055	0.05	0.08	0.03
512017	1201051748	28-MAR-2006 16:43	DONE	0	-0.4	pCi/g	-0.001	-0.081	-0.055	0.05	0.08	0.03
514175	1201056354	29-MAR-2006 15:32	DUSE	0	2.2	pCi/g	-0.001	-0.081	-0.055	0.05	0.08	0.03
515260	1201058709	29-MAR-2006 16:59	DONE	0	-0.48	pCi/g	-0.001	-0.081	-0.055	0.05	0.08	0.03
515263	1201058717	29-MAR-2006 22:27	DUSE	0	-0.28	pCi/g	-0.001	-0.081	-0.055	0.05	0.08	0.03
515264	1201058721	30-MAR-2006 09:13	DUSE	0	-0.26	pCi/g	-0.001	-0.081	-0.055	0.05	0.08	0.03
514144	1201056273	30-MAR-2006 18:04	DONE	0	0.11	pCi/g	-0.001	-0.081	-0.055	0.05	0.08	0.03
515871	1201060180	31-MAR-2006 23:48	DUSE	0	0.16	pCi/g	-0.001	-0.081	-0.055	0.05	0.08	0.03
515258	1201058701	01-APR-2006 09:23	DONE	0	-2	pCi/g	-0.001	-0.081	-0.055	0.05	0.08	0.03
515550	1201059422	02-APR-2006 07:36	DONE	0	-3	pCi/g	-0.001	-0.081	-0.055	0.05	0.08	0.03
515556	1201059443	03-APR-2006 06:56	DUSE	0	0.06	pCi/g	-0.001	-0.081	-0.055	0.05	0.08	0.03
516132	1201060710	03-APR-2006 12:42	DUSE	0	0.53	pCi/g	-0.001	-0.081	-0.055	0.05	0.08	0.03
516806	1201062214	04-APR-2006 22:21	DUSE	0	-0.01	pCi/g	-0.001	-0.081	-0.055	0.05	0.08	0.03
516800	1201062199	05-APR-2006 09:51	DUSE	0	-0.09	pCi/g	-0.001	-0.081	-0.055	0.05	0.08	0.03
512068	1201051873	05-APR-2006 09:52	DONE	0	-0.15	pCi/g	-0.001	-0.081	-0.055	0.05	0.08	0.03
512060	1201051841	05-APR-2006 10:05	DONE	0	1	pCi/g	-0.001	-0.081	-0.055	0.05	0.08	0.03
517558	1201063868	05-APR-2006 15:35	DONE	0	0.35	pCi/g	-0.001	-0.081	-0.055	0.05	0.08	0.03
517144	1201062899	05-APR-2006 15:35	DONE	0	0.89	pCi/g	-0.001	-0.081	-0.055	0.05	0.08	0.03
515901	1201060261	05-APR-2006 19:49	DUSE	0	1.6	pCi/g	-0.001	-0.081	-0.055	0.05	0.08	0.03
517138	1201062879	05-APR-2006 19:53	DUSE	0	-0.06	pCi/g	-0.001	-0.081	-0.055	0.05	0.08	0.03
517139	1201062883	06-APR-2006 08:11	DUSE	0	0.17	pCi/g	-0.001	-0.081	-0.055	0.05	0.08	0.03
516344	1201061149	06-APR-2006 13:23	DONE	0	0.81	pCi/g	-0.001	-0.081	-0.055	0.05	0.08	0.03
517153	1201062927	07-APR-2006 18:07	DONE	0	0.3	pCi/g	-0.001	-0.081	-0.055	0.05	0.08	0.03
518029	1201064909	07-APR-2006 23:26	DUSE	0	0.35	pCi/g	-0.001	-0.081	-0.055	0.05	0.08	0.03
518036	1201064937	07-APR-2006 23:26	DUSE	0	0.06	pCi/g	-0.001	-0.081	-0.055	0.05	0.08	0.03

Thorium-232 DUP: Limits LCL = 0 UCL = 20

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
511710	1201051084	15-MAR-2006 13:59	DONE	3	-0.43	percent	54.7	0	-180	293	20.0	119
509059	1201045078	16-MAR-2006 08:39	DONE	78	0.19	percent	54.7	0	-180	293	20.0	119
510647	1201048632	16-MAR-2006 23:45	DONE	28	-0.22	percent	54.7	0	-180	293	20.0	119
511635	1201050915	18-MAR-2006 15:00	DUSE	1	-0.45	percent	54.7	0	-180	293	20.0	119
511985	1201051675	18-MAR-2006 15:00	DUSE	88	0.28	percent	54.7	0	-180	293	20.0	119
511630	1201050906	20-MAR-2006 07:42	DONE	45	-0.08	percent	54.7	0	-180	293	20.0	119
513052	1201054067	22-MAR-2006 12:16	DUSE	39	-0.13	percent	54.7	0	-180	293	20.0	119
511996	1201051701	22-MAR-2006 14:23	DONE	7	-0.4	percent	54.7	0	-180	293	20.0	119
513053	1201054071	22-MAR-2006 19:41	DUSE	29	-0.21	percent	54.7	0	-180	293	20.0	119
513051	1201054063	23-MAR-2006 08:31	DUSE	56	0.01	percent	54.7	0	-180	293	20.0	119
513416	1201054857	23-MAR-2006 23:50	DONE	40	-0.13	percent	54.7	0	-180	293	20.0	119
511992	1201051687	25-MAR-2006 19:34	DONE	13	-0.35	percent	54.7	0	-180	293	20.0	119
513418	1201054865	26-MAR-2006 07:39	DONE	4	-0.42	percent	54.7	0	-180	293	20.0	119
513759	1201055495	27-MAR-2006 17:14	DUSE	24	-0.26	percent	54.7	0	-180	293	20.0	119
513435	1201054915	28-MAR-2006 11:41	DONE	744	5.8	percent	54.7	0	-180	293	20.0	119
512017	1201051749	28-MAR-2006 16:43	DONE	3	-0.43	percent	54.7	0	-180	293	20.0	119
514175	1201056355	29-MAR-2006 15:32	DUSE	44	-0.09	percent	54.7	0	-180	293	20.0	119
514144	1201056274	29-MAR-2006 19:54	DONE	16	-0.33	percent	54.7	0	-180	293	20.0	119

515263	1201058718	29-MAR-2006 22:27	DUSE	155	0.84	percent	54.7	0	-180	293	20.0	119
515260	1201058710	29-MAR-2006 22:27	DONE	38	-0.14	percent	54.7	0	-180	293	20.0	119
515264	1201058722	30-MAR-2006 09:13	DUSE	17	-0.32	percent	54.7	0	-180	293	20.0	119
515258	1201058702	01-APR-2006 09:23	DONE	18	-0.31	percent	54.7	0	-180	293	20.0	119
515550	1201059423	02-APR-2006 07:36	DONE	10	-0.37	percent	54.7	0	-180	293	20.0	119
515556	1201059444	03-APR-2006 06:56	DUSE	27	-0.24	percent	54.7	0	-180	293	20.0	119
516132	1201060711	03-APR-2006 12:42	DUSE	31	-0.2	percent	54.7	0	-180	293	20.0	119
515871	1201060181	04-APR-2006 07:44	DUSE	2	-0.44	percent	54.7	0	-180	293	20.0	119
516806	1201062215	05-APR-2006 08:19	DUSE	14	-0.34	percent	54.7	0	-180	293	20.0	119
516800	1201062200	05-APR-2006 09:51	DUSE	143	0.74	percent	54.7	0	-180	293	20.0	119
512068	1201051874	05-APR-2006 09:52	DONE	35	-0.16	percent	54.7	0	-180	293	20.0	119
512060	1201051842	05-APR-2006 10:05	DONE	24	-0.26	percent	54.7	0	-180	293	20.0	119
517558	1201063869	05-APR-2006 15:35	DONE	33	-0.18	percent	54.7	0	-180	293	20.0	119
517144	1201062900	05-APR-2006 15:35	DONE	141	0.72	percent	54.7	0	-180	293	20.0	119
515901	1201060262	05-APR-2006 17:13	DUSE	27	-0.23	percent	54.7	0	-180	293	20.0	119
517138	1201062880	05-APR-2006 19:53	DUSE	20	-0.29	percent	54.7	0	-180	293	20.0	119
517139	1201062884	06-APR-2006 08:11	DUSE	30	-0.21	percent	54.7	0	-180	293	20.0	119
516344	1201061150	06-APR-2006 13:23	DONE	37	-0.15	percent	54.7	0	-180	293	20.0	119
517153	1201062928	07-APR-2006 18:07	DONE	40	-0.13	percent	54.7	0	-180	293	20.0	119
518029	1201064910	07-APR-2006 23:26	DUSE	2	-0.44	percent	54.7	0	-180	293	20.0	119
518036	1201064938	07-APR-2006 23:26	DUSE	29	-0.22	percent	54.7	0	-180	293	20.0	119

Thorium-232 LCS: Limits LCL = 75 UCL = 125

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
498910	1201021223	03-FEB-2006 12:18	DONE	79	-3	percent	100	75.0	83.3	117	125	8.33
499049	1201021535	03-FEB-2006 12:18	DONE	98	-0.26	percent	100	75.0	83.3	117	125	8.33
500715	1201025585	13-FEB-2006 16:03	DONE	114	1.7	percent	100	75.0	83.3	117	125	8.33
502831	1201030463	14-FEB-2006 20:33	DUSE	96	-0.44	percent	100	75.0	83.3	117	125	8.33
503670	1201032267	15-FEB-2006 23:29	DONE	109	1.1	percent	100	75.0	83.3	117	125	8.33
503667	1201032256	16-FEB-2006 21:40	DONE	92	-0.98	percent	100	75.0	83.3	117	125	8.33
499044	1201021522	17-FEB-2006 16:17	DONE	111	1.3	percent	100	75.0	83.3	117	125	8.33
505917	1201037593	27-FEB-2006 12:52	DUSE	97	-0.36	percent	100	75.0	83.3	117	125	8.33
507247	1201040735	28-FEB-2006 15:46	DONE	125	3.00	percent	100	75.0	83.3	117	125	8.33
504463	1201034136	28-FEB-2006 15:47	DONE	85	-2	percent	100	75.0	83.3	117	125	8.33
504462	1201034132	01-MAR-2006 16:22	DONE	109	1.1	percent	100	75.0	83.3	117	125	8.33
504467	1201034152	01-MAR-2006 16:22	DONE	90	-1	percent	100	75.0	83.3	117	125	8.33
508044	1201042748	02-MAR-2006 22:23	DONE	114	1.7	percent	100	75.0	83.3	117	125	8.33
508046	1201042756	06-MAR-2006 20:51	DONE	111	1.3	percent	100	75.0	83.3	117	125	8.33
508285	1201043299	07-MAR-2006 23:35	DONE	109	1.1	percent	100	75.0	83.3	117	125	8.33
507801	1201042216	08-MAR-2006 08:59	DONE	98	-0.23	percent	100	75.0	83.3	117	125	8.33
509083	1201045144	09-MAR-2006 07:20	DONE	116	1.9	percent	100	75.0	83.3	117	125	8.33
508587	1201044004	10-MAR-2006 13:18	DONE	110	1.2	percent	100	75.0	83.3	117	125	8.33
508589	1201044012	11-MAR-2006 09:34	DONE	115	1.8	percent	100	75.0	83.3	117	125	8.33
510495	1201048295	13-MAR-2006 13:51	DONE	90	-1	percent	100	75.0	83.3	117	125	8.33
510629	1201048589	13-MAR-2006 13:51	DONE	87	-2	percent	100	75.0	83.3	117	125	8.33
509832	1201046784	15-MAR-2006 09:16	DONE	89	-1	percent	100	75.0	83.3	117	125	8.33
511710	1201051086	15-MAR-2006 13:59	DONE	113	1.6	percent	100	75.0	83.3	117	125	8.33
510647	1201048634	16-MAR-2006 23:45	DONE	117	2	percent	100	75.0	83.3	117	125	8.33
511630	1201050908	20-MAR-2006 07:42	DONE	95	-0.59	percent	100	75.0	83.3	117	125	8.33
511996	1201051703	22-MAR-2006 14:23	DONE	108	0.96	percent	100	75.0	83.3	117	125	8.33

511992	1201051689	23-MAR-2006 21:21	DONE	99	-0.08	percent	100	75.0	83.3	117	125	8.33
513416	1201054859	23-MAR-2006 23:50	DONE	105	0.6	percent	100	75.0	83.3	117	125	8.33
513418	1201054867	27-MAR-2006 14:43	DONE	99	-0.07	percent	100	75.0	83.3	117	125	8.33
513435	1201054917	28-MAR-2006 11:41	DONE	117	2	percent	100	75.0	83.3	117	125	8.33
514144	1201056276	29-MAR-2006 19:54	DONE	84	-2	percent	100	75.0	83.3	117	125	8.33
515260	1201058712	29-MAR-2006 22:27	DONE	115	1.8	percent	100	75.0	83.3	117	125	8.33
515258	1201058704	01-APR-2006 09:23	DONE	111	1.3	percent	100	75.0	83.3	117	125	8.33
515550	1201059425	02-APR-2006 07:36	DONE	83	-2	percent	100	75.0	83.3	117	125	8.33
512068	1201051876	05-APR-2006 09:52	DONE	88	-2	percent	100	75.0	83.3	117	125	8.33
512060	1201051844	05-APR-2006 10:05	DONE	92	-0.92	percent	100	75.0	83.3	117	125	8.33
517558	1201063871	05-APR-2006 15:35	DONE	83	-2	percent	100	75.0	83.3	117	125	8.33
517144	1201062902	05-APR-2006 17:13	DONE	90	-1	percent	100	75.0	83.3	117	125	8.33
516344	1201061152	06-APR-2006 13:23	DONE	122	2.6	percent	100	75.0	83.3	117	125	8.33

Thorium-232 RER: Limits LCL = 0 UCL = 20

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
511710	1201051084	15-MAR-2006 13:59	DONE	0.23	-1	num	0.91	0	-0.411	2.23	20.0	0.66
509059	1201045078	16-MAR-2006 08:39	DONE	1.76	1.3	num	0.91	0	-0.411	2.23	20.0	0.66
510647	1201048632	16-MAR-2006 23:45	DONE	0.9	-0.01	num	0.91	0	-0.411	2.23	20.0	0.66
511635	1201050915	18-MAR-2006 15:00	DUSE	0.01	-1	num	0.91	0	-0.411	2.23	20.0	0.66
511985	1201051675	18-MAR-2006 15:00	DUSE	1.84	1.4	num	0.91	0	-0.411	2.23	20.0	0.66
511630	1201050906	20-MAR-2006 07:42	DONE	0.64	-0.41	num	0.91	0	-0.411	2.23	20.0	0.66
513052	1201054067	22-MAR-2006 12:16	DUSE	1.06	0.22	num	0.91	0	-0.411	2.23	20.0	0.66
511996	1201051701	22-MAR-2006 14:23	DONE	0.31	-0.9	num	0.91	0	-0.411	2.23	20.0	0.66
513053	1201054071	22-MAR-2006 19:41	DUSE	0.59	-0.48	num	0.91	0	-0.411	2.23	20.0	0.66
513051	1201054063	23-MAR-2006 08:31	DUSE	1.65	1.1	num	0.91	0	-0.411	2.23	20.0	0.66
513416	1201054857	23-MAR-2006 23:50	DONE	0.82	-0.13	num	0.91	0	-0.411	2.23	20.0	0.66
511992	1201051687	25-MAR-2006 19:34	DONE	0.42	-0.74	num	0.91	0	-0.411	2.23	20.0	0.66
513418	1201054865	26-MAR-2006 07:39	DONE	0.09	-1	num	0.91	0	-0.411	2.23	20.0	0.66
513759	1201055495	27-MAR-2006 17:14	DUSE	0.31	-0.91	num	0.91	0	-0.411	2.23	20.0	0.66
513435	1201054915	28-MAR-2006 11:41	DONE	1.7	1.2	num	0.91	0	-0.411	2.23	20.0	0.66
512017	1201051749	28-MAR-2006 16:43	DONE	0.08	-1	num	0.91	0	-0.411	2.23	20.0	0.66
514175	1201056355	29-MAR-2006 15:32	DUSE	1.81	1.4	num	0.91	0	-0.411	2.23	20.0	0.66
514144	1201056274	29-MAR-2006 19:54	DONE	0.47	-0.67	num	0.91	0	-0.411	2.23	20.0	0.66
515263	1201058718	29-MAR-2006 22:27	DUSE	1.88	1.5	num	0.91	0	-0.411	2.23	20.0	0.66
515260	1201058710	29-MAR-2006 22:27	DONE	0.48	-0.64	num	0.91	0	-0.411	2.23	20.0	0.66
515264	1201058722	30-MAR-2006 09:13	DUSE	0.24	-1	num	0.91	0	-0.411	2.23	20.0	0.66
515258	1201058702	01-APR-2006 09:23	DONE	0.61	-0.45	num	0.91	0	-0.411	2.23	20.0	0.66
515550	1201059423	02-APR-2006 07:36	DONE	0.7	-0.31	num	0.91	0	-0.411	2.23	20.0	0.66
515556	1201059444	03-APR-2006 06:56	DUSE	0.91	0.01	num	0.91	0	-0.411	2.23	20.0	0.66
516132	1201060711	03-APR-2006 12:42	DUSE	1.08	0.26	num	0.91	0	-0.411	2.23	20.0	0.66
515871	1201060181	04-APR-2006 07:44	DUSE	0.09	-1	num	0.91	0	-0.411	2.23	20.0	0.66
516806	1201062215	05-APR-2006 08:19	DUSE	0.46	-0.68	num	0.91	0	-0.411	2.23	20.0	0.66
516800	1201062200	05-APR-2006 09:51	DUSE	2.31	2.1	num	0.91	0	-0.411	2.23	20.0	0.66
512068	1201051874	05-APR-2006 09:52	DONE	1.48	0.87	num	0.91	0	-0.411	2.23	20.0	0.66
512060	1201051842	05-APR-2006 10:05	DONE	0.65	-0.39	num	0.91	0	-0.411	2.23	20.0	0.66
517558	1201063869	05-APR-2006 15:35	DONE	1.01	0.15	num	0.91	0	-0.411	2.23	20.0	0.66
517144	1201062900	05-APR-2006 15:35	DONE	2.43	2.3	num	0.91	0	-0.411	2.23	20.0	0.66
515901	1201060262	05-APR-2006 17:13	DUSE	1.04	0.2	num	0.91	0	-0.411	2.23	20.0	0.66
517138	1201062880	05-APR-2006 19:53	DUSE	0.76	-0.22	num	0.91	0	-0.411	2.23	20.0	0.66


517139	1201062884	06-APR-2006 08:11	DUSE	1.13	0.34	num	0.91	0	-0.411	2.23	20.0	0.66
516344	1201061150	06-APR-2006 13:23	DONE	1.21	0.46	num	0.91	0	-0.411	2.23	20.0	0.66
517153	1201062928	07-APR-2006 18:07	DONE	1.71	1.2	num	0.91	0	-0.411	2.23	20.0	0.66
518029	1201064910	07-APR-2006 23:26	DUSE	0.07	-1	num	0.91	0	-0.411	2.23	20.0	0.66
518036	1201064938	07-APR-2006 23:26	DUSE	0.47	-0.66	num	0.91	0	-0.411	2.23	20.0	0.66

Thorium-232 SPIKE: Limits LCL = 75 UCL = 125

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
499692	1201023012	02-FEB-2006 21:07	DONE	113	1.6	percent	100	75.0	83.3	117	125	8.33
498910	1201021222	03-FEB-2006 12:18	DONE	85	-2	percent	100	75.0	83.3	117	125	8.33
499049	1201021534	03-FEB-2006 12:18	DONE	133	4	percent	100	75.0	83.3	117	125	8.33
500715	1201025584	13-FEB-2006 16:03	DONE	95	-0.6	percent	100	75.0	83.3	117	125	8.33
502831	1201030462	14-FEB-2006 20:33	DUSE	101	0.12	percent	100	75.0	83.3	117	125	8.33
503670	1201032266	15-FEB-2006 23:29	DONE	110	1.2	percent	100	75.0	83.3	117	125	8.33
503667	1201032255	16-FEB-2006 21:41	DONE	106	0.72	percent	100	75.0	83.3	117	125	8.33
499044	1201021521	17-FEB-2006 16:17	DONE	121	2.5	percent	100	75.0	83.3	117	125	8.33
505917	1201037592	27-FEB-2006 12:52	DUSE	101	0.12	percent	100	75.0	83.3	117	125	8.33
507247	1201040734	28-FEB-2006 15:46	DONE	119	2.3	percent	100	75.0	83.3	117	125	8.33
504463	1201034135	28-FEB-2006 15:47	DONE	103	0.36	percent	100	75.0	83.3	117	125	8.33
504462	1201034131	01-MAR-2006 16:22	DONE	99	-0.08	percent	100	75.0	83.3	117	125	8.33
504467	1201034151	01-MAR-2006 16:22	DONE	95	-0.61	percent	100	75.0	83.3	117	125	8.33
508044	1201042747	02-MAR-2006 22:23	DONE	85	-2	percent	100	75.0	83.3	117	125	8.33
508046	1201042755	04-MAR-2006 21:34	DONE	125	3.00	percent	100	75.0	83.3	117	125	8.33
508285	1201043303	07-MAR-2006 23:35	DONE	84	-2	percent	100	75.0	83.3	117	125	8.33
507801	1201042215	08-MAR-2006 08:59	DONE	78	-3	percent	100	75.0	83.3	117	125	8.33
509083	1201045143	08-MAR-2006 16:39	DONE	91	-1	percent	100	75.0	83.3	117	125	8.33
508587	1201044003	09-MAR-2006 13:56	DONE	112	1.4	percent	100	75.0	83.3	117	125	8.33
508589	1201044011	09-MAR-2006 16:01	DONE	90	-1	percent	100	75.0	83.3	117	125	8.33
510495	1201048294	13-MAR-2006 13:51	DONE	84	-2	percent	100	75.0	83.3	117	125	8.33
510629	1201048588	13-MAR-2006 13:51	DONE	90	-1	percent	100	75.0	83.3	117	125	8.33
509832	1201046783	15-MAR-2006 09:16	DONE	94	-0.67	percent	100	75.0	83.3	117	125	8.33
511710	1201051085	15-MAR-2006 13:59	DONE	114	1.7	percent	100	75.0	83.3	117	125	8.33
510647	1201048633	16-MAR-2006 23:45	DONE	106	0.72	percent	100	75.0	83.3	117	125	8.33
511630	1201050907	20-MAR-2006 07:42	DONE	90	-1	percent	100	75.0	83.3	117	125	8.33
511996	1201051702	22-MAR-2006 14:23	DONE	119	2.3	percent	100	75.0	83.3	117	125	8.33
511992	1201051688	23-MAR-2006 21:21	DONE	125	3	percent	100	75.0	83.3	117	125	8.33
513416	1201054858	23-MAR-2006 23:50	DONE	111	1.3	percent	100	75.0	83.3	117	125	8.33
513418	1201054866	26-MAR-2006 07:39	DONE	112	1.4	percent	100	75.0	83.3	117	125	8.33
514144	1201056275	29-MAR-2006 19:54	DONE	115	1.8	percent	100	75.0	83.3	117	125	8.33
515260	1201058711	29-MAR-2006 22:27	DONE	102	0.24	percent	100	75.0	83.3	117	125	8.33
515258	1201058703	01-APR-2006 09:23	DONE	105	0.6	percent	100	75.0	83.3	117	125	8.33
515550	1201059424	02-APR-2006 07:36	DONE	100	0	percent	100	75.0	83.3	117	125	8.33
512068	1201051875	05-APR-2006 09:52	DONE	88	-2	percent	100	75.0	83.3	117	125	8.33
512060	1201051843	05-APR-2006 10:05	DONE	99	-0.11	percent	100	75.0	83.3	117	125	8.33
517558	1201063870	05-APR-2006 15:35	DONE	109	1.1	percent	100	75.0	83.3	117	125	8.33
516344	1201061151	06-APR-2006 13:23	DONE	82	-2	percent	100	75.0	83.3	117	125	8.33
517144	1201062901	07-APR-2006 13:44	DONE	82	-2	percent	100	75.0	83.3	117	125	8.33


SPC Graph for Total Uranium KPA in Solids 4/20/2006

Total Uranium BLANK

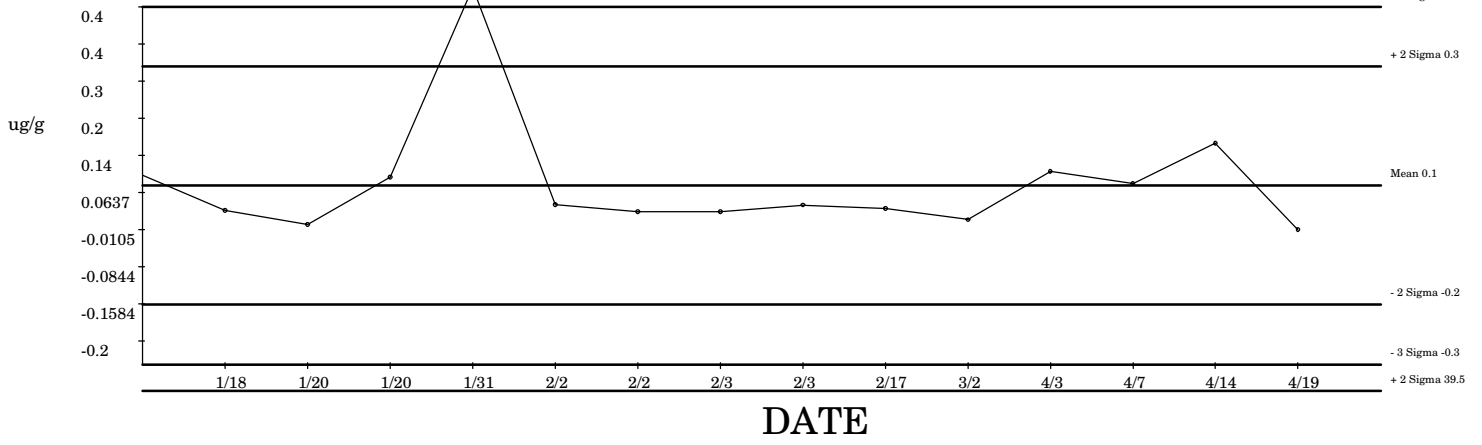


DATE

Total Uranium DUP

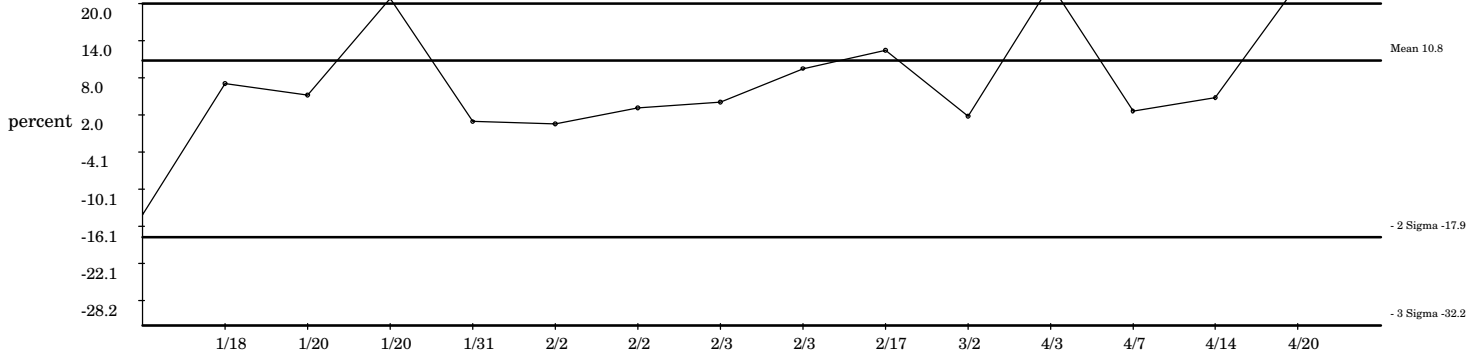

DATE

Total Uranium LCS

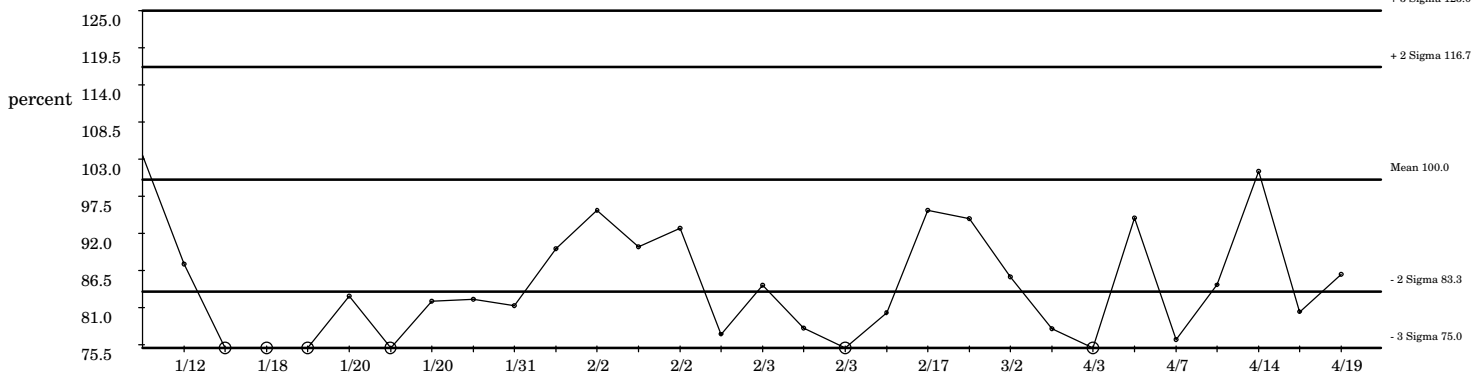

DATE

Total Uranium RER


dec
Data contains 1 point(s)

○ Denotes Outlier

DATE

SPC Graph for Total Uranium KPA in Solids 4/20/2006

Total Uranium SPIKE

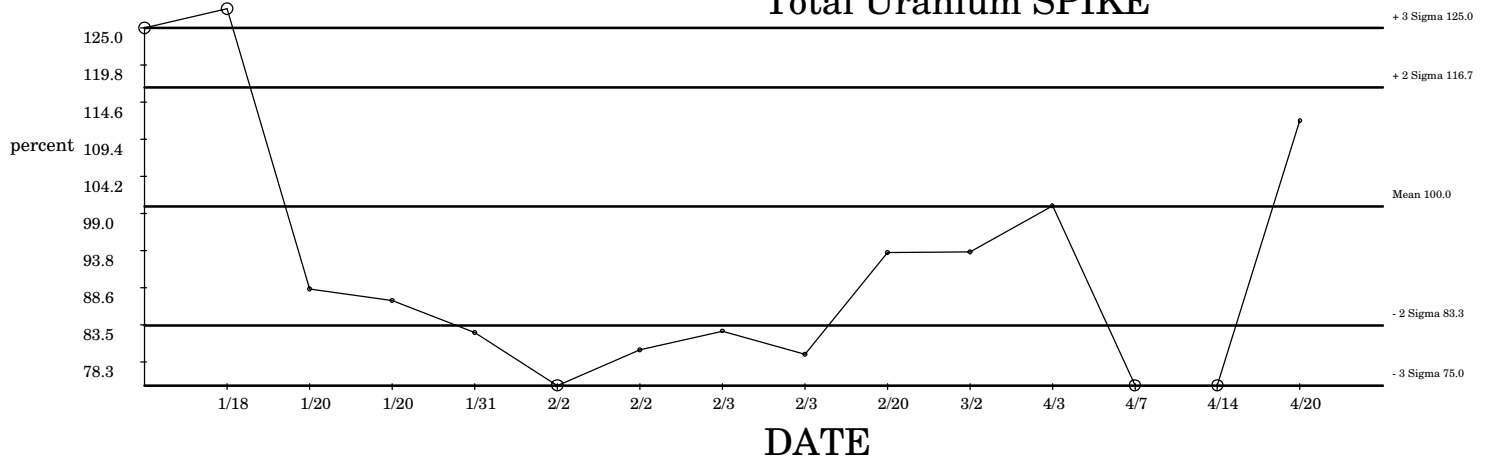

Data used for Total Uranium KPA in Solids 21-APR-2006

Total Uranium BLANK: Limits LCL = -.3 UCL = .4

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
492781	1201007372	12-JAN-2006 13:38	DONE	0.06	-0.17	ug/g	0.08	-0.279	-0.16	0.32	0.43	0.12
494246	1201010694	18-JAN-2006 10:17	DUSE	0.03	-0.42	ug/g	0.08	-0.279	-0.16	0.32	0.43	0.12
493748	1201009625	20-JAN-2006 11:52	DUSE	0	-0.65	ug/g	0.08	-0.279	-0.16	0.32	0.43	0.12
493750	1201009630	20-JAN-2006 12:06	DUSE	0.09	0.14	ug/g	0.08	-0.279	-0.16	0.32	0.43	0.12
496204	1201015077	31-JAN-2006 13:42	DONE	0.47	3.3	ug/g	0.08	-0.279	-0.16	0.32	0.43	0.12
499915	1201023682	02-FEB-2006 13:17	DONE	0.04	-0.32	ug/g	0.08	-0.279	-0.16	0.32	0.43	0.12
495063	1201012509	02-FEB-2006 14:02	DONE	0.03	-0.44	ug/g	0.08	-0.279	-0.16	0.32	0.43	0.12
496854	1201016615	03-FEB-2006 10:55	DONE	0.03	-0.44	ug/g	0.08	-0.279	-0.16	0.32	0.43	0.12
496856	1201016624	03-FEB-2006 14:13	DONE	0.04	-0.33	ug/g	0.08	-0.279	-0.16	0.32	0.43	0.12
503736	1201032423	17-FEB-2006 15:58	DONE	0.03	-0.39	ug/g	0.08	-0.279	-0.16	0.32	0.43	0.12
504168	1201033463	02-MAR-2006 09:57	DONE	0.01	-0.57	ug/g	0.08	-0.279	-0.16	0.32	0.43	0.12
515698	1201059829	03-APR-2006 10:06	DUSE	0.11	0.24	ug/g	0.08	-0.279	-0.16	0.32	0.43	0.12
517556	1201063863	07-APR-2006 13:10	DONE	0.08	0.03	ug/g	0.08	-0.279	-0.16	0.32	0.43	0.12
519916	1201069138	14-APR-2006 10:53	DUSE	0.16	0.71	ug/g	0.08	-0.279	-0.16	0.32	0.43	0.12
521637	1201073174	19-APR-2006 10:37	DONE	-0.01	-0.74	ug/g	0.08	-0.279	-0.16	0.32	0.43	0.12

Total Uranium DUP: Limits LCL = -32.2 UCL = 20

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
492781	1201007373	12-JAN-2006 13:43	DONE	2.05	-0.61	percent	10.8	-32	-18	39.5	20.0	14.3
494246	1201010695	18-JAN-2006 10:22	DUSE	7.05	-0.26	percent	10.8	-32	-18	39.5	20.0	14.3
493748	1201009626	20-JAN-2006 11:57	DUSE	5.2	-0.39	percent	10.8	-32	-18	39.5	20.0	14.3
493750	1201009631	20-JAN-2006 12:09	DUSE	20.9	0.7	percent	10.8	-32	-18	39.5	20.0	14.3
496204	1201015078	31-JAN-2006 12:18	DONE	0.87	-0.69	percent	10.8	-32	-18	39.5	20.0	14.3
499915	1201023683	02-FEB-2006 13:22	DONE	0.52	-0.72	percent	10.8	-32	-18	39.5	20.0	14.3
495063	1201012510	02-FEB-2006 14:07	DONE	3.13	-0.54	percent	10.8	-32	-18	39.5	20.0	14.3
496854	1201016616	03-FEB-2006 10:58	DONE	4.08	-0.47	percent	10.8	-32	-18	39.5	20.0	14.3
496856	1201016625	03-FEB-2006 14:17	DONE	9.49	-0.09	percent	10.8	-32	-18	39.5	20.0	14.3
503736	1201032424	17-FEB-2006 16:03	DONE	12.4	0.11	percent	10.8	-32	-18	39.5	20.0	14.3
504168	1201033464	02-MAR-2006 10:01	DONE	1.78	-0.63	percent	10.8	-32	-18	39.5	20.0	14.3
515698	1201059830	03-APR-2006 10:09	DUSE	43.3	2.3	percent	10.8	-32	-18	39.5	20.0	14.3
517556	1201063864	07-APR-2006 13:14	DONE	2.53	-0.58	percent	10.8	-32	-18	39.5	20.0	14.3
519916	1201069139	14-APR-2006 12:42	DUSE	4.8	-0.42	percent	10.8	-32	-18	39.5	20.0	14.3
521637	1201073175	20-APR-2006 15:13	DONE	43.8	2.3	percent	10.8	-32	-18	39.5	20.0	14.3

Total Uranium LCS: Limits LCL = 75 UCL = 125

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
492781	1201007376	12-JAN-2006 13:52	DONE	96.4	-0.43	percent	100	75.0	83.3	117	125	8.33
492781	1201007375	12-JAN-2006 14:39	DONE	87.4	-2	percent	100	75.0	83.3	117	125	8.33
494246	1201010697	18-JAN-2006 10:28	DUSE	63.8	-4	percent	100	75.0	83.3	117	125	8.33
494246	1201010698	18-JAN-2006 10:30	DUSE	65.6	-4	percent	100	75.0	83.3	117	125	8.33
493748	1201009628	20-JAN-2006 12:01	DUSE	70.8	-3	percent	100	75.0	83.3	117	125	8.33
493748	1201009629	20-JAN-2006 12:05	DUSE	82.6	-2	percent	100	75.0	83.3	117	125	8.33
493750	1201009633	20-JAN-2006 12:17	DUSE	70.1	-4	percent	100	75.0	83.3	117	125	8.33
493750	1201009634	20-JAN-2006 12:19	DUSE	81.9	-2	percent	100	75.0	83.3	117	125	8.33
496204	1201015081	31-JAN-2006 12:31	DONE	82.2	-2	percent	100	75.0	83.3	117	125	8.33
496204	1201015080	31-JAN-2006 13:21	DONE	81.3	-2	percent	100	75.0	83.3	117	125	8.33
499915	1201023685	02-FEB-2006 13:29	DONE	89.8	-1	percent	100	75.0	83.3	117	125	8.33
499915	1201023686	02-FEB-2006 13:31	DONE	95.4	-0.55	percent	100	75.0	83.3	117	125	8.33
495063	1201012512	02-FEB-2006 14:15	DONE	90	-1	percent	100	75.0	83.3	117	125	8.33
495063	1201012513	02-FEB-2006 14:19	DONE	92.7	-0.87	percent	100	75.0	83.3	117	125	8.33
496854	1201016618	03-FEB-2006 11:06	DONE	77	-3	percent	100	75.0	83.3	117	125	8.33
496854	1201016619	03-FEB-2006 11:07	DONE	84.3	-2	percent	100	75.0	83.3	117	125	8.33
496856	1201016627	03-FEB-2006 14:24	DONE	77.9	-3	percent	100	75.0	83.3	117	125	8.33
496856	1201016628	03-FEB-2006 14:26	DONE	74.6	-3	percent	100	75.0	83.3	117	125	8.33
503736	1201032426	17-FEB-2006 16:09	DONE	80.3	-2	percent	100	75.0	83.3	117	125	8.33
503736	1201032427	17-FEB-2006 16:11	DONE	95.4	-0.55	percent	100	75.0	83.3	117	125	8.33
504168	1201033466	02-MAR-2006 10:08	DONE	94.2	-0.7	percent	100	75.0	83.3	117	125	8.33
504168	1201033467	02-MAR-2006 10:12	DONE	85.5	-2	percent	100	75.0	83.3	117	125	8.33
515698	1201059833	03-APR-2006 10:15	DUSE	77.9	-3	percent	100	75.0	83.3	117	125	8.33
515698	1201059832	03-APR-2006 10:20	DUSE	65.5	-4	percent	100	75.0	83.3	117	125	8.33
517556	1201063867	07-APR-2006 13:19	DONE	94.3	-0.69	percent	100	75.0	83.3	117	125	8.33
517556	1201063866	07-APR-2006 13:24	DONE	76.2	-3	percent	100	75.0	83.3	117	125	8.33
519916	1201069141	14-APR-2006 11:04	DUSE	84.4	-2	percent	100	75.0	83.3	117	125	8.33
519916	1201069142	14-APR-2006 11:06	DUSE	101	0.14	percent	100	75.0	83.3	117	125	8.33
521637	1201073177	19-APR-2006 10:46	DONE	80.4	-2	percent	100	75.0	83.3	117	125	8.33
521637	1201073178	19-APR-2006 10:48	DONE	85.9	-2	percent	100	75.0	83.3	117	125	8.33

Total Uranium RER: Limits LCL = 2.1 UCL = 2.1

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
521637	1201073175	20-APR-2006 15:13	DONE	2.11		dec	2.11	2.11	2.11	2.11	2.11	0

Total Uranium SPIKE: Limits LCL = 75 UCL = 125

Batch ID	Samp ID	Run Date	Status	Value	Deviation	Units	Mean	LCL	LWL	UWL	UCL	Stdev
492781	1201007374	12-JAN-2006 13:46	DONE	38.6	-7	percent	100	75.0	83.3	117	125	8.33
494246	1201010696	18-JAN-2006 10:25	DUSE	168	8.2	percent	100	75.0	83.3	117	125	8.33
493748	1201009627	20-JAN-2006 11:58	DUSE	88.5	-1	percent	100	75.0	83.3	117	125	8.33
493750	1201009632	20-JAN-2006 12:13	DUSE	86.9	-2	percent	100	75.0	83.3	117	125	8.33
496204	1201015079	31-JAN-2006 13:18	DONE	82.4	-2	percent	100	75.0	83.3	117	125	8.33
499915	1201023684	02-FEB-2006 13:26	DONE	56	-5	percent	100	75.0	83.3	117	125	8.33
495063	1201012511	02-FEB-2006 14:11	DONE	80	-2	percent	100	75.0	83.3	117	125	8.33
496854	1201016617	03-FEB-2006 11:02	DONE	82.6	-2	percent	100	75.0	83.3	117	125	8.33
496856	1201016626	03-FEB-2006 14:21	DONE	79.3	-2	percent	100	75.0	83.3	117	125	8.33
503736	1201032425	20-FEB-2006 10:29	DONE	93.6	-0.77	percent	100	75.0	83.3	117	125	8.33
504168	1201033465	02-MAR-2006 10:05	DONE	93.7	-0.76	percent	100	75.0	83.3	117	125	8.33
515698	1201059831	03-APR-2006 11:04	DUSE	100	0.02	percent	100	75.0	83.3	117	125	8.33
517556	1201063865	07-APR-2006 13:18	DONE	66.6	-4	percent	100	75.0	83.3	117	125	8.33
519916	1201069140	14-APR-2006 11:00	DUSE	29.5	-8	percent	100	75.0	83.3	117	125	8.33
521637	1201073176	20-APR-2006 15:15	DONE	112	1.4	percent	100	75.0	83.3	117	125	8.33

STANDARDS DATA

CERTIFICATE OF CALIBRATION ALPHA STANDARD SOLUTION

0159

Radionuclide: Th-230
Half Life: $(7.54 \pm 0.03) \times 10^4$ years
Catalog No.: 7230
Source No.: 678-28-1
Customer: GENERAL ENGINEERING LABS
P.O.No.: 2507 RD
Reference Date: 1 Sep 99 12:00 PST.
Contained Radioactivity: Th-230: 9.740 μ Ci (360.4 kBq)

Description of Solution

- a. Mass of solution: 4.89252 grams in 5 mL flame sealed ampoule
- b. Chemical form: Thorium nitrate in 0.1M nitric acid
- c. Carrier content: 10 μ g Th/mL of solution
- d. Density: 1.0016

gram/ml @ 20°C.

Radioimpurities

Am-241: See Technical Data Sheet

Radioactive Daughters

Ra-226: See Technical Data Sheet

Radionuclide Concentration

Th-230: 1.991 μ Ci/gram of solution (73.67 kBq/gram of solution)

Method of Calibration

Weighed aliquots of the solution were assayed using a liquid scintillation counter.

Uncertainty of Measurement

- a. Systematic uncertainty in instrument calibration: $\pm 2.0\%$
- b. Random uncertainty in assay: $\pm 0.8\%$
- c. Random uncertainty in weighing(s): $\pm 0.0\%$
- d. Total uncertainty at the 99% confidence level: $\pm 2.2\%$

NIST Traceability

This calibration is implicitly traceable to the National Institute of Standards and Technology.

Leak Test(s)

See reverse side for Leak Test(s) applied to this source.

Notes

1. IPL participates in an NIST measurement assurance program to establish and maintain implicit traceability for a number of nuclides, based on the blind assay (and later NIST certification) of Standard Reference Materials. (As in NRC Regulatory Guide 4.15)
2. Nuclear data were taken from Table of Radioactive Isotopes (1986), edited by Virginia Shirley.

Daniel James Van Dalsen
QUALITY CONTROL

26-Aug-99
Date Signed



ISOTOPE PRODUCTS LABORATORIES

1800 N. KEYSTONE STREET
BURBANK, CALIFORNIA 91504

818-843-7000 FAX 818-843-6168

0159



Th-230 TECHNICAL DATA

The Th-230 used to prepare your order was taken from Isotope Products Laboratories Lot #6481 and had the following composition as of December 15, 1994.

<u>NUCLIDE</u>	<u>ATOM%</u>	<u>ACTIVITY%</u>
Th-229	<0.001	<1.23 x 10 ⁻²
Th-230	83.71	99.79
Th-232	16.29	1.08 x 10 ⁻⁴
Ra-226 (daughter Th-230)	----	0.15
Am-241	----	0.05

Isotopic composition provided by Oak Ridge National Laboratory.

No other alpha emitting nuclides were detected.

If you have any questions, please contact Technical Service.

Corporate and
Sales Offices
1800 N. Keystone Street
Irvine, California
91504
818-833-7000
818-833-6163



Standard Traceability Log Rad

Source Material Info		A Solution Material Info	
Parent Code:	0159	Isotope:	Thorium-230
Prepared By:	Joe Davis	Prepared By:	Joe Davis
Carrier Conc:	0.1M HNO ₃	Prep Date:	09/21/1999
Reference Date:	09/01/1999	Verification Date:	06/19/2004
Ampoule Mass (g):	4.89252 g	Expiration Date:	06/19/2005
Uncertainty:	+/- 2.2 %	Primary Code:	0159-A
LogBook No:	RC S 023 102	Dilution(mL):	100 mL
		Mass of Parent(g):	4.7484 g
		Density(g/mL):	0.9992

Calculations Converting parent activity to dpm/mL | dpm/g

$(\text{Mass of parent(g)}) * (\text{Parm Activity (uCi/g)}) * (\text{conversion dpm to uCi}) / (\text{Dilution Vol}) = \text{Parent Activity (dpm/mL)}$
$(\text{Mass of parent(g)}) * (\text{Parm Activity (uCi/g)}) * (\text{conversion dpm to uCi}) / \text{Density (g/mL)} / (\text{Dilution Vol}) = \text{Parent Activity (dpm/g)}$
$(4.7484 \text{ g}) * (1.991 \text{ uCi/g}) * (2220000 \text{ dpm/uCi}) / (100 \text{ mL}) = 209880.2297 \text{ dpm/mL}$
$(4.7484 \text{ g}) * (1.991 \text{ uCi/g}) * (2220000 \text{ dpm/uCi}) / (0.9992 \text{ g/mL}) / (100 \text{ mL}) = 210051.8397 \text{ dpm/g}$

Secondary Standards

Prep Date	Preparer	Mass Primary	Dilution (mL)	Code	Conc dpm/mL	Verification Date	Expiration Date
01/29/2001	Angela Albee	.0992	100	0159-H	208.37 dpm/mL	01/29/2001	01/29/2002
02/28/2001	Angela Albee	1.0451	1000	0159-I-102	219.525 dpm/mL	03/06/2002	03/06/2003
02/28/2001	Angela Albee	1.0451	1000	0159-I-202	219.525 dpm/mL	03/12/2002	03/12/2003
09/21/1999	Joe Davis	.1172	100	0159-B	246.18 dpm/mL	09/21/1999	09/21/2000
09/23/1999	Joe Davis	.1016	100	0159-C	213.41 dpm/mL	09/23/1999	09/23/2000
01/10/2000	Joe Davis	.1008	100	0159-D	211.56 dpm/mL	01/10/2000	01/10/2001
02/16/2000	Richard Kinney	.2422	500	0159-E	101.75 dpm/mL	02/16/2000	02/16/2001
03/20/2000	Joe Davis	.0998	100	0159-F	209.63 dpm/mL	03/20/2000	03/20/2001
07/28/2000	Robert Timm	1.0046	1000	0159-G	211.02 dpm/mL	07/28/2000	07/28/2001
05/10/2001	Angela Albee	.0987	1000	0159-J	210.1569 dpm/mL	05/10/2001	05/10/2002
08/31/2001	Lonnie Morris	.0416	100	0159-K	87.31 dpm/mL	09/23/2002	09/23/2003
06/07/2002	Angela Albee	1.0002	1000	0159-L	207.278 dpm/mL	06/07/2002	06/07/2003
01/16/2003	Angela Albee	4.5144	1000	0159-M	947.483 dpm/mL	01/16/2003	01/16/2004
02/27/2003	Angela Albee	1.1079	1000	0159-N	232.526 dpm/mL	02/27/2004	02/27/2005
06/23/2004	Amanda Fehr	1.14	1000	0159-O	239.459 dpm/mL	07/03/2005	07/03/2006

General Engineering Laboratories, LLC
Version 1.0 9/18/2000

Verification for Th-230 Standard 0159-O

A. Fehr
7/3/2005

Isotope	Detector CPM	BKG CPM	NET CPM	Detector Eff	Standard Amt Used (mL)	Source DPM/mL
0159-N N1	258.0000	23.3000	234.7000	0.9696	1.0000	242.0585809
0159-N N2	259.3000	23.3000	236.0000	0.9696	1.0000	243.3993399
0159-N N3	255.4000	23.3000	232.1000	0.9696	1.0000	239.3770627

Mean Value (Counting) =	241.6116612	dpm/mL	100.903182	% of known
Stdev =	2.048043318	dpm/mL	0.00847659	
Certificate Value =	239.449	dpm/mL		
Lower Limit =	237.5155745	dpm/mL		
Upper Limit =	245.7077478	dpm/mL		
Rule 1 Pass/Fail	Pass	Pass	Pass	
Two sigma =	4.096086636			
10 % of Mean =	24.16116612			
Rule 2 (Pass/Fail)	Pass			

Verification Rules

Rule 1 = The certificate value (NOT including any uncertainty) shall lie within the 95% confidence interval determined from the mean and two sigma standard deviation of the three measurements

Rule 2 = The two sigma value used for the 95% confidence interval shall not exceed 10% of the mean value of the three verification measurements.

The analyst prepared three standard verification sources for Th-230 source 0159-O by transferring 1.0 mL portions of the standard to glass liquid scintillation vials. Ten mL of Ready Gel liquid scintillation cocktail was added to each vial and the vials were shaken to mix. A Blank vial was prepared in a similar fashion using 1 mL of DI water and 10 mL of Ready Gel cocktail. The standard verification vials and Background source were dark adapted for two hours and counted on LSC Yellow (Wallac) using Protocol 26 for alpha source standard verification. The alpha efficiency calibration which was used for verification calculations was performed using NIST source 0556-A (Th-230). Calibration data is recorded in this logbook under Th-230 0556-A. Each verification source calculation was performed as follows:

$$\text{Source dpm/g} = (A - B)/(C)(D)$$

where:

- A = Ver. source cpm,
- B = BKG cpm,
- C = System efficiency, (cpm/dpm), and
- D = mass used for standard verification.

Reference RAD SOP M-001

Amanda L. Fehr 7/3/05

Angela A. Johnson
7/5/05

CERTIFICATE OF CALIBRATION

Standard Radionuclide Source

61762-278

Ac-227 5 mL Liquid in Flame Sealed Vial

This standard radionuclide source was prepared gravimetrically from a calibrated master solution. The master solution was calibrated using a germanium gamma spectrometer system.

Radionuclide purity and calibration were checked by alpha spectroscopy. The nuclear decay rate and assay date for this source are given below.

Analytics maintains traceability to the National Institute of Standards and Technology through participation in a Measurements Assurance Program as described in USNRC Reg. Guide 4.15, Revision 1, February 1979.

ISOTOPE:	Ac-227
ACTIVITY (dps):	2.085 E5
HALF-LIFE:	21.77 years
CALIBRATION DATE:	June 8, 2001 12:00 EST
TOTAL UNCERTAINTY*:	5.0%
SYSTEMATIC:	2.0%
RANDOM:	3.0%


*99% Confidence Level

Impurities: γ -impurities (other than decay products) <0.1%
 α -impurities <0.3%


5.3136 grams 2M HNO₃ solution, carrier free.

P O NUMBER 2533RD, Item 2

SOURCE PREPARED BY:

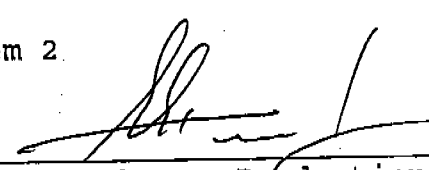
E. A. Taskaev, Production Manager

Q A APPROVED:


6/26/01



Standard Traceability Log Rad

Source Material Info		A Solution Material Info	
Parent Code:	0387	Isotope:	Actinium-227
Prepared By:	Angela Johnson	Prepared By:	Angela Johnson
Carrier Conc:	2 M HNO3	Prep Date:	07/17/2001
Reference Date:	06/08/2001	Verification Date:	07/01/2002
Ampoule Mass (g):	5.3136 g	Expiration Date:	07/01/2003
Uncertainty:	+/- 5 %	Primary Code:	0387-A
LogBook No:	RC S 034	Dilution(mL):	100 mL
		Mass of Parent(g):	4.7794 g
		Density(g/mL):	1.0370

Calculations Converting parent activity to dpm/mL|dpm/g

$$(\text{Mass of parent(g)}) * (\text{Parm Activity (dps)}) * (\text{conversion dpm to dps}) / (\text{Ampoule Mass(g)} * (\text{Dilution Vol})) = \text{Parent Activity (dpm/mL)}$$

$$(\text{Mass of parent(g)}) * (\text{Parm Activity (dps)}) * (\text{conversion dpm to dps}) / \text{Density} / (\text{Ampoule Mass (g)} * (\text{Dilution Vol})) = \text{Parent Activity (dpm/g)}$$

$$(4.7794 \text{ g}) * (208500 \text{ dps}) * (59.9 \text{ dpm/dps}) / (5.3136 \text{ g} * 100 \text{ mL}) = 112335.5983 \text{ dpm/mL}$$

$$(4.7794 \text{ g}) * (208500 \text{ dps}) * (59.9 \text{ dpm/dps}) / (1.0370 \text{ g/mL}) / (5.3136 \text{ g} * 100 \text{ mL}) = 108330.3019 \text{ dpm/g}$$

Secondary Standards

Prep Date	Preparer	Mass Primary	Dilution (mL)	Code	Conc dpm/mL	Verification Date	Expiration Date
07/17/2001	Lonnie Morris	.4684	1000	0387-B-102	50.8266 dpm/mL	07/11/2005	07/11/2006
07/17/2001	Lonnie Morris	.4684	1000	0387-B-202	50.827 dpm/mL	07/11/2004	07/11/2005

General Engineering Laboratories, LLC
Version 1.0 9/18/2000

Verification for Ac-227 Standard 0387-B

A. Fehr 7/13/2005	Isotope	Value	Uncertainty
	0387-B #1	193.600	38.1000
	0387-B #2	181.200	36.2000
	0387-B #3	192.900	52.4000

Mean Value (Counting) = 189.233 0.9416936
 Stdev = 6.965869173

Target = 200.95
 Lower Limit = 175.301595
 Upper Limit = 203.1650717
 Rule 1 Pass/Fail **Pass Pass Pass**
 Two sigma = 13.93173835
 10 % of Mean = 18.92333333
 Rule 2 (Pass/Fail) **Pass**

The analyst prepared three standard verification sources for standard 0387-B using 0.1 mL for each source. Each standard was combined with 0.1 mL of Th-230 standard 0159-K and 50 micrograms of cerium carrier in a disposable centrifuge tube. Each standard was diluted to 20 mL with 0.1 M HCl. Three mL of 48% HF was added to precipitate cerium (and Thorium) fluoride. After 30 minutes, each sample was filtered following routine procedures for alpha spectroscopy source preparation. Each source was counted using routine alpha spec procedures. DPM values for Ac-227 were calculated by comparison to Th-230 certified values.

Amanda L. Fehr
 7/13/05

CERTIFICATE OF CALIBRATION
Standard Radionuclide Source

68509-278

U-232 5 mL Liquid in Flame Sealed Vial

This standard radionuclide source was prepared using an aliquot measured gravimetrically from a master radionuclide solution standard. The master radionuclide solution standard was calibrated by the Department Des Applications Et De La Metrologie Des Rayonnements Ionisants (DAMRI), Paris, France, as Number 23236.

Radionuclide purity and calibration were checked using a germanium gamma spectrometer system. The nuclear decay rate and assay date for this source are given below.

ANALYTICS maintains traceability to the National Institute of Standards and Technology through Measurements Assurance Programs as described in USNRC Reg. Guide 4.15, Revision 1.

ISOTOPE:	U-232
ACTIVITY (dps):	3.779 E3
CALIBRATION DATE:	June 18, 2004 12:00 EST
HALF-LIFE:	68.9 years
RELATIVE EXPANDED: UNCERTAINTY (k=2):	3.3%

Impurities: Am-241 <0.15%
U-233 <0.3%

5.20343 grams 1M HNO₃ solution.

P O NUMBER 3243 RD, Item 1

SOURCE PREPARED BY:

M. Dimitrova
M. Dimitrova, Radiochemist

Q A APPROVED:

ACU/6/23/04

RECEIVED
11/26/04



Standard Traceability Log Rad

Source Material Info		A Solution Material Info	
Parent Code:	0688	Isotope:	Uranium-232
Prepared By:	Amanda Fehr	Prepared By:	Amanda Fehr
Carrier Conc:	1M HNO3	Prep Date:	06/25/2004
Reference Date:	06/18/2004	Verification Date:	01/12/2006
Ampoule Mass (g):	5.20343 g	Expiration Date:	01/12/2007
Uncertainty:	+/- 3.3 %	Primary Code:	0688-A
LogBook No:	RC-S-037-087	Dilution(mL):	100 mL
		Mass of Parent(g):	4.9894 g
		Density(g/mL):	1.0276

Calculations Converting parent activity to dpm/mL|dpm/g

$$(\text{Mass of parent(g)}) * (\text{Parm Activity (dps)}) * (\text{conversion dpm to dps}) / (\text{Ampoule Mass(g)} * (\text{Dilution Vol})) = \text{Parent Activity (dpm/mL)}$$

$$(\text{Mass of parent(g)}) * (\text{Parm Activity (dps)}) * (\text{conversion dpm to dps}) / \text{Density} / (\text{Ampoule Mass (g)} * (\text{Dilution Vol})) = \text{Parent Activity (dpm/g)}$$

$$(4.9894 \text{ g}) * (3779 \text{ dps}) * (59.9 \text{ dpm/dps}) / (5.20343 \text{ g} * 100 \text{ mL}) = 2170.5126 \text{ dpm/mL}$$

$$(4.9894 \text{ g}) * (3779 \text{ dps}) * (59.9 \text{ dpm/dps}) / (1.0276 \text{ g/mL}) / (5.20343 \text{ g} * 100 \text{ mL}) = 2112.2178 \text{ dpm/g}$$

Secondary Standards

Prep Date	Preparer	Mass Primary	Dilution (mL)	Code	Conc dpm/mL	Verification Date	Expiration Date
06/18/2004	Brenda Burke	2.203	250	0688-B	18.6439 g/mL	06/28/2005	06/28/2006
07/06/2004	Tim Chandler	2.2243	250	0688-C	18.8242 dpm/mL	08/14/2004	08/14/2005
07/06/2004	Amanda Fehr	26.03	1000	0688-D	55.0728 dpm/mL	07/06/2004	07/06/2005
04/19/2005	Amanda Fehr	26.01	1000	0688-E	55.0305 dpm/mL	05/04/2005	05/04/2006
05/27/2005	Brenda Burke	.612	250	0688-F	5.17934 dpm/mL	05/31/2005	05/31/2006
06/23/2005	Brenda Burke	2.227	250	0688-G	18.847 dpm/mL	06/28/2005	06/28/2006
01/06/2006	Mary Avins	26.01	1000	0688-H	55.0305 dpm/mL	01/12/2006	01/12/2007

General Engineering Laboratories, LLC
Version 1.0 9/18/2000

Verification for Uranium-232 Standard 0688-H

Analyst: M Avins	Isotope	Value	Uncertainty	
Date: 1/12/06	0688-H N1	2.46	pCi/L 0.292	pCi/L
	0688-H N2	2.49	pCi/L 0.383	pCi/L
	0688-H N3	2.48	pCi/L 0.315	pCi/L
Mean Value (Counting) =	2.477	pCi/L	0.9992767	% of known
Stdev =	0.015275252	pCi/L		
Target =	2.48	pCi/L		
Lower Limit =	2.446116162	pCi/L		
Upper Limit =	2.507217171	pCi/L		
Rule 1 Pass/Fail	Pass	Pass	Pass	
Two sigma =	0.030550505			
10 % of Mean =	0.247666667			
Rule 2 (Pass/Fail)	Pass			

The analyst prepared three standard verification sources for standard **0688-H** using 0.1 mL for each source. Each standard was combined with 0.1 mL of **U-238** standard **0858-B** and 50 micrograms of Nd carrier in a disposable centrifuge tube. Each standard was diluted to 4 mL with 2 M HCl, and 2 mL of DI water. One mL of TiCl₃ was added. Two mL of 48% HF was added to precipitate Nd (and **Uranium**) fluoride. After 30 minutes, each sample was filtered following routine procedures for alpha spectroscopy source preparation. Each source was counted using routine alpha spec procedures. DPM values for **U-232** were calculated by comparison to **U-238** certified values.

Reference SOP RAD M-001

Mary L. Avins
1/12/06

Amanda L. Loh
1/24/06



National Institute of Standards & Technology

Certificate

Standard Reference Material 4321C Natural Uranium Radioactivity Standard

This Standard Reference Material (SRM) consists of radioactive natural uranium nitrate and nitric acid dissolved in 5 mL of distilled water. The solution is contained in a flame-sealed NIST borosilicate-glass ampoule. The SRM is intended for the calibration of alpha-particle counting instruments and for the monitoring of radiochemical procedures.

Radiological Hazard

The SRM ampoule contains uranium-238, uranium-235, and uranium-234 with a total activity of approximately 2600 Bq. Uranium decays by alpha-particle emission. The progeny of uranium-238, uranium-235, and uranium-234 have a total activity of approximately 2600 Bq and decay by alpha- and beta-particle emission. None of the alpha or beta particles escape from the SRM ampoule. During the decay process X-rays and gamma rays with energies from 11 keV to 2.0 MeV are also emitted. Most of these photons escape from the SRM ampoule but their intensities are so small that they do not represent a radiation hazard. Approximate unshielded dose rates at several distances (as of the reference time) are given in note [a]*. The SRM should be used only by persons qualified to handle radioactive material.

Chemical Hazard

The SRM ampoule contains nitric acid (HNO_3) with a concentration of 1 mole per liter of water. The solution is corrosive and represents a health hazard if it comes in contact with eyes or skin. If the ampoule is to be opened to transfer the solution, the recommended procedure is given on page 2. The ampoule should be opened only by persons qualified to handle both radioactive material and strong acid solution.

Storage and Handling

The SRM should be stored and used at a temperature between 5 and 65 °C. The solution in an unopened ampoule should remain stable and homogeneous until at least August 2007.

The ampoule (or any subsequent container) should always be clearly marked as containing radioactive material. If the ampoule is transported it should be packed, marked, labeled, and shipped in accordance with the applicable national, international, and carrier regulations. The solution in the ampoule is a dangerous good (hazardous material) both because of the radioactivity and because of the strong acid.

Preparation

This Standard Reference Material was prepared in the Physics Laboratory, Ionizing Radiation Division, Radioactivity Group, J.M.R. Hutchinson, Group Leader. The overall technical direction and physical measurements leading to certification were provided by L.L. Lucas of the Radioactivity Group.

The support aspects involved in the preparation, certification, and issuance of this SRM were coordinated through the Standard Reference Materials Program by N.M. Trahey.

Gaithersburg, Maryland 20899
November 1997

Thomas E. Gills, Chief
Standard Reference Materials Program

Recommended Procedure for Opening the SRM Ampoule

- 1) If the SRM solution is to be diluted, it is recommended that the diluting solution have a composition comparable to that of the SRM solution.
- 2) Wear eye protection, gloves, and protective clothing and work over a tray with absorbent paper in it. Work in a fume hood. In addition to the radioactive material, the solution contains strong acid and is corrosive.
- 3) Shake the ampoule to wet all of the inside surface of the ampoule. Return the ampoule to the upright position.
- 4) Check that all of the liquid has drained out of the neck of the ampoule. If necessary, gently tap the neck to speed the process.
- 5) Holding the ampoule upright, score the narrowest part of the neck with a scribe or diamond pencil.
- 6) Lightly wet the scored line. This reduces the crack propagation velocity and makes for a cleaner break.
- 7) Hold the ampoule upright with a paper towel, a wiper, or a support jig. Position the scored line away from you. Using a paper towel or wiper to avoid contamination, snap off the top of the ampoule by pressing the narrowest part of the neck away from you while pulling the tip of the ampoule towards you.
- 8) Transfer the solution from the ampoule using a pycnometer or a pipet with dispenser handle. **NEVER PIPETTE BY MOUTH.**
- 9) Seal any unused SRM solution in a flame-sealed glass ampoule, if possible, to minimize the evaporation loss.

See also reference [4]*.

PROPERTIES OF SRM 4321C
(Certified values are shown in bold type)

Source identification number	NIST SRM 4321C		
Physical Properties:			
Source description	Liquid in flame-sealed NIST borosilicate-glass ampoule		
Ampoule specifications	Body outside diameter	(16.5 ± 0.5) mm	
	Wall Thickness	(0.60 ± 0.04) mm	
	Barium content	Less than 2.5%	
	Lead-oxide content	Less than 0.02%	
	Other heavy elements	Trace quantities	
Solution density	(1.053 ± 0.001) g·mL ⁻¹ at 21.4 °C [b]*		
Solution mass	(5.258 ± 0.002) g [b]		
Chemical Properties:			
Solution composition	Chemical Formula	Concentration (mol·L ⁻¹)	Mass Fraction (g·g ⁻¹)
	H ₂ O	53	0.91
	HNO ₃	1.0	0.06
	UO ₂ (NO ₃) ₂	0.09	0.03
Radiological Properties:			
Radionuclide	Natural Uranium (Mixture of U-238, U-235, and U-234)		
Reference time	1200 EST, 1 August 1997		
Massic activity of the solution [c]	U-238: 242.0 Bq·g ⁻¹ U-235: 11.14 Bq·g ⁻¹ U-234: 233.1 Bq·g ⁻¹		
Relative expanded uncertainty (k=2)	U-238: 0.60% [d] [e] U-235: 0.62% [d] [e] U-234: 0.98% [d] [e]		
Mass fraction of uranium	(0.01960 ± 0.00010) g·g ⁻¹ [b]		
Photon-emitting impurities	None detected [f]		
Half lives used	Uranium-238: (4.468 ± 0.003) × 10 ⁹ a [g] Uranium-235: (7.038 ± 0.005) × 10 ⁸ a [g] Uranium-234: (2.455 ± 0.006) × 10 ⁵ a [g]		
Measuring instruments	Mass spectrometer, silicon surface-barrier detector, and 4π(α+β) liquid-scintillation counting systems.		

EVALUATION OF THE UNCERTAINTY OF THE MASSIC ACTIVITY [d]*

Input Quantity x_i , the source of uncertainty (and individual uncertainty components where appropriate)	Method Used To Evaluate $u(x_i)$, the standard uncertainty of x_i (A) denotes evaluation by statistical methods (B) denotes evaluation by other methods	Relative Uncertainty Of Input Quantity, $u(x_i)/x_i$, (%) [h]	Relative Sensitivity Factor, $ \partial y/\partial x_i \cdot$ (x_i/y) [i]	Relative Uncertainty Of Output Quantity, $u_i(y)/y$, (%) [j]
Isotopic uranium atom fraction in SRM 960	Standard deviation of the mean for repeated mass-spectrometric measurements (A)	U-238: 0.001	1.0	0.001
		U-235: 0.07	1.0	0.07
		U-234: 0.31	1.0	0.31
Half life	Standard uncertainty of the half life (A)	U-238: 0.07	1.0	0.07
		U-235: 0.07	1.0	0.07
		U-234: 0.25	1.0	0.25
Uranium mass fraction in SRM 960	Certificate value (B)	0.003	1.0	0.003
Quantitative dissolution	Estimated (B)	0.25	1.0	0.25
Gravimetric measurements	Estimated (B)	0.10	1.0	0.10
Photon-emitting impurities	Limit of detection (B) [k]	100.	0.001	0.10
Relative Combined Standard Uncertainty of the Output Quantity, $u_c(y)/y$, (%)			U-238:	0.30
			U-235:	0.31
			U-234:	0.49
Coverage Factor, k				<u>x 2</u>
Relative Expanded Uncertainty of the Output Quantity, U/y , (%)			U-238:	0.60
			U-235:	0.62
			U-234:	0.98

NOTES

- [a] The Sievert is the SI unit for dose equivalent. See reference [1]. One μSv is equal to 0.1 mrem.
 Distance from Ampoule (cm): 1 30 100
 Approximate Dose Rate ($\mu\text{Sv/h}$): <0.1
- [b] The stated uncertainty is two times the standard uncertainty.
- [c] **Massic activity** is the preferred name for the quantity activity divided by the total mass of the sample. See reference [1].
- [d] The reported value, y , of massic activity (activity per unit mass) at the reference time was not measured directly but was derived from measurements and calculations of other quantities. This can be expressed as $y = f(x_1, x_2, x_3, \dots, x_n)$, where f is a mathematical function derived from the assumed model of the measurement process.
- The value, x_i , used for each input quantity i has a **standard uncertainty**, $u(x_i)$, that generates a corresponding uncertainty in y , $u_i(y) \equiv |\partial y / \partial x_i| \cdot u(x_i)$, called a **component of combined standard uncertainty** of y .
- The **combined standard uncertainty** of y , $u_c(y)$, is the positive square root of the sum of the squares of the components of combined standard uncertainty.
- The combined standard uncertainty is multiplied by a coverage factor of $k = 2$ to obtain U , the **expanded uncertainty** of y .
- Since it can be assumed that the possible estimated values of the massic activity are approximately normally distributed with approximate standard deviation $u_c(y)$, the unknown value of the massic activity is believed to lie in the interval $y \pm U$ with a level of confidence of approximately 95 percent.
- For further information on the expression of uncertainties, see references [2] and [3].
- [e] The value of each standard uncertainty component, and hence the value of the expanded uncertainty itself, is a best estimate based upon all available information, but is only approximately known. That is to say, the "uncertainty of the uncertainty" is large and not well known. This is true for uncertainties evaluated by statistical methods (e.g., the relative standard deviation of the standard deviation of the mean for the massic count rate is approximately 50%) and for uncertainties evaluated by other methods (which could easily be over estimated or under estimated by substantial amounts). The unknown value of the expanded uncertainty is believed to lie in the interval $U/2$ to $2U$ (i.e., within a factor of 2 of the estimated value).
- [f] Estimated limits of detection for photon-emitting impurities are:
 $1.4 \gamma \cdot \text{s}^{-1} \cdot \text{g}^{-1}$ for energies between 8 and 59 keV,
 $1.1 \gamma \cdot \text{s}^{-1} \cdot \text{g}^{-1}$ for energies between 67 and 88 keV,
 $0.5 \gamma \cdot \text{s}^{-1} \cdot \text{g}^{-1}$ for energies between 102 and 197 keV,
 $0.3 \gamma \cdot \text{s}^{-1} \cdot \text{g}^{-1}$ for energies between 205 and 762 keV,
 $0.2 \gamma \cdot \text{s}^{-1} \cdot \text{g}^{-1}$ for energies between 770 and 996 keV, and
 $0.1 \gamma \cdot \text{s}^{-1} \cdot \text{g}^{-1}$ for energies between 1006 and 1900 keV,
 provided that the photons are separated in energy by 4 keV or more from photons emitted in the decay of uranium-238, uranium-235, uranium-234, or their progeny.
- [g] The stated uncertainty is the standard uncertainty. See reference [5].

- [h] Relative standard uncertainty of the input quantity x_i .
- [i] The relative change in the output quantity y divided by the relative change in the input quantity x_i . If $|\partial y/\partial x_i| \cdot (x_i/y) = 1.0$, then a 1% change in x_i results in a 1% change in y . If $|\partial y/\partial x_i| \cdot (x_i/y) = 0.05$, then a 1% change in x_i results in a 0.05% change in y .
- [j] Relative component of combined standard uncertainty of output quantity y , rounded to two significant figures or less. The relative component of combined standard uncertainty of y is given by $u_i(y)/y \equiv |\partial y/\partial x_i| \cdot u(x_i)/y = |\partial y/\partial x_i| \cdot (x_i/y) \cdot u(x_i)/x_i$. The numerical values of $u(x_i)/x_i$, $|\partial y/\partial x_i| \cdot (x_i/y)$, and $u_i(y)/y$, all dimensionless quantities, are listed in columns 3, 4, and 5, respectively. Thus, the value in column 5 is equal to the value in column 4 multiplied by the value in column 3. The input quantities are independent, or very nearly so. Hence the covariances are zero or negligible.
- [k] The standard uncertainty for each undetected impurity that might reasonably be expected to be present is estimated to be equal to the estimated limit of detection for that impurity, i.e. $u(x_i)/x_i = 100\%$. $|\partial y/\partial x_i| \cdot (x_i/y) = \{(\text{response per Bq of impurity})/(\text{response per Bq of U-238})\} \cdot \{(\text{Bq of impurity})/(\text{Bq of U-238})\}$. Thus $u_i(y)/y$ is the relative change in y if the impurity were present with a massic activity equal to the estimated limit of detection.

REFERENCES

- [1] International Organization for Standardization (ISO), *ISO Standards Handbook - Quantities and Units*, 1993. Available from the American National Standards Institute, 11 West 42nd Street, New York, NY 10036, U.S.A. 1-212-642-4900.
- [2] International Organization for Standardization (ISO), *Guide to the Expression of Uncertainty in Measurement*, 1993. Available from the American National Standards Institute, 11 West 42nd Street, New York, NY 10036, U.S.A. 1-212-642-4900. (Listed under ISO miscellaneous publications as "ISO Guide to the Expression 1993".)
- [3] B. N. Taylor and C. E. Kuyatt, *Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Results*, NIST Technical Note 1297, 1994. Available from the Superintendent of Documents, U.S. Government Printing Office, Washington, DC 20407, U.S.A.
- [4] National Council on Radiation Protection and Measurements Report No. 58, *A Handbook of Radioactivity Measurements Procedures*, Second Edition, 1985. Available from the National Council on Radiation Protection and Measurements, 7910 Woodmont Avenue, Bethesda, MD 20814 U.S.A.
- [5] Evaluated Nuclear Structure Data File (ENSDF), August 1997.



Standard Traceability Log Rad

Source Material Info		A Solution Material Info	
Parent Code:	0858	Isotope:	Uranium-238
Prepared By:	Mary Avins	Prepared By:	Mary Avins
Carrier Conc:	HNO3	Prep Date:	11/21/2005
Reference Date:	08/01/1997	Verification Date:	11/21/2005
Ampoule Mass (g):	5.258 g	Expiration Date:	11/21/2006
Uncertainty:	+/- .6 %	Primary Code:	0858-A
LogBook No:	RC-S-041-034	Dilution(mL):	100 mL
		Mass of Parent(g):	4.972 g
		Density(g/mL):	1.0155

Calculations Converting parent activity to dpm/mL|dpm/g

$(\text{Mass of parent(g)}) * (\text{Parm Activity (Bq/g)}) * (\text{conversion dpm to Bq}) / (\text{Dilution Vol}) = \text{Parent Activity (dpm/mL)}$
$(\text{Mass of parent(g)}) * (\text{Parm Activity (Bq/g)}) * (\text{conversion dpm to Bq}) / \text{Density (g/mL)} / (\text{Dilution Vol}) = \text{Parent Activity (dpm/g)}$
$(4.972 \text{ g}) * (242 \text{ Bq/g}) * (60 \text{ dpm/Bq}) / (100 \text{ mL}) = 721.9344 \text{ dpm/mL}$
$(4.972 \text{ g}) * (242 \text{ Bq/g}) * (60 \text{ dpm/Bq}) / (1.0155 \text{ g/mL}) / (100 \text{ mL}) = 710.9460 \text{ dpm/g}$

Secondary Standards

Prep Date	Preparer	Mass Primary	Dilution (mL)	Code	Conc dpm/mL	Verification Date	Expiration Date
11/21/2005	Mary Avins	8.2104	100	0858-B	58.3715 dpm/mL	11/21/2005	11/21/2006

General Engineering Laboratories, LLC
Version 1.0 9/18/2000

CERTIFICATE OF CALIBRATION
Standard Radionuclide Source

70361-278

5 mL Liquid in Flame Sealed Vial

This standard radionuclide source was prepared using aliquots measured gravimetrically from master radionuclide solution sources. The Am-241 was calibrated by 4 pi alpha liquid scintillation counting. All other radionuclides were calibrated using a germanium gamma spectrometer system. Calibration and purity were checked using a germanium gamma spectrometer system. At the time of calibration no interfering gamma-ray emitting impurities were detected. The gamma-ray emission rates for the most intense gamma-ray lines are given. Analytics maintains traceability to the National Institute of Standards and Technology through a Measurements Assurance Program as described in USNRC Regulatory Guide 4.15, Rev. 1, February, 1979.

Calibration date: April 1, 2005 12:00 EST


ISOTOPE	GAMMA-RAY ENERGY	HALF-LIFE	GAMMA-RAYS PER SECOND	TOTAL UNCERTAINTY %
Am-241	59.5	432 Y	3372	4.5
Cd-109	88	462.6 d	4698	3.3
Co-57	122	271.79 d	2450	3.0
Ce-139	166	137.6 d	3496	2.8
Hg-203	279	46.61 d	7565	2.7
Sn-113	392	115.1 d	4711	2.6
Cs-137	662	30.07 Y	3109	3.0
Y-88	898	106.6 d	12320	2.6
Co-60	1173	5.2714 Y	5769	2.7
Co-60	1332	5.2714 Y	5830	2.6
Y-88	1836	106.6 d	12860	2.6

5.32720 grams 4M HCl solution.
P O NUMBER 2704RD, Item 1

SOURCE PREPARED BY: M. Taskaeva
M. Taskaeva, Radiochemist

Q A APPROVED: [Signature] 04-11-2005

This standard will expire one year after the calibration date.



U.S. DEPARTMENT OF COMMERCE
National Institute of Standards & Technology
Gaithersburg, MD 20899

Certificate of Participation

Analytics, Incorporated
Atlanta, Georgia

is a participant for the period January 1, 2005, through December 31, 2005, in a radioactivity measurements assurance program conducted by the National Institute of Standards and Technology, in cooperation with the Nuclear Energy Institute. Continued participation is evidenced by dated Reports of Traceability issued for particular radionuclides, which indicate the deviation of the participant's reported value from that measured by the National Institute of Standards and Technology. The significance of these Reports is addressed below.*

For the Director,

A handwritten signature in black ink, appearing to read "Michael P. Unterweger".

Michael P. Unterweger, Acting Leader
Radioactivity Group
Physics Laboratory

* As guidance for the proper use of Reports of Traceability, it should be emphasized that the National Institute of Standards and Technology is concerned only with fostering good measurements capability and consistency with the national measurements system. The assurance of the proper application of that capability to the ultimate consumer products is the responsibility of each manufacturer of these products and of the Federal regulatory agencies.

A continuing traceability program in radioactivity demonstrates, to the degree established by the periodic assays of calibrated radioactivity samples, a continuing competence to maintain the methods and standards necessary for accurate measurement. Such a program cannot, however, endorse each and every measurement nor the final product, any more than a spot check can vouch for every unchecked item. Care should be taken, therefore, not to imply such endorsement. The proper use of this Report is governed by section 200.114 of Title 15 of the Code of Federal Regulations. These regulations may be met if Reports are quoted only in their entirety. Excerpts out of context may be misleading.

ANALYTICS

1380 Seaboard Industrial Blvd.
Atlanta, Georgia 30318-U.S.A.

Phone (404) 352-8677
Fax (404) 352-2837
customerservice@analytinc.com
www.analytinc.com

ANALYSIS OF UNCERTAINTY FOR MIXED GAMMA STANDARDS

BATCH 120

CALIBRATION DATE: April 1, 2005 12:00 EST

Isotope	Energy (keV)	Calibration Method ¹	Statistics ²	Calibration ²	Peak Fitting ²	Geometry ²	Impurities ²	Weighing ²	Combined Standard Uncertainty ²	Relative Expanded Uncertainty ² (k=2)
Cd-109	88	HPGe	0.16	1.1	0.88	0.8	0	0.2	1.64	3.3
Co-57	122	HPGe	0.23	1.1	0.71	0.7	0	0.2	1.52	3.0
Ce-139	166	HPGe	0.17	1.0	0.58	0.7	0	0.2	1.38	2.8
Hg-203	279	HPGe	0.11	1.1	0.34	0.7	0	0.2	1.37	2.7
Sn-113	392	HPGe	0.21	1.0	0.35	0.7	0	0.2	1.30	2.6
Cs-137	662	HPGe	0.36	1.1	0.60	0.7	0	0.2	1.49	3.0
Y-88	898	HPGe	0.19	1.0	0.33	0.7	0	0.2	1.29	2.6
Co-60	1173	HPGe	0.31	.97	0.45	0.7	0	0.2	1.33	2.7
Co-60	1332	HPGe	0.33	.93	0.48	0.7	0	0.2	1.32	2.6
Y-88	1836	HPGe	0.24	1.0	0.35	0.7	0	0.2	1.31	2.6

Optional Additional Isotopes

Pb-210	46.5	4π LS	0.33	1.1	0	0.9	0.30	0.2	1.50	3.0
Am-241	59.5	4π LS	0.33	1.1	0	0.9	0.30	0.2	1.50	3.0
Sr-85	514	IC	0.30	1.1	0	0.7	0.17	0.2	1.36	2.7
Cs-134	605	IC	0.30	1.0	0	0.8	0.17	0.2	1.34	2.7
Cs-134	796	IC	0.30	1.0	0	0.8	0.17	0.2	1.34	2.7
Mn-54	835	IC	0.30	1.0	0	0.8	0.17	0.2	1.34	2.7
Zn-65	1116	IC	0.30	1.0	0	0.8	0.17	0.2	1.34	2.7

Calibration Methods:

- 4π LS (4 pi Liquid Scintillation Counting)
- HPGe (High Purity Germanium Gamma Ray Spectrometer)
- IC (Gamma Ray Ionization Chamber)

²As Percent (%) from counting data

No interfering gamma emitting impurities were detected during calibration. Depending on the resolution and energy dispersion (keV/channel) of the measuring system, the following spectral conflicts may occur: (1) between the 88 keV gamma-ray and the X-rays emitted in the decay of Hg-203, (2) between the 1333 keV gamma-ray and the 1325 keV single escape peak from the 1836 keV gamma-ray.



Standard Traceability Log Rad

Source Material Info		A Solution Material Info	
Parent Code:	0781	Isotope:	Mixed Gamma
Prepared By:	Amanda Fehr	Prepared By:	Amanda Fehr
Carrier Conc:	4M HCL	Prep Date:	04/26/2005
Reference Date:	04/01/2005	Verification Date:	04/27/2005
Ampoule Mass (g):	5.3272 g	Expiration Date:	04/27/2006
Uncertainty:	+/- 3 %	Primary Code:	0781-A
LogBook No:	RC-S-039-065	Dilution(mL):	100 mL
		Mass of Parent(g):	5.1233 g
		Density(g/mL):	5.4962

Calculations Converting parent activity to dpm/mL|dpm/g

$(\text{Mass of parent(g)}) * (\text{Parm Activity (dpm)}) * (\text{conversion dpm to dpm}) / (\text{Ampoule Mass(g)} * (\text{Dilution Vol})) = \text{Parent Activity (dpm/mL)}$
$(\text{Mass of parent(g)}) * (\text{Parm Activity (dpm)}) * (\text{conversion dpm to dpm}) / \text{Density} / (\text{Ampoule Mass (g)} * (\text{Dilution Vol})) = \text{Parent Activity (dpm/g)}$
$(5.1233 \text{ g}) * (219149.436 \text{ dpm}) * (1 \text{ dpm/dpm}) / (5.3272 \text{ g} * 100 \text{ mL}) = 2107.6143 \text{ dpm/mL}$
$(5.1233 \text{ g}) * (219149.436 \text{ dpm}) * (1 \text{ dpm/dpm}) / (5.4962 \text{ g/mL}) / (5.3272 \text{ g} * 100 \text{ mL}) = 383.4709 \text{ dpm/g}$

Secondary Standards

Prep Date	Preparer	Mass Primary	Dilution (mL)	Code	Conc dpm/mL	Verification Date	Expiration Date
-----------	----------	--------------	---------------	------	-------------	-------------------	-----------------

General Engineering Laboratories, LLC

Version 1.0 9/18/2000

Verification for Mixed Gamma Standard 0781-A (AM-241 & Cs-137)

A. Fehr
4/29/2005

Am-241	Isotope	Result	Cs-137	Isotope	Result
	Mixed Gamma N1	9796		Mixed Gamma N1	3753
	Mixed Gamma N2	9930		Mixed Gamma N2	4015
	Mixed Gamma N3	10290		Mixed Gamma N3	3878
Mean Value (Counting) =	10005.33	102.47	Pass	3882.00	102.39
Stdev =	255.471	Rule 3 (Pass/Fail)		131.046	Pass
Certificate Value =	9764.6			3791.3	
Lower Limit =	9494.391719			3619.908413	
Upper Limit =	10516.27495			4144.091587	
Rule 1 (Pass/Fail)	Pass			Pass	
Two sigma =	510.9416144			262.091587	
10 % of Mean =	1000.53333333			388.20000000	
Rule 2 (Pass/Fail)	Pass			Pass	

Verification Rules

Rule 1 = The certificate value (NOT including any uncertainty) shall lie within the 95% confidence interval determined from the mean and two sigma standard deviation of the three measurements

Rule 2 = The two sigma value used for the 95% confidence interval shall not exceed 10% of the mean value of the three verification measurements.

Rule 3 = The determined mean value shall be within 10% of the certificate value.

Amanda L. Fehr 4/29/05

Angela L. Johnson 5/6/05

Verification for Mixed Gamma Standard 0781-A (Co-60)

A. Fehr 4/29/2005	Isotope	Result pCi/L	
	Mixed Gamma N1	6132	
	Mixed Gamma N2	6073	
	Mixed Gamma N3	6240	
Mean Value (Counting) =	6148.33	pCi/L	102.365 Pass
Stdev =	84.690	pCi/L	Rule 3 (Pass/Fail)
Certificate Value =	6006.3	pCi/L	
Lower Limit =	5978.954074	pCi/L	
Upper Limit =	6317.712592	pCi/L	
Rule 1 Pass/Fail	Pass		
Two sigma =	169.3792589		
10 % of Mean =	614.8333333		
Rule 2 (Pass/Fail)	Pass		

Verification Rules

Rule 1 = The certificate value (NOT including any uncertainty) shall lie within the 95% confidence interval determined from the mean and two sigma standard deviation of the three measurements

Rule 2 = The two sigma value used for the 95% confidence interval shall not exceed 10% of the mean value of the three verification measurements.

Rule 3 = The determined mean value shall be within 10% of the certificate value.

Amanda L. Fehr 4/29/05

*Angela L. Johnson
5/6/05*

DEUTSCHER KALIBRIERDIENST (DKD)

Kalibrierlaboratorium für Meßgrößen der Radioaktivität
Calibration laboratory for measurements of radioactivity

AKKREDITIERT DURCH DIE PHYSIKALISCH-TECHNISCHE BUNDESANSTALT (PTB)



Amersham Buchler GmbH & Co KG
Postfach 11 49 Gieselweg 1
D-38001 Braunschweig D-38110 Braunschweig

Telefon (05307) 930-0
Telefax (05307) 930-293
Telefax-Zentrale 930-237

02628
DKD-K- 06501
95-10

Kalibrierschein Calibration Certificate

Kalibrierzeichen
Calibration mark

Gegenstand Object	Radioactive Reference Solution	<p>Der Deutsche Kalibrierdienst ist Unterzeichner des multilateralen Übereinkommens der Western European Calibration Cooperation (WECC) zur gegenseitigen Anerkennung der Kalibrierscheine. Die Kalibrierung erfolgt auf der Grundlage des zwischen der Physikalisch-Technischen Bundesanstalt und dem Träger abgeschlossenen Vertrages. Dieser Kalibrierschein dokumentiert die Rückführbarkeit auf nationale Normale zur Darstellung der physikalischen Einheiten in Übereinstimmung mit dem Internationalen Einheitensystem (SI). Für die Einhaltung einer angemessenen Frist zur Wiederholung der Kalibrierung ist der Benutzer verantwortlich.</p> <p><i>The Deutscher Kalibrierdienst is signatory to the multilateral agreement of the Western European Calibration Cooperation (WECC) for the mutual recognition of calibration certificates. The calibration is performed according to the stipulations of the contract between the Physikalisch-Technische Bundesanstalt and the holder of the calibration laboratory.</i></p> <p><i>This calibration certificate documents the traceability to national standards, which realize the physical units of measurement according to the International System of Units (SI).</i></p> <p><i>The user is obliged to have the object recalibrated at appropriate intervals.</i></p>
Hersteller Manufacturer	Amersham Buchler GmbH & Co KG Postfach 11 49 Gieselweg 1 D-38001 Braunschweig D-38110 Braunschweig	
Typ Type	RBZB44	
Strahler-Nr. Source number	ET 491	
Auftraggeber Customer	Amersham Corporation 2636 S. Clearbrook Drive Arlington Heights, IL 60005 USA-Arlington Heights, IL	
Auftragsnummer Work order number	112116	
Anzahl der Seiten des Kalibrierscheines Number of pages of the certificate	2	
Referenzdatum Reference date	1 January 1995	

Dieser Kalibrierschein darf nur vollständig und unverändert weiterverbreitet werden. Auszüge oder Änderungen bedürfen der Genehmigung sowohl der Physikalisch-Technischen Bundesanstalt als auch des ausstellenden Kalibrierlaboratoriums.

Kalibrierscheine ohne Unterschrift und Stempel haben keine Gültigkeit.

This calibration certificate may not be reproduced other than in full except with the permission of both the Physikalisch-Technische Bundesanstalt and the issuing laboratory.

Calibration certificates without signature and seal are not valid.

Stempel Seal	Datum Date	Leiter des Kalibrierlaboratoriums Head of the calibration laboratory	Stellvertreter Deputy	Bearbeiter Person responsible
	18 October 1995	Dr. Dornhöfer	 Dr. Thieme	 E. Schulz PC-5-013-4

02628
DKD-K-06501
95-10

Radioactive Reference Solution

Solution No.: ET 491

Drawing No.: VZ-2058

Nuclide: Lead-210

Radioactive concentration: 38.1 kBq/g

Reference date: 1 January 1995 at 12.00 GMT

Mass of solution: (5.182 ± 0.001) g

Volume of solution: approx. 5 ml

Chemical composition: Solution in 1.2 M HNO₃
Carrier: Pb (NO₃)₂, Bi (NO₃)₃; each 20 mg/l of the corresponding element.

Measuring method: The activity was determined by comparison with a reference solution by measurement with a Ge-detector with MCA.

Traceability: Additional to the direct traceability to the PTB through the DKD this product satisfies the quality assurance requirements of USNRC Regulatory Guide 4.15 Revision 1, February 1979, for achieving NIST traceability through Amersham's participation in the NEI-NIST Measurements Assurance Program of the Nuclear Power Industry.

Uncertainty: The relative uncertainty of the activity is ± 3 %.

The declared uncertainty U is an expanded uncertainty $U = k * u_c$ with a coverage factor of $k = 3$. The combined uncertainty u_c is the sum of all uncertainties which can be evaluated by statistical means (uncertainty type A, u_A) and all other uncertainties (uncertainty type B, u_B) whereby $u_c^2 = u_A^2 + u_B^2$.
(Ref.: NIST Technical Note 1297 / WECC-Doc. 19-1990)

Radioactive impurities: Related to Pb-210 (equal 100 %) the following radioactive impurities were detected:
Ra-226: 0.003 %



LC-5-013-47

TRACEABILITY TO NIST

Amersham Corporation
2636 S. Clearbrook Drive
Arlington Heights, IL 60005
tel (708) 593-6300
fax (708) 593-8091



Traceability is the ability to relate the accuracy of measurement of radionuclides to the National Institute of Standards and Technology (NIST). Traceability is achieved by participation in a Measurements Assurance Program linked to NIST and production of certified materials in accordance with a quality assurance program.

Amersham participates in measurement assurance programs conducted by NIST in cooperation with the Nuclear Energy Institute (NEI, formerly USCEA). Additionally, our production facilities and measurement laboratories operate under routinely audited quality assurance programs.

Therefore, Amersham certified standardized products meet or exceed, the NRC requirements for measurements traceable to NIST.

278004C



Standard Traceability Log Rad

Source Material Info		A Solution Material Info	
Parent Code:	ET491	Isotope:	Lead-210
Prepared By:	Garret Ray	Prepared By:	Garret Ray
Carrier Conc:	1.2M HNO3	Prep Date:	03/01/1996
Reference Date:	01/01/1995	Verification Date:	07/12/2005
Ampoule Mass (g):	5.182 g	Expiration Date:	07/12/2006
Uncertainty:	+/- 3 %	Primary Code:	ET491-A
LogBook No:	RC S 014 004	Dilution(mL):	100 mL
		Mass of Parent(g):	5.0547 g
		Density(g/mL):	1.0000

Calculations Converting parent activity to dpm/mL|dpm/g

$(\text{Mass of parent(g)}) * (\text{Parm Activity (kBq/g)}) * (\text{conversion dpm to kBq}) / (\text{Dilution Vol}) = \text{Parent Activity (dpm/mL)}$
$(\text{Mass of parent(g)}) * (\text{Parm Activity (kBq/g)}) * (\text{conversion dpm to kBq}) / \text{Density (g/mL)} / (\text{Dilution Vol}) = \text{Parent Activity (dpm/g)}$
$(5.0547 \text{ g}) * (38.1 \text{ kBq/g}) * (60000 \text{ dpm/kBq}) / (100 \text{ mL}) = 115550.4420 \text{ dpm/mL}$
$(5.0547 \text{ g}) * (38.1 \text{ kBq/g}) * (60000 \text{ dpm/kBq}) / (1.0000 \text{ g/mL}) / (100 \text{ mL}) = 115550.4420 \text{ dpm/g}$

Secondary Standards

Prep Date	Preparer	Mass Primary	Dilution (mL)	Code	Conc dpm/mL	Verification Date	Expiration Date
10/20/1997	Richard Kinney	.467	100	ET491-B	524.45 dpm/ml	03/01/1997	03/01/1998
10/29/1997	Richard Kinney	3.0992	500	ET491-C	696.09 dpm/mL	10/29/1998	10/29/1999
04/03/2001	Angela Johnson	.5184	100	ET491-D	582.17 dpm/mL	04/16/2003	04/16/2004
09/15/2003	Angela Johnson	.5132	100	ET491-E	576.33 dpm/mL	11/11/2005	11/11/2006

General Engineering Laboratories, LLC
Version 1.0 9/18/2000

Verification for Pb-210 Standard ET491-E

A. Fehr
11/11/2005

Isotope	Detector CPM	BKG CPM	NET CPM	Detector Eff Mass. Used (mL)	Source DPM/mL
ET491-E N1	1098.1000	21.6000	1098.1000	1.0000	416.9502415
ET491-E N2	1124.3000	21.6000	1124.3000	1.0000	426.8984214
ET491-E N3	1105.2000	21.6000	1105.2000	1.0000	419.6461223
Average =					421.1649284

Mean Value (Counting) = 421.1649284 % of known
 Stdev = 5.145060708 0.01221626

Certificate Value = 410.9
 Lower Limit = 410.874807
 Upper Limit = 431.4550498
 Rule 1 Pass/Fail Pass Pass
 Two sigma = 10.29012142
 10 % of Mean = 42.11649284
 Rule 2 (Pass/Fail) Pass

Verification Rules

- Rule 1 = The certificate value (NOT including any uncertainty) shall lie within the 95% confidence interval determined from the mean and two sigma standard deviation of the three measurements
- Rule 2 = The two sigma value used for the 95% confidence interval shall not exceed 10% of the mean value of the three verification measurements.

The analyst prepared three calibration sources for source ET491-E by transferring 1.0 mL portions of the standard to glass liquid scintillation vials. Ten mL of Ready Gel liquid scintillation cocktail was added to each vial and the vials were shaken to mix. A Blank vial was prepared in a similar fashion using 1 mL of DI water and 10 mL of Ready Gel cocktail. The calibration vials and background source were dark adapted for two hours and counted on LSC Yellow (Wallac) using Protocol 31 for Pb-210 standard verification. The efficiency calibration which was used for verification calculations was performed on 4/19/04 using source 0356-A (Pb-210). Each verification source calculation was performed as follows:

$$\text{Source dpm/g} = (A - B)/(C)(D)$$

where:

- A = Ver. source cpm,
- B = BKG cpm,
- C = System efficiency, (cpm/dpm), and
- D = mass used for standard verification.

Reference RAD SOP M-001

Amanda L. Fehr 11/11/05

STANDARDIZATION OF LEAD CARRIER

DATE: 1/30/2006
 LOT NUMBER: 1006864

	LEAD PRECIPITATES				Average	Std. Dev.	
	1	2	3	4			
Weight of carrier added	1.00	1.01	1.00	1.01	13.88	± 0.05	0.003604
Aliquot (1.00 mL)	1	1	1	1	13.81	± 0.12	0.008355
filter + ppt	0.0975	0.0970	0.0979	0.0978			
filter	0.0836	0.0832	0.0840	0.0839			
Wt. of ppt., g	0.0139	0.0138	0.0139	0.0139	13.88	mg Pb/mL	
					13.81	mg Pb/g	
mg Ca/mL	13.90	13.80	13.90	13.90			
mg Ca/g	13.90	13.66	13.90	13.76			

0.5% of Mean Value = 0.069 Pass

A satisfactory standardization is obtained when results give a standard deviation of less than 0.5% of the mean value.

0873



Certificate of Analysis

Catalog No: 060092-17

Lot No: 1006726

Storage: Ambient

Matrix: 1M HNO₃

Container: 250 ml Narrow Mouth, HDPE

Quality System
Audited & Registered
by NSF-ISR to ISO 9001:2000

Date Received: 4/19/05

Expiration Date: 6/17/2007

Description: Uranium 500 µg/L ± 0.5% in 1M HNO₃

Element	Symbol	CAS No	Source Lot No	Purity %	Concentration ug/L
Uranium Total	U	7440-61-1	7075.42.5	100	500

Certified By:

Mark Filla

This standard was prepared gravimetrically using balances calibrated with NIST traceable weights (NIST Test Number 2/264157-00). Only calibrated Class A volumetric glassware was used to prepare this standard. Sub-boiled distilled acid and megaohm deionized water were used to stabilize the product. All raw materials were checked for stoichiometry and purity prior to use. This standard has been spectrometrically certified by an independent source, which is directly traceable to NIST.

RUNLOGS



Instrument Run Log

ID	Sample Type	Analyst	Instrument	Dil	Run Date	Batch Id	Status	Geometry	Cal Date
158269001	SAMPLE	LCW1	1001		07-APR-2006 18:07	517153	DONE		
158269002	SAMPLE	LCW1	1003		07-APR-2006 18:07	517153	DONE		
158269003	SAMPLE	LCW1	1004		07-APR-2006 18:07	517153	DONE		
158269004	SAMPLE	LCW1	1005		07-APR-2006 18:07	517153	DONE		
158270001	SAMPLE	LCW1	1007		07-APR-2006 18:07	517153	DONE		
158270002	SAMPLE	LCW1	1009		07-APR-2006 18:07	517153	DONE		
158437001	SAMPLE	LCW1	1010		07-APR-2006 18:07	517153	DONE		
158437002	SAMPLE	LCW1	1011		07-APR-2006 18:07	517153	DONE		
158437004	SAMPLE	LCW1	1021		07-APR-2006 18:07	517153	DONE		
158438001	SAMPLE	LCW1	1023		07-APR-2006 18:07	517153	DONE		
158438002	SAMPLE	LCW1	1026		07-APR-2006 18:07	517153	DONE		
158438003	SAMPLE	LCW1	1027		07-APR-2006 18:07	517153	DONE		
158438005	SAMPLE	LCW1	1029		07-APR-2006 18:07	517153	DONE		
1201062927	MB	LCW1	1030		07-APR-2006 18:07	517153	DONE		
1201062928	DUP	LCW1	1032		07-APR-2006 18:07	517153	DONE		
1201062929	MS	LCW1	1034		07-APR-2006 18:07	517153	DONE		
158437003	SAMPLE	LCW1	1016		08-APR-2006 08:46	517153	DONE		
158438004	SAMPLE	LCW1	1017		08-APR-2006 08:46	517153	DONE		
1201062930	LCS	LCW1	1018		08-APR-2006 08:46	517153	DONE		

Version 1.1 9/5/05

General Engineering Laboratories, LLC



Instrument Run Log

ID	Sample Type	Analyst	Instrument	Dil	Run Date	Batch Id	Status	Geometry	Cal Date
158269001	SAMPLE	LCW1	1032		08-APR-2006 15:43	517155	DONE		
158269002	SAMPLE	LCW1	1033		08-APR-2006 15:43	517155	DONE		
158269003	SAMPLE	LCW1	1034		08-APR-2006 15:43	517155	DONE		
158269004	SAMPLE	LCW1	1037		08-APR-2006 15:43	517155	DONE		
158270001	SAMPLE	LCW1	1038		08-APR-2006 15:43	517155	DONE		
158270002	SAMPLE	LCW1	1040		08-APR-2006 15:43	517155	DONE		
158437001	SAMPLE	LCW1	1041		08-APR-2006 15:43	517155	DONE		
158437002	SAMPLE	LCW1	1042		08-APR-2006 15:43	517155	DONE		
158437003	SAMPLE	LCW1	1043		08-APR-2006 15:43	517155	DONE		
158437004	SAMPLE	LCW1	1044		08-APR-2006 15:43	517155	DONE		
158438001	SAMPLE	LCW1	1045		08-APR-2006 15:43	517155	DONE		
158438002	SAMPLE	LCW1	1046		08-APR-2006 15:43	517155	DONE		
158438003	SAMPLE	LCW1	1047		08-APR-2006 15:43	517155	DONE		
158438004	SAMPLE	LCW1	1048		08-APR-2006 15:43	517155	DONE		
158438005	SAMPLE	LCW1	1077		08-APR-2006 15:43	517155	DONE		
1201062931	MB	LCW1	1078		08-APR-2006 15:43	517155	DONE		
1201062932	DUP	LCW1	1079		08-APR-2006 15:43	517155	DONE		
1201062933	MS	LCW1	1080		08-APR-2006 15:43	517155	DONE		
1201062934	LCS	LCW1	1081		08-APR-2006 15:43	517155	DONE		

Version 1.1 9/5/05

General Engineering Laboratories, LLC



Instrument Run Log

ID	Sample Type	Analyst	Instrument	Dil	Run Date	Batch Id	Status	Geometry	Cal Date
158269001	SAMPLE	MJH1	GAMMA16		10-APR-2006 21:53	513802	DONE	CAN	22-MAR-2006
158269002	SAMPLE	MJH1	GAMMA16		10-APR-2006 23:57	513802	DONE	CAN	22-MAR-2006
158269003	SAMPLE	MJH1	GAMMA16		11-APR-2006 06:14	513802	DONE	CAN	22-MAR-2006
158269004	SAMPLE	MJH1	GAMMA16		11-APR-2006 10:22	513802	DONE	CAN	22-MAR-2006
158270001	SAMPLE	MJH1	GAMMA16		11-APR-2006 14:29	513802	DONE	CAN	22-MAR-2006
1201055609	LCS	MJH1	WELL		11-APR-2006 14:31	513802	DONE	CAN	29-DEC-2005
158270002	SAMPLE	MJH1	GAMMA10		11-APR-2006 23:18	513802	DONE	CAN	15-FEB-2006
1201055607	MB	MJH1	GAMMA13		11-APR-2006 23:19	513802	DONE	CAN	22-JUN-2005
1201055608	DUP	MJH1	GAMMA16		11-APR-2006 23:19	513802	DONE	CAN	22-MAR-2006

Version 1.1 9/5/05

General Engineering Laboratories, LLC



Instrument Run Log

ID	Sample Type	Analyst	Instrument	Dil	Run Date	Batch Id	Status	Geometry	Cal Date
158048001	SAMPLE	BXF1	PIC1A		09-APR-2006 09:57	517517	DONE	Tuffryn Filter	29-JUL-2005
158048002	SAMPLE	BXF1	PIC1B		09-APR-2006 09:57	517517	DONE	Tuffryn Filter	29-JUL-2005
1201063764	MB	BXF1	PIC3C		09-APR-2006 09:57	517517	DONE	Tuffryn Filter	29-JUL-2005
1201063765	DUP	BXF1	PIC3D		09-APR-2006 09:57	517517	DONE	Tuffryn Filter	29-JUL-2005
1201063766	MS	BXF1	PIC4A		09-APR-2006 09:57	517517	DONE	Tuffryn Filter	29-JUL-2005
1201063767	LCS	BXF1	PIC4B		09-APR-2006 09:57	517517	DONE	Tuffryn Filter	29-JUL-2005
158048003	SAMPLE	BXF1	PIC1C		09-APR-2006 09:57	517517	DONE	Tuffryn Filter	29-JUL-2005
158048004	SAMPLE	BXF1	PIC1D		09-APR-2006 09:57	517517	DONE	Tuffryn Filter	29-JUL-2005
158048005	SAMPLE	BXF1	PIC2A		09-APR-2006 09:57	517517	DONE	Tuffryn Filter	29-JUL-2005
158269001	SAMPLE	BXF1	PIC2B		09-APR-2006 09:57	517517	DONE	Tuffryn Filter	29-JUL-2005
158269002	SAMPLE	BXF1	PIC2C		09-APR-2006 09:58	517517	DONE	Tuffryn Filter	29-JUL-2005
158269003	SAMPLE	BXF1	PIC2D		09-APR-2006 09:58	517517	DONE	Tuffryn Filter	29-JUL-2005
158269004	SAMPLE	BXF1	PIC3B		09-APR-2006 09:58	517517	DONE	Tuffryn Filter	29-JUL-2005

Version 1.1 9/5/05

General Engineering Laboratories, LLC



Instrument Run Log

ID	Sample Type	Analyst	Instrument	Dil	Run Date	Batch Id	Status	Geometry	Cal Date
158269001	SAMPLE	DRS1	KPA11AUTO1		19-APR-2006 10:06	521637	DONE		
158269002	SAMPLE	DRS1	KPA11AUTO1		19-APR-2006 10:08	521637	DONE		
158269003	SAMPLE	DRS1	KPA11AUTO1		19-APR-2006 10:10	521637	DONE		
158269004	SAMPLE	DRS1	KPA11AUTO1		19-APR-2006 10:12	521637	DONE		
158270001	SAMPLE	DRS1	KPA11AUTO1		19-APR-2006 10:14	521637	DONE		
158270002	SAMPLE	DRS1	KPA11AUTO1		19-APR-2006 10:16	521637	DONE		
158437001	SAMPLE	DRS1	KPA11AUTO1		19-APR-2006 10:18	521637	DONE		
158437002	SAMPLE	DRS1	KPA11AUTO1		19-APR-2006 10:21	521637	DONE		
158437003	SAMPLE	DRS1	KPA11AUTO1		19-APR-2006 10:23	521637	DONE		
158438003	SAMPLE	DRS1	KPA11AUTO1		19-APR-2006 10:31	521637	DONE		
158438004	SAMPLE	DRS1	KPA11AUTO1		19-APR-2006 10:33	521637	DONE		
1201073174	MB	DRS1	KPA11AUTO1		19-APR-2006 10:37	521637	DONE		
1201073177	LCS	DRS1	KPA11AUTO1		19-APR-2006 10:46	521637	DONE		
1201073178	LCSD	DRS1	KPA11AUTO1		19-APR-2006 10:48	521637	DONE		
158437004	SAMPLE	DRS1	KPA11AUTO1		20-APR-2006 15:03	521637	DONE		
158438001	SAMPLE	DRS1	KPA11AUTO1		20-APR-2006 15:06	521637	DONE		
158438002	SAMPLE	DRS1	KPA11AUTO1		20-APR-2006 15:08	521637	DONE		
158438005	SAMPLE	DRS1	KPA11AUTO1		20-APR-2006 15:11	521637	DONE		
1201073175	DUP	DRS1	KPA11AUTO1		20-APR-2006 15:13	521637	DONE		
1201073176	MS	DRS1	KPA11AUTO1		20-APR-2006 15:15	521637	DONE		

Version 1.1 9/5/05
General Engineering Laboratories, LLC